

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
 Data File : BM043400.D
 Acq On : 18 Dec 2023 19:21
 Operator : MA/JU
 Sample : PB157834BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK834

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	31	34	40	rVB	124789	151502	2.15%	0.168%
2	3.810	102	106	123	rBV	1519532	2333641	33.11%	2.588%
3	4.140	158	162	172	rVB	95410	131101	1.86%	0.145%
4	7.151	668	674	686	rVB	1796390	2836661	40.24%	3.146%
5	7.328	698	704	719	rVB	1359678	2219683	31.49%	2.462%
6	7.522	729	737	747	rBV	1691607	2744320	38.93%	3.044%
7	7.992	810	817	828	rBV	1564360	2500176	35.47%	2.773%
8	8.704	930	938	949	rBV	2061815	3335624	47.32%	3.700%
9	9.163	1009	1016	1029	rBV	1616171	2675881	37.96%	2.968%
10	9.886	1130	1139	1147	rBV	1295459	2168511	30.77%	2.405%
11	10.422	1222	1230	1241	rBV	1859966	3176245	45.06%	3.523%
12	10.516	1244	1246	1254	rVB8	5694	9005	0.13%	0.010%
13	10.804	1287	1295	1308	rVB	2065206	3553425	50.41%	3.941%
14	10.945	1308	1319	1335	rBV	2022728	3495816	49.60%	3.878%
15	11.598	1426	1430	1435	rVB8	4157	8800	0.12%	0.010%
16	12.386	1555	1564	1569	rBV2	32222	53949	0.77%	0.060%
17	13.521	1751	1757	1763	rBV2	24154	41994	0.60%	0.047%
18	13.598	1766	1770	1773	rBV4	7705	12567	0.18%	0.014%
19	14.039	1839	1845	1854	rBV	3013032	4156925	58.98%	4.611%
20	14.321	1885	1893	1903	rBV	3533584	5342429	75.79%	5.926%
21	14.621	1937	1944	1953	rBV	2859691	4208517	59.71%	4.668%
22	14.721	1958	1961	1966	rVB7	6037	8425	0.12%	0.009%
23	14.821	1970	1978	1998	rBV	1642776	2496547	35.42%	2.769%
24	15.045	2010	2016	2023	rVB	9295	20433	0.29%	0.023%
25	15.615	2106	2113	2121	rBV	4435712	6212270	88.14%	6.891%
26	15.733	2125	2133	2144	rBV	1371978	1842966	26.15%	2.044%
27	15.851	2150	2153	2159	rVB3	19871	28018	0.40%	0.031%
28	16.180	2205	2209	2214	rVB8	5912	10475	0.15%	0.012%
29	16.398	2241	2246	2251	rBV8	14439	27439	0.39%	0.030%
30	17.051	2350	2357	2361	rBV7	6226	12041	0.17%	0.013%
31	17.133	2364	2371	2372	rVV6	4729	8904	0.13%	0.010%
32	17.151	2372	2374	2379	rVB6	9707	14922	0.21%	0.017%
33	17.362	2403	2410	2420	rBV	3160392	4575848	64.92%	5.075%
34	17.462	2420	2427	2440	rVV2	4471691	6497818	92.19%	7.207%
35	17.562	2442	2444	2449	rVB6	6452	8465	0.12%	0.009%
36	17.633	2450	2456	2458	rBV6	6854	10995	0.16%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043400.D
Acq On : 18 Dec 2023 19:21
Operator : MA/JU
Sample : PB157834BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK834

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	19.315	2738	2742	2747	rBV2	50442	72717	1.03%	0.081%
38	19.386	2750	2754	2758	rBV	45393	58367	0.83%	0.065%
39	19.750	2810	2816	2828	rBV	5370300	6903823	97.95%	7.658%
40	21.539	3115	3120	3127	rBV	3541316	4443100	63.04%	4.928%
41	23.809	3498	3506	3516	rBV2	3593631	7048543	100.00%	7.818%
42	23.968	3525	3533	3542	rVB	2215077	4697151	66.64%	5.210%




Sum of corrected areas: 90156039

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043400.D
Acq On : 18 Dec 2023 19:21
Operator : MA/JU
Sample : PB157834BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK834

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

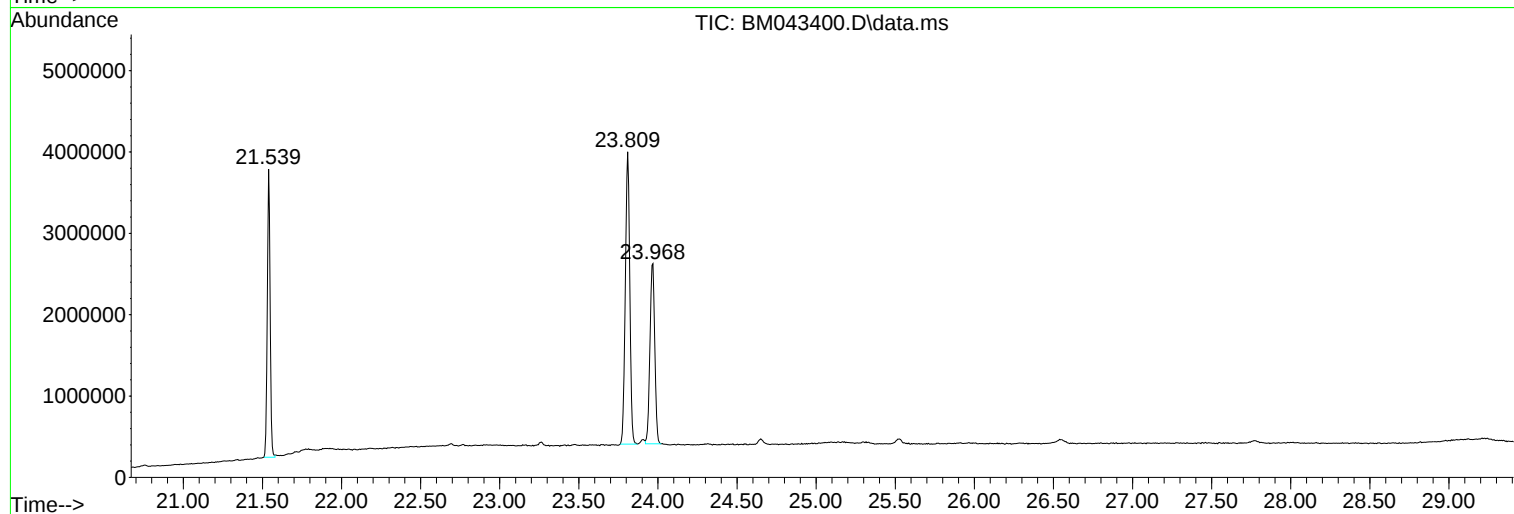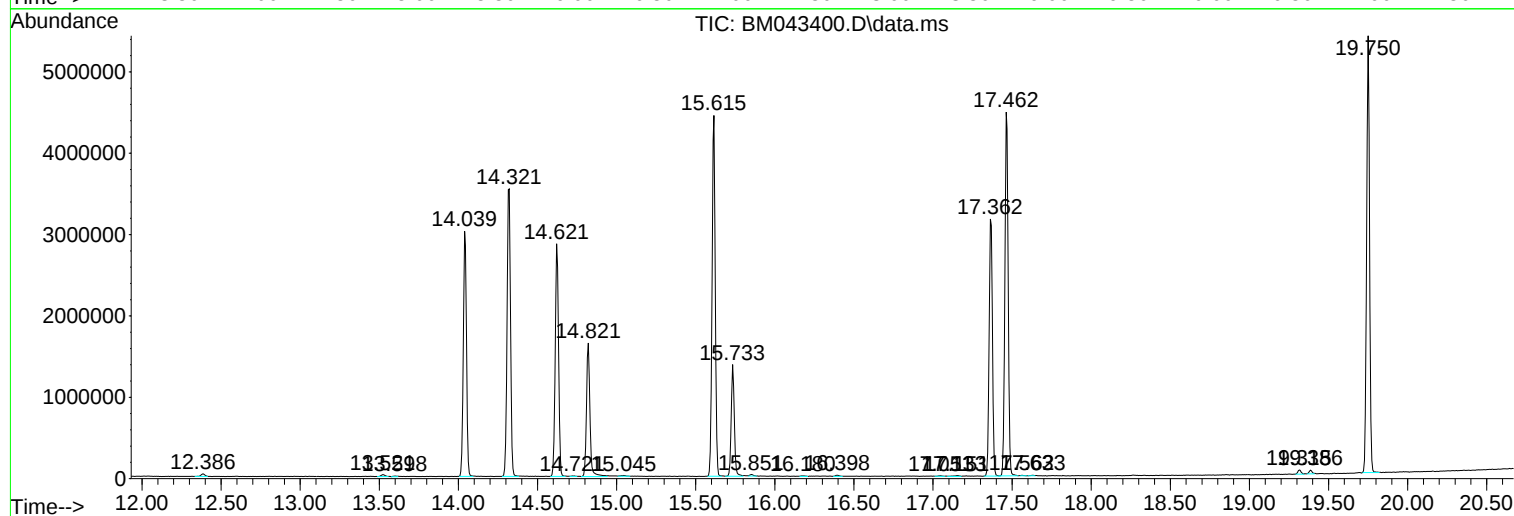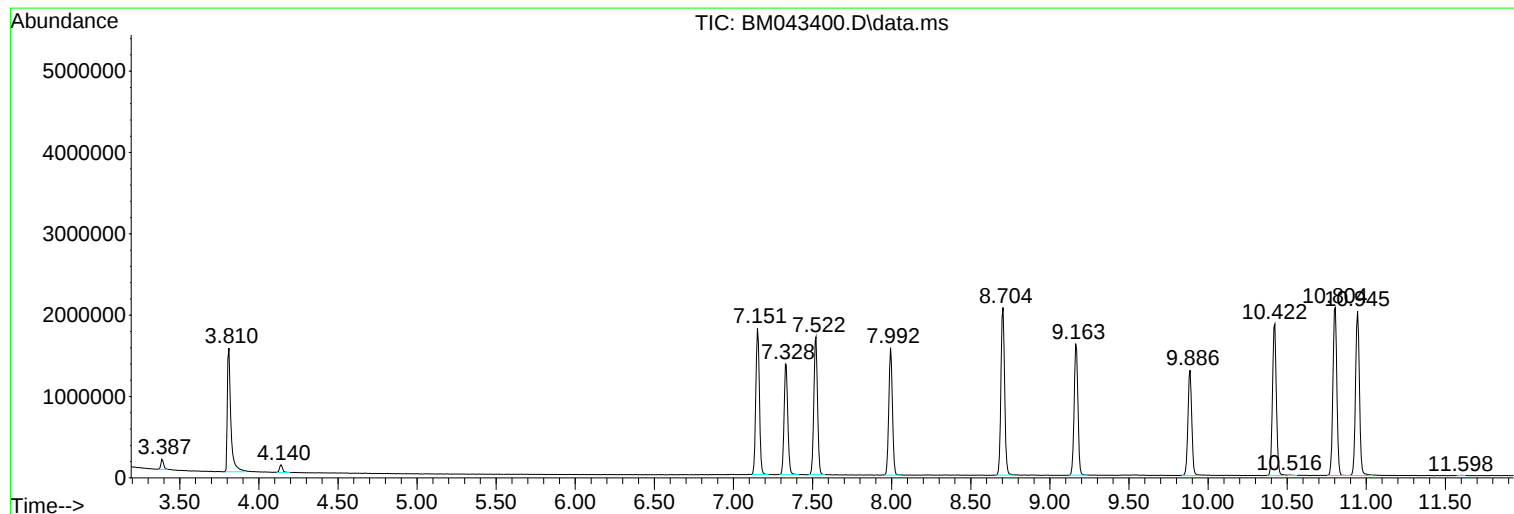

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043400.D
Acq On : 18 Dec 2023 19:21
Operator : MA/JU
Sample : PB157834BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK834

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043400.D
Acq On : 18 Dec 2023 19:21
Operator : MA/JU
Sample : PB157834BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK834

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc