

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
 Data File : BM043412.D
 Acq On : 19 Dec 2023 03:11
 Operator : MA/JU
 Sample : PB157834BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK834

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	44	rVB	153377	202235	2.39%	0.178%
2	3.805	102	105	128	rBV	2069489	3109381	36.74%	2.742%
3	4.140	157	162	171	rVB	111127	161516	1.91%	0.142%
4	7.151	667	674	686	rBV	2445263	3849710	45.49%	3.394%
5	7.328	695	704	718	rBV	1873219	2975682	35.16%	2.624%
6	7.516	727	736	746	rBV	2321008	3678032	43.46%	3.243%
7	7.993	807	817	825	rBV	2117542	3338927	39.45%	2.944%
8	8.704	929	938	951	rBV	2874292	4686890	55.38%	4.133%
9	9.163	1007	1016	1024	rBV	2317527	3749953	44.31%	3.306%
10	9.881	1128	1138	1151	rBV	1805864	3096763	36.59%	2.731%
11	10.416	1221	1229	1241	rBV	2683564	4552927	53.79%	4.014%
12	10.798	1285	1294	1306	rBV	2998728	5081091	60.04%	4.480%
13	10.945	1311	1319	1332	rBV	2885768	4913919	58.06%	4.333%
14	12.386	1557	1564	1569	rBV	45560	77155	0.91%	0.068%
15	13.522	1753	1757	1762	rBV	45867	72272	0.85%	0.064%
16	13.598	1765	1770	1776	rVB9	8430	18276	0.22%	0.016%
17	14.039	1838	1845	1858	rBV	4131793	5962222	70.45%	5.257%
18	14.316	1885	1892	1907	rVB2	5024547	7556201	89.28%	6.663%
19	14.622	1936	1944	1953	rBV	4227952	6098829	72.06%	5.378%
20	14.727	1958	1962	1967	rBV7	6967	11944	0.14%	0.011%
21	14.822	1971	1978	1994	rBV	1927709	2949642	34.85%	2.601%
22	14.986	2002	2006	2011	rVV7	5358	9165	0.11%	0.008%
23	15.039	2011	2015	2021	rVB9	9700	20201	0.24%	0.018%
24	15.616	2105	2113	2123	rBV	5836376	8463498	100.00%	7.463%
25	15.733	2126	2133	2149	rBV	1657150	2309203	27.28%	2.036%
26	15.851	2149	2153	2159	rVB3	25816	42810	0.51%	0.038%
27	16.398	2241	2246	2251	rVB3	17697	29903	0.35%	0.026%
28	16.557	2267	2273	2280	rVB3	10795	20606	0.24%	0.018%
29	17.039	2352	2355	2359	rBV5	9415	13295	0.16%	0.012%
30	17.151	2368	2374	2379	rBV5	10271	22421	0.26%	0.020%
31	17.368	2404	2411	2420	rBV	3965815	5783207	68.33%	5.099%
32	17.463	2420	2427	2442	rBV	5668256	7891297	93.24%	6.958%
33	17.621	2449	2454	2463	rBV	13471	32635	0.39%	0.029%
34	18.257	2558	2562	2566	rBV6	10040	19129	0.23%	0.017%
35	19.315	2738	2742	2749	rBV2	51328	72225	0.85%	0.064%
36	19.386	2750	2754	2758	rVB	45943	60846	0.72%	0.054%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043412.D
Acq On : 19 Dec 2023 03:11
Operator : MA/JU
Sample : PB157834BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK834

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	19.751	2810	2816	2825	rBV	5573083	7073847	83.58%	6.237%
38	21.539	3115	3120	3129	rVB	3441087	4304118	50.86%	3.795%
39	23.803	3498	3505	3516	rVB2	3269700	6541696	77.29%	5.768%
40	23.962	3525	3532	3543	rVB	2199109	4558454	53.86%	4.019%




Sum of corrected areas: 113412123

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043412.D
Acq On : 19 Dec 2023 03:11
Operator : MA/JU
Sample : PB157834BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK834

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

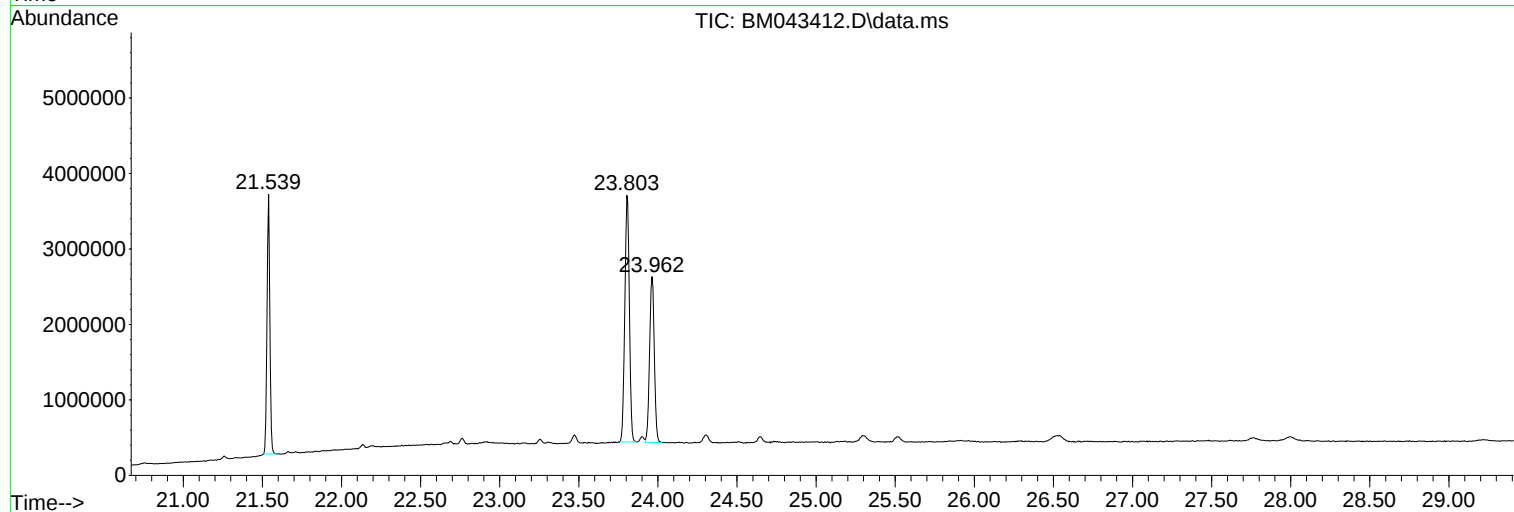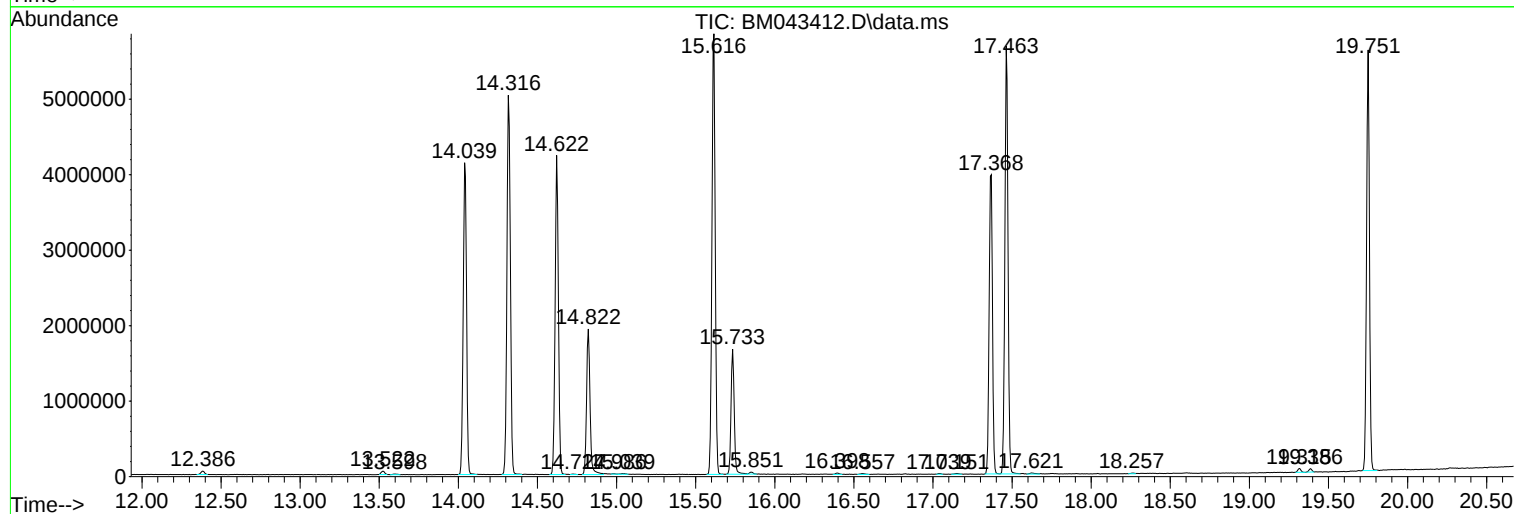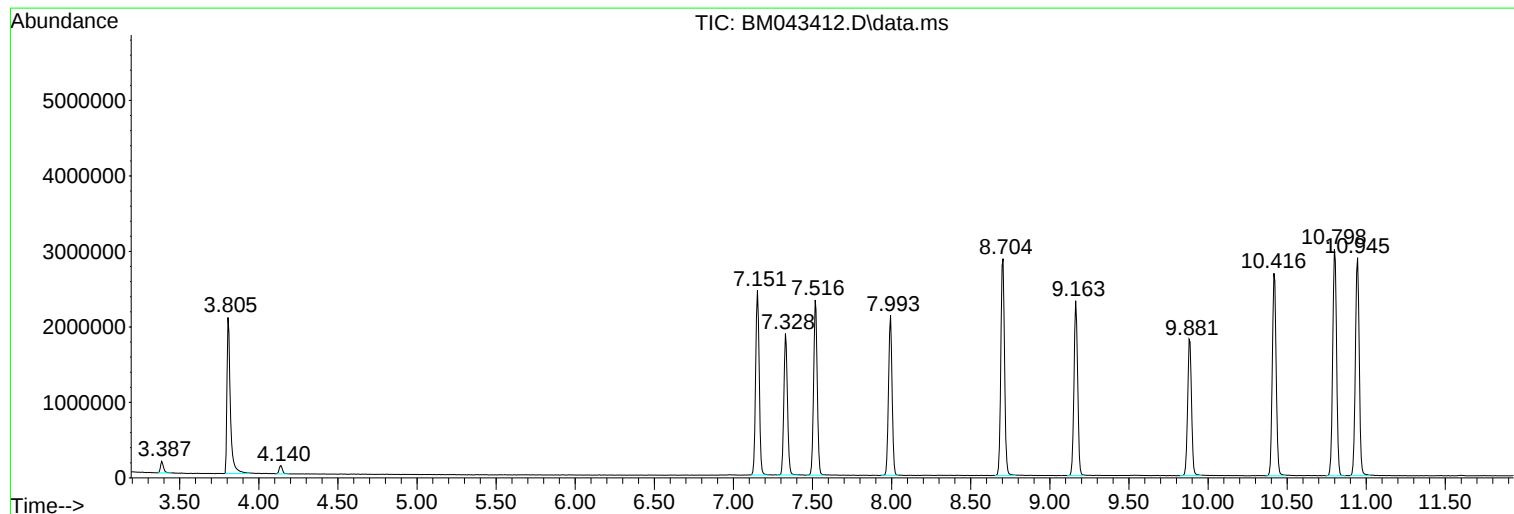

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043412.D
Acq On : 19 Dec 2023 03:11
Operator : MA/JU
Sample : PB157834BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK834

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043412.D
Acq On : 19 Dec 2023 03:11
Operator : MA/JU
Sample : PB157834BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK834

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc