

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121915\
 Data File : BM003626.D
 Acq On : 19 Dec 2015 18:56
 Operator : UM/SJ
 Sample : G4801-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9C67

Quant Time: Dec 20 01:40:32 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 20 01:33:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	17271	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	89704	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	62129	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	162512	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	251476	20.00	ng/ul	0.00
86) Perylene-d12	23.55	264	299656	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	446	1.39	ng/uL	0.00
5) Phenol-d5	6.87	99	15337	10.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	9982	12.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	13300	11.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	10063	7.98	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	7274	11.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	8174	11.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	14348	10.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	17761	9.98	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	68343	13.31	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	67882	11.61	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	9528	9.53	ng/ul	0.00
58) Fluorene-d10	15.35	176	57676	13.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	8349	9.12	ng/ul	0.00
71) Anthracene-d10	17.20	188	96029	12.99	ng/ul	0.00
79) Pyrene-d10	19.50	212	126522	11.52	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	187640	12.61	ng/ul	0.00


Target Compounds						Qvalue
45) Dimethylphthalate	13.80	163	53784	10.24	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121915\
Data File : BM003626.D
Acq On : 19 Dec 2015 18:56
Operator : UM/SJ
Sample : G4801-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9C67

Quant Time: Dec 20 01:40:32 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 20 01:33:56 2015
Response via : Initial Calibration

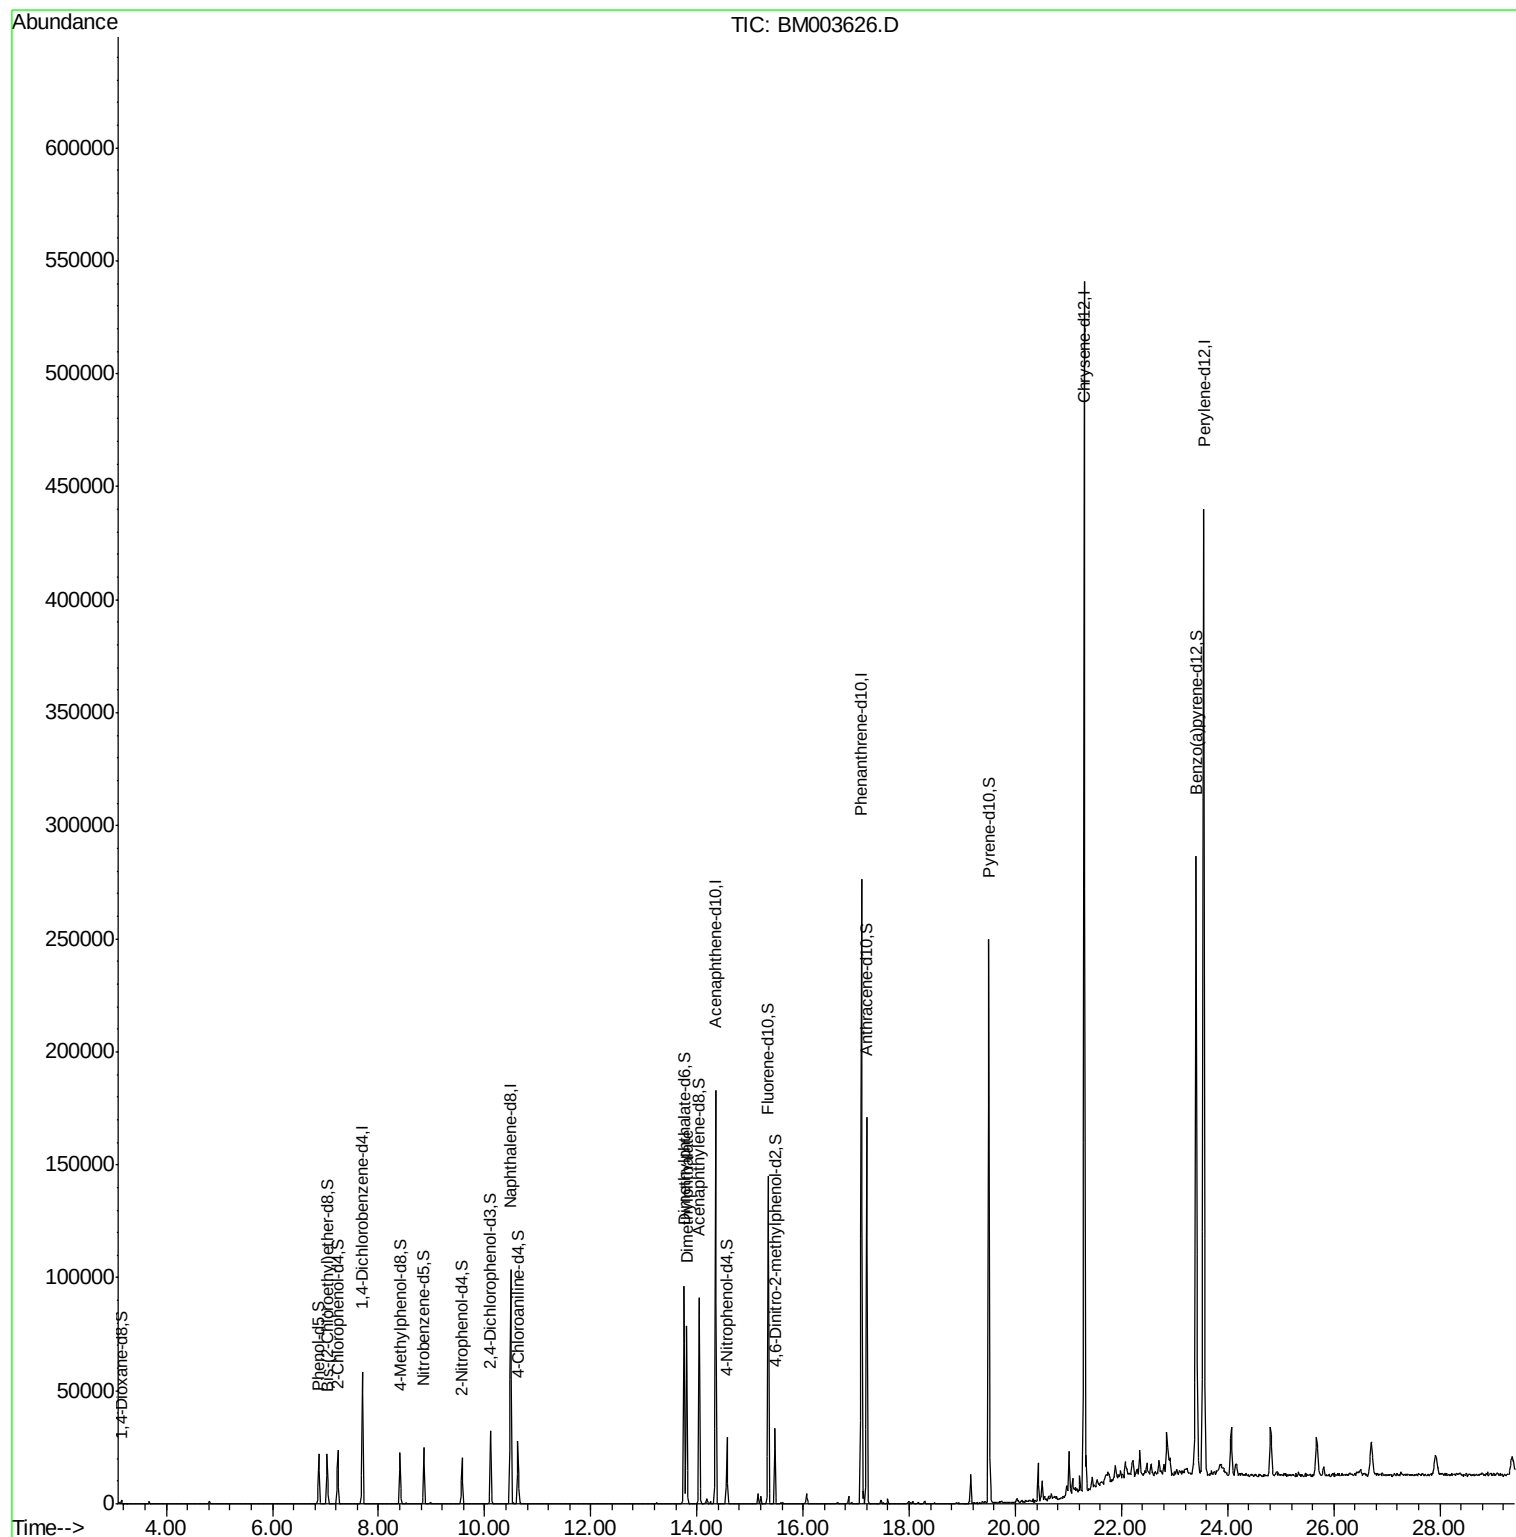

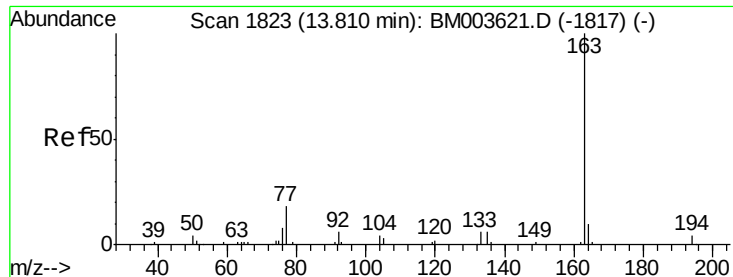

#45

Dimethylphthalate

Concen: 10.24 ng/ul

RT: 13.80 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BM003626.D

Acq: 19 Dec 2015 18:56

Instrument :

BNA_M

ClientSampleId :

G9C67


Tgt Ion:163 Resp: 53784

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 10.1 7.8 11.8

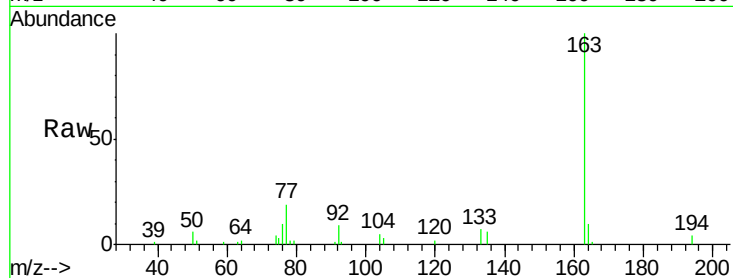

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

