

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121915\
 Data File : BM003633.D
 Acq On : 19 Dec 2015 23:06
 Operator : UM/SJ
 Sample : G4801-26
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9C74

Quant Time: Dec 20 01:42:09 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 20 01:33:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	22748	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	114736	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	76538	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	192600	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	273206	20.00	ng/ul	0.00
86) Perylene-d12	23.55	264	309553	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	2469	5.85	ng/uL	0.00
5) Phenol-d5	6.87	99	60838	31.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	35319	34.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	51877	33.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	55167	33.22	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	27382	32.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	30833	32.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	54008	31.59	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	69138	30.37	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	213369	33.73	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	243352	33.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	40705	33.03	ng/ul	0.00
58) Fluorene-d10	15.34	176	182093	34.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	27251	25.10	ng/ul	0.00
71) Anthracene-d10	17.20	188	305749	34.89	ng/ul	0.00
79) Pyrene-d10	19.50	212	381766	31.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.41	264	529744	34.45	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.80	163	75945	11.74	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121915\
Data File : BM003633.D
Acq On : 19 Dec 2015 23:06
Operator : UM/SJ
Sample : G4801-26
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9C74

Quant Time: Dec 20 01:42:09 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 20 01:33:56 2015
Response via : Initial Calibration

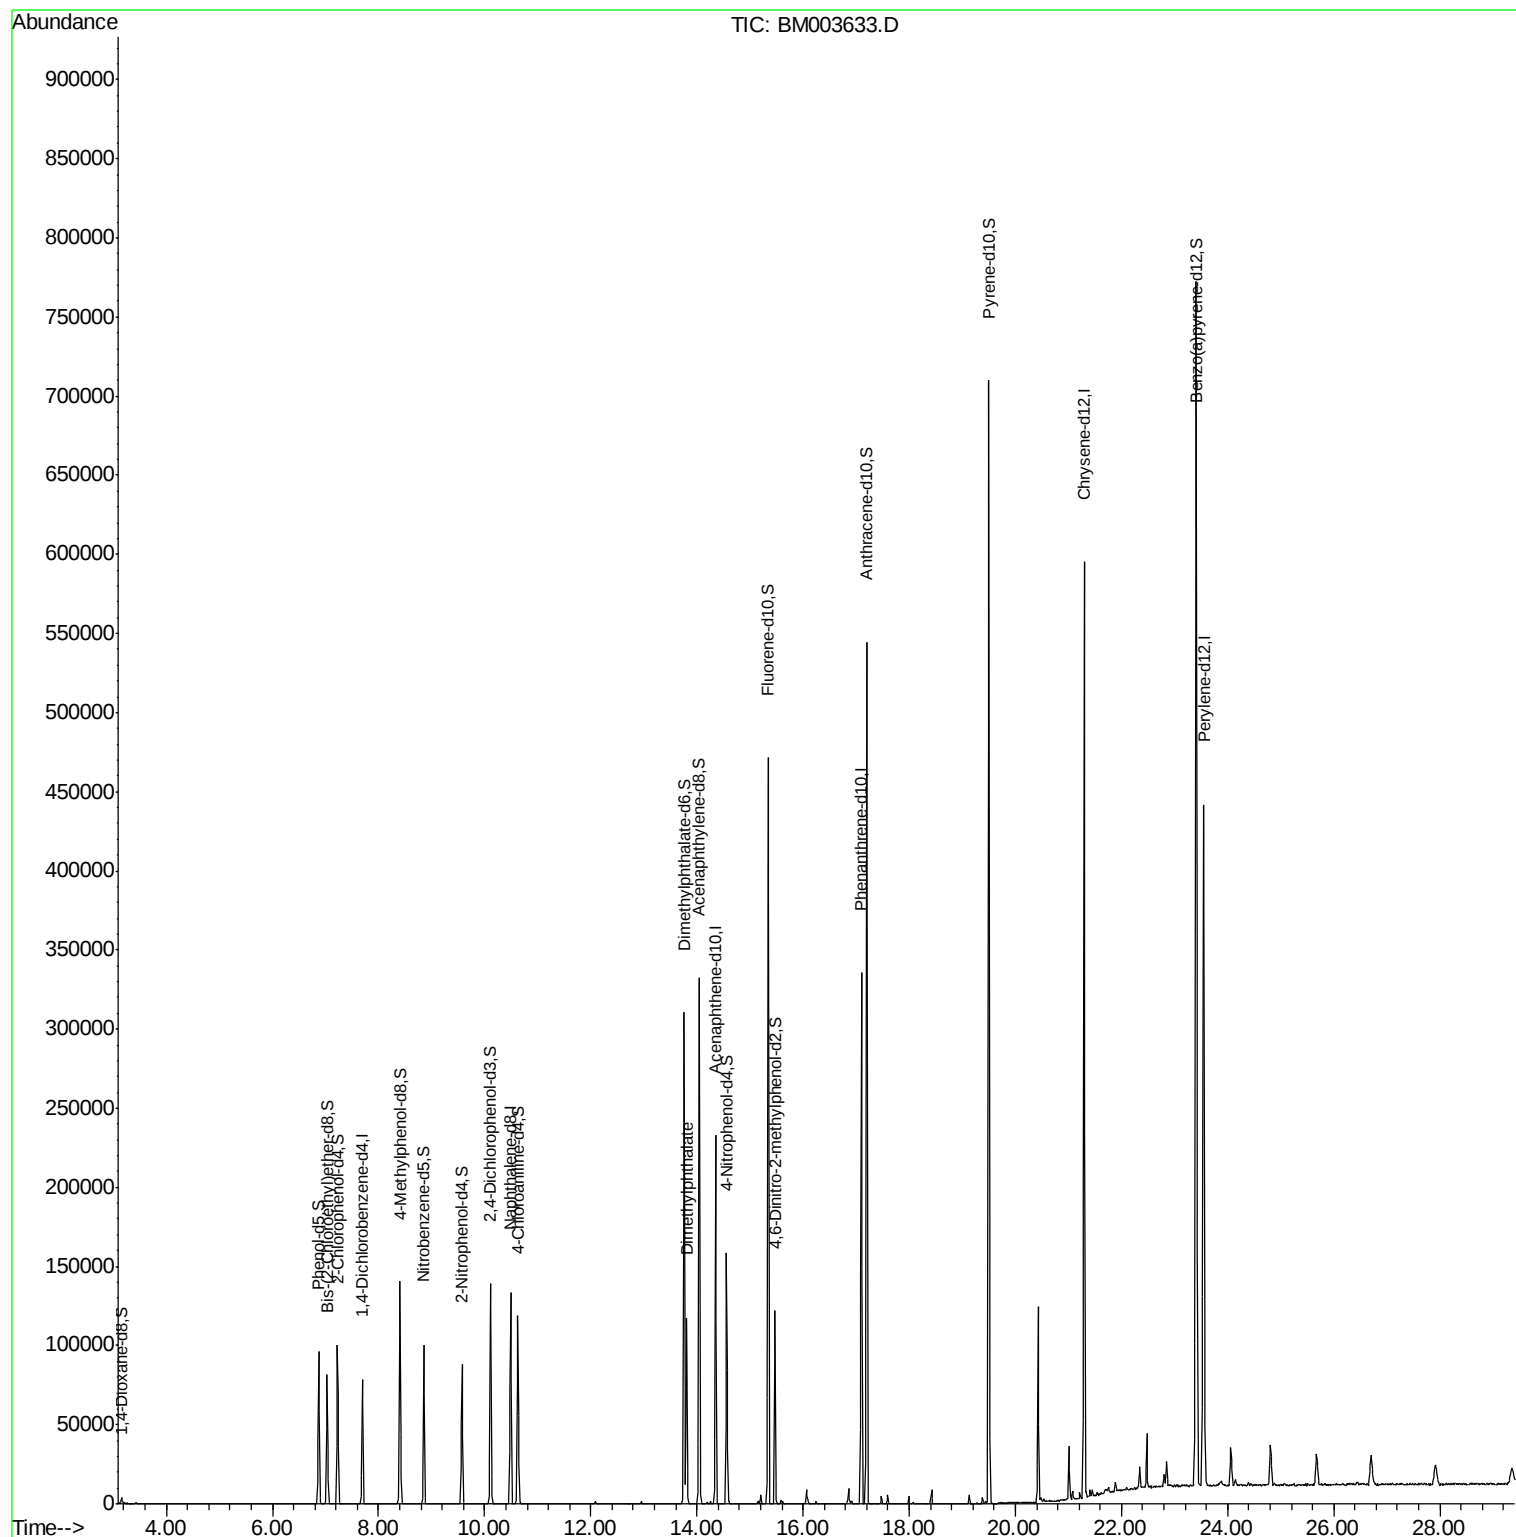

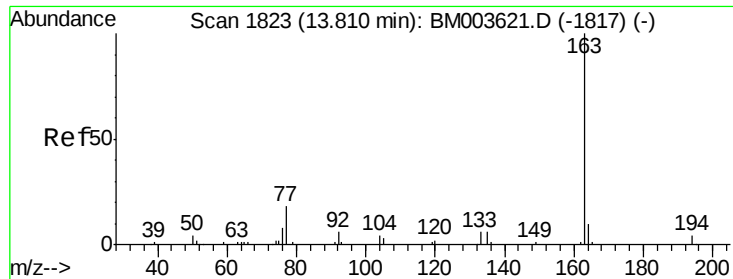

#45

Dimethylphthalate

Concen: 11.74 ng/ul

RT: 13.80 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BM003633.D

Acq: 19 Dec 2015 23:06

Instrument :

BNA_M

ClientSampleId :

G9C74


Tgt Ion:163 Resp: 75945

Ion Ratio Lower Upper

163 100

194 3.7 3.2 4.8

164 10.2 7.8 11.8

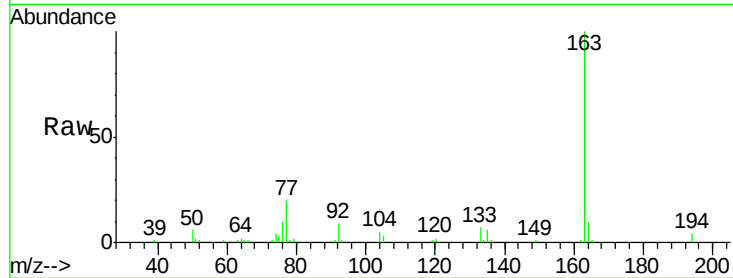

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

