

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121915\
 Data File : BM003635.D
 Acq On : 20 Dec 2015 00:17
 Operator : UM/SJ
 Sample : G4801-28
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9C76

Quant Time: Dec 20 01:42:31 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 20 01:33:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	44783	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	217377	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	142749	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	337162	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	410978	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	401475	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	4547	5.47	ng/uL	0.00
5) Phenol-d5	6.87	99	104229	27.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	57917	28.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	88631	28.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	91875	28.11	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	45812	29.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	51982	29.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	88962	27.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	111692	25.90	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	323747	27.44	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	376649	28.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	61099	26.59	ng/ul	0.00
58) Fluorene-d10	15.34	176	271126	27.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	43942	23.12	ng/ul	0.00
71) Anthracene-d10	17.20	188	430476	28.06	ng/ul	0.00
79) Pyrene-d10	19.50	212	510165	28.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	577607	28.96	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.81	163	147832	12.25	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121915\
Data File : BM003635.D
Acq On : 20 Dec 2015 00:17
Operator : UM/SJ
Sample : G4801-28
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9C76

Quant Time: Dec 20 01:42:31 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 20 01:33:56 2015
Response via : Initial Calibration

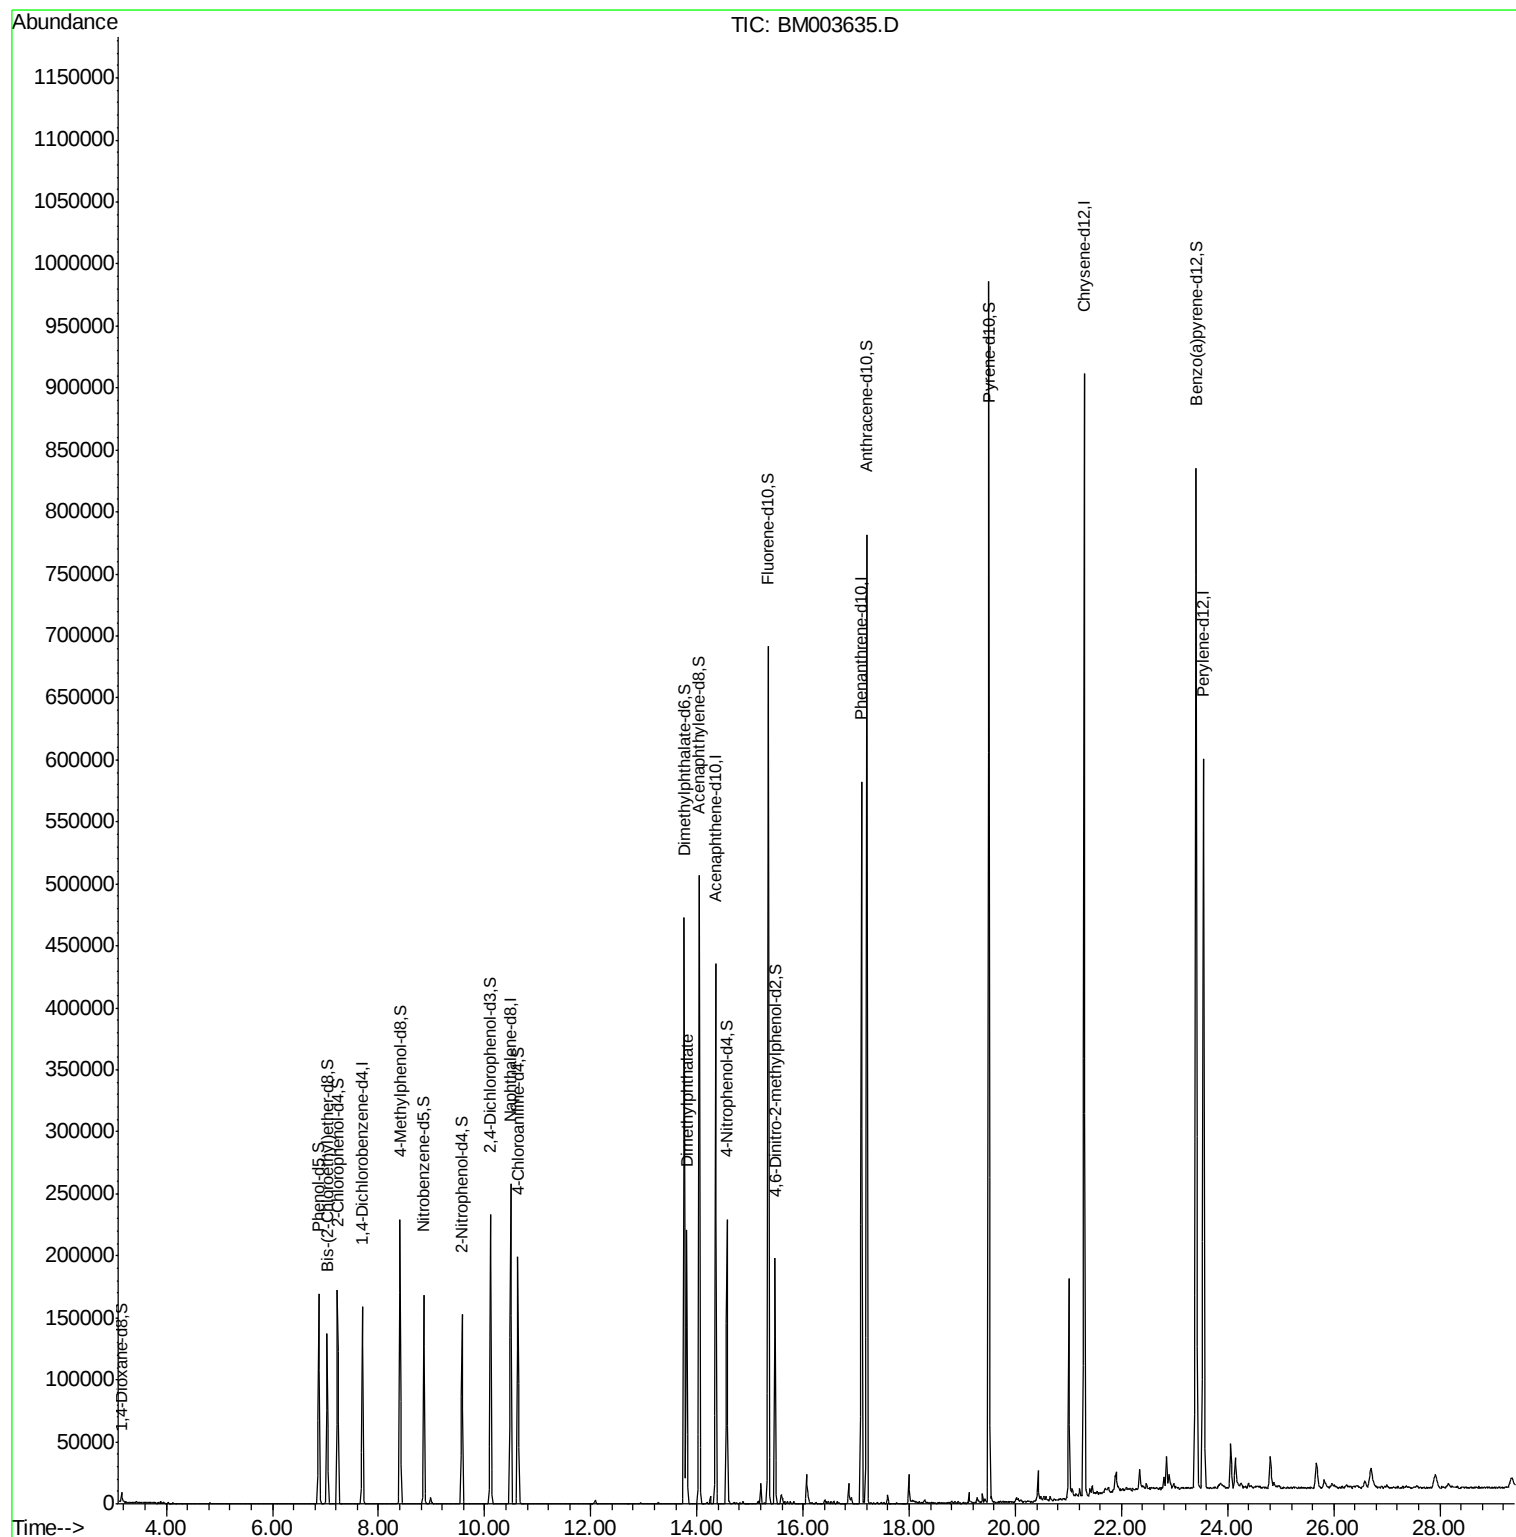

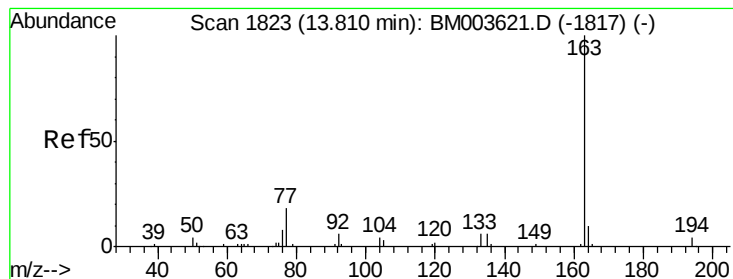

#45

Dimethylphthalate

Concen: 12.25 ng/ul

RT: 13.81 min Scan# 1823

Delta R.T. -0.00 min

Lab File: BM003635.D


Acq: 20 Dec 2015 00:17

Instrument :

BNA_M

ClientSampleId :

G9C76

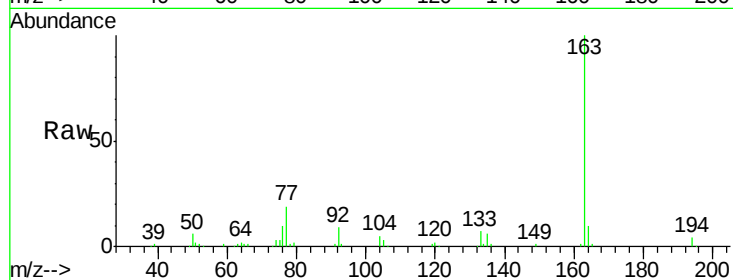


Tgt Ion:163 Resp: 147832

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 9.8 7.8 11.8

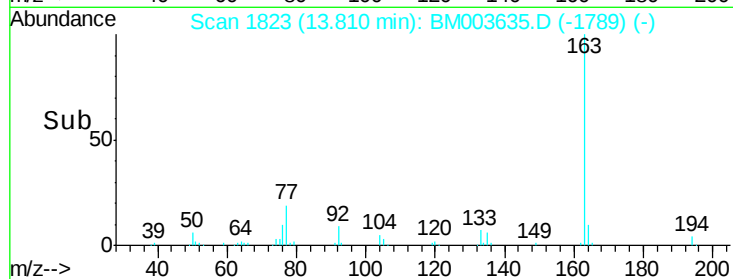

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

