

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121915\
 Data File : BM003634.D
 Acq On : 19 Dec 2015 23:42
 Operator : UM/SJ
 Sample : G4801-27
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9C75

Quant Time: Dec 20 01:42:20 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 20 01:33:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	39756	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	189230	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	117975	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	279168	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	339757	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	333597	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	3653	4.95	ng/uL	0.00
5) Phenol-d5	6.87	99	83177	24.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	48061	26.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	72111	26.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	72529	24.99	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	36841	26.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	41867	27.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	71774	25.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	87678	23.36	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	262093	26.88	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	303335	27.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	45495	23.95	ng/ul	0.00
58) Fluorene-d10	15.34	176	221612	27.47	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	32312	20.54	ng/ul	0.00
71) Anthracene-d10	17.20	188	351431	27.67	ng/ul	0.00
79) Pyrene-d10	19.50	212	418839	28.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	473534	28.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.81	163	186905	18.74	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121915\
Data File : BM003634.D
Acq On : 19 Dec 2015 23:42
Operator : UM/SJ
Sample : G4801-27
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9C75

Quant Time: Dec 20 01:42:20 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 20 01:33:56 2015
Response via : Initial Calibration

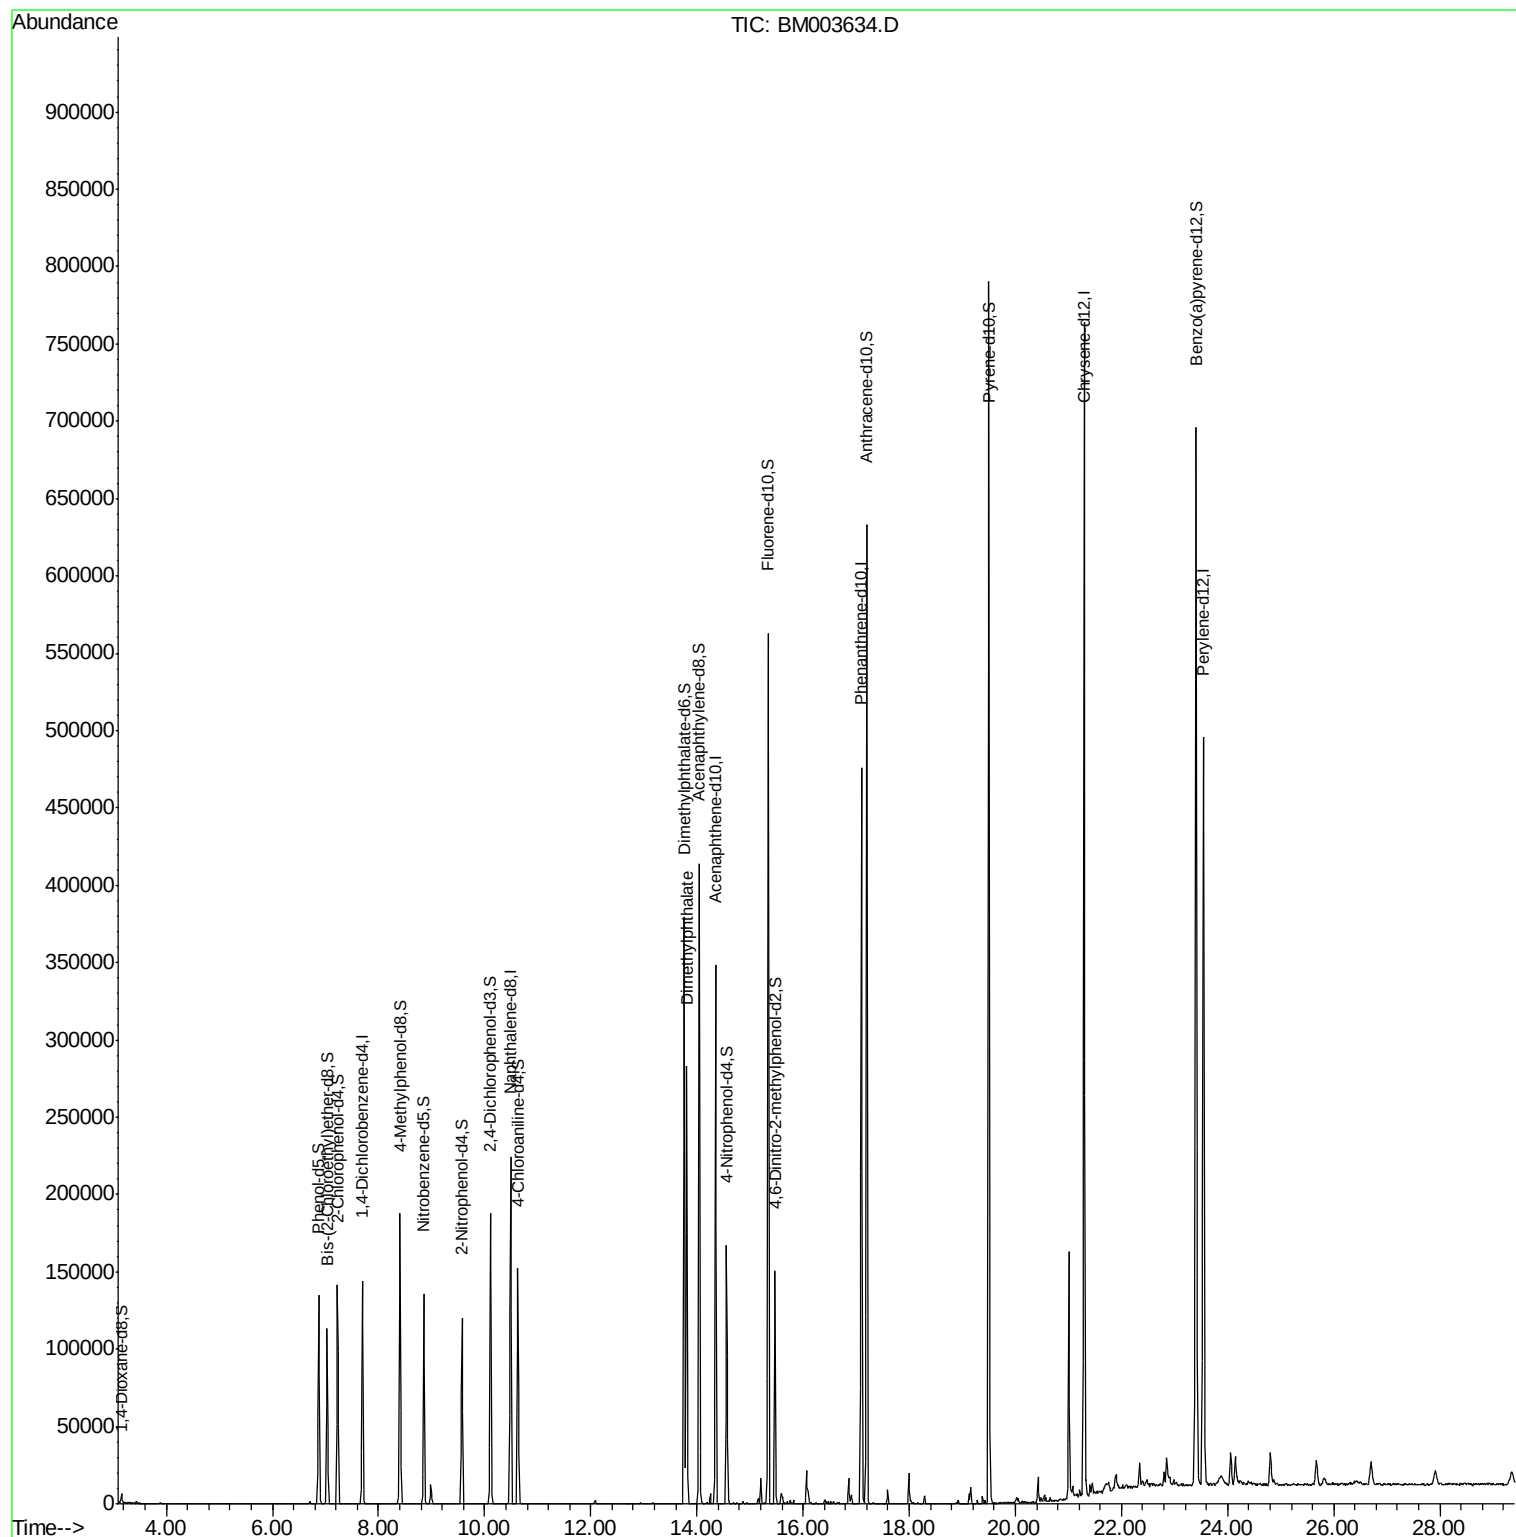

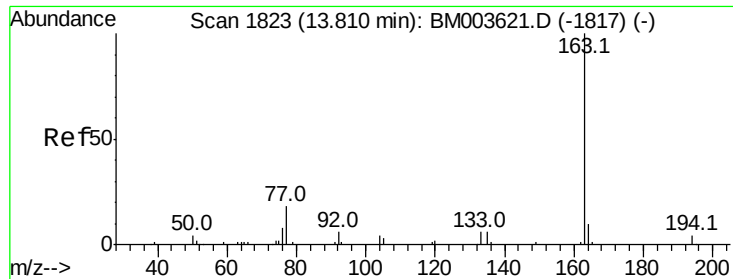

#45

Dimethylphthalate

Concen: 18.74 ng/ul

RT: 13.81 min Scan# 1823

Delta R.T. -0.00 min

Lab File: BM003634.D

Acq: 19 Dec 2015 23:42

Instrument :

BNA_M

ClientSampleId :

G9C75


Tot Ion:163 Resp: 186905

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.7 7.8 11.8

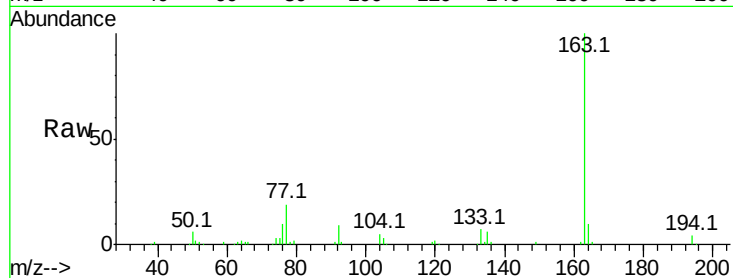

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

