

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121915\
 Data File : BM003637.D
 Acq On : 20 Dec 2015 01:29
 Operator : UM/SJ
 Sample : G4801-30
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9C78

Quant Time: Dec 20 02:53:50 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 20 01:33:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	35038	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	171826	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	110376	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	264409	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	338391	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	347395	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	3648	5.61	ng/uL	0.00
5) Phenol-d5	6.87	99	84473	28.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	49010	31.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	73020	30.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	75289	29.44	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	38148	30.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	42598	30.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	72987	28.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	93191	27.34	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	273330	29.96	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	318621	30.68	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	49548	27.88	ng/ul	0.00
58) Fluorene-d10	15.34	176	230992	30.61	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	36184	24.28	ng/ul	0.00
71) Anthracene-d10	17.20	188	373125	31.02	ng/ul	0.00
79) Pyrene-d10	19.50	212	452623	30.62	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	550349	31.89	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.81	163	159563	17.10	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121915\
Data File : BM003637.D
Acq On : 20 Dec 2015 01:29
Operator : UM/SJ
Sample : G4801-30
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9C78

Quant Time: Dec 20 02:53:50 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 20 01:33:56 2015
Response via : Initial Calibration

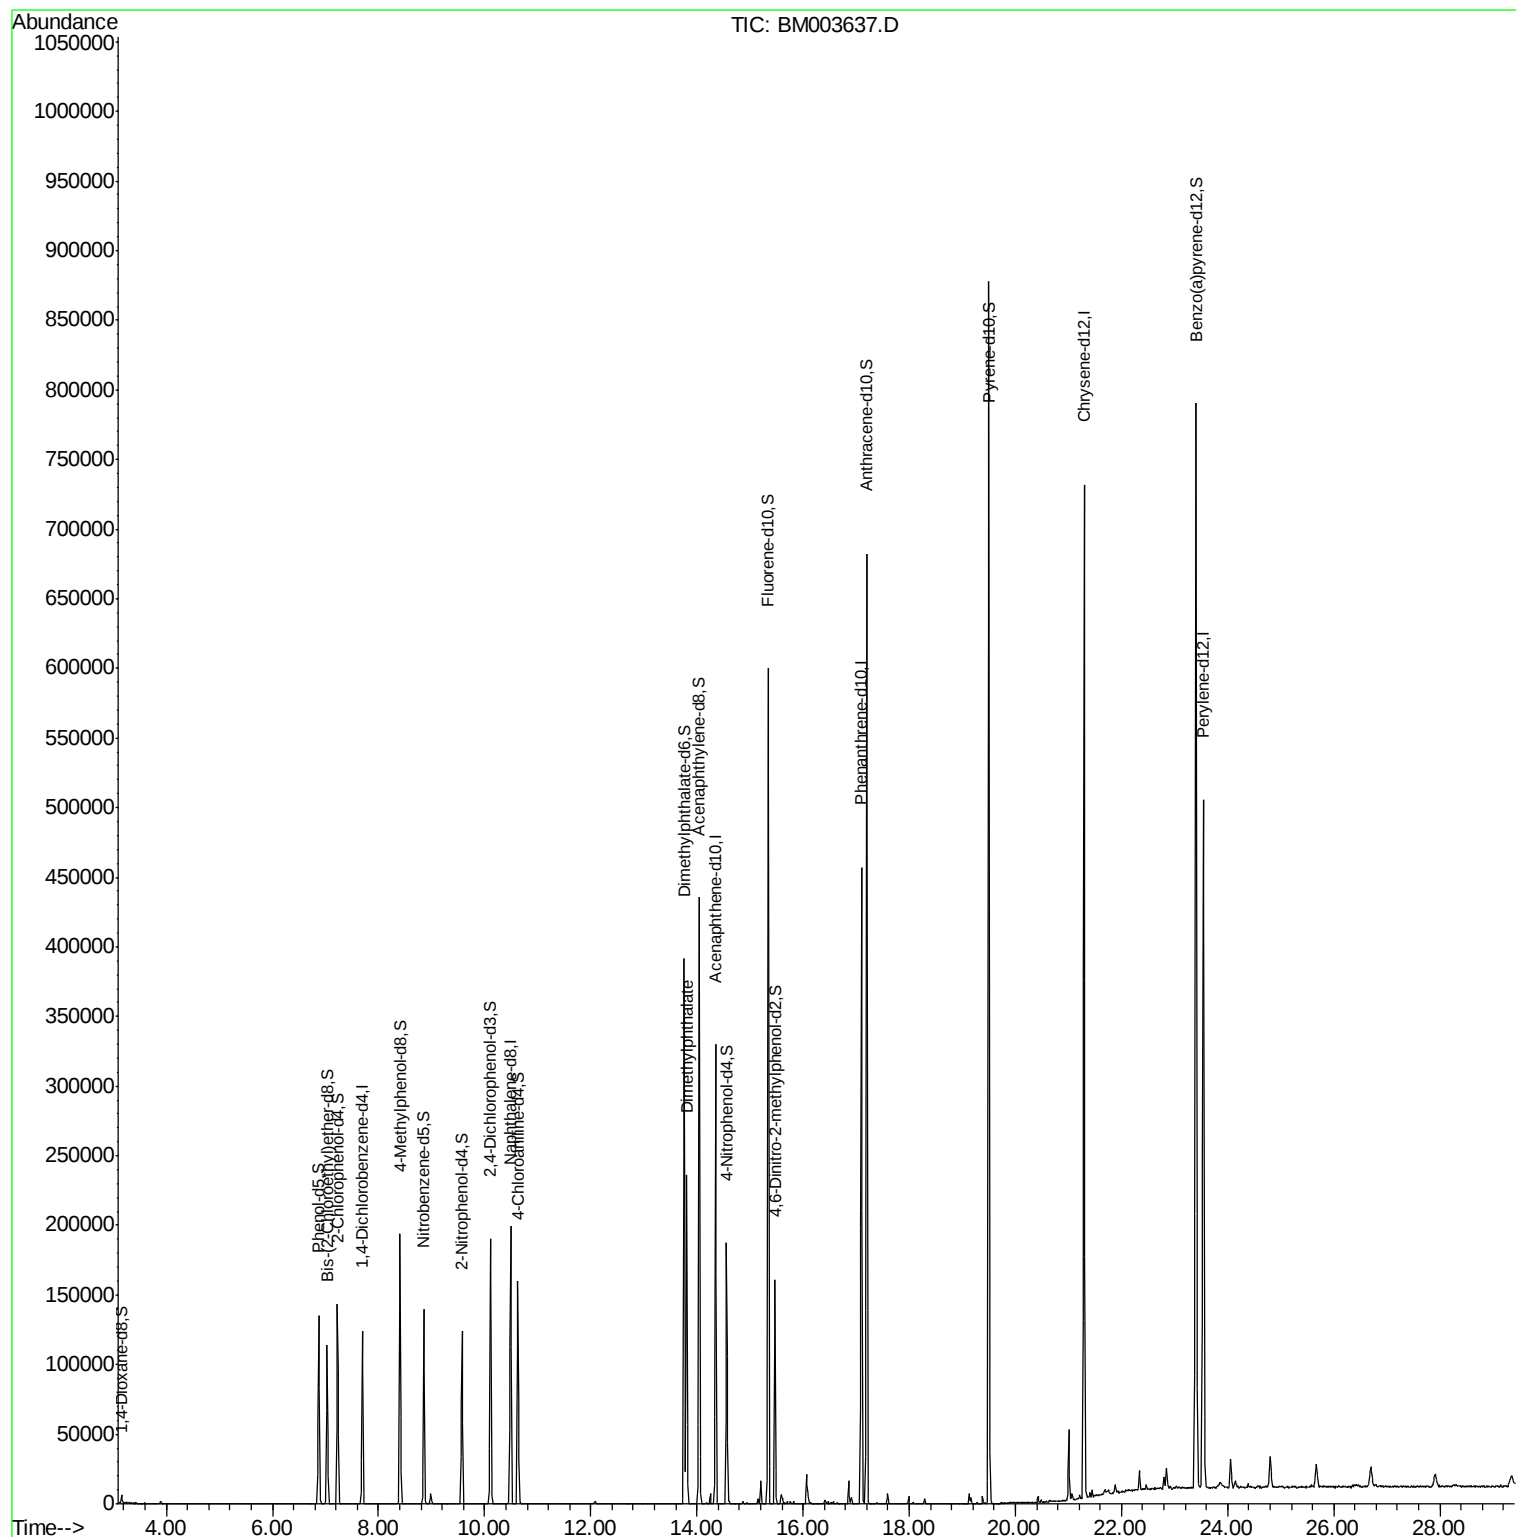

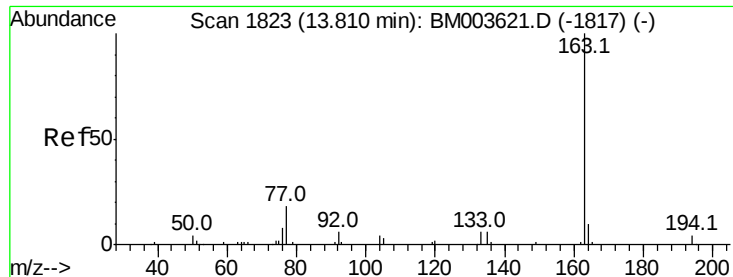

#45

Dimethylphthalate

Concen: 17.10 ng/ul

RT: 13.81 min Scan# 1823

Delta R.T. -0.00 min

Lab File: BM003637.D

Acq: 20 Dec 2015 01:29

Instrument :

BNA_M

ClientSampleId :

G9C78


Tot Ion:163 Resp: 159563

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 9.6 7.8 11.8

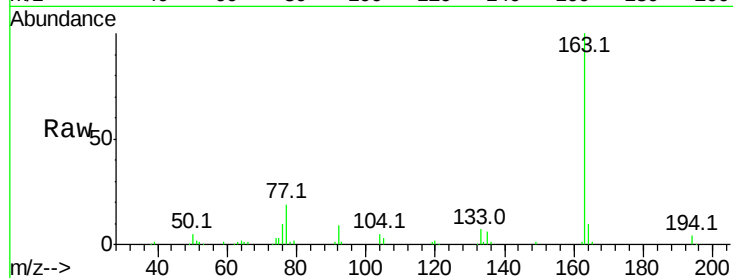

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

