

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121915\
 Data File : BM003622.D
 Acq On : 19 Dec 2015 16:33
 Operator : UM/SJ
 Sample : PB87324BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.157	8	12	19	rVB	6839	9243	0.56%	0.075%
2	6.869	638	643	651	rBB	139106	216853	13.12%	1.757%
3	7.034	665	671	679	rBB	124890	186555	11.28%	1.511%
4	7.234	699	705	712	rBB	147076	235231	14.23%	1.906%
5	7.698	778	784	790	rBB	99610	151358	9.15%	1.226%
6	8.410	899	905	912	rBB	195936	309661	18.73%	2.508%
7	8.857	974	981	988	rBB	148051	237764	14.38%	1.926%
8	9.575	1097	1103	1110	rBB	131741	208153	12.59%	1.686%
9	10.110	1188	1194	1202	rBB	199589	315796	19.10%	2.558%
10	10.486	1252	1258	1265	rBB	175055	283147	17.13%	2.294%
11	10.628	1275	1282	1293	rBB	178376	292478	17.69%	2.369%
12	12.080	1526	1529	1533	rBB	2380	3257	0.20%	0.026%
13	13.763	1809	1815	1822	rBB	453299	616587	37.29%	4.995%
14	14.045	1856	1863	1874	rBB	447860	670423	40.55%	5.431%
15	14.186	1882	1887	1892	rBV	3510	5902	0.36%	0.048%
16	14.351	1909	1915	1922	rBB2	312022	467903	28.30%	3.790%
17	14.563	1945	1951	1962	rBB	216289	299388	18.11%	2.425%
18	15.345	2078	2084	2091	rBB	615949	879031	53.16%	7.121%
19	15.474	2100	2106	2112	rBB	187555	257891	15.60%	2.089%
20	15.586	2122	2125	2128	rBB	4019	4808	0.29%	0.039%
21	17.098	2376	2382	2389	rBB2	439155	619799	37.49%	5.021%
22	17.198	2393	2399	2411	rBB2	724200	1019054	61.63%	8.255%
23	19.133	2724	2728	2732	rBV	7247	8779	0.53%	0.071%
24	19.386	2768	2771	2776	rBV	5082	6283	0.38%	0.051%
25	19.503	2784	2791	2801	rVB	922531	1265778	76.56%	10.254%
26	20.427	2946	2948	2952	rVB	1851	1782	0.11%	0.014%
27	20.974	3037	3041	3046	rVV2	2294	2822	0.17%	0.023%
28	21.027	3046	3050	3055	rVV2	2747	3981	0.24%	0.032%
29	21.080	3055	3059	3064	rVV	6518	8862	0.54%	0.072%
30	21.215	3076	3082	3086	rBV3	2886	4288	0.26%	0.035%
31	21.303	3091	3097	3102	rVV	710910	923927	55.88%	7.485%
32	21.339	3102	3103	3109	rVB	7082	6158	0.37%	0.050%
33	21.450	3120	3122	3124	rBV	2635	2256	0.14%	0.018%
34	21.886	3193	3196	3200	rVB2	4099	4207	0.25%	0.034%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121915\
Data File : BM003622.D
Acq On : 19 Dec 2015 16:33
Operator : UM/SJ
Sample : PB87324BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK24

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Title : SVOA CALIBRATION

35	22.350	3270	3275	3279	rBV2	11688	16114	0.97%	0.131%
36	22.809	3349	3353	3357	rBV	9102	12612	0.76%	0.102%
37	22.856	3357	3361	3368	rVB2	13523	19688	1.19%	0.159%
38	23.409	3447	3455	3466	rBV	882936	1653404	100.00%	13.394%
39	23.550	3471	3479	3492	rVB2	531069	983751	59.50%	7.969%
40	24.062	3561	3566	3572	rVB	18512	33776	2.04%	0.274%
41	24.809	3688	3693	3700	rVB2	20562	43366	2.62%	0.351%
42	25.685	3836	3842	3853	rVB4	14468	36361	2.20%	0.295%
43	26.703	4009	4015	4016	rBV4	9742	16047	0.97%	0.130%


Sum of corrected areas: 12344524

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121915\
Data File : BM003622.D
Acq On : 19 Dec 2015 16:33
Operator : UM/SJ
Sample : PB87324BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK24

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

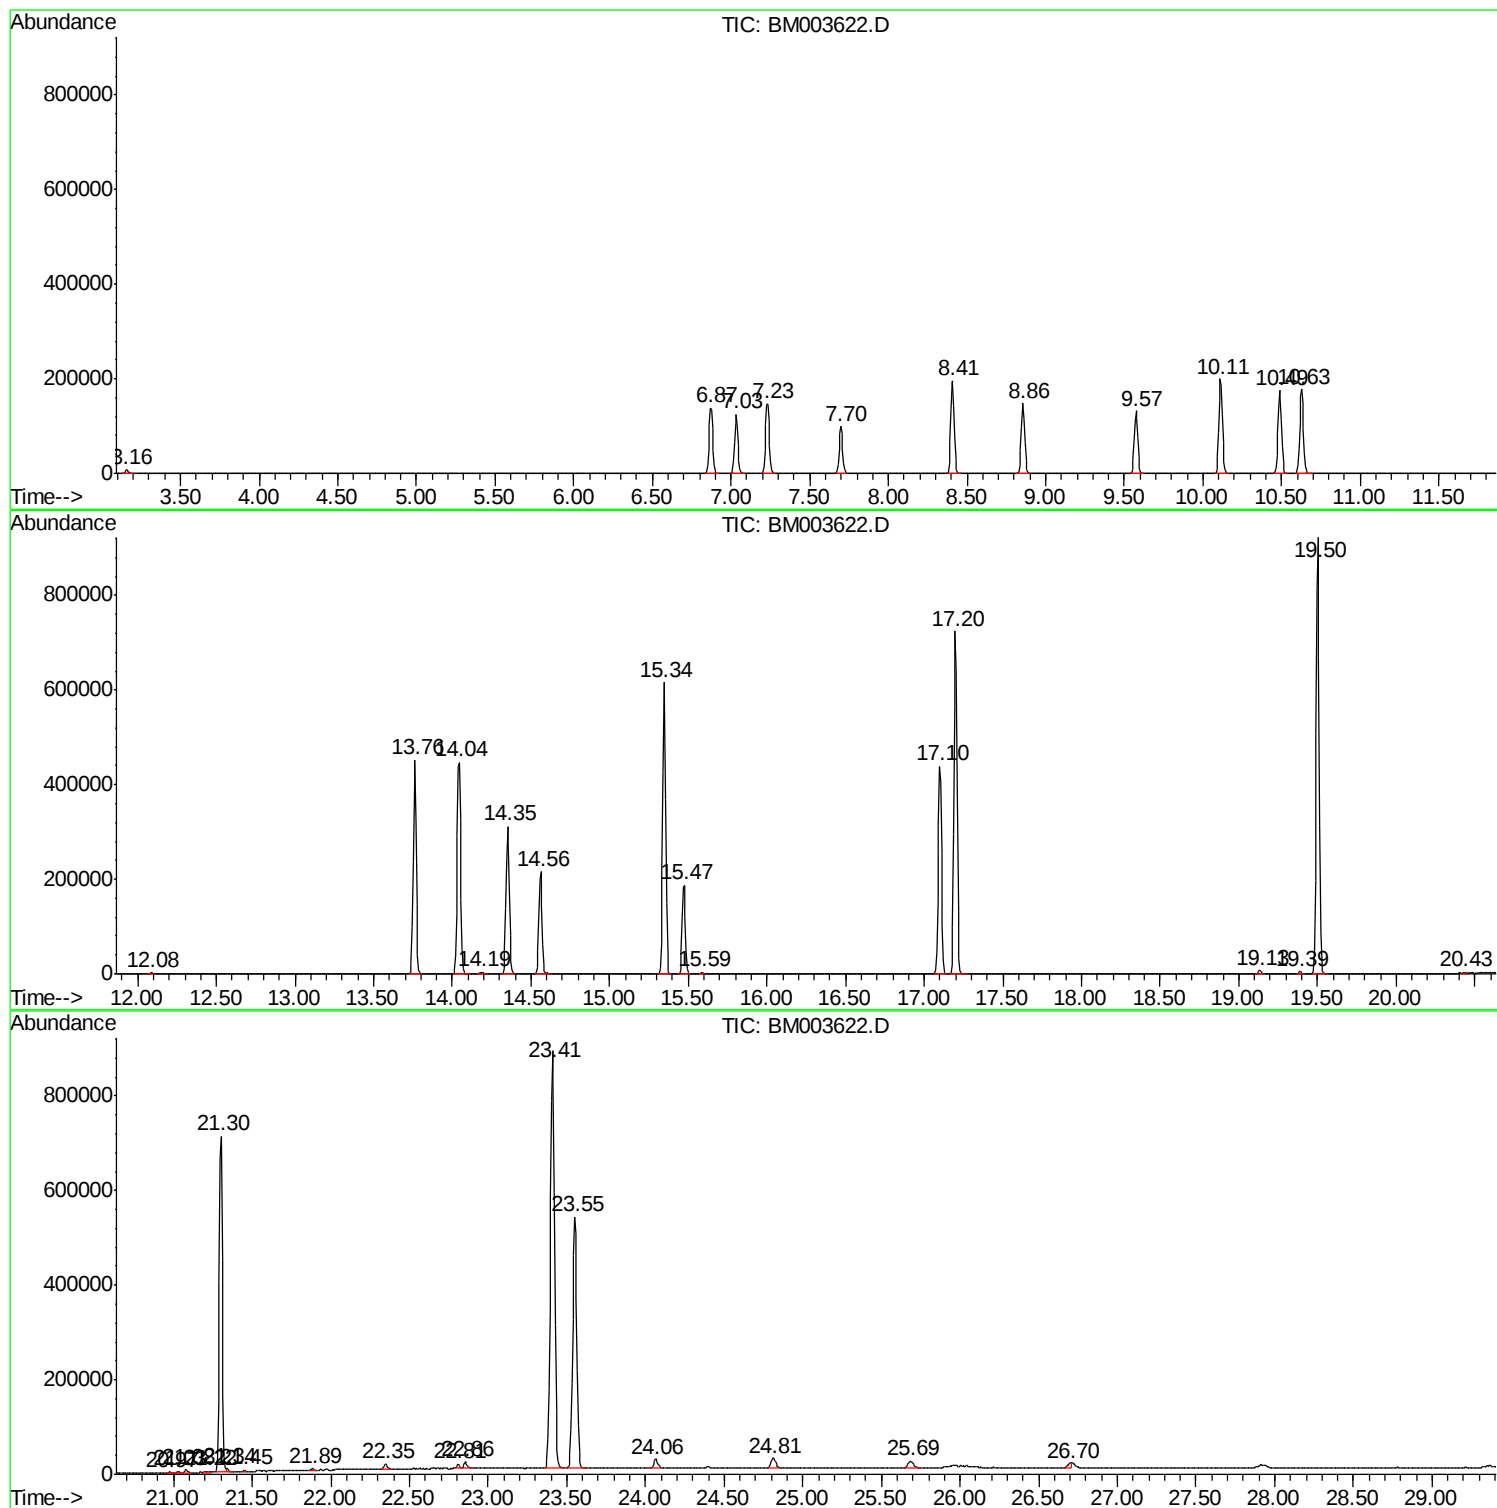

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121915\
Data File : BM003622.D
Acq On : 19 Dec 2015 16:33
Operator : UM/SJ
Sample : PB87324BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK24

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121915\
Data File : BM003622.D
Acq On : 19 Dec 2015 16:33
Operator : UM/SJ
Sample : PB87324BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK24

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc