


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121915\
 Data File : BM003614.D
 Acq On : 19 Dec 2015 11:46
 Operator : UM/SJ
 Sample : DFTPP60
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP60

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
 Title : SVOA CALIBRATION
 Last Update : Mon Dec 21 16:14:53 2015

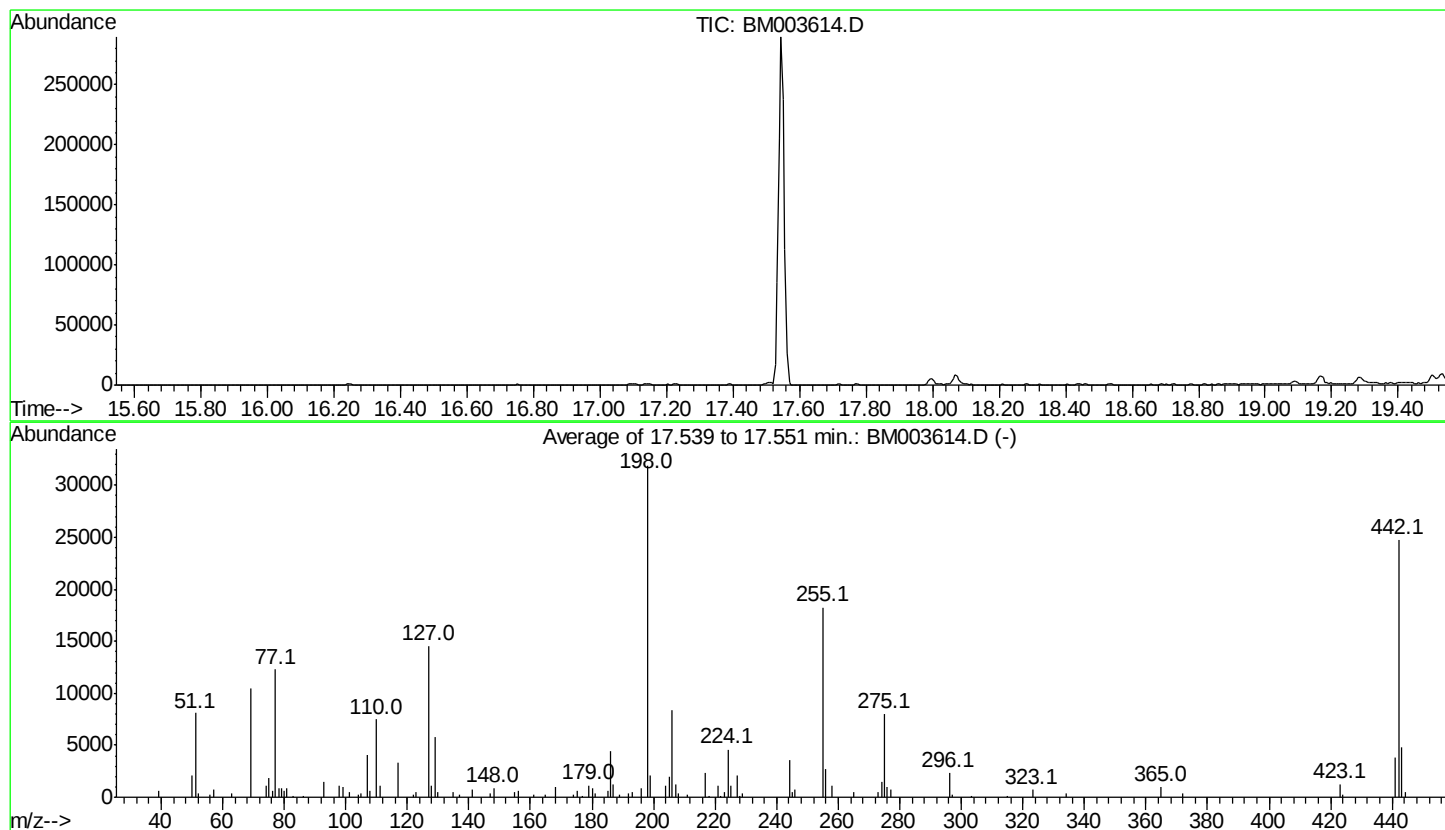

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	8080	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.6	10411	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.7	14577	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31893	PASS
199	198	5	9	6.8	2155	PASS
275	198	10	60	25.1	8005	PASS
365	198	1	100	3.2	1014	PASS
441	443	0.01	100	78.6	3785	PASS
442	198	50	100	77.8	24806	PASS
443	442	15	24	19.4	4815	PASS

Scan 2452 (17.509 min): BM003614.D
DFTPP60

m/z	Abundance
166.10	415.0
167.10	1858.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.10	657.0
50.10	2037.0
51.10	8029.0
52.00	434.0
56.00	303.0
57.00	673.0
63.00	368.0
69.00	10273.0
74.10	1016.0
75.00	1722.0
76.00	553.0
77.10	11672.0
78.10	840.0
79.00	768.0
80.00	618.0
81.00	841.0
93.00	1381.0
98.00	1012.0
99.00	968.0
101.00	465.0
104.00	343.0
105.00	308.0
107.00	3954.0
108.00	631.0
110.00	6940.0
111.00	1103.0
117.00	3136.0
122.00	323.0
123.00	448.0
127.00	12997.0
128.00	1061.0
129.00	5218.0
130.00	429.0
135.00	459.0
137.00	301.0
140.90	638.0
147.00	344.0
148.00	776.0
155.00	394.0
156.00	500.0
167.10	1560.0
168.00	978.0
175.00	496.0
179.00	1030.0
180.00	769.0
181.00	328.0
185.00	546.0
186.10	3801.0
187.00	1043.0
192.00	382.0
193.00	363.0
196.10	654.0
198.00	27440.0
199.00	2027.0
204.00	941.0
205.00	1723.0
206.10	7206.0
207.00	1010.0
208.00	341.0
217.00	1889.0
221.00	971.0
223.00	428.0
224.10	3827.0
225.00	938.0
227.00	1726.0
229.00	300.0
244.10	2849.0
245.10	401.0
246.00	536.0
255.10	14397.0
256.10	2183.0
258.00	851.0
265.00	382.0
273.00	437.0
274.00	1168.0
275.10	6498.0
276.10	776.0
277.00	615.0
296.10	1778.0
323.00	611.0
365.00	752.0
372.10	323.0
423.10	941.0
441.10	2456.0
442.10	16220.0
443.10	3325.0
444.10	332.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.10	815.0
50.10	2361.0
51.10	9248.0
52.10	470.0
55.90	353.0
57.00	792.0
63.00	436.0
69.00	12254.0
74.00	1225.0
75.00	2052.0
76.00	716.0
77.10	14518.0
78.10	950.0
79.00	1024.0
80.00	761.0
81.00	1071.0
83.00	314.0
86.00	398.0
93.00	1636.0
98.00	1364.0
99.00	1117.0
101.00	680.0
104.00	465.0
105.00	406.0
107.00	4707.0
108.00	776.0
110.00	8765.0
111.00	1376.0
117.00	4000.0
122.00	339.0
123.00	489.0
127.00	17232.0
128.00	1258.0
129.00	6713.0
130.00	592.0
135.00	559.0
137.00	355.0
140.90	924.0
147.00	507.0
148.00	1089.0
155.00	509.0
156.00	733.0
161.00	430.0
165.00	404.0
166.10	324.0
167.00	2000.0
168.00	1089.0
174.00	402.0
175.00	756.0
177.00	308.0
179.00	1434.0
180.00	1002.0
181.00	469.0
185.00	680.0
186.10	5362.0
187.00	1564.0
189.00	340.0
192.00	423.0
193.00	569.0
196.00	989.0
198.00	37544.0
199.00	2526.0
204.00	1430.0
205.00	2231.0
206.10	9643.0
207.10	1515.0
208.00	328.0
211.00	384.0
217.00	2807.0
218.00	345.0
221.10	1381.0
221.70	348.0
223.00	643.0
224.10	5343.0
225.10	1389.0
227.00	2388.0
228.00	339.0
229.00	499.0
244.10	4186.0
245.10	496.0
246.00	960.0
255.10	21416.0
256.00	3100.0
258.00	1283.0
265.00	530.0
273.00	584.0
274.00	1740.0
275.10	9292.0
276.00	1293.0
277.00	914.0
296.10	2925.0
297.00	390.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

303.10	313.0
314.90	310.0
323.10	792.0
334.10	534.0
365.00	1206.0
372.10	412.0
423.10	1506.0
424.10	446.0
441.10	4269.0
442.10	28776.0
443.10	5619.0
444.10	518.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.00	557.0
50.00	1771.0
51.10	6963.0
52.00	382.0
57.00	581.0
63.00	318.0
69.00	8706.0
74.00	921.0
75.00	1606.0
76.10	562.0
77.10	10630.0
78.10	720.0
79.00	686.0
80.00	515.0
81.00	821.0
93.00	1285.0
98.00	1029.0
99.00	916.0
101.00	497.0
104.90	309.0
107.00	3487.0
108.00	545.0
110.00	6723.0
111.00	986.0
117.00	3019.0
123.00	484.0
127.00	13502.0
128.00	1053.0
129.00	5265.0
130.00	411.0
135.00	442.0
141.00	666.0
147.00	390.0
148.00	774.0
155.00	409.0
156.00	685.0
161.00	325.0
164.90	316.0
167.00	1626.0
168.00	816.0
174.00	314.0
175.00	615.0
179.00	1048.0
180.00	826.0
181.00	300.0
185.00	508.0
186.10	4250.0
187.00	1179.0
189.00	303.0
192.00	364.0
193.00	418.0
196.00	888.0
198.00	30696.0
199.00	1912.0
204.10	1147.0
205.00	2014.0
206.10	8417.0
207.10	1055.0
208.00	314.0
211.00	325.0
217.00	2252.0
221.10	1090.0
223.00	475.0
224.10	4585.0
225.00	1167.0
227.00	2034.0
229.10	329.0
244.10	3654.0
245.00	458.0
246.00	781.0
255.10	18896.0
256.10	2724.0
258.00	1047.0
265.00	488.0
273.00	564.0
274.00	1472.0
275.10	8225.0
276.00	1046.0
277.00	747.0
296.00	2347.0
297.00	360.0
323.10	776.0
334.10	523.0
365.00	1086.0
372.10	402.0
423.10	1351.0
424.10	407.0
441.10	4630.0
442.10	29424.0
443.10	5501.0
444.10	530.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60