


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:53:18 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

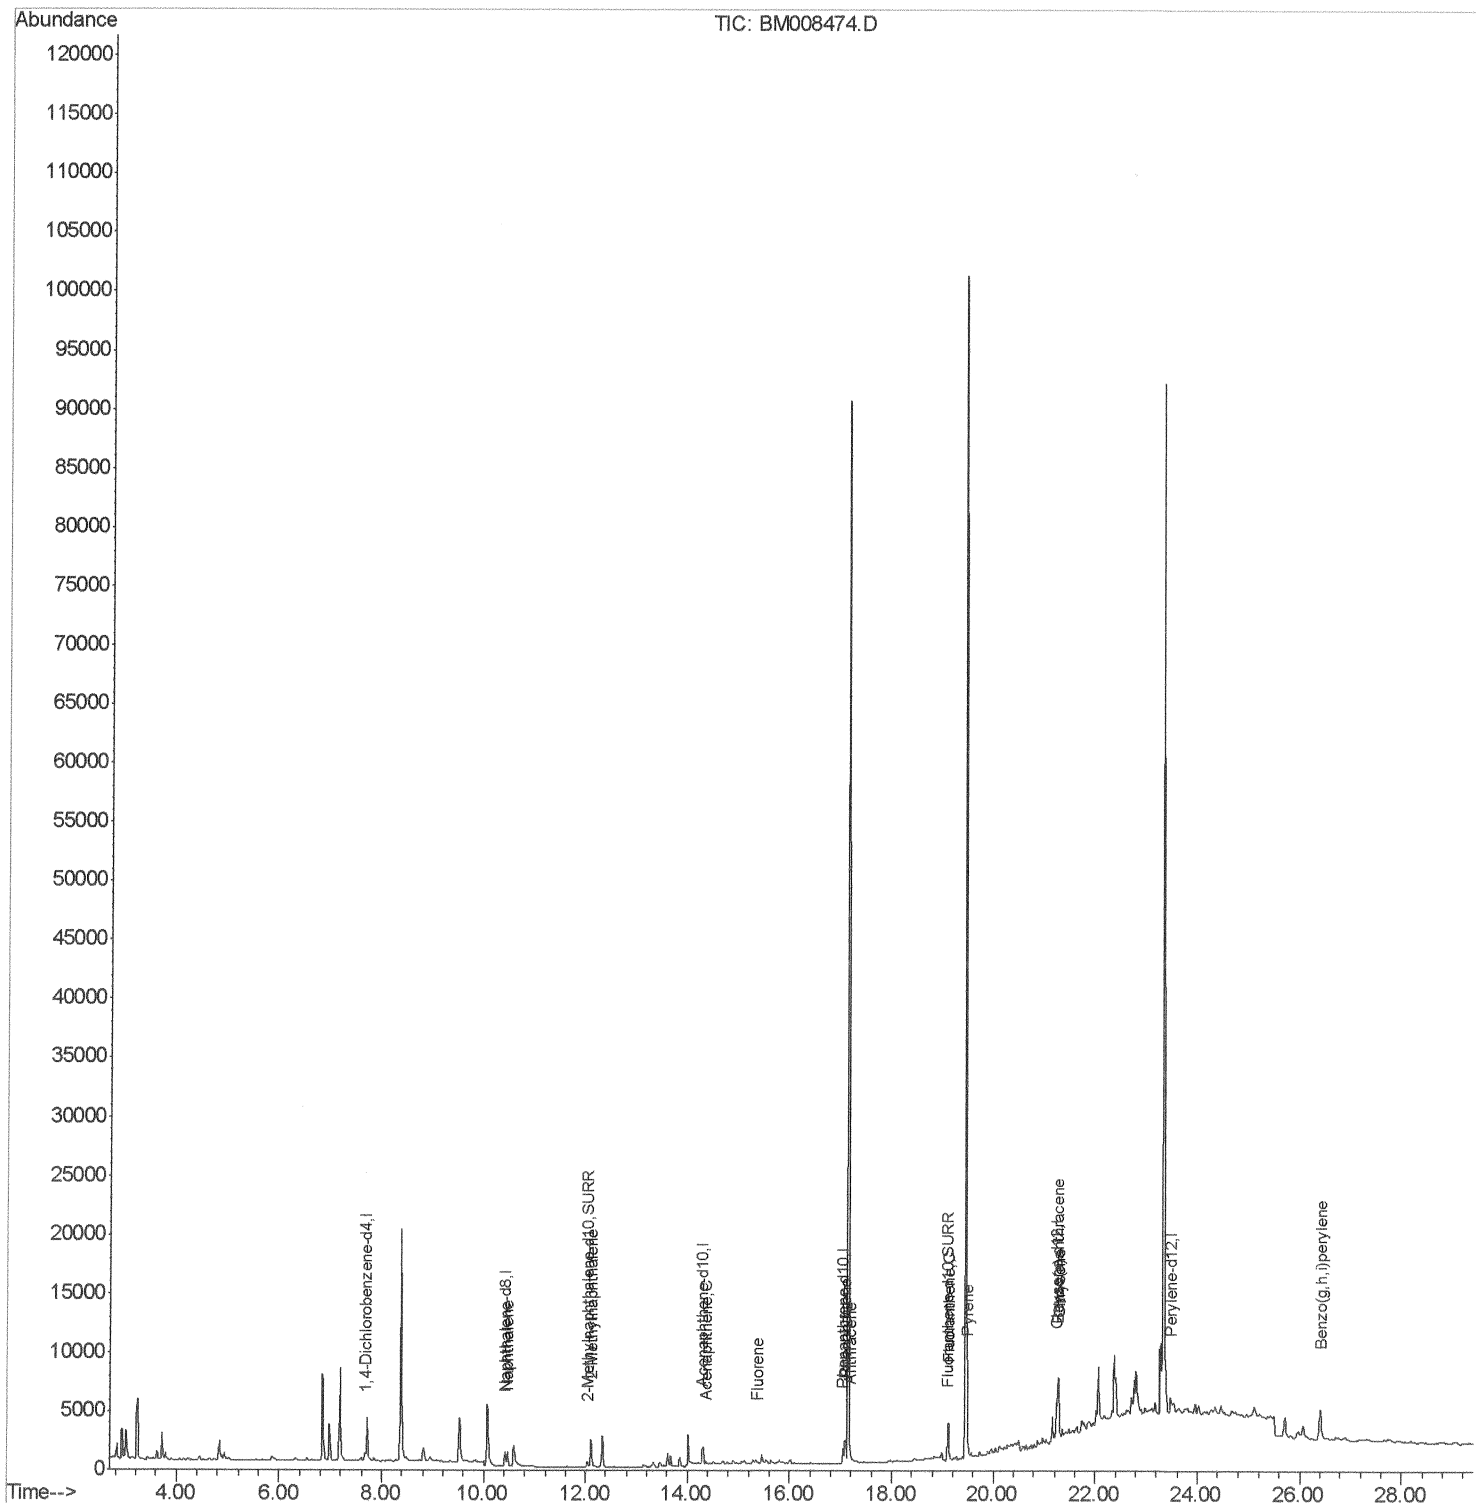




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:48:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

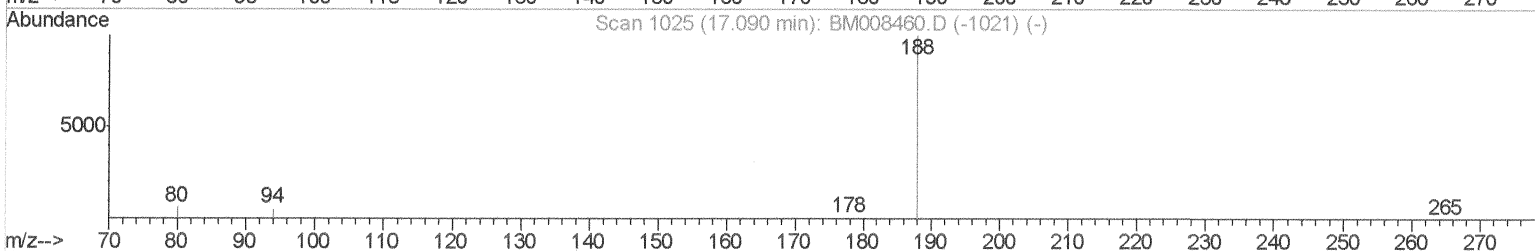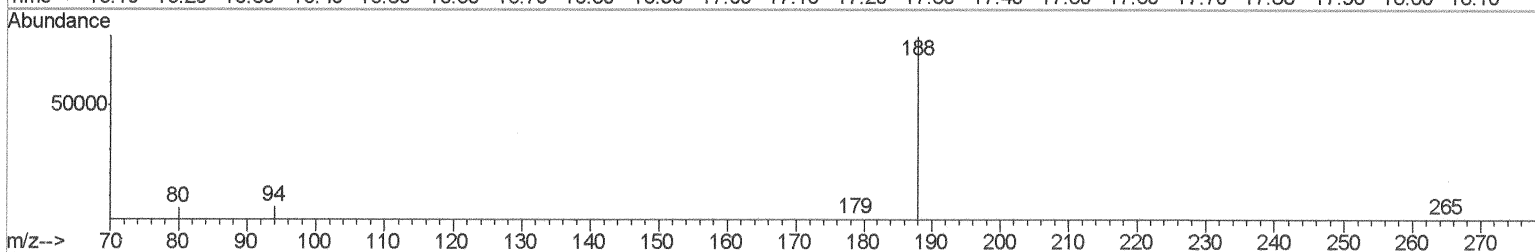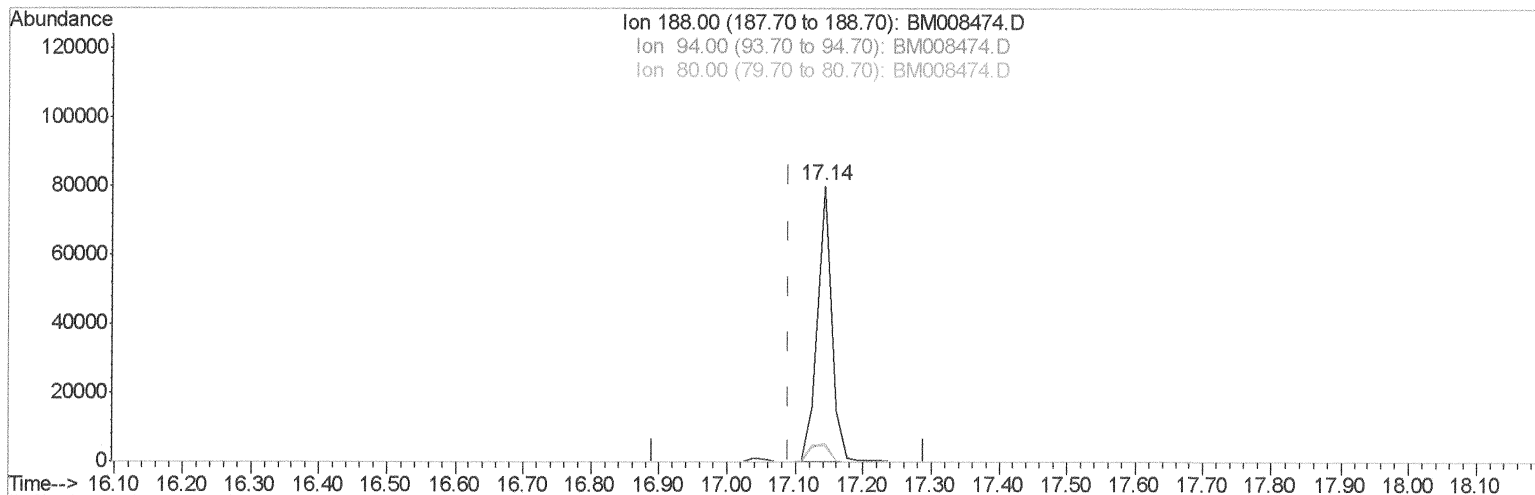

TIC: BM008474.D

(10) Phenanthrene-d10 (I)

17.142min (+0.052) 0.40ng/ul

response 115016

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.68#
80.00	11.80	5.96#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:48:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

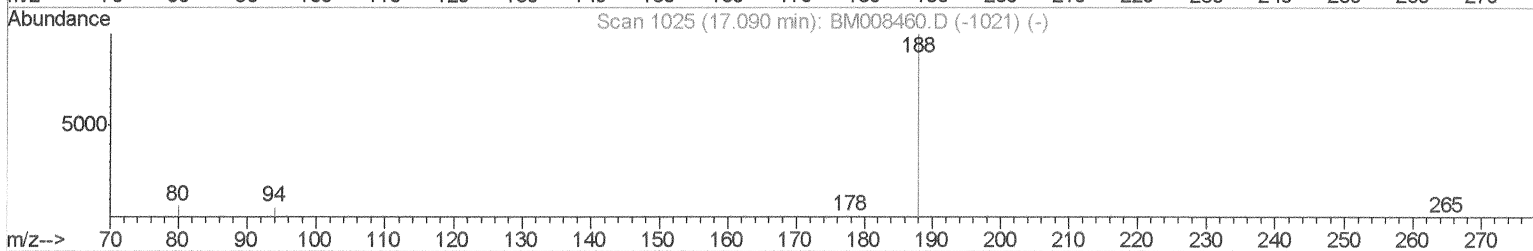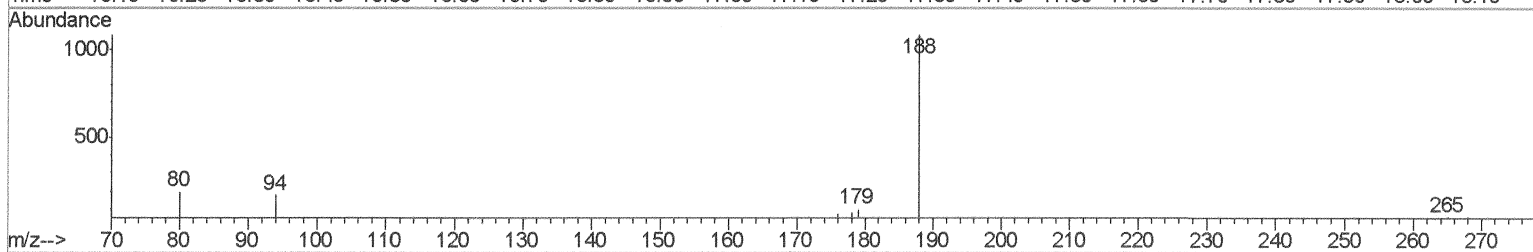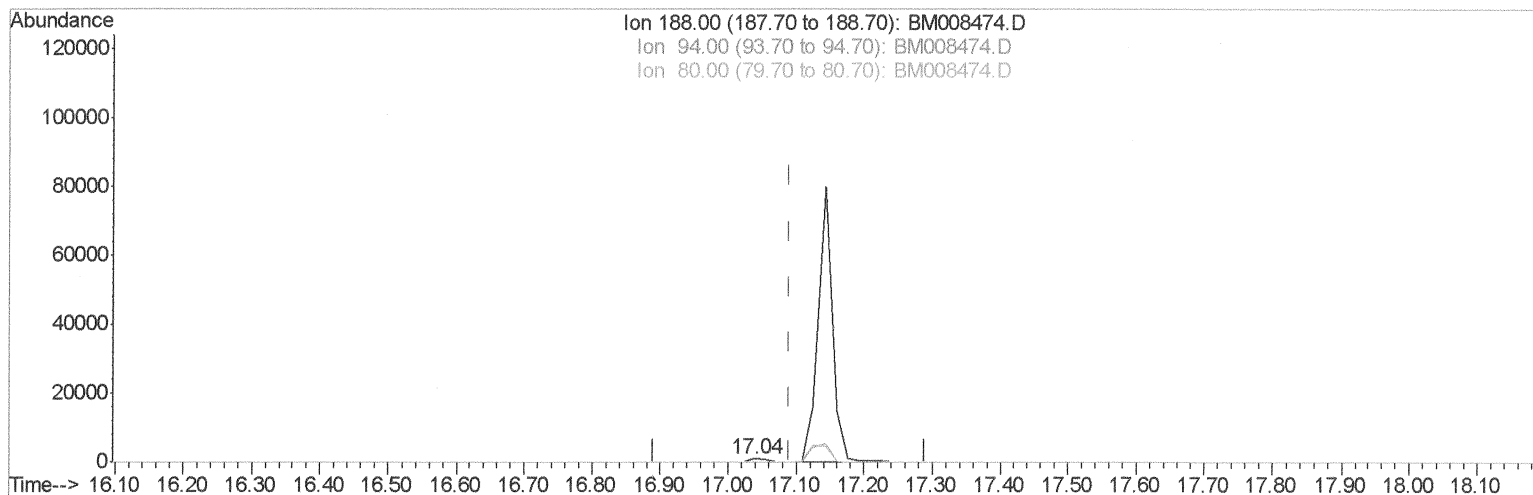

TIC: BM008474.D

(10) Phenanthrene-d10 (I)

17.039min (-0.051) 0.40ng/ul m

SJ 12/21/16

response 1757

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	16.16#
80.00	11.80	17.54#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:49:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

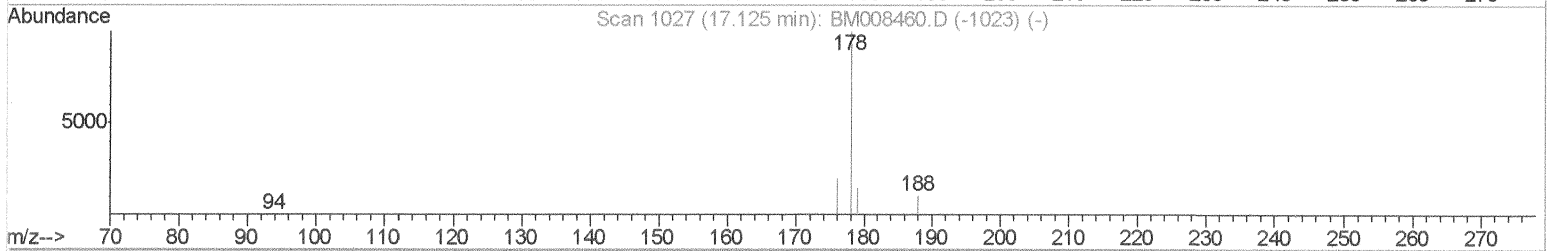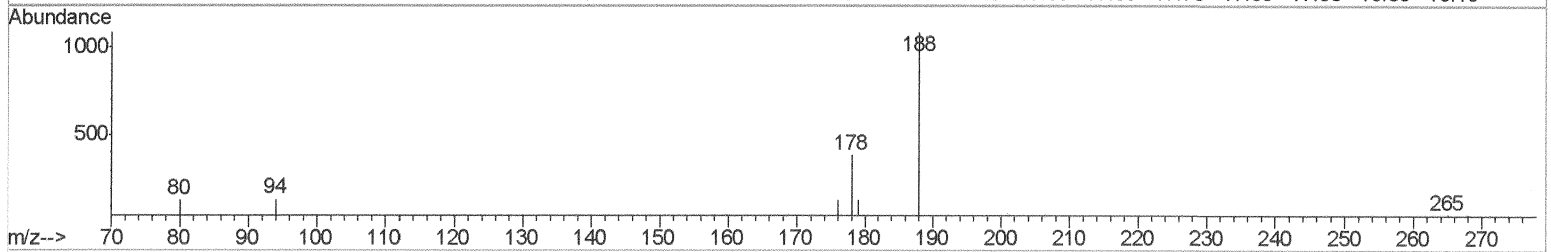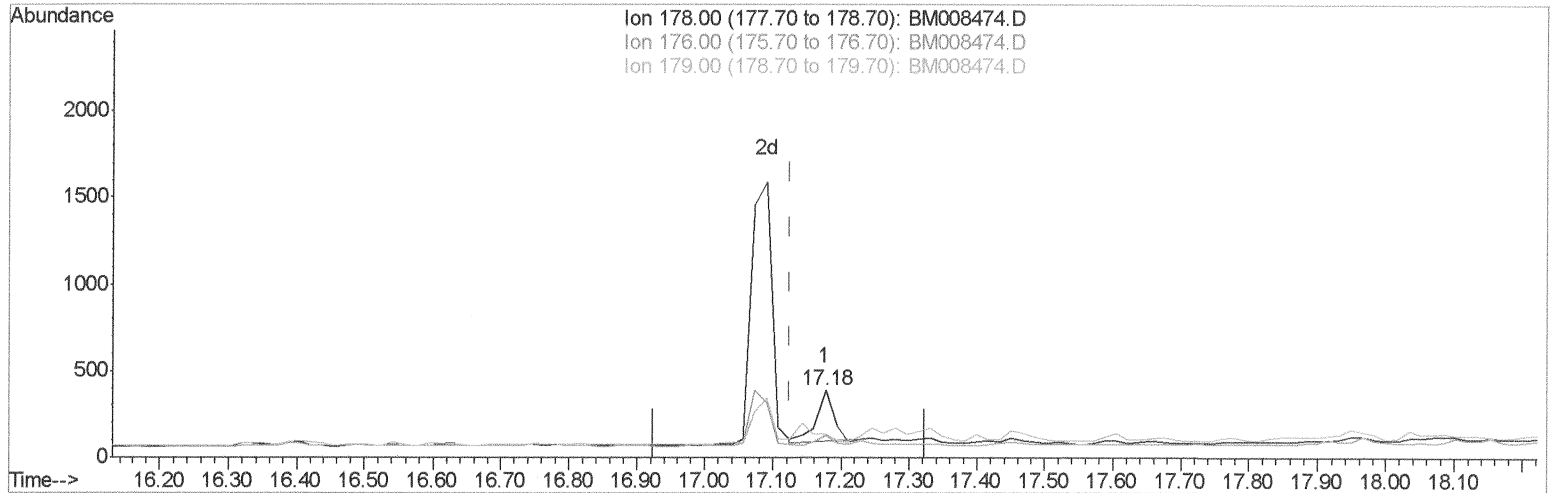

TIC: BM008474.D

(12) Phenanthrene

17.176min (+0.052) 0.09ng/ul

response 490

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	33.76#
179.00	17.00	34.79#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:49:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

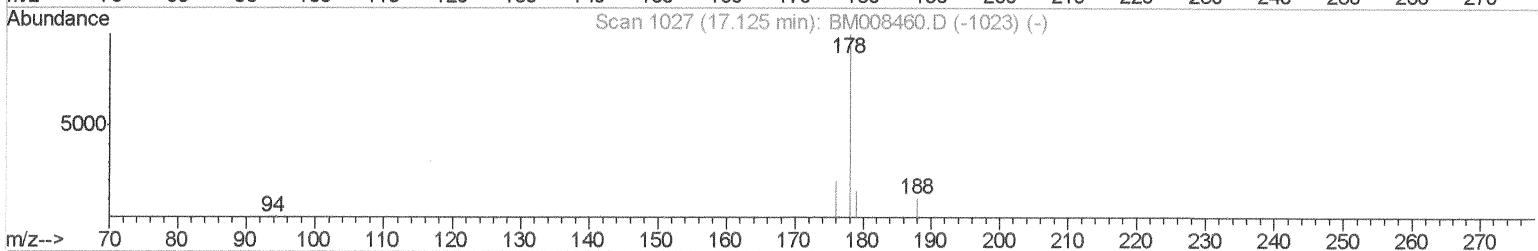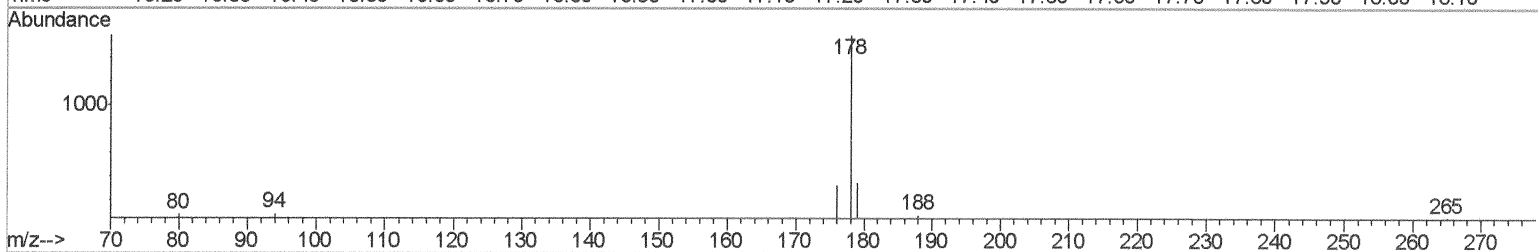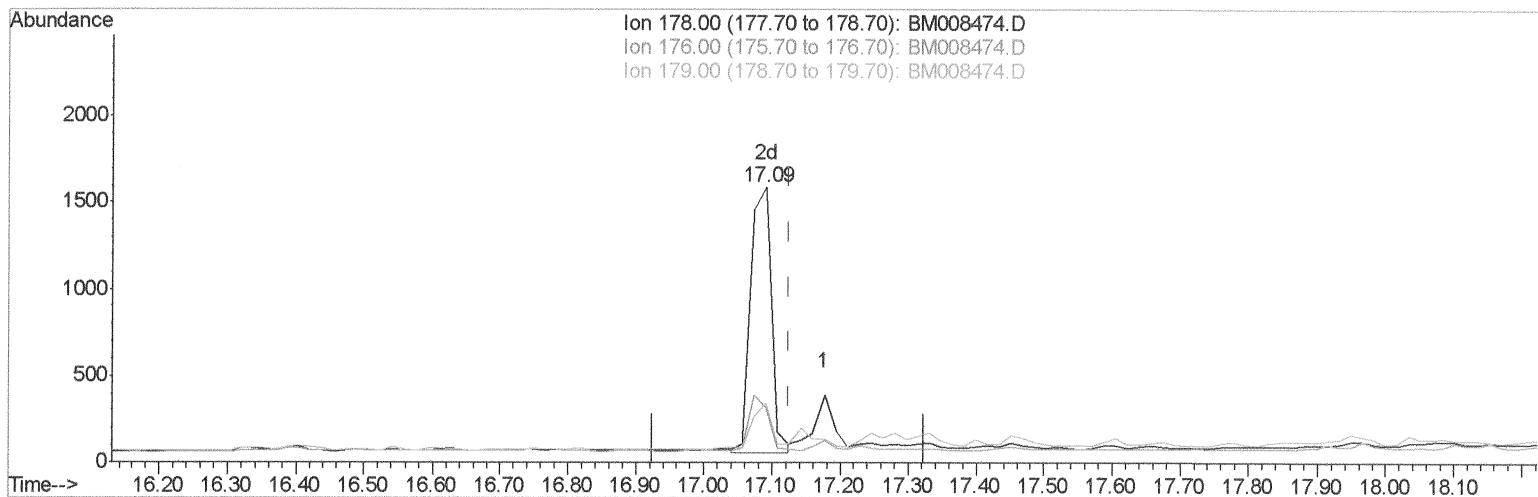

TIC: BM008474.D

(12) Phenanthrene

17.090min (-0.034) 0.60ng/ul m

SJ 12/21/16

response 3223

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	20.08
179.00	17.00	21.90#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:49:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

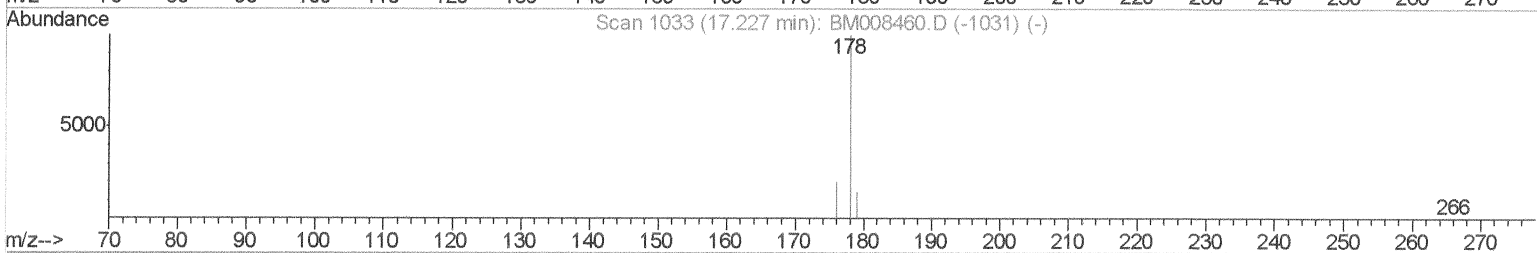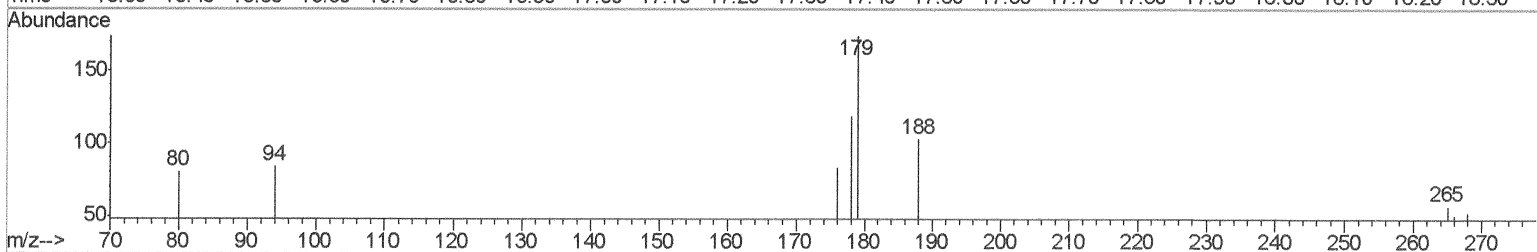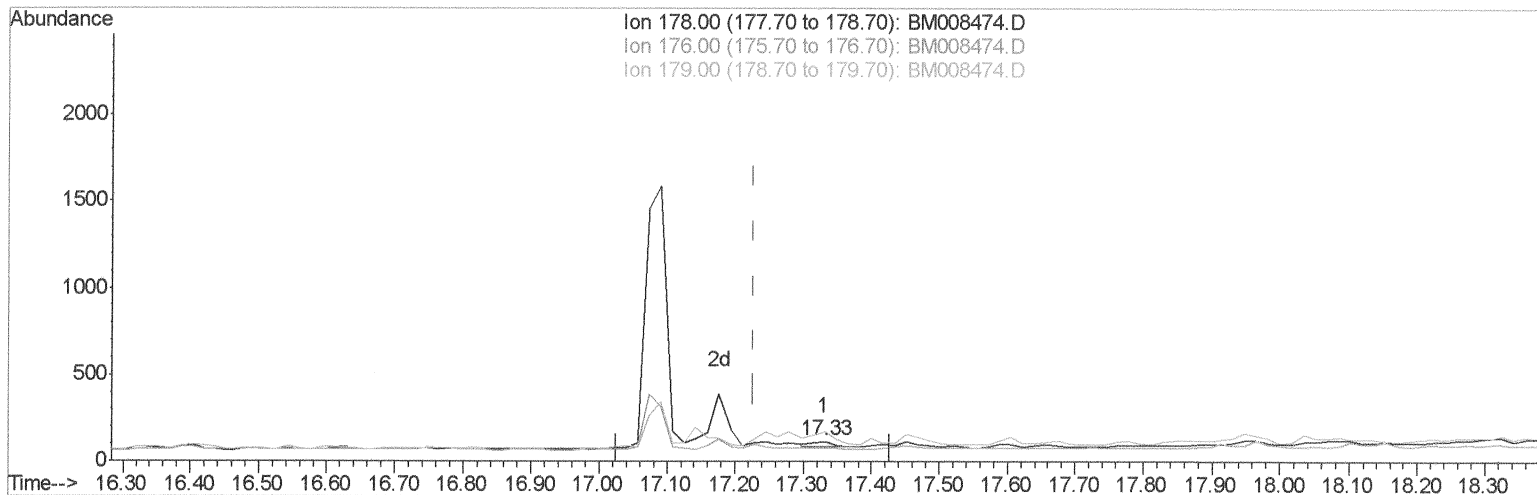

TIC: BM008474.D

(13) Anthracene

17.331min (+0.103) 0.01ng/ul

response 71

Ion	Exp%	Act%
178.00	100	100
176.00	22.60	69.75#
179.00	18.40	146.22#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:49:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

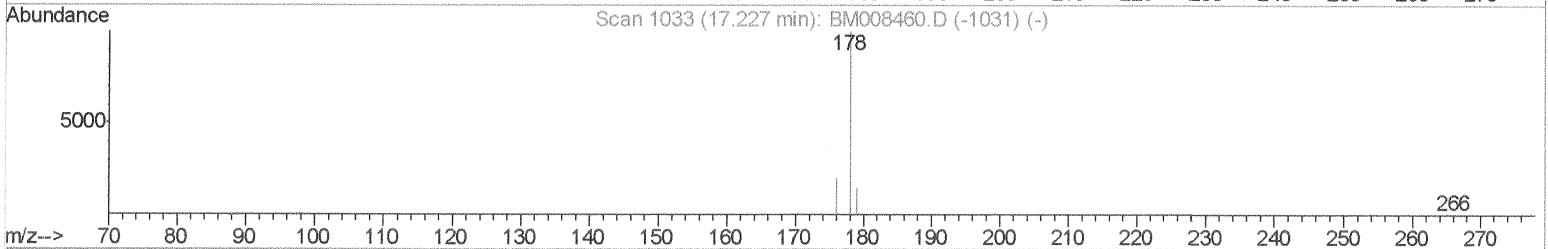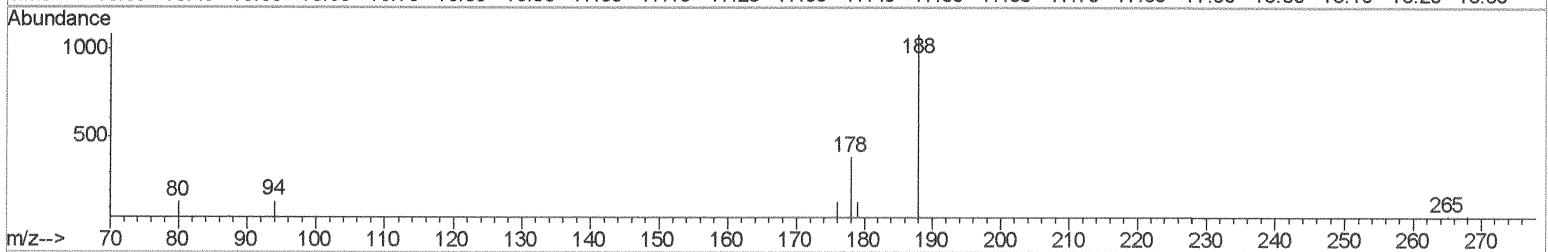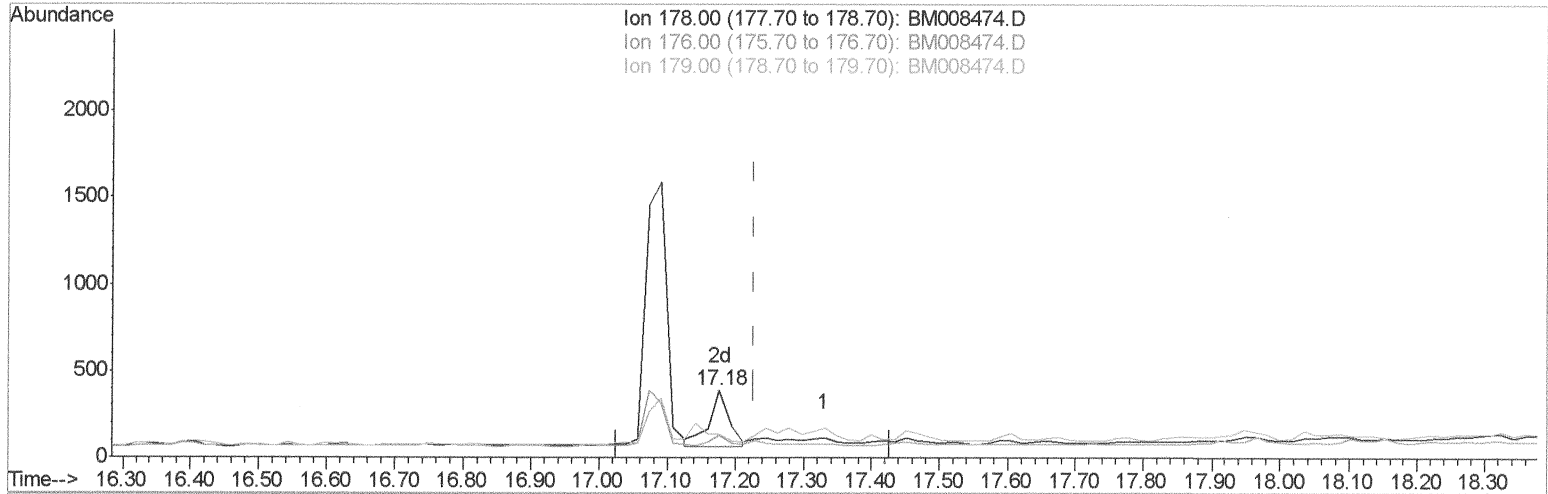

TIC: BM008474.D

(13) Anthracene

17.176min (-0.051) 0.12ng/ul m

SJ 12/21/16

response 641

Ion	Exp%	Act%
178.00	100	100
176.00	22.60	33.76#
179.00	18.40	34.79#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:49:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

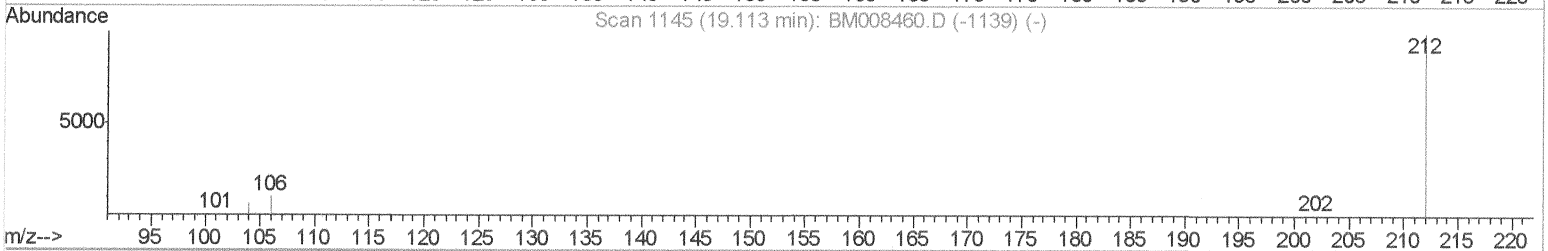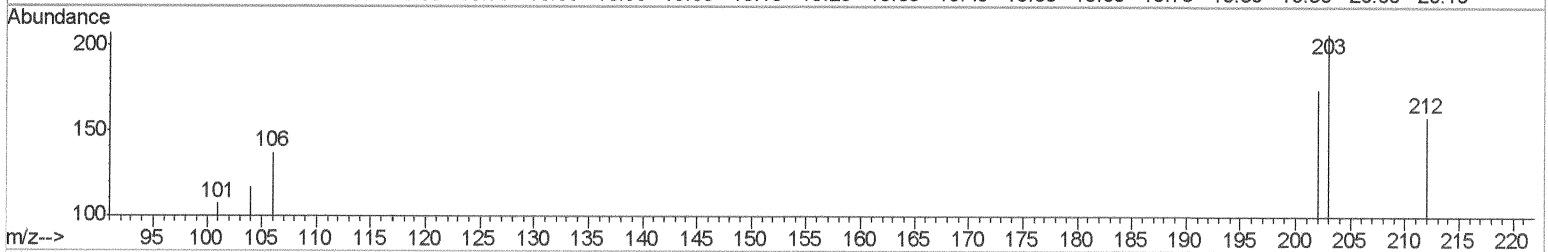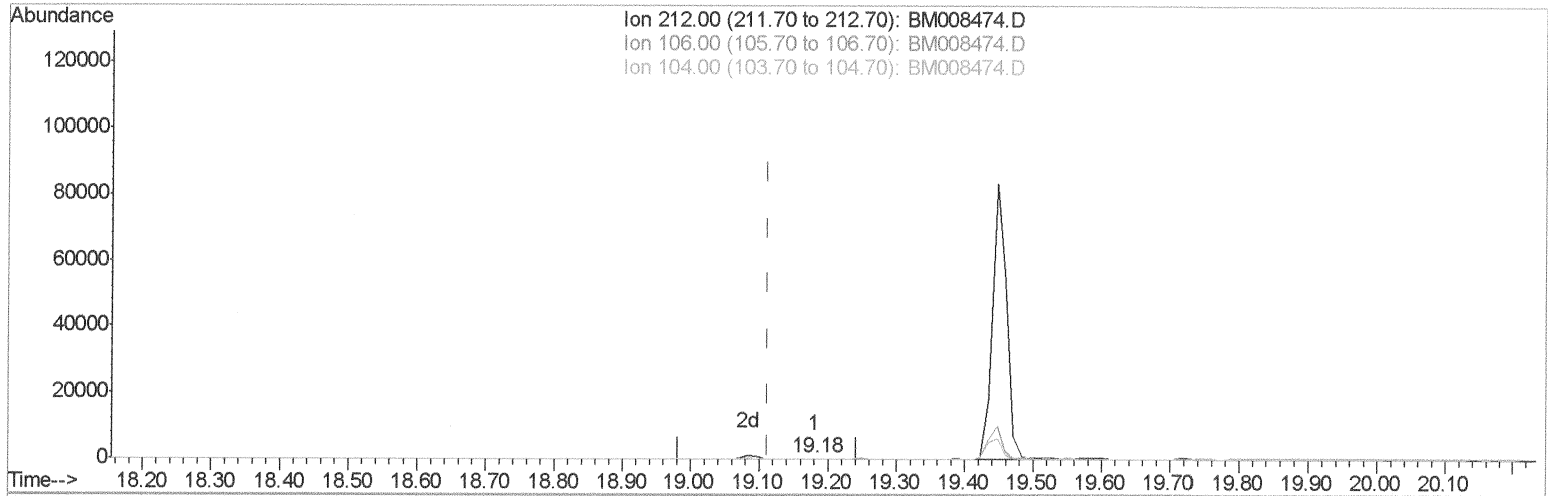

TIC: BM008474.D

(14) Fluoranthene-d10 (SURR)

19.181min (+0.068) 0.02ng/ul

response 85

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:49:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

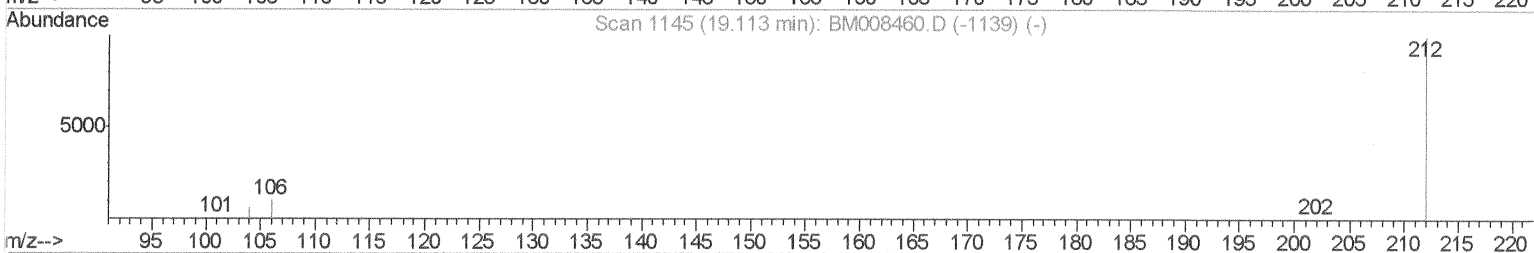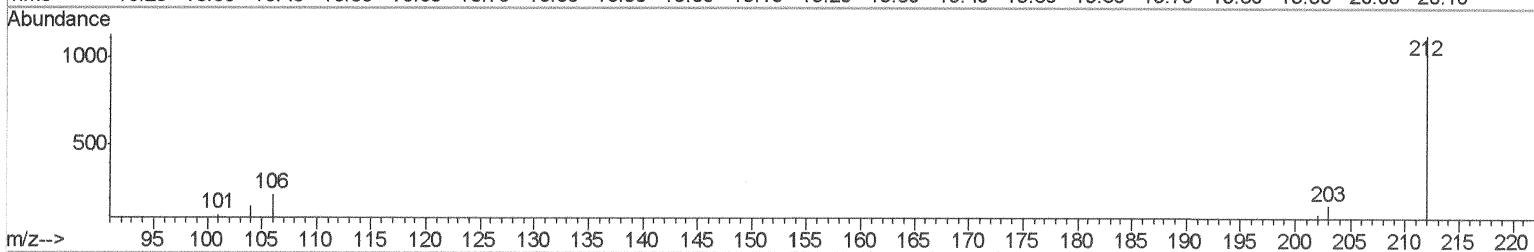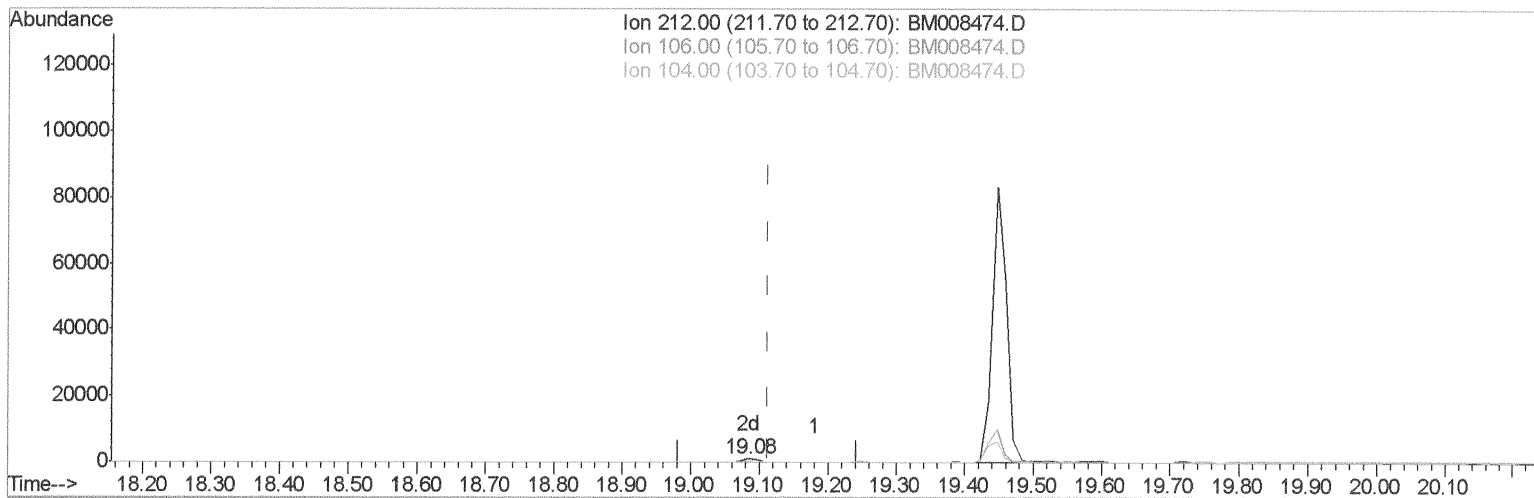

TIC: BM008474.D

(14) Fluoranthene-d10 (SURR)

19.084min (-0.029) 0.33ng/ul m

SJ 12/21/16

response 1574

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:49:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

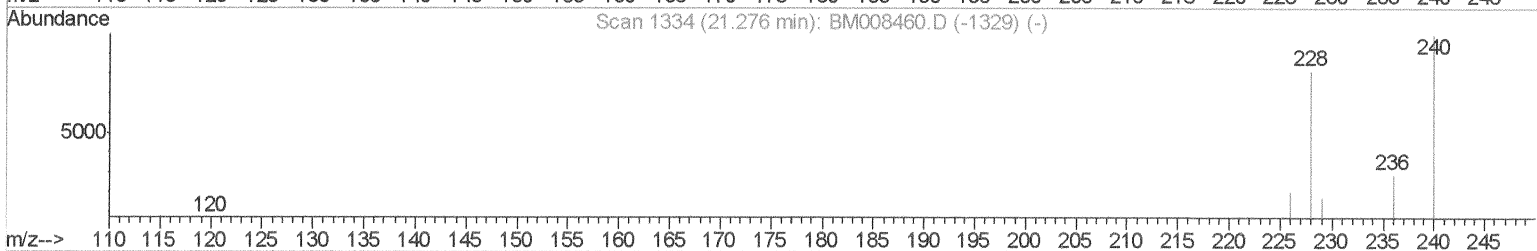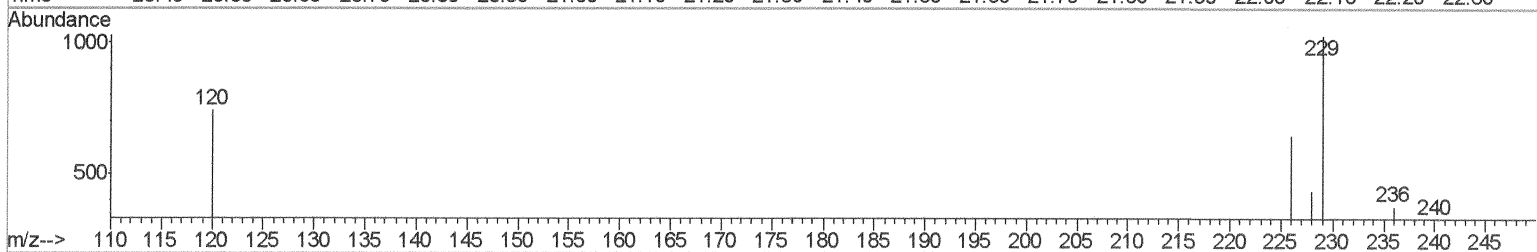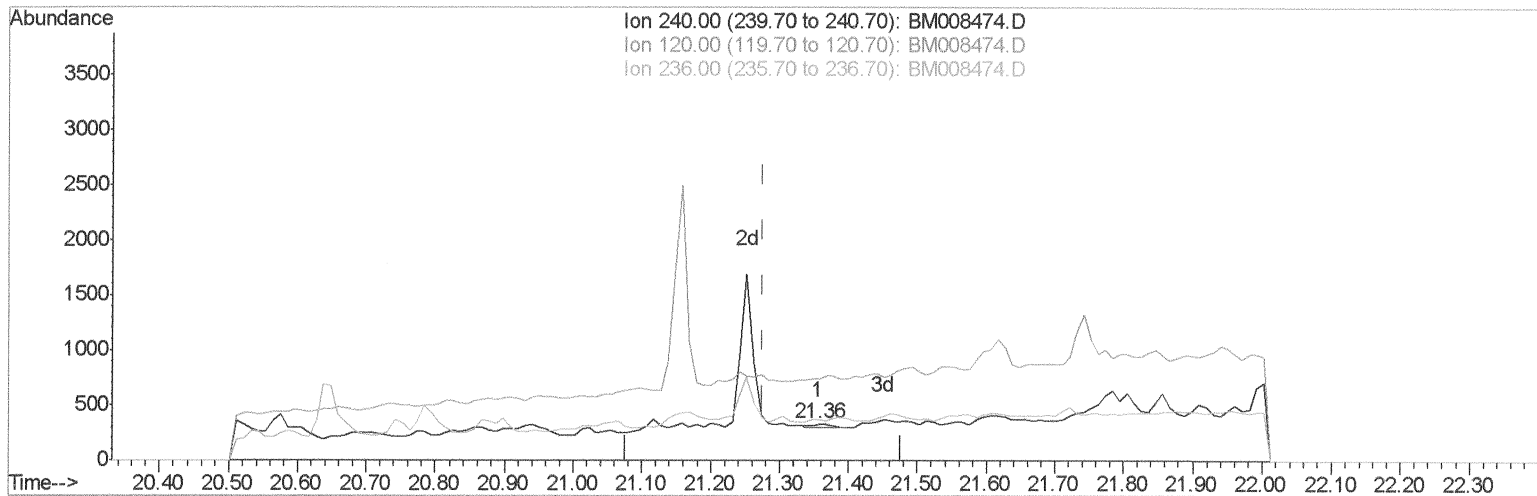

TIC: BM008474.D

(16) Chrysene-d12 (I)

21.356min (+0.080) 0.40ng/ul

response 81

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	222.16#
236.00	34.90	112.87#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:49:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

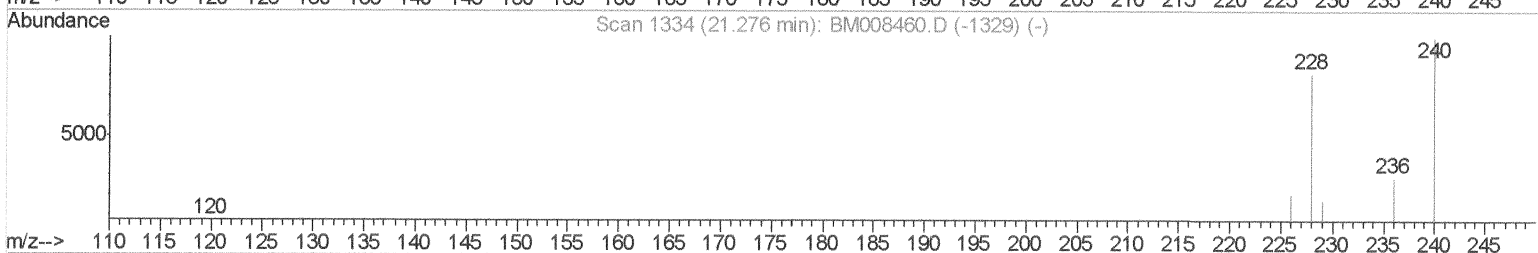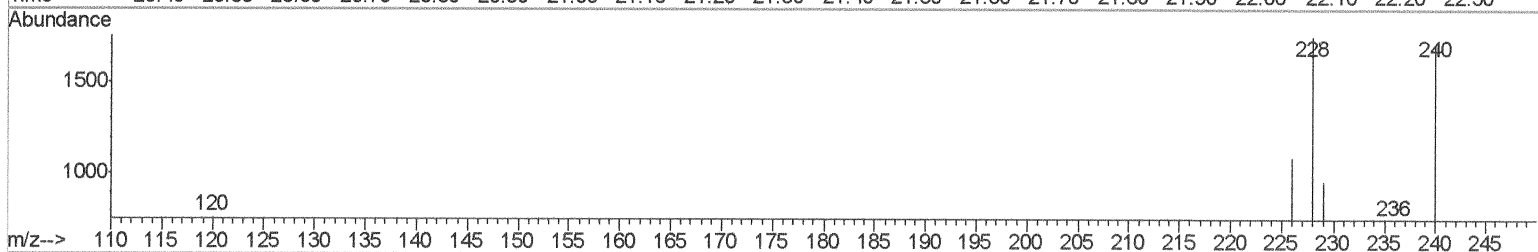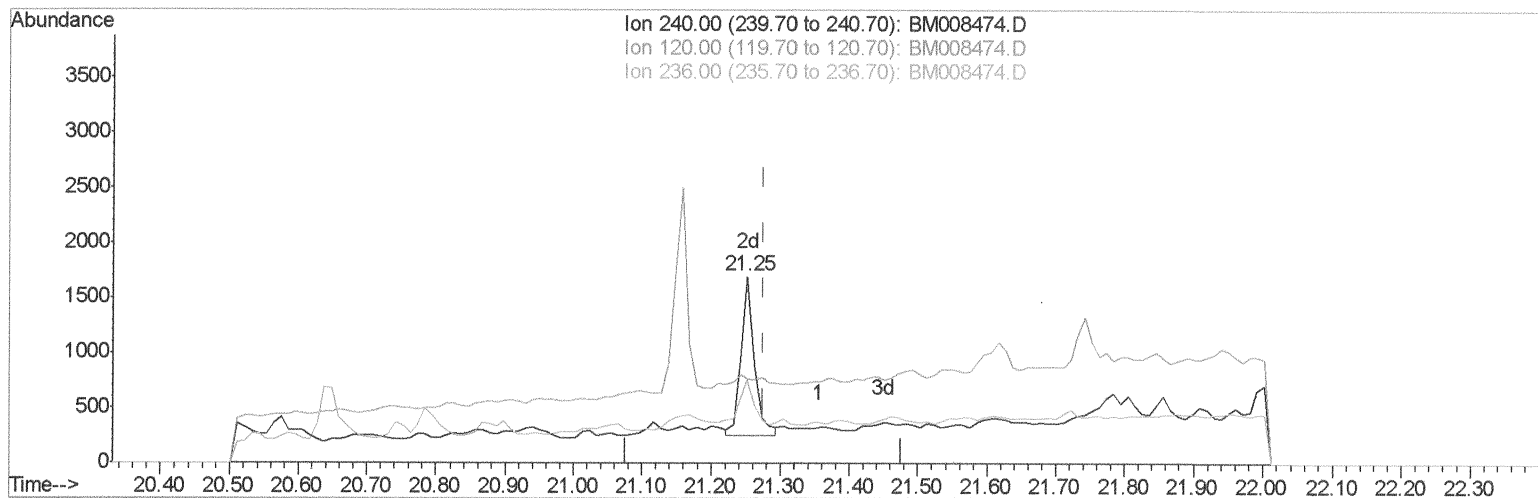

TIC: BM008474.D

(16) Chrysene-d12 (I)

21.252min (-0.024) 0.40ng/ul m

SJ 12/21/16

response 2000

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	45.26#
236.00	34.90	44.67#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:51:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

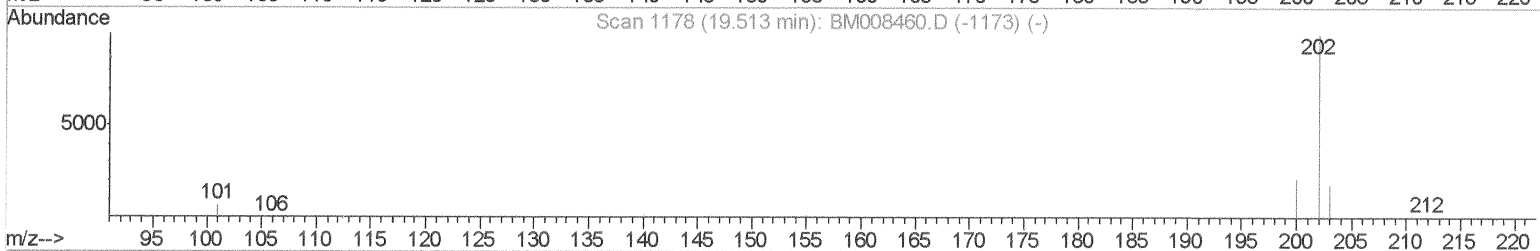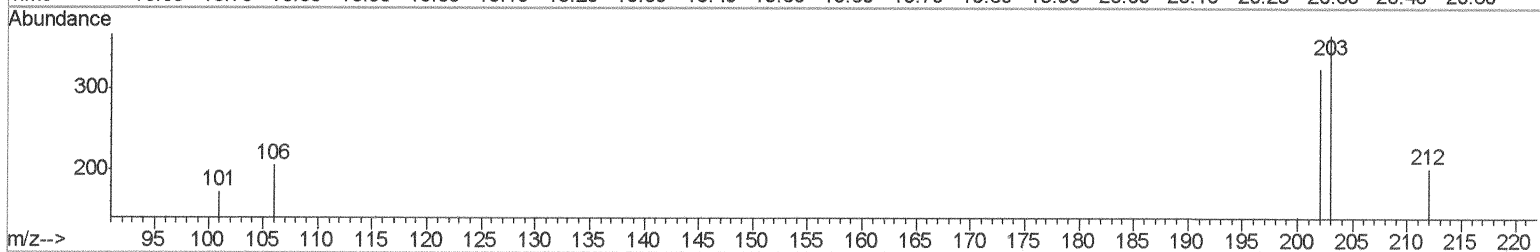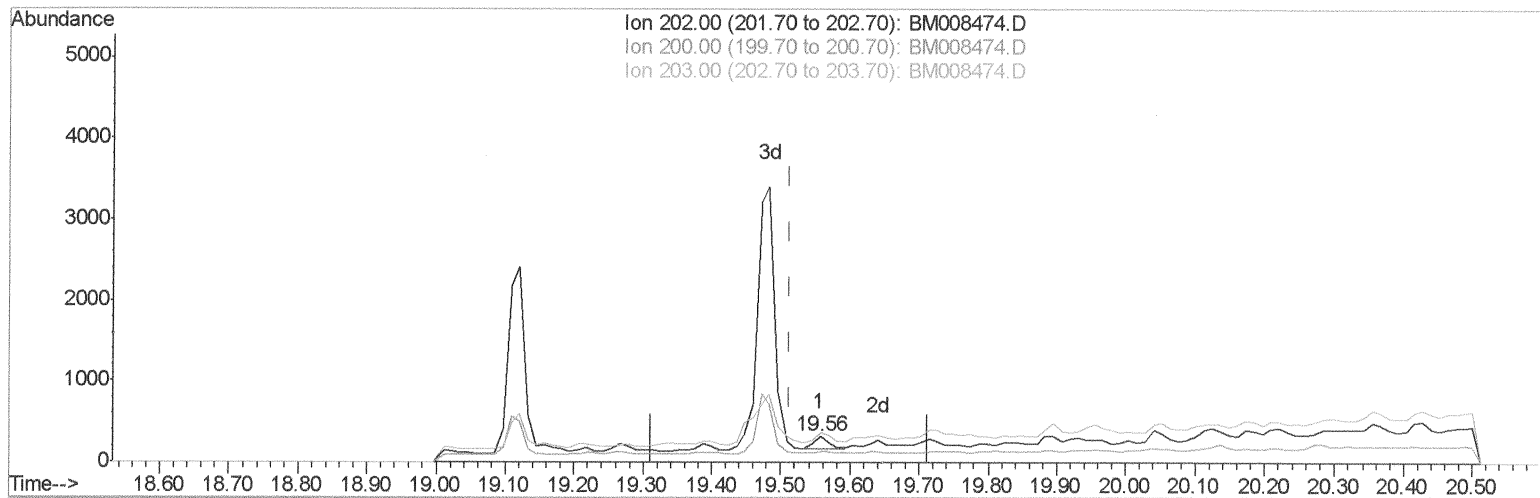

TIC: BM008474.D

(17) Pyrene

19.556min (+0.044) 0.03ng/ul

response 240

Ion	Exp%	Act%
202.00	100	100
200.00	22.80	44.44#
203.00	19.50	112.96#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:51:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

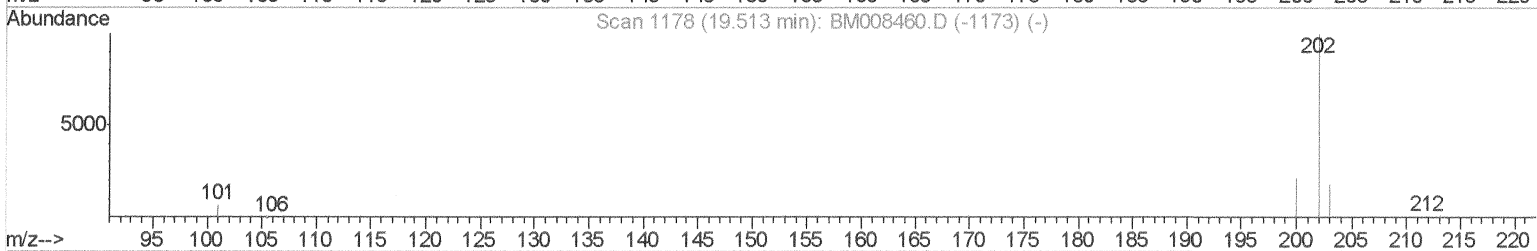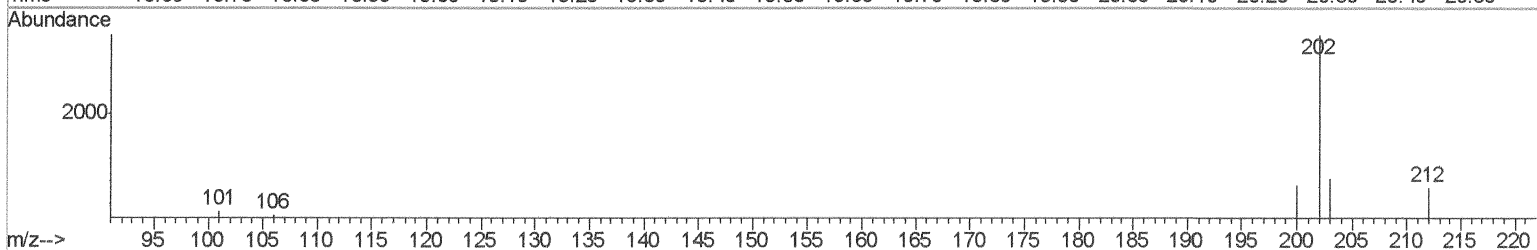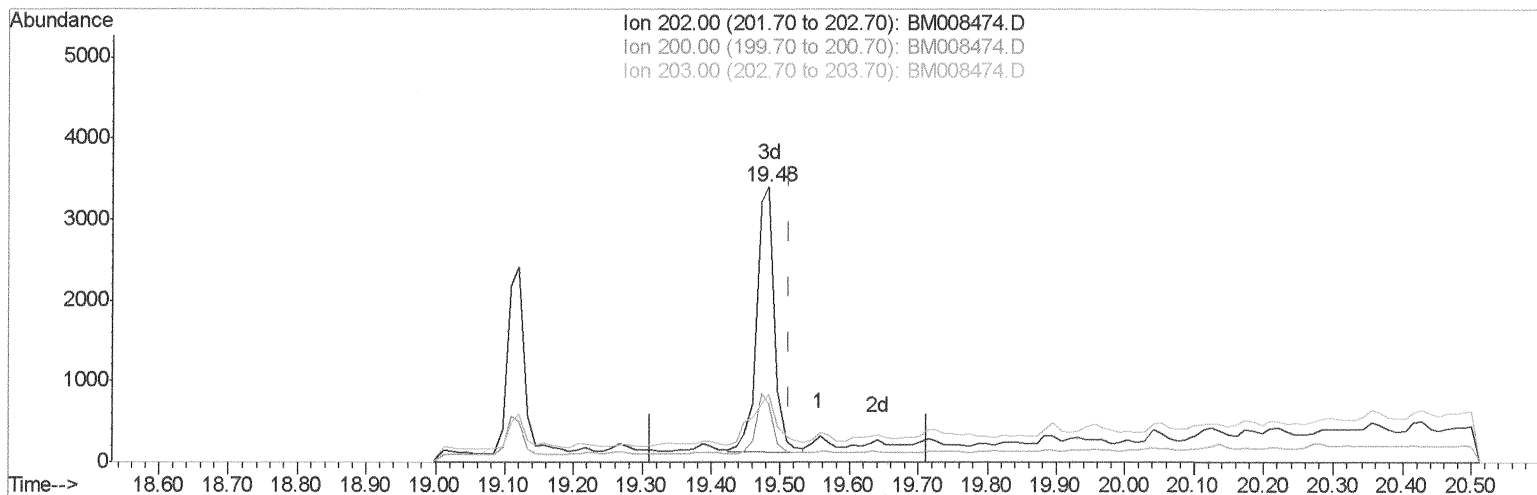

TIC: BM008474.D

(17) Pyrene

19.484min (-0.029) 0.77ng/ul m

SJ 12/21/16

response 5944

Ion	Exp%	Act%
202.00	100	100
200.00	22.80	21.50
203.00	19.50	24.97#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:51:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

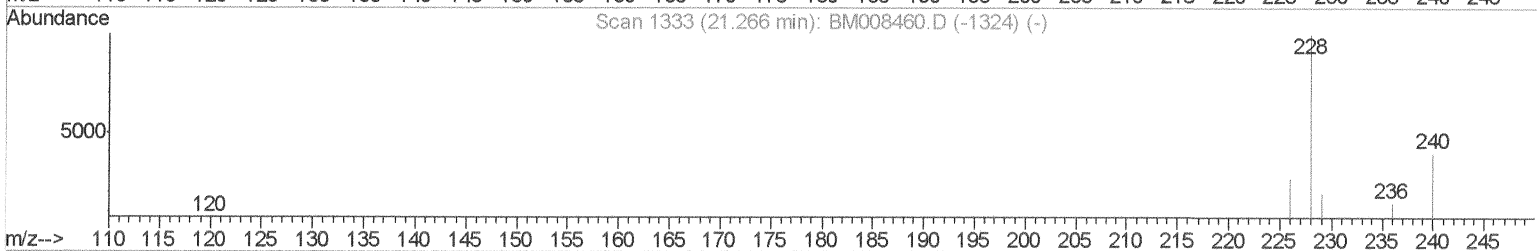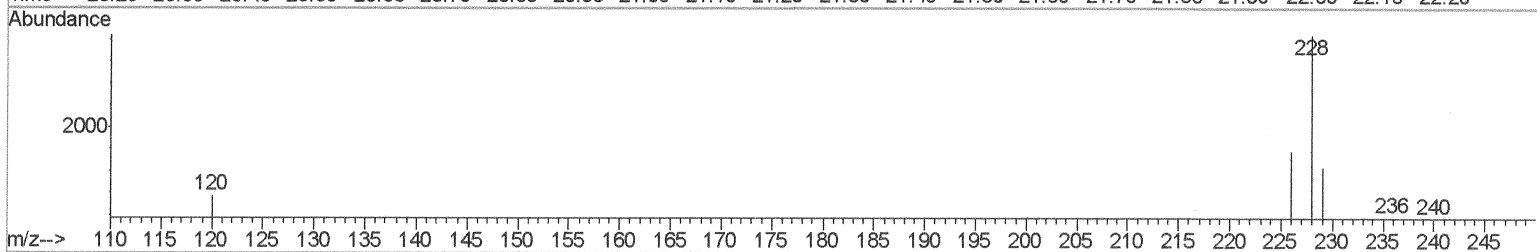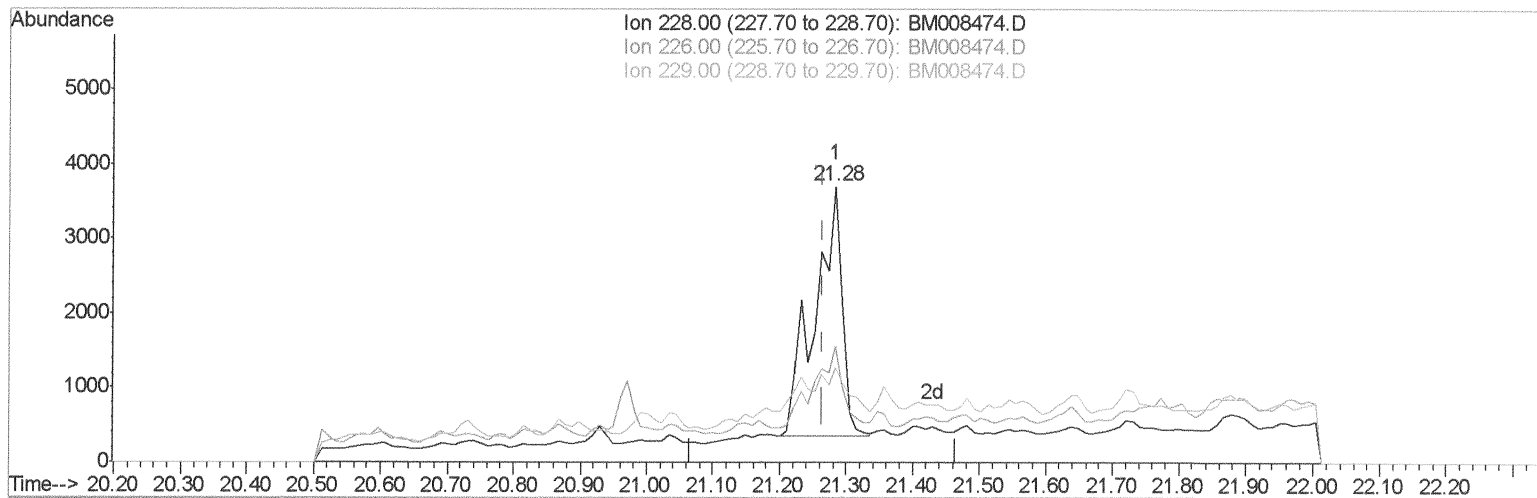

TIC: BM008474.D

(18) Benzo(a)anthracene

21.283min (+0.018) 1.45ng/ul

response 9493

Ion	Exp%	Act%
228.00	100	100
226.00	28.50	42.18#
229.00	21.30	34.46#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:51:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

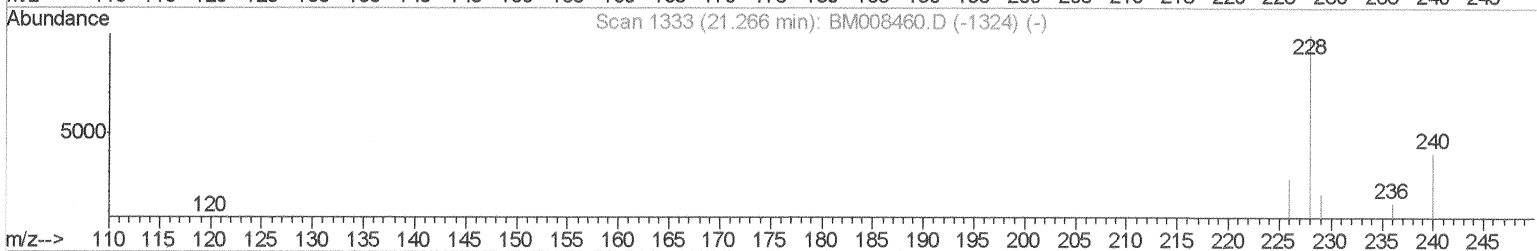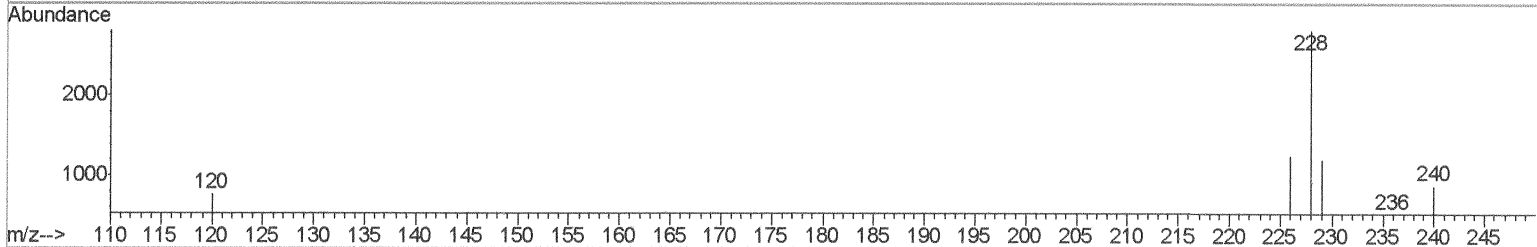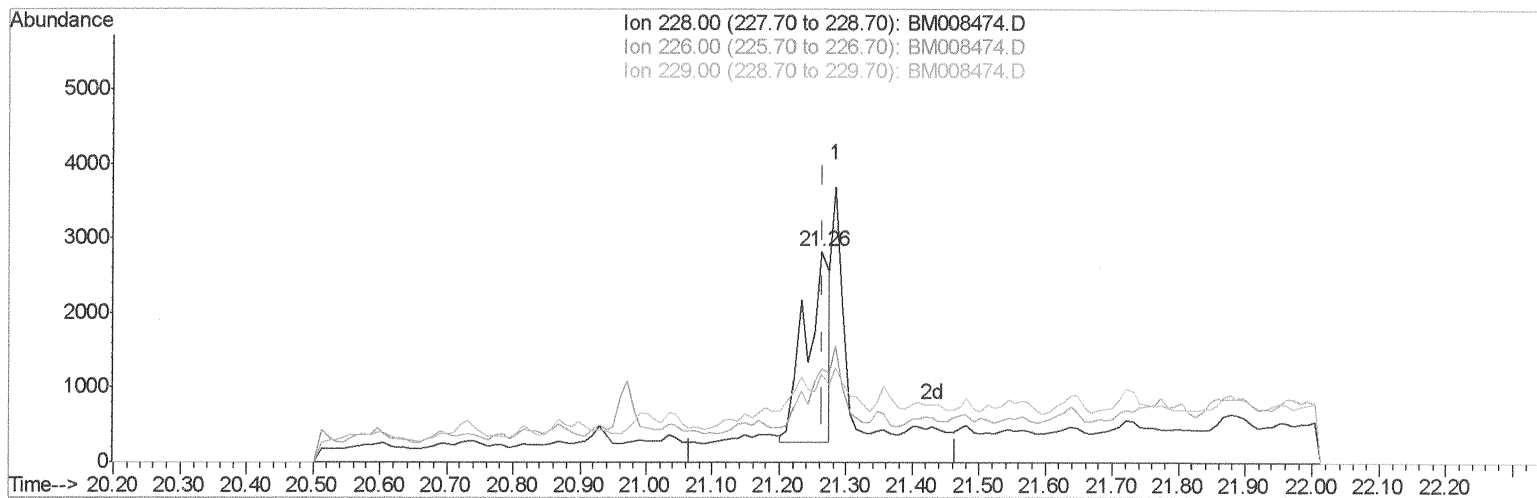

TIC: BM008474.D

(18) Benzo(a)anthracene

21.262min (-0.003) 0.97ng/ul m

51 12/21/16

response 6392

Ion	Exp%	Act%
228.00	100	100
226.00	28.50	44.46#
229.00	21.30	42.48#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:51:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

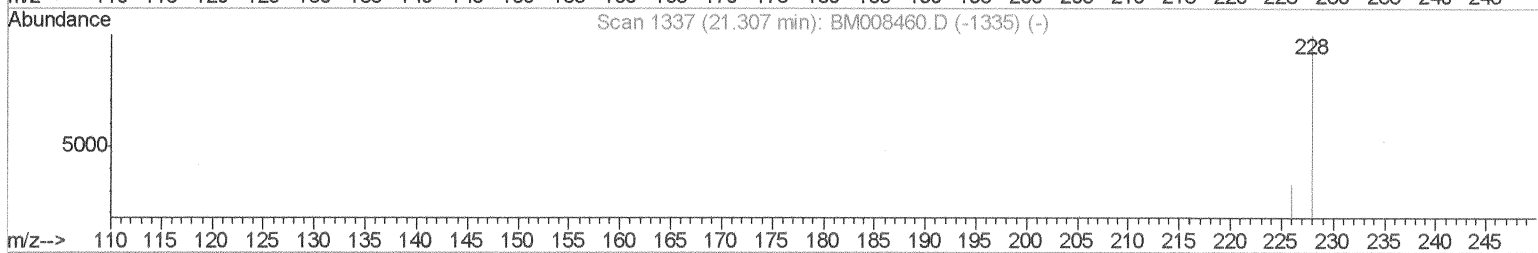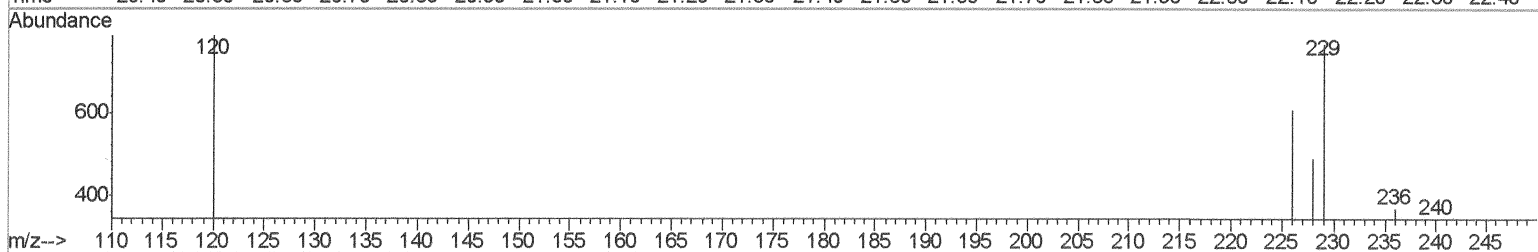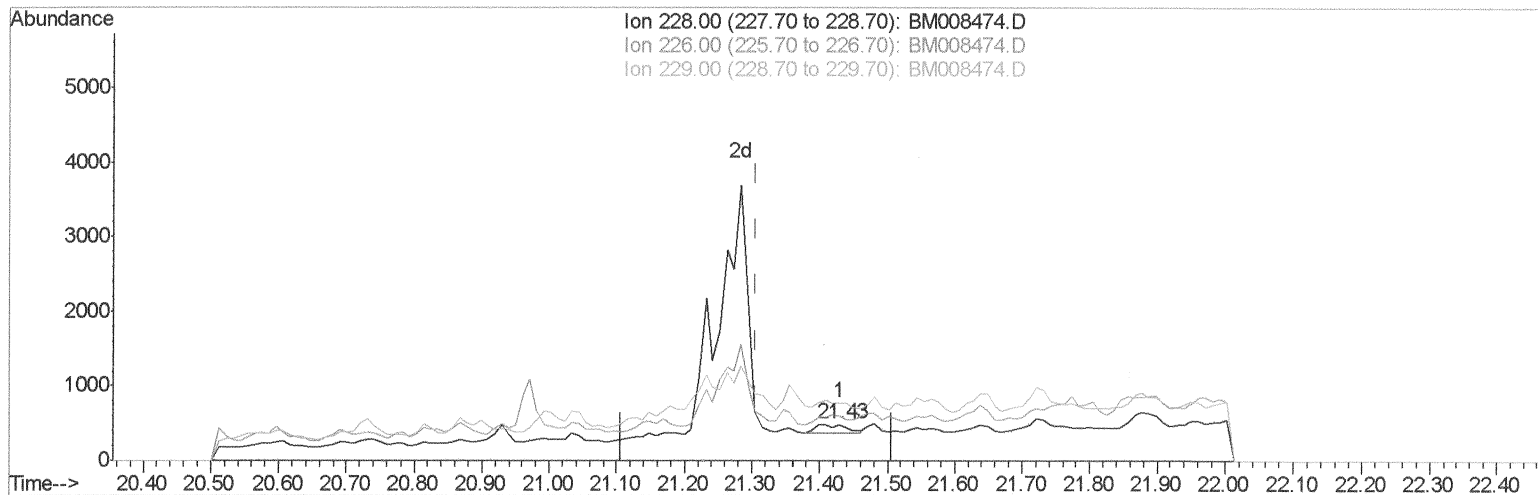

TIC: BM008474.D

(19) Chrysene

21.429min (+0.122) 0.05ng/ul

response 376

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	124.29#
229.00	22.10	156.53#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:51:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

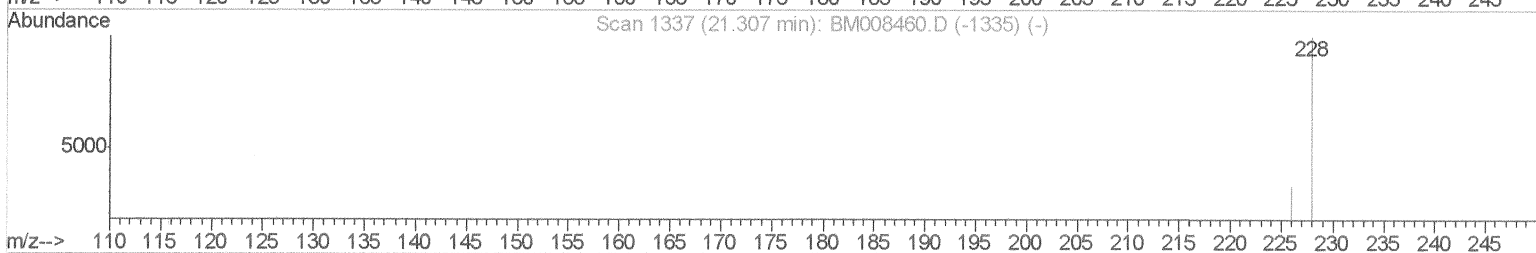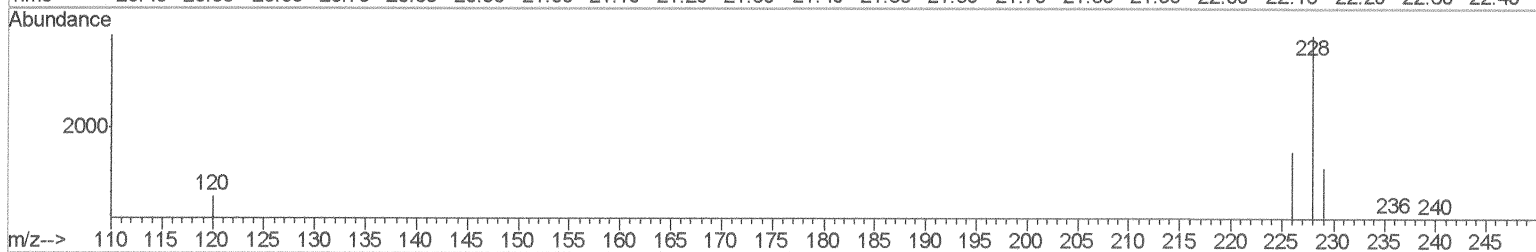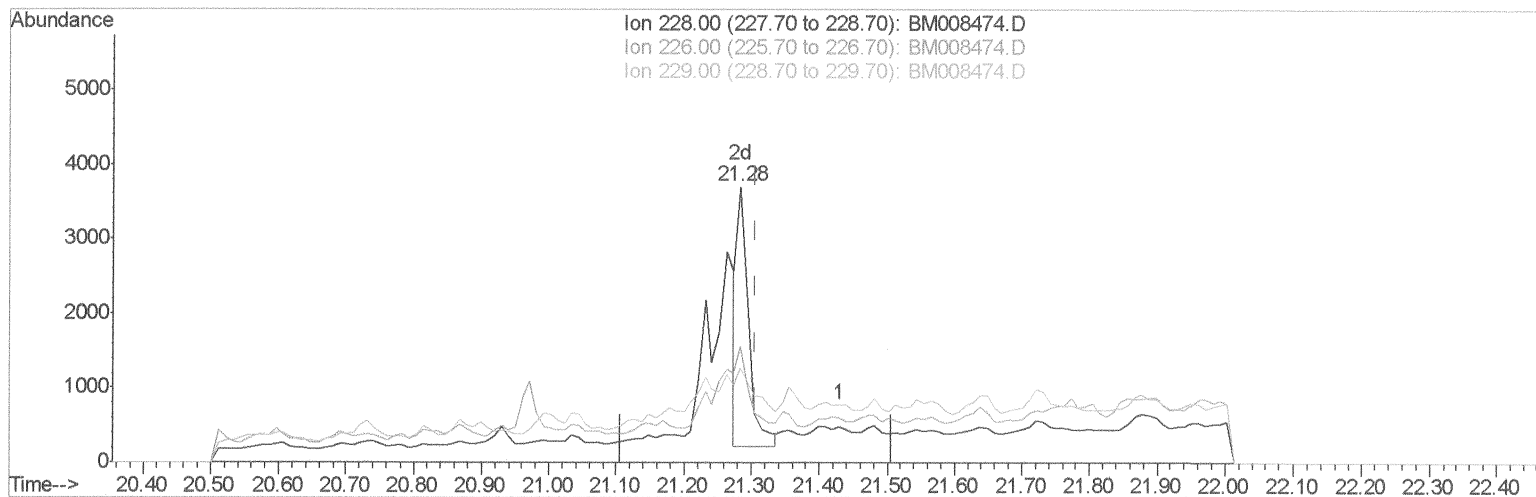

TIC: BM008474.D

(19) Chrysene

21.283min (-0.024) 0.55ng/ul m SJ 12/21/16

response 3947

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	42.18#
229.00	22.10	34.46#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:51:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

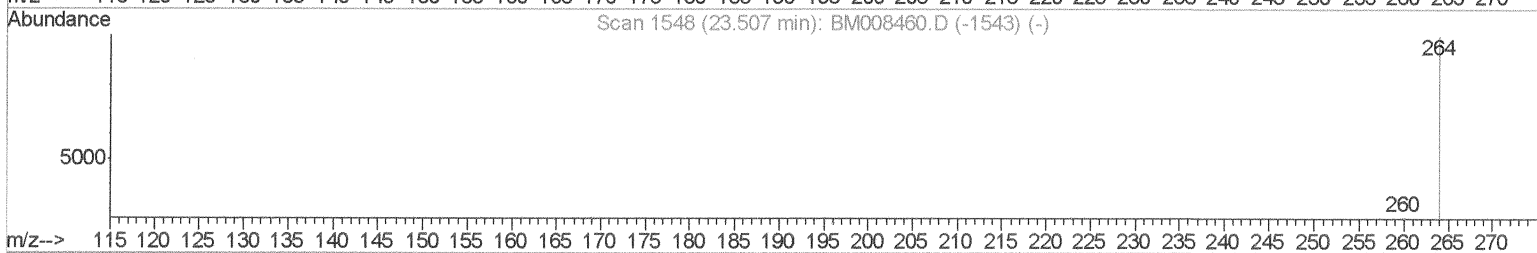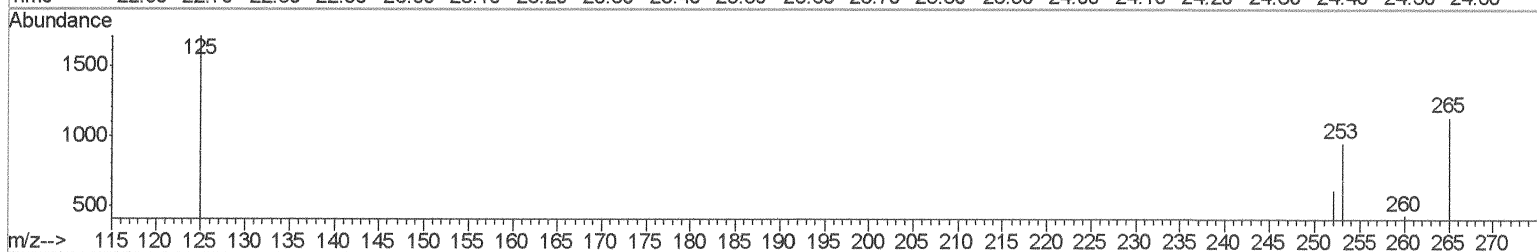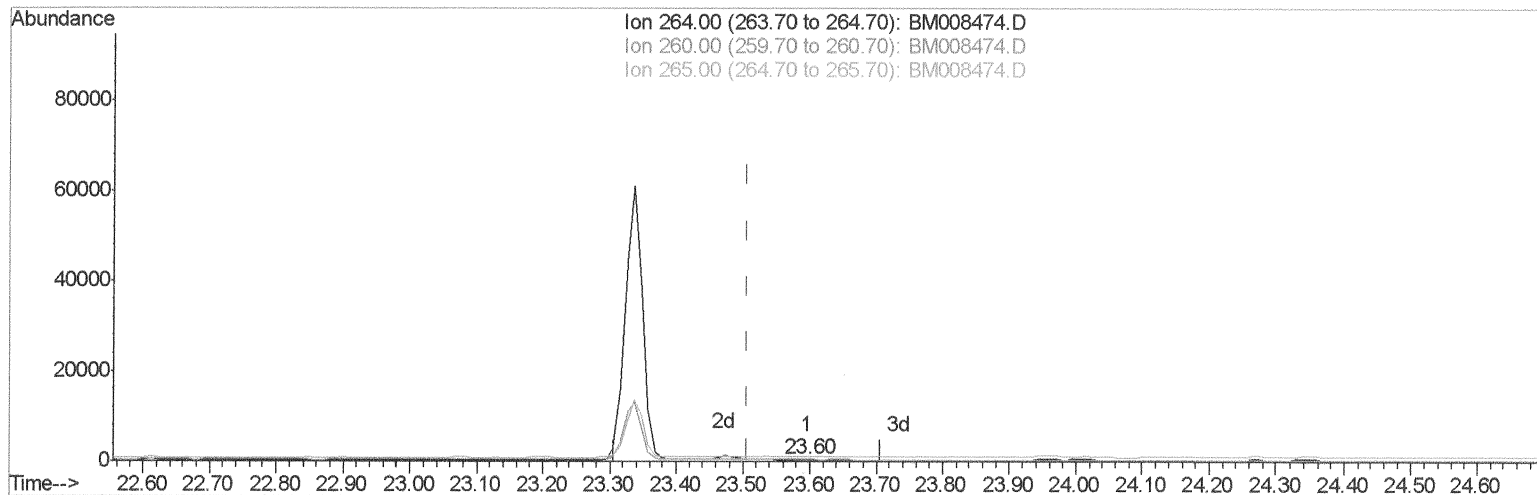

TIC: BM008474.D

(20) Perylene-d12 (I)

23.597min (+0.091) 0.40ng/ul

response 173

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	106.30#
265.00	103.50	274.82#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:51:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

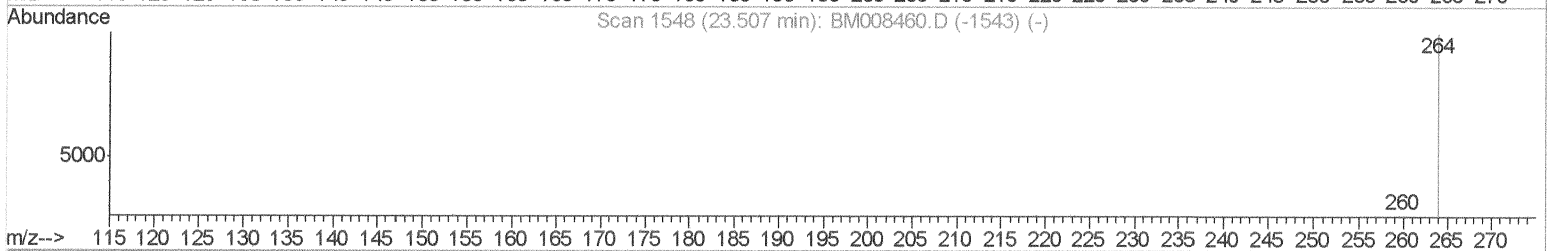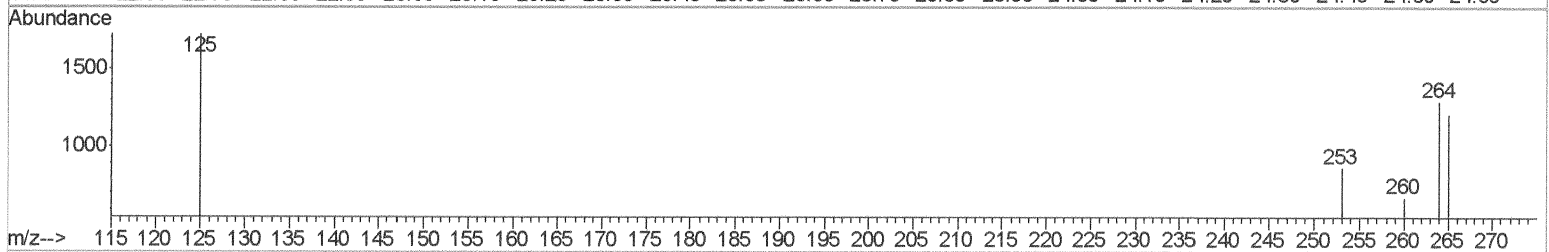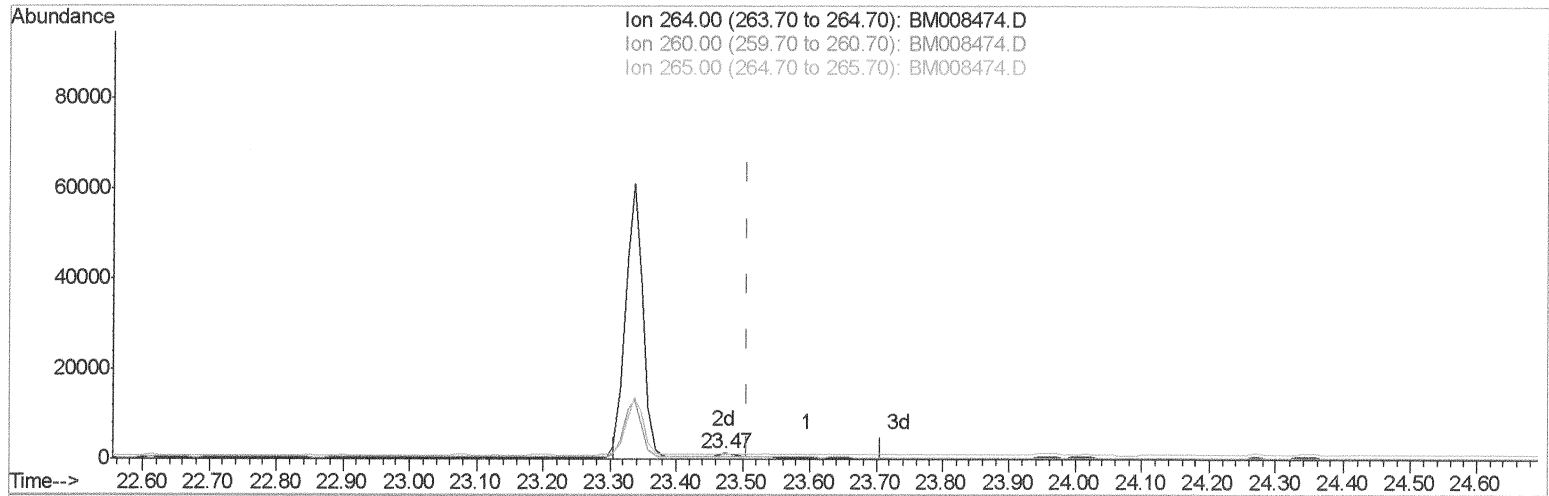

TIC: BM008474.D

(20) Perylene-d12 (I)

23.472min (-0.035) 0.40ng/ul m SJ 12/21/16

response 1646

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	52.10#
265.00	103.50	93.71
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:52:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

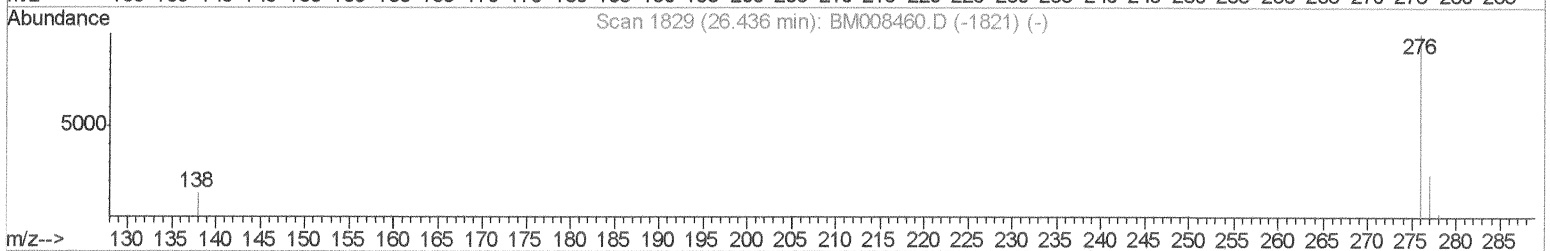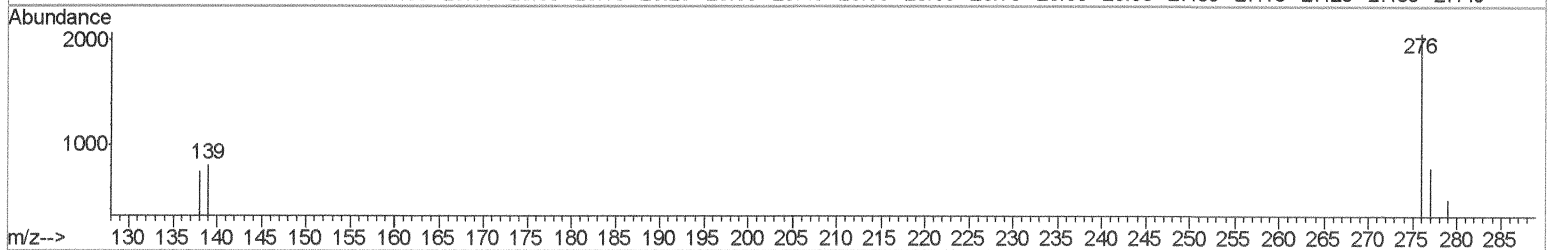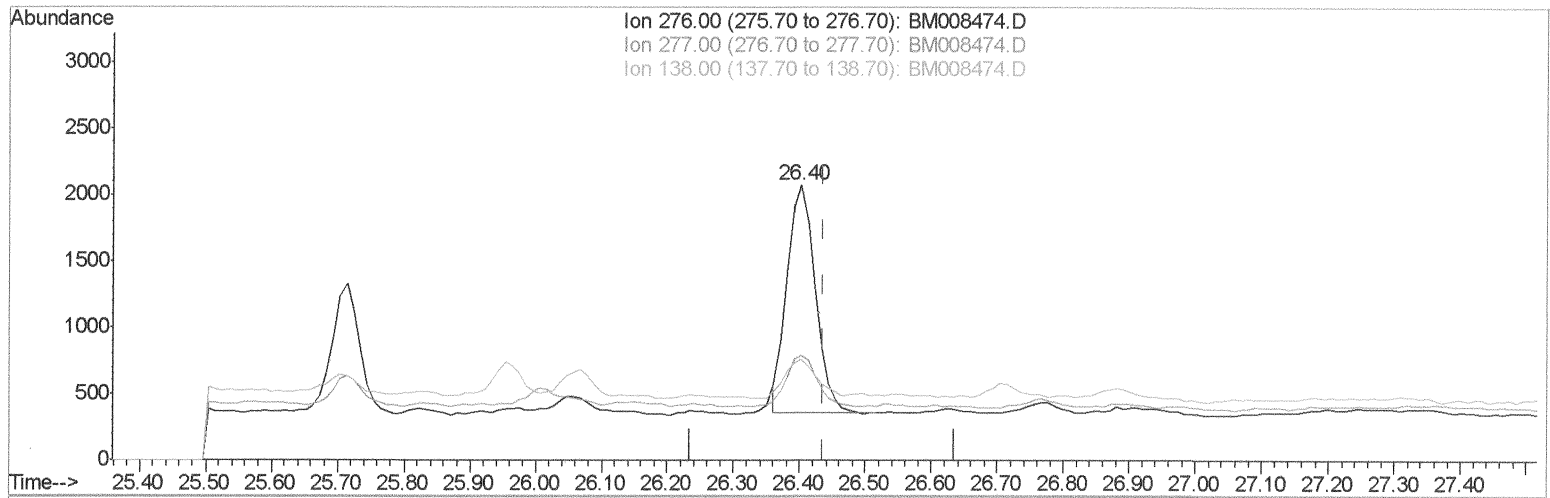

TIC: BM008474.D

(26) Benzo(g,h,i)perylene

26.401min (-0.034) 0.84ng/ul

response 5136

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	38.19#
138.00	25.60	36.69#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
Data File : BM008474.D
Acq On : 20 Dec 2016 11:22
Operator : UM/SJ
Sample : H5905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA811

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:52:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

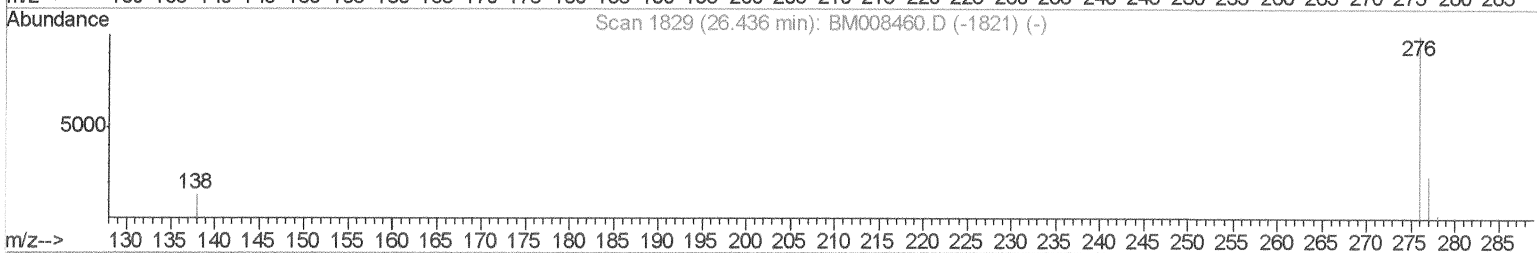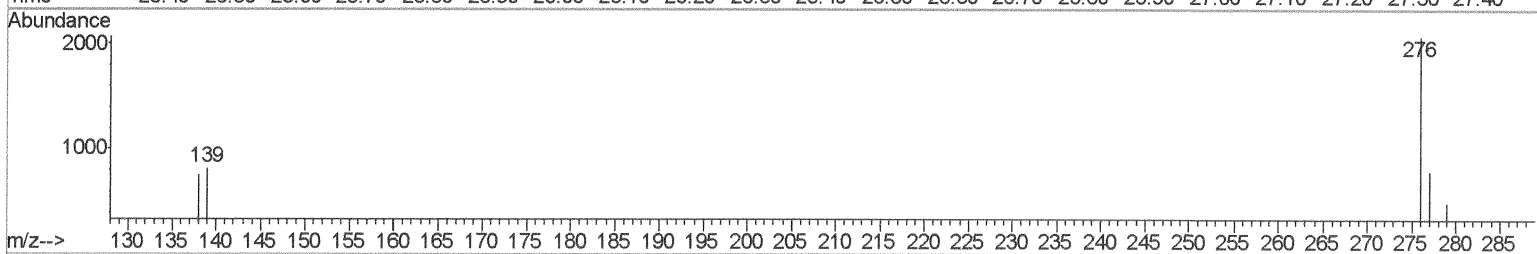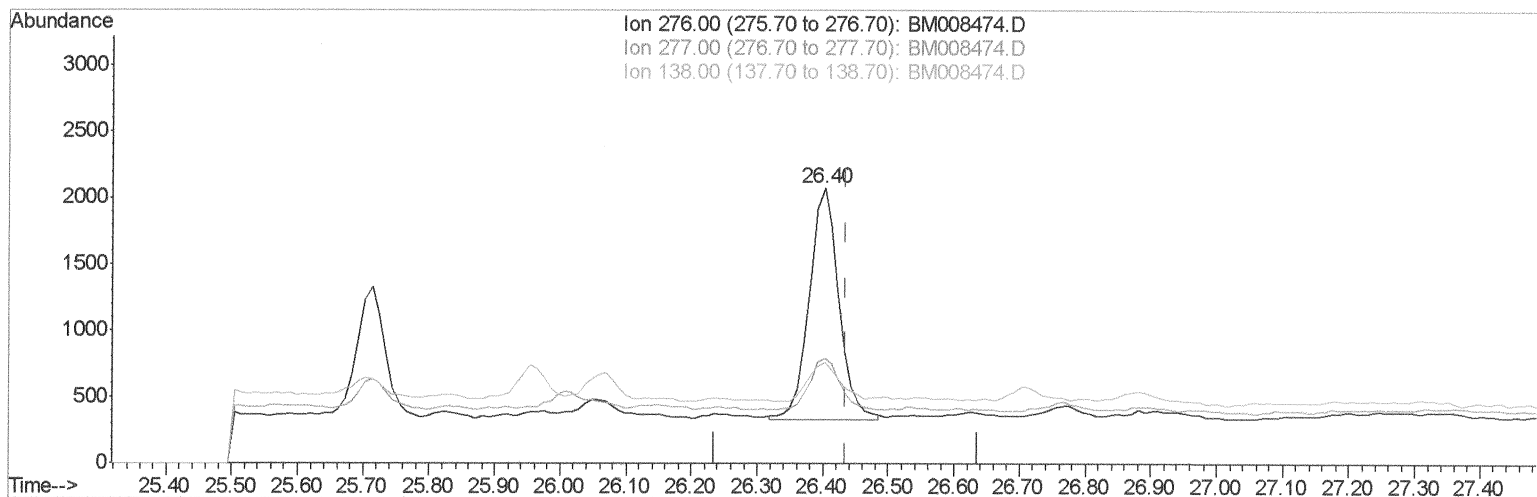

TIC: BM008474.D

(26) Benzo(g,h,i)perylene

26.401min (-0.034) 0.90ng/ul m SJ 12/21/16

response 5544

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	38.19#
138.00	25.60	36.69#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM121916\
 Data File : BM008474.D
 Acq On : 20 Dec 2016 11:22
 Operator : UM/SJ
 Sample : H5905-11
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA811

Manual Integrations
 APPROVED

sohil
 12/20/2016 6:31:48 PM

Quant Time: Dec 20 14:53:18 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 20 04:48:59 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	517	0.40	ng/ul	-0.06
2) Naphthalene-d8	10.43	136	1656	0.40	ng/ul	-0.06
6) Acenaphthene-d10	14.30	164	988	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.04	188	1757m	0.40	ng/ul	-0.05
16) Chrysene-d12	21.25	240	2000m	0.40	ng/ul	-0.02
20) Perylene-d12	23.47	264	1646m	0.40	ng/ul	-0.03

} SJ 12/21/16

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.03	152	709	0.28	ng/ul	-0.07
14) Fluoranthene-d10	19.08	212	1574m	0.33	ng/ul	-0.03

} SJ 12/21/16

Target Compounds

					Qvalue
3) Naphthalene	10.48	128	1782	0.38	ng/ul 97
5) 2-Methylnaphthalene	12.10	142	1931	0.62	ng/ul 95
8) Acenaphthene	14.35	153	143	0.04	ng/ul# 83
9) Fluorene	15.36	166	176	0.05	ng/ul# 80
12) Phenanthrene	17.09	178	3223m	0.60	ng/ul
13) Anthracene	17.18	178	641m	0.12	ng/ul
15) Fluoranthene	19.12	202	3940	0.60	ng/ul 89
17) Pyrene	19.48	202	5944m	0.77	ng/ul
18) Benzo(a)anthracene	21.26	228	6392m	0.97	ng/ul
19) Chrysene	21.28	228	3947m	0.55	ng/ul
26) Benzo(g,h,i)perylene	26.40	276	5544m	0.90	ng/ul

} SJ 12/21/16

} SJ 12/21/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed