

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121916\
 Data File : BM008456.D
 Acq On : 20 Dec 2016 00:01
 Operator : UM/SJ
 Sample : H5970-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA851

Manual Integrations
 APPROVED

sohil
 12/20/2016 6:31:22 PM

Quant Time: Dec 20 13:01:47 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 20 04:48:59 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	356	0.40	ng/ul	-0.05
2) Naphthalene-d8	10.44	136	1216	0.40	ng/ul	-0.05
6) Acenaphthene-d10	14.30	164	720	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.06	188	1334m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.27	240	1274	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	1411	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	339	0.18	ng/ul	-0.04
14) Fluoranthene-d10	19.10	212	692	0.19	ng/ul	-0.02
Target Compounds						Ovalue
5) 2-Methylnaphthalene	12.13	142	200	0.09	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121916\
Data File : BM008456.D
Acq On : 20 Dec 2016 00:01
Operator : UM/SJ
Sample : H5970-12
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DA851

Manual Integrations
APPROVED

sohil
12/20/2016 6:31:22 PM

Quant Time: Dec 20 13:01:47 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 04:48:59 2016
Response via : Initial Calibration

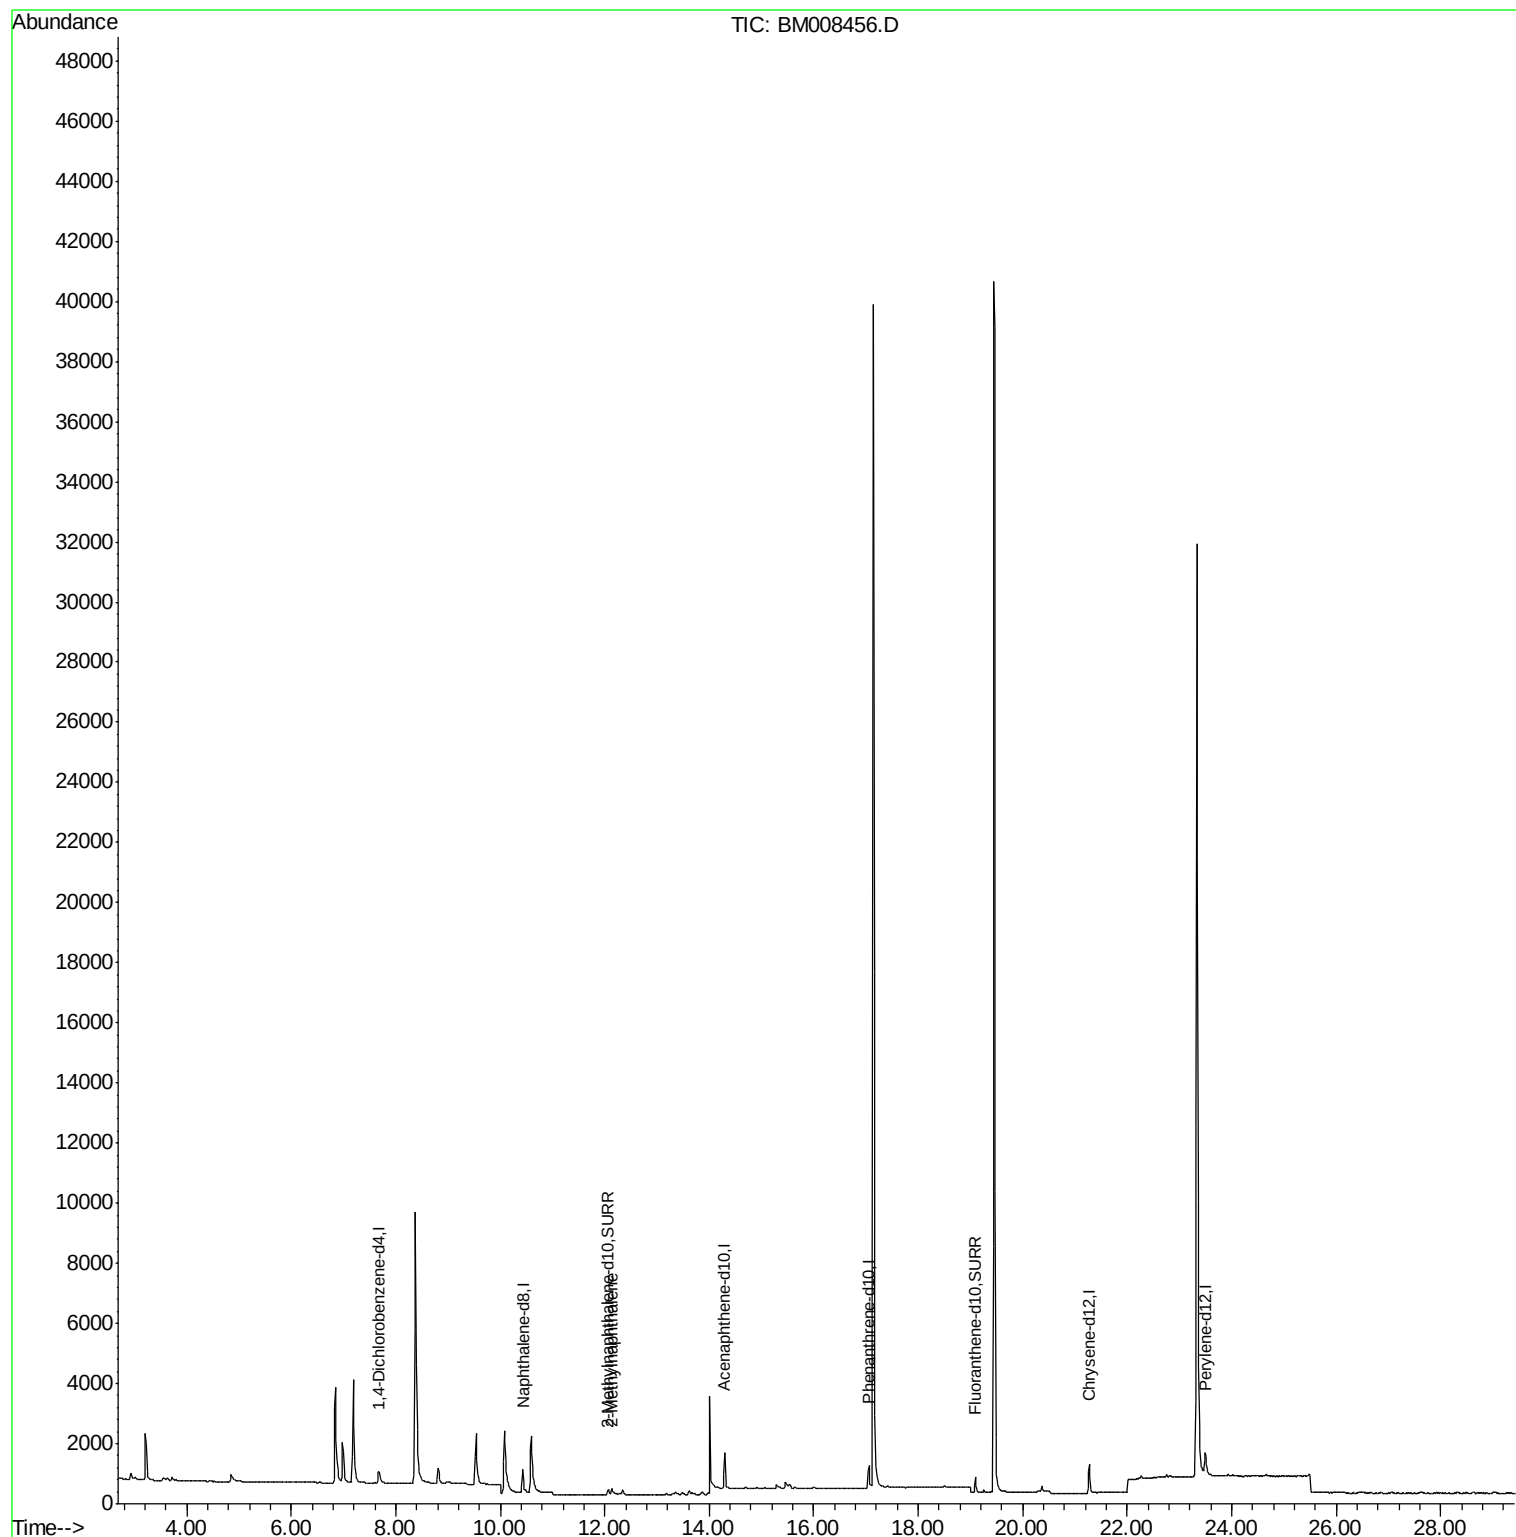

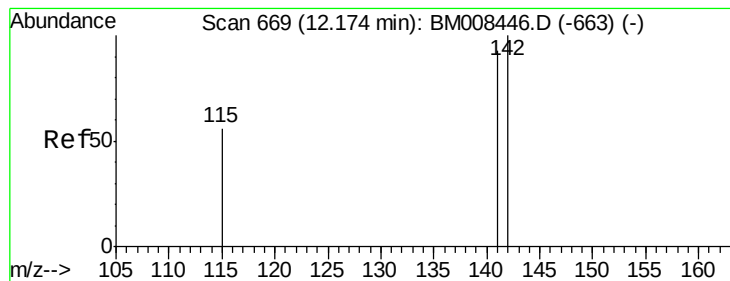

#5

2-Methylnaphthalene

Concen: 0.09 ng/ul

RT: 12.13 min Scan# 665

Delta R.T. -0.04 min

Lab File: BM008456.D

Acq: 20 Dec 2016 00:01

Instrument :

BNA_M

ClientSampleId :

DA851

Tot Ion:142 Resp: 200

Ion Ratio Lower Upper

142 100

141 88.5 72.6 108.8

Manual Integrations

APPROVED

sohil

12/20/2016 6:31:22 PM

