

Data File : BM024201.D

Acq On : 20 Dec 2019 13:40

Operator : JU

Sample : SSTDCCC020

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Dec 21 00:06:57 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Dec 21 00:03:57 2019

Response via : Initial Calibration

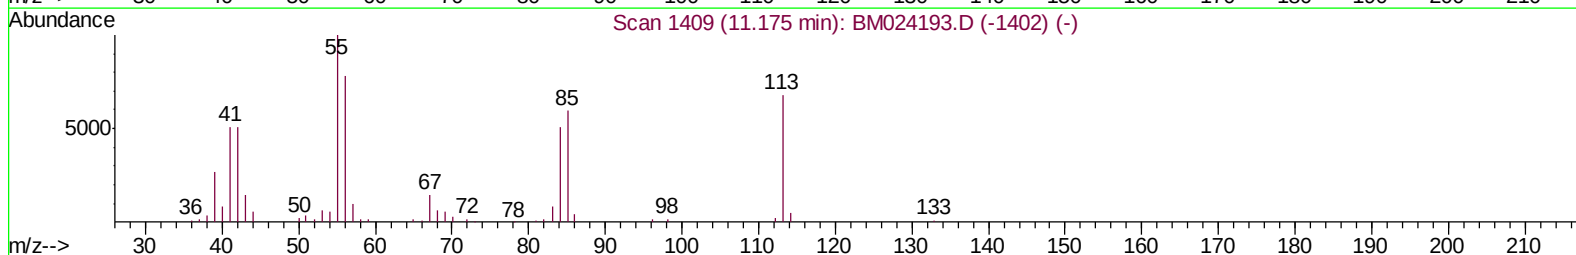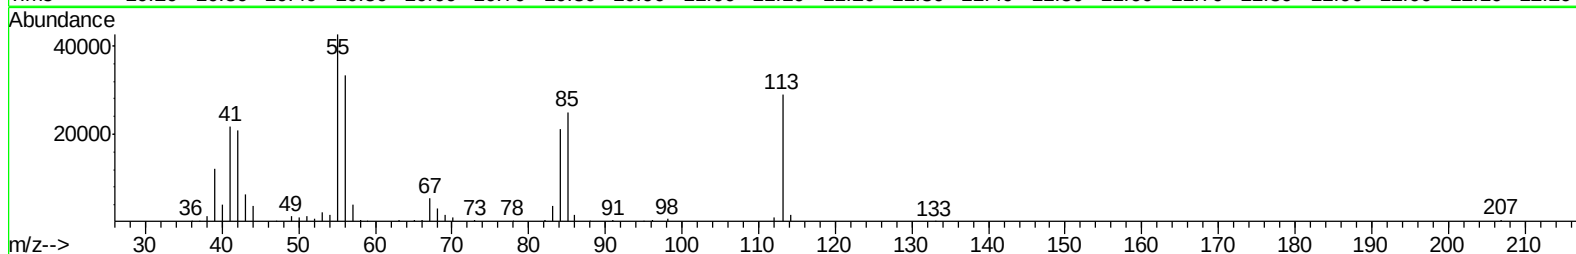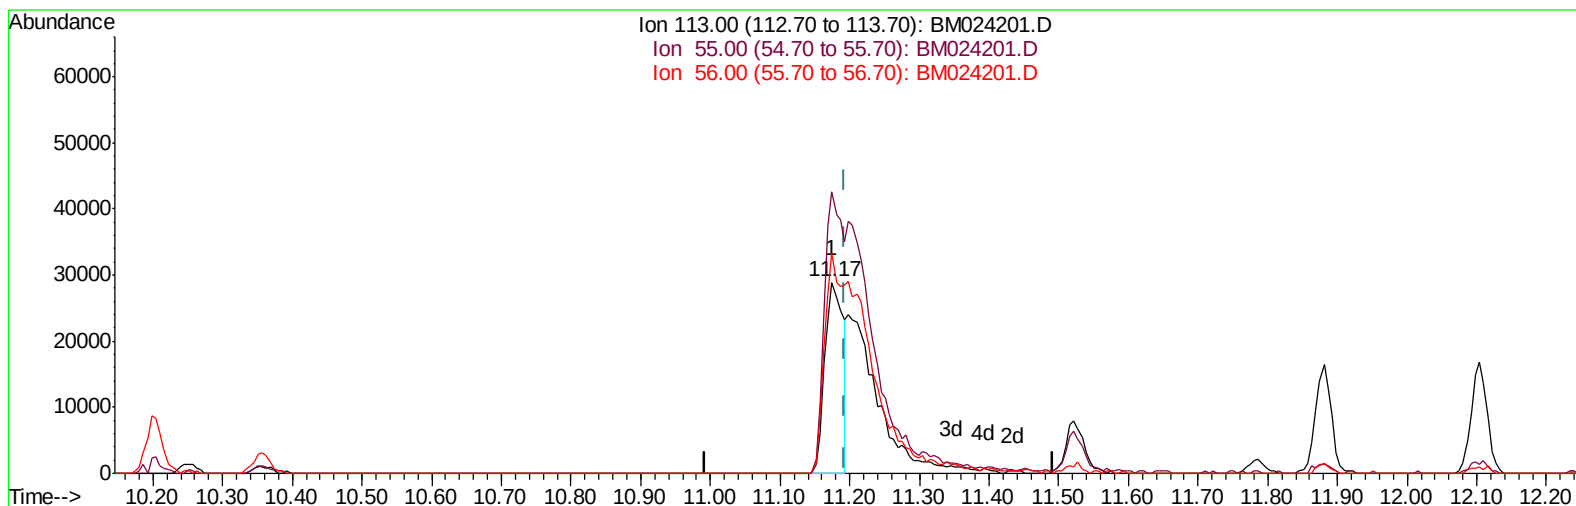

TIC: BM024201.D

(32) Caprolactam

11.175min (-0.018) 7.41ng/ul

response 53109

Ion	Exp%	Act%
113.00	100	100
55.00	151.30	147.59
56.00	121.00	115.47
0.00	0.00	0.00