
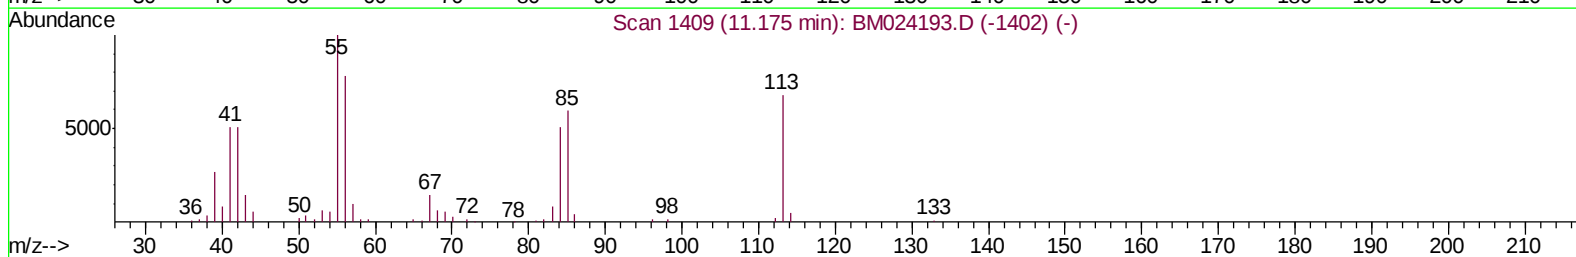
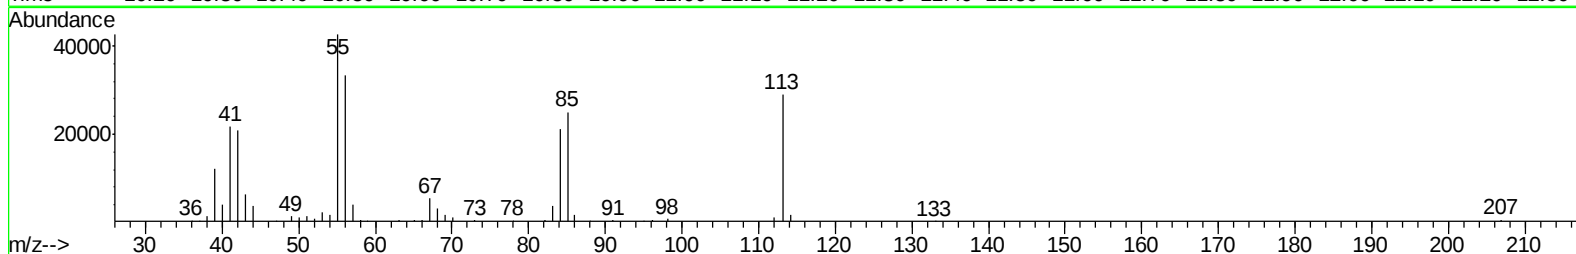


Data File : BM024201.D
Acq On : 20 Dec 2019 13:40
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 21 00:06:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 21 00:03:57 2019
Response via : Initial Calibration

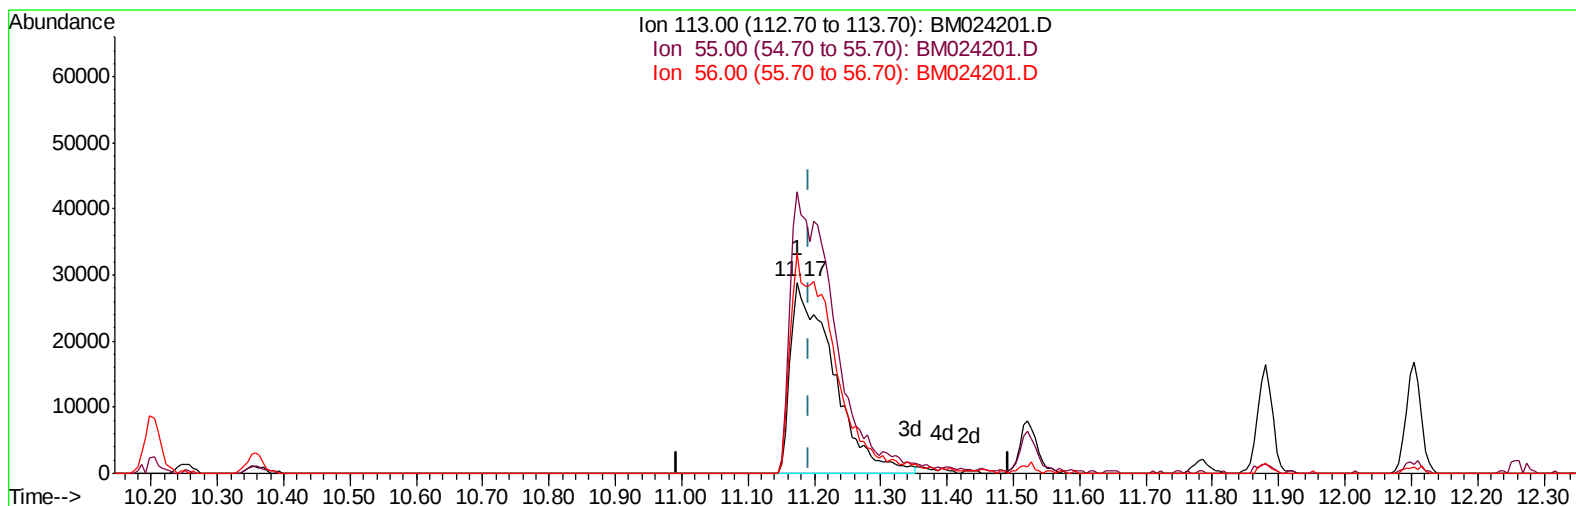

TIC: BM024201.D

(32) Caprolactam

11.175min (-0.018) 17.77ng/ul m

response 127312

Ion	Exp%	Act%
113.00	100	100
55.00	151.30	147.59
56.00	121.00	115.47
0.00	0.00	0.00