
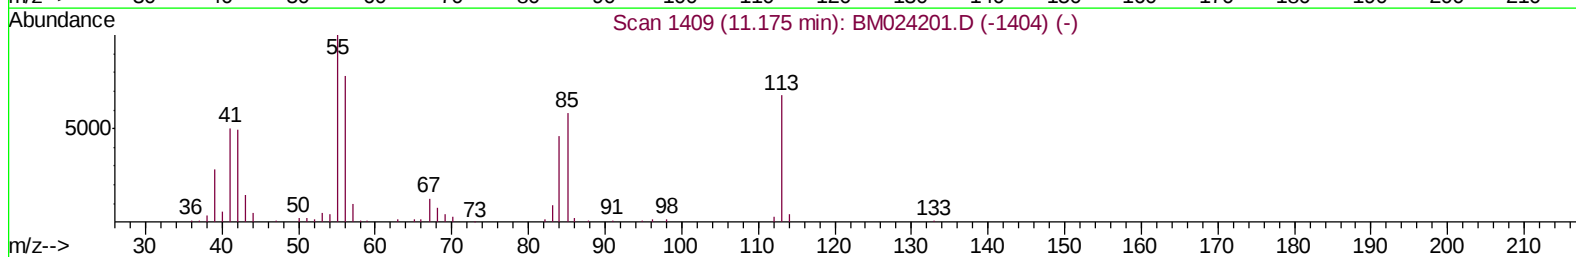
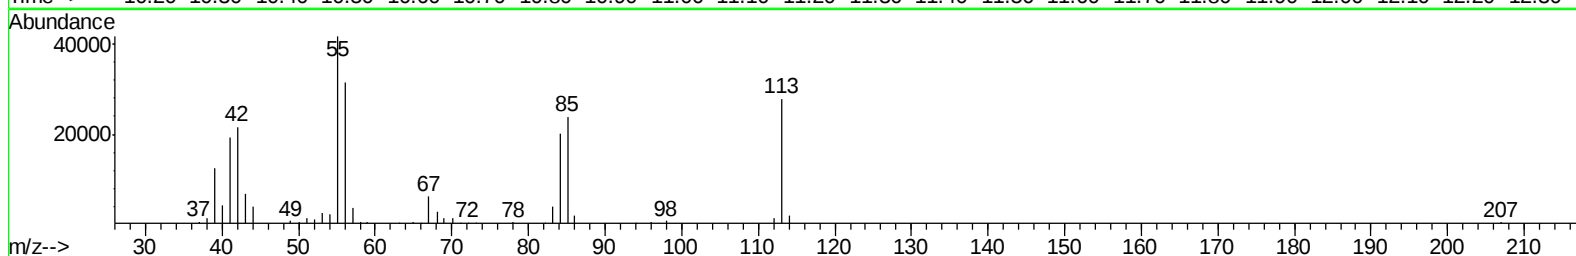


Data File : BM024202.D
Acq On : 20 Dec 2019 14:16
Operator : JU
Sample : K4649-02MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Dec 21 00:36:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 21 00:34:28 2019
Response via : Initial Calibration

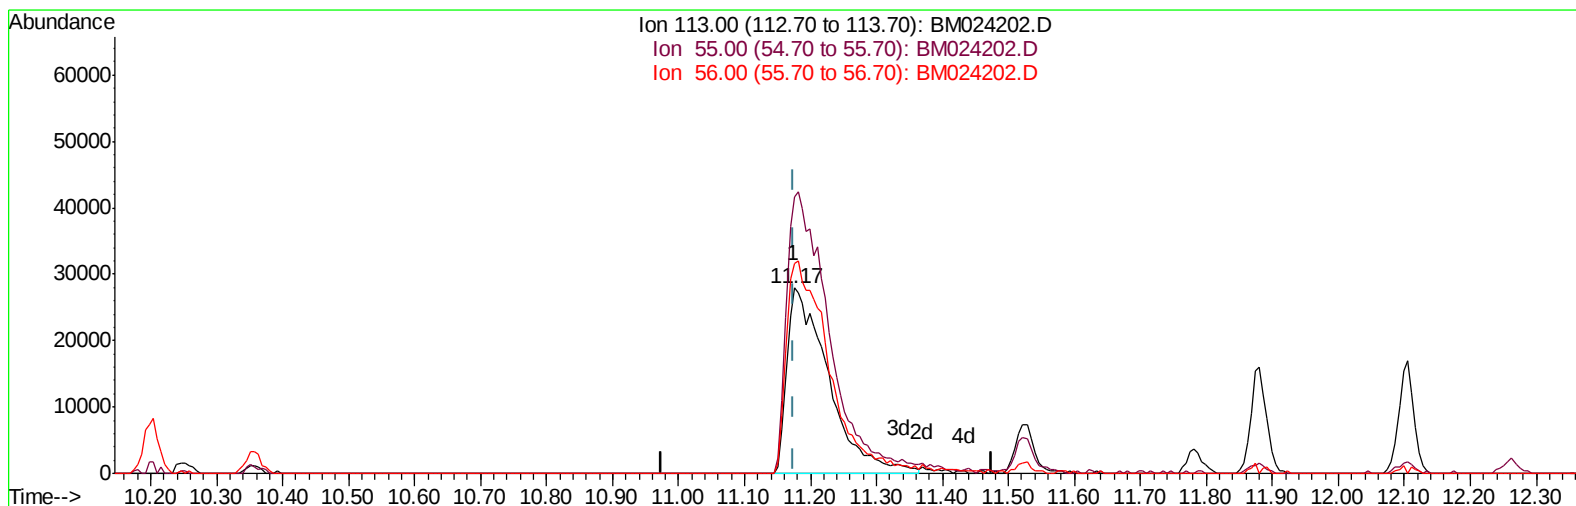

TIC: BM024202.D

(32) Caprolactam

11.175min (+0.000) 18.15ng/ul m

response 120959

Ion	Exp%	Act%
113.00	100	100
55.00	151.30	149.33
56.00	121.00	113.21
0.00	0.00	0.00