
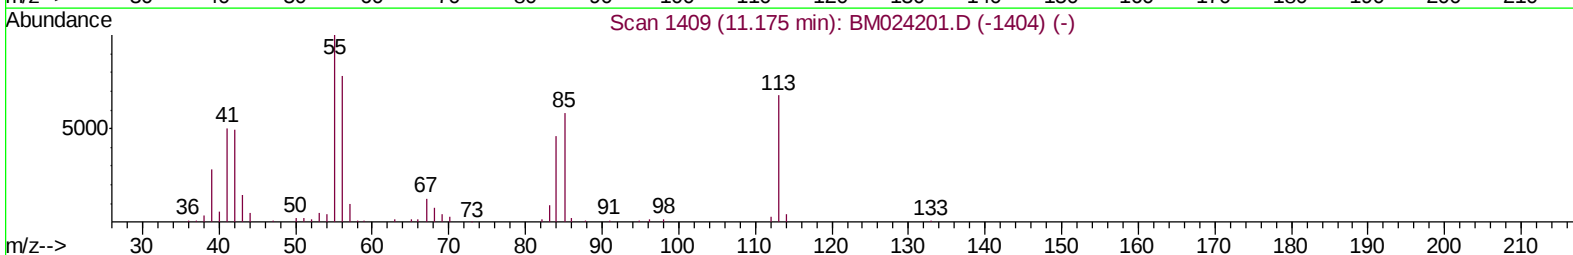
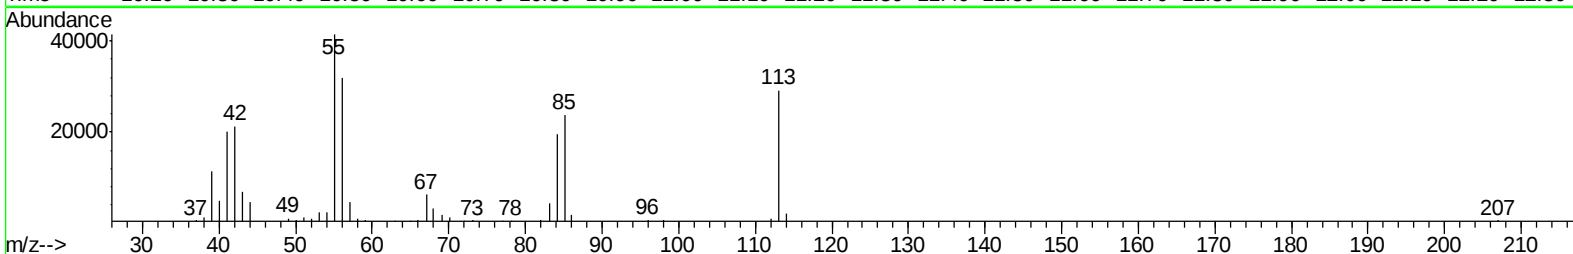


Data File : BM024203.D
Acq On : 20 Dec 2019 14:52
Operator : JU
Sample : K4649-03MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Dec 21 00:37:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 21 00:34:28 2019
Response via : Initial Calibration

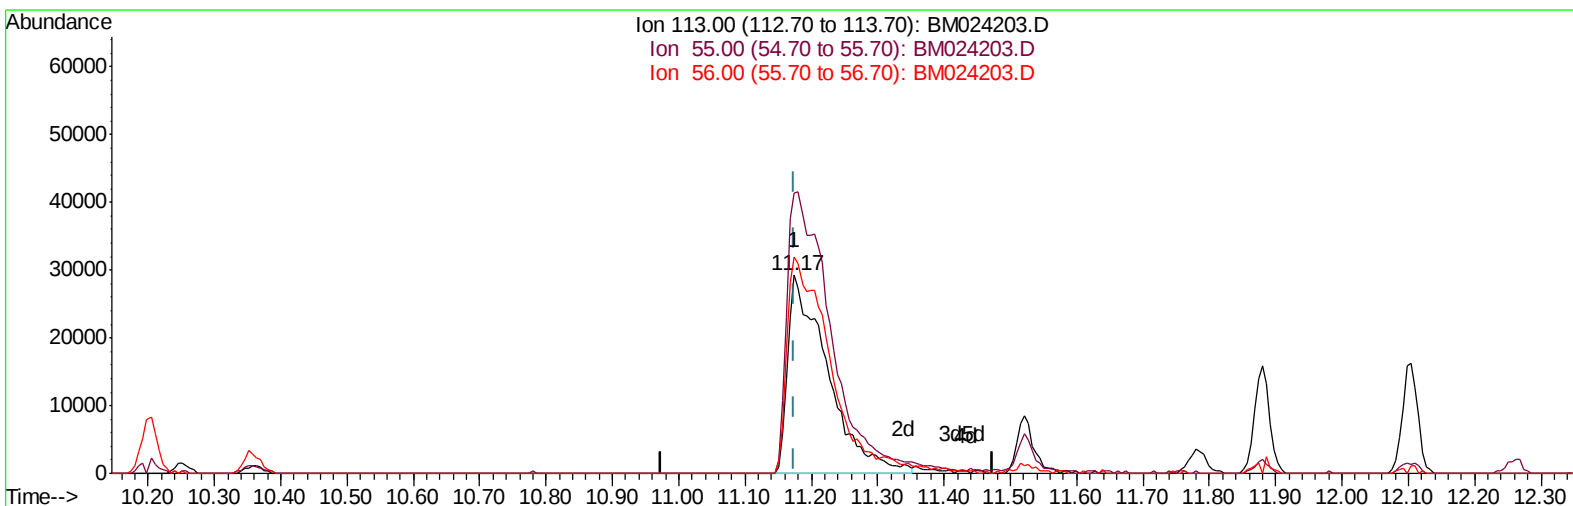

TIC: BM024203.D

(32) Caprolactam

11.175min (+0.000) 17.55ng/ul m

response 120715

Ion	Exp%	Act%
113.00	100	100
55.00	151.30	141.96
56.00	121.00	109.53
0.00	0.00	0.00