
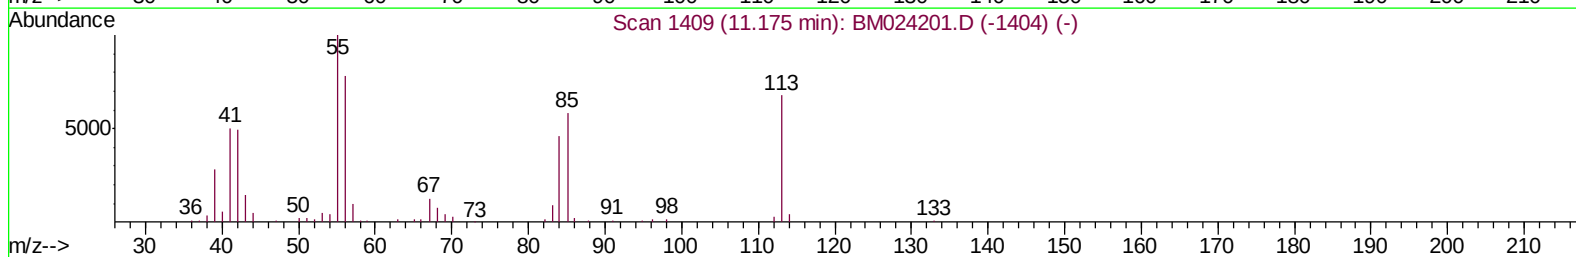
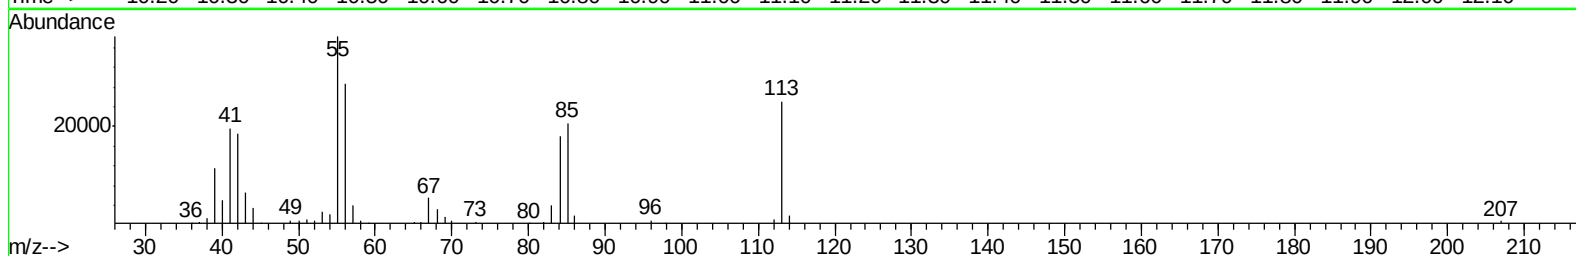


Data File : BM024211.D
Acq On : 20 Dec 2019 19:39
Operator : JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 21 00:40:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 21 00:34:28 2019
Response via : Initial Calibration

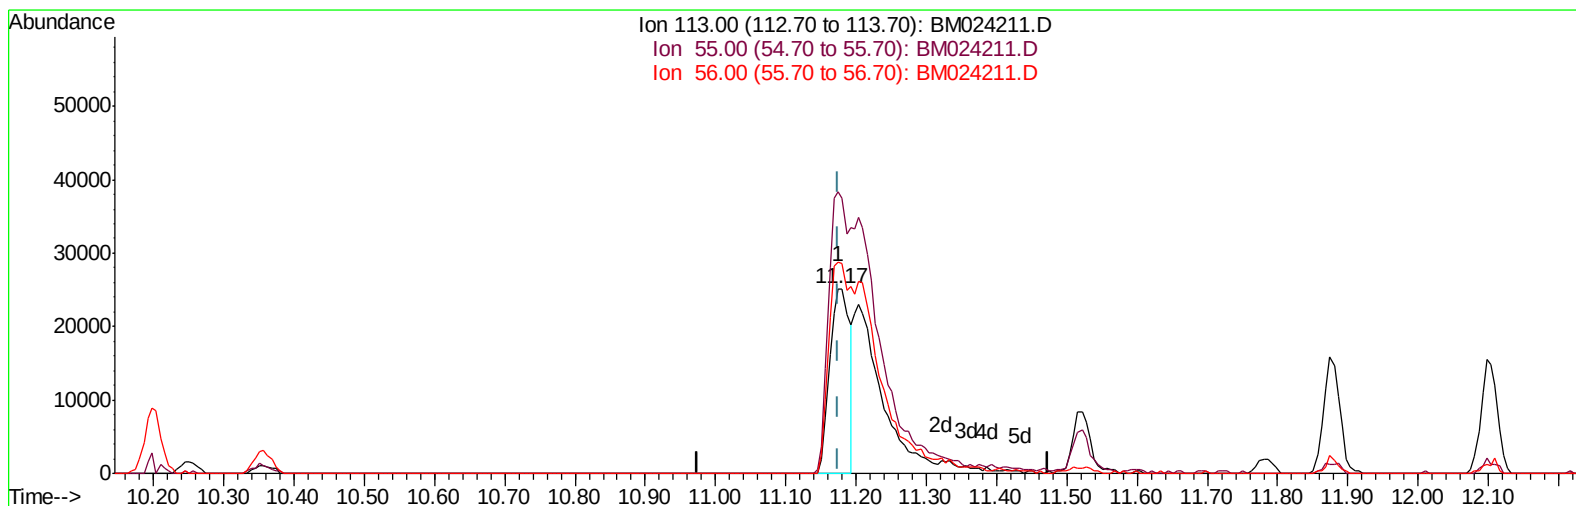

TIC: BM024211.D

(32) Caprolactam

11.174min (-0.000) 6.89ng/ul

response 49308

Ion	Exp%	Act%
113.00	100	100
55.00	151.30	152.58
56.00	121.00	114.67
0.00	0.00	0.00