

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121923\
 Data File : BM043473.D
 Acq On : 20 Dec 2023 20:41
 Operator : MA/JU
 Sample : 05912-03
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3L4

Quant Time: Dec 20 23:15:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.979	152	5762	0.400	ng/ul	0.00
4) Naphthalene-d8	10.785	136	17827	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.611	164	8898	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188	1339115	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.54
23) Perylene-d12	23.947	264	16897	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	25992	3.570	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.374	152	6935	0.275	ng/ul	0.00
18) Fluoranthene-d10	19.376	212	12993	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.419	88	672	0.092	ng/ul#	59
26) Benzo(a)pyrene	23.795	252	5087	0.080	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121923\
Data File : BM043473.D
Acq On : 20 Dec 2023 20:41
Operator : MA/JU
Sample : 05912-03
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3L4

Quant Time: Dec 20 23:15:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration




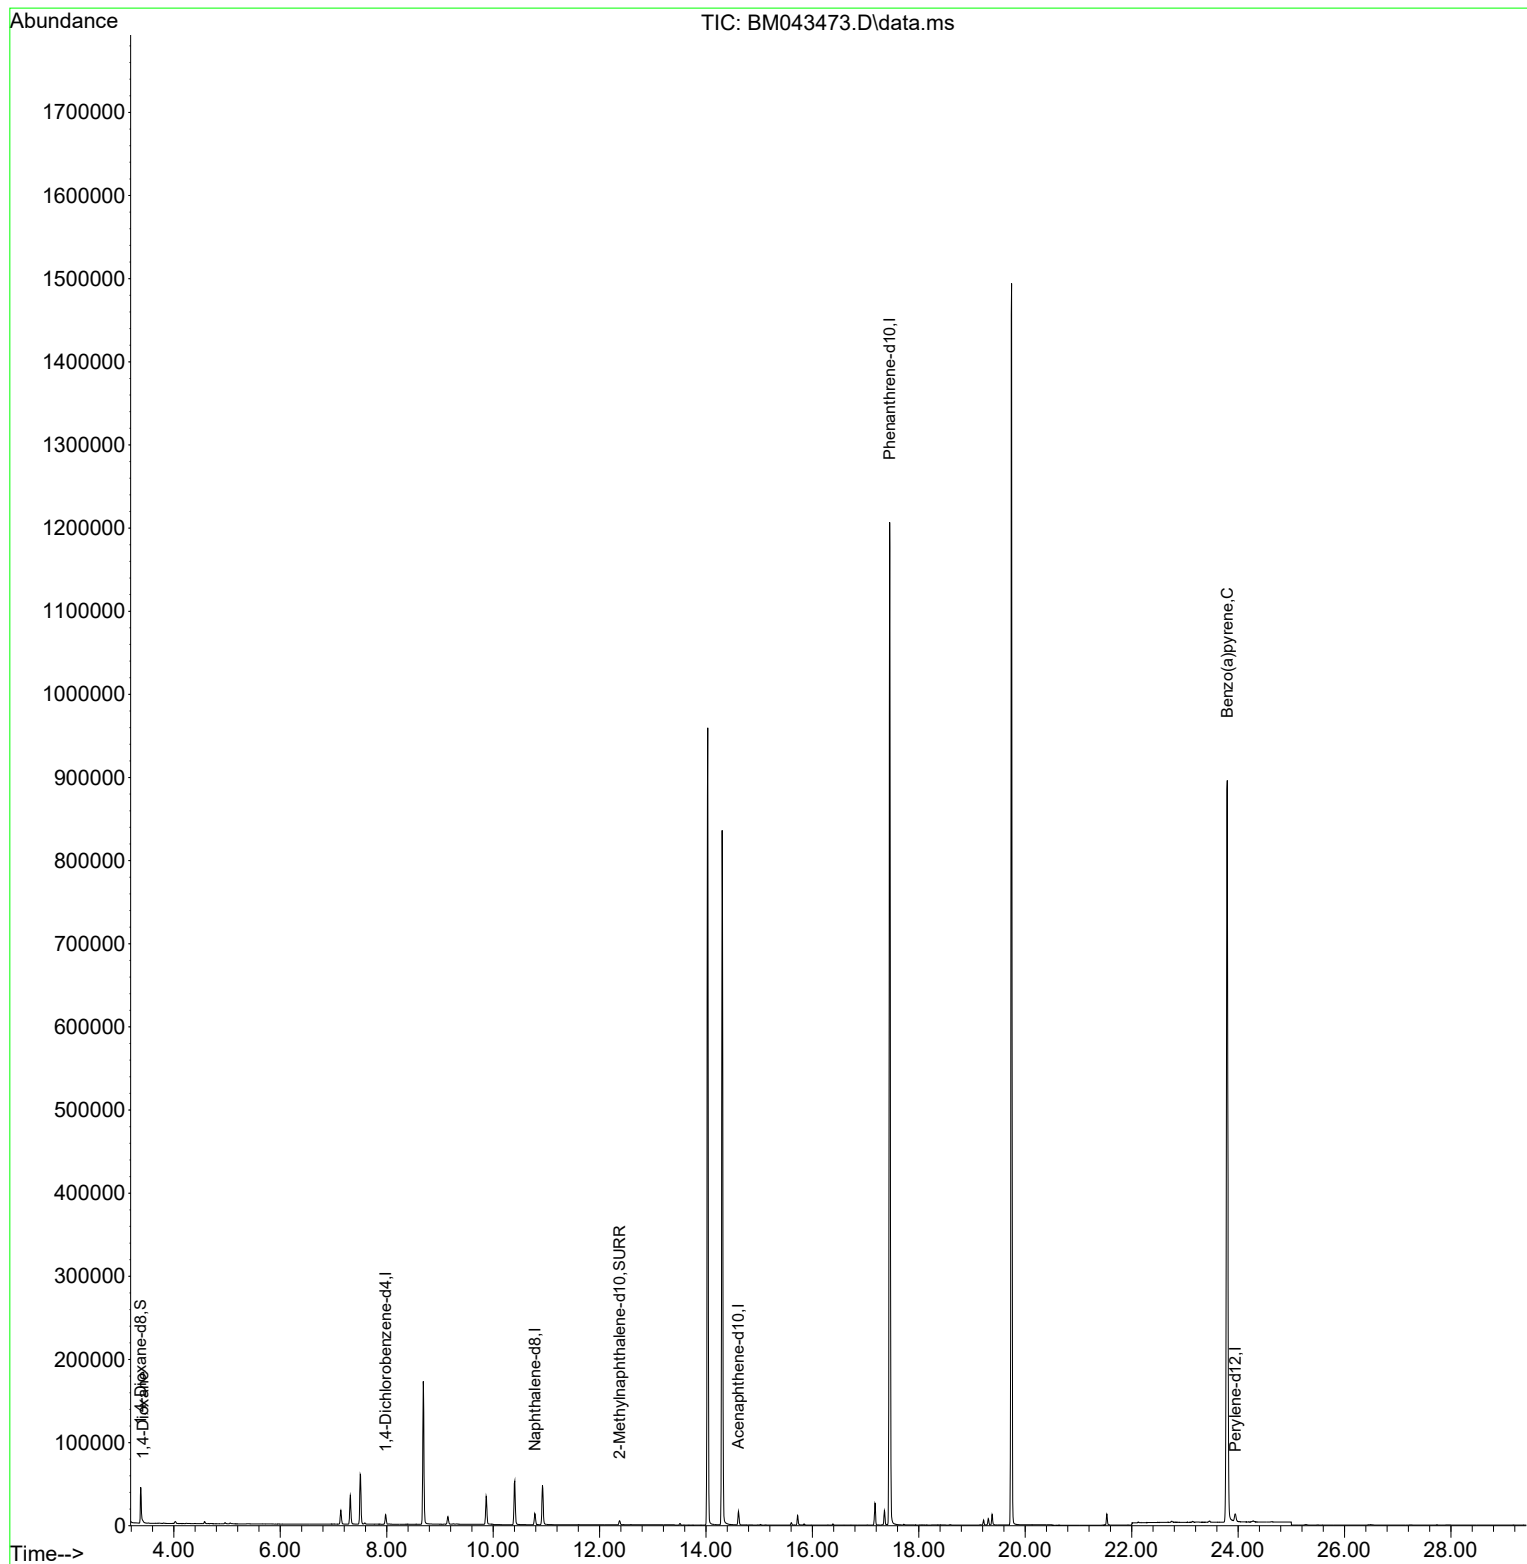


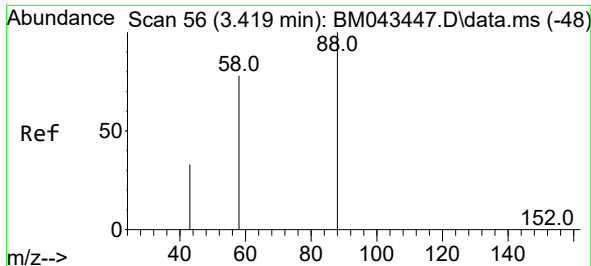

#2
1,4-Dioxane
Concen: 0.092 ng/ul
RT: 3.419 min Scan# 50
Delta R.T. -0.000 min
Lab File: BM043473.D
Acq: 20 Dec 2023 20:41

Instrument :
BNA_M
ClientSampleId :
BH3L4

Tgt Ion: 88 Resp: 672
Ion Ratio Lower Upper
88 100
43 75.8 27.9 41.9#
58 38.5 43.4 65.2#

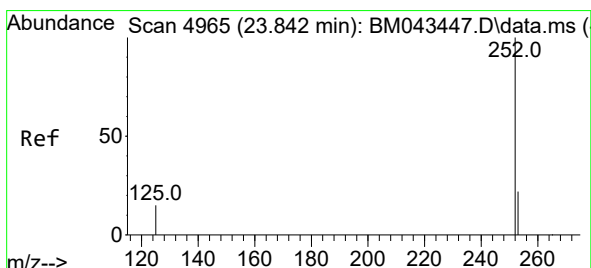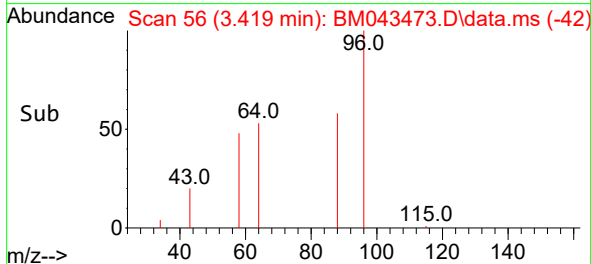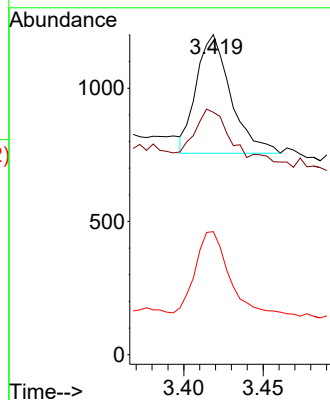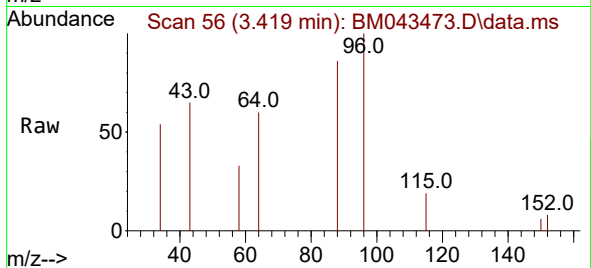

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.795 min Scan# 4949
Delta R.T. -0.053 min
Lab File: BM043473.D
Acq: 20 Dec 2023 20:41

Tgt Ion: 252 Resp: 5087
Ion Ratio Lower Upper
252 100
253 46.4 20.2 30.2#
125 46.4 13.5 20.3#

