

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121923\
 Data File : BM043491.D
 Acq On : 21 Dec 2023 08:04
 Operator : MA/JU
 Sample : 05912-18
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 22 00:05:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.979	152	6598	0.400	ng/ul	0.00
4) Naphthalene-d8	10.785	136	21520	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.611	164	11361	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188	1583920	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.54
23) Perylene-d12	23.942	264	22205	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.377	96	23511	2.820	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.374	152	7558	0.248	ng/ul	0.00
18) Fluoranthene-d10	19.376	212	16126	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
25) Benzo(k)fluoranthene	23.208	252	2794	0.027	ng/ul#	1
26) Benzo(a)pyrene	23.787	252	7046	0.085	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121923\
Data File : BM043491.D
Acq On : 21 Dec 2023 08:04
Operator : MA/JU
Sample : 05912-18
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Dec 22 00:05:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration

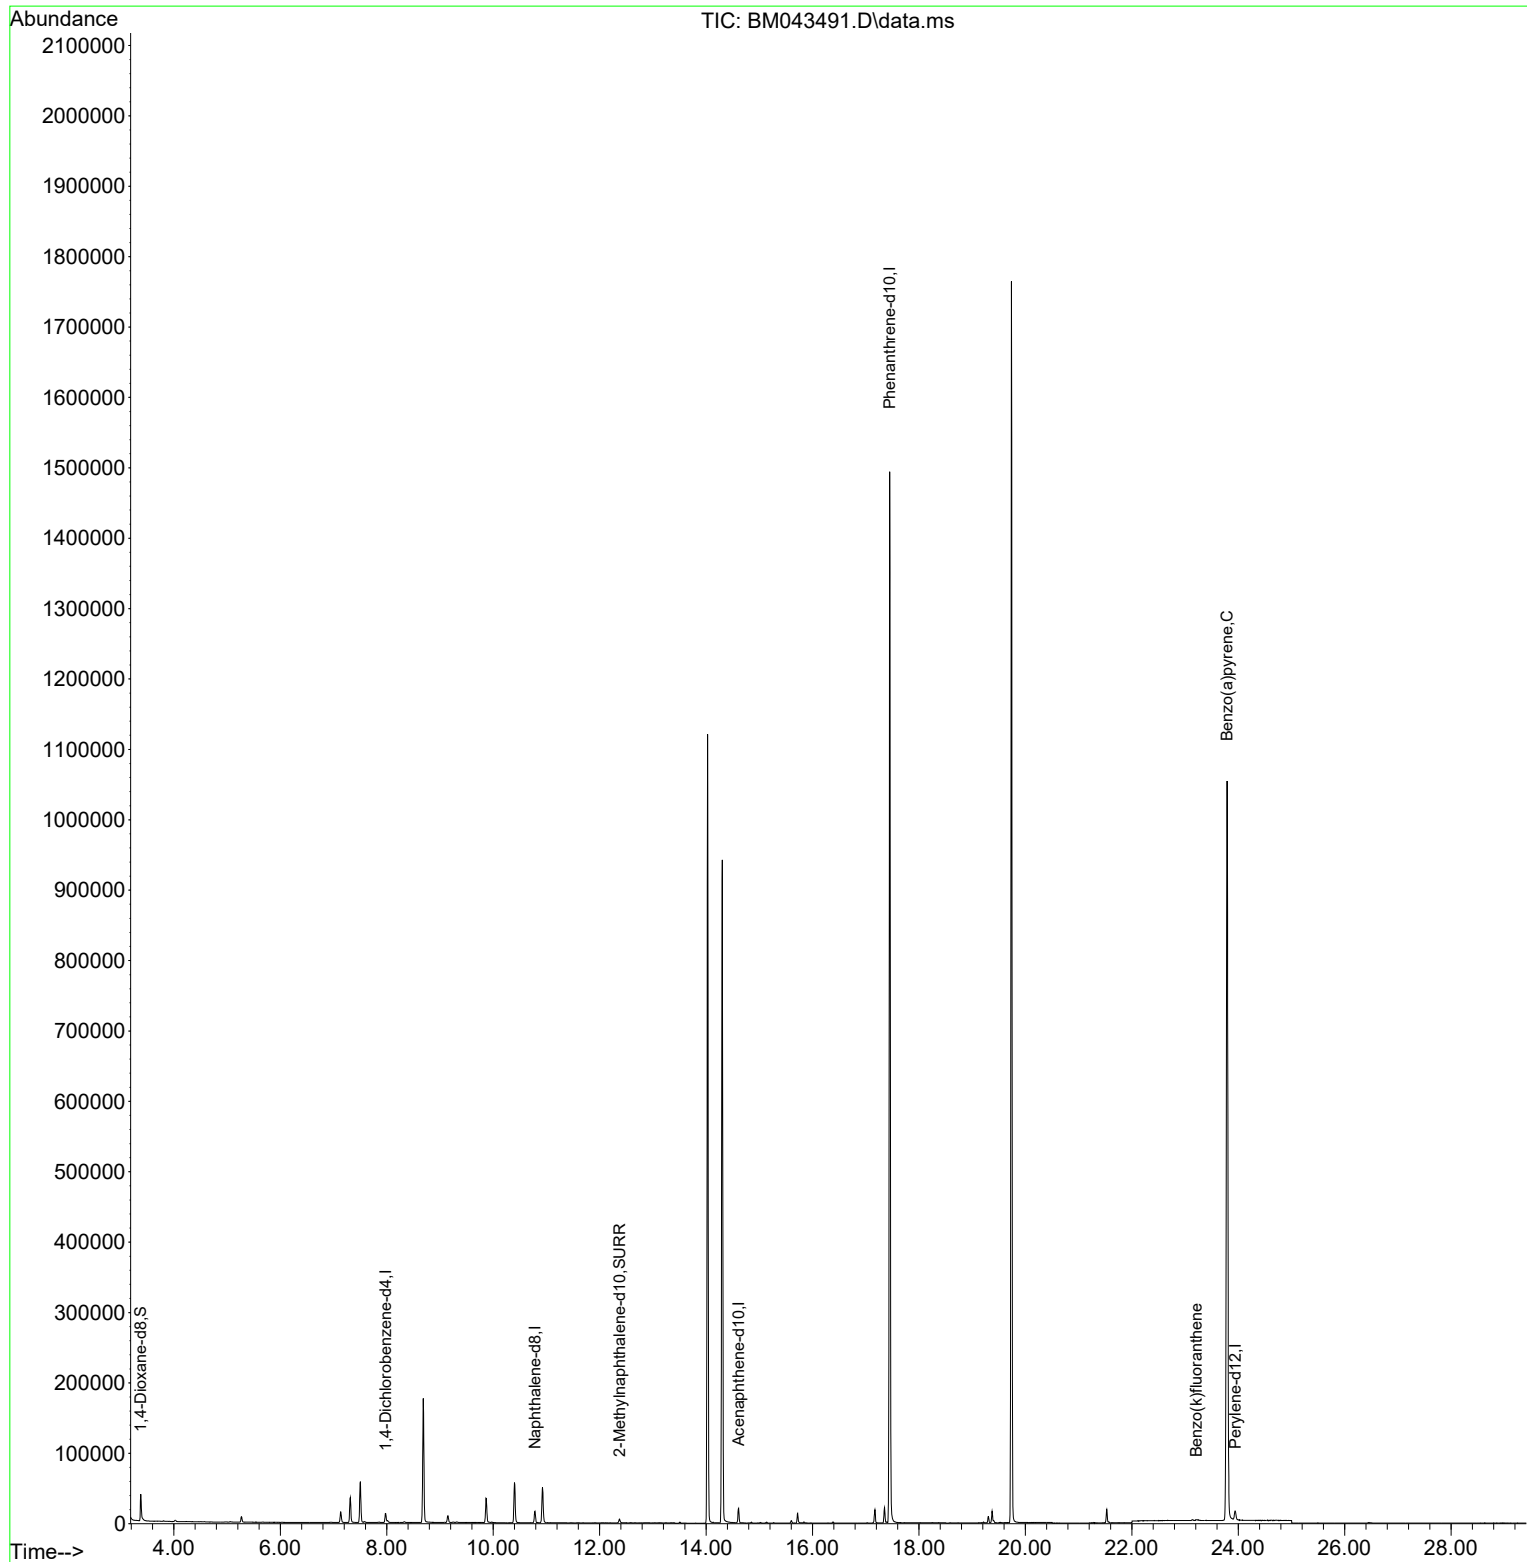


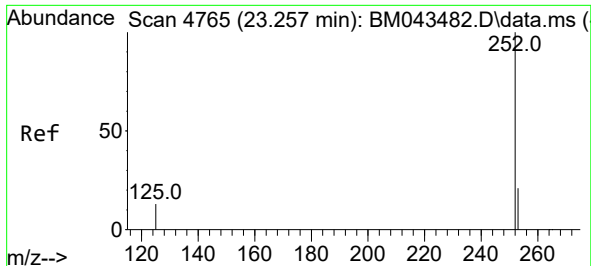


#25
Benzo(k)fluoranthene
Concen: 0.027 ng/ul
RT: 23.208 min Scan# 4765
Delta R.T. -0.058 min
Lab File: BM043491.D
Acq: 21 Dec 2023 08:04

Instrument :
BNA_M
ClientSampleId :

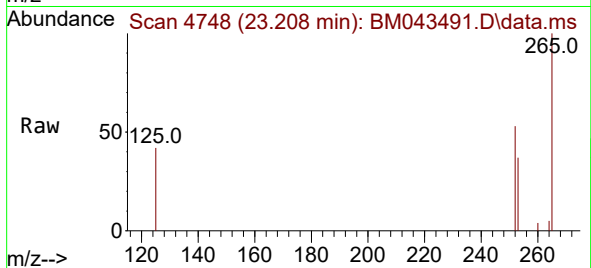

Tgt Ion:252 Resp: 2794
Ion Ratio Lower Upper
252 100
253 70.2 18.6 28.0#
125 78.8 11.8 17.8#

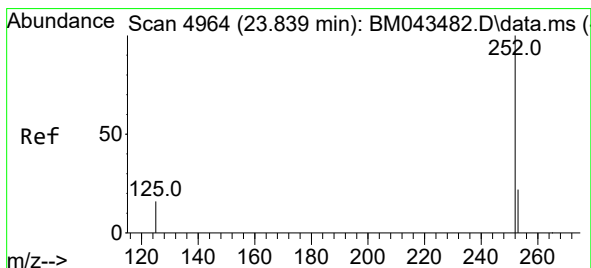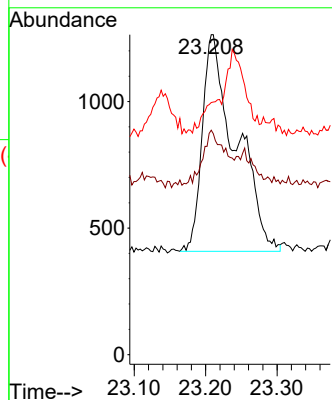

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.787 min Scan# 4946
Delta R.T. -0.061 min
Lab File: BM043491.D
Acq: 21 Dec 2023 08:04

Tgt Ion:252 Resp: 7046
Ion Ratio Lower Upper
252 100
253 46.5 20.2 30.2#
125 48.2 13.5 20.3#

