

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121923\
 Data File : BM043492.D
 Acq On : 21 Dec 2023 08:40
 Operator : MA/JU
 Sample : 05912-19
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 22 00:05:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.979	152	5813	0.400	ng/ul	0.00
4) Naphthalene-d8	10.785	136	18325	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.610	164	9527	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188	1298437	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.54
23) Perylene-d12	23.941	264	17920	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	22580	3.074	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.374	152	6578	0.253	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	12774	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.418	88	662	0.090	ng/ul#	47
26) Benzo(a)pyrene	23.789	252	4803	0.072	ng/ul#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121923\
Data File : BM043492.D
Acq On : 21 Dec 2023 08:40
Operator : MA/JU
Sample : 05912-19
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Dec 22 00:05:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration

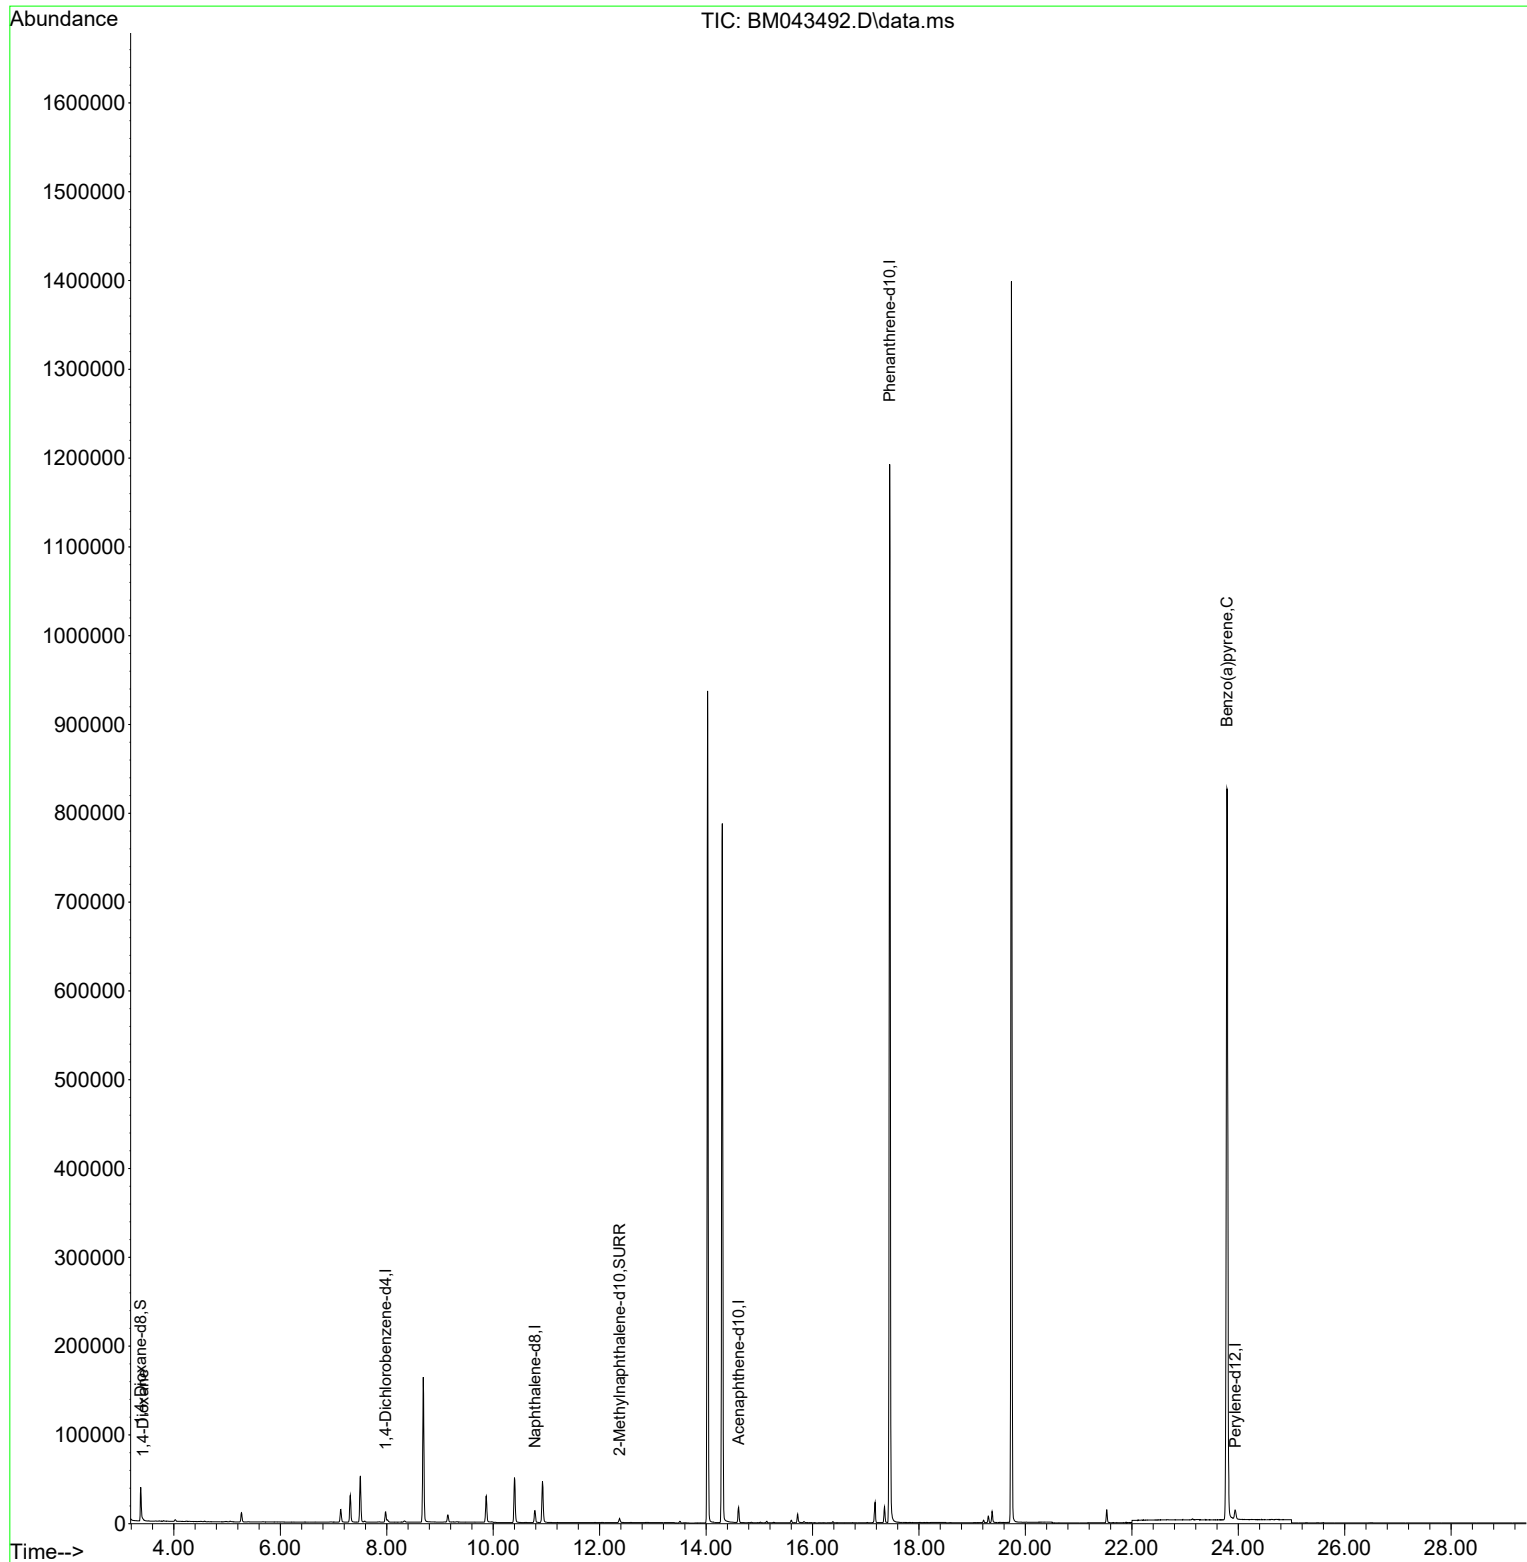



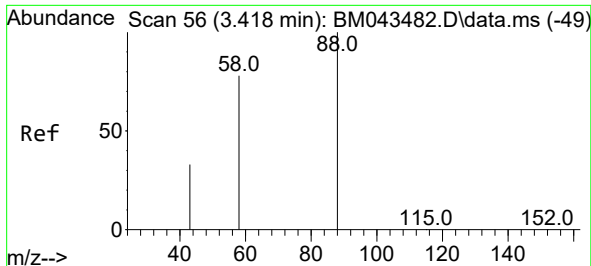


#2
1,4-Dioxane
Concen: 0.090 ng/ul
RT: 3.418 min Scan# 50
Delta R.T. -0.000 min
Lab File: BM043492.D
Acq: 21 Dec 2023 08:40


Instrument :
BNA_M
ClientSampleId :

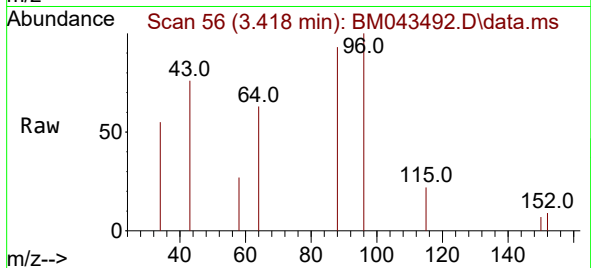

Tgt Ion: 88 Resp: 662
Ion Ratio Lower Upper
88 100
43 82.4 27.9 41.9#
58 29.1 43.4 65.2#

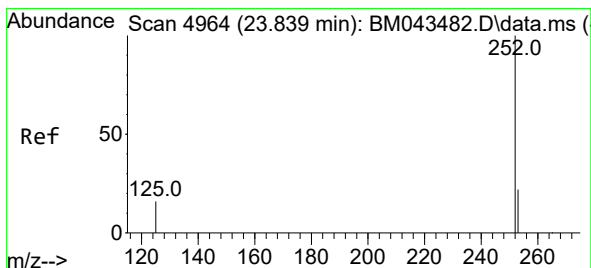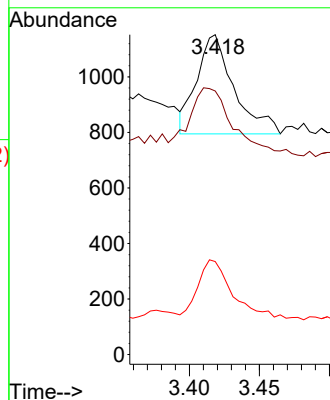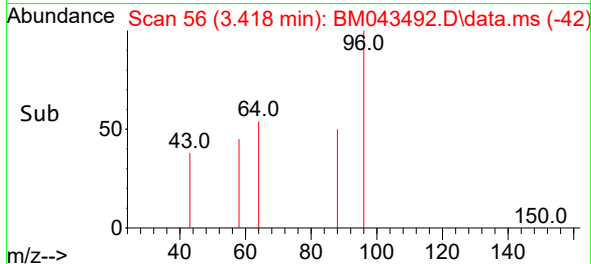

#26
Benzo(a)pyrene
Concen: 0.072 ng/ul
RT: 23.789 min Scan# 4947
Delta R.T. -0.059 min
Lab File: BM043492.D
Acq: 21 Dec 2023 08:40

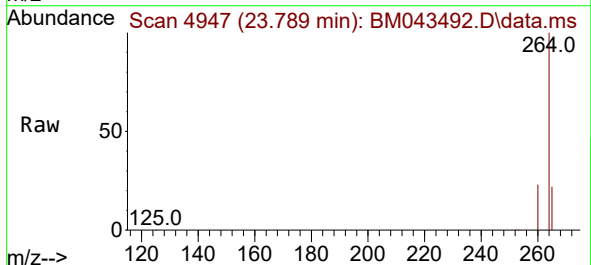

Tgt Ion: 252 Resp: 4803
Ion Ratio Lower Upper
252 100
253 49.9 20.2 30.2#
125 51.4 13.5 20.3#

