

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121923\
 Data File : BM043433.D
 Acq On : 19 Dec 2023 18:53
 Operator : MA/JU
 Sample : 05830-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AD0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/22/2023

Quant Time: Dec 19 23:36:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.983	152	5932	0.400	ng/ul	0.00
4) Naphthalene-d8	10.790	136	17968	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.615	164	9163	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.358	188	18541m	0.400	ng/ul	0.00
17) Chrysene-d12	21.536	240	13632m	0.400	ng/ul	0.00
23) Perylene-d12	23.950	264	18163	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	39937	5.328	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.379	152	8339	0.328	ng/ul	0.00
18) Fluoranthene-d10	19.380	212	15805	0.325	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.414	88	230886	30.716	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121923\
Data File : BM043433.D
Acq On : 19 Dec 2023 18:53
Operator : MA/JU
Sample : 05830-06
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
H0AD0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/20/2023
Supervised By :mohammad ahmed 12/22/2023


Quant Time: Dec 19 23:36:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration

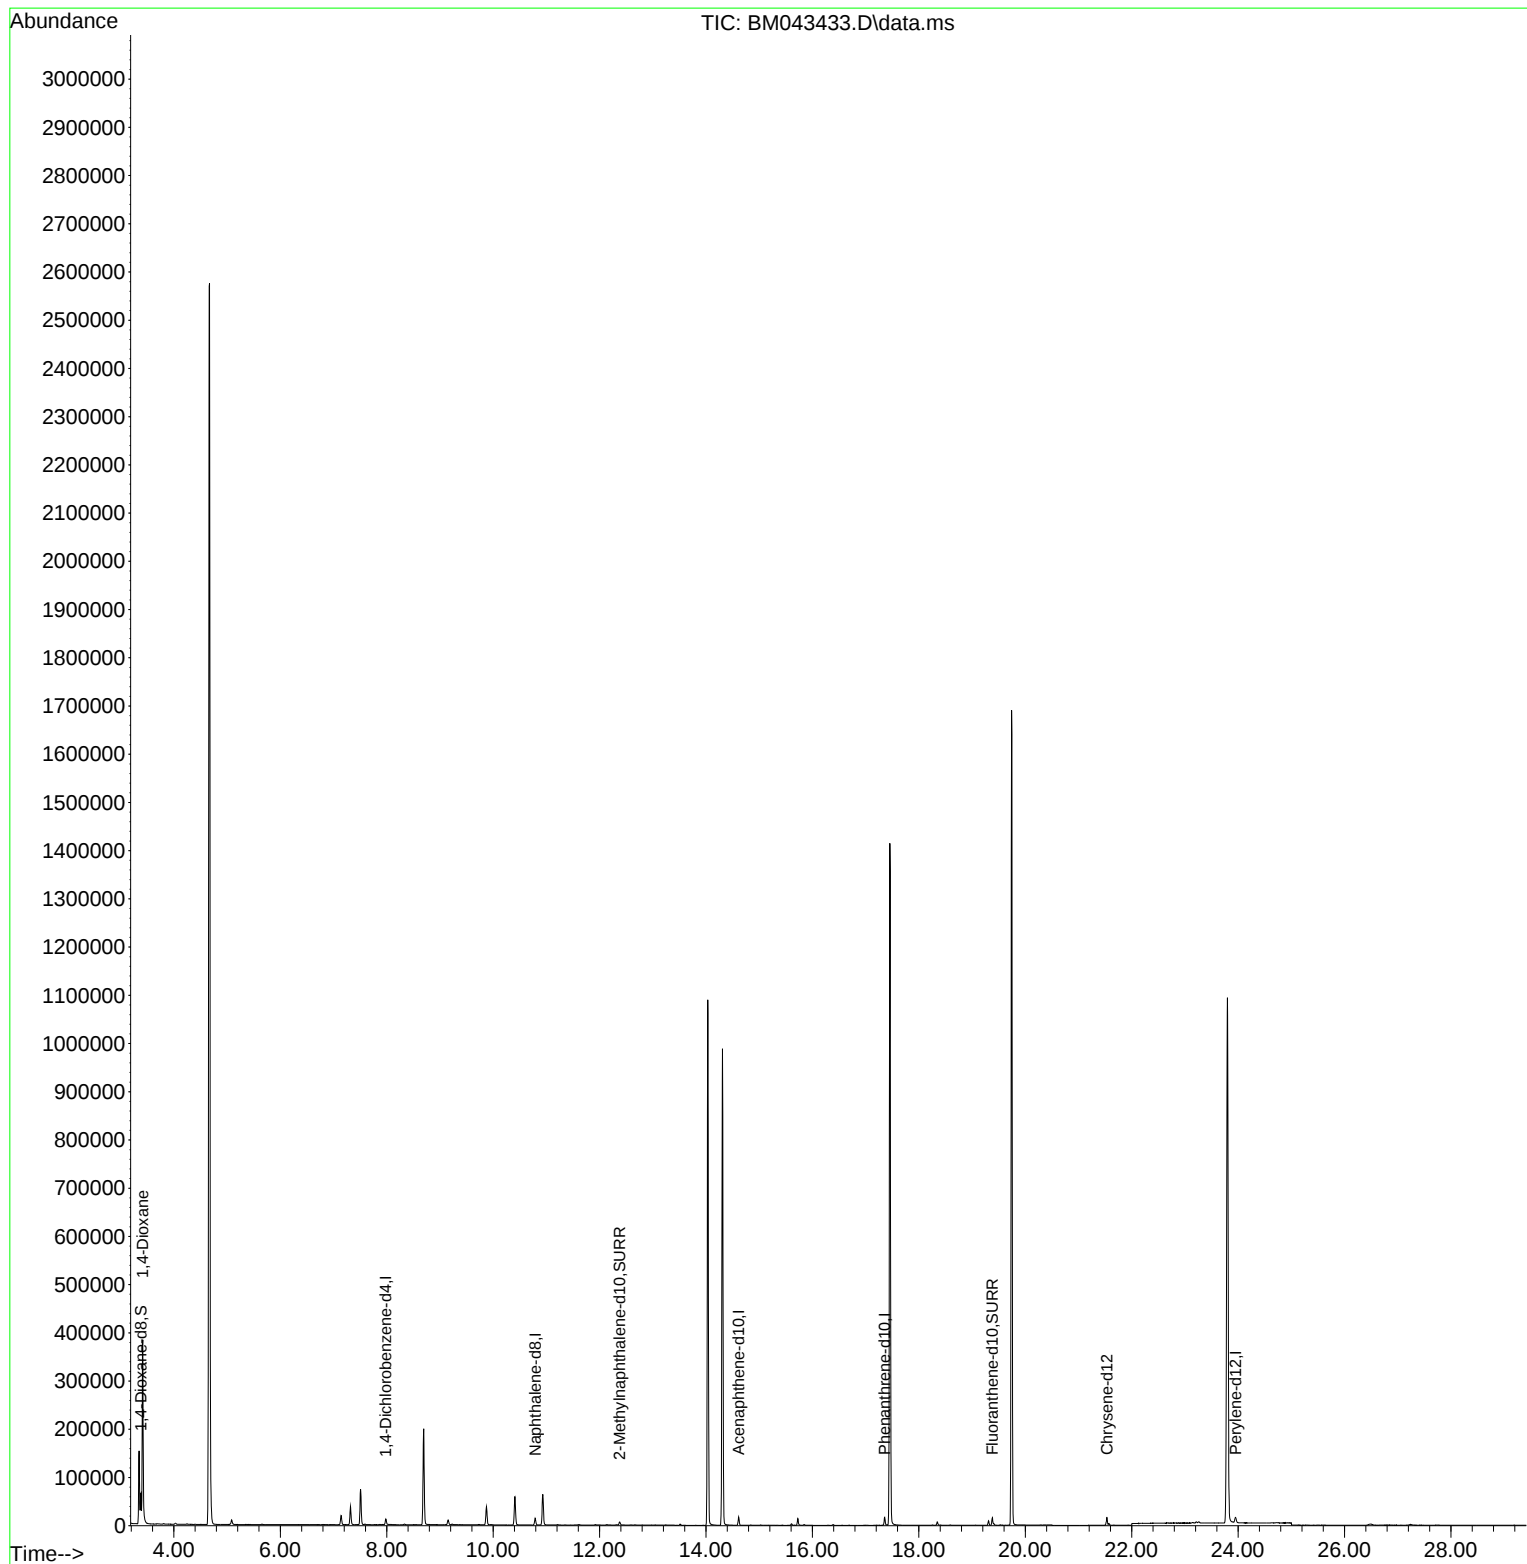

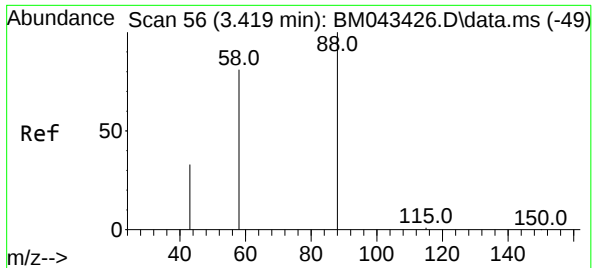

#2
 1,4-Dioxane
 Concen: 30.716 ng/ul
 RT: 3.414 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM043433.D
 Acq: 19 Dec 2023 18:53

Instrument :
 BNA_M
 ClientSampleId :
 H0AD0

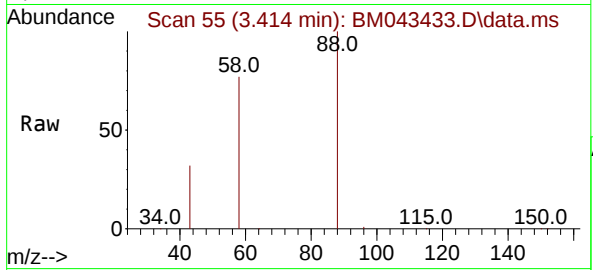

Tgt Ion: 88 Resp: 230880
 Ion Ratio Lower Upper
 88 100
 43 32.2 27.9 41.9
 58 76.7 43.4 65.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/22/2023

