




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

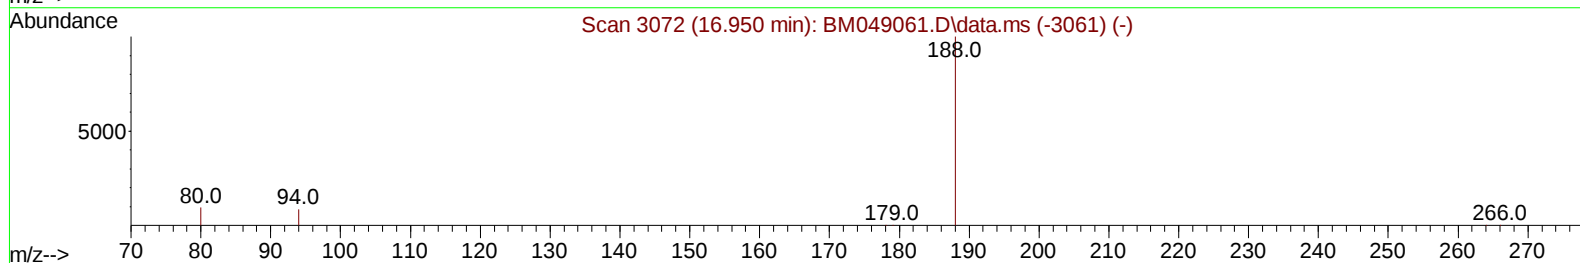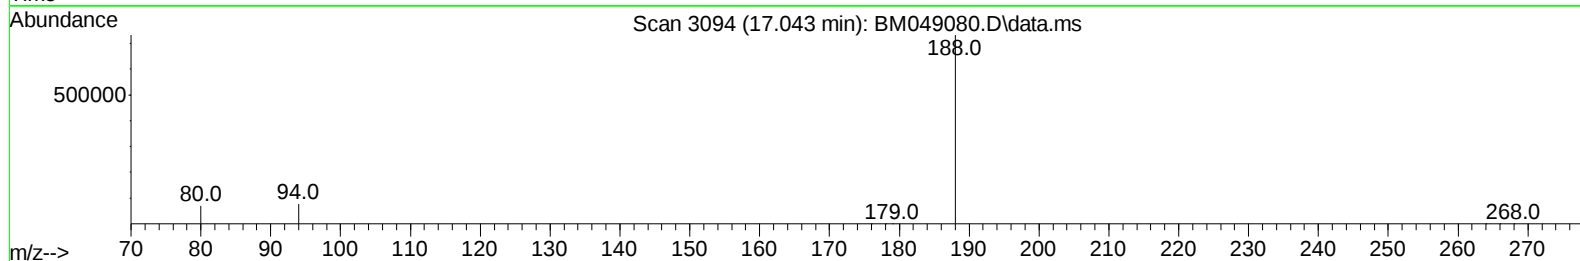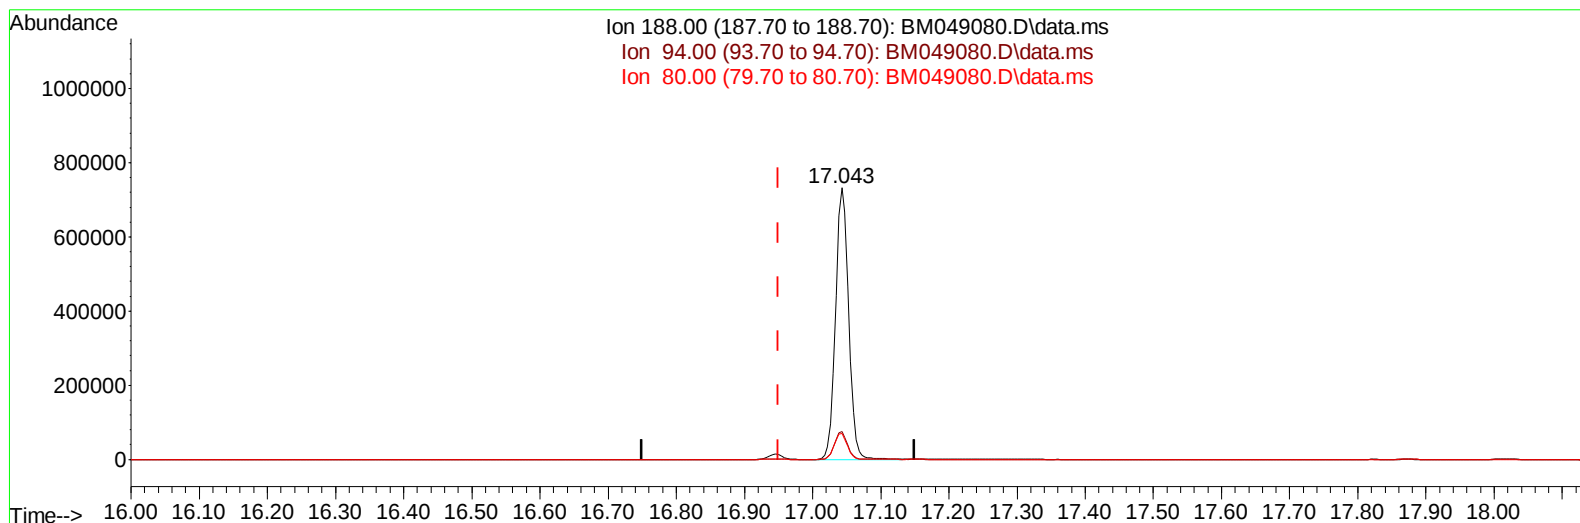

TIC: BM049080.D\data.ms

**(13) Phenanthrene-d10 (I)**

**17.043min (+ 0.093) 0.40 ng/u1**

**response 976040**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 188.00 | 100.00 | 100.00 |
| 94.00  | 9.80   | 10.40  |
| 80.00  | 10.70  | 9.51   |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

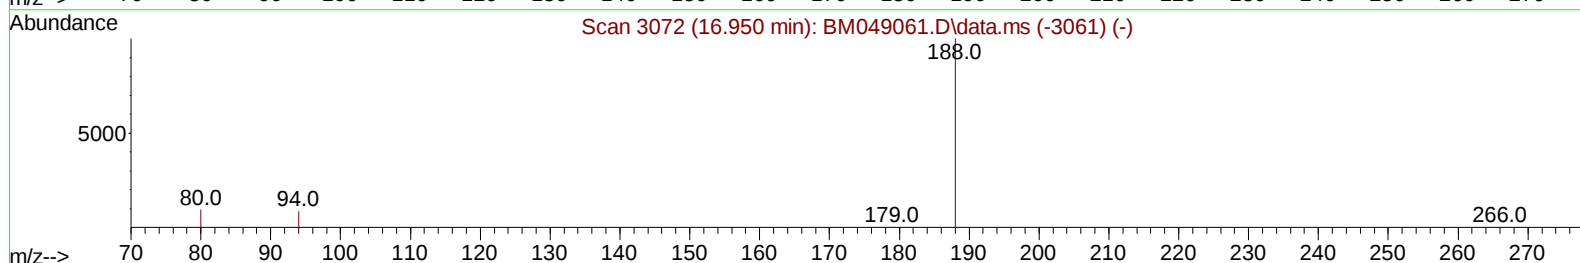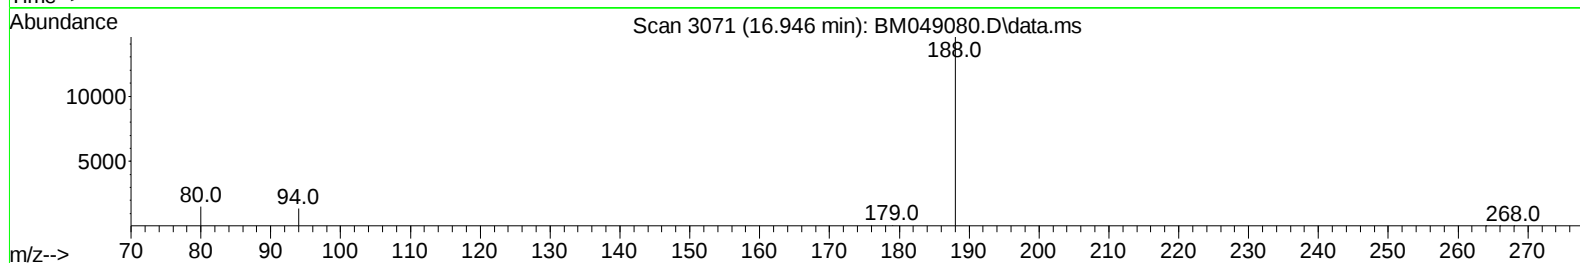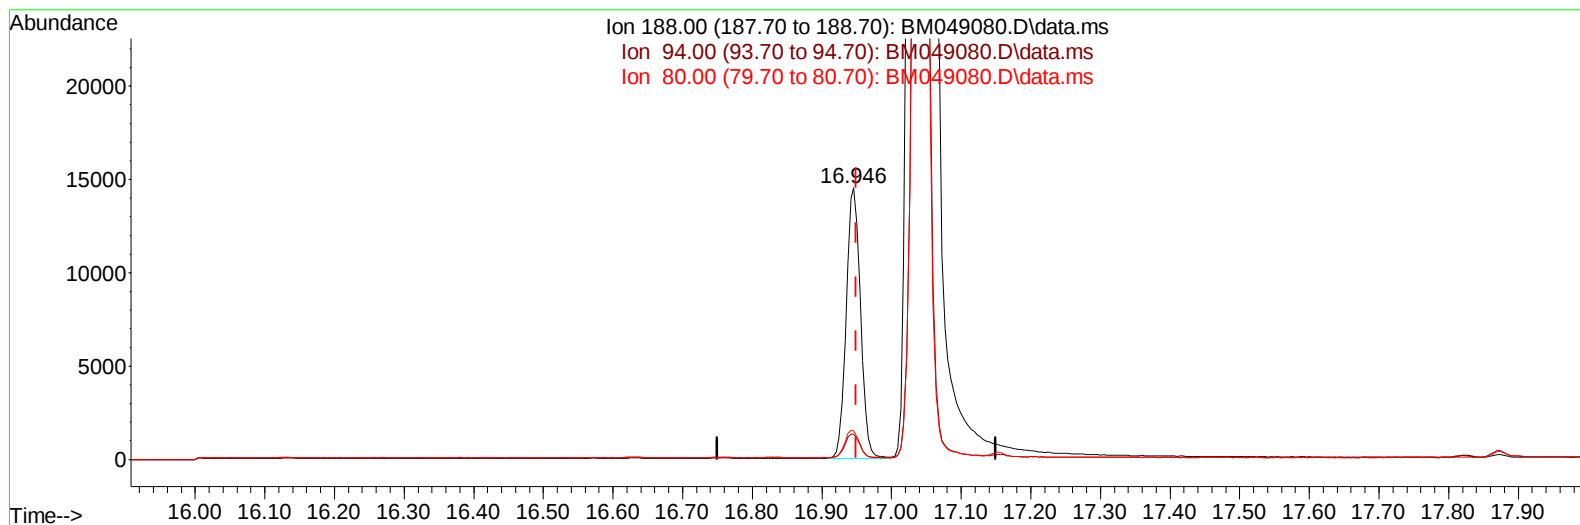

TIC: BM049080.D\data.ms

**(13) Phenanthrene-d10 (I)**

**16.946min (-0.004) 0.40 ng/ul m**

**response 20619**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 188.00 | 100.00 | 100.00 |
| 94.00  | 9.80   | 9.43   |
| 80.00  | 10.70  | 10.41  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

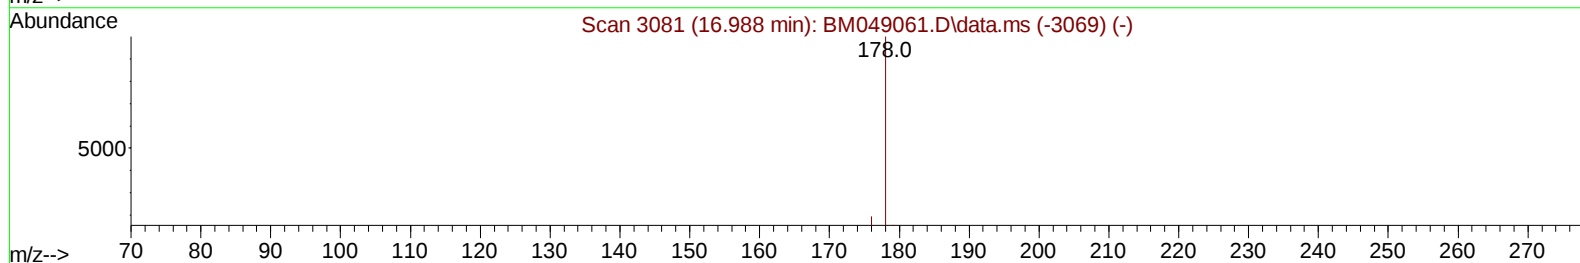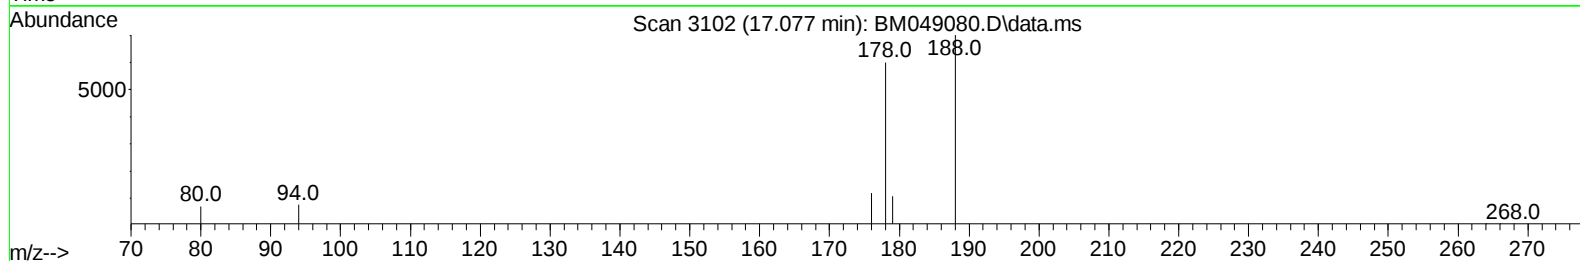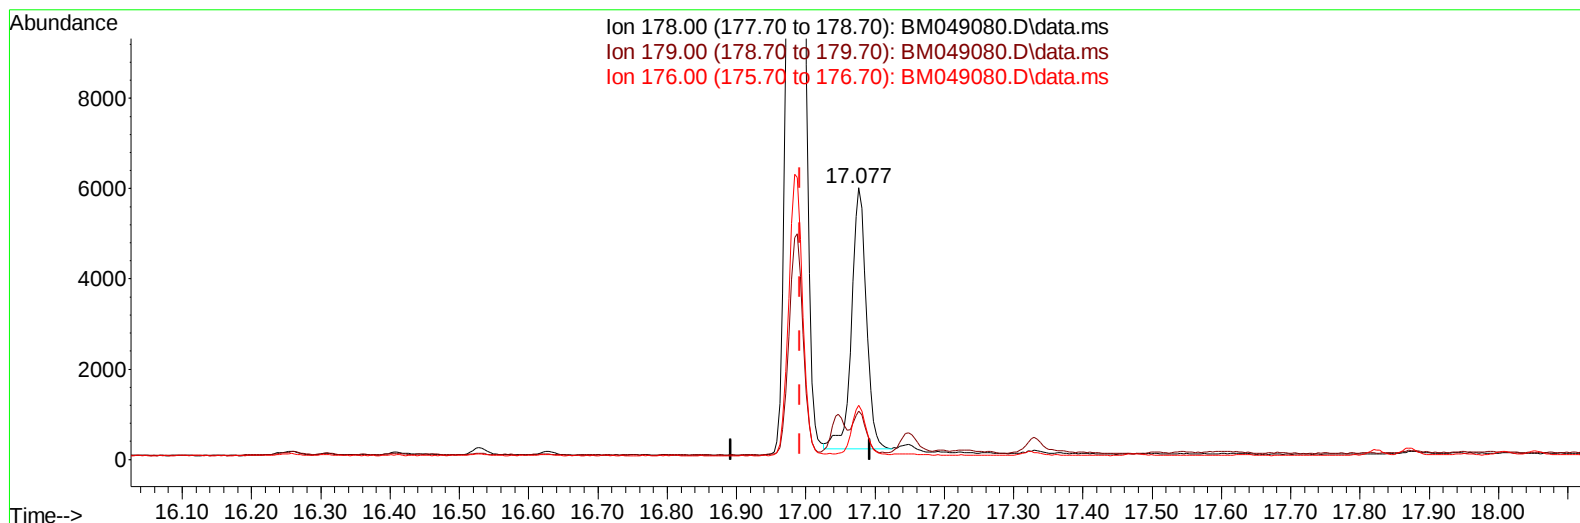

TIC: BM049080.D\data.ms

(15) Phenanthrene

17.077min (+ 0.084) 0.16 ng/u1

response 8603

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 178.00 | 100.00 | 100.00 |
| 179.00 | 16.20  | 17.79  |
| 176.00 | 20.20  | 19.92  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

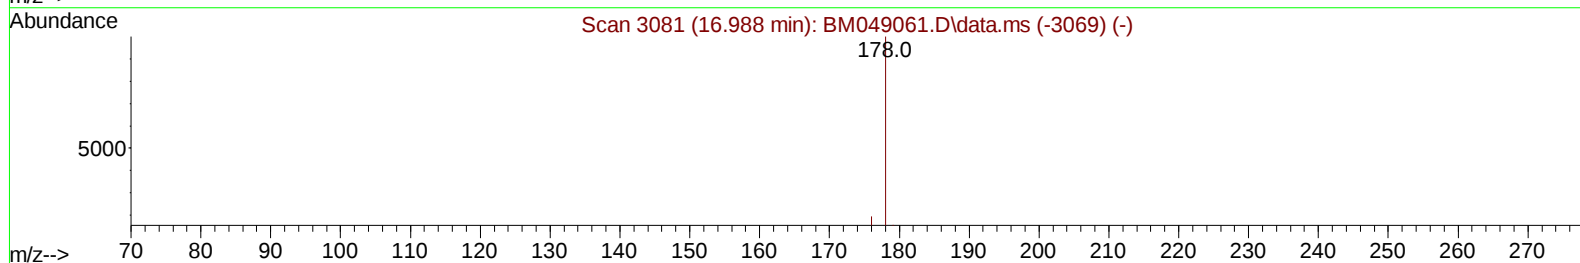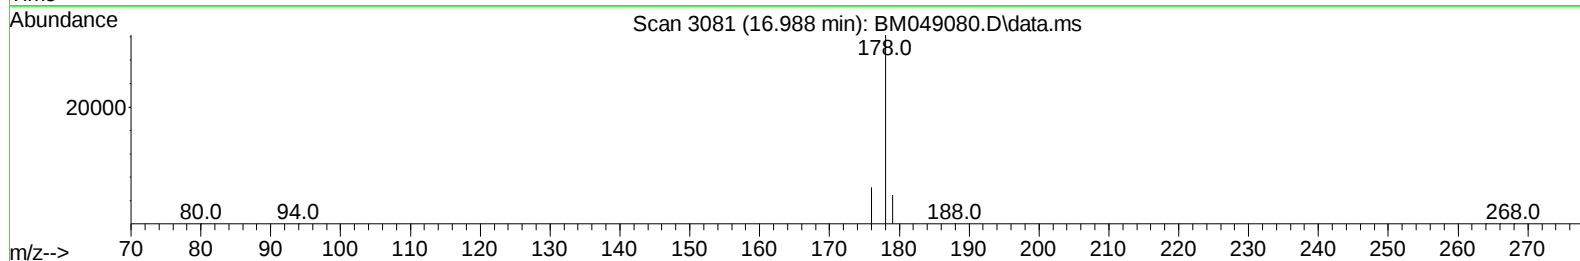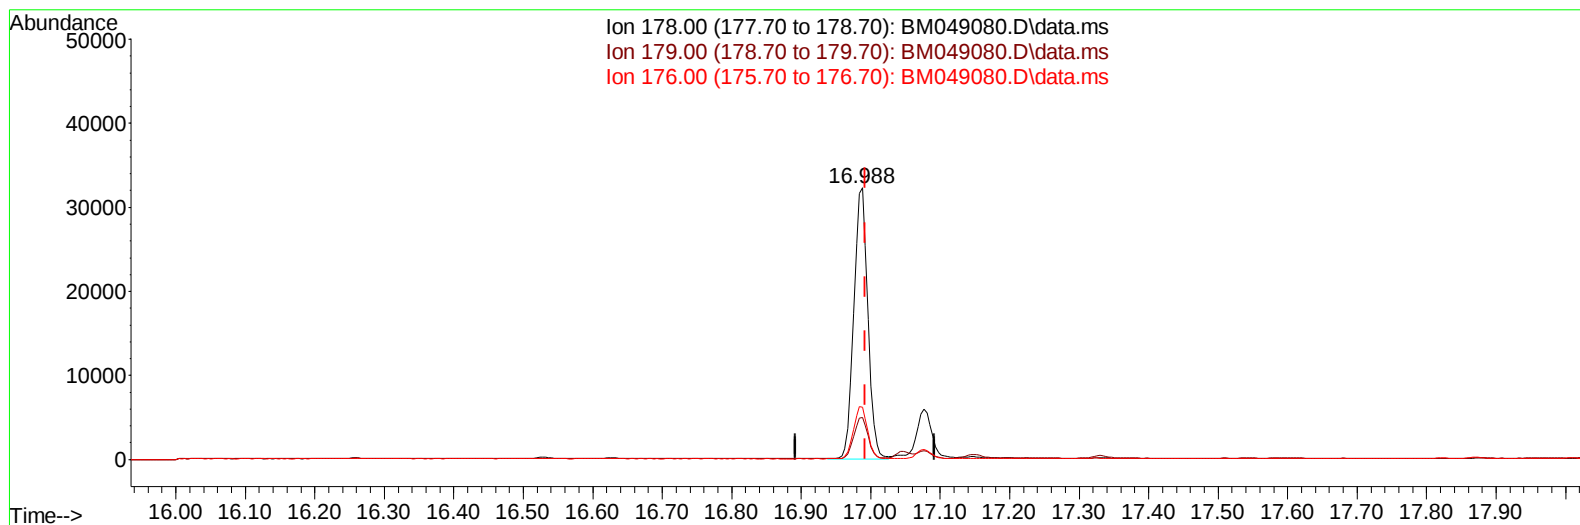

TIC: BM049080.D\data.ms

(15) Phenanthrene

16.988min (-0.004) 0.84 ng/ul m

response 45433

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 178.00 | 100.00 | 100.00 |
| 179.00 | 16.20  | 15.48  |
| 176.00 | 20.20  | 19.35  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

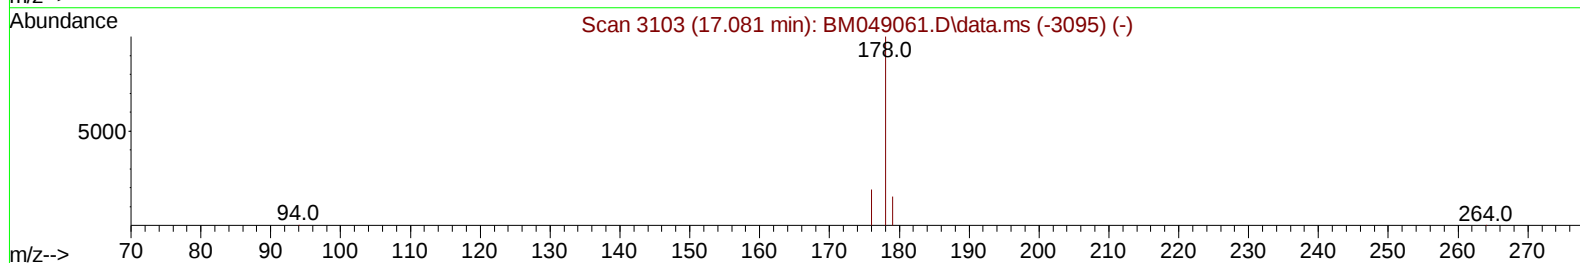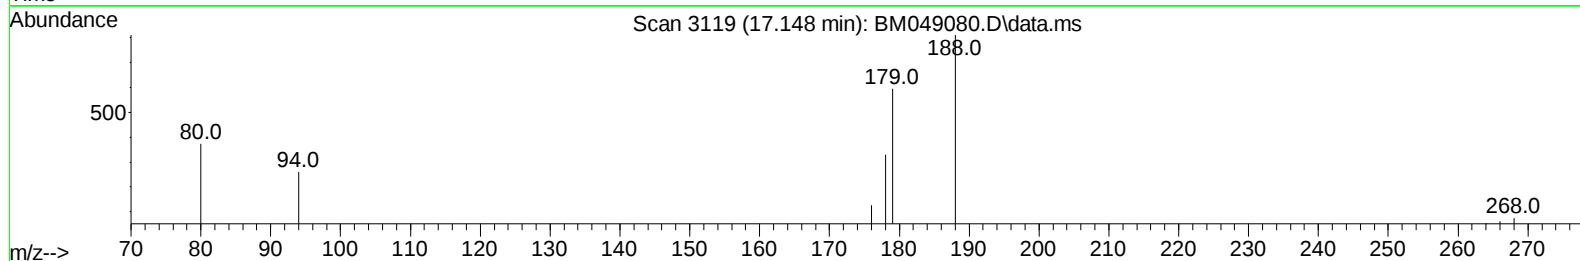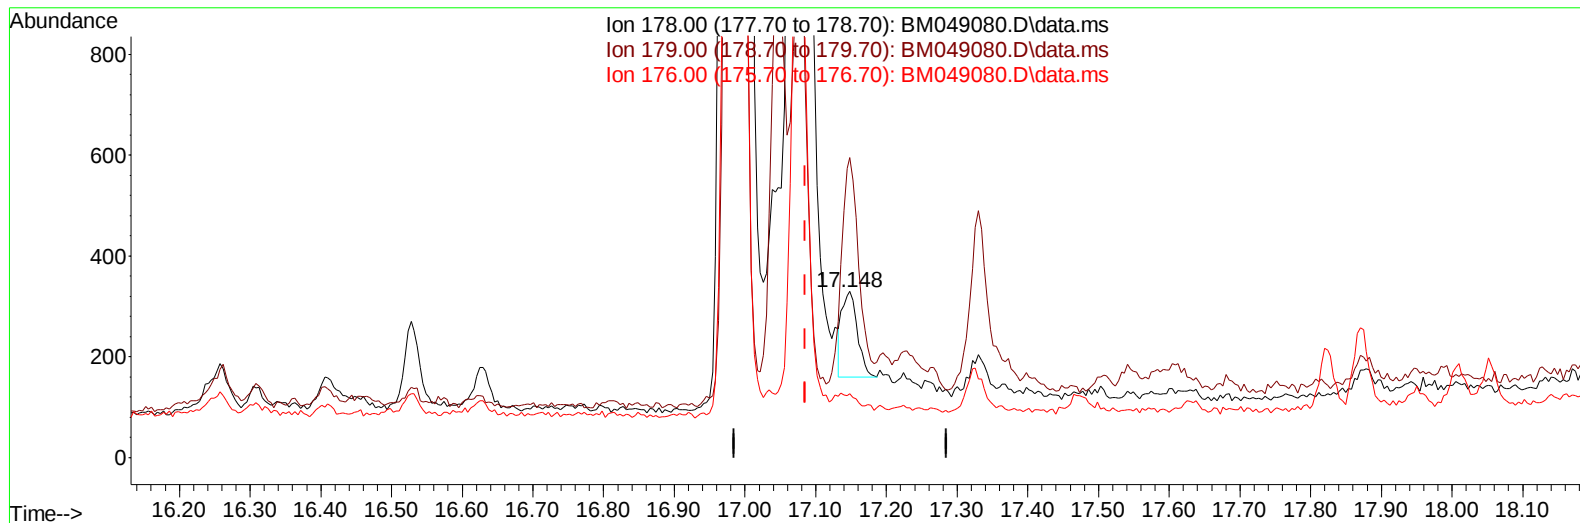

TIC: BM049080.D\data.ms

(16) Anthracene

17.148min (+ 0.063) 0.01 ng/u1

response 261

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 178.00 | 100.00 | 100.00  |
| 179.00 | 16.10  | 180.85# |
| 176.00 | 19.10  | 38.30#  |
| 0.00   | 0.00   | 0.00    |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

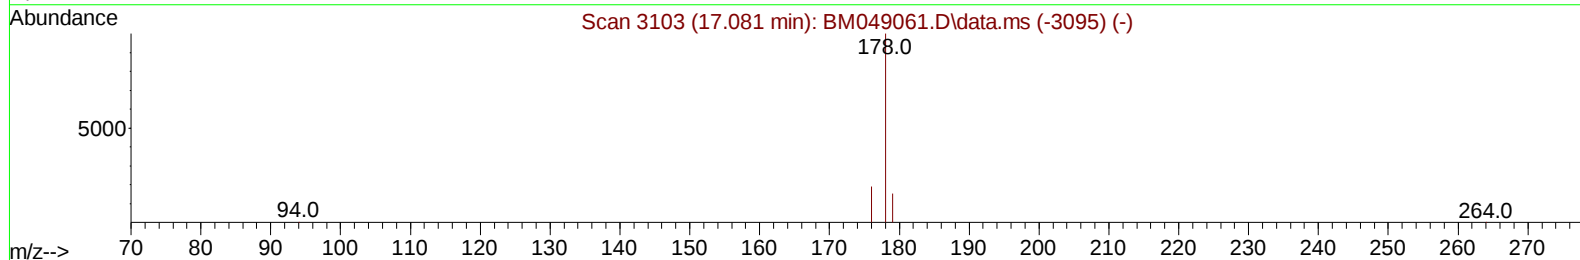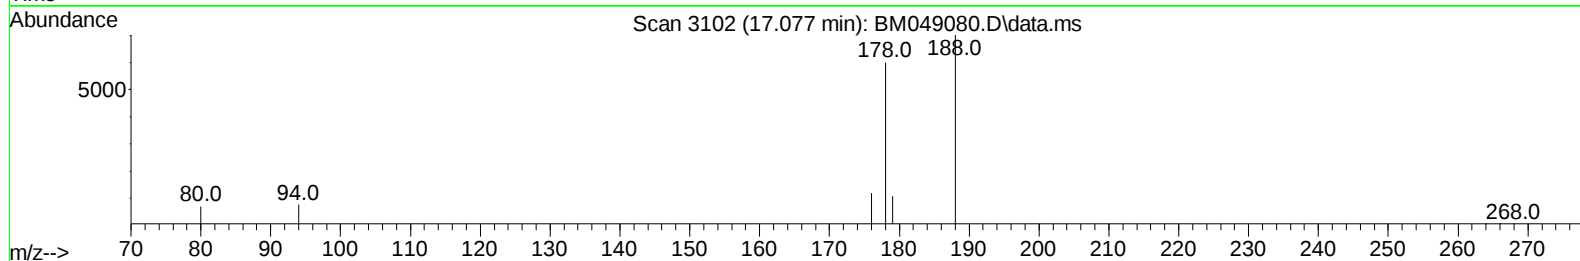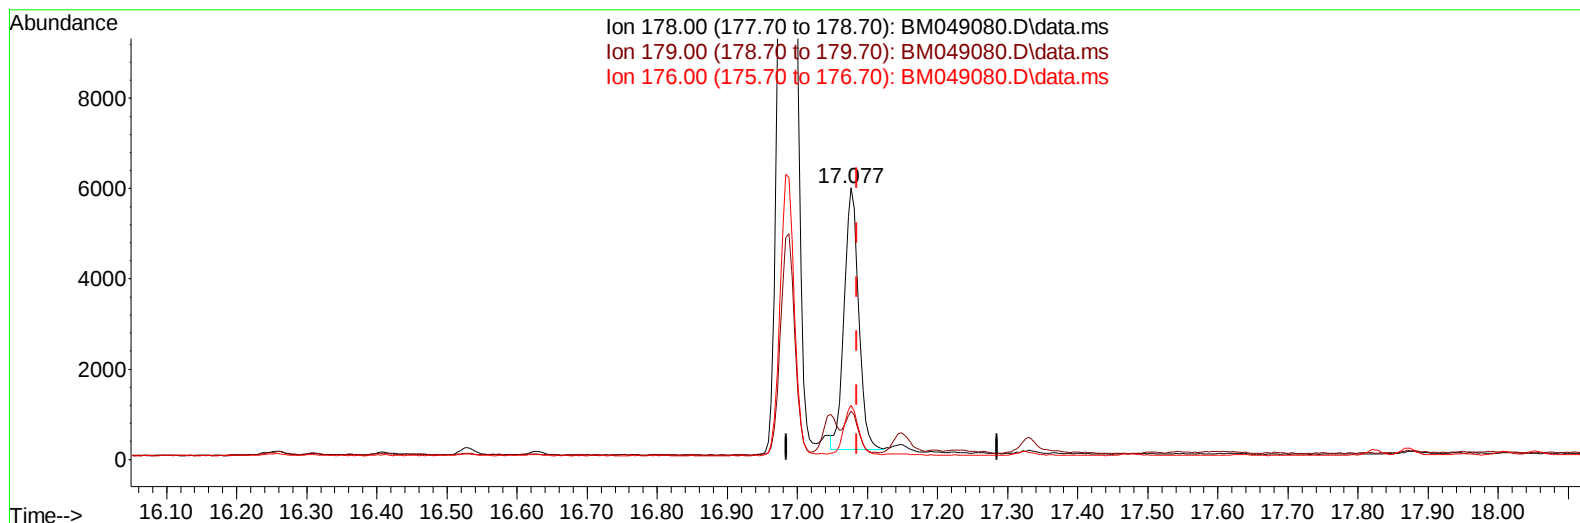

TIC: BM049080.D\data.ms

(16) Anthracene

17.077min (-0.008) 0.17 ng/ul m

response 8349

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 178.00 | 100.00 | 100.00 |
| 179.00 | 16.10  | 17.79  |
| 176.00 | 19.10  | 19.92  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

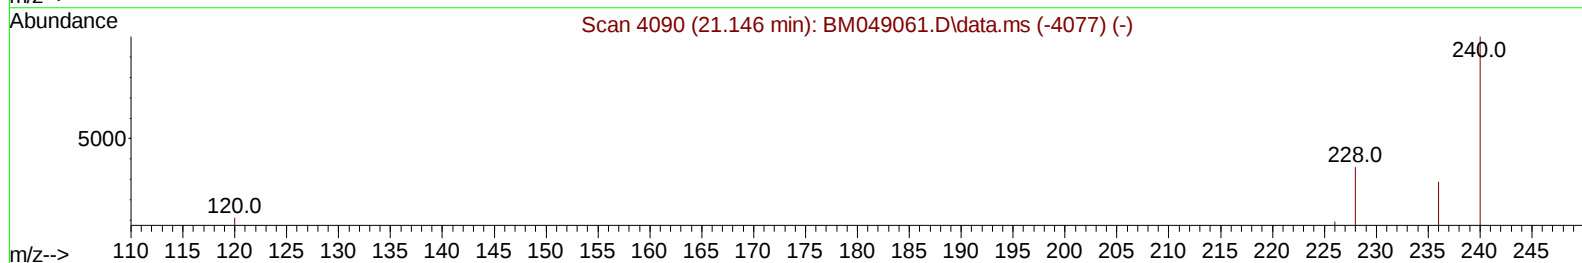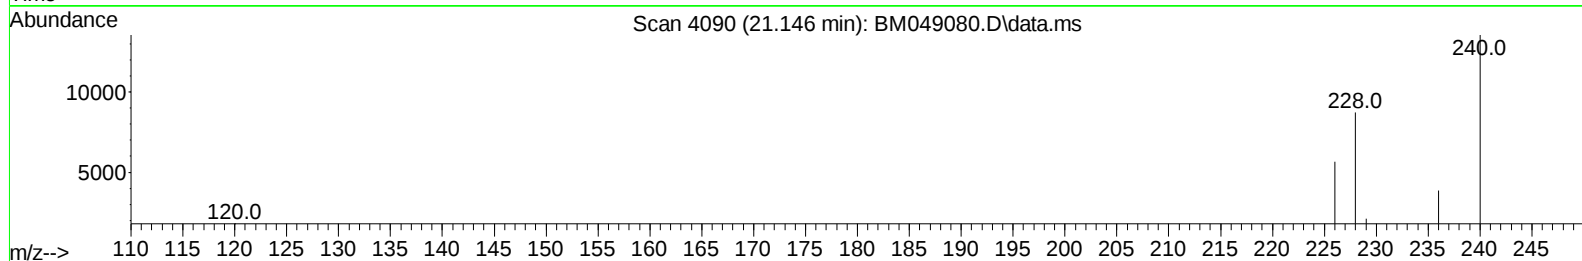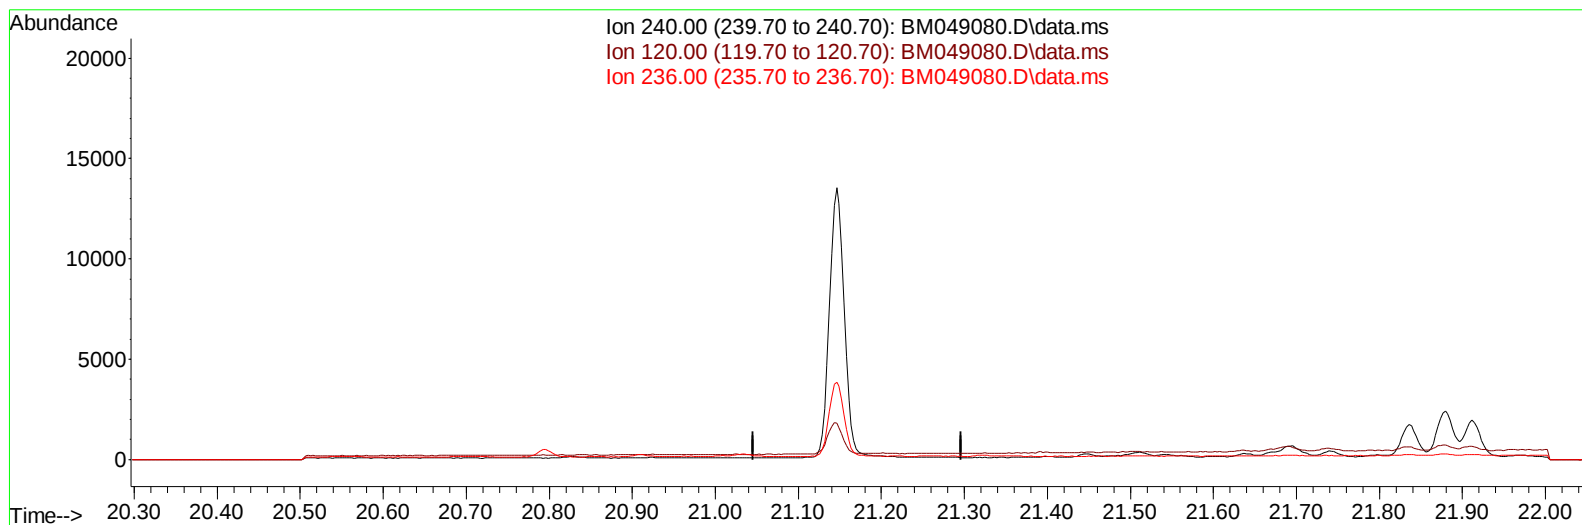

TIC: BM049080.D\data.ms

(17) Chrysene-d12

21.146min (-21.146) 0.00 ng/u1

response 0

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 240.00 | 100.00 | 0.00  |
| 120.00 | 14.50  | 0.00# |
| 236.00 | 29.80  | 0.00# |
| 0.00   | 0.00   | 0.00  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

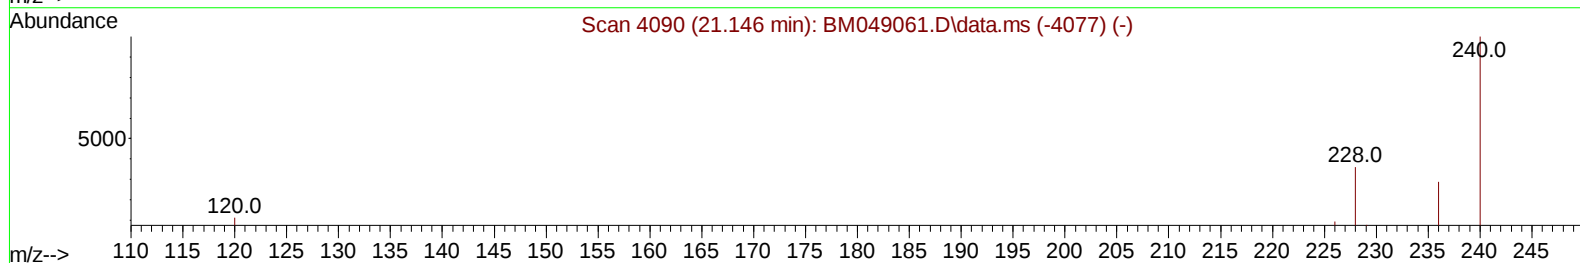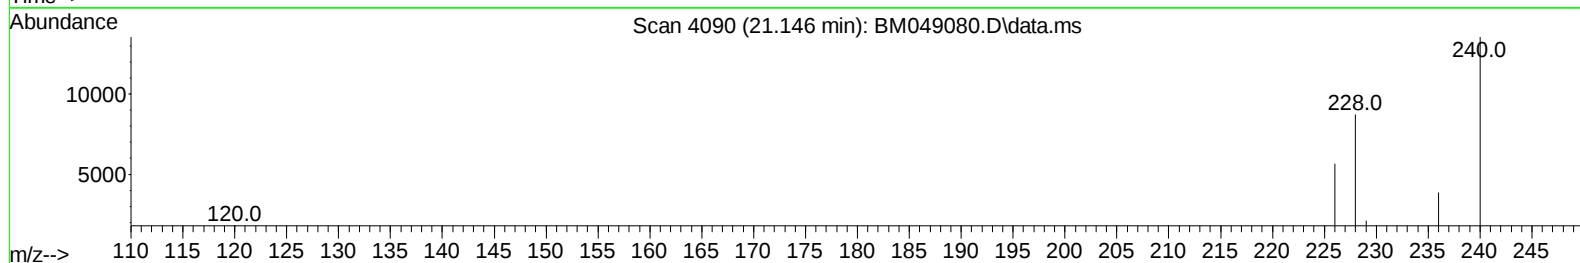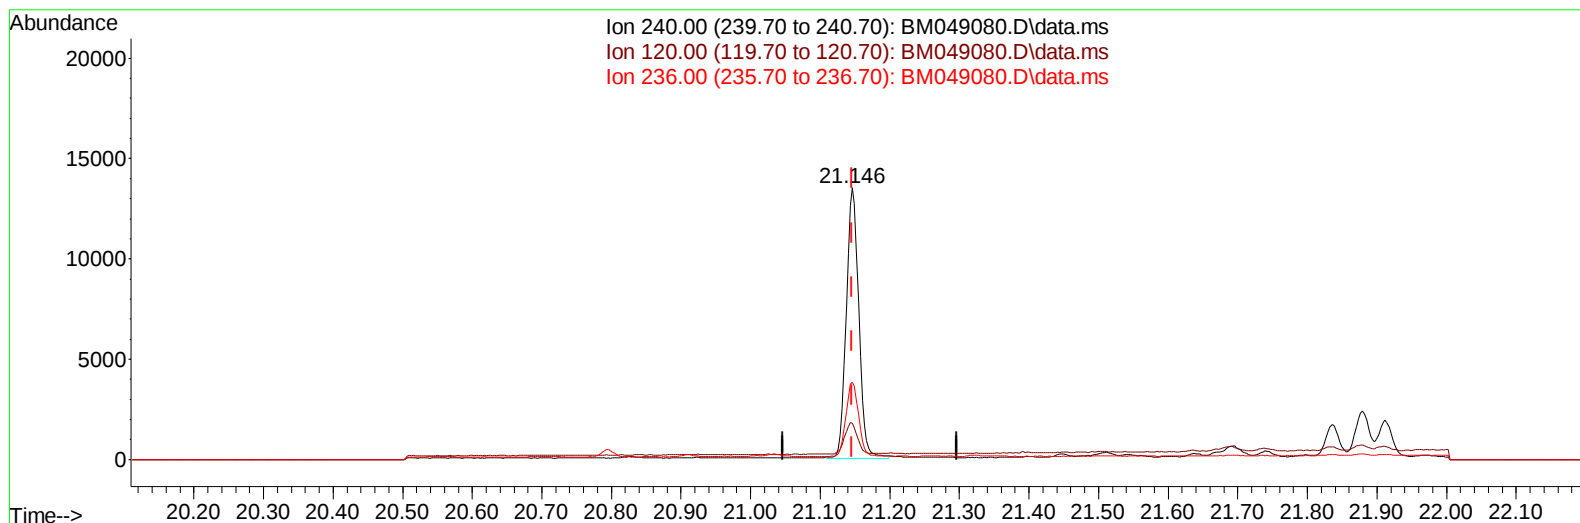

TIC: BM049080.D\data.ms

(17) Chrysene-d12

21.146min (+ 0.000) 0.40 ng/ul m

response 16897

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 240.00 | 100.00 | 100.00 |
| 120.00 | 14.50  | 13.28  |
| 236.00 | 29.80  | 28.48  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

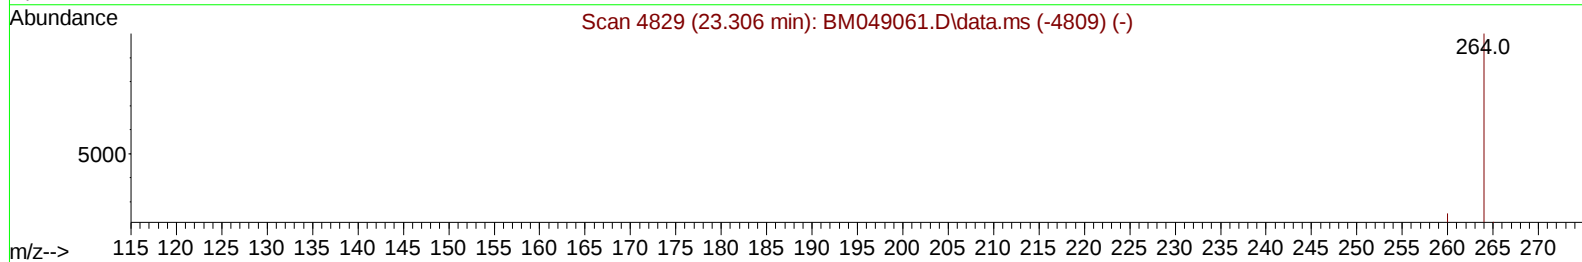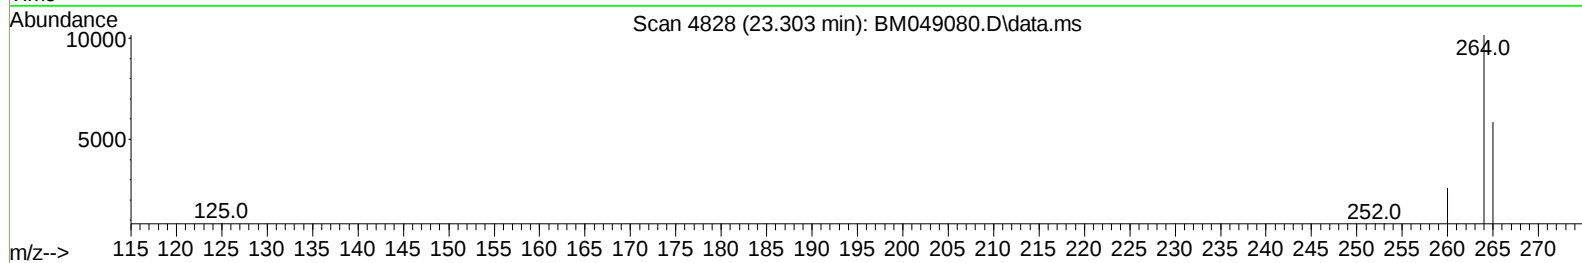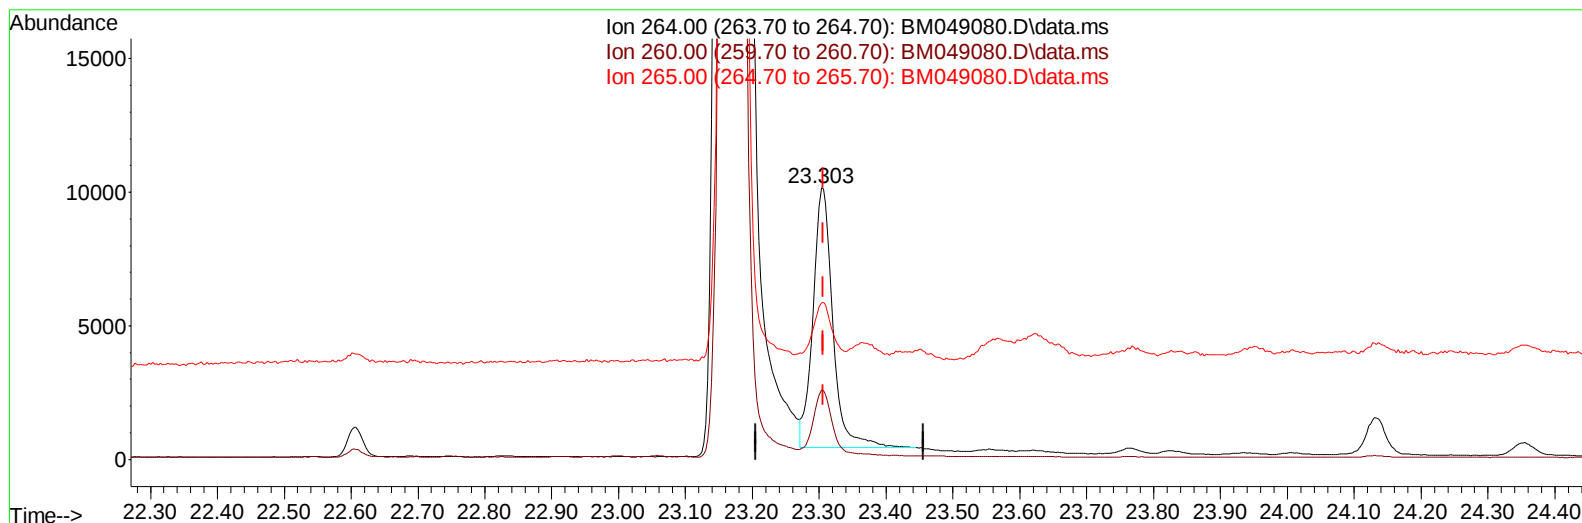

TIC: BM049080.D\data.ms

(23) Perylene-d12 (I)

23.303min (-0.003) 0.40 ng/u1

response 19859

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 25.80  | 25.49  |
| 265.00 | 78.30  | 57.57# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

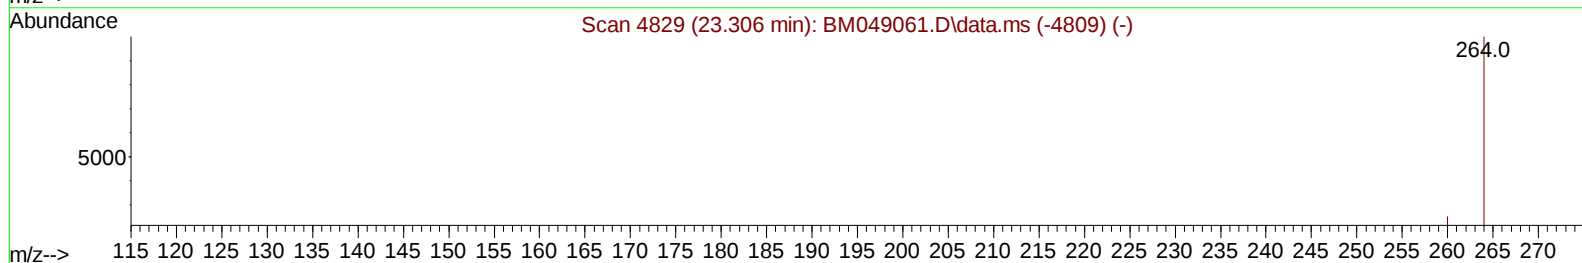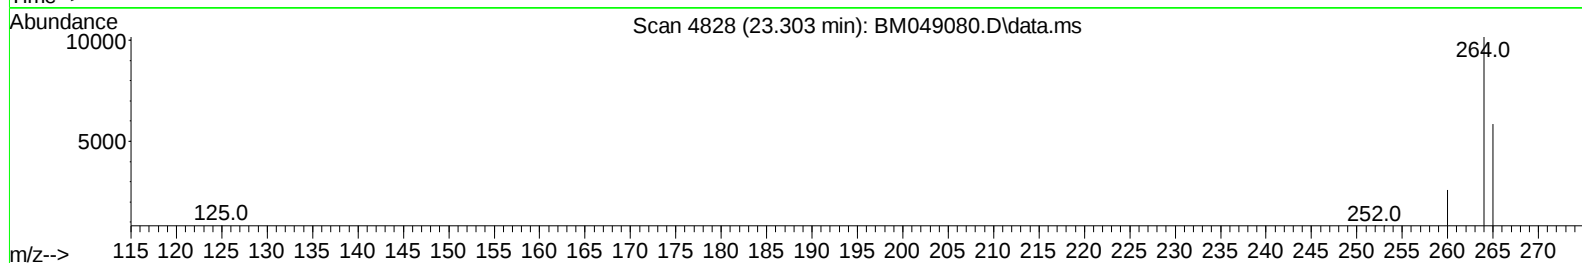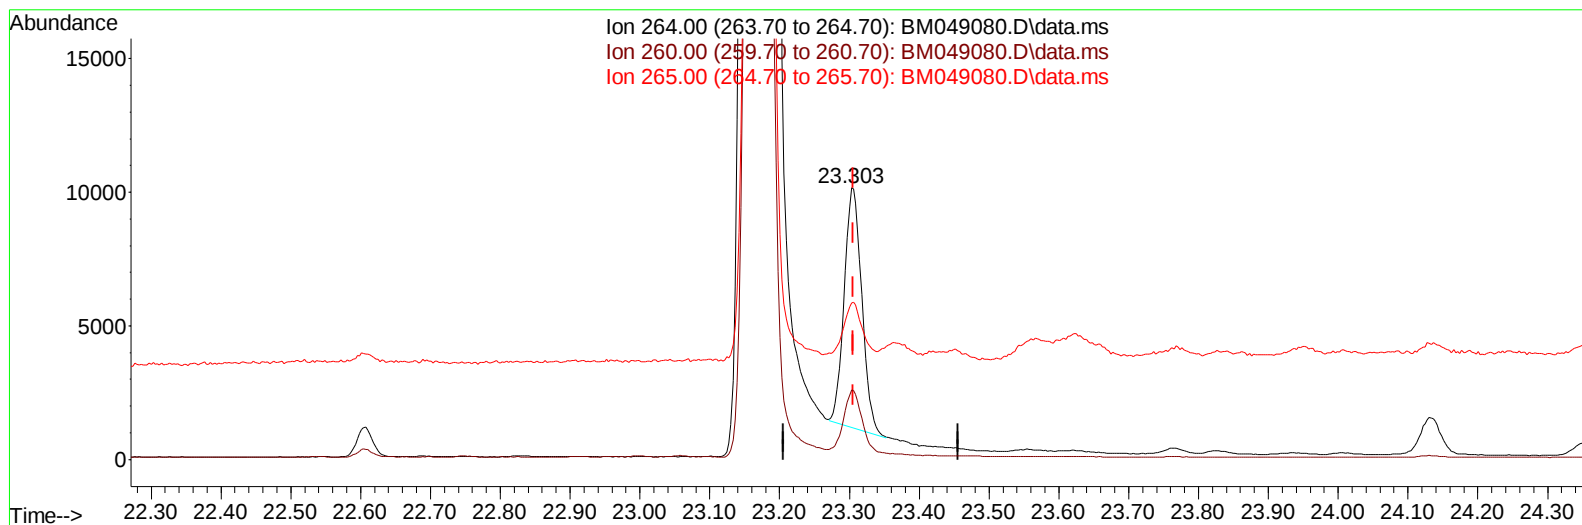

TIC: BM049080.D\data.ms

(23) Perylene-d12 (I)

23.303min (-0.003) 0.40 ng/ul m

response 15744

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 25.80  | 25.49  |
| 265.00 | 78.30  | 57.57# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

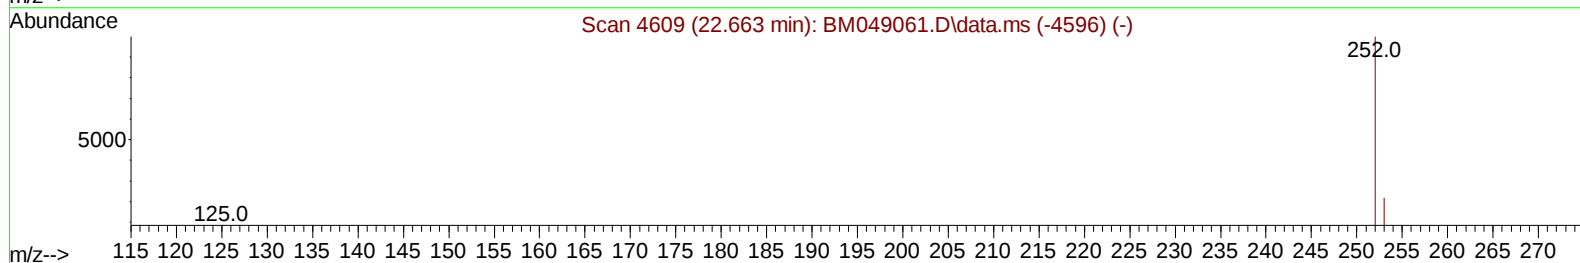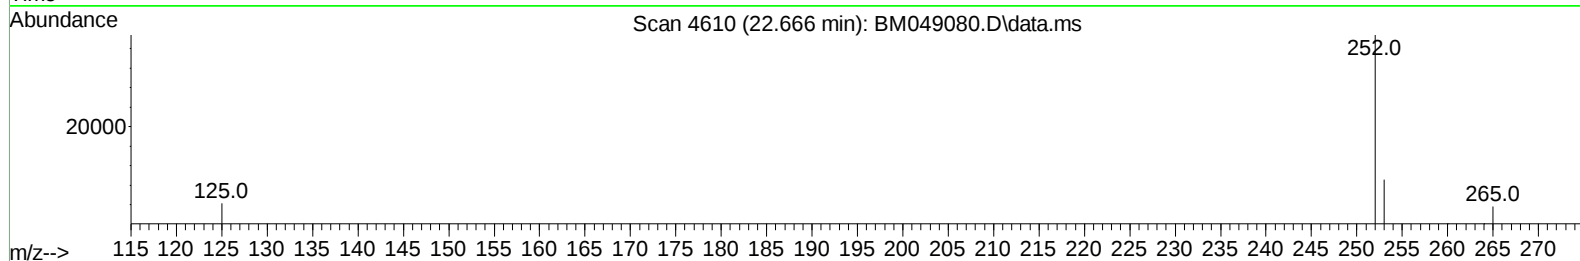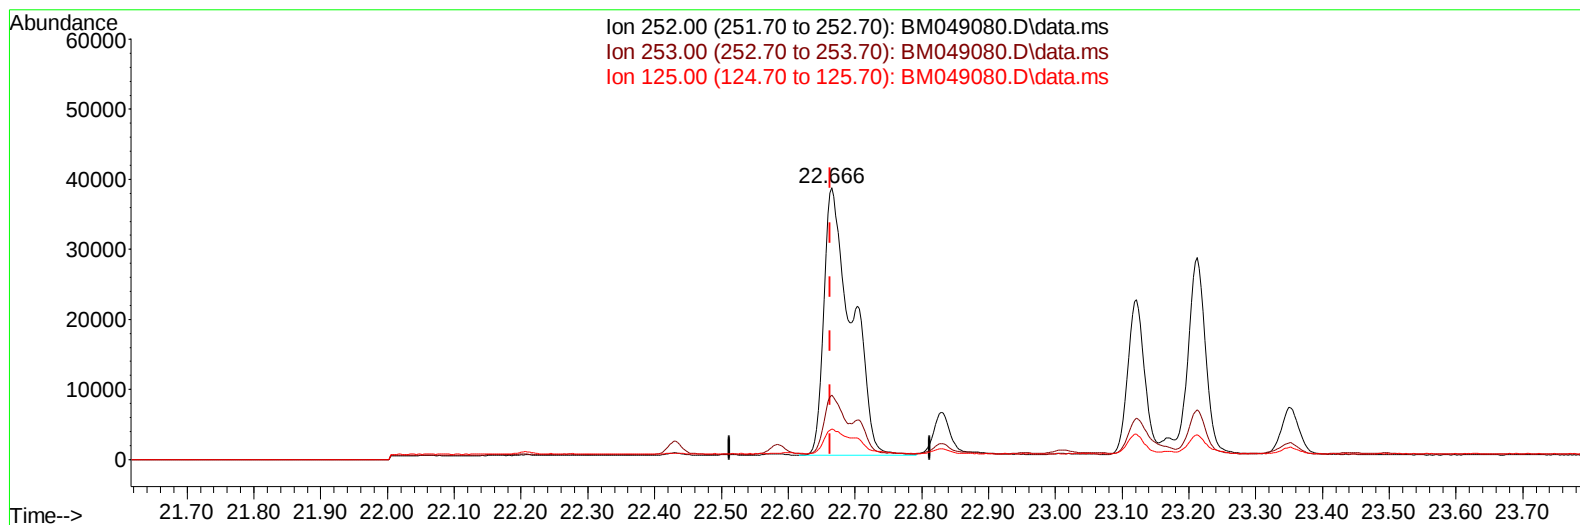

TIC: BM049080.D\data.ms

(24) Benzo(b)fluoranthene

22.666min (+ 0.003) 2.18 ng/u1

response 109818

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 26.30  | 23.69  |
| 125.00 | 15.40  | 11.21  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

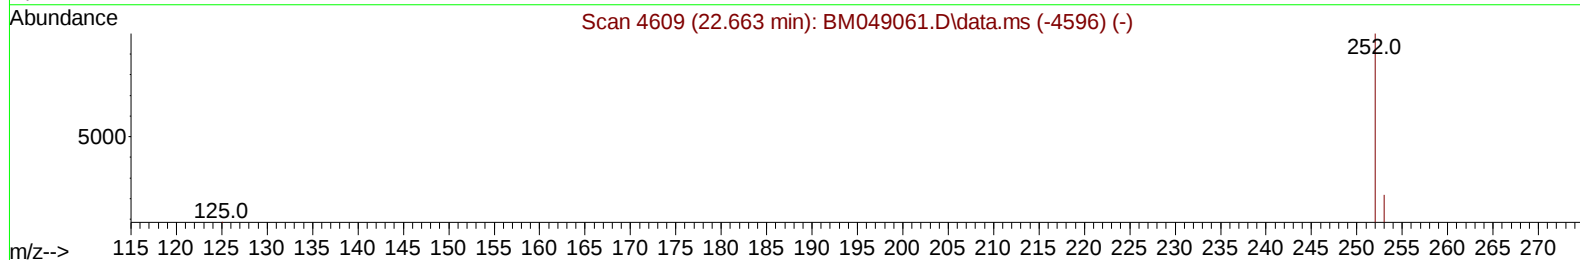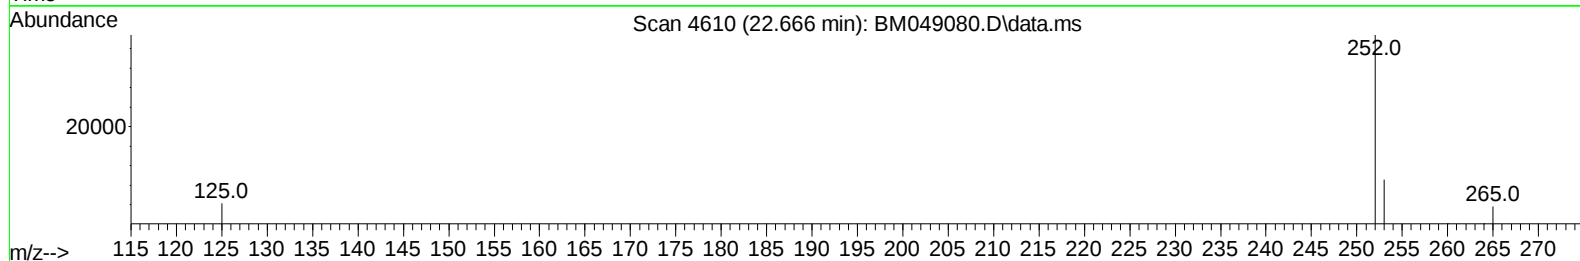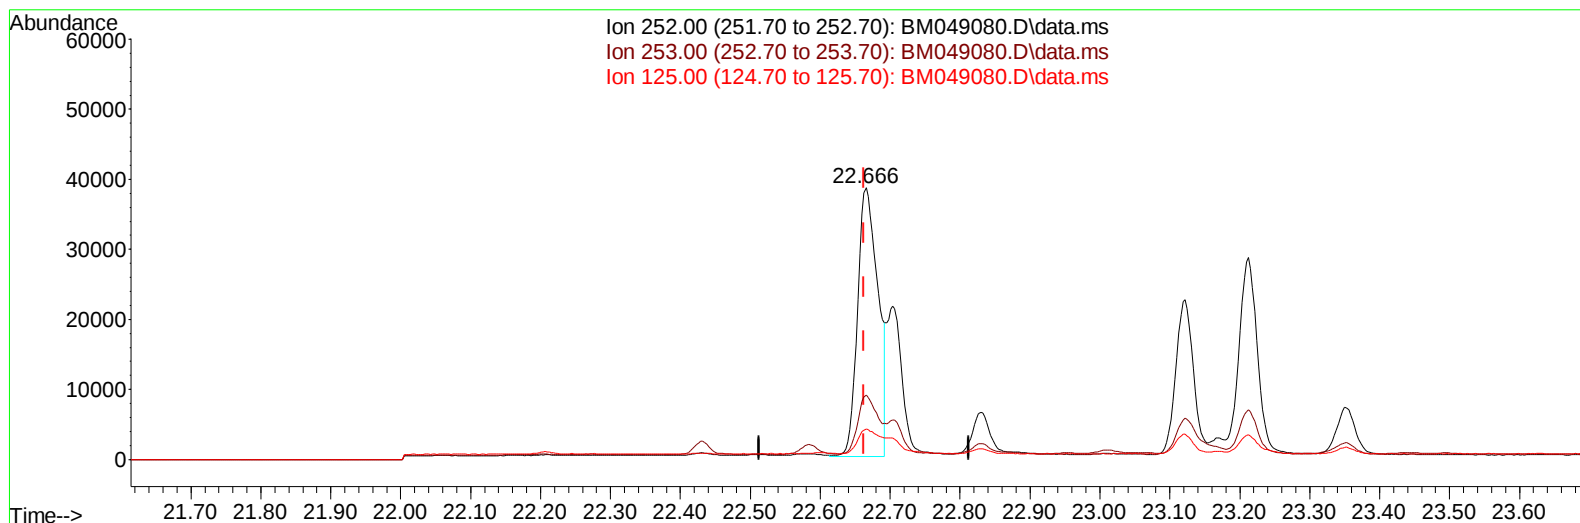

TIC: BM049080.D\data.ms

## (24) Benzo(b)fluoranthene

22.666min (+ 0.003) 1.55 ng/u1 m

response 78057

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 26.30  | 23.69  |
| 125.00 | 15.40  | 11.21  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

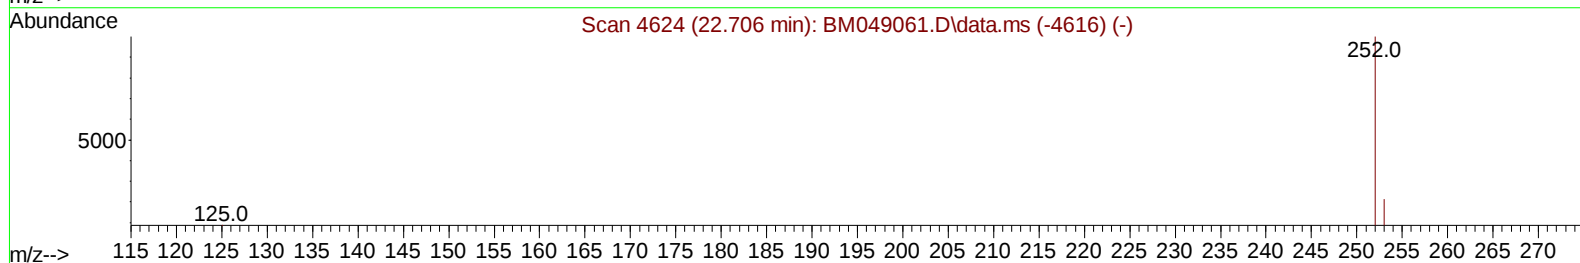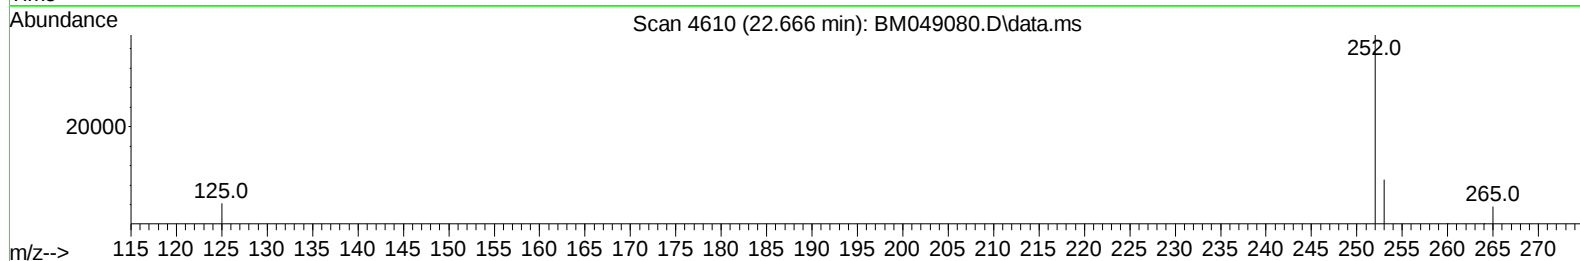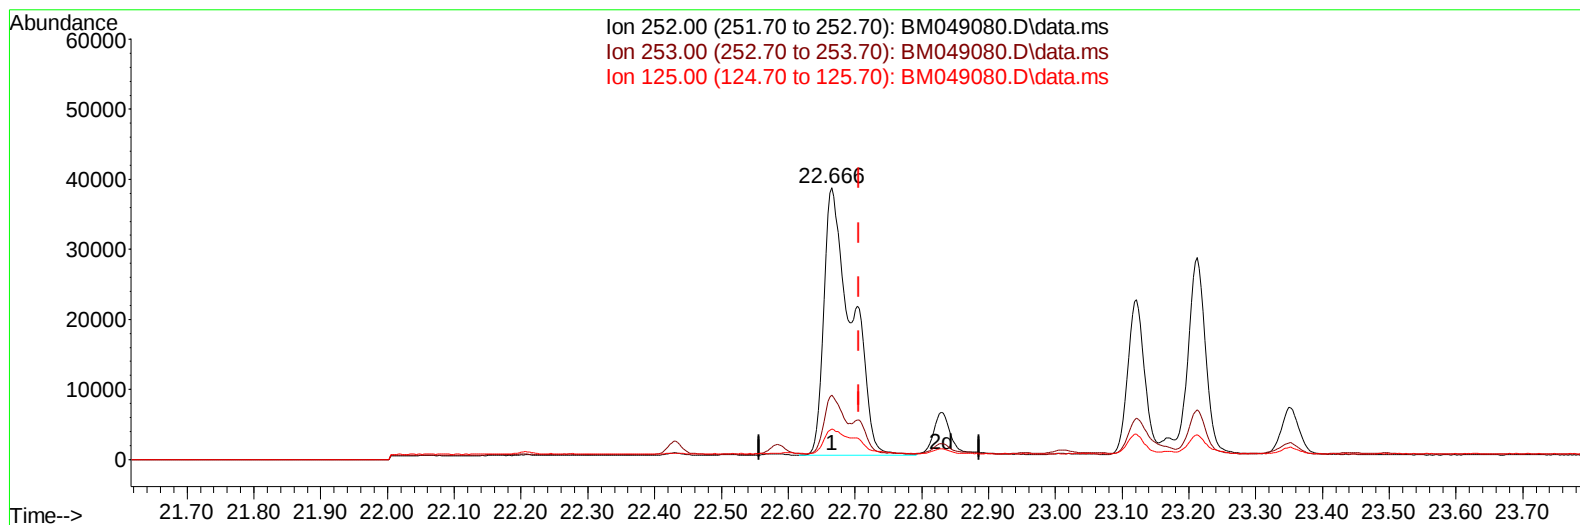

TIC: BM049080.D\data.ms

(25) Benzo(k)fluoranthene

22.666min (-0.041) 1.99 ng/u1

response 109818

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 26.60  | 23.69  |
| 125.00 | 15.70  | 11.21# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

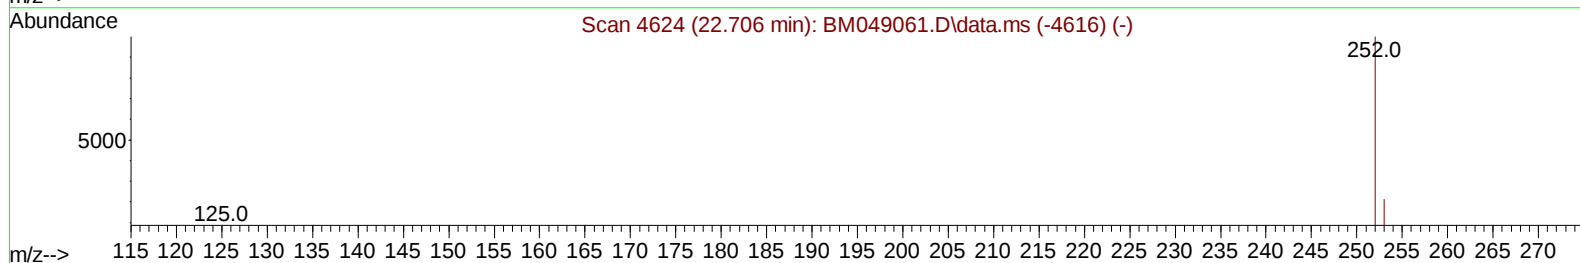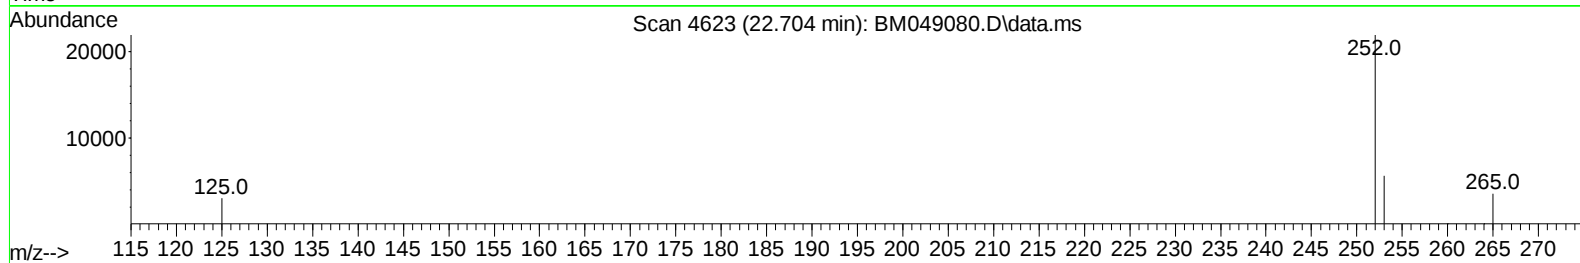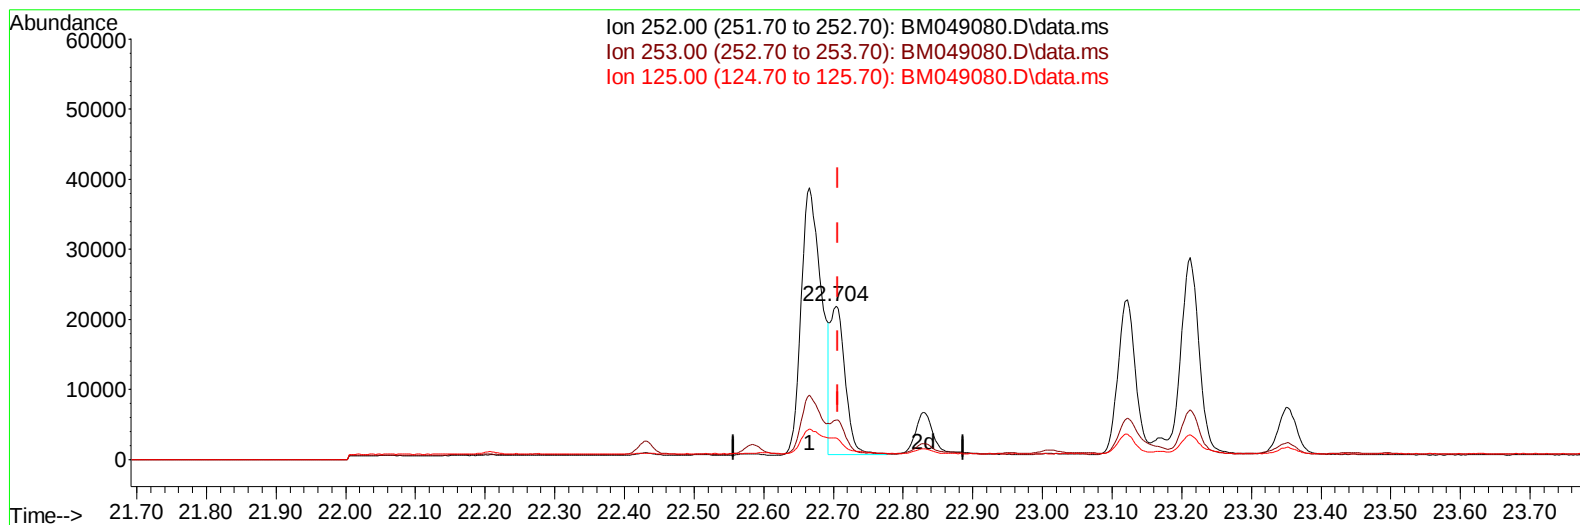

TIC: BM049080.D\data.ms

## (25) Benzo(k)fluoranthene

22.704min (-0.003) 0.57 ng/u1 m

response 31709

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 26.60  | 25.85  |
| 125.00 | 15.70  | 13.82  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

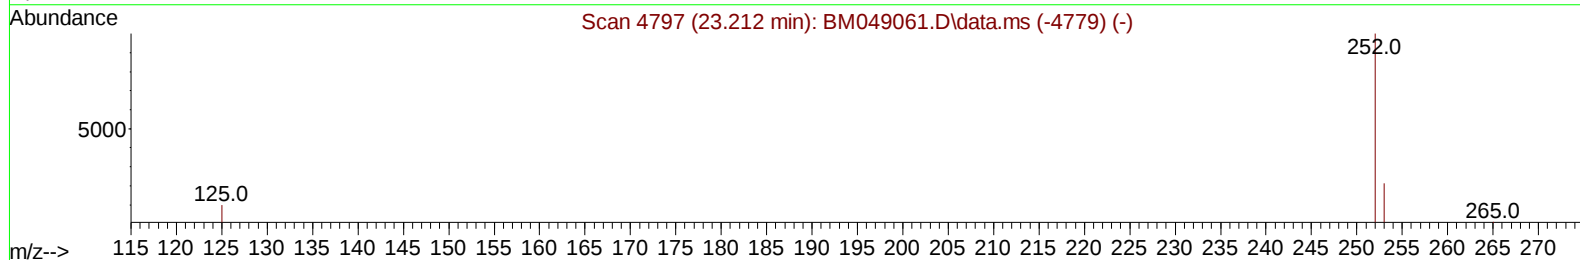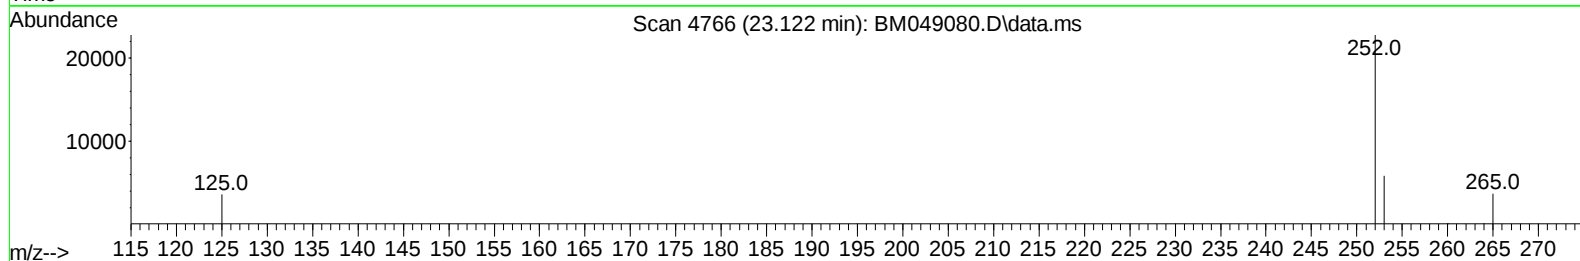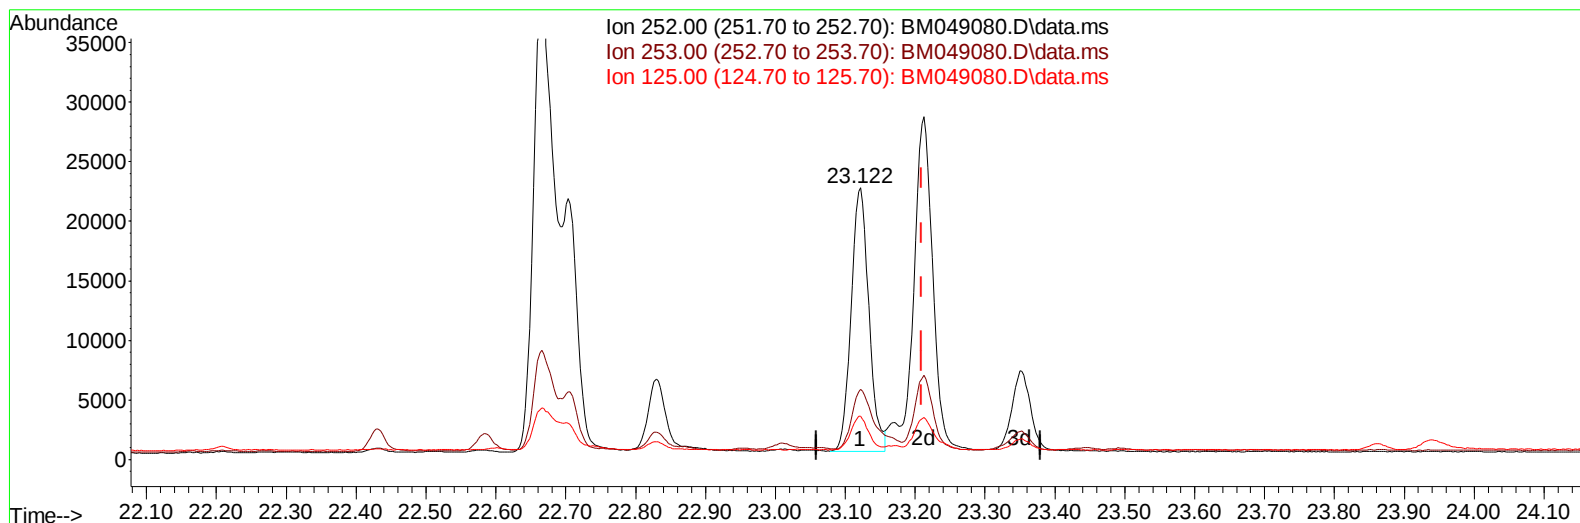

TIC: BM049080.D\data.ms

(26) Benzo(a)pyrene (C)

23.122min (-0.088) 0.81 ng/u1

response 38952

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 28.00  | 25.90  |
| 125.00 | 18.50  | 15.93  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
 Data File : BM049080.D  
 Acq On : 19 Dec 2024 21:29  
 Operator : RC/JU  
 Sample : P5226-11  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 E2AN6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 18 15:33:13 2024  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
 Supervised By :mohammad ahmed 12/26/2024

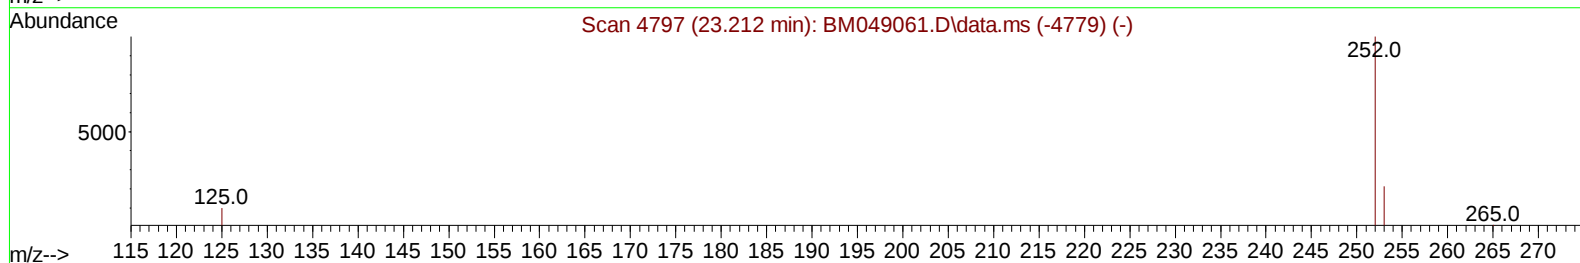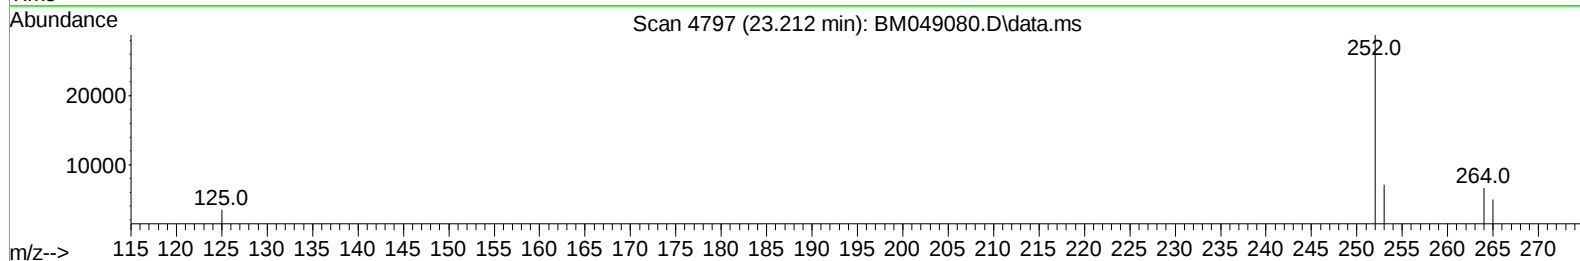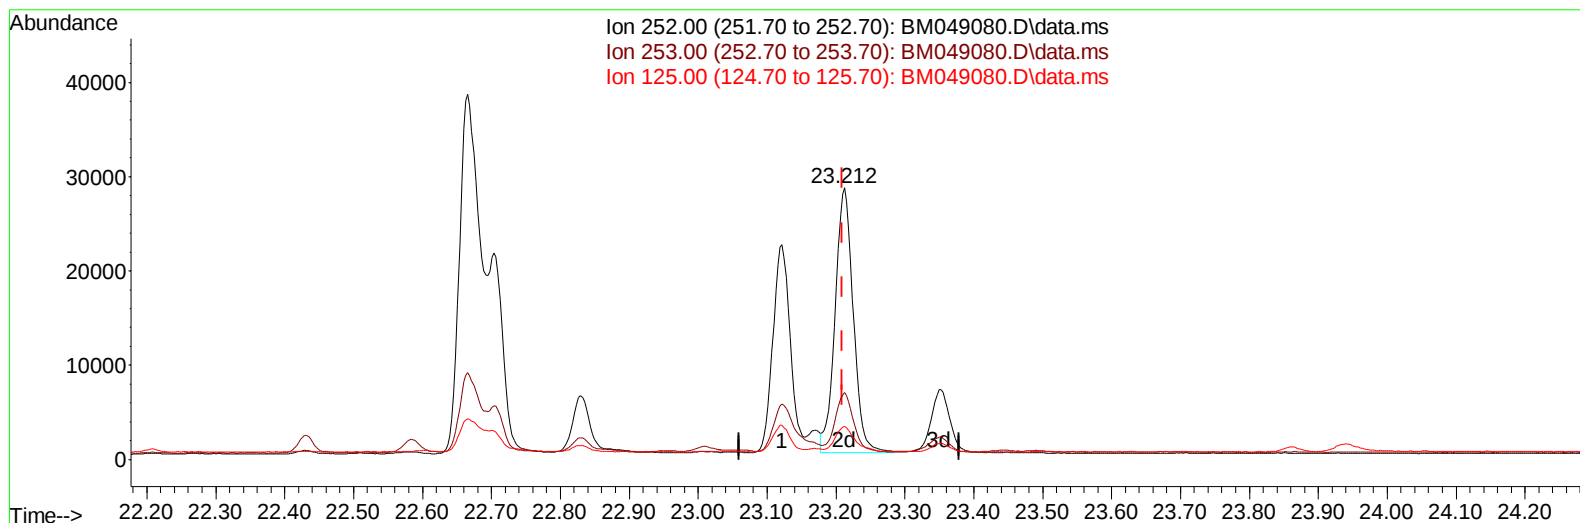

TIC: BM049080.D\data.ms

(26) Benzo(a)pyrene (C)

23.212min (+ 0.003) 1.06 ng/ul m

response 51332

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 28.00  | 24.64  |
| 125.00 | 18.50  | 12.18# |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
 Data File : BM049080.D  
 Acq On : 19 Dec 2024 21:29  
 Operator : RC/JU  
 Sample : P5226-11  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 E2AN6

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/21/2024  
 Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 19 22:33:43 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 18 15:33:13 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| -----                       |        |      |          |       |        |          |
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.560  | 152  | 6272     | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.325 | 136  | 18060    | 0.400 | ng/ul  | 0.00     |
| 9) Acenaphthene-d10         | 14.200 | 164  | 9661     | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 16.946 | 188  | 20619m   | 0.400 | ng/ul  | 0.00     |
| 17) Chrysene-d12            | 21.146 | 240  | 16897m   | 0.400 | ng/ul  | 0.00     |
| 23) Perylene-d12            | 23.303 | 264  | 15744m   | 0.400 | ng/ul  | 0.00     |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.151  | 96   | 27186    | 3.758 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 11.925 | 152  | 5358     | 0.221 | ng/ul  | 0.00     |
| 18) Fluoranthene-d10        | 18.982 | 212  | 10760    | 0.224 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       | Qvalue |          |
| 5) Naphthalene              | 10.374 | 128  | 1005     | 0.022 | ng/ul# | 77       |
| 10) Acenaphthylene          | 13.913 | 152  | 14763    | 0.369 | ng/ul  | 99       |
| 12) Fluorene                | 15.255 | 166  | 1655     | 0.050 | ng/ul# | 97       |
| 15) Phenanthrene            | 16.988 | 178  | 45433m   | 0.844 | ng/ul  |          |
| 16) Anthracene              | 17.077 | 178  | 8349m    | 0.169 | ng/ul  |          |
| 19) Fluoranthene            | 19.010 | 202  | 145206   | 2.377 | ng/ul  | 99       |
| 20) Pyrene                  | 19.373 | 202  | 120594   | 1.851 | ng/ul  | 99       |
| 21) Benzo(a)anthracene      | 21.129 | 228  | 50349    | 0.857 | ng/ul  | 97       |
| 22) Chrysene                | 21.181 | 228  | 57558    | 0.912 | ng/ul  | 98       |
| 24) Benzo(b)fluoranthene    | 22.666 | 252  | 78057m   | 1.552 | ng/ul  |          |
| 25) Benzo(k)fluoranthene    | 22.704 | 252  | 31709m   | 0.575 | ng/ul  |          |
| 26) Benzo(a)pyrene          | 23.212 | 252  | 51332m   | 1.064 | ng/ul  |          |
| 27) Indeno(1,2,3-cd)pyrene  | 25.444 | 276  | 41421    | 0.607 | ng/ul  | 94       |
| 28) Dibenzo(a,h)anthracene  | 25.454 | 278  | 9189     | 0.173 | ng/ul  | 93       |
| 29) Benzo(g,h,i)perylene    | 26.094 | 276  | 41004    | 0.747 | ng/ul  | 99       |
| -----                       |        |      |          |       |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121924\  
Data File : BM049080.D  
Acq On : 19 Dec 2024 21:29  
Operator : RC/JU  
Sample : P5226-11  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2AN6

## Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:33:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/26/2024

