

Data Path : Z:\HPCHEM1\BNA M\Data\BM122015\
 Data File : BM003648.D
 Acq On : 20 Dec 2015 11:19
 Operator : UM/SJ
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD02056

Quant Time: Dec 21 02:18:18 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 20 01:33:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	30000	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	140697	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	89376	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	218720	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	263032	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	236270	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	4335	7.78	ng/uL	0.00
5) Phenol-d5	6.87	99	50915	20.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	26917	19.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	42891	20.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	43822	20.01	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	21671	21.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	24070	20.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	44690	21.32	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	60839	21.80	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	146174	19.79	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	176477	20.98	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	29653	20.61	ng/ul	0.00
58) Fluorene-d10	15.34	176	127292	20.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	24115	19.56	ng/ul	0.00
71) Anthracene-d10	17.20	188	209650	21.07	ng/ul	0.00
79) Pyrene-d10	19.50	212	243746	21.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	244680	20.85	ng/ul	0.00

Target Compounds

						Ovalue
2) 1,4-Dioxane	3.19	88	5286	8.08	ng/ul	93
4) Benzaldehyde	6.84	77	32056	21.98	ng/ul	97
6) Phenol	6.90	94	54178	20.34	ng/ul	100
8) Bis(2-Chloroethyl)ether	7.12	93	38974	19.81	ng/ul	99
10) 2-Chlorophenol	7.26	128	44320	20.67	ng/ul	97
11) 2-Methylphenol	8.15	108	42507	20.16	ng/ul	100
12) 2,2'-oxybis(1-Chloropropan	8.23	45	39208	19.75	ng/ul	100
14) Acetophenone	8.52	105	69897	20.43	ng/ul	100
15) N-Nitroso-di-n-propylamine	8.50	70	32992	19.91	ng/ul	98
16) 4-Methylphenol	8.47	108	47333	20.14	ng/ul	99
17) Hexachloroethane	8.77	117	16600	20.35	ng/ul	98
20) Nitrobenzene	8.90	77	49172	20.86	ng/ul	99
21) Isophorone	9.42	82	94281	20.06	ng/ul	99
23) 2-Nitrophenol	9.60	139	27277	21.42	ng/ul	98
24) 2,4-Dimethylphenol	9.67	107	54402	20.87	ng/ul	99
25) Bis(2-Chloroethoxy)methane	9.90	93	55871	19.73	ng/ul	99
27) 2,4-Dichlorophenol	10.14	162	45553	20.91	ng/ul	99
28) Naphthalene	10.54	128	151439	20.89	ng/ul	99
30) 4-Chloroaniline	10.65	127	61569	21.82	ng/ul	99
31) Hexachlorobutadiene	10.82	225	27915	20.81	ng/ul	98
32) Caprolactam	11.40	113	15823	19.44	ng/ul	96
33) 4-Chloro-3-methylphenol	11.79	107	53719	21.02	ng/ul	100
34) 2-Methylnaphthalene	12.16	142	111914	20.67	ng/ul	99

Data Path : Z:\HPCHEM1\BNA M\Data\BM122015\
 Data File : BM003648.D
 Acq On : 20 Dec 2015 11:19
 Operator : UM/SJ
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 SSTD02056

Quant Time: Dec 21 02:18:18 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 20 01:33:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.38	142	106621	20.73	ng/ul	100
37) 1,2,4,5-Tetrachlorobenzene	12.53	216	55674	20.59	ng/ul	100
38) Hexachlorocyclopentadiene	12.51	237	18612	12.85	ng/ul	98
39) 2,4,6-Trichlorophenol	12.77	196	37298	20.41	ng/ul	99
40) 2,4,5-Trichlorophenol	12.85	196	41981	20.80	ng/ul	99
41) 1,1'-Biphenyl	13.18	154	148033	20.39	ng/ul	100
42) 2-Chloronaphthalene	13.22	162	113691	20.85	ng/ul	99
43) 2-Nitroaniline	13.43	65	31907	21.14	ng/ul	97
45) Dimethylphthalate	13.81	163	149126	19.73	ng/ul	100
46) 2,6-Dinitrotoluene	13.93	165	30521	20.73	ng/ul	95
48) Acenaphthylene	14.07	152	193174	21.01	ng/ul	99
49) 3-Nitroaniline	14.26	138	35961	21.89	ng/ul	99
50) Acenaphthene	14.42	153	127808	20.81	ng/ul	98
51) 2,4-Dinitrophenol	14.47	184	14701	18.83	ng/ul	99
53) 4-Nitrophenol	14.57	109	25525	20.96	ng/ul	97
54) Dibenzofuran	14.75	168	181041	20.65	ng/ul	100
55) 2,4-Dinitrotoluene	14.72	165	48226	21.57	ng/ul	99
56) 2,3,4,6-Tetrachlorophenol	14.98	232	35886	20.63	ng/ul	98
57) Diethylphthalate	15.17	149	158373	19.81	ng/ul	99
59) Fluorene	15.40	166	148075	21.05	ng/ul	99
60) 4-Chlorophenyl-phenylether	15.40	204	70007	20.50	ng/ul	98
61) 4-Nitroaniline	15.43	138	40662	22.28	ng/ul	98
64) 4,6-Dinitro-2-methylphenol	15.49	198	26558	20.11	ng/ul	97
65) N-Nitrosodiphenylamine	15.61	169	130031	20.31	ng/ul	99
66) 4-Bromophenyl-phenylether	16.29	248	43582	20.01	ng/ul	96
67) Hexachlorobenzene	16.41	284	50176	20.72	ng/ul	98
68) Atrazine	16.56	200	49181	20.00	ng/ul	99
69) Pentachlorophenol	16.76	266	26908	19.69	ng/ul	98
70) Phenanthrene	17.14	178	250366	20.69	ng/ul	100
72) Anthracene	17.23	178	258660	20.96	ng/ul	100
73) 1,2,3,4-Tetrachlorobenzene	13.15	216	61402	20.48	ng/uL	98
74) Pentachlorobenzene	14.67	250	57770	20.46	ng/uL	98
75) Carbazole	17.50	167	244038	21.67	ng/ul	100
76) Di-n-butylphthalate	18.07	149	285385	19.48	ng/ul	100
77) Fluoranthene	19.16	202	306239	22.02	ng/ul	100
80) Pvrene	19.53	202	319021	21.07	ng/ul	99
81) Butylbenzylphthalate	20.43	149	145600	20.34	ng/ul	99
82) 3,3'-Dichlorobenzidine	21.22	252	110759	22.03	ng/ul	99
83) Benzo(a)anthracene	21.29	228	327554	20.66	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.22	149	212083	19.90	ng/ul	99
85) Chrysene	21.33	228	312396	20.43	ng/ul	100
87) Di-n-octyl phthalate	22.09	149	393970	24.13	ng/ul	100
88) Benzo(b)fluoranthene	22.87	252	307103	21.56	ng/ul	99
89) Benzo(k)fluoranthene	22.91	252	291255	21.58	ng/ul	99
91) Benzo(a)pyrene	23.45	252	282898	20.76	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.81	276	285675	19.48	ng/ul	99
93) Dibenzo(a,h)anthracene	25.82	278	241615	19.64	ng/ul	100
94) Benzo(a,h,i)perylene	26.50	276	226329	18.79	ng/ul	99


Data Path : Z:\HPCHEM1\BNA M\Data\BM122015\
Data File : BM003648.D
Acq On : 20 Dec 2015 11:19
Operator : UM/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD02056

Quant Time: Dec 21 02:18:18 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 20 01:33:56 2015
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						

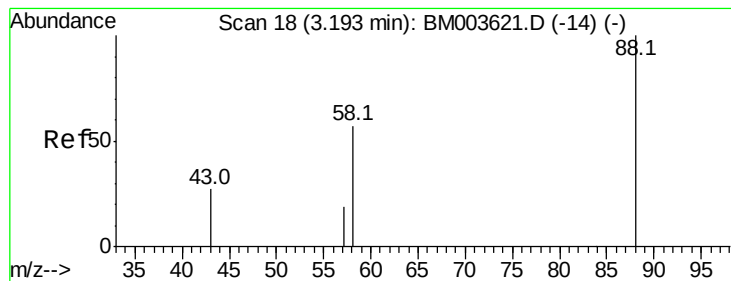

#2

1,4-Dioxane

Concen: 8.08 ng/uL

RT: 3.19 min Scan# 18

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056




Tot Ion: 88 Resp: 5286

Ion Ratio Lower Upper

88 100

43 22.1 21.0 31.6

58 55.1 47.8 71.8



#4

Benzaldehyde

Concen: 21.98 ng/uL

RT: 6.84 min Scan# 638

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19




Tgt Ion: 77 Resp: 32056


Ion Ratio Lower Upper

77 100

105 102.9 80.6 120.8

106 94.1 77.7 116.5



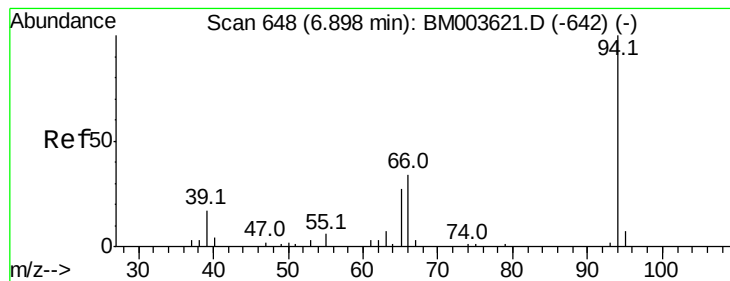

#6

Phenol

Concen: 20.34 ng/ul

RT: 6.90 min Scan# 648

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056


Tot Ion: 94 Resp: 54178

Ion Ratio Lower Upper




94 100

65 26.1 21.0 31.6

66 36.6 29.3 43.9

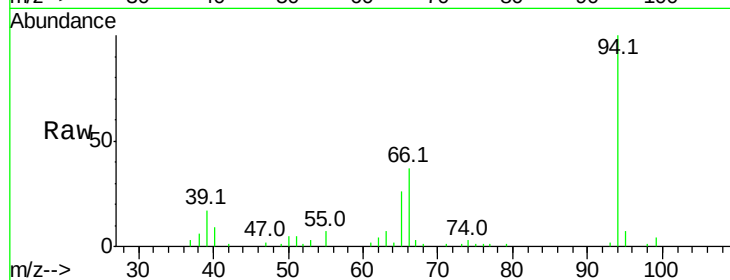

Abundance Ion 94.00 (93.70 to 94.70): BM003648.D (-614) (-)

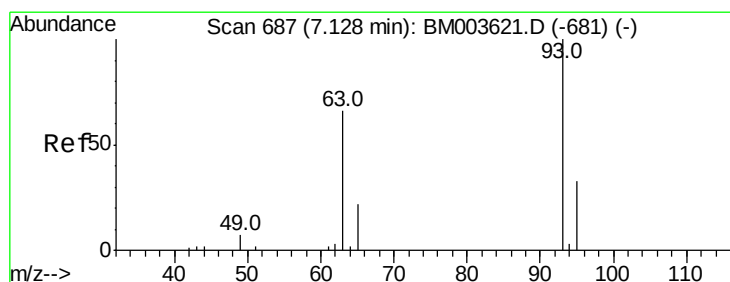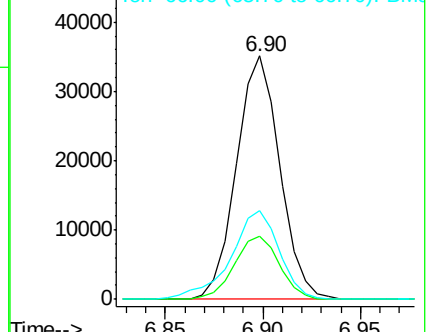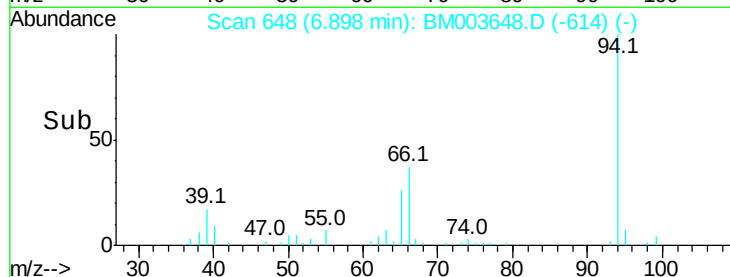

#8

Bis(2-Chloroethyl)ether

Concen: 19.81 ng/ul

RT: 7.12 min Scan# 686

Delta R.T. -0.01 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Tgt Ion: 93 Resp: 38974

Ion Ratio Lower Upper



93 100


63 68.1 53.5 80.3

95 33.0 26.2 39.2

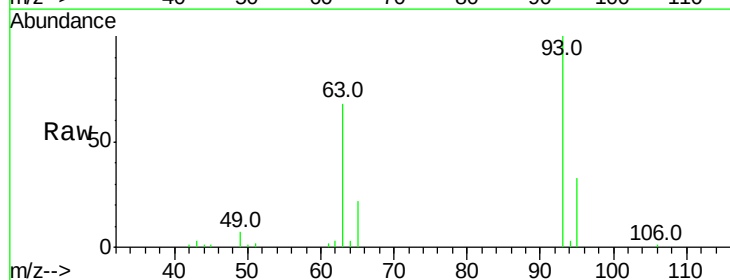

Abundance Ion 93.00 (92.70 to 93.70): BM003648.D (-653) (-)

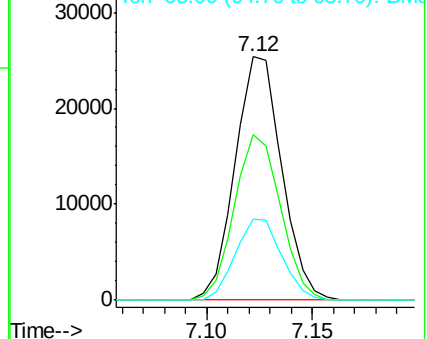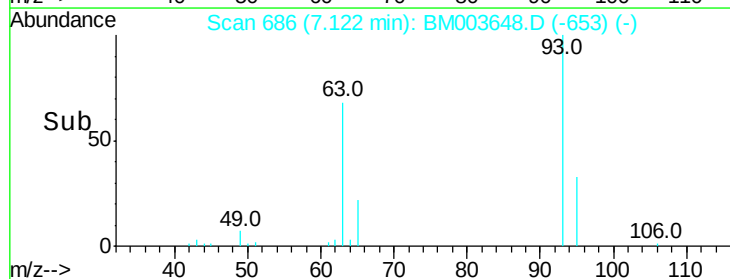

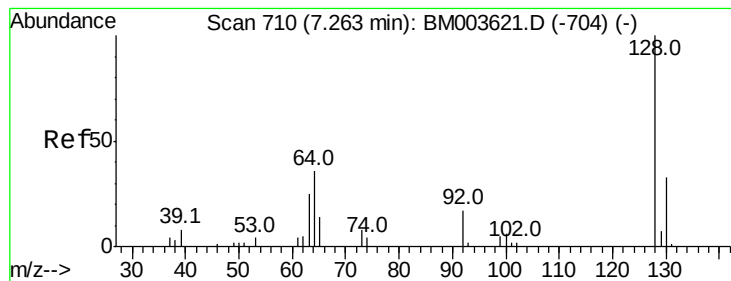

#10

2-Chlorophenol

Concen: 20.67 ng/ul

RT: 7.26 min Scan# 710

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056


Tot Ion:128 Resp: 44320

Ion Ratio Lower Upper

128 100

64 37.8 31.9 47.9




130 32.8 25.6 38.4



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 130.00 (129.70 to 130.70): E

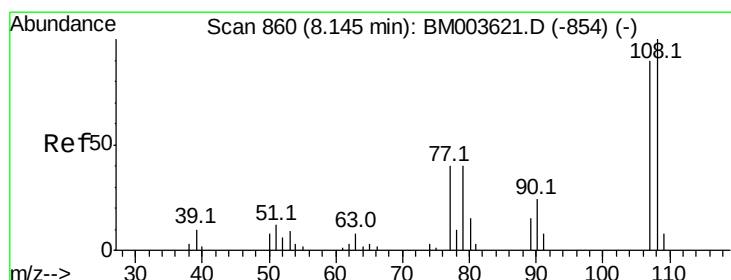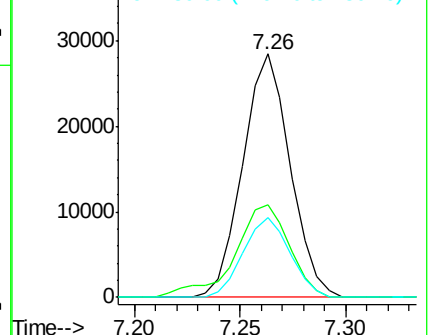

#11

2-Methylphenol

Concen: 20.16 ng/ul

RT: 8.15 min Scan# 860

Delta R.T. -0.00 min

Lab File: BM003648.D


Acq: 20 Dec 2015 11:19

Tgt Ion:108 Resp: 42507

Ion Ratio Lower Upper



108 100


107 90.5 72.4 108.6



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E




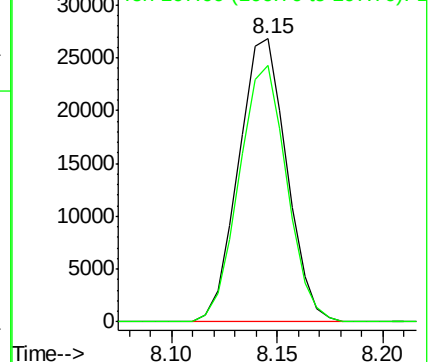


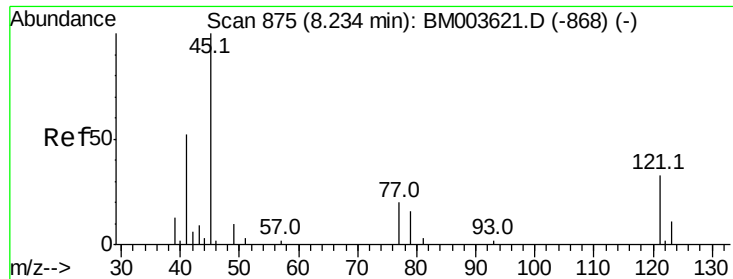

#12
2,2'-oxvbis(1-Chloropropane)
Concen: 19.75 ng/ul
RT: 8.23 min Scan# 875
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19




Instrument :
BNA_M
ClientSampleId :
SSTD02056


Tot Ion: 45 Resp: 39208
Ion Ratio Lower Upper
45 100
77 20.1 15.9 23.9
79 15.4 12.5 18.7

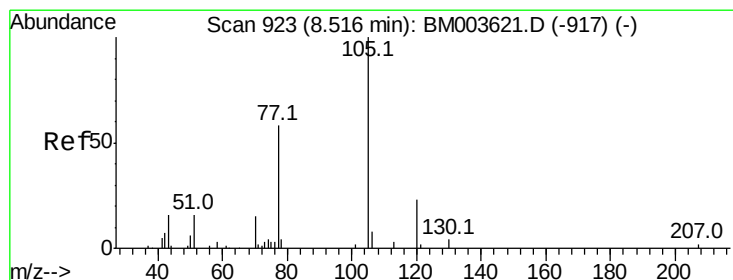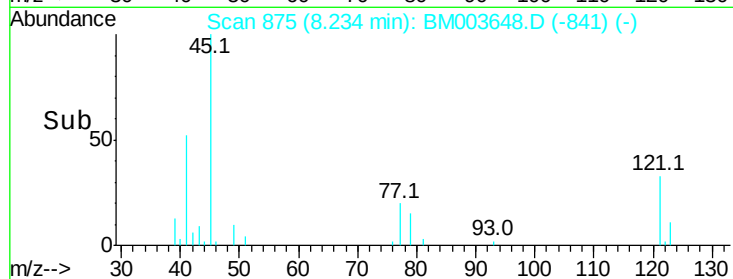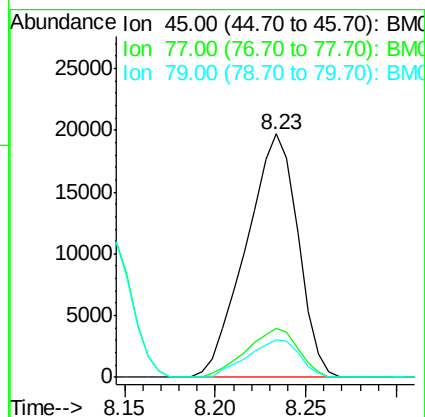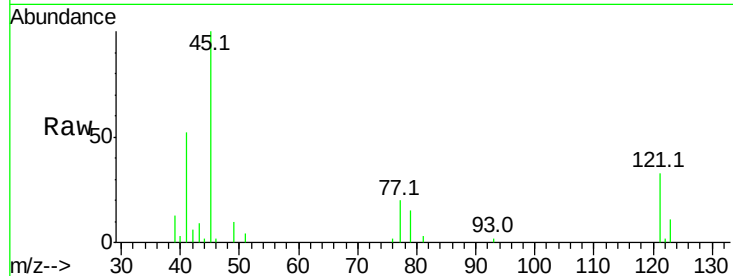

#14
Acetophenone
Concen: 20.43 ng/ul
RT: 8.52 min Scan# 923
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Tgt Ion: 105 Resp: 69897
Ion Ratio Lower Upper
105 100
77 74.1 59.0 88.4
51 20.6 16.4 24.6

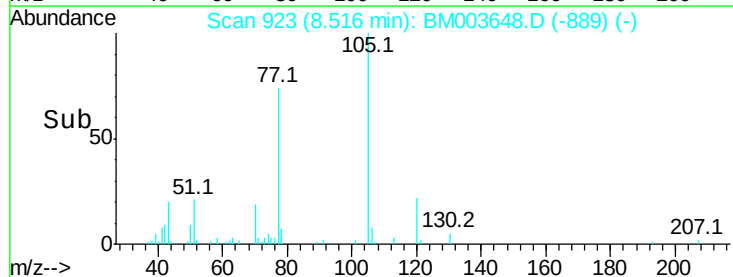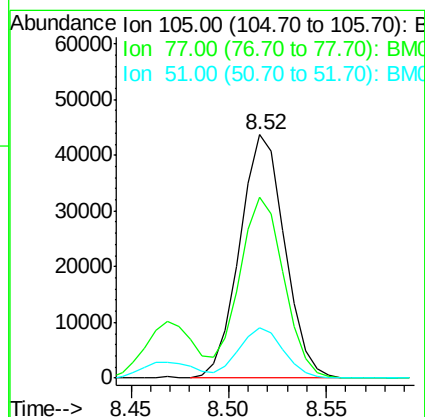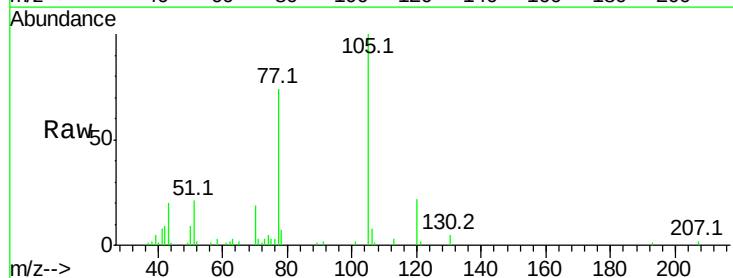



#15

N-Nitroso-di-n-propylamine

Concen: 19.91 ng/ul

RT: 8.50 min Scan# 921

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056

Tot Ion: 70 Resp: 32992


Ion Ratio Lower Upper

70 100

42 45.5 35.4 53.0

101 10.6 8.4 12.6

130 23.7 18.2 27.4






Abundance Ion 70.00 (69.70 to 70.70): BM003648.D (-887) (-)

Ion 42.00 (41.70 to 42.70): BM003648.D (-887) (-)

Ion 101.00 (100.70 to 101.70): BM003648.D (-887) (-)

Ion 130.00 (129.70 to 130.70): BM003648.D (-887) (-)

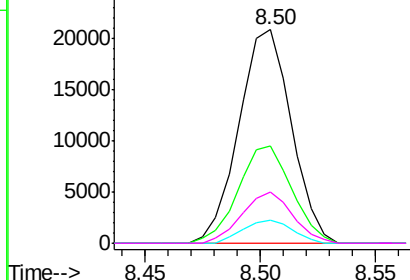

#16

4-Methylphenol

Concen: 20.14 ng/ul

RT: 8.47 min Scan# 915

Delta R.T. -0.01 min

Lab File: BM003648.D


Acq: 20 Dec 2015 11:19

Tgt Ion: 108 Resp: 47333

Ion Ratio Lower Upper



108 100


107 114.5 90.3 135.5



Abundance Ion 108.00 (107.70 to 108.70): BM003648.D (-882) (-)

Ion 107.00 (106.70 to 107.70): BM003648.D (-882) (-)

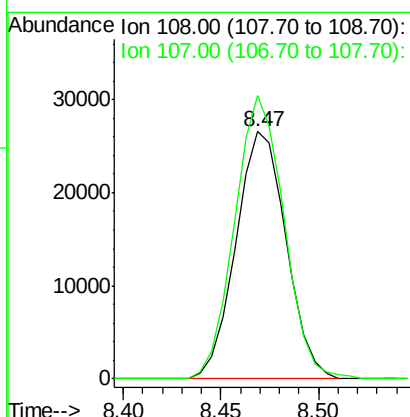







#17
Hexachloroethane
Concen: 20.35 ng/ul
RT: 8.77 min Scan# 966
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Instrument :
BNA_M
ClientSampleId :
SSTD02056

Tot Ion:117 Resp: 16600
Ion Ratio Lower Upper
117 100
201 103.5 81.5 122.3
199 64.6 50.6 76.0




Abundance Ion 117.00 (116.70 to 117.70): E
Ion 201.00 (200.70 to 201.70): E
Ion 199.00 (198.70 to 199.70): E


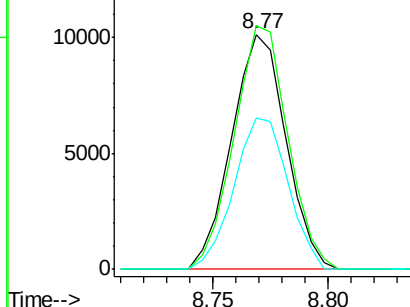



#20
Nitrobenzene
Concen: 20.86 ng/ul
RT: 8.90 min Scan# 988
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Tgt Ion: 77 Resp: 49172
Ion Ratio Lower Upper
77 100
123 49.7 39.0 58.4
65 13.1 10.4 15.6



Abundance Ion 77.00 (76.70 to 77.70): BM
Ion 123.00 (122.70 to 123.70): E
Ion 65.00 (64.70 to 65.70): BM

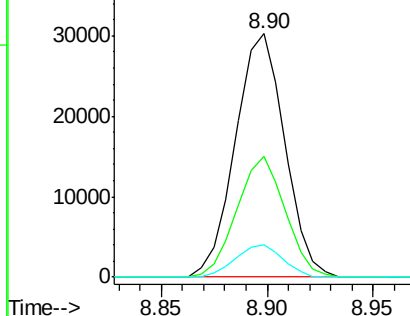



#21

Isophorone

Concen: 20.06 ng/ul

RT: 9.42 min Scan# 1076

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056





Tot Ion: 82 Resp: 94281

Ion Ratio Lower Upper

82 100

95 7.8 6.4 9.6

138 18.9 14.9 22.3

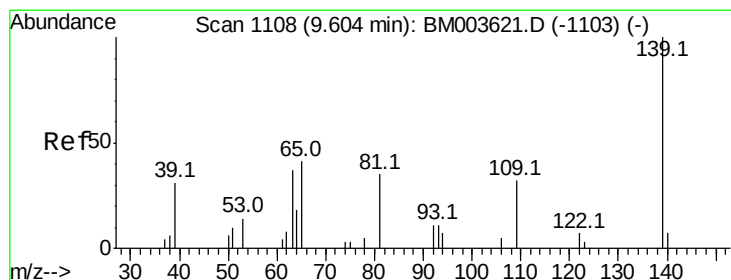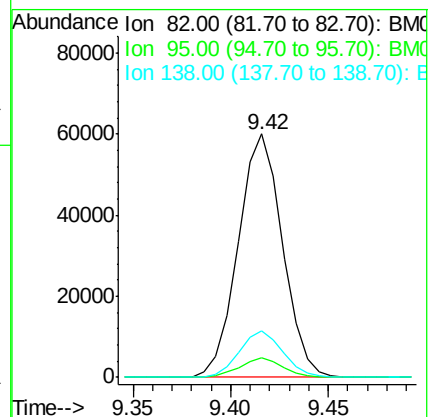

#23

2-Nitrophenol

Concen: 21.42 ng/ul

RT: 9.60 min Scan# 1108

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19




Tgt Ion: 139 Resp: 27277


Ion Ratio Lower Upper

139 100

65 47.2 36.3 54.5

109 31.9 26.4 39.6



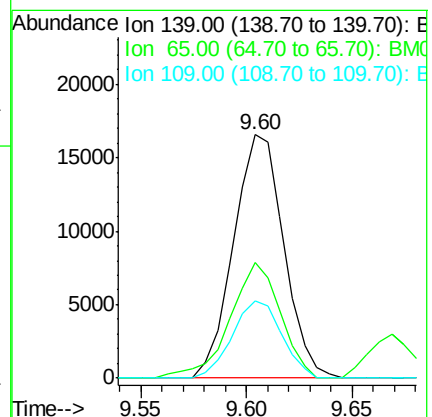
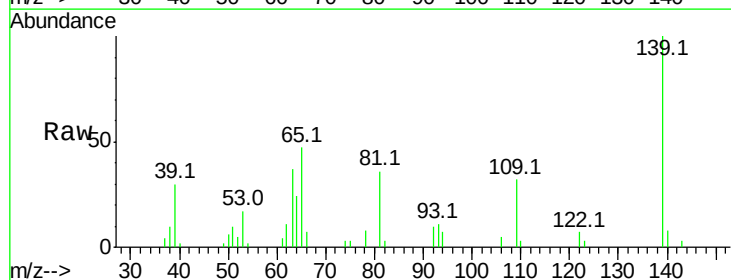


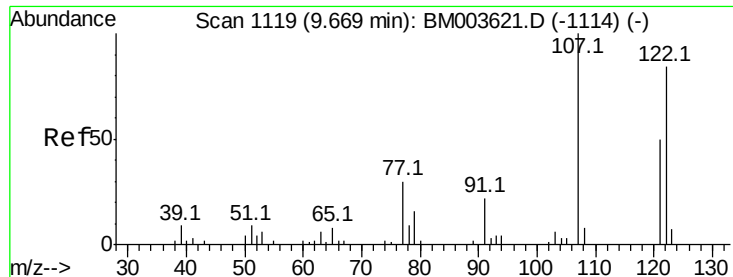

#24
 2,4-Dimethylphenol
 Concen: 20.87 ng/ul
 RT: 9.67 min Scan# 1119
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02056


Tot Ion:107 Resp: 54402
 Ion Ratio Lower Upper
 107 100
 121 52.0 40.6 61.0
 122 85.7 67.8 101.6

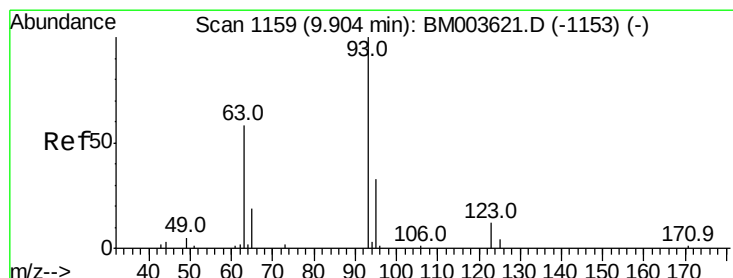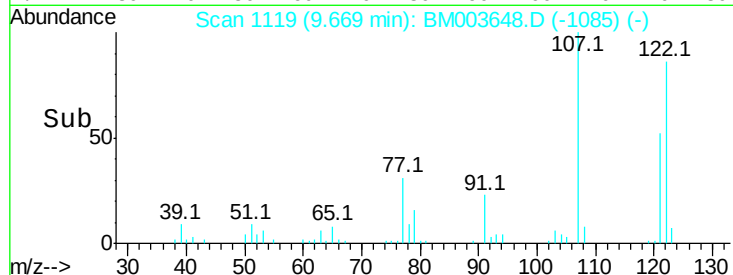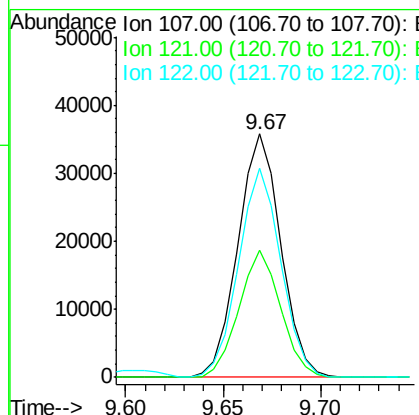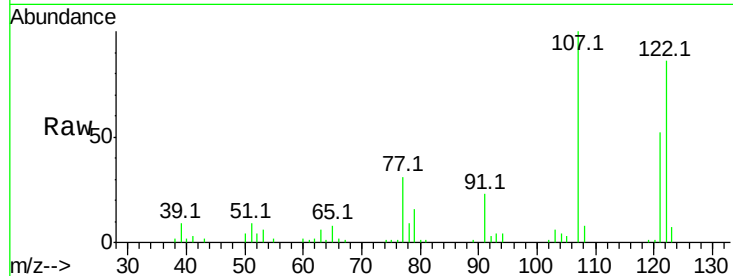

#25
 Bis(2-Chloroethoxy)methane
 Concen: 19.73 ng/ul
 RT: 9.90 min Scan# 1159
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion: 93 Resp: 55871
 Ion Ratio Lower Upper
 93 100
 95 32.3 25.8 38.8
 123 11.3 9.8 14.8

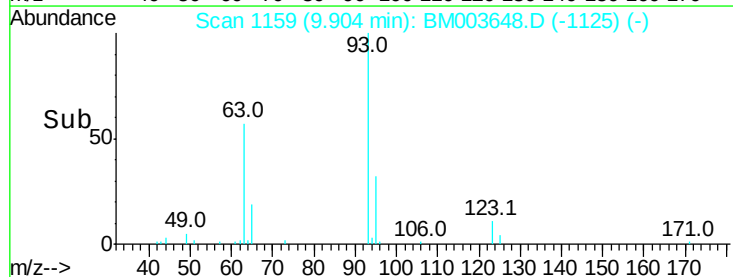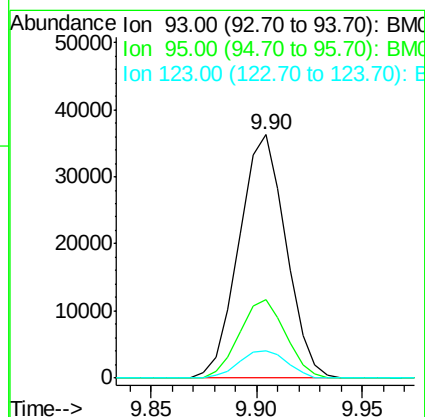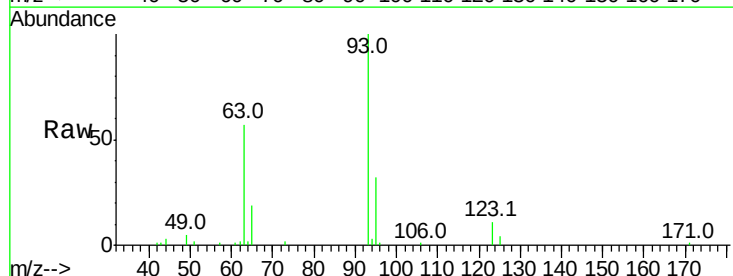







#27
 2,4-Dichlorophenol
 Concen: 20.91 ng/ul
 RT: 10.14 min Scan# 1199
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Instrument :
 BNA_M
 ClientSampleID :
 SST02056

Tot Ion:162 Resp: 45553
 Ion Ratio Lower Upper
 162 100
 164 65.6 52.1 78.1
 98 36.4 28.4 42.6




Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 98.00 (97.70 to 98.70): B


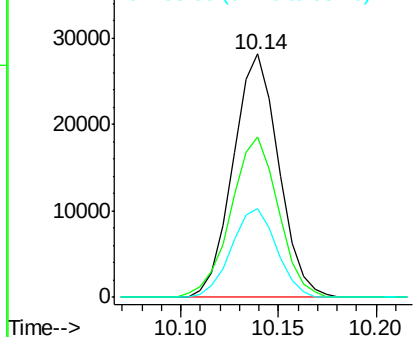



#28
 Naphthalene
 Concen: 20.89 ng/ul
 RT: 10.54 min Scan# 1267
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion:128 Resp: 151439
 Ion Ratio Lower Upper
 128 100
 129 10.6 8.8 13.2
 127 12.9 10.5 15.7



Abundance Ion 128.00 (127.70 to 128.70): E
 Ion 129.00 (128.70 to 129.70): E
 Ion 127.00 (126.70 to 127.70): E




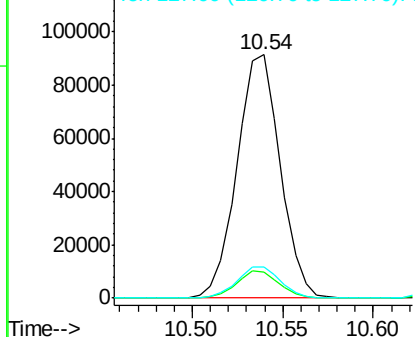


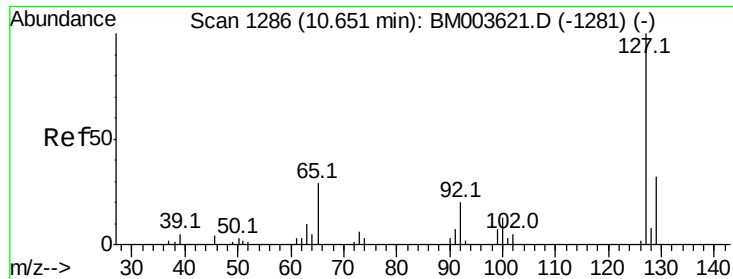

#30
4-Chloroaniline
Concen: 21.82 ng/ul
RT: 10.65 min Scan# 1286
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19




Instrument :
BNA_M
ClientSampleId :
SSTD02056


Tot Ion:127 Resp: 61569
Ion Ratio Lower Upper
127 100
129 32.1 25.4 38.2

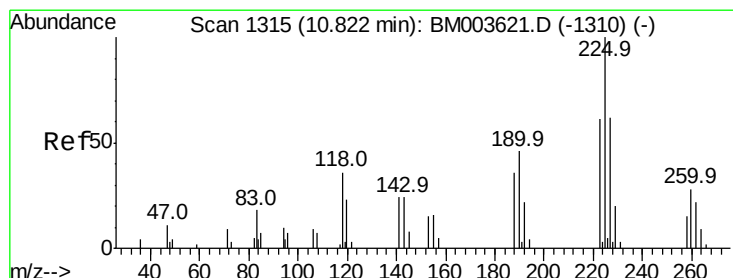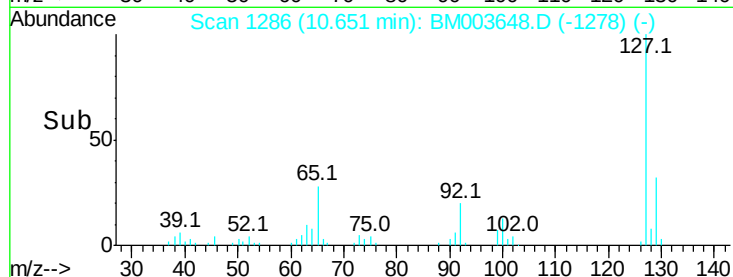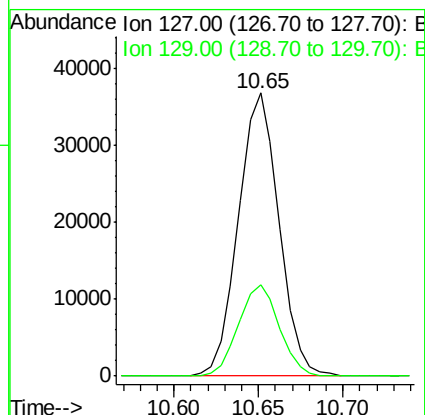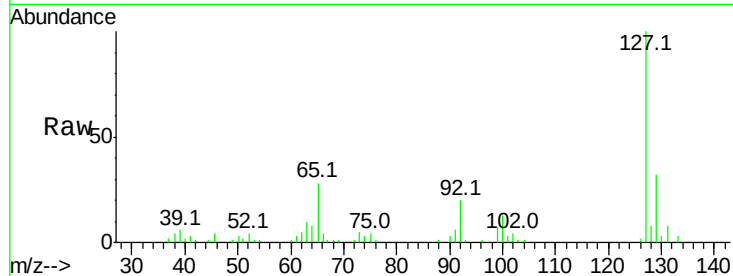

#31
Hexachlorobutadiene
Concen: 20.81 ng/ul
RT: 10.82 min Scan# 1315
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Tgt Ion:225 Resp: 27915
Ion Ratio Lower Upper
225 100
223 62.1 51.4 77.2
227 63.8 50.7 76.1

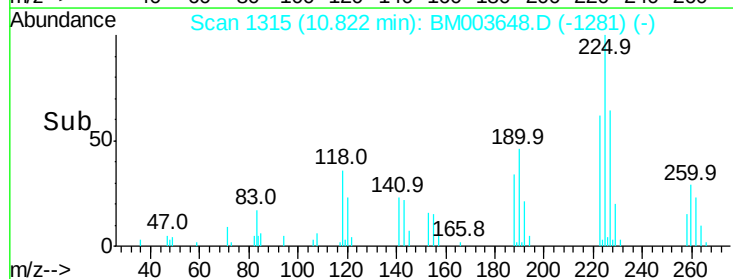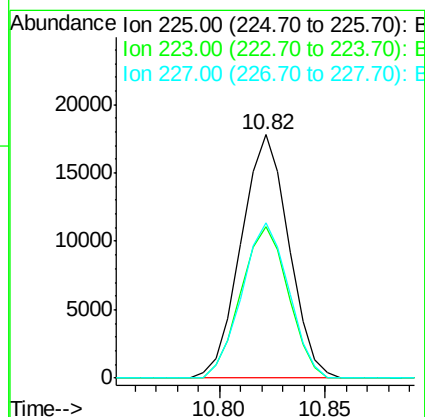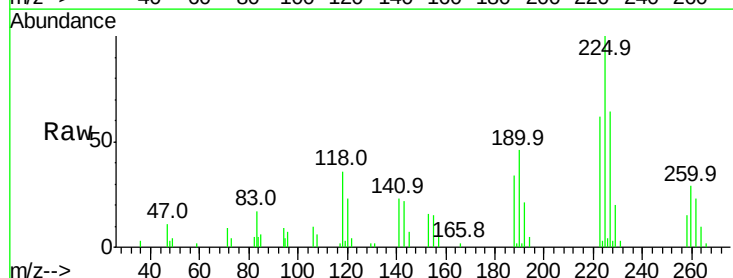

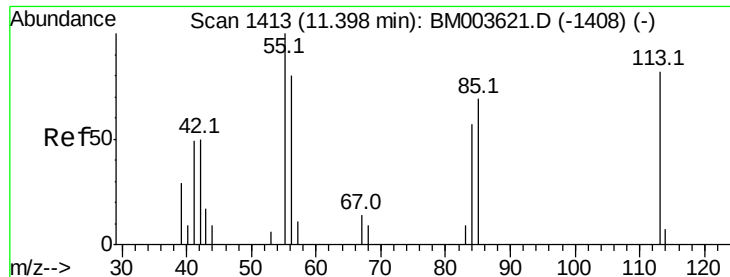

#32

Caprolactam

Concen: 19.44 ng/ul

RT: 11.40 min Scan# 1413

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056


Tot Ion:113 Resp: 15823

Ion Ratio Lower Upper

113 100

55 120.8 101.9 152.9




56 98.6 81.2 121.8

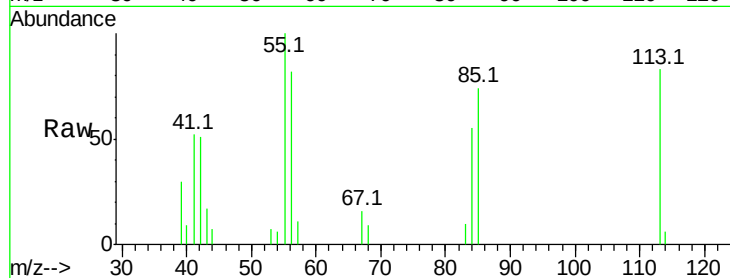

Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BM003621.D (-1408) (-)

Ion 56.00 (55.70 to 56.70): BM003621.D (-1408) (-)

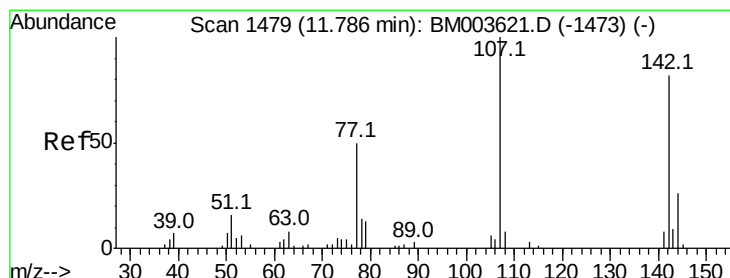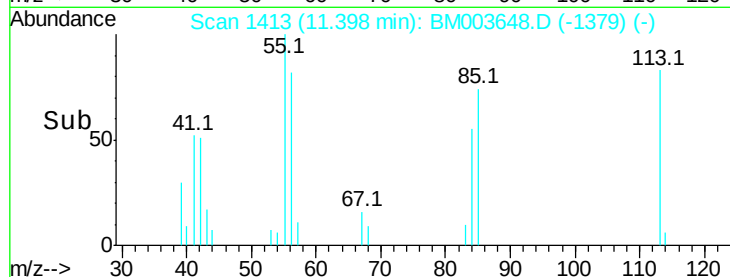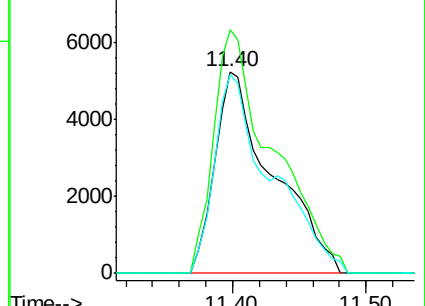

#33

4-Chloro-3-methylphenol

Concen: 21.02 ng/ul

RT: 11.79 min Scan# 1479

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Tgt Ion:107 Resp: 53719

Ion Ratio Lower Upper

107 100

144 25.6 20.4 30.6



142 78.5 62.5 93.7

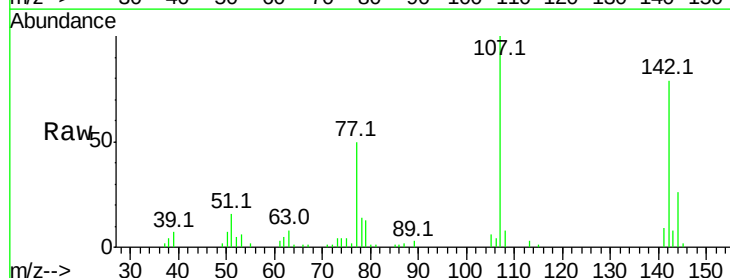


Abundance Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E

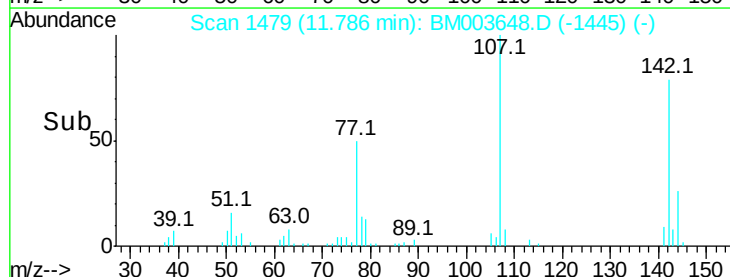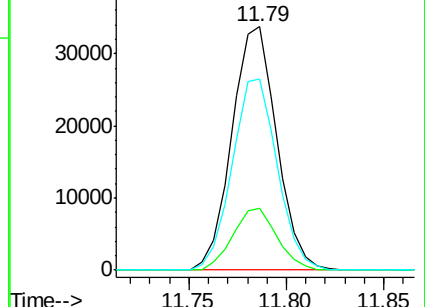

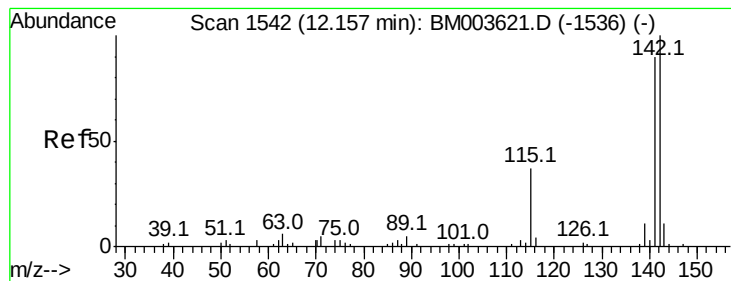

#34

2-Methylnaphthalene

Concen: 20.67 ng/ul

RT: 12.16 min Scan# 1542

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :


SSTD02056

Tot Ion:142 Resp: 111914

Ion Ratio Lower Upper




142 100

141 90.6 71.6 107.4



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

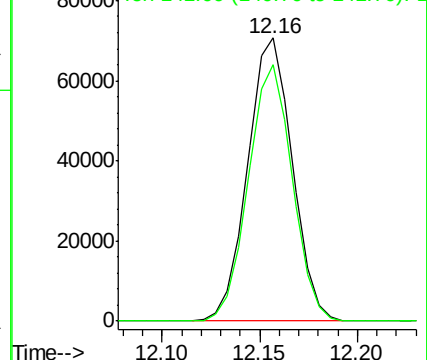

#35

1-Methylnaphthalene

Concen: 20.73 ng/ul

RT: 12.38 min Scan# 1580

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Tgt Ion:142 Resp: 106621

Ion Ratio Lower Upper

142 100

141 93.1 74.9 112.3



116 3.9 3.1 4.7




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

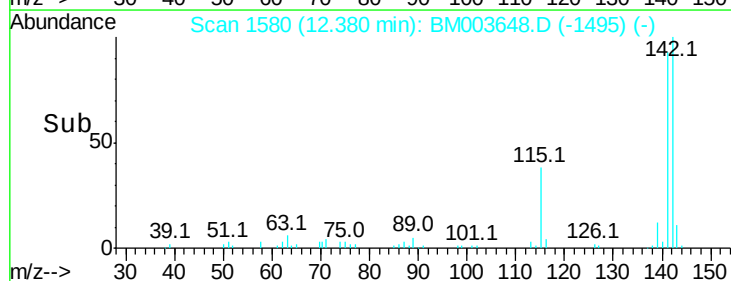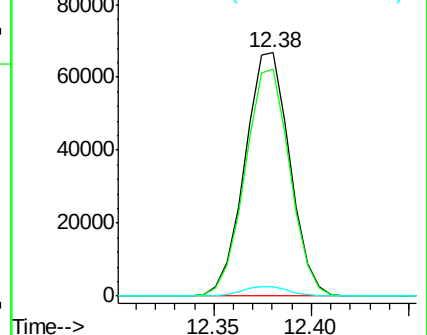



#37

1,2,4,5-Tetrachlorobenzene

Concen: 20.59 ng/ul

RT: 12.53 min Scan# 1606

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056

Tot Ion:216 Resp: 55674


Ion Ratio Lower Upper

216 100

214 78.0 62.5 93.7

179 22.2 18.2 27.2

108 18.2 14.2 21.2






Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E

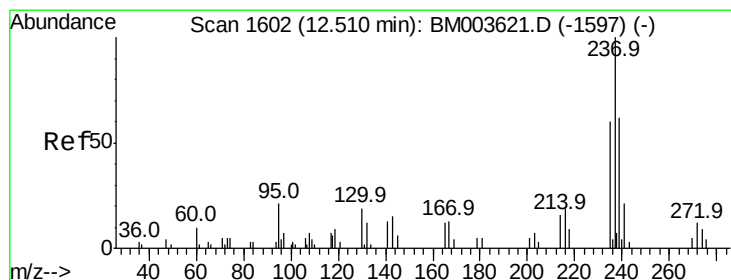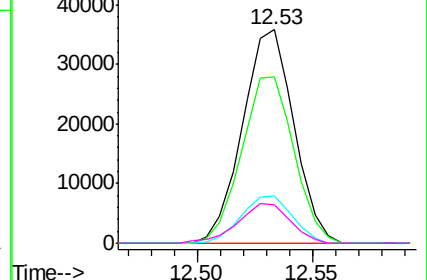

#38

Hexachlorocyclopentadiene

Concen: 12.85 ng/ul

RT: 12.51 min Scan# 1602

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Tgt Ion:237 Resp: 18612

Ion Ratio Lower Upper

237 100

235 61.6 50.4 75.6



272 11.8 9.6 14.4




Abundance Ion 237.00 (236.70 to 237.70): E

Ion 235.00 (234.70 to 235.70): E

Ion 272.00 (271.70 to 272.70): E



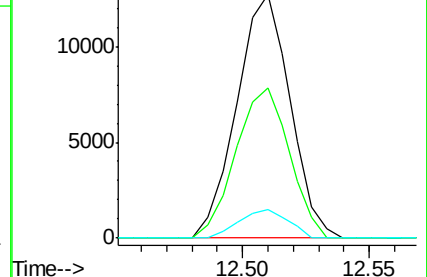



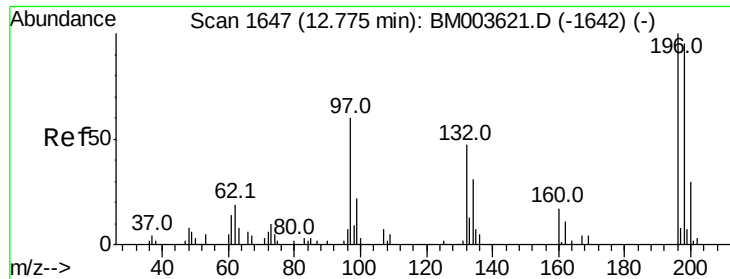

#39
 2,4,6-Trichlorophenol
 Concen: 20.41 ng/ul
 RT: 12.77 min Scan# 1647
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02056


Tot Ion:196 Resp: 37298
 Ion Ratio Lower Upper
 196 100
 198 97.2 76.6 114.8
 200 30.5 24.7 37.1

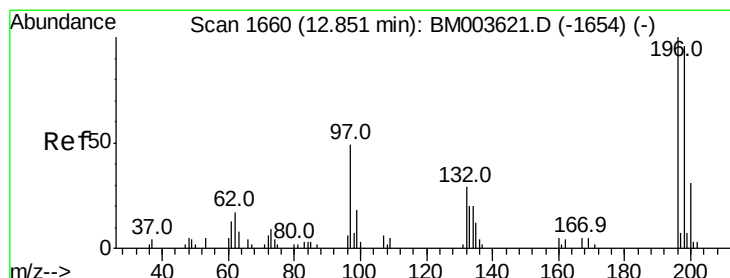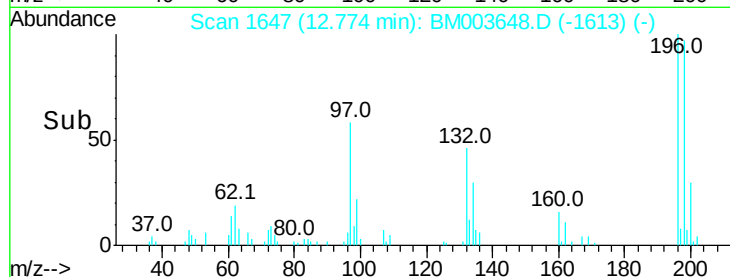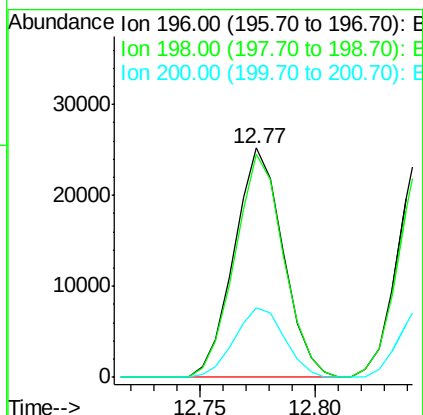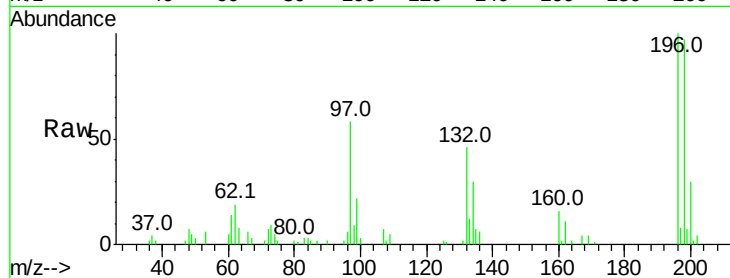

#40
 2,4,5-Trichlorophenol
 Concen: 20.80 ng/ul
 RT: 12.85 min Scan# 1659
 Delta R.T. -0.01 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion:196 Resp: 41981
 Ion Ratio Lower Upper
 196 100
 198 95.3 76.9 115.3
 200 31.2 25.0 37.4


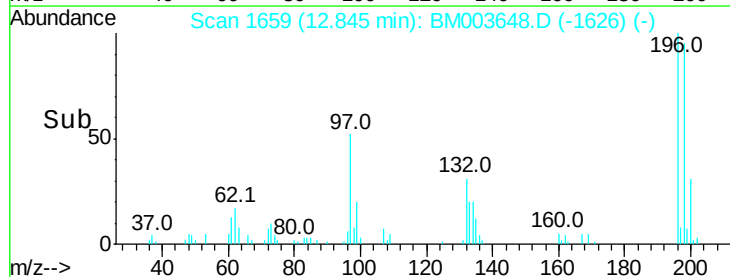
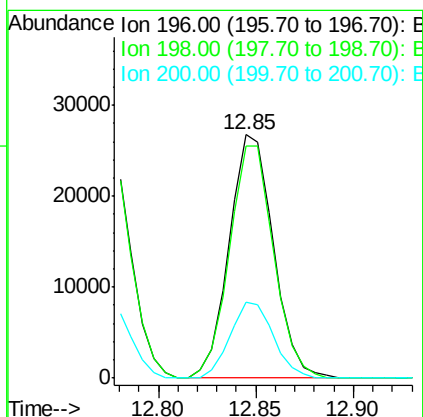
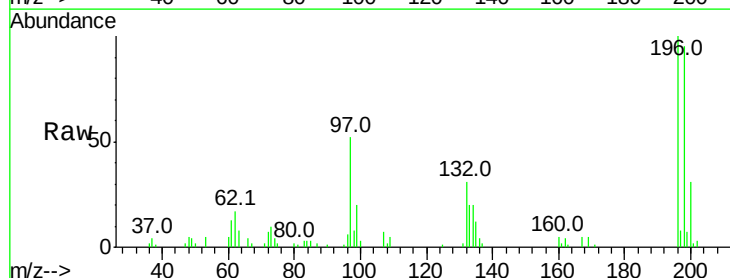




#41
 1,1'-Biphenyl
 Concen: 20.39 ng/ul
 RT: 13.18 min Scan# 1716
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02056


Tot Ion:	154	Resp:	148033
Ion	Ratio	Lower	Upper
154	100		
153	40.1	32.1	48.1
76	11.2	9.5	14.3

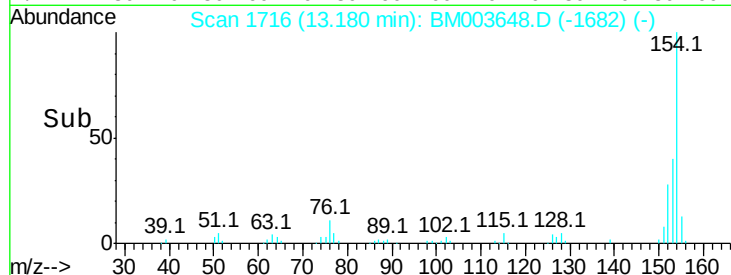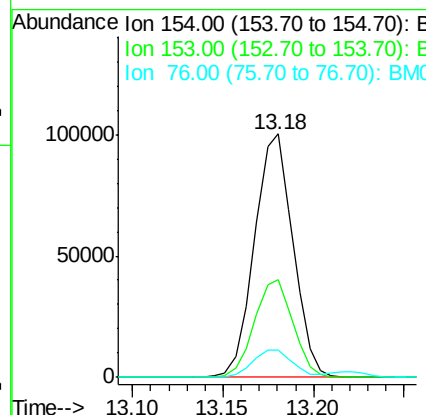

#42
 2-Chloronaphthalene
 Concen: 20.85 ng/ul
 RT: 13.22 min Scan# 1723
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion:	162	Resp:	113691
Ion	Ratio	Lower	Upper
162	100		
164	32.8	25.9	38.9
127	41.3	34.1	51.1

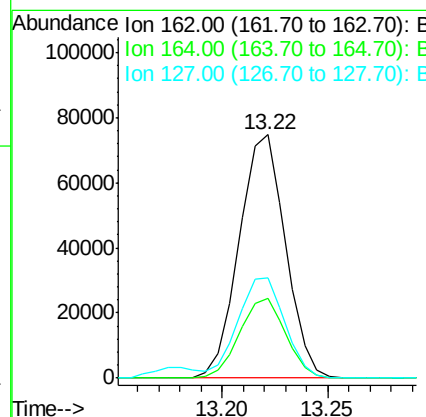







#43
2-Nitroaniline
Concen: 21.14 ng/ul
RT: 13.43 min Scan# 1758
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Instrument :
BNA_M
ClientSampleId :
SSTD02056

Tot Ion: 65 Resp: 31907
Ion Ratio Lower Upper
65 100
92 75.3 60.4 90.6
138 119.6 99.8 149.6




Abundance Ion 65.00 (64.70 to 65.70): BM003648.D (-1753) (-)
Ion 92.00 (91.70 to 92.70): BM003648.D (-1753) (-)
Ion 138.00 (137.70 to 138.70): BM003648.D (-1753) (-)


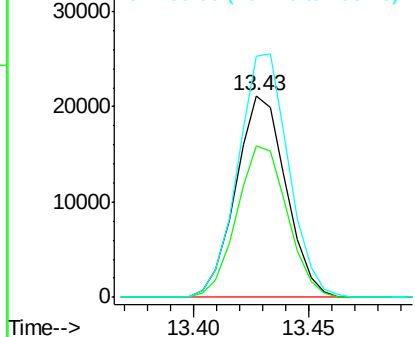



#45
Dimethylphthalate
Concen: 19.73 ng/ul
RT: 13.81 min Scan# 1823
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Tgt Ion:163 Resp: 149126
Ion Ratio Lower Upper
163 100
194 3.7 3.2 4.8
164 9.8 7.8 11.8



Abundance Ion 163.00 (162.70 to 163.70): BM003648.D (-1789) (-)
Ion 194.00 (193.70 to 194.70): BM003648.D (-1789) (-)
Ion 164.00 (163.70 to 164.70): BM003648.D (-1789) (-)




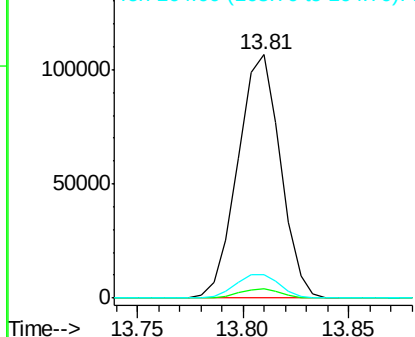




#46
 2,6-Dinitrotoluene
 Concen: 20.73 ng/ul
 RT: 13.93 min Scan# 1844
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02056


Tot Ion:165 Resp: 30521
 Ion Ratio Lower Upper
 165 100
 89 57.0 42.4 63.6
 121 22.1 16.6 24.8

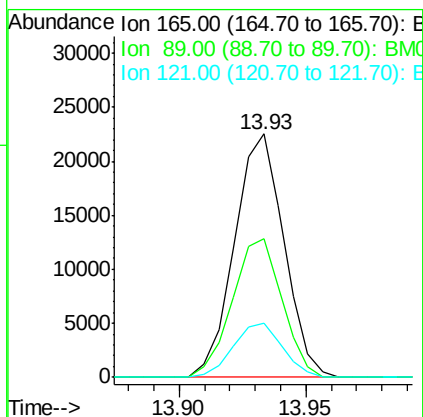

#48
 Acenaphthylene
 Concen: 21.01 ng/ul
 RT: 14.07 min Scan# 1867
 Delta R.T. -0.01 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion:152 Resp: 193174
 Ion Ratio Lower Upper
 152 100
 151 20.2 15.7 23.5
 153 13.2 10.5 15.7

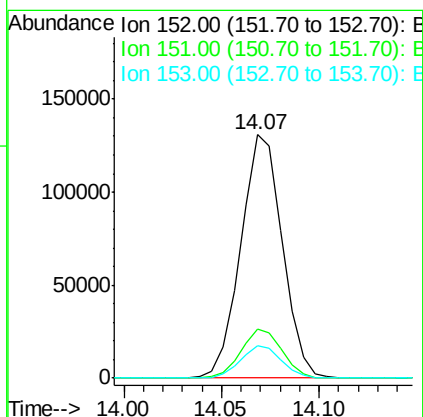



#49

3-Nitroaniline

Concen: 21.89 ng/ul

RT: 14.26 min Scan# 1900

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056


Tot Ion:138 Resp: 35961

Ion Ratio Lower Upper

138 100

108 11.1 8.7 13.1




92 108.8 88.2 132.4



Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BM

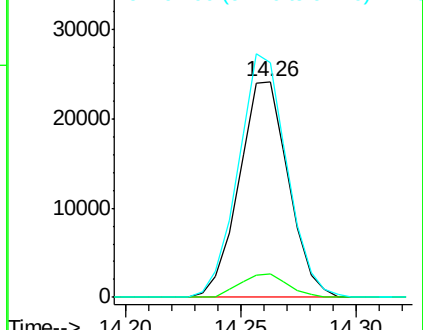

#50

Acenaphthene

Concen: 20.81 ng/ul

RT: 14.42 min Scan# 1926

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Tgt Ion:153 Resp: 127808

Ion Ratio Lower Upper

153 100

152 47.2 38.3 57.5



154 87.6 71.8 107.8




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

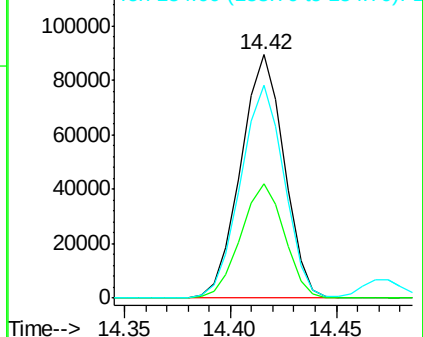



#51

2,4-Dinitrophenol

Concen: 18.83 ng/ul

RT: 14.47 min Scan# 1936

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleID :

SSTD02056


Tot Ion:184 Resp: 14701

Ion Ratio Lower Upper

184 100

63 56.2 46.5 69.7




154 68.2 54.6 82.0



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 63.00 (62.70 to 63.70): BM

Ion 154.00 (153.70 to 154.70): E

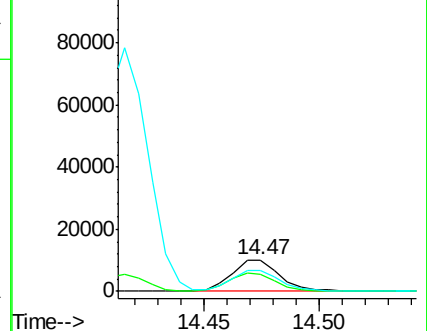

#53

4-Nitrophenol

Concen: 20.96 ng/ul

RT: 14.57 min Scan# 1953

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Tgt Ion:109 Resp: 25525

Ion Ratio Lower Upper

109 100

139 127.7 103.7 155.5



65 115.7 89.4 134.2




Abundance Ion 109.00 (108.70 to 109.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 65.00 (64.70 to 65.70): BM

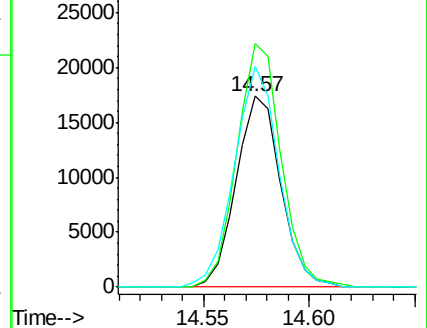



#54

Dibenzenofuran

Concen: 20.65 ng/ul

RT: 14.75 min Scan# 1983

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampled :


SSTD02056

Tot Ion:168 Resp: 181041

Ion Ratio Lower Upper

168 100

139 40.4 32.2 48.2



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

14.75



150000

100000

50000

0

Time-->



#55

2,4-Dinitrotoluene

Concen: 21.57 ng/ul

RT: 14.72 min Scan# 1978

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Tgt Ion:165 Resp: 48226

Ion Ratio Lower Upper

165 100

63 37.6 29.8 44.6

182 2.9 2.2 3.4



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BM0

Ion 182.00 (181.70 to 182.70): E

14.72

40000


30000


20000

10000

0

Time-->







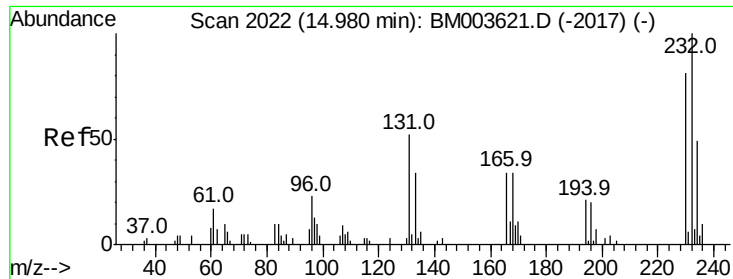

#56
 2,3,4,6-Tetrachlorophenol
 Concen: 20.63 ng/ul
 RT: 14.98 min Scan# 2022
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02056


Tot Ion:	232	Resp:	35886
Ion	Ratio	Lower	Upper
232	100		
131	50.9	39.4	59.2
130	2.9	2.2	3.2
166	34.3	26.6	39.8

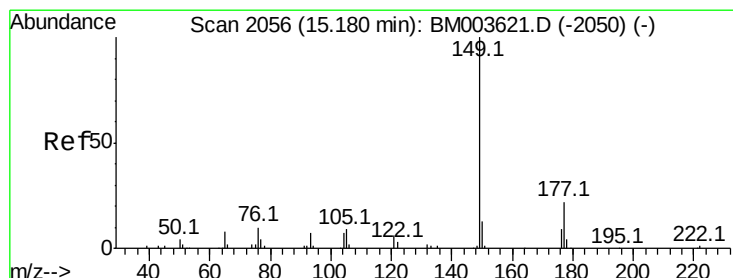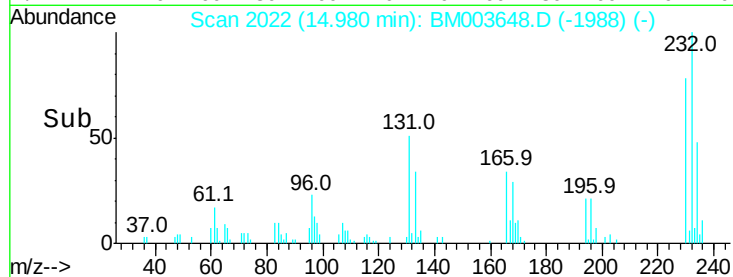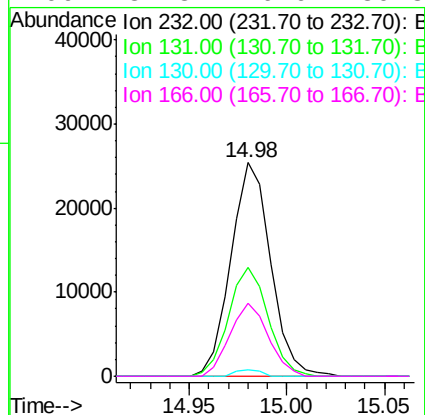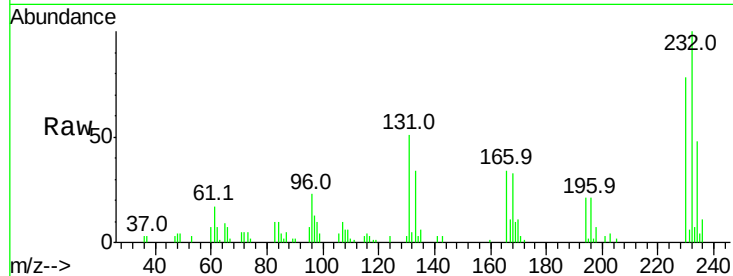

#57
 Diethylphthalate
 Concen: 19.81 ng/ul
 RT: 15.17 min Scan# 2055
 Delta R.T. -0.01 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion:	149	Resp:	158373
Ion	Ratio	Lower	Upper
149	100		
177	21.0	17.4	26.2
150	12.6	10.0	15.0

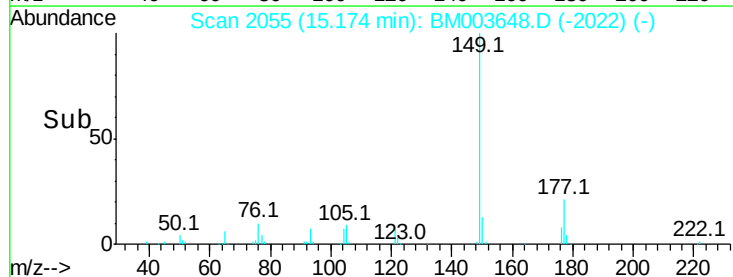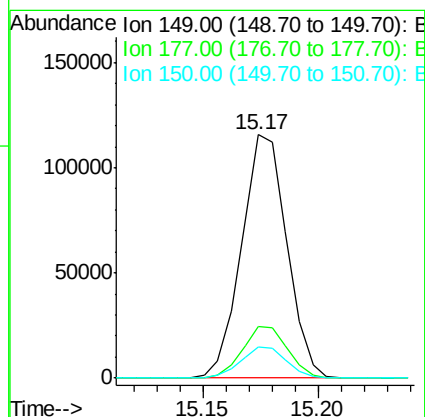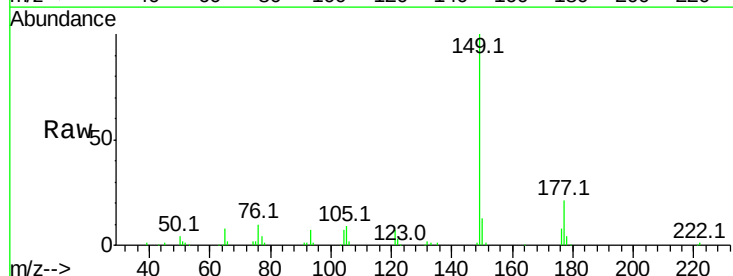


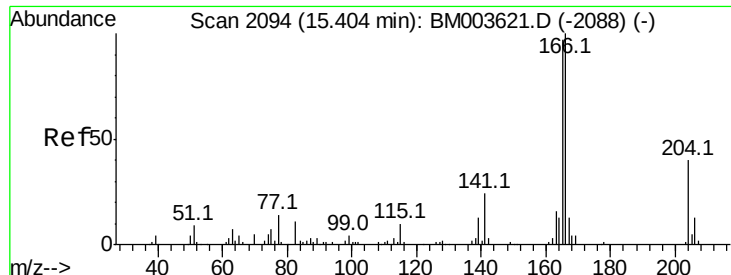




#59
Fluorene
 Concen: 21.05 ng/ul
 RT: 15.40 min Scan# 2094
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Instrument :
 BNA_M
 ClientSampleId :
 SSTD02056

Tot Ion:166 Resp: 148075
 Ion Ratio Lower Upper
 166 100
 165 97.4 78.5 117.7
 167 13.5 10.7 16.1

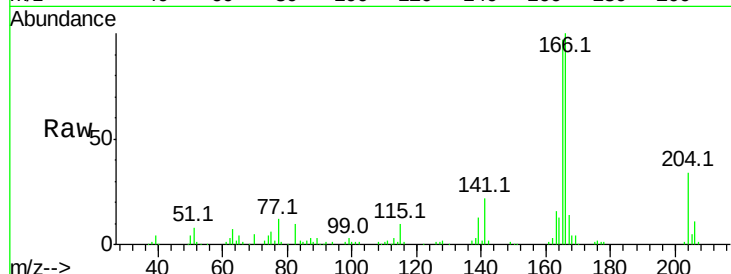


Abundance Ion 166.00 (165.70 to 166.70): E
 Ion 165.00 (164.70 to 165.70): E
 Ion 167.00 (166.70 to 167.70): E


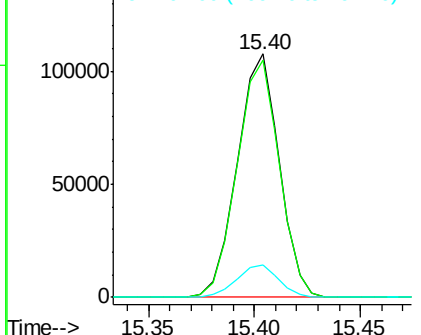



#60
4-Chlorophenyl-phenylether
 Concen: 20.50 ng/ul
 RT: 15.40 min Scan# 2093
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion:204 Resp: 70007
 Ion Ratio Lower Upper
 204 100
 206 32.0 26.2 39.4
 141 66.5 54.6 81.8



Abundance Ion 204.00 (203.70 to 204.70): E
 Ion 206.00 (205.70 to 206.70): E
 Ion 141.00 (140.70 to 141.70): E




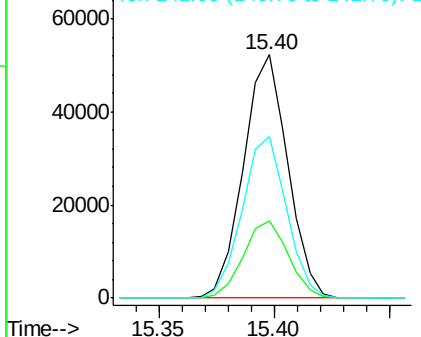




#61
4-Nitroaniline
Concen: 22.28 ng/ul
RT: 15.43 min Scan# 2098
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19




Instrument :
BNA_M
ClientSampleId :
SSTD02056


Tot Ion:138 Resp: 40662
Ion Ratio Lower Upper
138 100
92 47.7 40.6 60.8
108 83.1 67.0 100.6

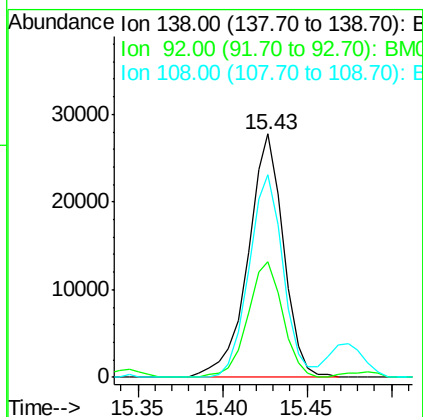

#64
4,6-Dinitro-2-methylphenol
Concen: 20.11 ng/ul
RT: 15.49 min Scan# 2108
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Tgt Ion:198 Resp: 26558
Ion Ratio Lower Upper
198 100
182 4.4 3.1 4.7
77 27.0 20.1 30.1

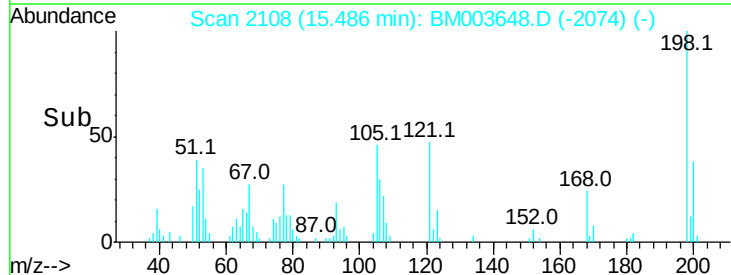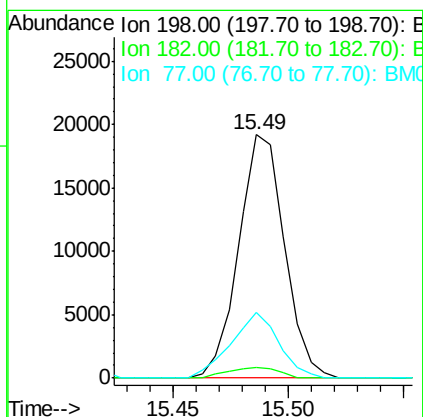







#65
 N-Nitrosodiphenylamine
 Concen: 20.31 ng/ul
 RT: 15.61 min Scan# 2129
 Delta R.T. -0.01 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Instrument :
 BNA_M
 ClientSampleId :
 SSTD02056

Tot Ion:169 Resp: 130031
 Ion Ratio Lower Upper
 169 100
 168 66.6 53.8 80.8
 167 36.1 29.3 43.9




Abundance Ion 169.00 (168.70 to 169.70): E
 Ion 168.00 (167.70 to 168.70): E
 Ion 167.00 (166.70 to 167.70): E


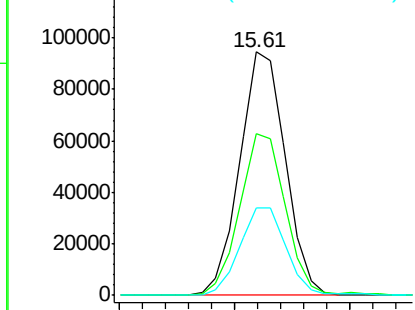



#66
 4-Bromophenyl-phenylether
 Concen: 20.01 ng/ul
 RT: 16.29 min Scan# 2245
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion:248 Resp: 43582
 Ion Ratio Lower Upper
 248 100
 250 96.7 78.7 118.1
 141 84.5 72.2 108.2



Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

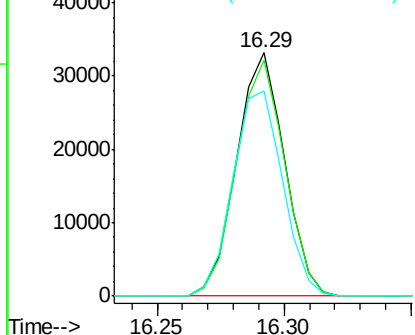







#67
Hexachlorobenzene
Concen: 20.72 ng/ul
RT: 16.41 min Scan# 2265
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Instrument :
BNA_M
ClientSampleId :
SSTD02056

Tot Ion:284 Resp: 50176
Ion Ratio Lower Upper
284 100
142 39.4 33.1 49.7
249 33.6 27.1 40.7




Abundance Ion 284.00 (283.70 to 284.70): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E

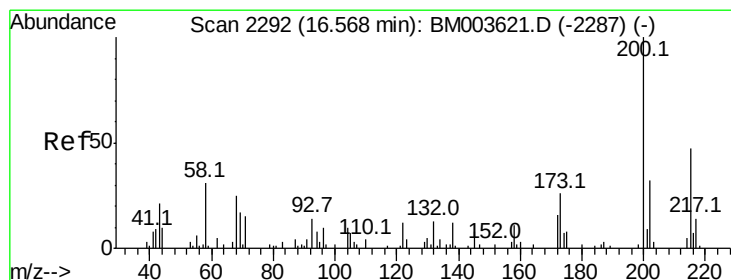
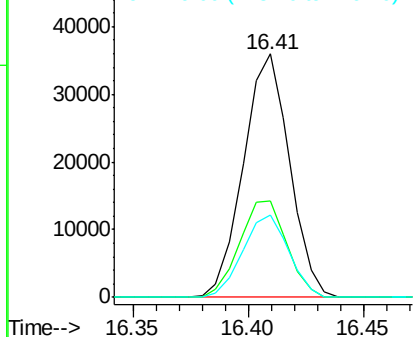



#68
Atrazine
Concen: 20.00 ng/ul
RT: 16.56 min Scan# 2291
Delta R.T. -0.01 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Tgt Ion:200 Resp: 49181
Ion Ratio Lower Upper
200 100
173 26.6 21.6 32.4
215 46.5 37.0 55.4

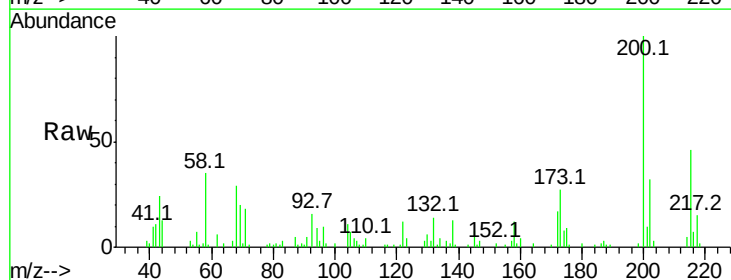

Abundance Ion 200.00 (199.70 to 200.70): E
Ion 173.00 (172.70 to 173.70): E
Ion 215.00 (214.70 to 215.70): E

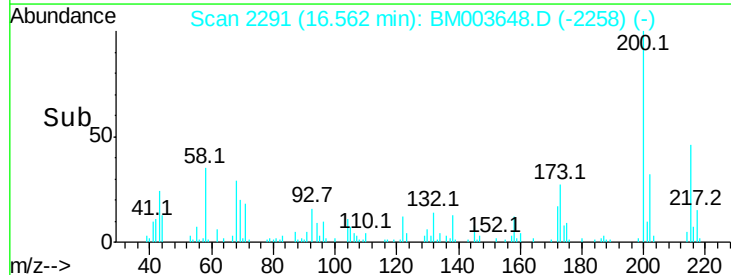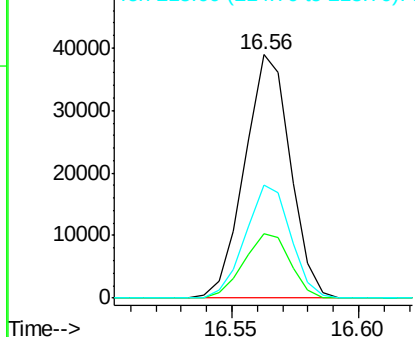


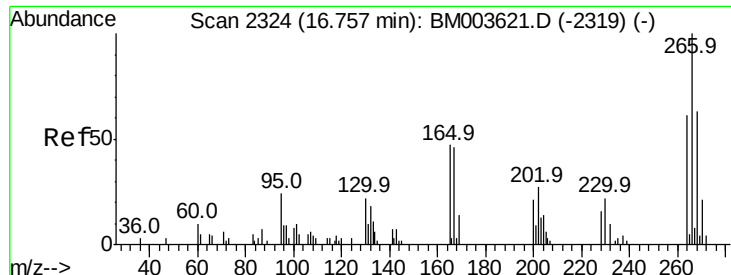




#69
 Pentachlorophenol
 Concen: 19.69 ng/ul
 RT: 16.76 min Scan# 2324
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Instrument :
 BNA_M
 ClientSampled :
 SSTD02056

Tot Ion	Ratio	Lower	Upper
266	100		
264	61.7	50.5	75.7
268	64.6	50.9	76.3

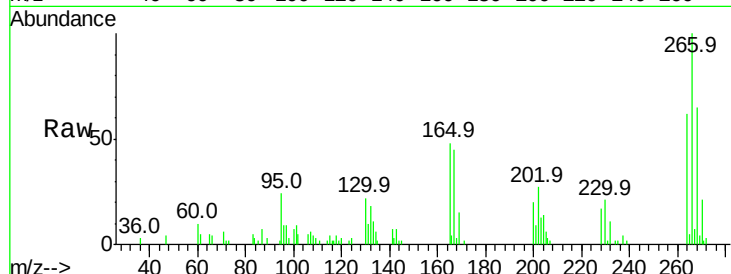


Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E


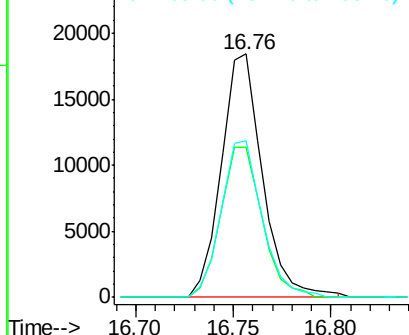



#70
 Phenanthrene
 Concen: 20.69 ng/ul
 RT: 17.14 min Scan# 2389
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.5	12.2	18.4
176	19.4	15.6	23.4



Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

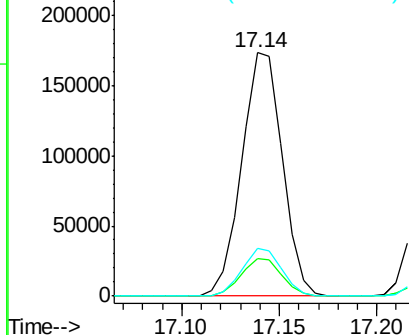


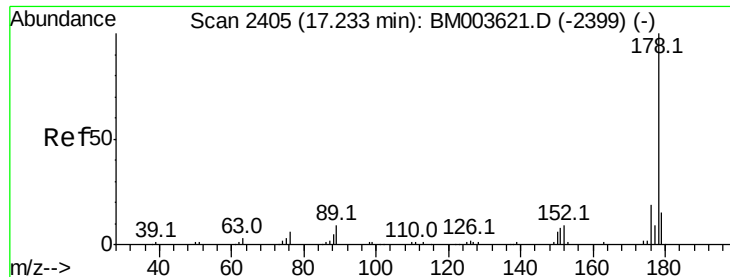




#72
 Anthracene
 Concen: 20.96 ng/uL
 RT: 17.23 min Scan# 2405
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Instrument :
 BNA_M
 ClientSampleId :
 SSTD02056

Tot Ion:178 Resp: 258660
 Ion Ratio Lower Upper
 178 100
 179 15.2 12.1 18.1
 176 18.7 14.8 22.2

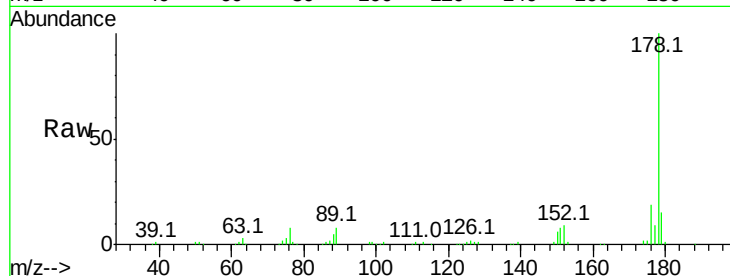


Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

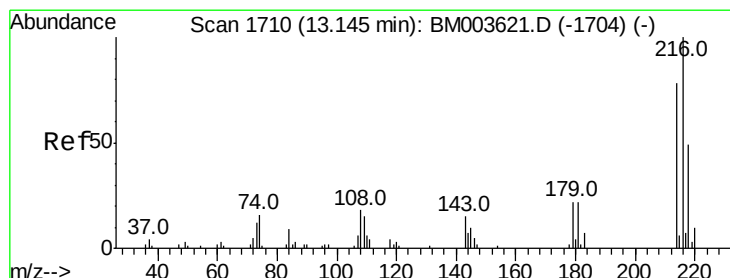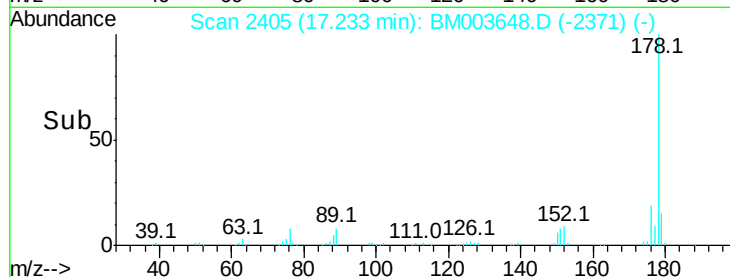
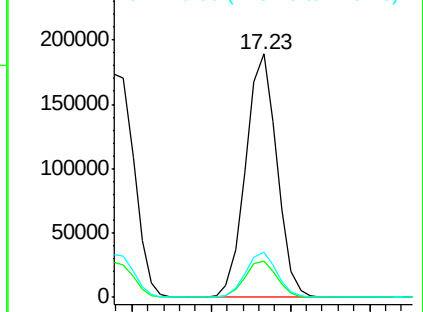



#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 20.48 ng/uL
 RT: 13.15 min Scan# 1710
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion:216 Resp: 61402
 Ion Ratio Lower Upper
 216 100
 214 79.2 62.5 93.7
 218 49.7 38.4 57.6

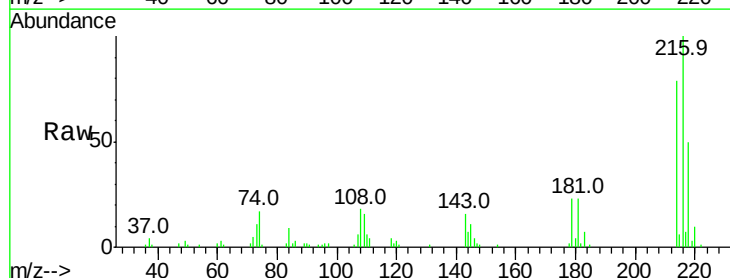

Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 218.00 (217.70 to 218.70): E

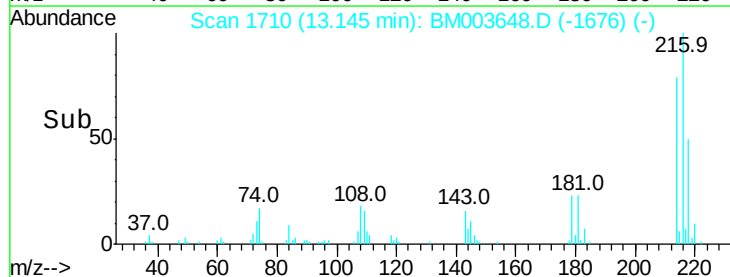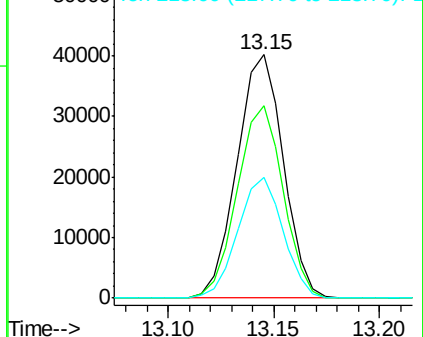

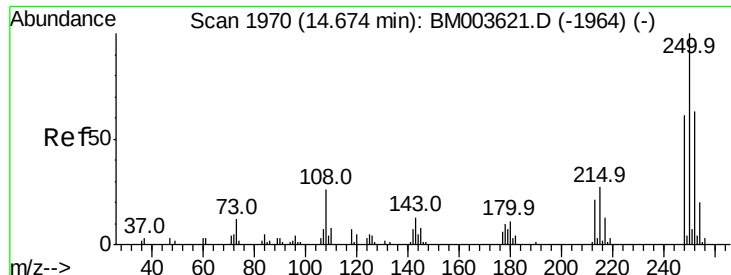

#74

Pentachlorobenzene

Concen: 20.46 ng/uL

RT: 14.67 min Scan# 1970

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056


Tot Ion:250 Resp: 57770

Ion Ratio Lower Upper

250 100

248 61.8 50.6 75.8




252 62.5 51.4 77.0



Abundance Ion 250.00 (249.70 to 250.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 252.00 (251.70 to 252.70): E

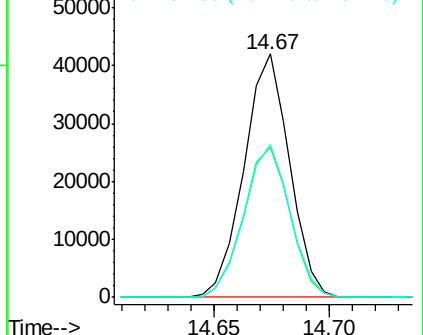

#75

Carbazole

Concen: 21.67 ng/uL

RT: 17.50 min Scan# 2451

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Tgt Ion:167 Resp: 244038

Ion Ratio Lower Upper

167 100

166 21.5 17.0 25.6



139 13.9 11.0 16.4




Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E




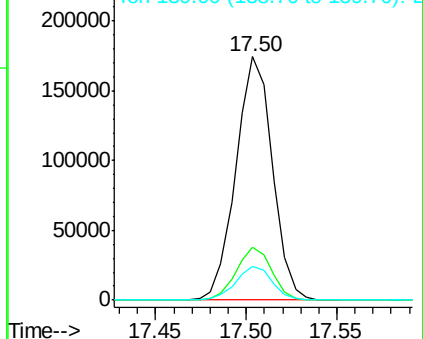




#76
Di-n-butylphthalate
Concen: 19.48 ng/ul
RT: 18.07 min Scan# 2547
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19




Instrument :
BNA_M
ClientSampleId :
SSTD02056


Tot Ion:149 Resp: 285385
Ion Ratio Lower Upper
149 100
150 9.1 7.4 11.0
104 5.0 4.0 6.0

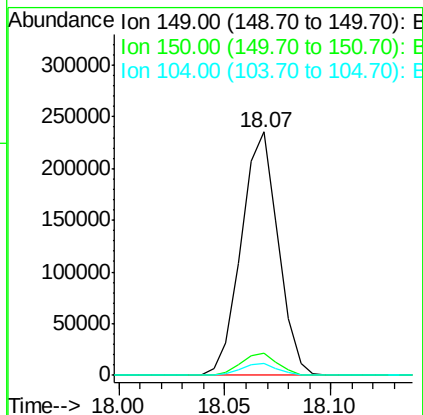

#77
Fluoranthene
Concen: 22.02 ng/ul
RT: 19.16 min Scan# 2733
Delta R.T. -0.00 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Tgt Ion:202 Resp: 306239
Ion Ratio Lower Upper
202 100
101 10.8 8.8 13.2
100 8.2 6.6 9.8

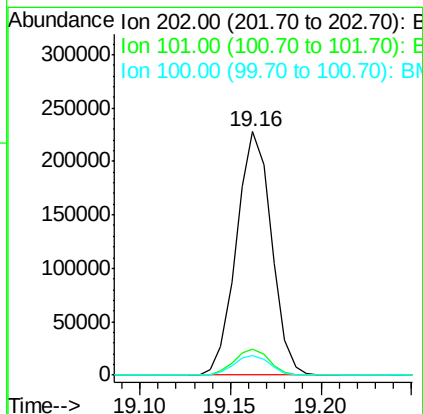


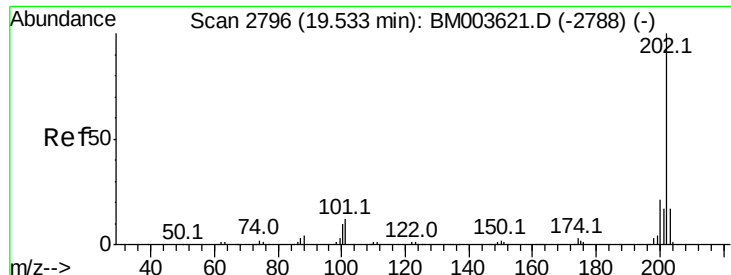




#80
Pvrene
Concen: 21.07 ng/ul
RT: 19.53 min Scan# 2795
Delta R.T. -0.01 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Instrument :
BNA_M
ClientSampleId :
SSTD02056

Tot Ion	Ratio	Lower	Upper
202	100		
101	12.5	10.2	15.2
100	10.4	8.5	12.7




Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B


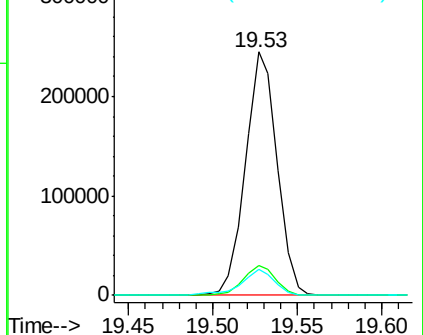



#81
Butylbenzylphthalate
Concen: 20.34 ng/ul
RT: 20.43 min Scan# 2949
Delta R.T. -0.01 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Tgt Ion	Ratio	Lower	Upper
149	100		
91	67.2	53.4	80.2
206	20.0	16.6	24.8



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 91.00 (90.70 to 91.70): BM0
Ion 206.00 (205.70 to 206.70): E




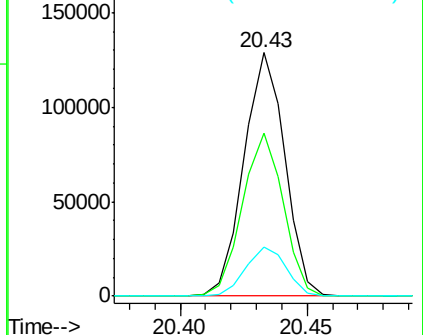




#82
 3,3'-Dichlorobenzidine
 Concen: 22.03 ng/ul
 RT: 21.22 min Scan# 3083
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02056


Tot Ion:252 Resp: 110759
 Ion Ratio Lower Upper
 252 100
 254 64.2 52.2 78.2
 126 11.1 9.4 14.2

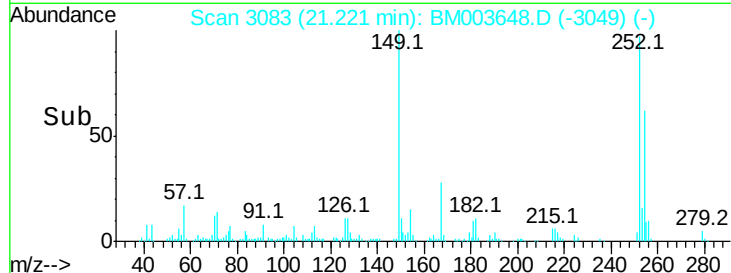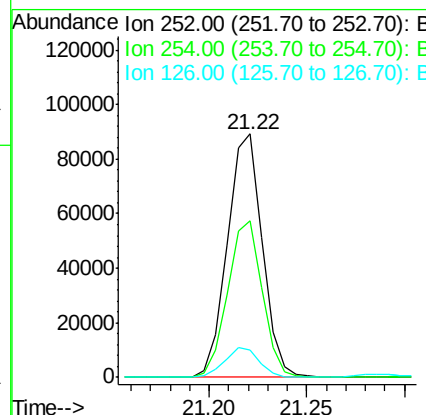

#83
 Benzo(a)anthracene
 Concen: 20.66 ng/ul
 RT: 21.29 min Scan# 3094
 Delta R.T. -0.00 min
 Lab File: BM003648.D
 Acq: 20 Dec 2015 11:19

Tgt Ion:228 Resp: 327554
 Ion Ratio Lower Upper
 228 100
 229 19.7 15.7 23.5
 226 26.4 21.8 32.6

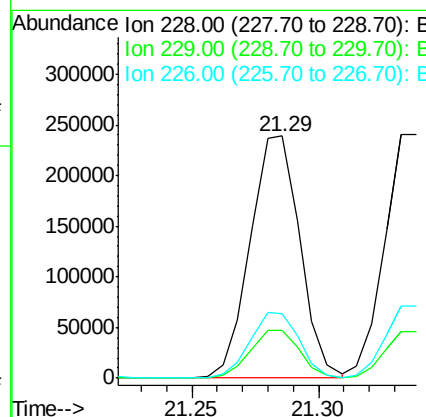



#84

Bis(2-ethylhexyl)phthalate

Concen: 19.90 ng/ul

RT: 21.22 min Scan# 3082

Delta R.T. -0.00 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056


Tot Ion:149 Resp: 212083

Ion Ratio Lower Upper

149 100

167 27.5 21.6 32.4




279 4.0 3.0 4.4



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

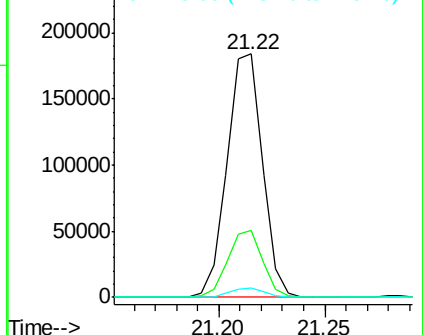

#85

Chrysene

Concen: 20.43 ng/ul

RT: 21.33 min Scan# 3102

Delta R.T. -0.01 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Tgt Ion:228 Resp: 312396

Ion Ratio Lower Upper

228 100

226 29.7 24.0 36.0



229 19.4 15.6 23.4




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

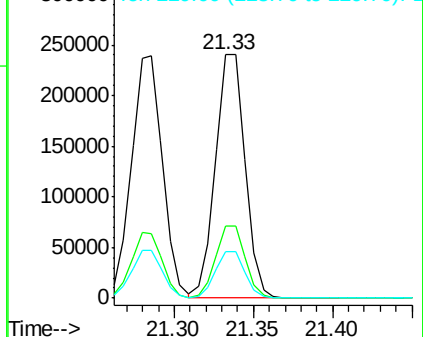

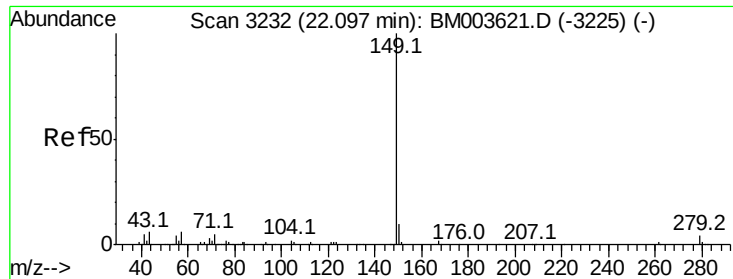

#87

Di-n-octyl phthalate

Concen: 24.13 ng/ul

RT: 22.09 min Scan# 3231

Delta R.T. -0.01 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Instrument :

BNA_M




ClientSampleId :

SSTD02056

Tgt Ion:149 Resp: 393970

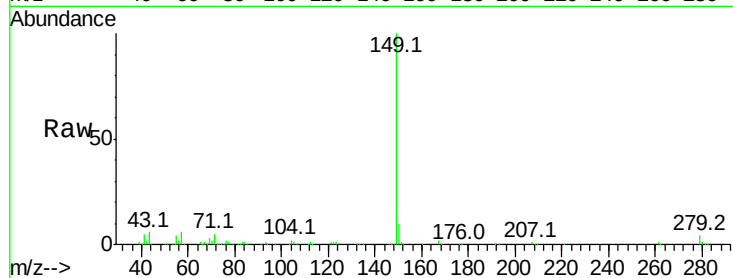

Abundance Ion 149.00 (148.70 to 149.70): E

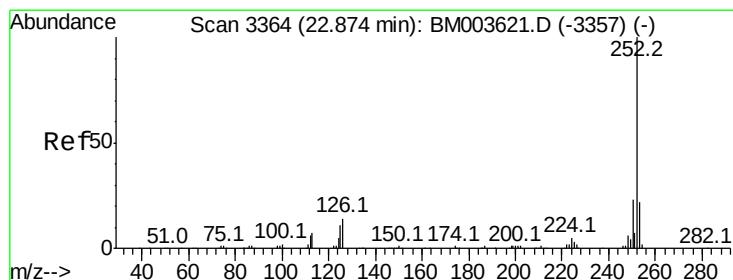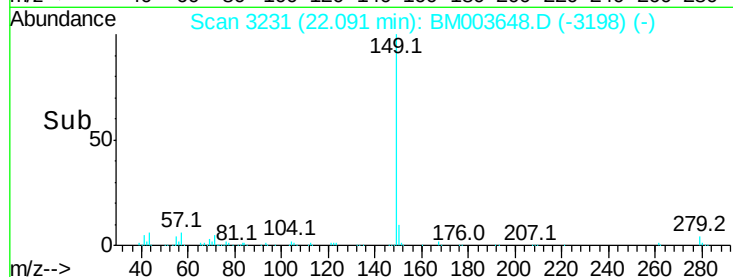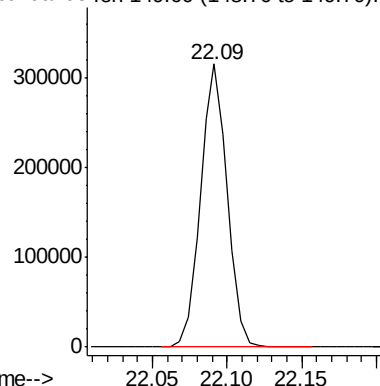

#88

Benzo(b)fluoranthene

Concen: 21.56 ng/ul

RT: 22.87 min Scan# 3363


Delta R.T. -0.01 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Tgt Ion:252 Resp: 307103



Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.5	26.3
125	10.3	8.5	12.7

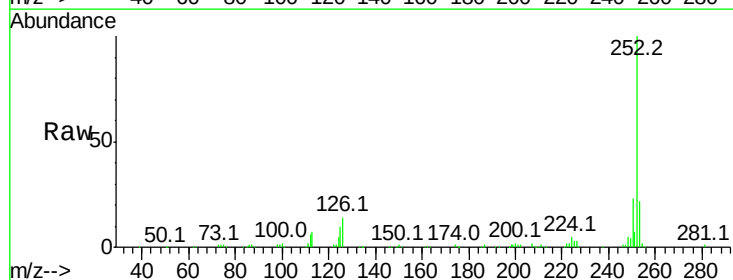


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



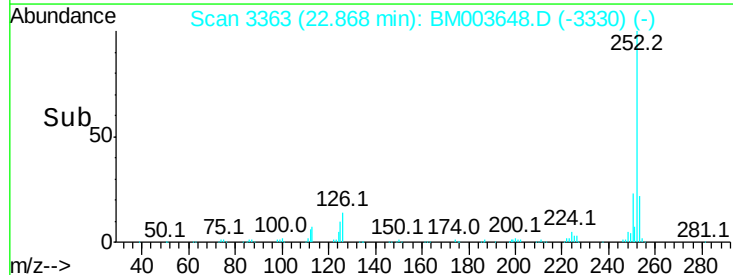
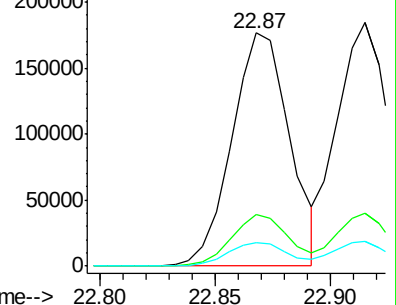




#89
Benzo(k)fluoranthene
Concen: 21.58 ng/ul
RT: 22.91 min Scan# 3371
Delta R.T. -0.01 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19




Instrument :
BNA_M
ClientSampleId :
SSTD02056


Tot Ion	Ratio	Lower	Upper
252	100		
253	21.9	17.3	25.9
125	10.4	8.2	12.2

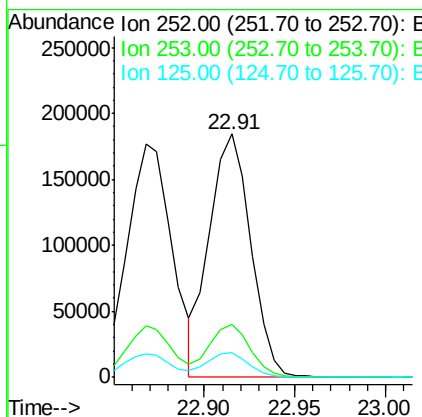

#91
Benzo(a)pyrene
Concen: 20.76 ng/ul
RT: 23.45 min Scan# 3462
Delta R.T. -0.01 min
Lab File: BM003648.D
Acq: 20 Dec 2015 11:19

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.6	17.2	25.8
125	10.7	9.0	13.6

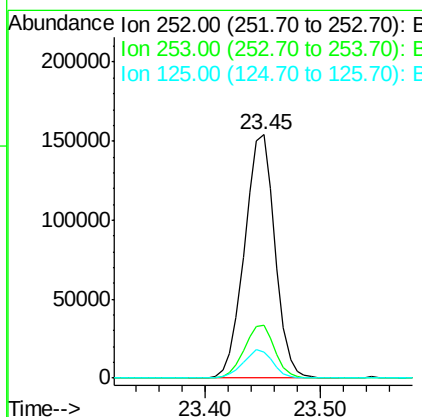

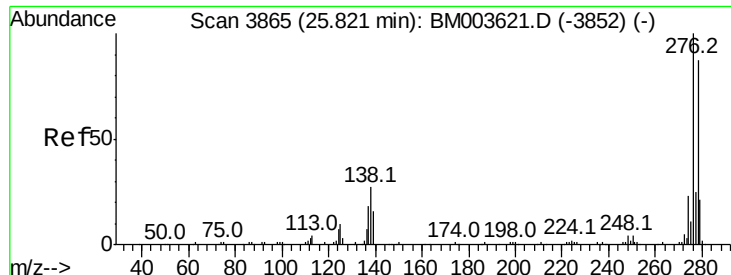

#92

Indeno(1,2,3-cd)pyrene

Concen: 19.48 ng/ul

RT: 25.81 min Scan# 3863

Delta R.T. -0.01 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056


Tot Ion:276 Resp: 285675

Ion Ratio Lower Upper

276 100

138 26.5 22.3 33.5




277 25.2 20.2 30.2



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

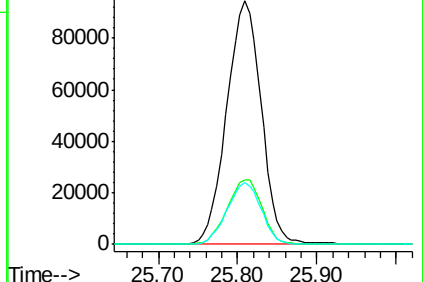

#93

Dibenzo(a,h)anthracene

Concen: 19.64 ng/ul

RT: 25.82 min Scan# 3865

Delta R.T. -0.01 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19


Tgt Ion:278 Resp: 241615

Ion Ratio Lower Upper

278 100

139 17.4 13.9 20.9



279 23.7 19.0 28.4




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

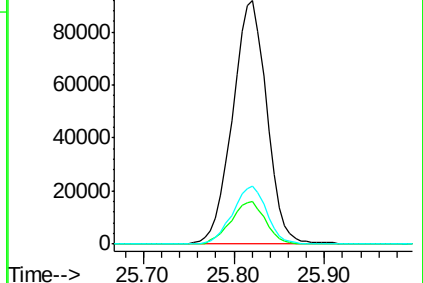

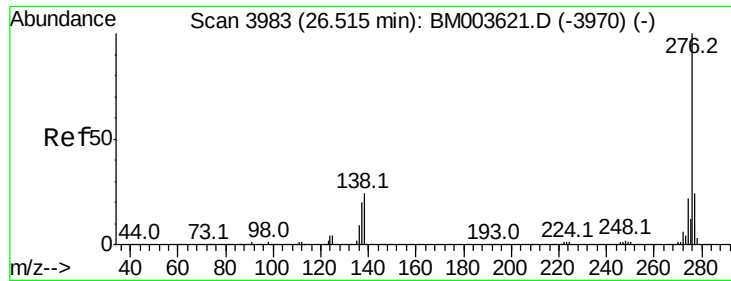

#94

Benzo(a,h,i)perylene

Concen: 18.79 ng/ul

RT: 26.50 min Scan# 3981

Delta R.T. -0.01 min

Lab File: BM003648.D

Acq: 20 Dec 2015 11:19

Instrument :

BNA_M

ClientSampleId :

SSTD02056


Tot Ion:276 Resp: 226329

Ion Ratio Lower Upper

276 100

138 22.7 18.9 28.3

277 23.5 19.2 28.8



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

