

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122015\
 Data File : BM003652.D
 Acq On : 20 Dec 2015 13:42
 Operator : UM/SJ
 Sample : G4801-24
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9C72

Quant Time: Dec 21 02:22:52 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 21 02:19:57 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	20269	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	98362	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	61932	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	150940	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	190242	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	167241	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	2308	6.13	ng/uL	0.00
5) Phenol-d5	6.87	99	57310	33.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	32303	35.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	48045	34.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	50611	34.21	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	24939	34.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	28395	35.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	49906	34.06	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	64769	33.19	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	180143	35.19	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	215130	36.92	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	31626	31.72	ng/ul	0.00
58) Fluorene-d10	15.35	176	157525	37.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	23613	27.76	ng/ul	0.00
71) Anthracene-d10	17.20	188	259515	37.79	ng/ul	0.00
79) Pyrene-d10	19.50	212	311661	37.51	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	318075	38.29	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.80	163	82237	15.71	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122015\
Data File : BM003652.D
Acq On : 20 Dec 2015 13:42
Operator : UM/SJ
Sample : G4801-24
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9C72

Quant Time: Dec 21 02:22:52 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 21 02:19:57 2015
Response via : Initial Calibration

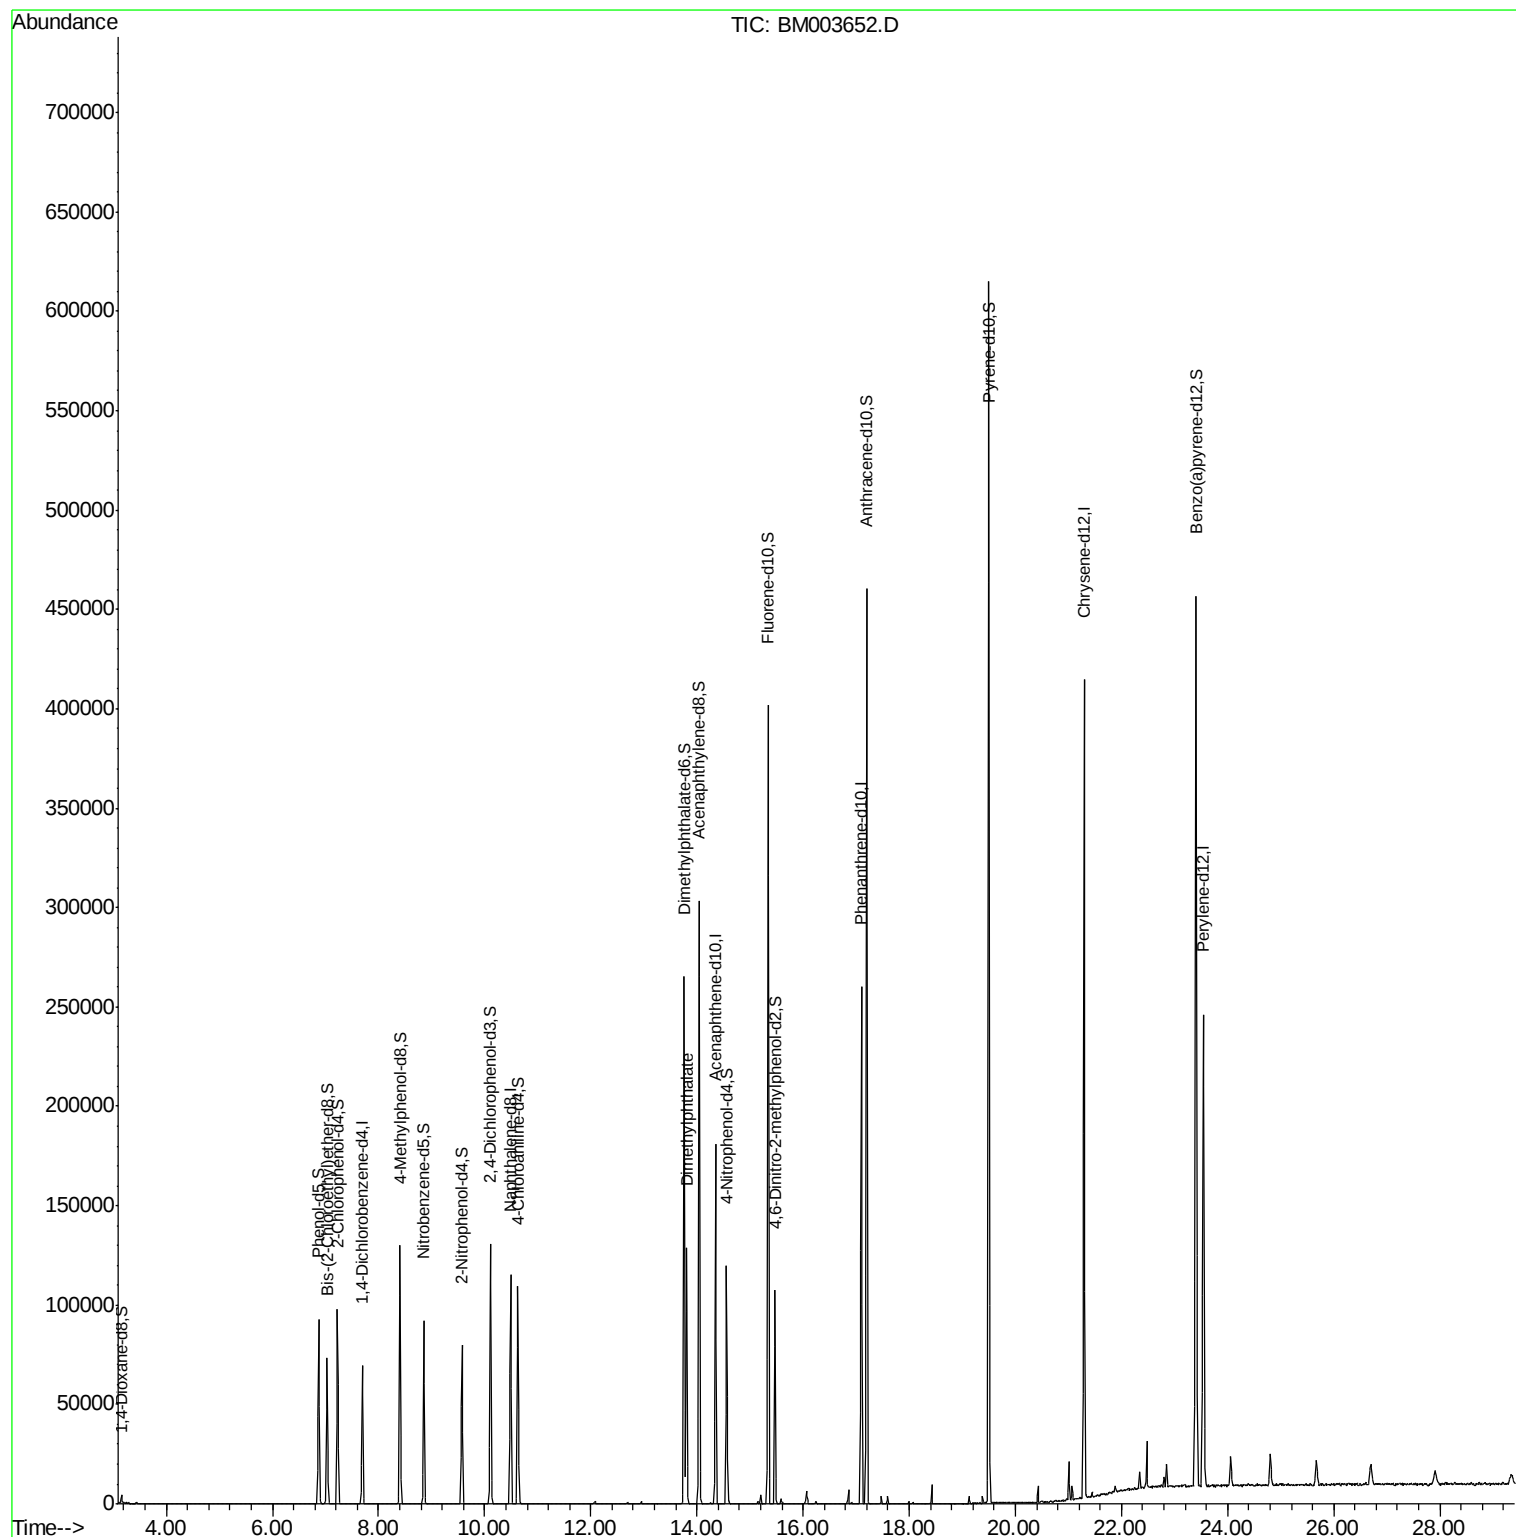

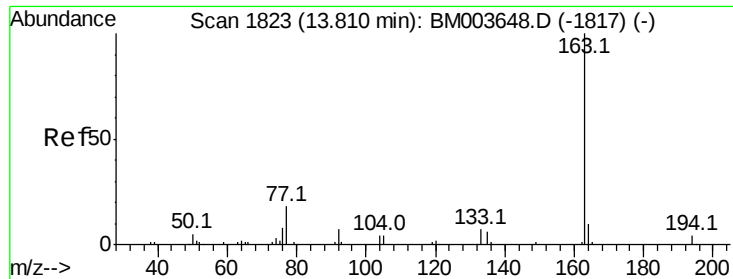

#45

Dimethylphthalate

Concen: 15.71 ng/ul

RT: 13.80 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BM003652.D

Acq: 20 Dec 2015 13:42

Instrument :

BNA_M

ClientSampleId :

G9C72


Tot Ion:163 Resp: 82237

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 10.5 7.8 11.8

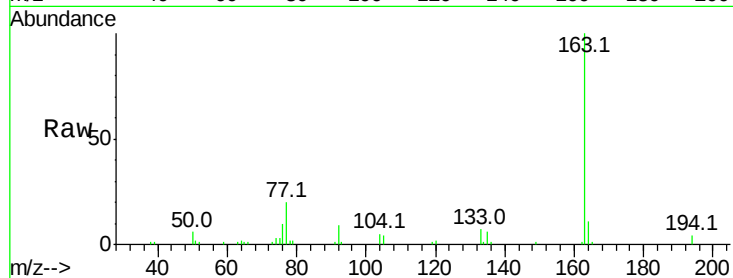

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

