

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122015\
 Data File : BM003658.D
 Acq On : 20 Dec 2015 17:17
 Operator : UM/SJ
 Sample : G4867-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9DA1

Manual Integrations
 APPROVED

apatel
 12/22/2015 12:19:20 PM

Quant Time: Dec 23 12:17:16 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 21 02:19:57 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	23163	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	104724	20.00	ng/ul	0.02
36) Acenaphthene-d10	14.35	164	71321	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	155002	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	221841	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	204196	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	396	0.92	ng/uL	0.00
5) Phenol-d5	6.87	99	14650	7.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	32648	31.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	43413	27.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	30794	18.21	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	32170	42.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	31984	37.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	53785	34.47	ng/ul	0.02
29) 4-Chloroaniline-d4	10.67	131	10527m	5.07	ng/ul	0.05
44) Dimethylphthalate-d6	13.77	166	199208	33.80	ng/ul	0.01
47) Acenaphthylene-d8	14.05	160	227030	33.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	11599m	10.10	ng/ul	0.02
58) Fluorene-d10	15.35	176	170102	34.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	30183	34.55	ng/ul	0.00
71) Anthracene-d10	17.20	188	256398	36.36	ng/ul	0.00
79) Pyrene-d10	19.51	212	325820	33.62	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.41	264	362111	35.70	ng/ul	0.01

Target Compounds

					Ovalue
6) Phenol	6.90	94	9174	4.46	ng/ul 97
11) 2-Methylphenol	8.15	108	16142	9.92	ng/ul 100
14) Acetophenone	8.50	105	15892	6.02	ng/ul# 59
16) 4-Methylphenol	8.47	108	8259	4.55	ng/ul 88
24) 2,4-Dimethylphenol	9.68	107	72490	37.36	ng/ul 99
28) Naphthalene	10.60	128	10965670	2032.37	ng/ul 97
34) 2-Methylnaphthalene	12.19	142	2791730	692.84	ng/ul 100
41) 1,1'-Biophenyl	13.18	154	283330	48.91	ng/ul 100
45) Dimethylphthalate	13.82	163	25998	4.31	ng/ul# 89
48) Acenaphthylene	14.07	152	247224	33.69	ng/ul# 92
50) Acenaphthene	14.43	153	801749	163.60	ng/ul 98
54) Dibenzofuran	14.75	168	87619	12.53	ng/ul 94
59) Fluorene	15.40	166	378552	67.42	ng/ul 99
70) Phenanthrene	17.15	178	684549	79.84	ng/ul 100
72) Anthracene	17.24	178	174586	19.97	ng/ul 98
75) Carbazole	17.52	167	105169	13.18	ng/ul# 90
77) Fluoranthene	19.17	202	107795	10.94	ng/ul 99
80) Pyrene	19.54	202	178921	14.01	ng/ul 98
83) Benzo(a)anthracene	21.29	228	42433m	3.17	ng/ul
85) Chrysene	21.34	228	40971	3.18	ng/ul 95
88) Benzo(b)fluoranthene	22.89	252	23296	1.89	ng/ul# 89

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122015\
Data File : BM003658.D
Acq On : 20 Dec 2015 17:17
Operator : UM/SJ
Sample : G4867-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9DA1

Manual Integrations
APPROVED

apatel
12/22/2015 12:19:20 PM

Quant Time: Dec 23 12:17:16 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 21 02:19:57 2015
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						


Data Path : Z:\HPCHEM1\BNA M\DATA\BM122015\
Data File : BM003658.D
Acq On : 20 Dec 2015 17:17
Operator : UM/SJ
Sample : G4867-04
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
G9DA1

Manual Integrations
APPROVED

apatel
12/22/2015 12:19:20 PM

Quant Time: Dec 23 12:17:16 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 21 02:19:57 2015
Response via : Initial Calibration

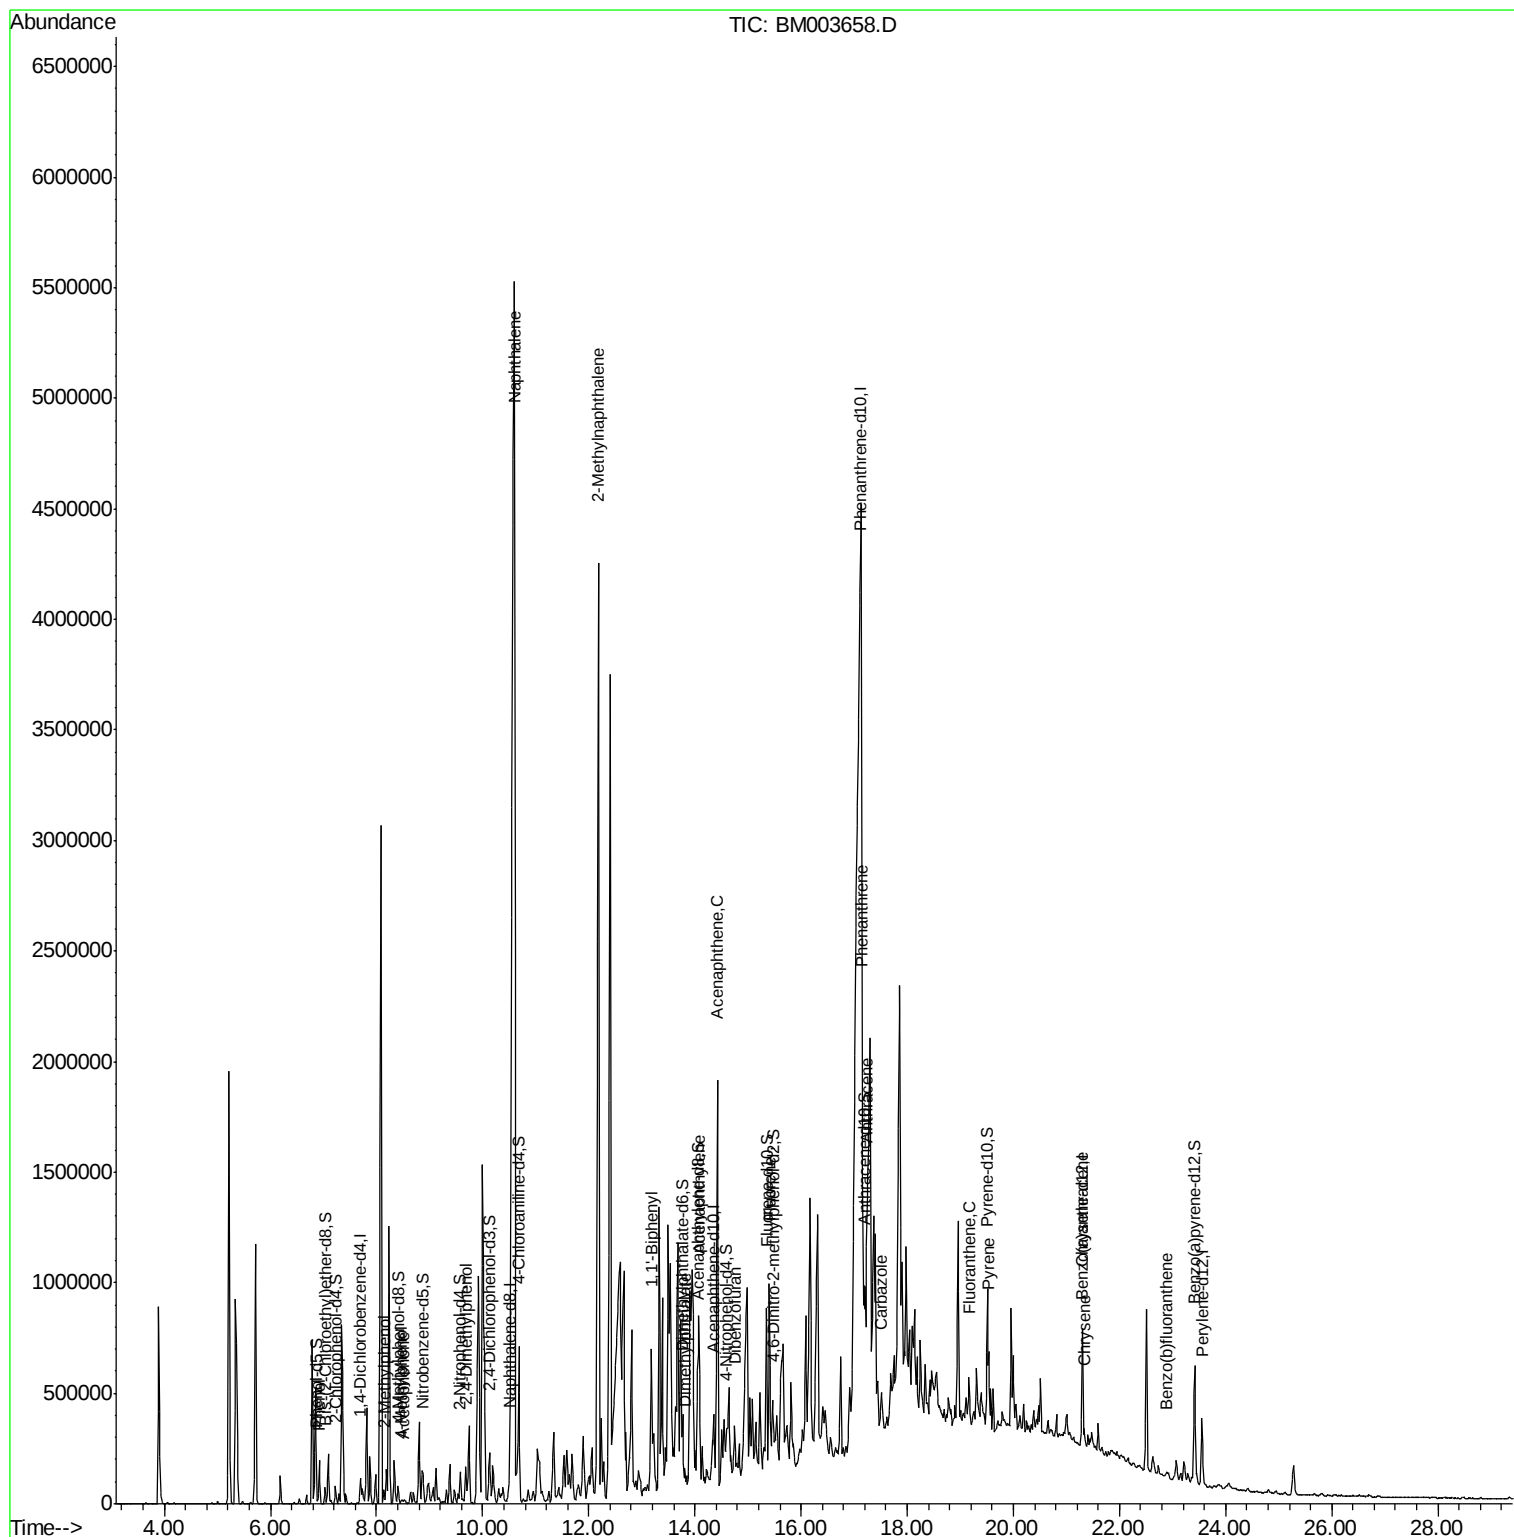

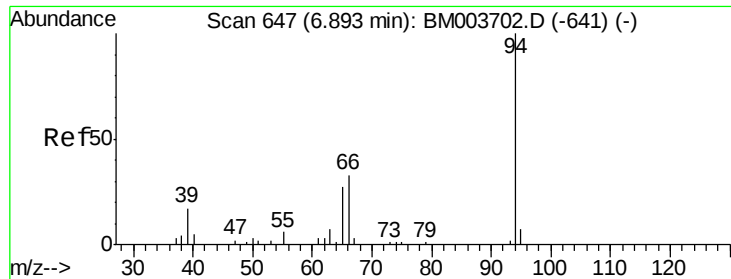

#6

Phenol

Concen: 4.46 ng/ul

RT: 6.90 min Scan# 648

Delta R.T. 0.00 min

Lab File: BM003658.D

Acq: 20 Dec 2015 17:17

Instrument :

BNA_M


ClientSampleId :

G9DA1

Tot Ion:	94	Resp:	9174
Ion	Ratio	Lower	Upper
94	100		
65	29.4	21.0	31.6
66	36.3	29.3	43.9

Manual Integrations
APPROVED


apatel
12/22/2015 12:19:20 PM





Abundance Ion 94.00 (93.70 to 94.70): BM003702.D (-641) (-)

Ion 65.00 (64.70 to 65.70): BM003702.D (-641) (-)

Ion 66.00 (65.70 to 66.70): BM003702.D (-641) (-)

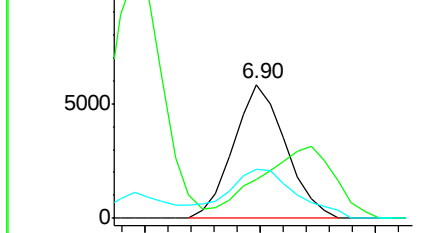

Time-->



#11

2-Methylphenol

Concen: 9.92 ng/ul


RT: 8.15 min Scan# 860

Delta R.T. 0.00 min

Lab File: BM003658.D


Acq: 20 Dec 2015 17:17

Tgt Ion:	108	Resp:	16142
Ion	Ratio	Lower	Upper
108	100		
107	90.6	72.4	108.6







Abundance Ion 108.00 (107.70 to 108.70): BM003702.D (-853) (-)

Ion 107.00 (106.70 to 107.70): BM003702.D (-853) (-)

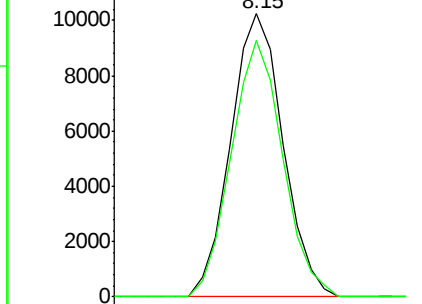

Time-->



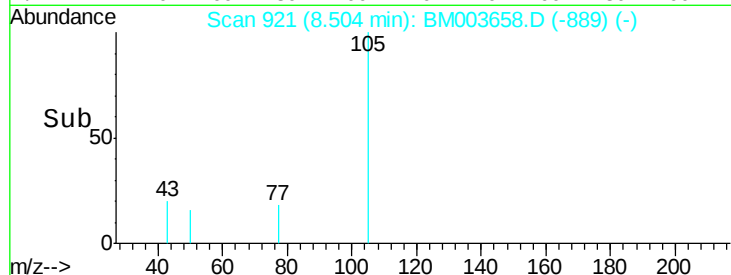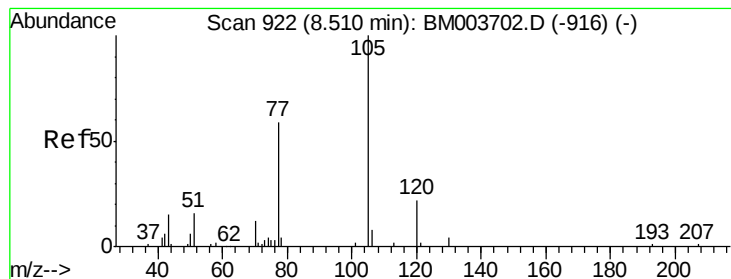

#14

Acetophenone

Concen: 6.02 ng/ul

RT: 8.50 min Scan# 921

Delta R.T. -0.01 min

Lab File: BM003658.D

Acq: 20 Dec 2015 17:17

Tot Ion:	105	Resp:	15892
Ion Ratio	Lower	Upper	
105	100		
77	34.2	59.0	88.4#
51	11.2	16.4	24.6#

Instrument :





BNA_M

ClientSampleId :

G9DA1

Manual Integrations
APPROVED

apatel
12/22/2015 12:19:20 PM

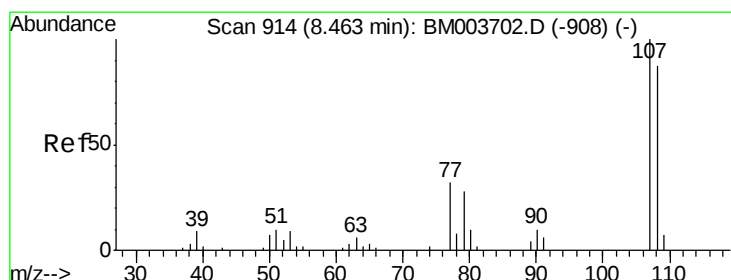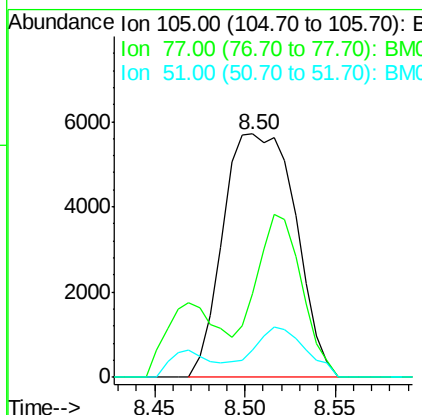

#16

4-Methylphenol

Concen: 4.55 ng/ul


RT: 8.47 min Scan# 915


Delta R.T. 0.00 min

Lab File: BM003658.D

Acq: 20 Dec 2015 17:17

Tgt Ion:	108	Resp:	8259
Ion Ratio	Lower	Upper	
108	100		
107	125.6	90.3	135.5

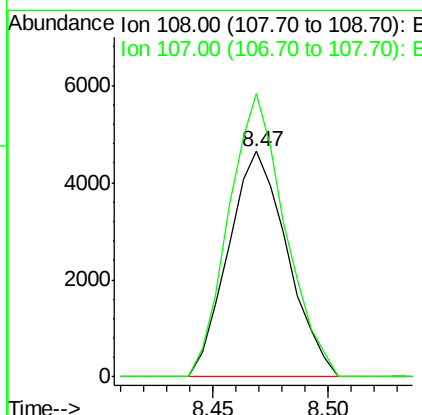



#24

2,4-Dimethylphenol

Concen: 37.36 ng/ul

RT: 9.68 min Scan# 1121

Delta R.T. 0.01 min

Lab File: BM003658.D

Acq: 20 Dec 2015 17:17

Instrument :

BNA_M





ClientSampleId :

G9DA1

Tot Ion:	107	Resp:	72490
Ion Ratio	Lower	Upper	
107	100		
121	50.6	40.6	61.0
122	83.4	67.8	101.6

Manual Integrations
APPROVED

apatel
12/22/2015 12:19:20 PM

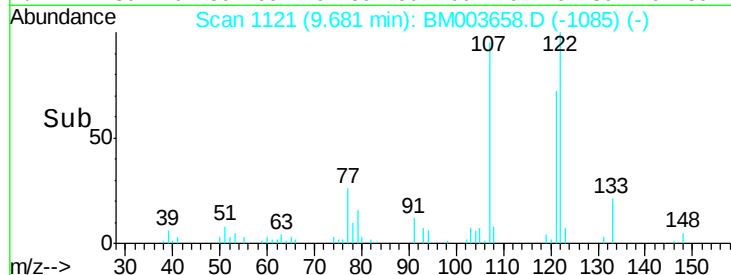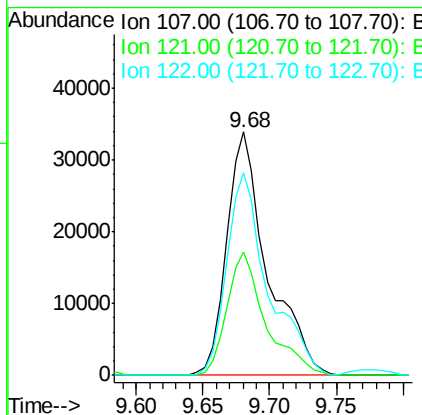

#28

Naphthalene

Concen: 2032.37 ng/ul




RT: 10.60 min Scan# 1278


Delta R.T. 0.06 min

Lab File: BM003658.D

Acq: 20 Dec 2015 17:17

Tgt Ion:	128	Resp:	10965670
Ion Ratio	Lower	Upper	
128	100		
129	11.5	8.8	13.2
127	14.8	10.5	15.7

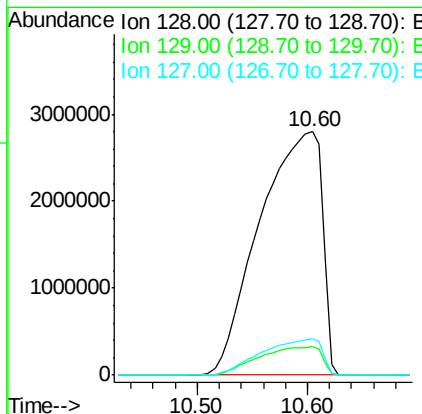

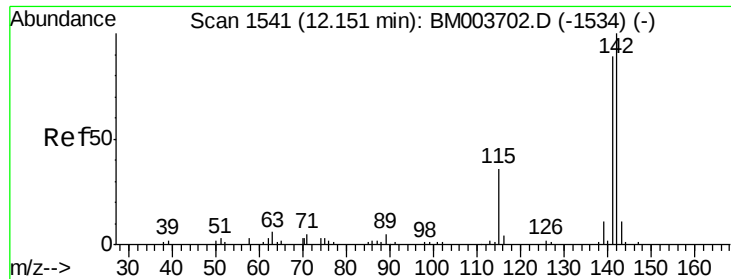





#34
2-Methylnaphthalene
Concen: 692.84 ng/ul
RT: 12.19 min Scan# 1547
Delta R.T. 0.03 min
Lab File: BM003658.D
Acq: 20 Dec 2015 17:17

Instrument :
BNA_M
ClientSampleID :
G9DA1

Tot Ion:142 Resp: 2791730
Ion Ratio Lower Upper
142 100
141 89.7 71.6 107.4




Manual Integrations
APPROVED


apatel
12/22/2015 12:19:20 PM

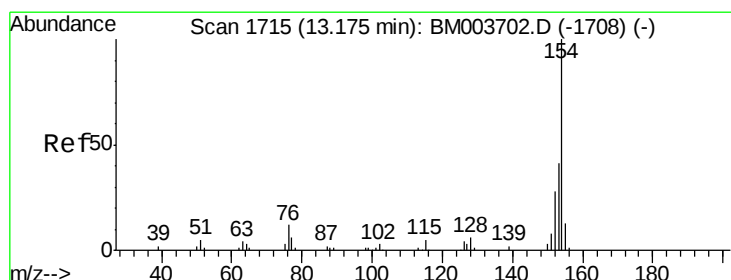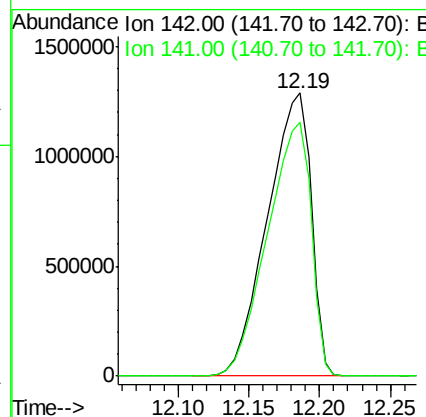

#41
1,1'-Biphenyl
Concen: 48.91 ng/ul
RT: 13.18 min Scan# 1716
Delta R.T. 0.00 min
Lab File: BM003658.D
Acq: 20 Dec 2015 17:17

Tgt Ion:154 Resp: 283330
Ion Ratio Lower Upper
154 100
153 40.3 32.1 48.1
76 11.6 9.5 14.3

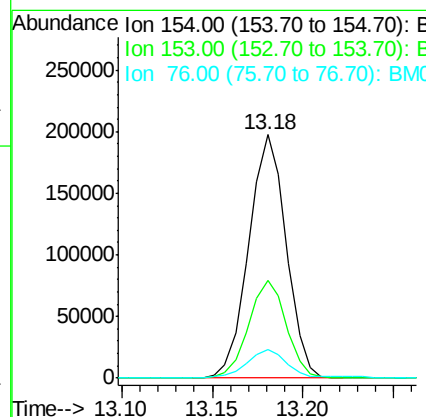

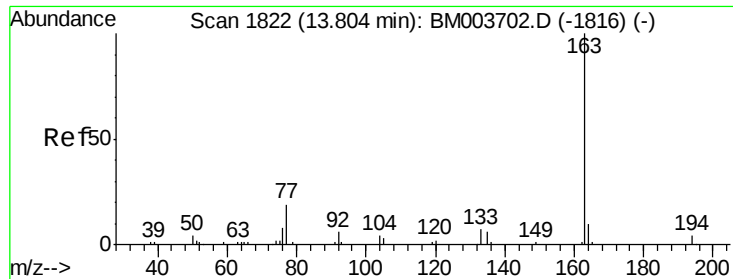





#45
Dimethylphthalate
Concen: 4.31 ng/ul
RT: 13.82 min Scan# 1824
Delta R.T. 0.01 min
Lab File: BM003658.D
Acq: 20 Dec 2015 17:17

Instrument :
BNA_M
ClientSampleId :
G9DA1

Tot Ion	Ratio	Resp	Lower	Upper
163	100	25998		
194	3.7		3.2	4.8
164	15.6		7.8	11.8#




Manual Integrations
APPROVED


apatel
12/22/2015 12:19:20 PM

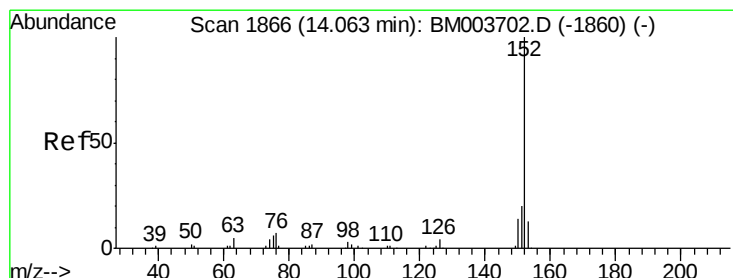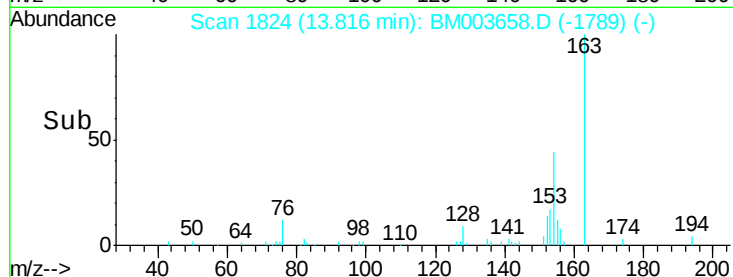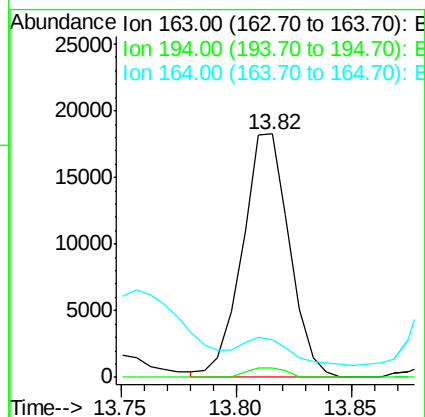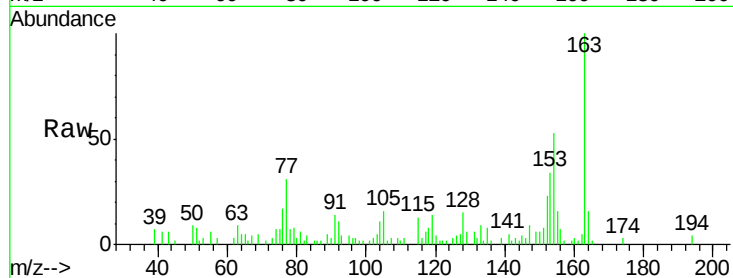

#48
Acenaphthylene
Concen: 33.69 ng/ul
RT: 14.07 min Scan# 1868
Delta R.T. 0.01 min
Lab File: BM003658.D
Acq: 20 Dec 2015 17:17

Tgt Ion	Ratio	Resp	Lower	Upper
152	100	247224		
151	20.9		15.7	23.5
153	19.8		10.5	15.7#

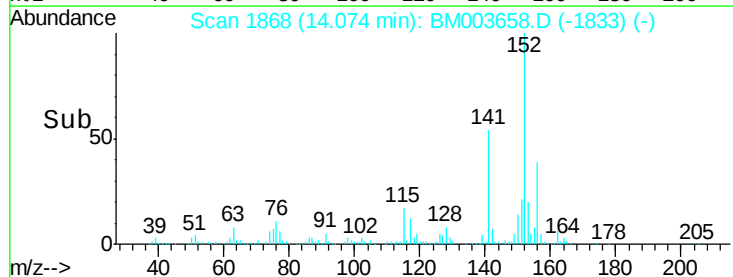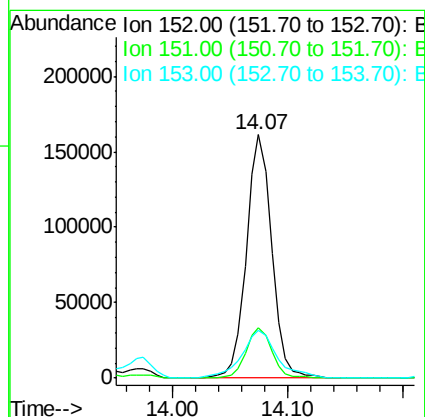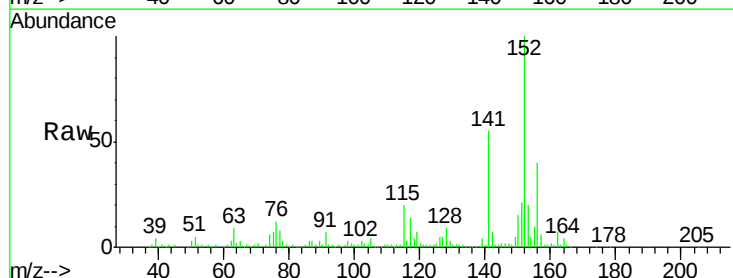

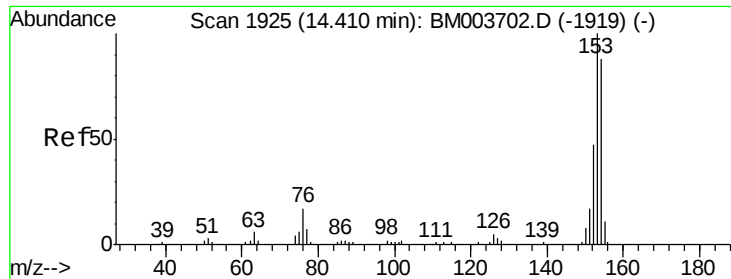


#50
Acenaphthene
Concen: 163.60 ng/ul
RT: 14.43 min Scan# 1928
Delta R.T. 0.01 min
Lab File: BM003658.D
Acq: 20 Dec 2015 17:17

Instrument :
BNA_M
ClientSampleId :
G9DA1




Tot Ion	Ratio	Lower	Upper
153	100		
152	48.0	38.3	57.5
154	87.2	71.8	107.8

Manual Integrations
APPROVED

apatel
12/22/2015 12:19:20 PM




Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

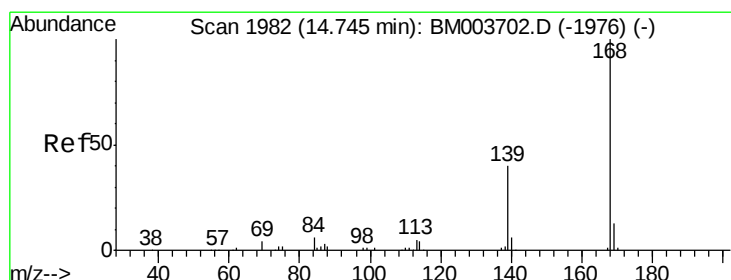
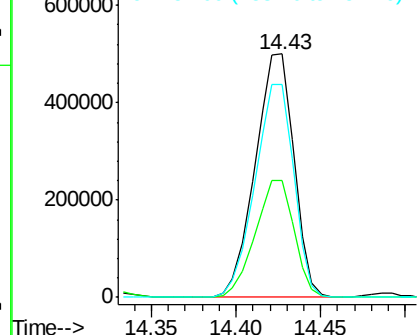



#54
Dibenzofuran
Concen: 12.53 ng/ul
RT: 14.75 min Scan# 1983
Delta R.T. 0.00 min
Lab File: BM003658.D
Acq: 20 Dec 2015 17:17

Tgt Ion	Ratio	Lower	Upper
168	100		
139	43.9	32.2	48.2



Abundance Ion 168.00 (167.70 to 168.70): E
Ion 139.00 (138.70 to 139.70): E

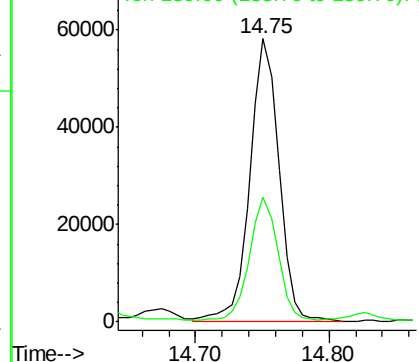

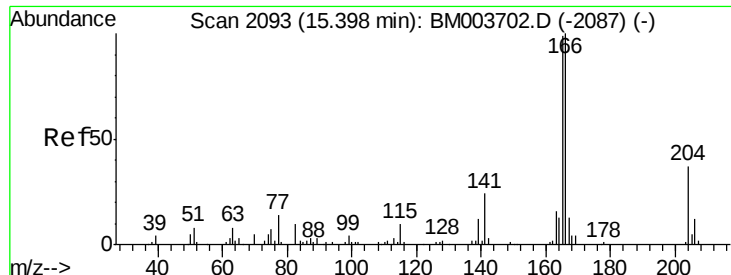





#59
Fluorene
Concen: 67.42 ng/ul
RT: 15.40 min Scan# 2094
Delta R.T. 0.00 min
Lab File: BM003658.D
Acq: 20 Dec 2015 17:17

Instrument :
BNA_M
ClientSampleId :
G9DA1

Tot Ion	Ratio	Resp	Lower	Upper
166	100	378552		
165	98.7	78.5	117.7	
167	13.7	10.7	16.1	




Manual Integrations
APPROVED


apatel
12/22/2015 12:19:20 PM

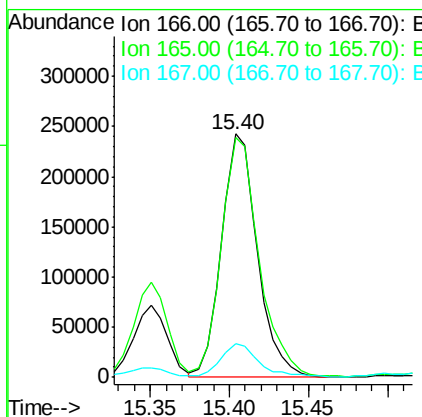

#70
Phenanthrene
Concen: 79.84 ng/ul
RT: 17.15 min Scan# 2391
Delta R.T. 0.01 min
Lab File: BM003658.D
Acq: 20 Dec 2015 17:17

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	684549		
179	15.0	12.2	18.4	
176	19.6	15.6	23.4	

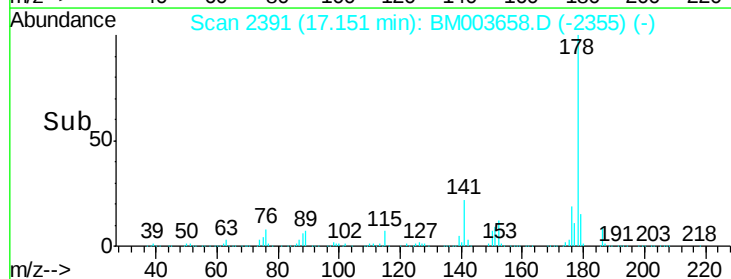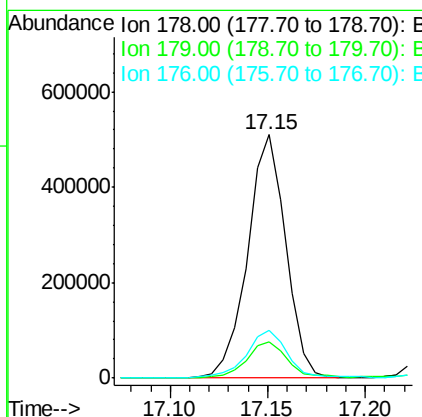



#72

Anthracene

Concen: 19.97 ng/ul

RT: 17.24 min Scan# 2406

Delta R.T. 0.01 min

Lab File: BM003658.D

Acq: 20 Dec 2015 17:17

Instrument :

BNA_M

ClientSampleId :

G9DA1

Tot Ion:178 Resp: 174586

Ion Ratio Lower Upper


178 100

179 15.7 12.1 18.1

176 19.3 14.8 22.2

Manual Integrations
APPROVED




apatel
12/22/2015 12:19:20 PM



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

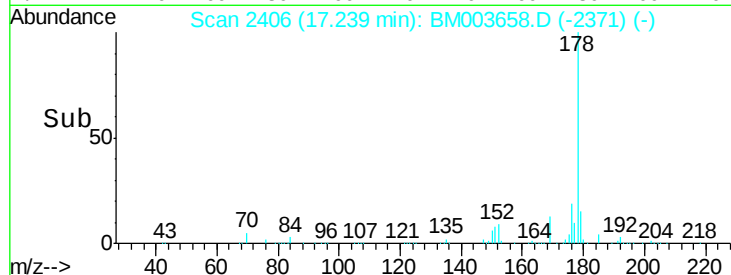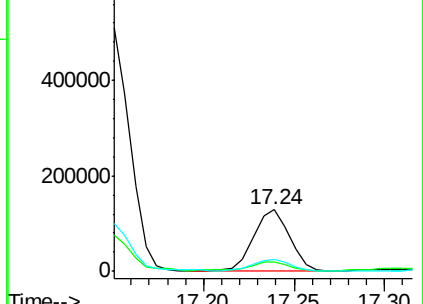

#75

Carbazole

Concen: 13.18 ng/ul

RT: 17.52 min Scan# 2453

Delta R.T. 0.01 min

Lab File: BM003658.D

Acq: 20 Dec 2015 17:17


Tgt Ion:167 Resp: 105169

Ion Ratio Lower Upper

167 100

166 22.4 17.0 25.6



139 22.4 11.0 16.4#




Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

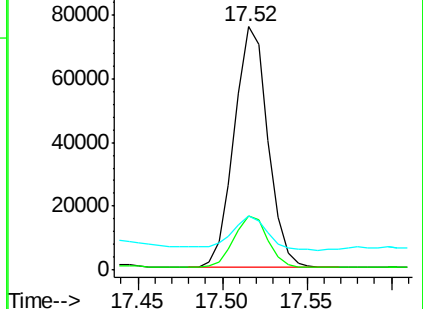

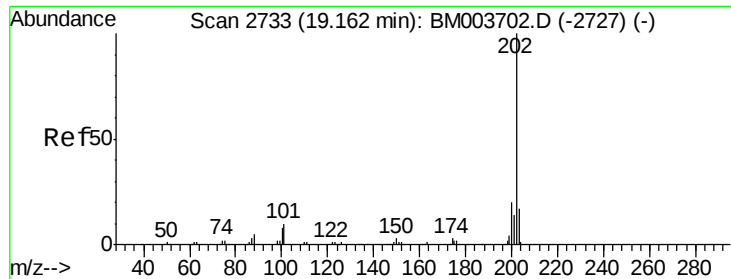

#77

Fluoranthene

Concen: 10.94 ng/ul

RT: 19.17 min Scan# 2734

Delta R.T. 0.01 min

Lab File: BM003658.D

Acq: 20 Dec 2015 17:17

Instrument :

BNA_M





ClientSampleId :

G9DA1

Tot Ion:	202	Resp:	107795
Ion Ratio	Lower	Upper	
202	100		
101	11.7	8.8	13.2
100	8.2	6.6	9.8

Manual Integrations
APPROVED

apatel
12/22/2015 12:19:20 PM

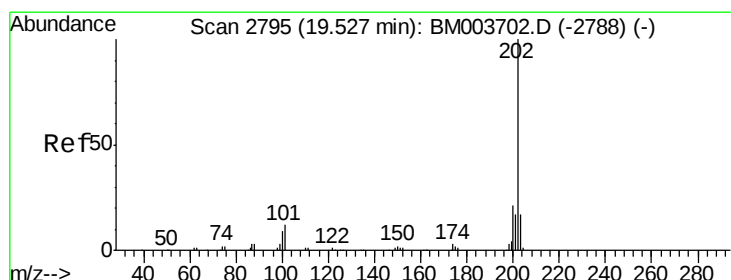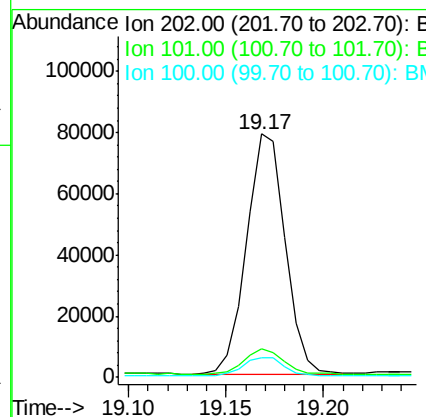

#80

Pyrene

Concen: 14.01 ng/ul




RT: 19.54 min Scan# 2797


Delta R.T. 0.01 min

Lab File: BM003658.D

Acq: 20 Dec 2015 17:17

Tgt Ion:	202	Resp:	178921
Ion Ratio	Lower	Upper	
202	100		
101	12.0	10.2	15.2
100	9.9	8.5	12.7

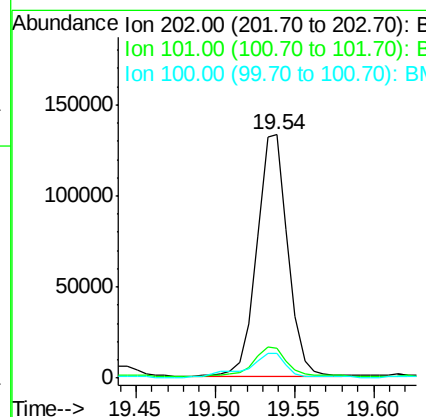

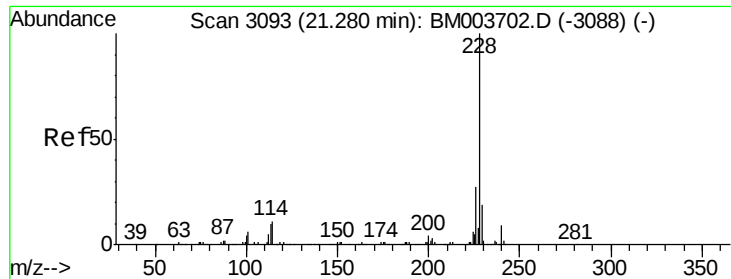





#83
Benzo(a)anthracene
Concen: 3.17 ng/ul m
RT: 21.29 min Scan# 3095
Delta R.T. 0.01 min
Lab File: BM003658.D
Acq: 20 Dec 2015 17:17

Instrument :
BNA_M
ClientSampleId :
G9DA1

Tot Ion	Ratio	Lower	Upper
228	100		
229	23.4	15.7	23.5
226	33.5	21.8	32.6




Manual Integrations
APPROVED


apatel
12/22/2015 12:19:20 PM

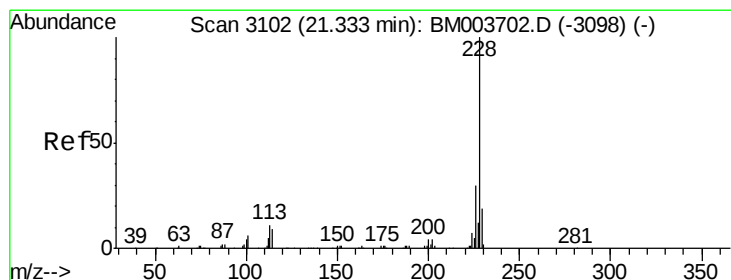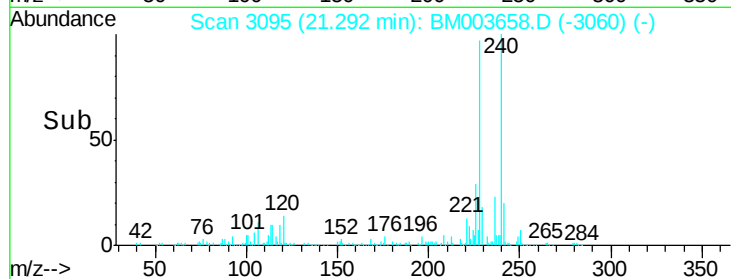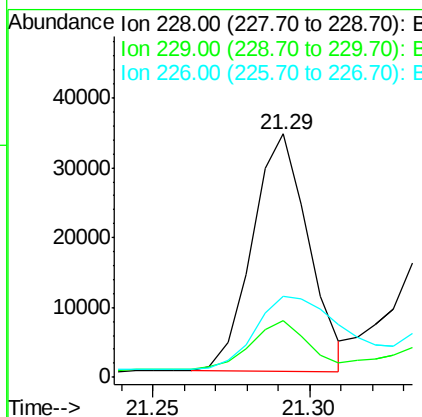

#85
Chrysene
Concen: 3.18 ng/ul
RT: 21.34 min Scan# 3104
Delta R.T. 0.01 min
Lab File: BM003658.D
Acq: 20 Dec 2015 17:17

Tgt Ion	Ratio	Lower	Upper
228	100		
226	32.6	24.0	36.0
229	22.4	15.6	23.4

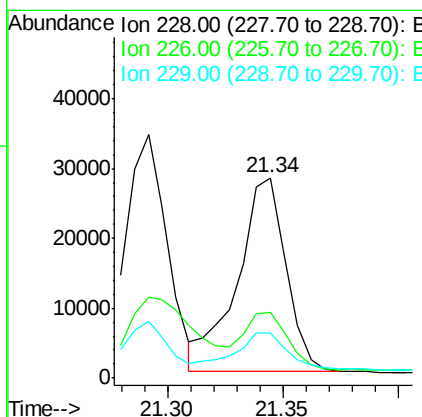

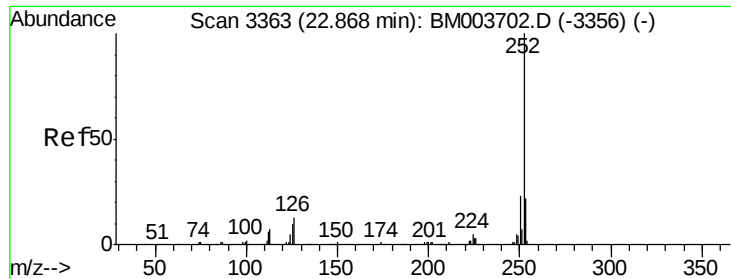

#88
 Benzo(b)fluoranthene
 Concen: 1.89 ng/ul
 RT: 22.89 min Scan# 3366
 Delta R.T. 0.02 min
 Lab File: BM003658.D
 Acq: 20 Dec 2015 17:17

Instrument :
 BNA_M
 ClientSampleId :
 G9DA1

Tot Ion	Ratio	Lower	Upper
252	100		
253	26.5	17.5	26.3#
125	15.9	8.5	12.7#

Manual Integrations
 APPROVED

apatel
 12/22/2015 12:19:20 PM

