

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122015\
 Data File : BM003650.D
 Acq On : 20 Dec 2015 12:30
 Operator : UM/SJ
 Sample : PB87401BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	18	rVB	6063	7457	0.64%	0.077%
2	6.869	637	643	652	rBB	138682	208606	17.97%	2.148%
3	7.034	665	671	679	rBB	110674	167390	14.42%	1.723%
4	7.228	698	704	712	rBB	145373	224646	19.35%	2.313%
5	7.698	778	784	790	rBB	89912	138467	11.93%	1.426%
6	8.404	898	904	912	rBB	192367	293735	25.30%	3.024%
7	8.851	974	980	988	rBB	138071	224172	19.31%	2.308%
8	9.575	1097	1103	1109	rBB	121968	193132	16.64%	1.988%
9	10.110	1188	1194	1202	rBB	192321	303051	26.10%	3.120%
10	10.486	1251	1258	1265	rBB	142367	229153	19.74%	2.359%
11	10.628	1275	1282	1294	rBB	200518	327036	28.17%	3.367%
12	12.080	1526	1529	1533	rBB	2096	2808	0.24%	0.029%
13	13.757	1808	1814	1822	rBB	381908	539072	46.43%	5.550%
14	14.039	1856	1862	1869	rBV	427249	624361	53.78%	6.428%
15	14.351	1909	1915	1921	rBB2	227839	333572	28.73%	3.434%
16	14.557	1945	1950	1963	rBB	186875	261170	22.50%	2.689%
17	15.345	2078	2084	2090	rBB	577285	803194	69.18%	8.269%
18	15.468	2101	2105	2112	rBB	163421	210791	18.16%	2.170%
19	15.586	2121	2125	2128	rBB	3844	4302	0.37%	0.044%
20	17.098	2376	2382	2388	rBB	309800	428795	36.93%	4.415%
21	17.198	2392	2399	2405	rBV	685106	953426	82.12%	9.816%
22	19.133	2724	2728	2733	rVB	5606	6624	0.57%	0.068%
23	19.386	2766	2771	2775	rBV	5050	5701	0.49%	0.059%
24	19.498	2784	2790	2801	rBV	831270	1160959	100.00%	11.953%
25	21.074	3056	3058	3062	rBV3	2053	2460	0.21%	0.025%
26	21.297	3090	3096	3101	rBV	452758	545901	47.02%	5.620%
27	22.339	3271	3273	3276	rBV4	2368	2269	0.20%	0.023%
28	22.803	3348	3352	3356	rBV2	6446	10413	0.90%	0.107%
29	22.850	3356	3360	3363	rVV2	2890	4084	0.35%	0.042%
30	23.403	3445	3454	3465	rBV	567830	1033483	89.02%	10.640%
31	23.544	3470	3478	3490	rVB2	232261	443136	38.17%	4.562%
32	24.062	3561	3566	3572	rVB4	4520	7807	0.67%	0.080%
33	24.227	3592	3594	3596	rBV2	1576	1197	0.10%	0.012%
34	24.797	3687	3691	3698	rBV3	4725	10679	0.92%	0.110%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122015\
Data File : BM003650.D
Acq On : 20 Dec 2015 12:30
Operator : UM/SJ
Sample : PB87401BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK01

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Title : SVOA CALIBRATION


Sum of corrected areas: 9713049

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122015\
Data File : BM003650.D
Acq On : 20 Dec 2015 12:30
Operator : UM/SJ
Sample : PB87401BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK01

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

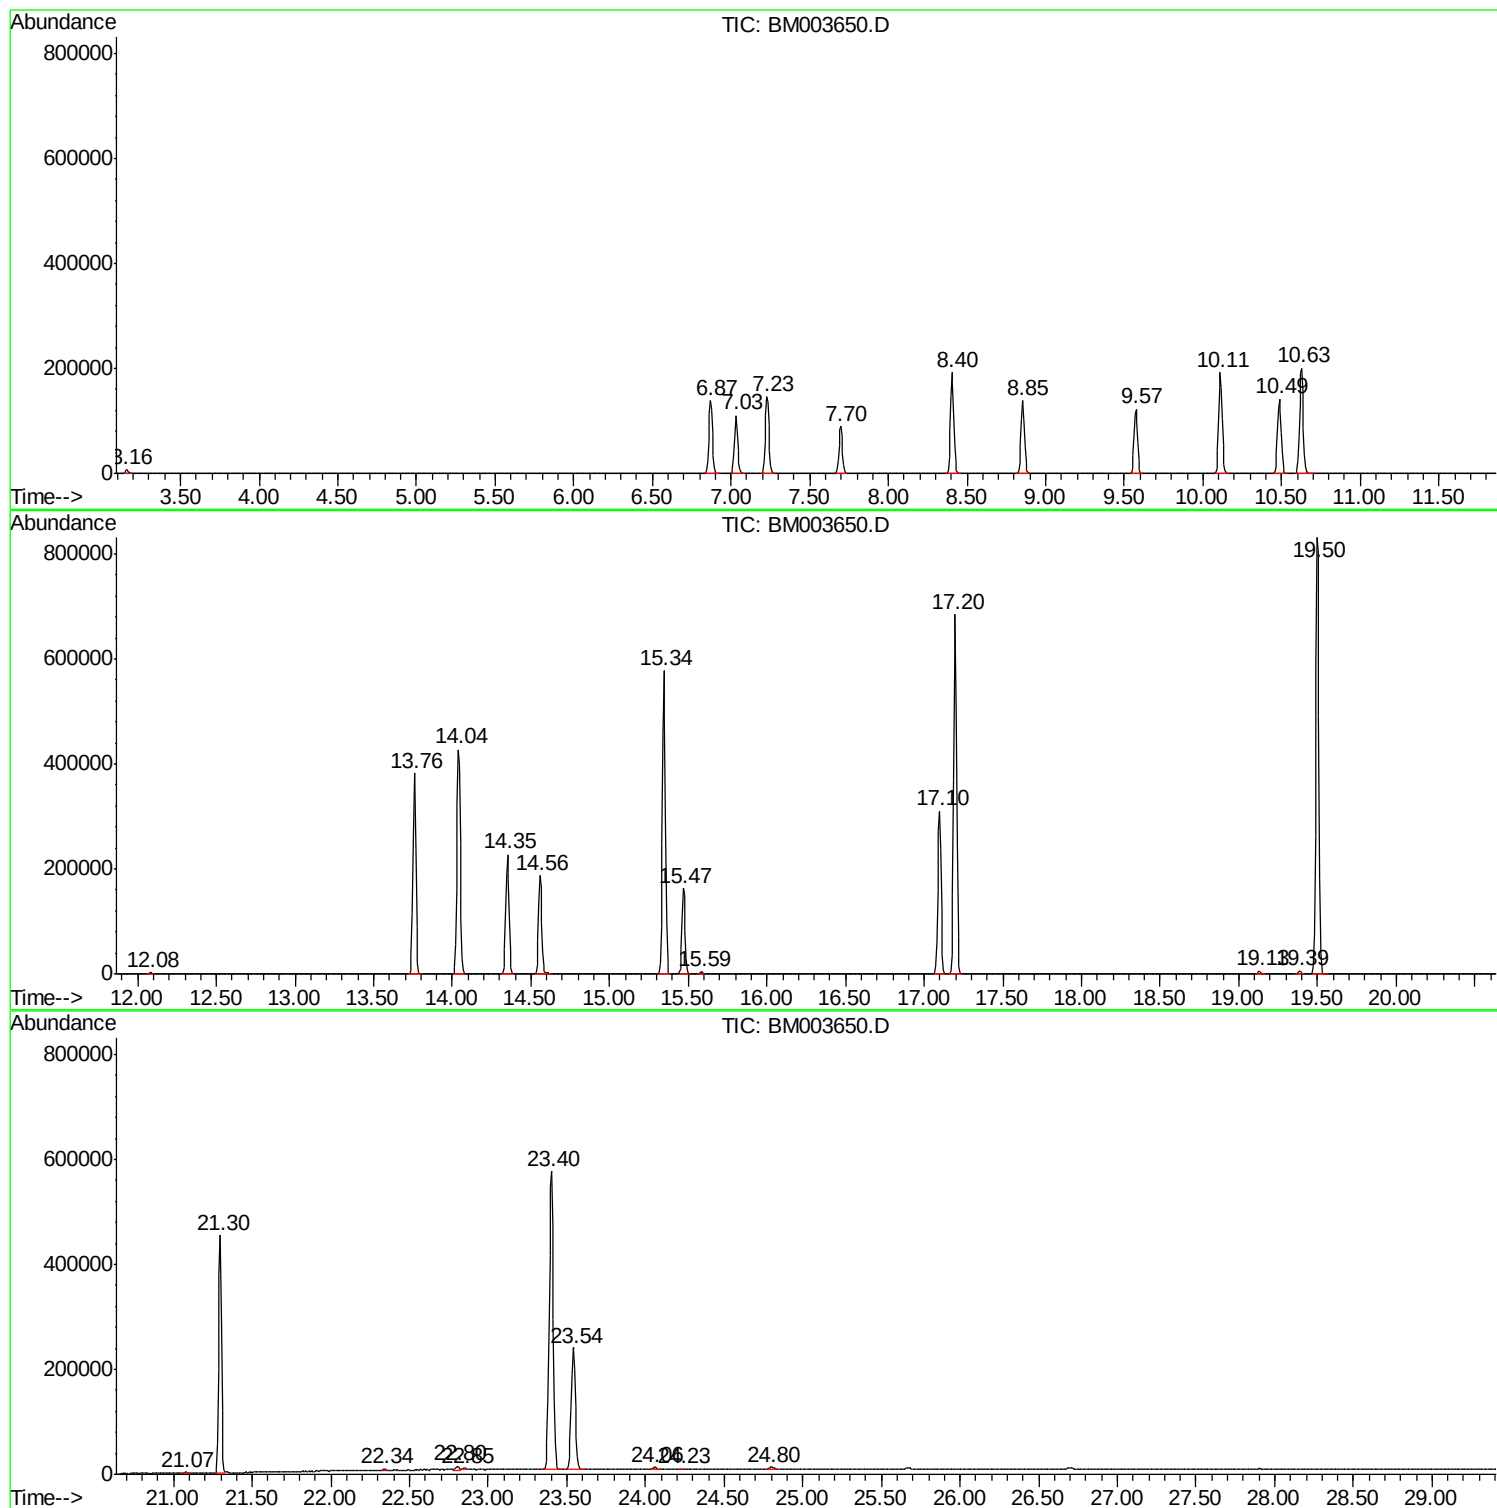

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122015\
Data File : BM003650.D
Acq On : 20 Dec 2015 12:30
Operator : UM/SJ
Sample : PB87401BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK01

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122015\
Data File : BM003650.D
Acq On : 20 Dec 2015 12:30
Operator : UM/SJ
Sample : PB87401BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK01

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc