


Data Path : Z:\HPCHEM1\BNA M\Data\BM122015\
 Data File : BM003647.D
 Acq On : 20 Dec 2015 09:20
 Operator : UM/SJ
 Sample : DFTPP61
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP61

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
 Title : SVOA CALIBRATION
 Last Update : Mon Dec 21 16:14:53 2015

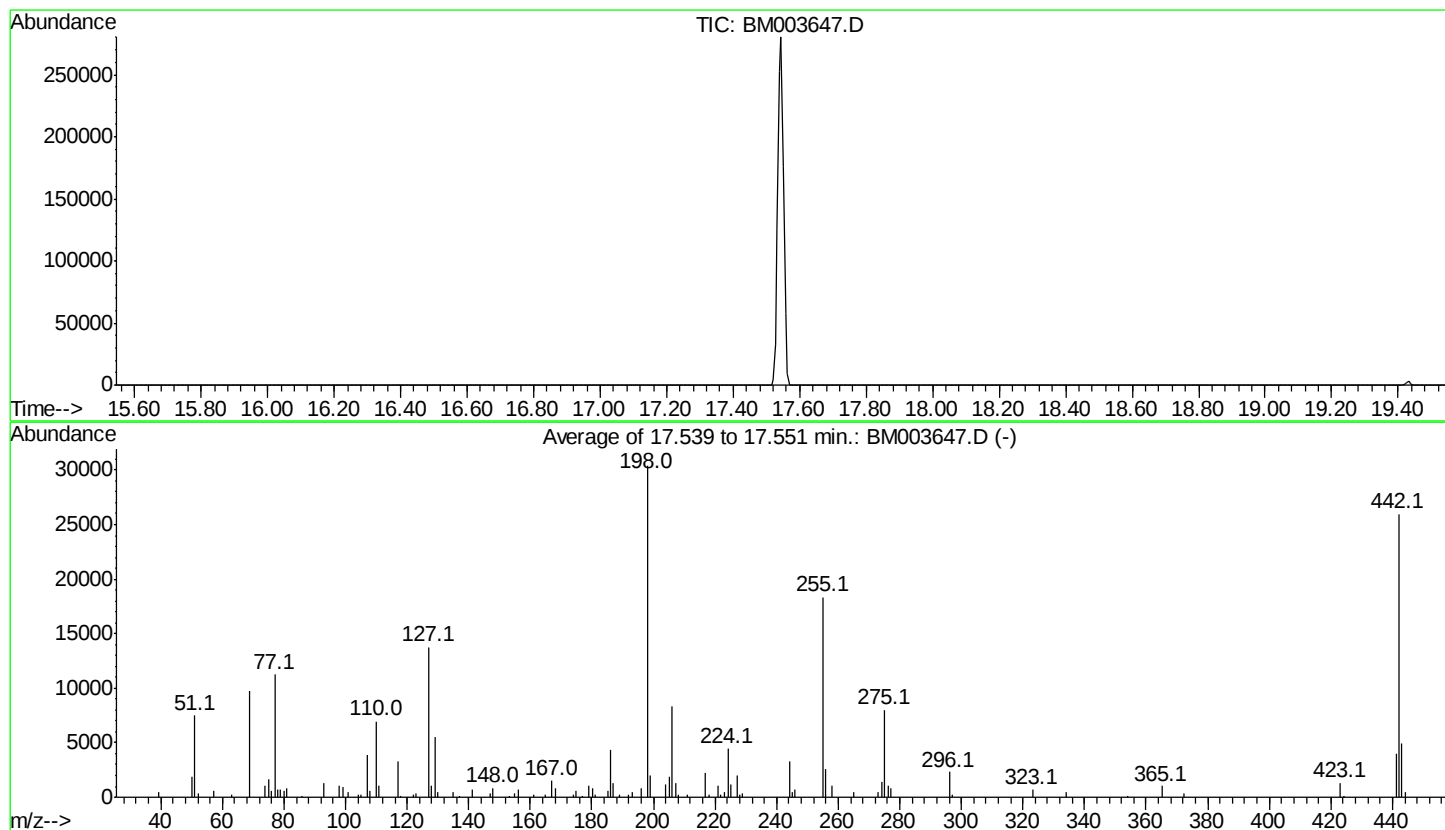

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	7491	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	9749	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.2	13749	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30400	PASS
199	198	5	9	6.6	2013	PASS
275	198	10	60	26.4	8039	PASS
365	198	1	100	3.4	1024	PASS
441	443	0.01	100	80.2	3963	PASS
442	198	50	100	85.5	25989	PASS
443	442	15	24	19.0	4943	PASS

m/z	Abundance
39.10	607.0
50.10	2280.0
51.10	9114.0
52.00	501.0
57.00	681.0
63.00	418.0
69.00	11680.0
74.00	1204.0
75.00	1905.0
76.10	645.0
77.10	13172.0
78.10	883.0
79.00	875.0
80.00	625.0
81.00	1036.0
86.00	334.0
93.00	1439.0
98.00	1275.0
99.00	1115.0
101.00	560.0
103.90	319.0
105.00	350.0
107.00	4519.0
108.00	762.0
110.00	8038.0
111.00	1180.0
117.00	3789.0
118.00	312.0
122.00	368.0
123.00	447.0
127.00	15832.0
128.00	1344.0
129.00	6329.0
130.00	629.0
135.00	540.0
136.90	306.0
141.00	833.0
147.00	475.0
148.00	916.0
153.00	331.0
155.00	492.0
156.10	726.0
161.10	420.0
165.00	391.0
167.00	1662.0
168.00	945.0
174.00	357.0
175.00	635.0
177.00	308.0
179.00	1171.0
180.00	877.0
181.00	394.0
185.00	604.0
186.00	4766.0
187.00	1431.0
189.00	320.0
191.90	397.0
193.00	460.0
196.00	858.0
198.00	32240.0
199.00	2336.0
204.00	1211.0
205.10	2055.0
206.10	8816.0
207.00	1234.0
208.00	354.0
210.90	357.0
217.00	2326.0
217.90	333.0
221.10	1118.0
221.90	300.0
223.00	505.0
224.10	4818.0
225.00	1142.0
227.00	2058.0
229.00	396.0
244.10	3326.0
245.10	471.0
246.00	722.0
255.10	18728.0
256.00	2700.0
258.00	1053.0
265.10	487.0
273.00	517.0
274.00	1495.0
275.10	8009.0
276.00	1077.0
277.00	778.0
296.00	2207.0
297.10	350.0
323.10	628.0
334.10	518.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

365.00	993.0
372.10	314.0
423.10	1218.0
441.10	3423.0
442.10	22248.0
443.10	4210.0
444.00	407.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

m/z	Abundance
39.10	597.0
50.00	2223.0
51.10	8599.0
52.00	427.0
57.00	690.0
63.00	404.0
69.00	11327.0
74.00	1186.0
75.00	1883.0
76.00	600.0
77.10	13057.0
78.10	857.0
79.00	827.0
80.00	685.0
81.00	1061.0
93.00	1648.0
98.00	1281.0
99.00	1060.0
101.00	598.0
104.00	353.0
105.00	309.0
107.00	4678.0
108.00	681.0
110.00	8167.0
111.00	1266.0
117.00	3783.0
121.90	332.0
123.00	485.0
127.10	15993.0
128.00	1213.0
129.00	6569.0
130.00	563.0
135.00	557.0
141.00	907.0
147.00	456.0
148.00	1112.0
155.00	452.0
156.00	826.0
161.10	403.0
165.00	346.0
167.00	1784.0
168.00	993.0
174.00	410.0
175.00	737.0
179.00	1306.0
180.10	943.0
181.00	431.0
185.10	685.0
186.10	5153.0
187.00	1427.0
189.00	343.0
192.00	447.0
193.00	485.0
196.00	985.0
198.00	36728.0
199.00	2280.0
204.10	1338.0
205.00	2291.0
206.10	10052.0
207.10	1521.0
208.00	364.0
211.00	382.0
217.00	2731.0
218.00	337.0
221.10	1371.0
221.90	419.0
223.00	574.0
224.10	5139.0
225.10	1436.0
227.00	2397.0
228.00	338.0
229.00	475.0
244.10	4056.0
245.00	549.0
246.00	943.0
255.10	21696.0
256.10	3042.0
258.00	1278.0
265.00	555.0
273.10	607.0
274.10	1694.0
275.10	9349.0
276.10	1158.0
277.00	900.0
296.00	2730.0
297.00	365.0
323.10	798.0
334.10	552.0
354.10	312.0
365.10	1225.0
372.10	424.0
423.10	1546.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

424.10	409.0
441.10	4611.0
442.10	30360.0
443.10	5885.0
444.10	545.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

m/z	Abundance
39.00	391.0
50.00	1151.0
51.10	4762.0
57.00	335.0
69.00	6242.0
74.10	683.0
75.00	1028.0
76.10	423.0
77.10	7474.0
78.10	476.0
79.00	511.0
80.00	358.0
81.00	519.0
93.00	923.0
98.00	735.0
99.00	577.0
101.00	390.0
107.00	2545.0
108.00	399.0
110.00	4649.0
111.00	730.0
117.00	2171.0
127.00	9422.0
128.00	737.0
129.00	3759.0
130.00	326.0
135.00	309.0
141.00	469.0
148.00	583.0
156.10	469.0
167.00	1071.0
168.00	528.0
175.00	458.0
179.00	873.0
180.00	565.0
185.00	396.0
186.10	3209.0
187.00	918.0
193.00	345.0
196.10	599.0
198.00	22232.0
199.00	1425.0
204.00	857.0
205.00	1413.0
206.10	6176.0
207.10	954.0
217.00	1620.0
221.00	853.0
223.00	379.0
224.10	3289.0
225.00	867.0
227.00	1560.0
228.00	306.0
229.00	356.0
244.10	2609.0
245.10	351.0
246.00	622.0
255.10	14581.0
256.10	1993.0
258.00	912.0
265.00	369.0
273.00	356.0
274.00	1102.0
275.10	6760.0
276.10	867.0
277.00	689.0
296.10	1969.0
323.10	621.0
334.10	380.0
365.00	854.0
372.10	333.0
423.10	1251.0
441.10	3856.0
442.10	25360.0
443.10	4734.0
444.10	413.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61