

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
 Data File : BM008497.D
 Acq On : 21 Dec 2016 01:53
 Operator : UM/SJ
 Sample : H6106-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7G8

Quant Time: Dec 21 02:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 02:43:00 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	417	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.43	136	1401	0.40	ng/ul	-0.05
6) Acenaphthene-d10	14.30	164	872	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.14	188	153333	0.40	ng/ul	0.07
16) Chrysene-d12	21.27	240	1318	0.40	ng/ul	0.00
20) Perylene-d12	23.48	264	1716	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	793	0.37	ng/ul	-0.03
14) Fluoranthene-d10	19.10	212	1544	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.29	166	322	0.10	ng/ul#	31
17) Pyrene	19.45	202	288	0.06	ng/ul#	1
23) Benzo(a)pyrene	23.33	252	610	0.10	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
Data File : BM008497.D
Acq On : 21 Dec 2016 01:53
Operator : UM/SJ
Sample : H6106-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA7G8

Quant Time: Dec 21 02:46:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 02:43:00 2016
Response via : Initial Calibration

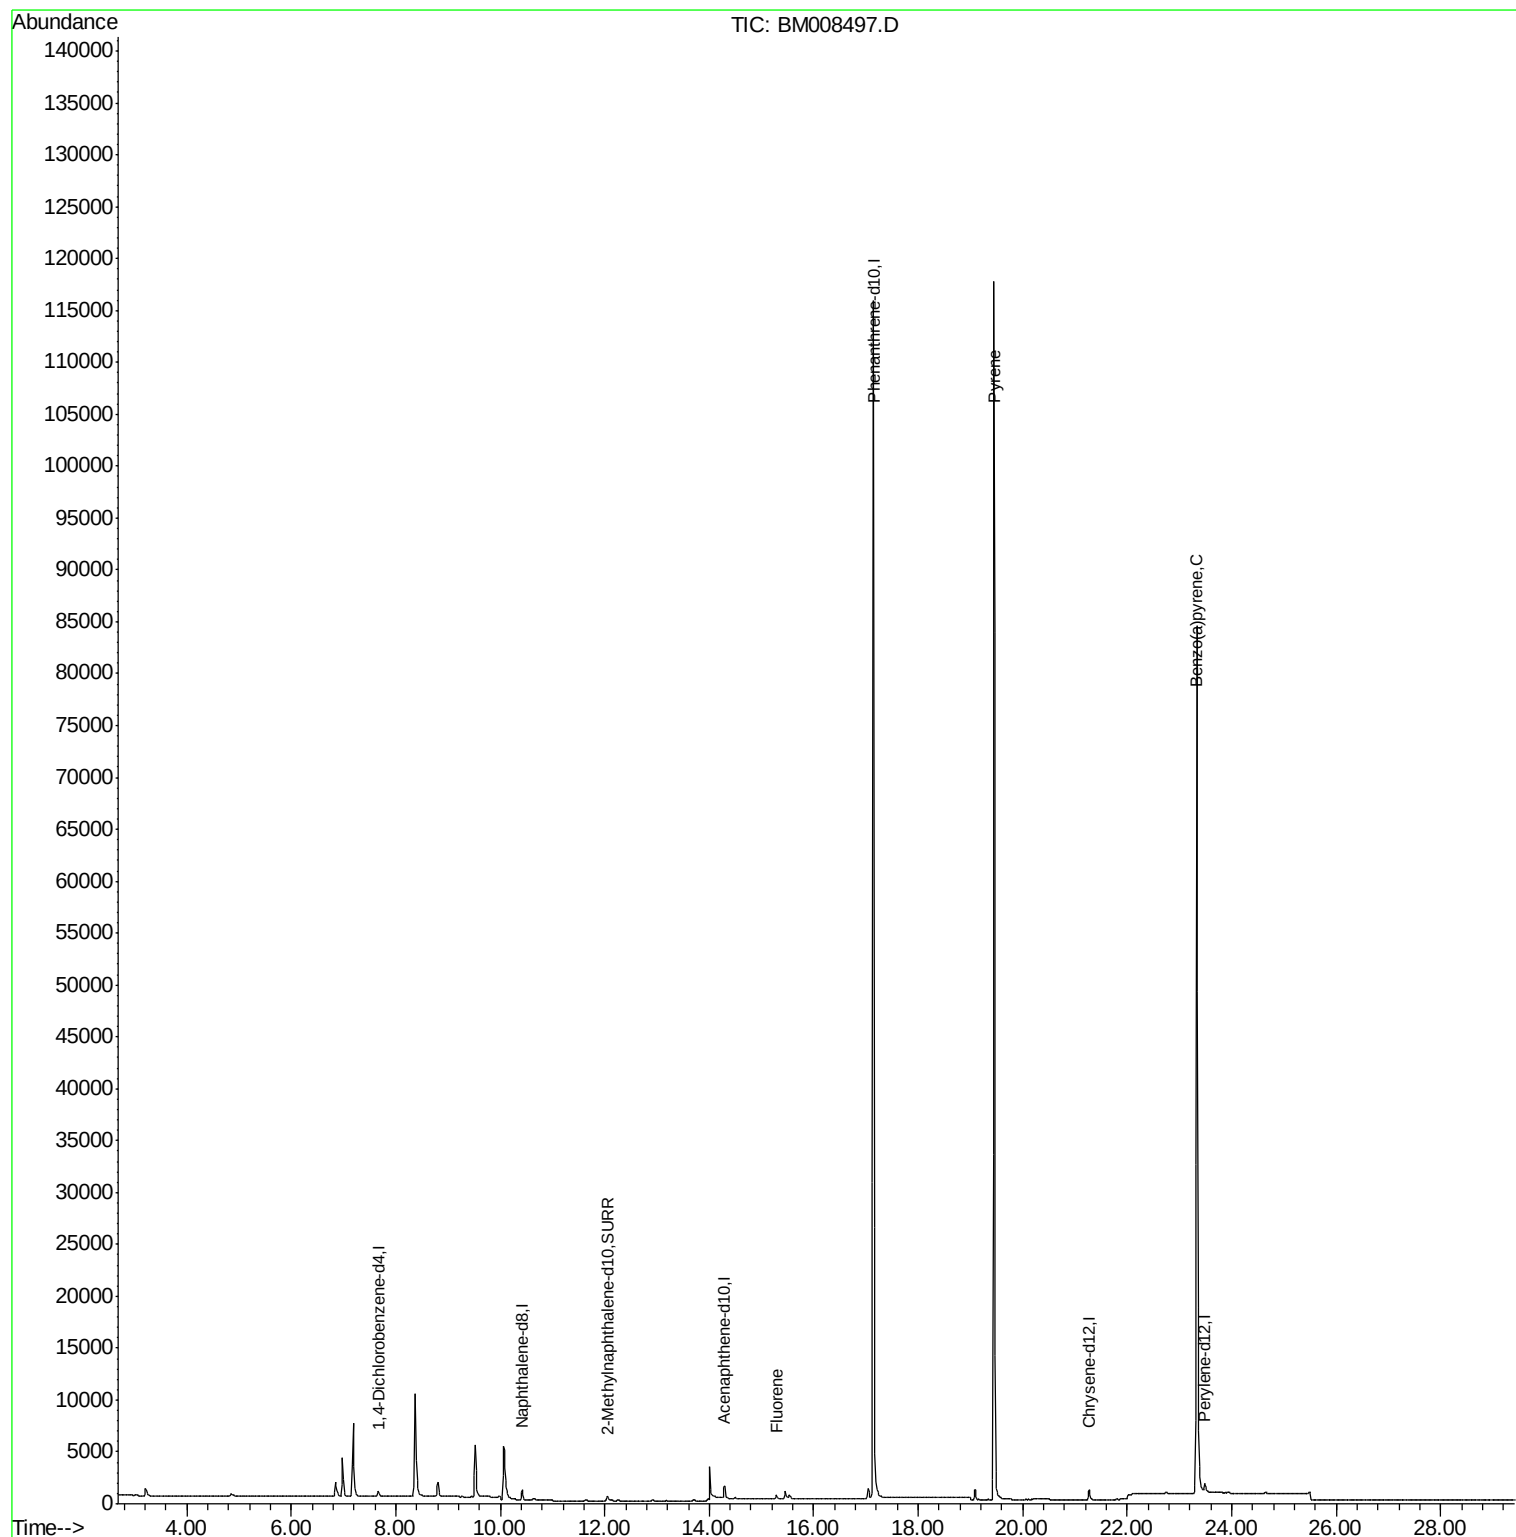

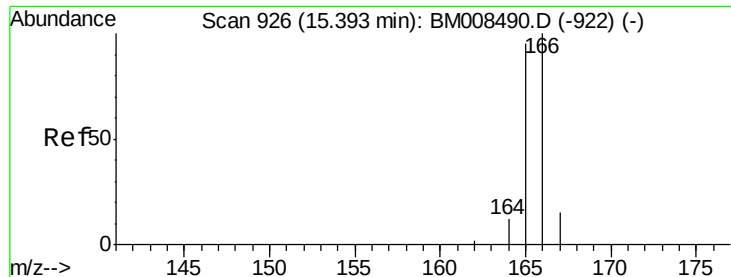

#9

Fluorene

Concen: 0.10 ng/ul

RT: 15.29 min Scan# 920

Delta R.T. -0.10 min

Lab File: BM008497.D

Acq: 21 Dec 2016 01:53

Instrument :

BNA_M

ClientSampleId :

DA7G8


Tgt Ion:166 Resp: 322

Ion Ratio Lower Upper

166 100

165 24.3 73.4 110.2#




167 44.2 14.6 22.0#

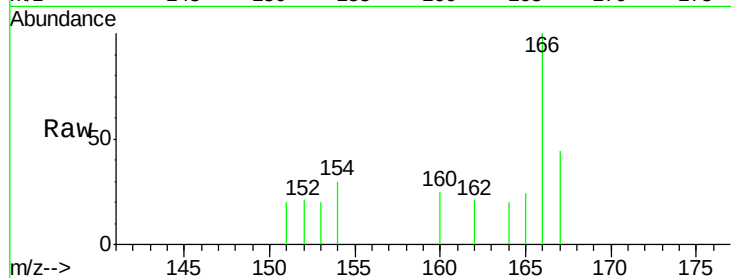

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

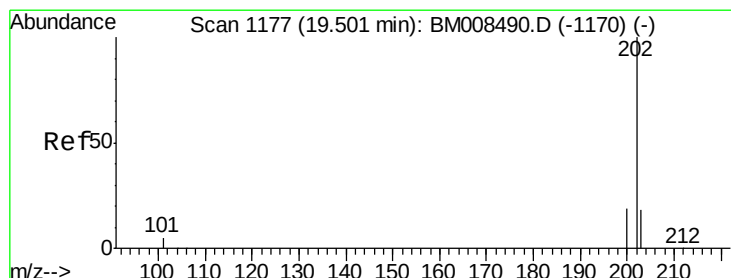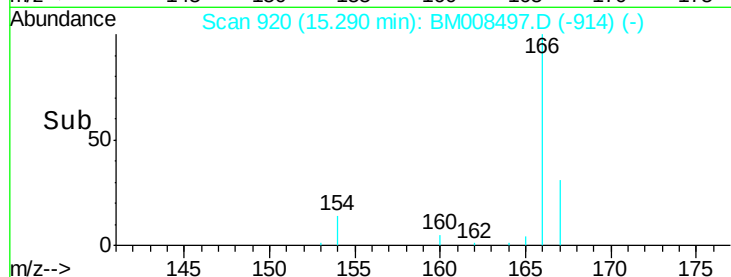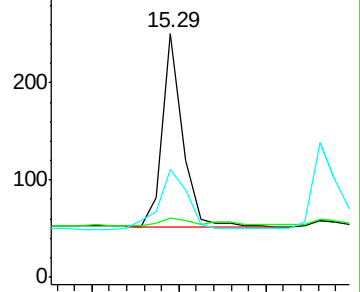

#17

Pyrene

Concen: 0.06 ng/ul

RT: 19.45 min Scan# 1173

Delta R.T. -0.05 min

Lab File: BM008497.D

Acq: 21 Dec 2016 01:53


Tgt Ion:202 Resp: 288

Ion Ratio Lower Upper

202 100

200 25.2 18.2 27.4



203 141.2 15.6 23.4#



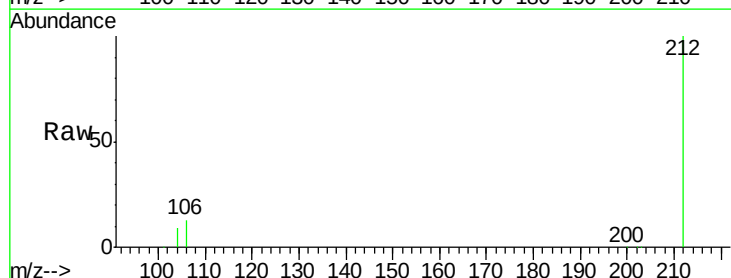


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

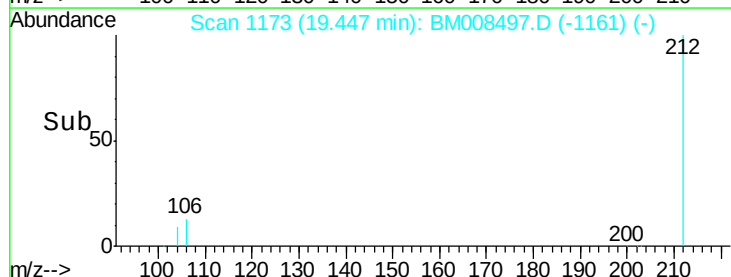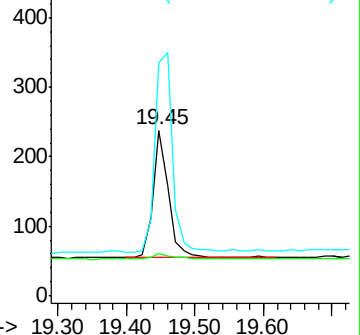

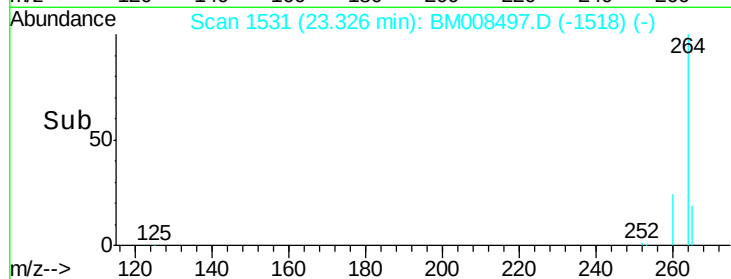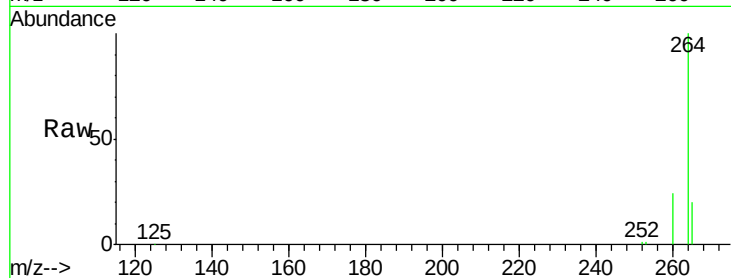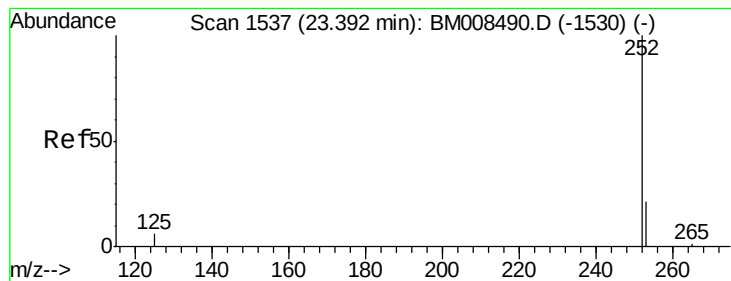

#23

Benzo(a)pyrene

Concen: 0.10 ng/ul

RT: 23.33 min Scan# 1531

Delta R.T. -0.07 min

Lab File: BM008497.D

Acq: 21 Dec 2016 01:53

Instrument :

BNA_M

ClientSampleId :

DA7G8

Tgt Ion: 252 Resp: 610

Ion Ratio Lower Upper

252 100

253 73.1 28.5 42.7#

125 57.0 18.1 27.1#

