

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
 Data File : BM008481.D
 Acq On : 20 Dec 2016 16:17
 Operator : UM/SJ
 Sample : PB95384BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 21 01:28:10 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 01:24:53 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK84

Manual Integrations
 APPROVED

sohil
 12/21/2016 6:20:45 PM

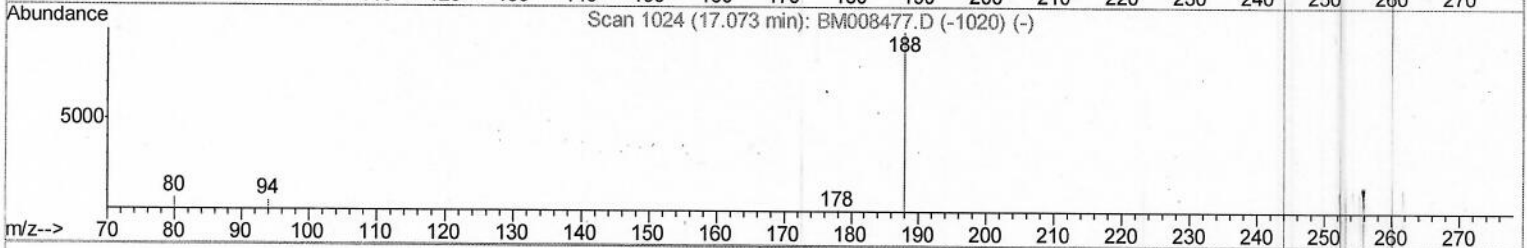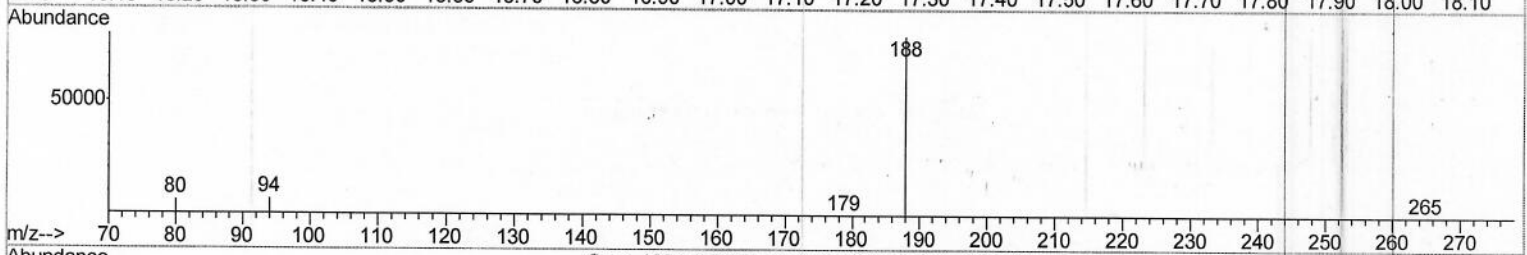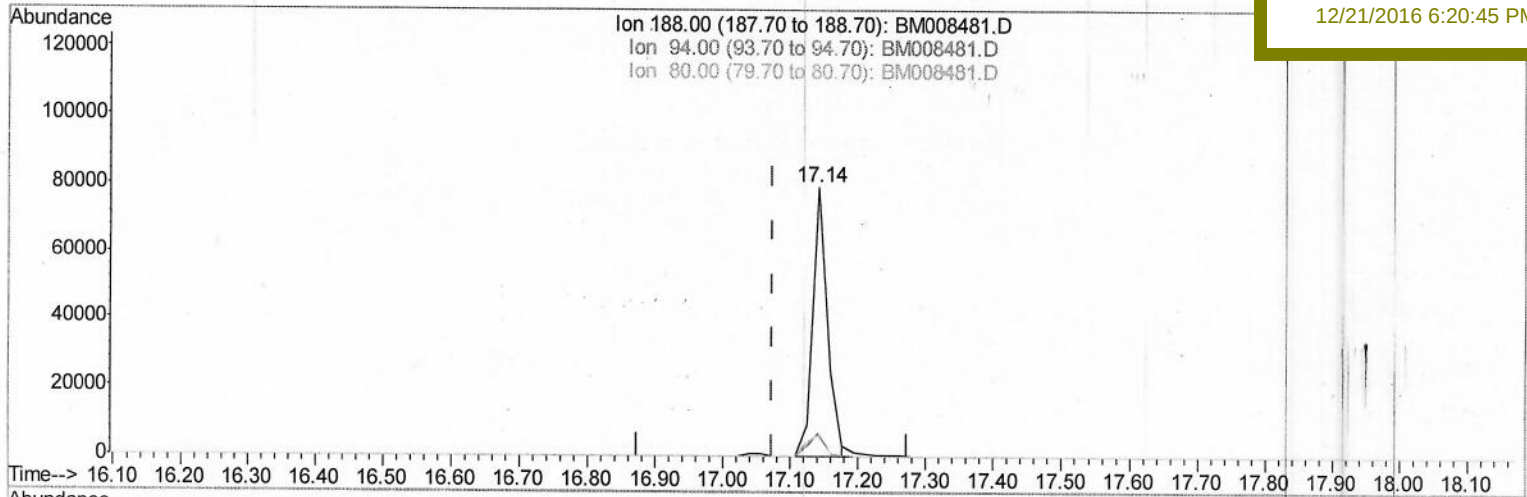

TIC: BM008481.D

(10) Phenanthrene-d10 (I)
 17.142min (+0.069) 0.40ng/ul
 response 118717

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	8.28#
80.00	11.80	7.69#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
 Data File : BM008481.D
 Acq On : 20 Dec 2016 16:17
 Operator : UM/SJ
 Sample : PB95384BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK84

Manual Integrations
 APPROVED

sohil
 12/21/2016 6:20:45 PM

Quant Time: Dec 21 01:28:10 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 01:24:53 2016
 Response via : Initial Calibration

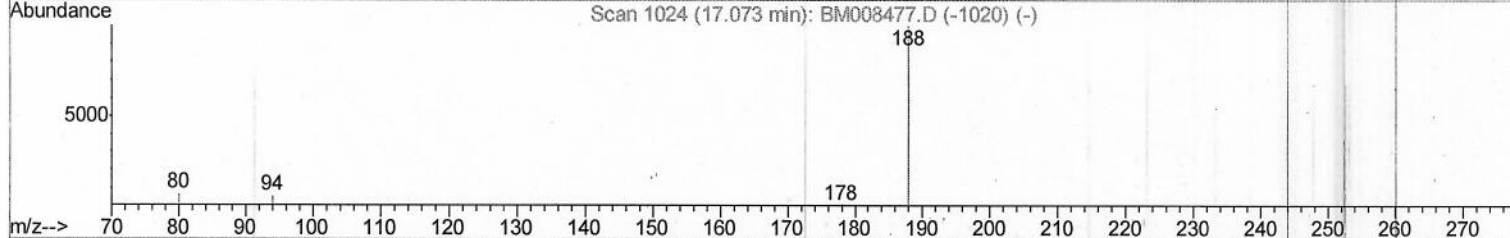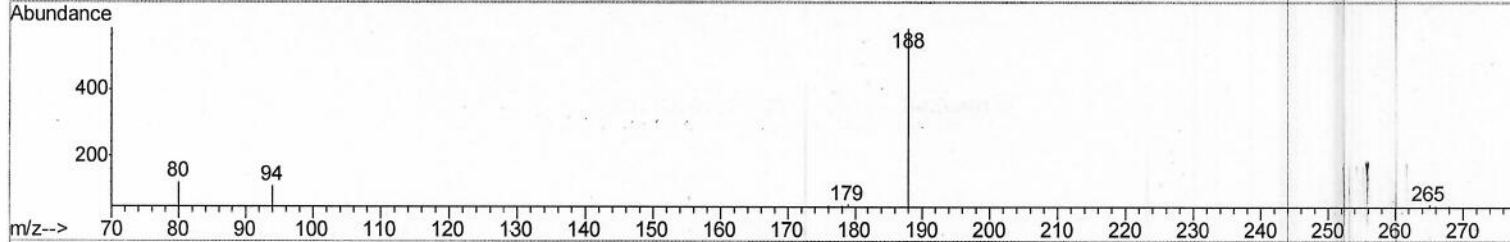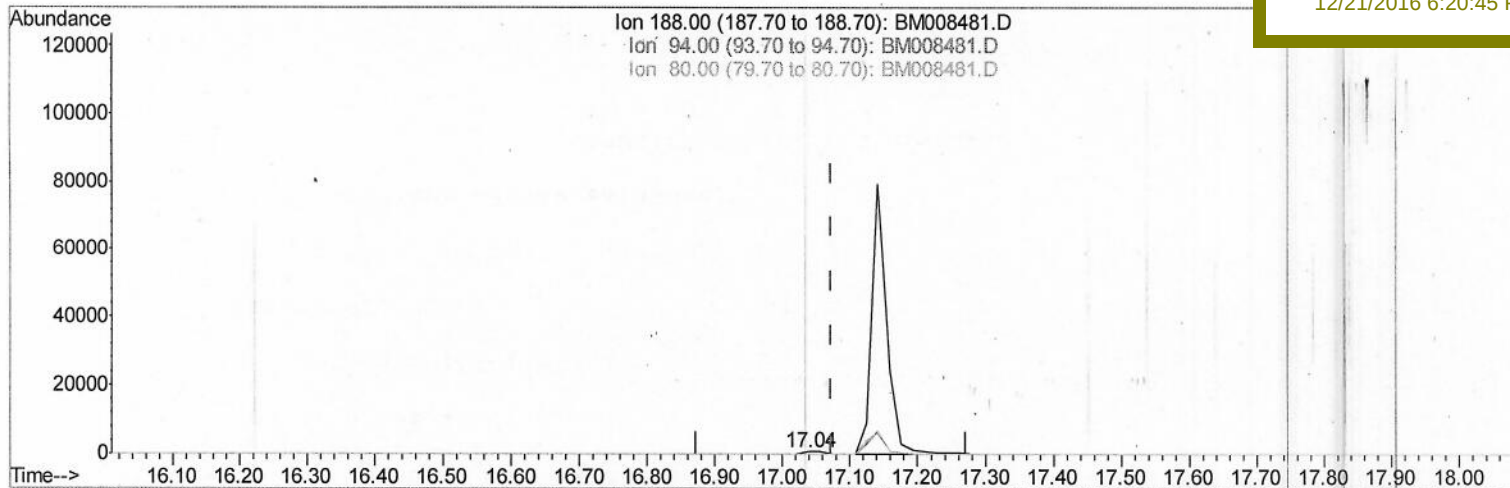

TIC: BM008481.D

(10) Phenanthrene-d10 (I)

17.039min (-0.034) 0.40ng/ul m

response 1225

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	18.93#
80.00	11.80	21.00#
0.00	0.00	0.00

S.J
 12/21/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
 Data File : BM008481.D
 Acq On : 20 Dec 2016 16:17
 Operator : UM/SJ
 Sample : PB95384BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 21 01:28:10 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 01:24:53 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK84

Manual Integrations
 APPROVED

sohil
 12/21/2016 6:20:45 PM

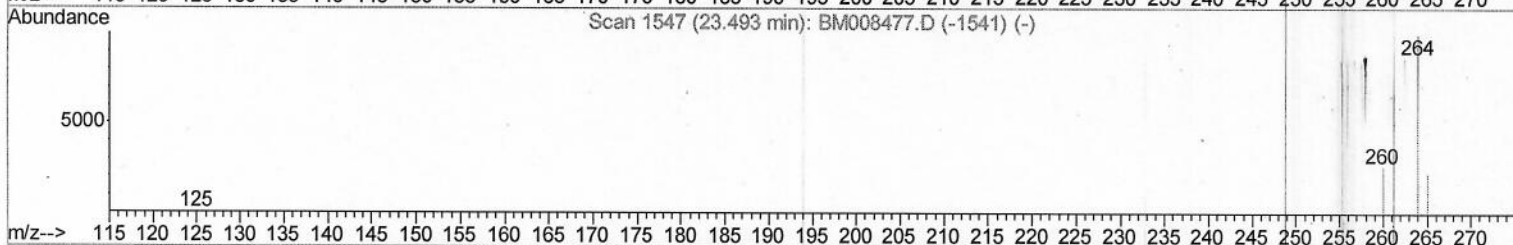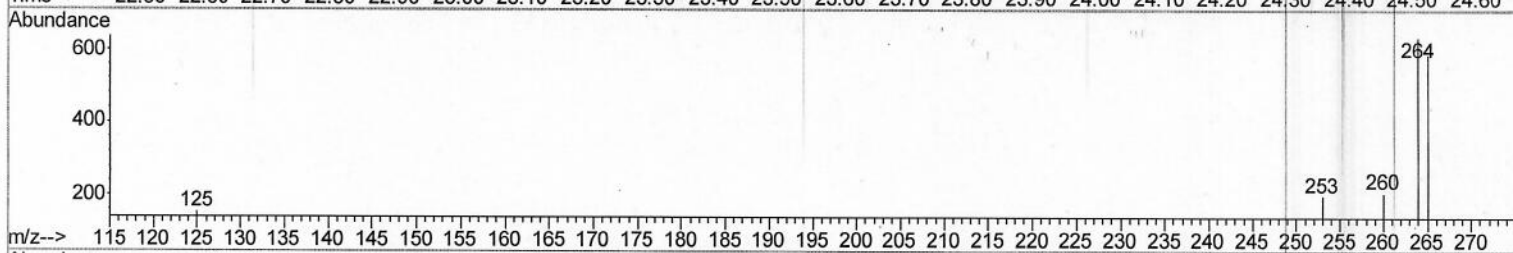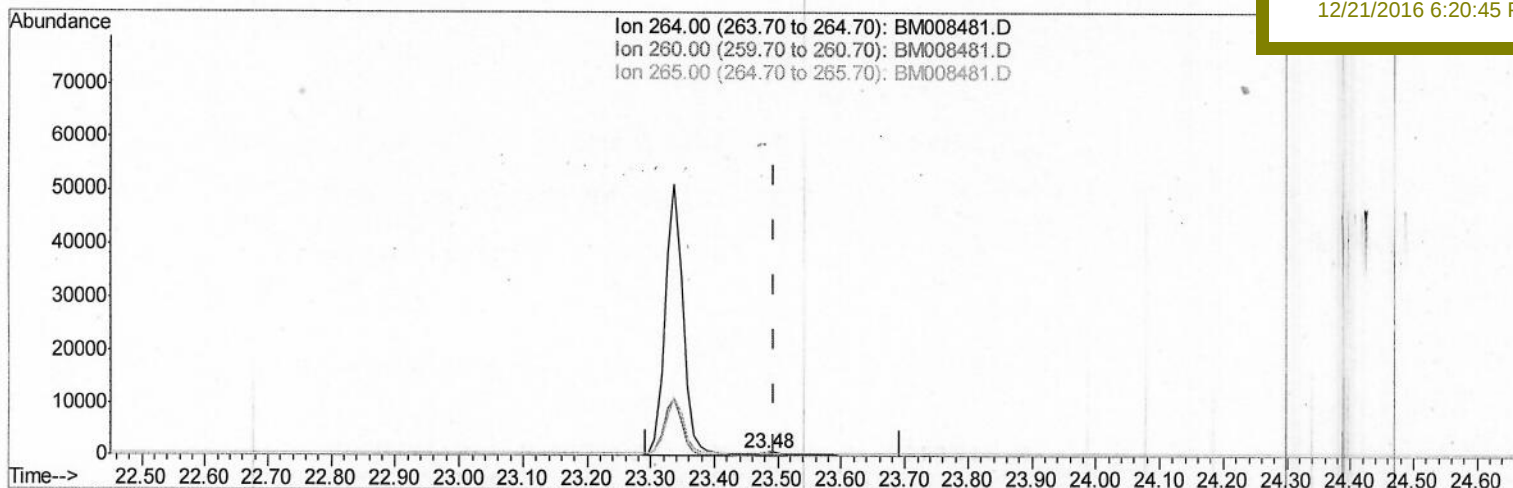

TIC: BM008481.D

(20) Perylene-d12 (I)

23.483min (-0.010) 0.40ng/ul

response 1482

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	32.65
265.00	103.50	92.78
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
 Data File : BM008481.D
 Acq On : 20 Dec 2016 16:17
 Operator : UM/SJ
 Sample : PB95384BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 21 01:28:10 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 01:24:53 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK84

Manual Integrations
 APPROVED

sohil
 12/21/2016 6:20:45 PM

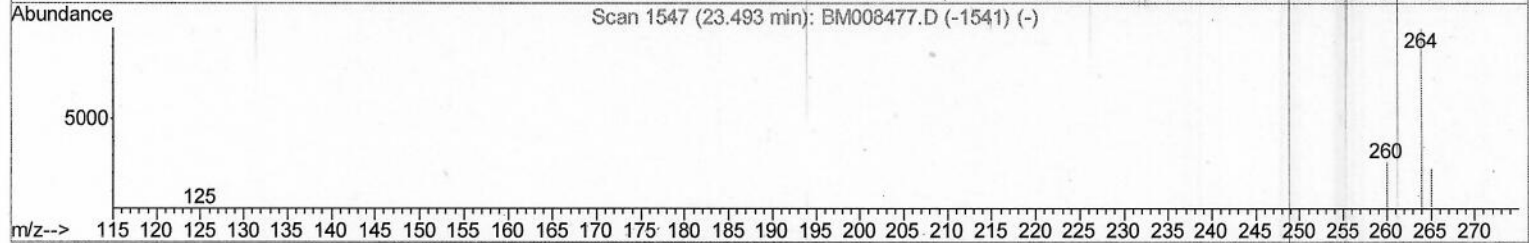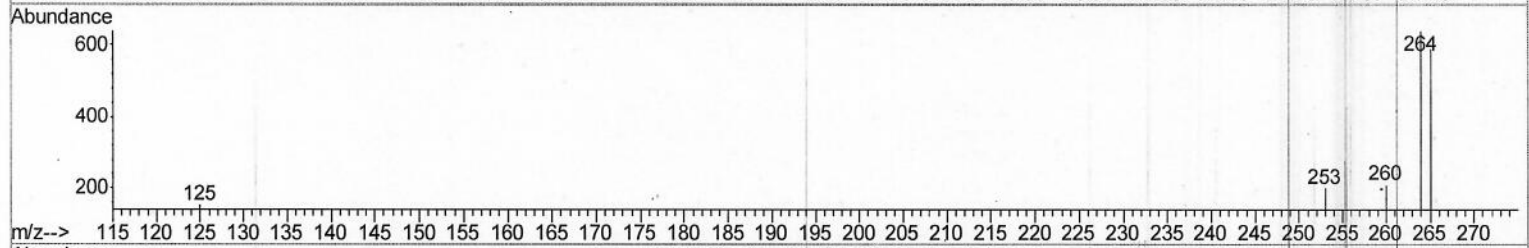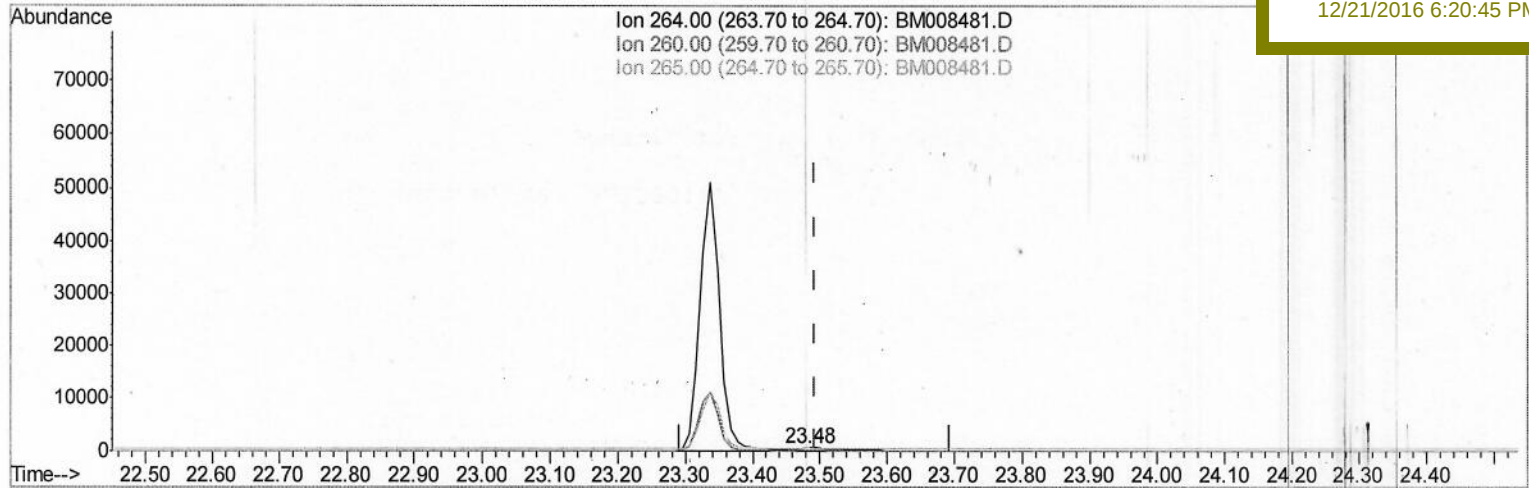

TIC: BM008481.D

(20) Perylene-d12 (I)

23.483min (-0.010) 0.40ng/ul m

response 1032

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	32.65
265.00	103.50	92.78
0.00	0.00	0.00

S.J
 12/21/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
 Data File : BM008481.D
 Acq On : 20 Dec 2016 16:17
 Operator : UM/SJ
 Sample : PB95384BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 21 02:08:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 01:24:53 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK84

Manual Integrations
 APPROVED

sohil
 12/21/2016 6:20:45 PM

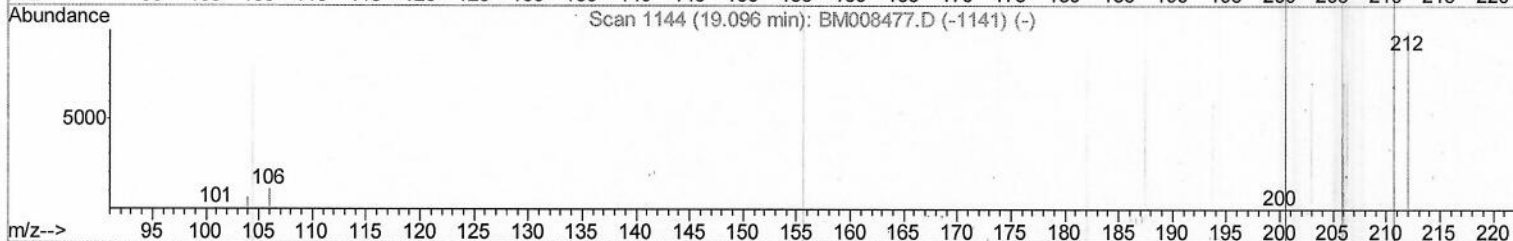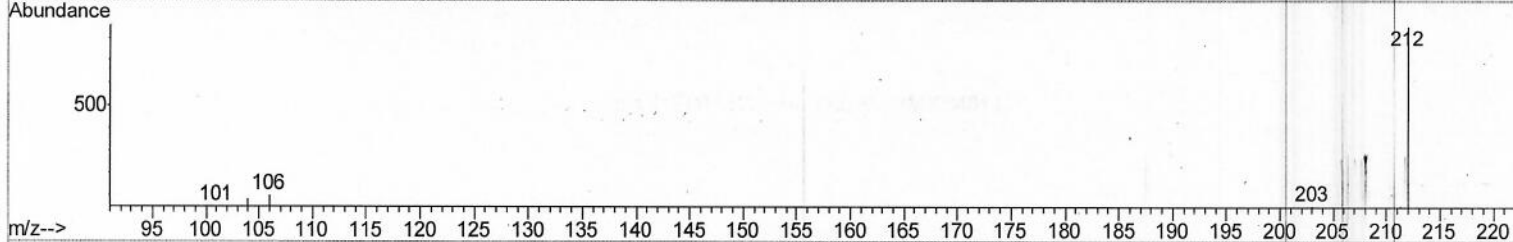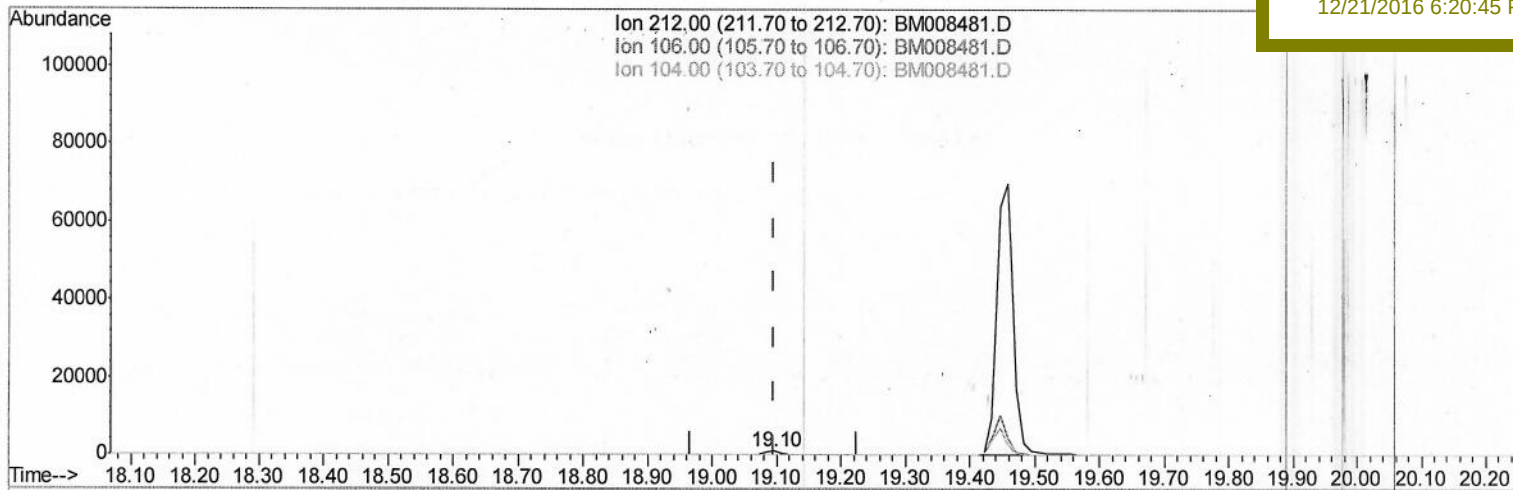

TIC: BM008481.D

(14) Fluoranthene-d10 (SURR)

19.096min (+0.000) 0.38ng/ul

response 1286

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	8.79#
104.00	15.60	4.98#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
 Data File : BM008481.D
 Acq On : 20 Dec 2016 16:17
 Operator : UM/SJ
 Sample : PB95384BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 21 02:08:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 01:24:53 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 Client Sampled :
 SBLK84

Manual Integrations
 APPROVED

sohil
 12/21/2016 6:20:45 PM

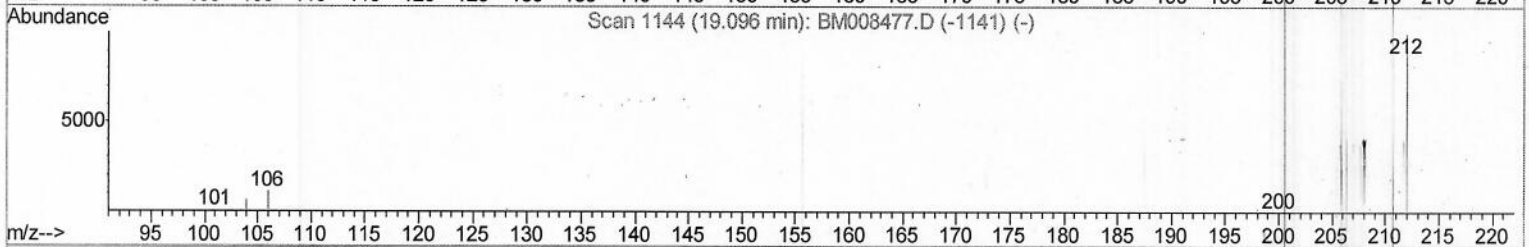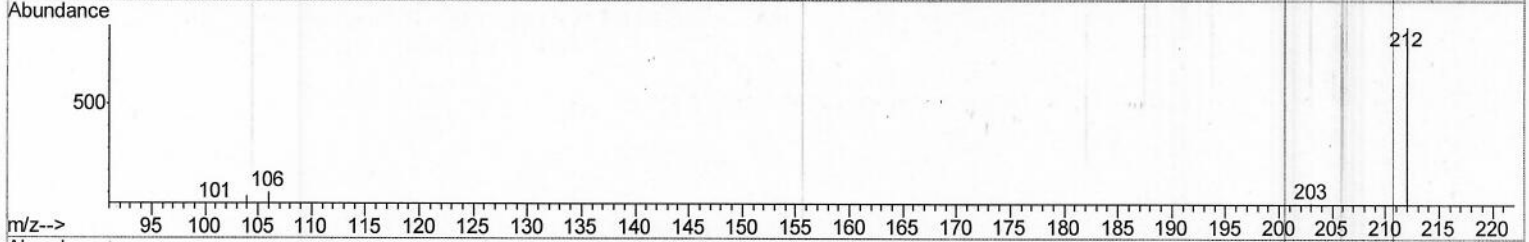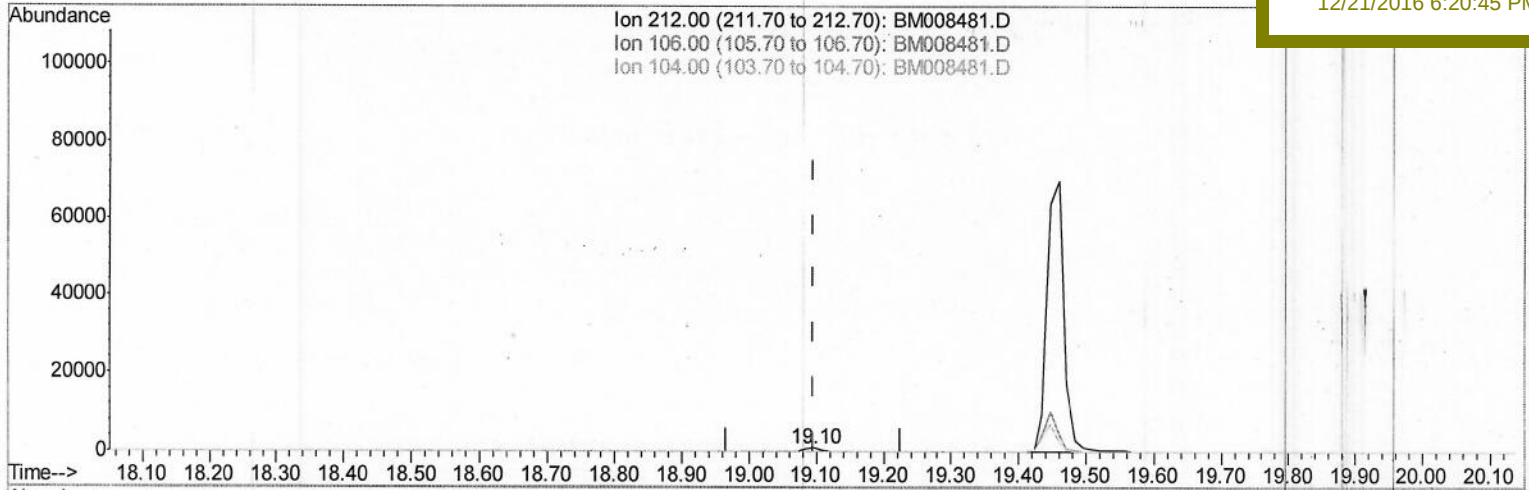

TIC: BM008481.D

(14) Fluoranthene-d10 (SURR)

19.096min (+0.000) 0.42ng/ul m

response 1401

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	8.07#
104.00	15.60	4.57#
0.00	0.00	0.00

S.J
 12/21/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
Data File : BM008481.D
Acq On : 20 Dec 2016 16:17
Operator : UM/SJ
Sample : PB95384BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 21 02:09:26 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 01:24:53 2016
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
SBLK84

Manual Integrations
APPROVED

sohil
12/21/2016 6:20:45 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	360	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.43	136	1187	0.40	ng/ul	-0.04
6) Acenaphthene-d10	14.30	164	704	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.04	188	1225m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.27	240	1190	0.40	ng/ul	0.01
20) Perylene-d12	23.48	264	1032m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	701	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.10	212	1401m	0.42	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

→ } SJ
→ } 12/21/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
Data File : BM008481.D
Acq On : 20 Dec 2016 16:17
Operator : UM/SJ
Sample : PB95384BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 21 02:09:26 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 01:24:53 2016
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
SBLK84

Manual Integrations
APPROVED

sohil
12/21/2016 6:20:45 PM

