

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
 Data File : BM008491.D
 Acq On : 20 Dec 2016 22:18
 Operator : UM/SJ
 Sample : H6039-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 21 10:25:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 02:43:00 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA8S9

Manual Integrations
 APPROVED

sohil
 12/21/2016 6:20:21 PM

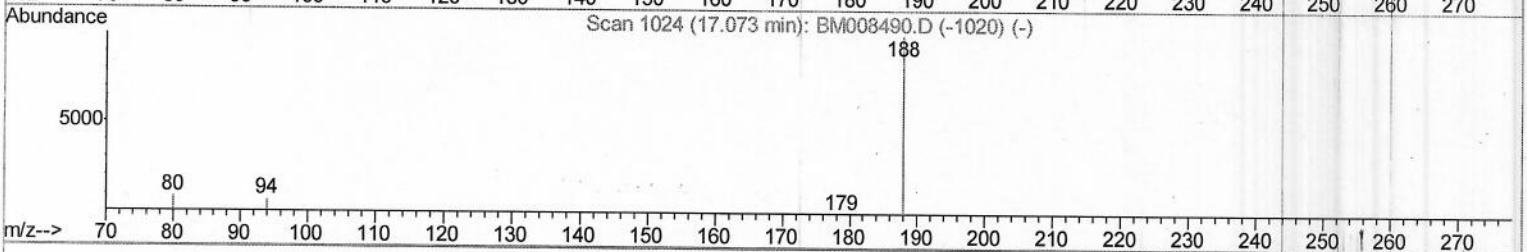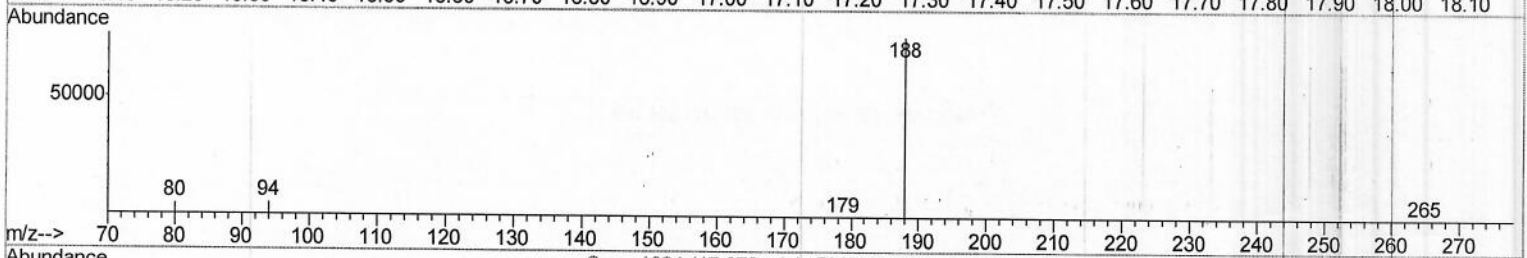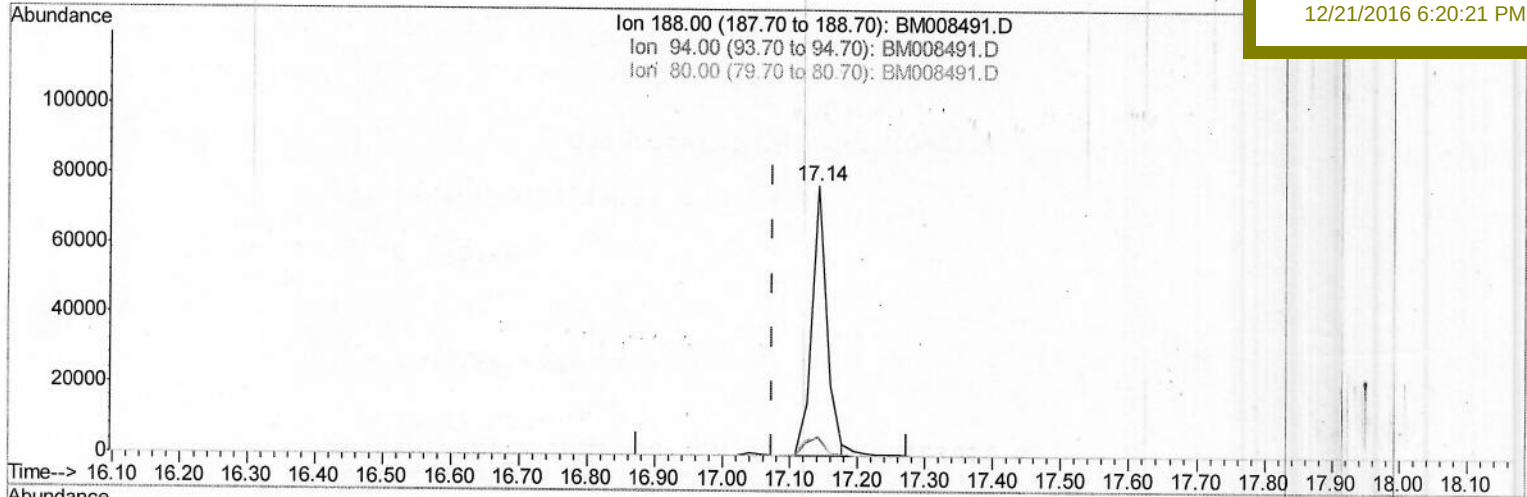

TIC: BM008491.D

(10) Phenanthrene-d10 (I)
 17.142min (+0.069) 0.40ng/ul
 response 118065

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.04#
80.00	11.80	6.44#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
 Data File : BM008491.D
 Acq On : 20 Dec 2016 22:18
 Operator : UM/SJ
 Sample : H6039-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 21 10:25:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 02:43:00 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA8S9

Manual Integrations
 APPROVED

sohil
 12/21/2016 6:20:21 PM

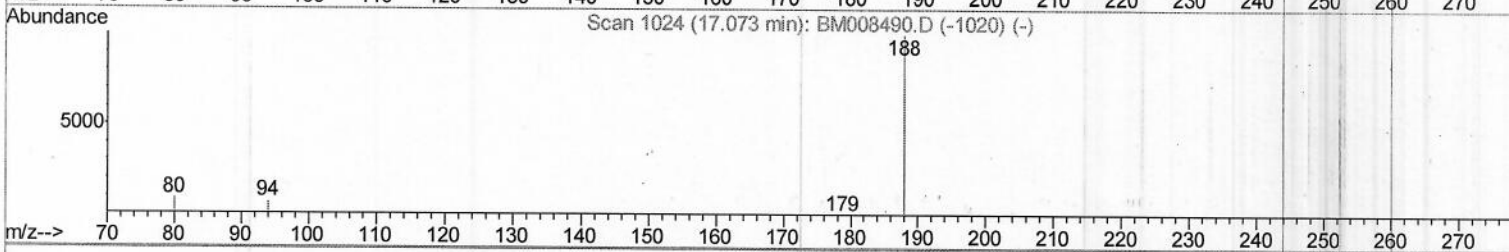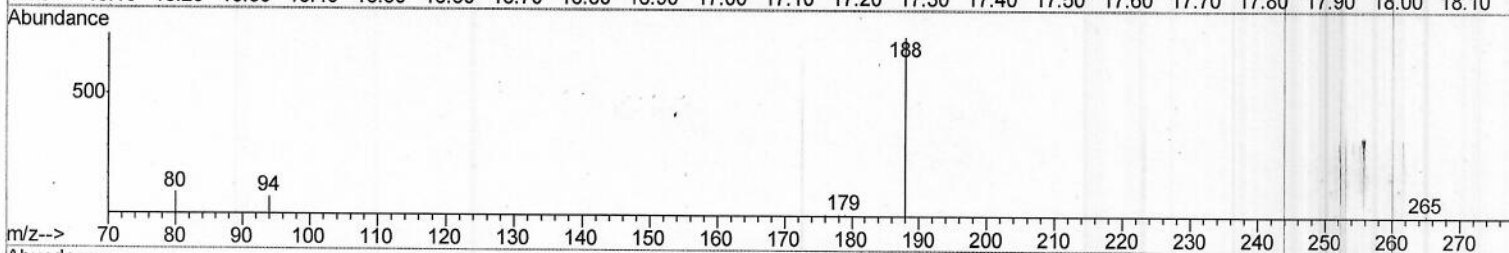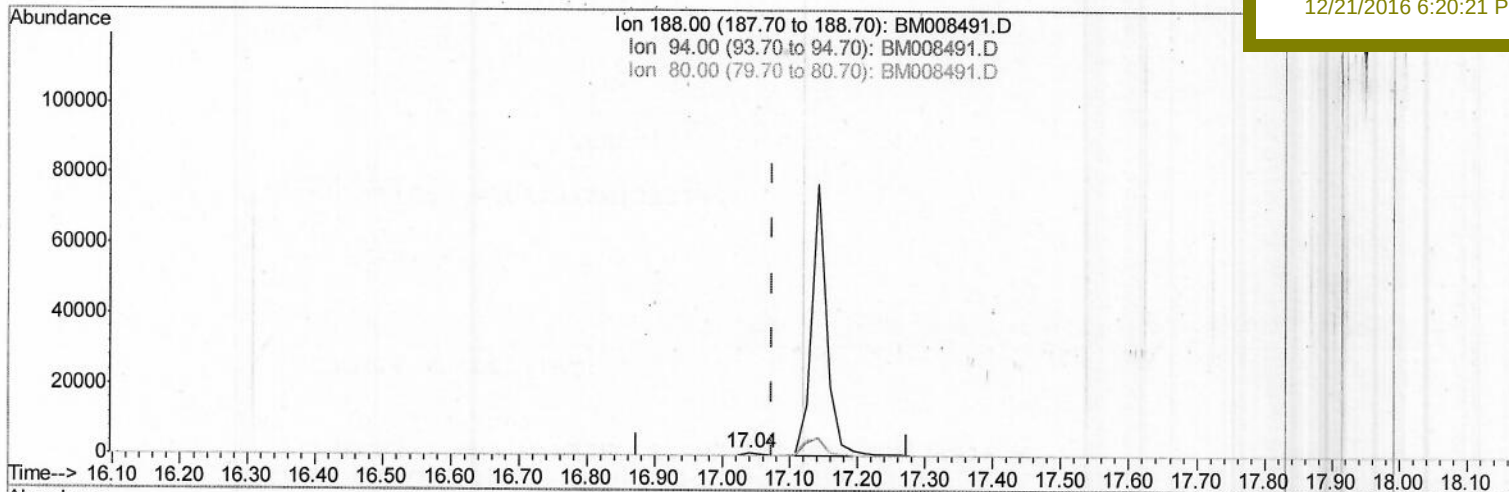

TIC: BM008491.D

(10) Phenanthrene-d10 (I)

17.039min (-0.034) 0.40ng/ul m

response 1545

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	15.49#
80.00	11.80	17.84#
0.00	0.00	0.00

S.J
 12/21/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
Data File : BM008491.D
Acq On : 20 Dec 2016 22:18
Operator : UM/SJ
Sample : H6039-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 21 13:15:27 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 02:43:00 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DA8S9

Manual Integrations
APPROVED

sohil
12/21/2016 6:20:21 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	385	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.43	136	1295	0.40	ng/ul	-0.05
6) Acenaphthene-d10	14.30	164	770	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.04	188	1545m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.27	240	1161	0.40	ng/ul	0.00
20) Perylene-d12	23.48	264	1521	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	623	0.31	ng/ul	-0.02
14) Fluoranthene-d10	19.10	212	1191	0.28	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

→ S.J
12/21/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122016\
Data File : BM008491.D
Acq On : 20 Dec 2016 22:18
Operator : UM/SJ
Sample : H6039-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 21 13:15:27 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 02:43:00 2016
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DA8S9

Manual Integrations

APPROVED

sohil

12/21/2016 6:20:21 PM

