





#24
 Indeno(1,2,3-cd)pyrene
 Concen: 0.83 ng/ul
 RT: 25.72 min Scan# 1761
 Delta R.T. -0.00 min
 Lab File: BM008479.D
 Acq: 20 Dec 2016 15:04

Instrument :
 BNA_M
 ClientSampleId :
 DA8R0

Tot Ion	Ratio	Lower	Upper
276	100		
138	17.4	19.1	28.7#
277	25.2	19.6	29.4




Manual Integrations
 APPROVED


sohil
 12/21/2016 6:19:41 PM

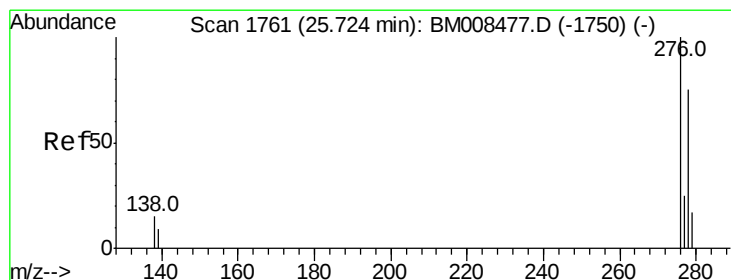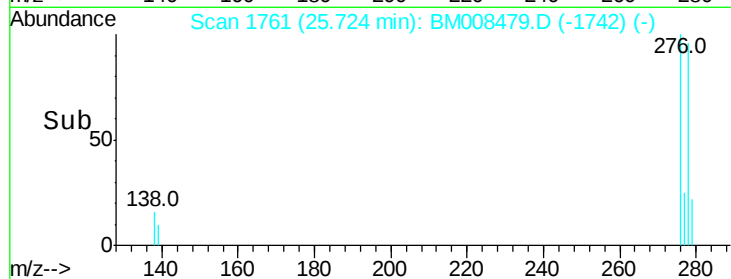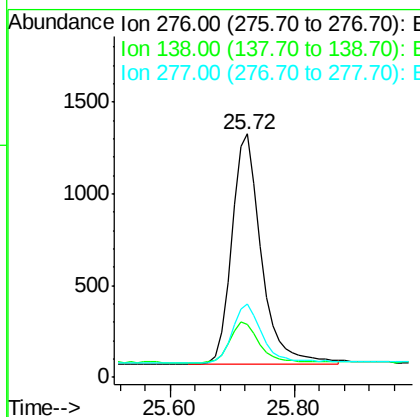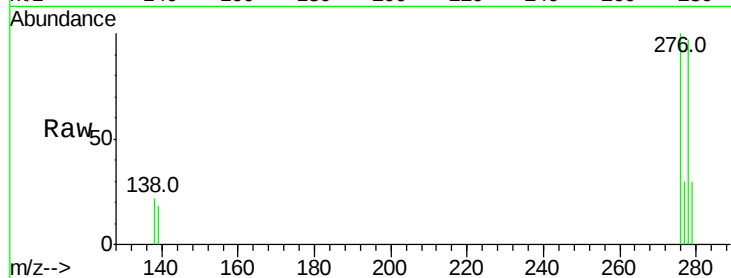

#25
 Dibenzo(a,h)anthracene
 Concen: 1.02 ng/ul
 RT: 25.72 min Scan# 1761
 Delta R.T. -0.01 min
 Lab File: BM008479.D
 Acq: 20 Dec 2016 15:04

Tgt Ion	Ratio	Lower	Upper
278	100		
139	18.4	17.4	26.0
279	31.3	25.9	38.9

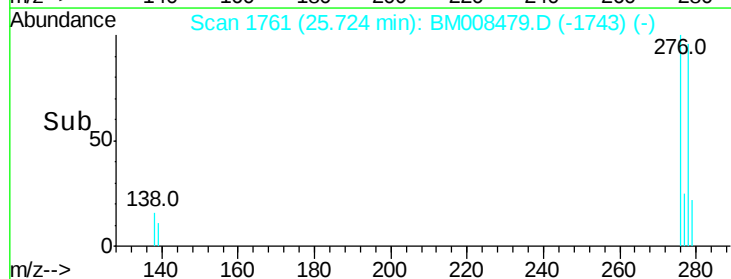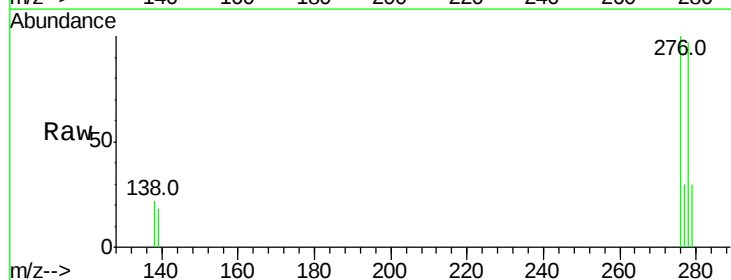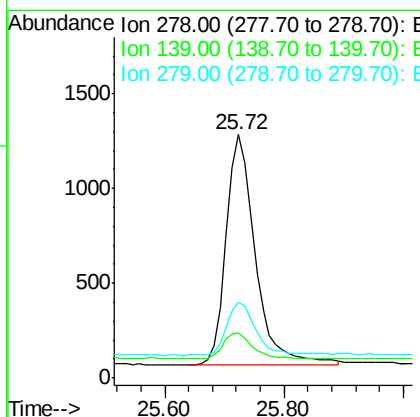

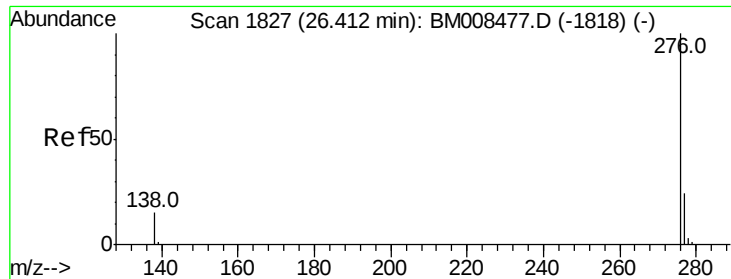

#26
 Benzo(a,h,i)perylene
 Concen: 1.04 ng/ul
 RT: 26.40 min Scan# 1826
 Delta R.T. -0.01 min
 Lab File: BM008479.D
 Acq: 20 Dec 2016 15:04

Instrument :
 BNA_M
 ClientSampleId :
 DA8R0

Tot Ion	Ratio	Lower	Upper
276	100		
277	27.8	21.8	32.8
138	19.9	20.5	30.7

Manual Integrations
 APPROVED

sohil
 12/21/2016 6:19:41 PM

