
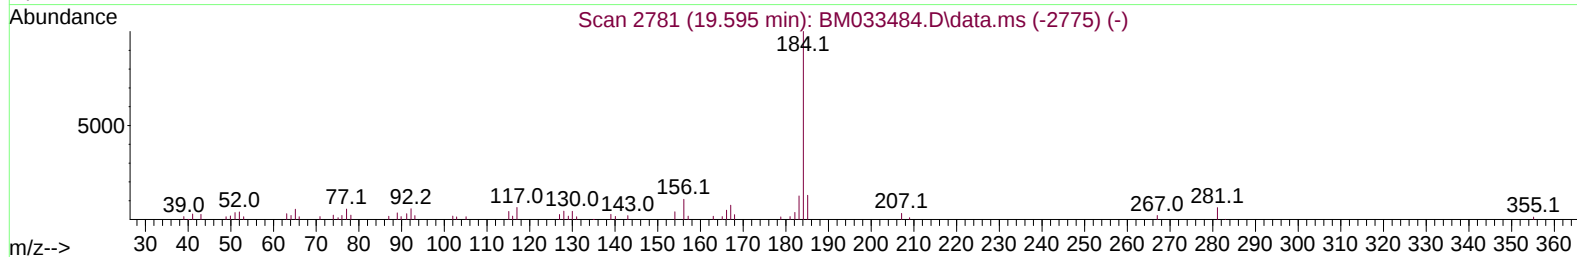
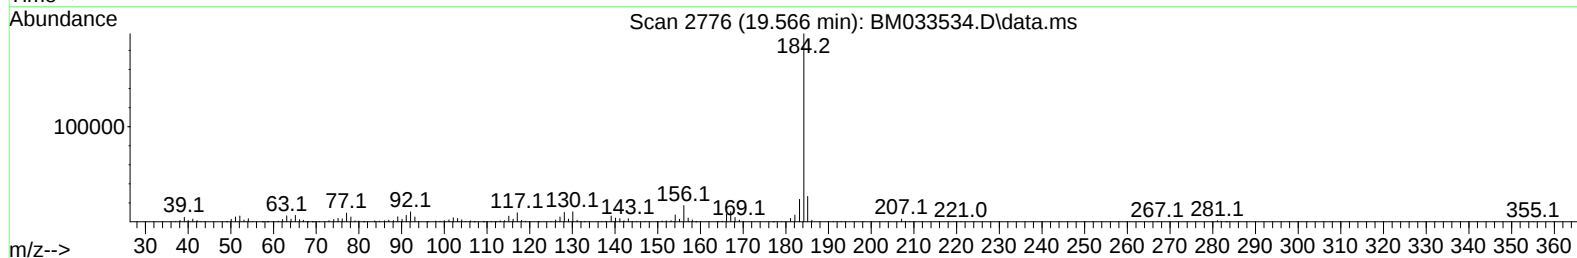


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122021\
Data File : BM033534.D
Acq On : 20 Dec 2021 10:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 04:24:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 21 03:57:10 2021
Response via : Initial Calibration

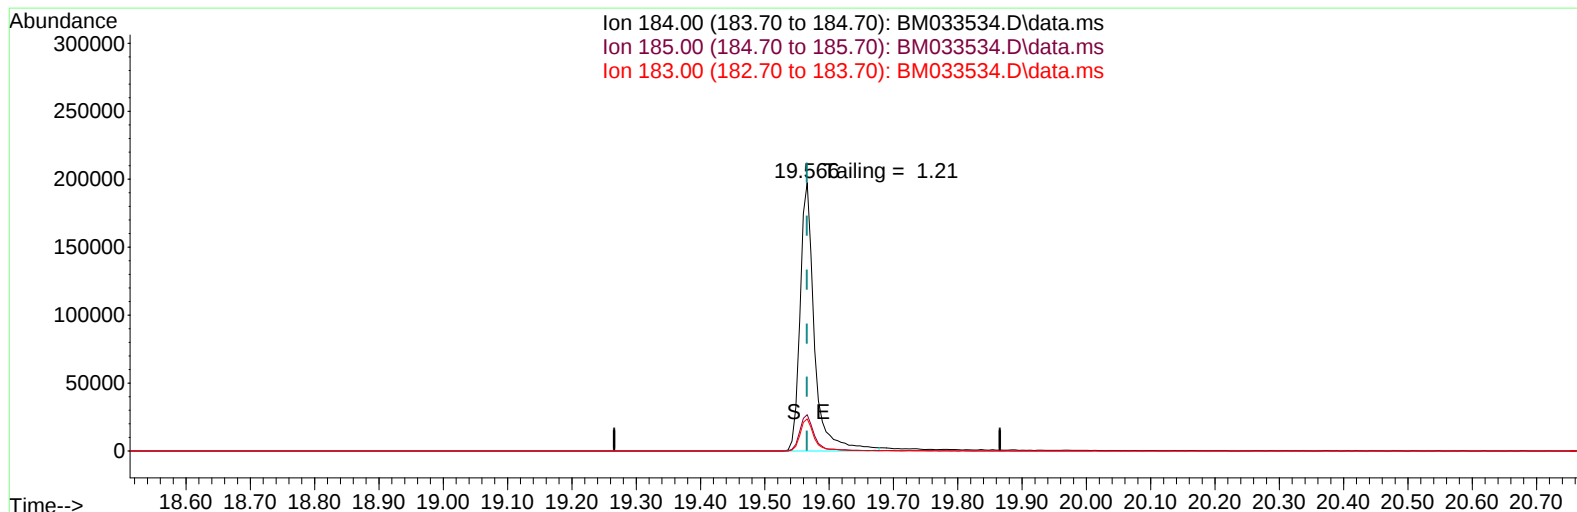

TIC: BM033534.D\data.ms

(77) Benzidine




19.566min (+ 0.000) 1185013.68 ng

response 315823

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.55
183.00	12.10	12.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122021\
Data File : BM033534.D
Acq On : 20 Dec 2021 10:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 04:24:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 21 03:57:10 2021
Response via : Initial Calibration

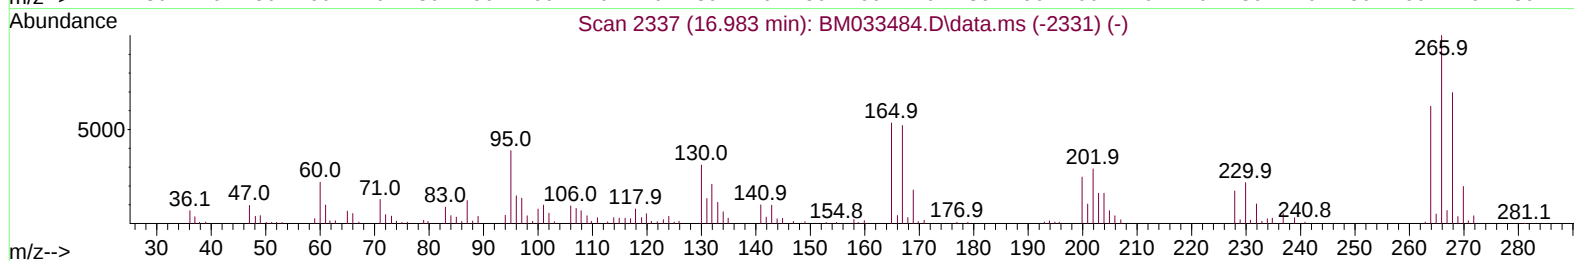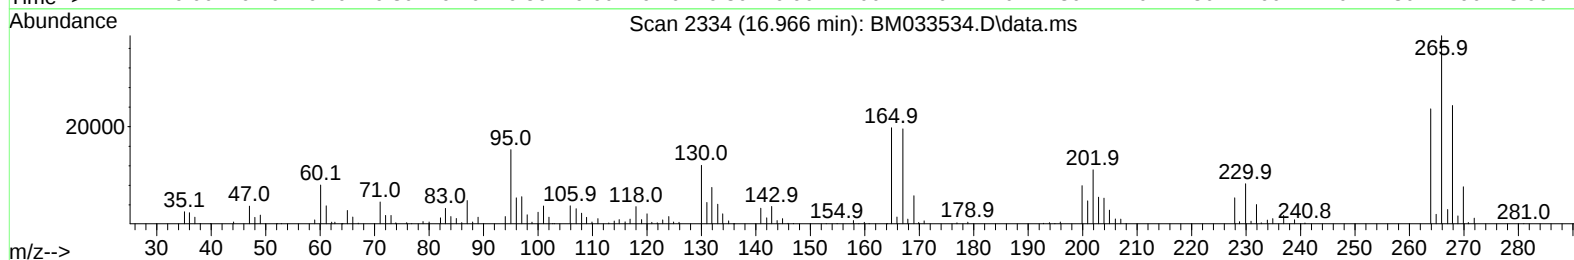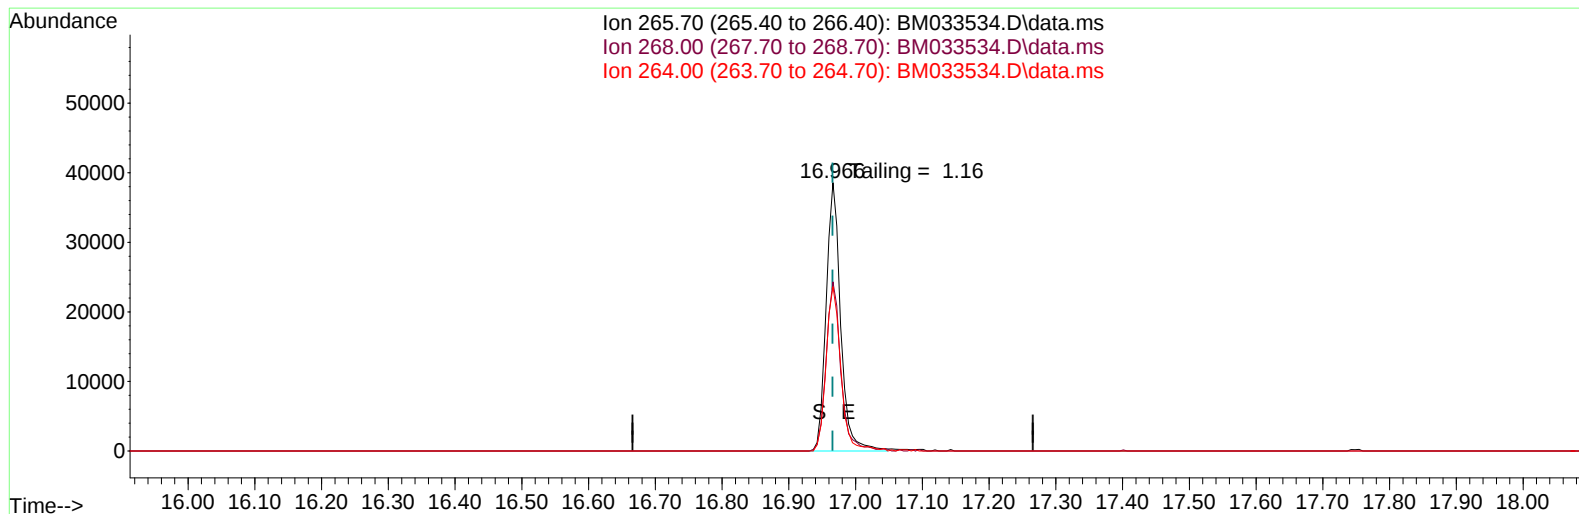

TIC: BM033534.D\data.ms

(70) Pentachlorophenol (C)

16.966min (+ 0.000) 0.00 ng

response 58895

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.01
264.00	61.40	61.23
0.00	0.00	0.00