

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122021\
 Data File : BM033544.D
 Acq On : 20 Dec 2021 17:32
 Operator : CG/JU
 Sample : M5079-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 338

Quant Time: Dec 21 03:59:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 21 03:57:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	26441	20.000	ng	0.00
21) Naphthalene-d8	10.731	136	103321	20.000	ng	# 0.00
39) Acenaphthene-d10	14.566	164	66469	20.000	ng	0.00
64) Phenanthrene-d10	17.319	188	130842	20.000	ng	# 0.00
76) Chrysene-d12	21.495	240	111868	20.000	ng	# 0.00
86) Perylene-d12	23.901	264	114980	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.484	112	174698	114.008	ng	0.00
7) Phenol-d6	7.090	99	227543	110.652	ng	0.00
23) Nitrobenzene-d5	9.096	82	179039	74.404	ng	0.00
42) 2,4,6-Tribromophenol	16.060	330	71444	95.551	ng	0.00
45) 2-Fluorobiphenyl	13.195	172	333543	69.415	ng	0.00
79) Terphenyl-d14	19.936	244	457278	64.353	ng	0.00
Target Compounds						
10) Phenol	7.119	94	9387	4.518	ng	Qvalue 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122021\
Data File : BM033544.D
Acq On : 20 Dec 2021 17:32
Operator : CG/JU
Sample : M5079-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
338

Quant Time: Dec 21 03:59:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 21 03:57:10 2021
Response via : Initial Calibration




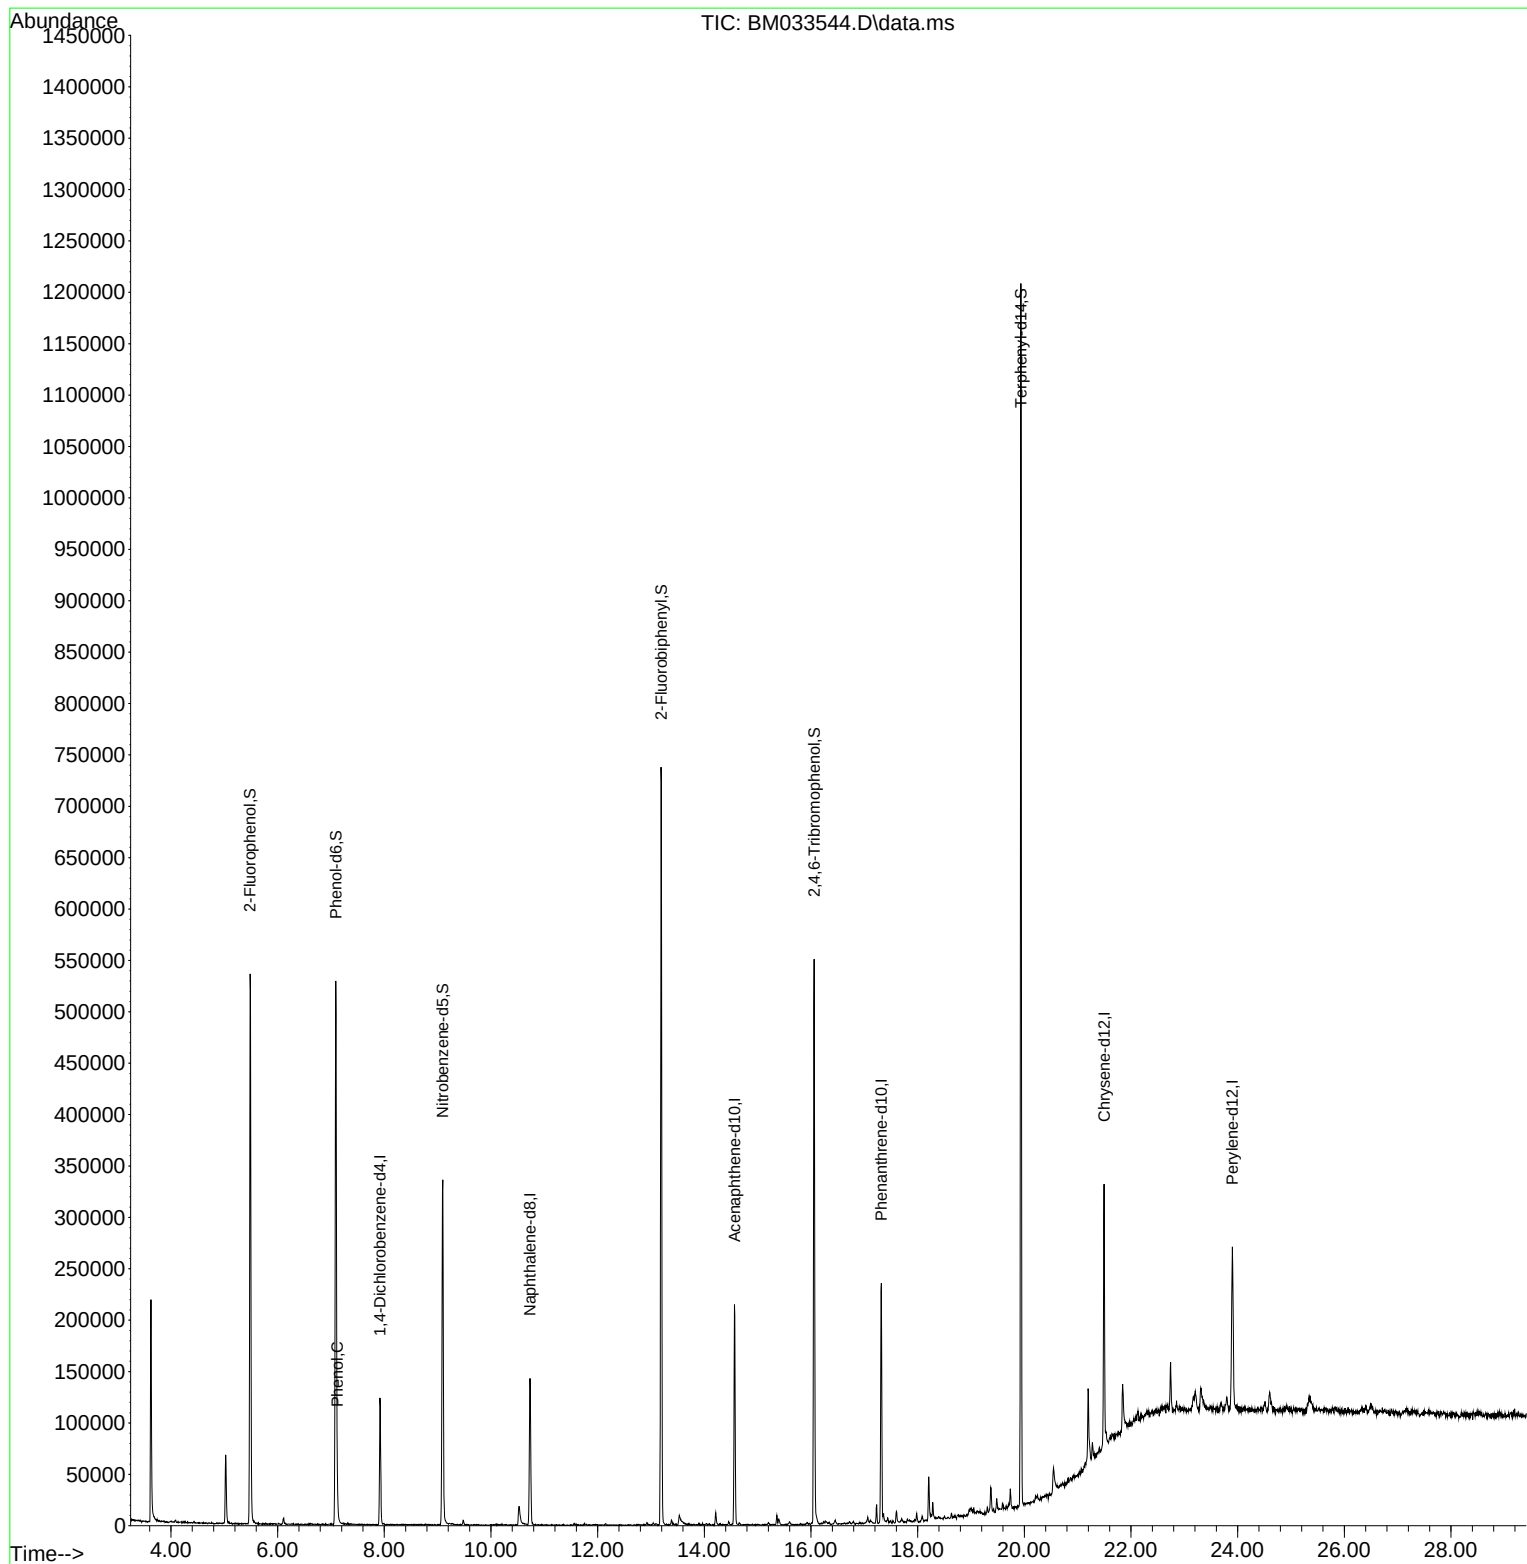


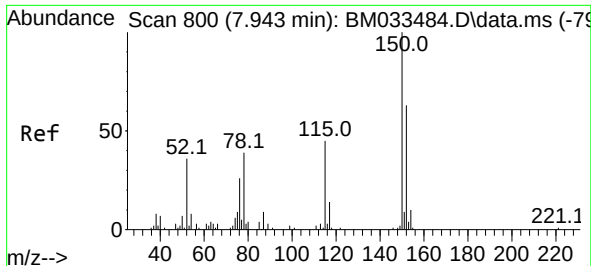

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.919 min Scan# 79
Delta R.T. 0.000 min
Lab File: BM033544.D
Acq: 20 Dec 2021 17:32




Instrument :
BNA_M
ClientSampleId :
338


Tgt Ion:152 Resp: 26441
Ion Ratio Lower Upper
152 100
150 142.8 128.9 193.3
115 68.1 53.0 79.6

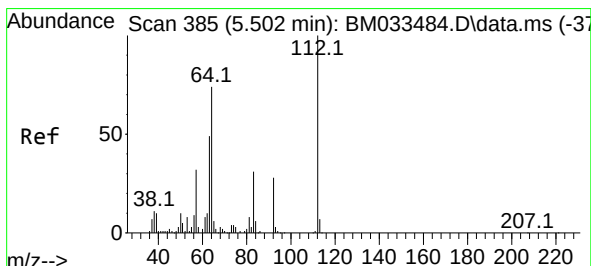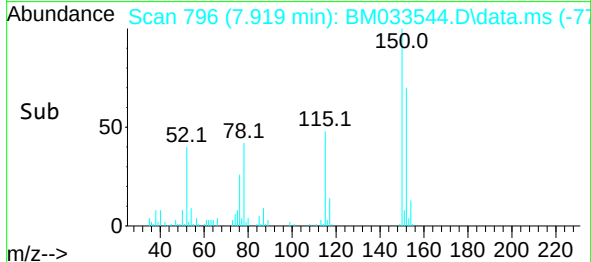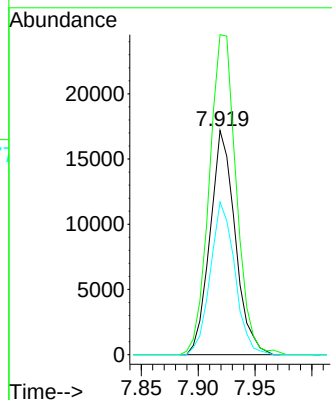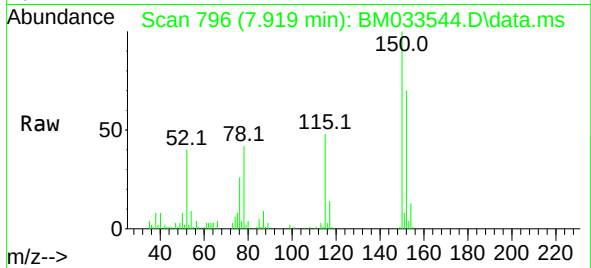

#5
2-Fluorophenol
Concen: 114.008 ng
RT: 5.484 min Scan# 382
Delta R.T. -0.000 min
Lab File: BM033544.D
Acq: 20 Dec 2021 17:32

Tgt Ion:112 Resp: 174698
Ion Ratio Lower Upper
112 100
64 70.6 55.5 83.3
63 47.2 31.3 46.9#


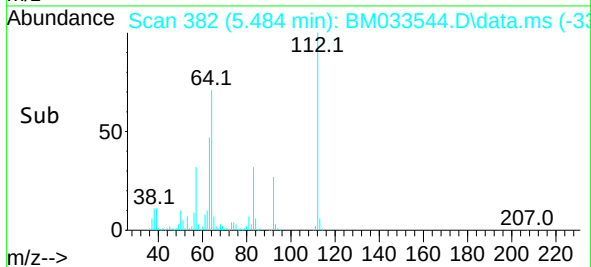
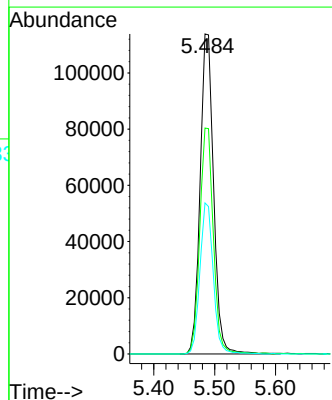
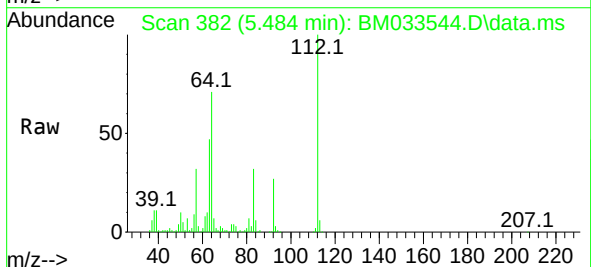


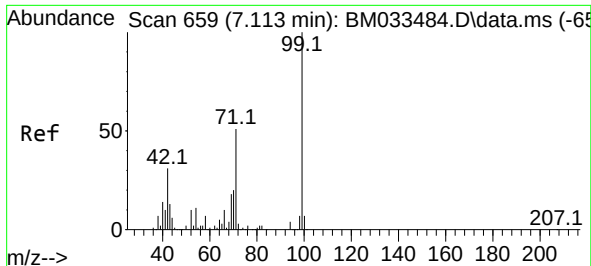

#7
Phenol-d6
Concen: 110.652 ng
RT: 7.090 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM033544.D
Acq: 20 Dec 2021 17:32




Instrument :
BNA_M
ClientSampleId :
338


Tgt Ion: 99 Resp: 227543
Ion Ratio Lower Upper
99 100
42 33.5 20.3 30.5#
71 54.6 34.5 51.7#

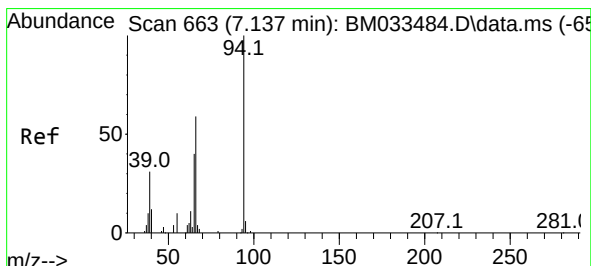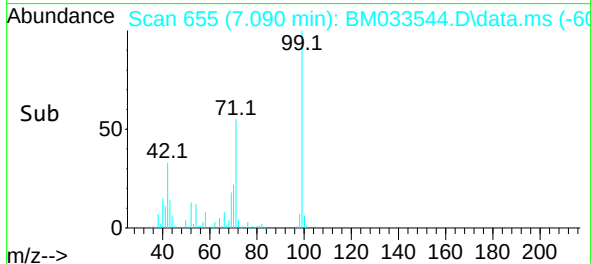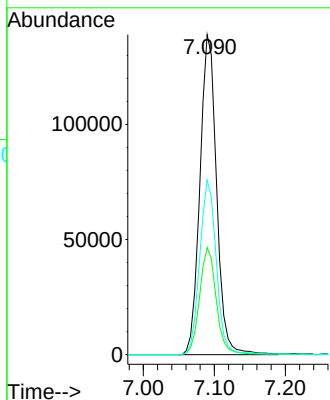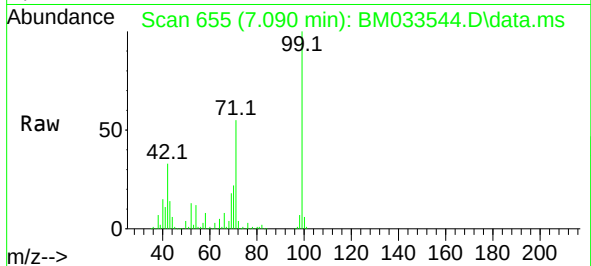

#10
Phenol
Concen: 4.518 ng
RT: 7.119 min Scan# 660
Delta R.T. -0.000 min
Lab File: BM033544.D
Acq: 20 Dec 2021 17:32

Tgt Ion: 94 Resp: 9387
Ion Ratio Lower Upper
94 100
65 44.2 15.5 55.5
66 64.9 28.5 68.5


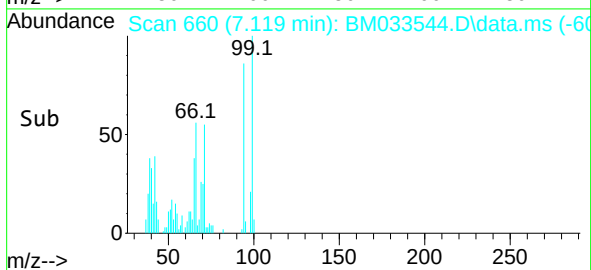
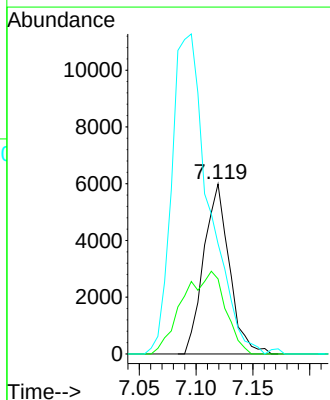
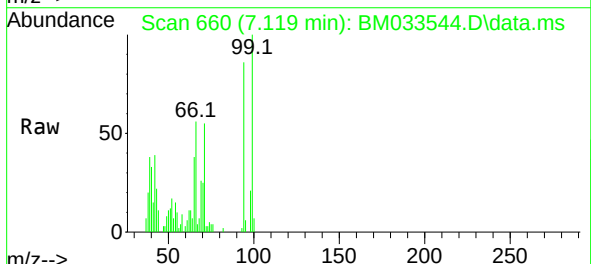


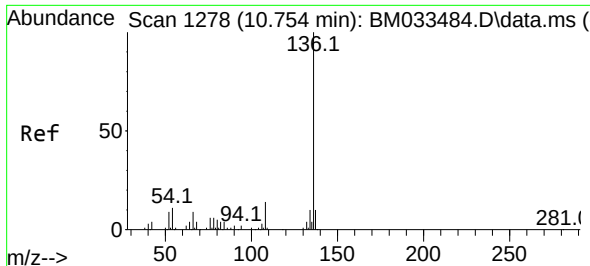

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.731 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM033544.D
Acq: 20 Dec 2021 17:32




Instrument :
BNA_M
ClientSampleId :
338


Tgt Ion:	136	Resp:	103321
Ion Ratio	Lower	Upper	
136	100		
137	10.5	8.6	13.0
54	11.5	8.3	12.5
68	4.4	5.0	7.6

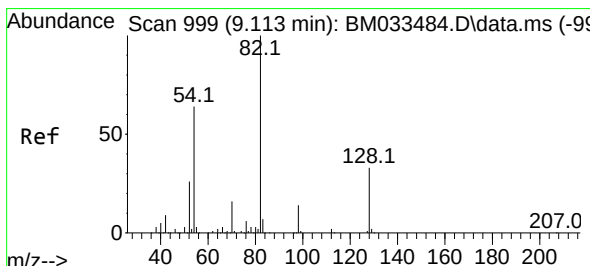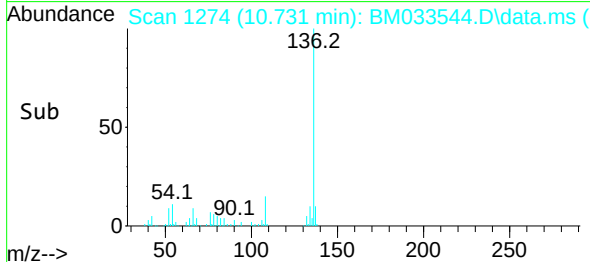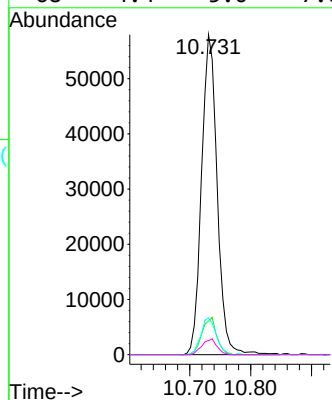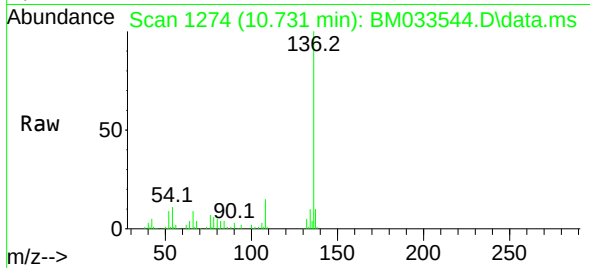

#23
Nitrobenzene-d5
Concen: 74.404 ng
RT: 9.096 min Scan# 996
Delta R.T. -0.000 min
Lab File: BM033544.D
Acq: 20 Dec 2021 17:32

Tgt Ion:	82	Resp:	179039
Ion Ratio	Lower	Upper	
82	100		
128	33.2	28.1	42.1
54	66.5	46.1	69.1


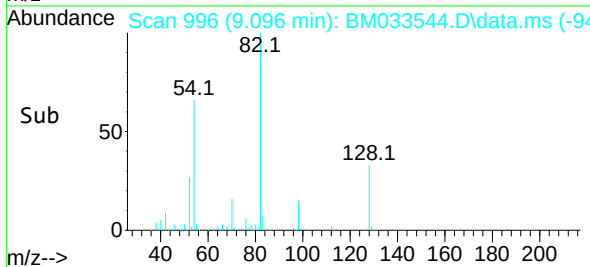
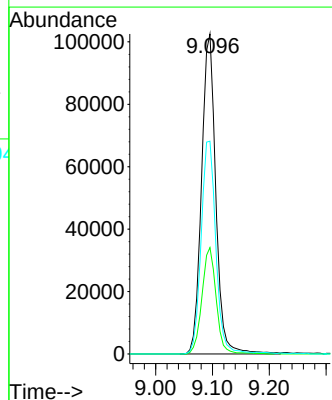
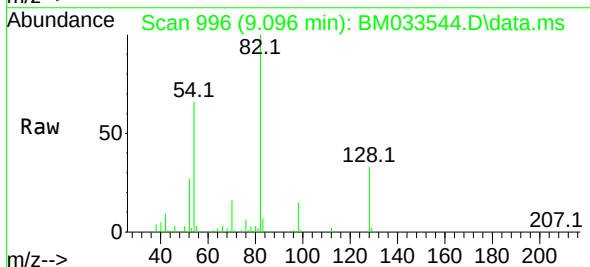


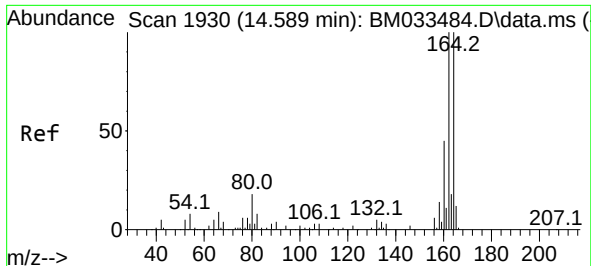

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.566 min Scan# 1926
Delta R.T. -0.000 min
Lab File: BM033544.D
Acq: 20 Dec 2021 17:32




Instrument :
BNA_M
ClientSampleId :
338


Tgt Ion:164 Resp: 66469
Ion Ratio Lower Upper
164 100
162 104.9 79.7 119.5
160 45.6 34.2 51.4

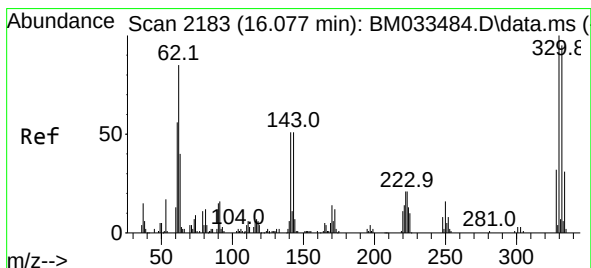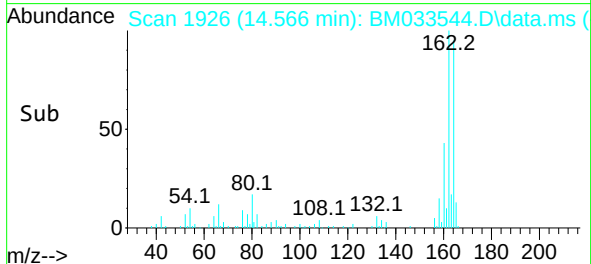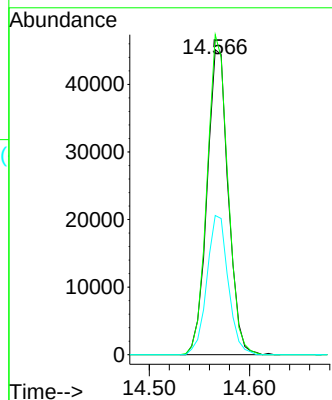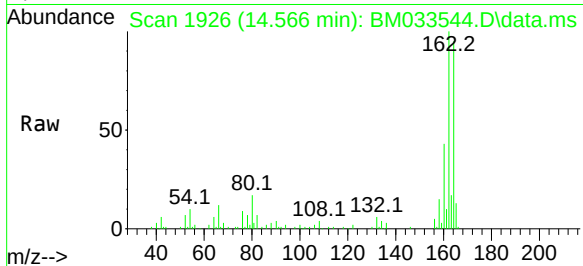

#42
2,4,6-Tribromophenol
Concen: 95.551 ng
RT: 16.060 min Scan# 2180
Delta R.T. -0.000 min
Lab File: BM033544.D
Acq: 20 Dec 2021 17:32

Tgt Ion:330 Resp: 71444
Ion Ratio Lower Upper
330 100
332 95.7 76.5 114.7
141 57.0 35.9 53.9#

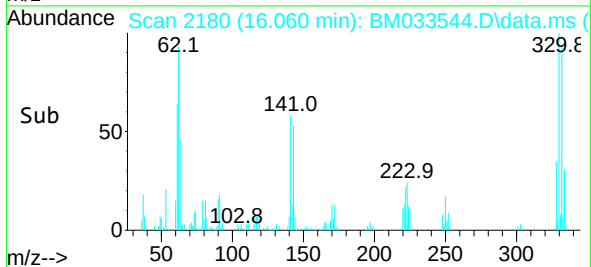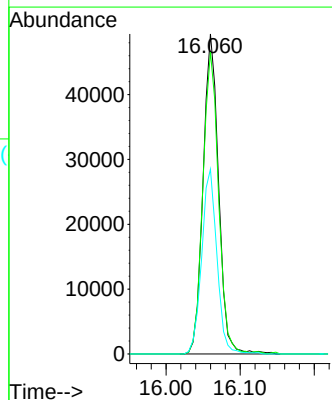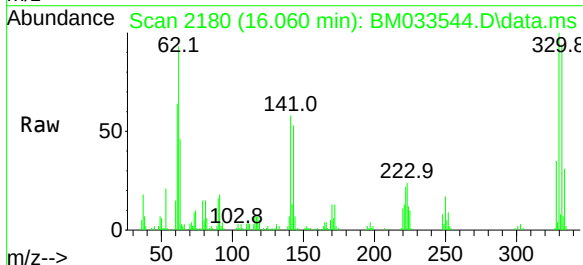

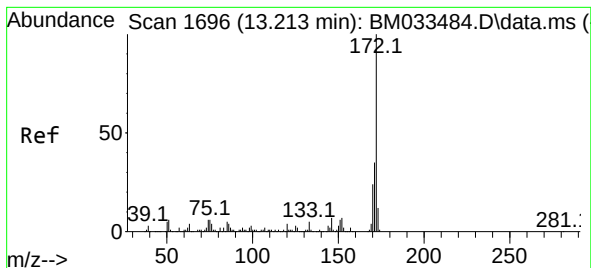

#45

2-Fluorobiphenyl

Concen: 69.415 ng

RT: 13.195 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM033544.D

Acq: 20 Dec 2021 17:32

Instrument :

BNA_M

ClientSampleId :

338





Tgt Ion:172 Resp: 333543

Ion Ratio Lower Upper

172 100

171 35.0 27.2 40.8

170 23.9 18.7 28.1

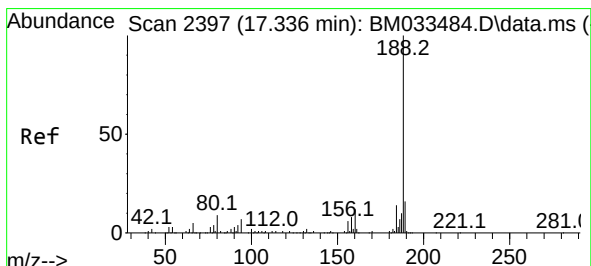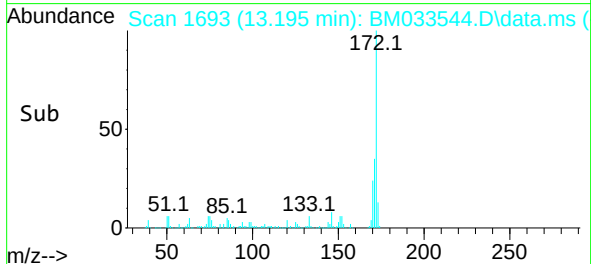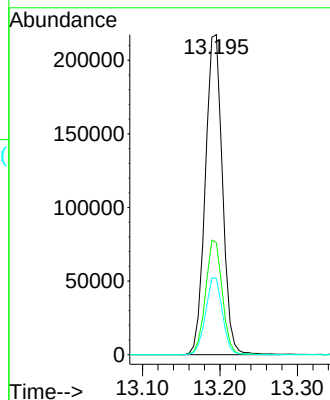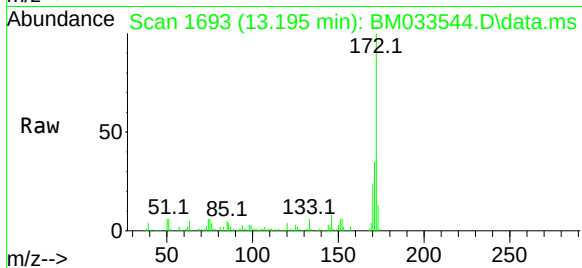

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.319 min Scan# 2394

Delta R.T. -0.000 min

Lab File: BM033544.D

Acq: 20 Dec 2021 17:32




Tgt Ion:188 Resp: 130842


Ion Ratio Lower Upper

188 100

94 7.4 7.5 11.3#

80 8.9 8.9 13.3#


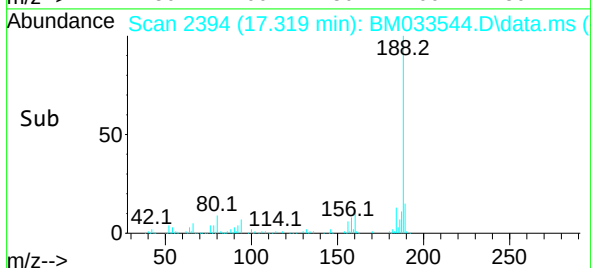
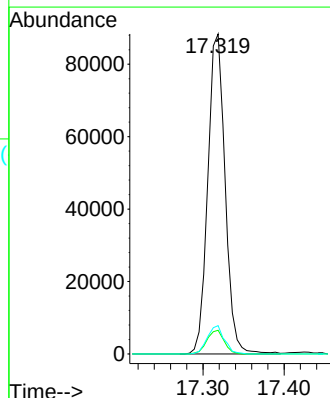
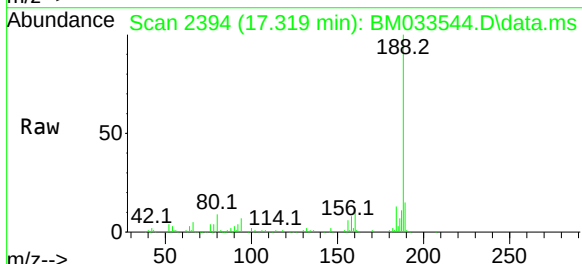


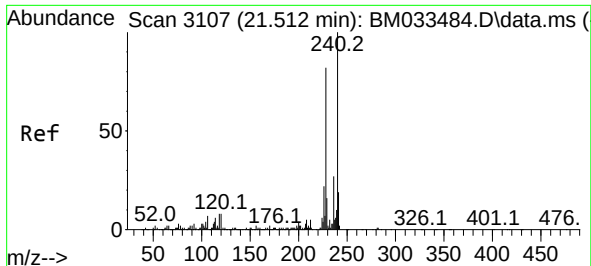

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.495 min Scan# 3107
Delta R.T. -0.000 min
Lab File: BM033544.D
Acq: 20 Dec 2021 17:32




Instrument :
BNA_M
ClientSampleId :
338


Tgt Ion:240 Resp: 111868
Ion Ratio Lower Upper
240 100
120 7.0 7.8 11.6#
236 24.6 20.3 30.5

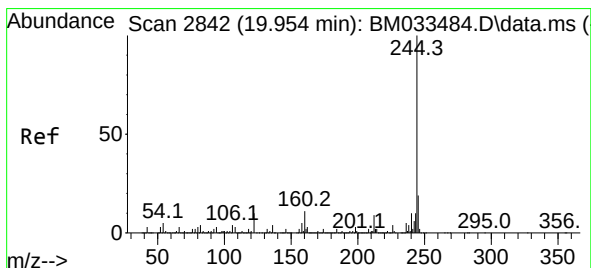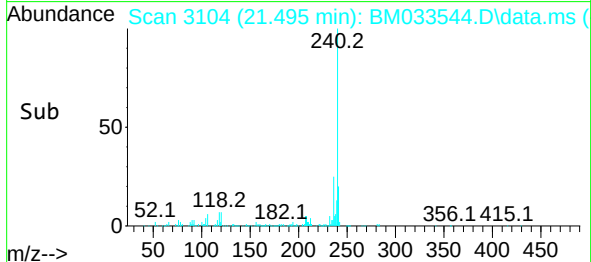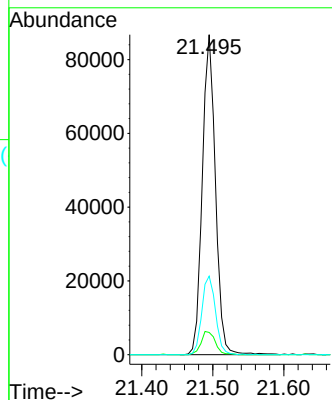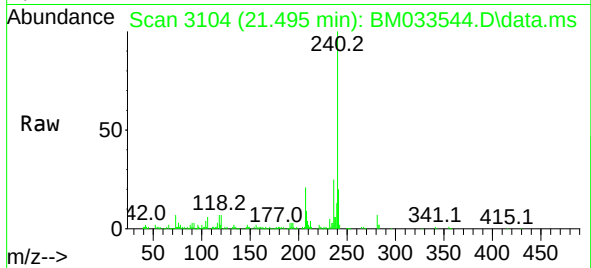

#79
Terphenyl-d14
Concen: 64.353 ng
RT: 19.936 min Scan# 2839
Delta R.T. -0.000 min
Lab File: BM033544.D
Acq: 20 Dec 2021 17:32

Tgt Ion:244 Resp: 457278
Ion Ratio Lower Upper
244 100
212 8.7 5.9 8.9
122 9.5 8.4 12.6

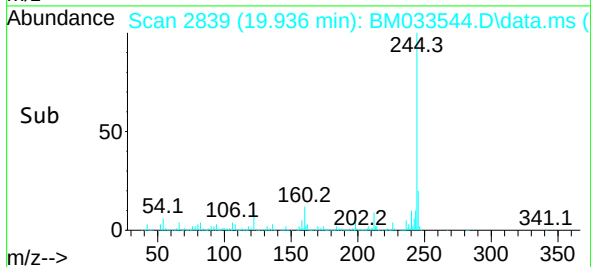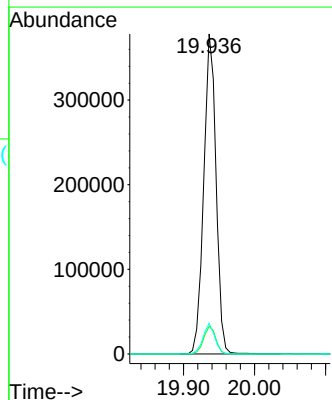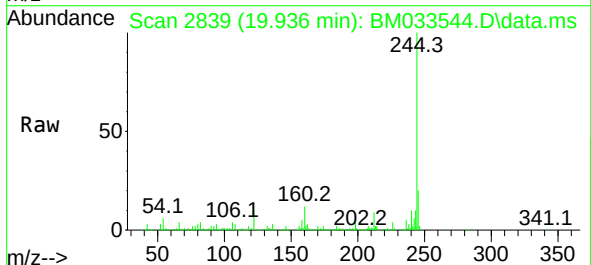

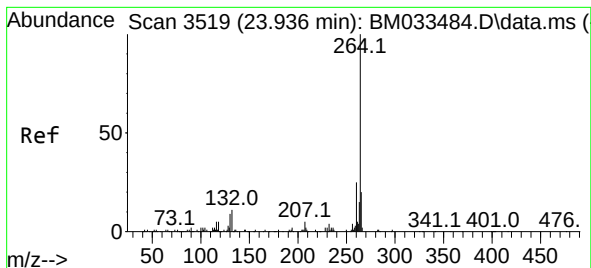

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.901 min Scan# 31

Delta R.T. -0.000 min

Lab File: BM033544.D


Acq: 20 Dec 2021 17:32

Instrument :

BNA_M

ClientSampleId :

338

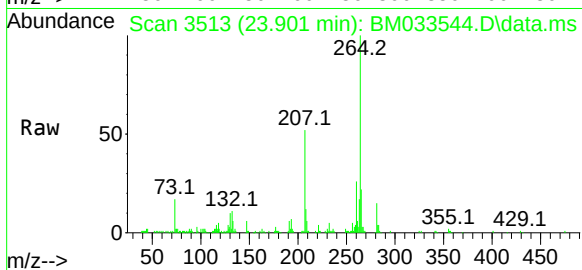

Tgt Ion:264 Resp: 114980

Ion Ratio Lower Upper

264 100

260 25.9 17.7 26.5

265 22.3 17.7 26.5

