


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122021\
 Data File : BM033534.D
 Acq On : 20 Dec 2021 10:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 21 03:57:10 2021

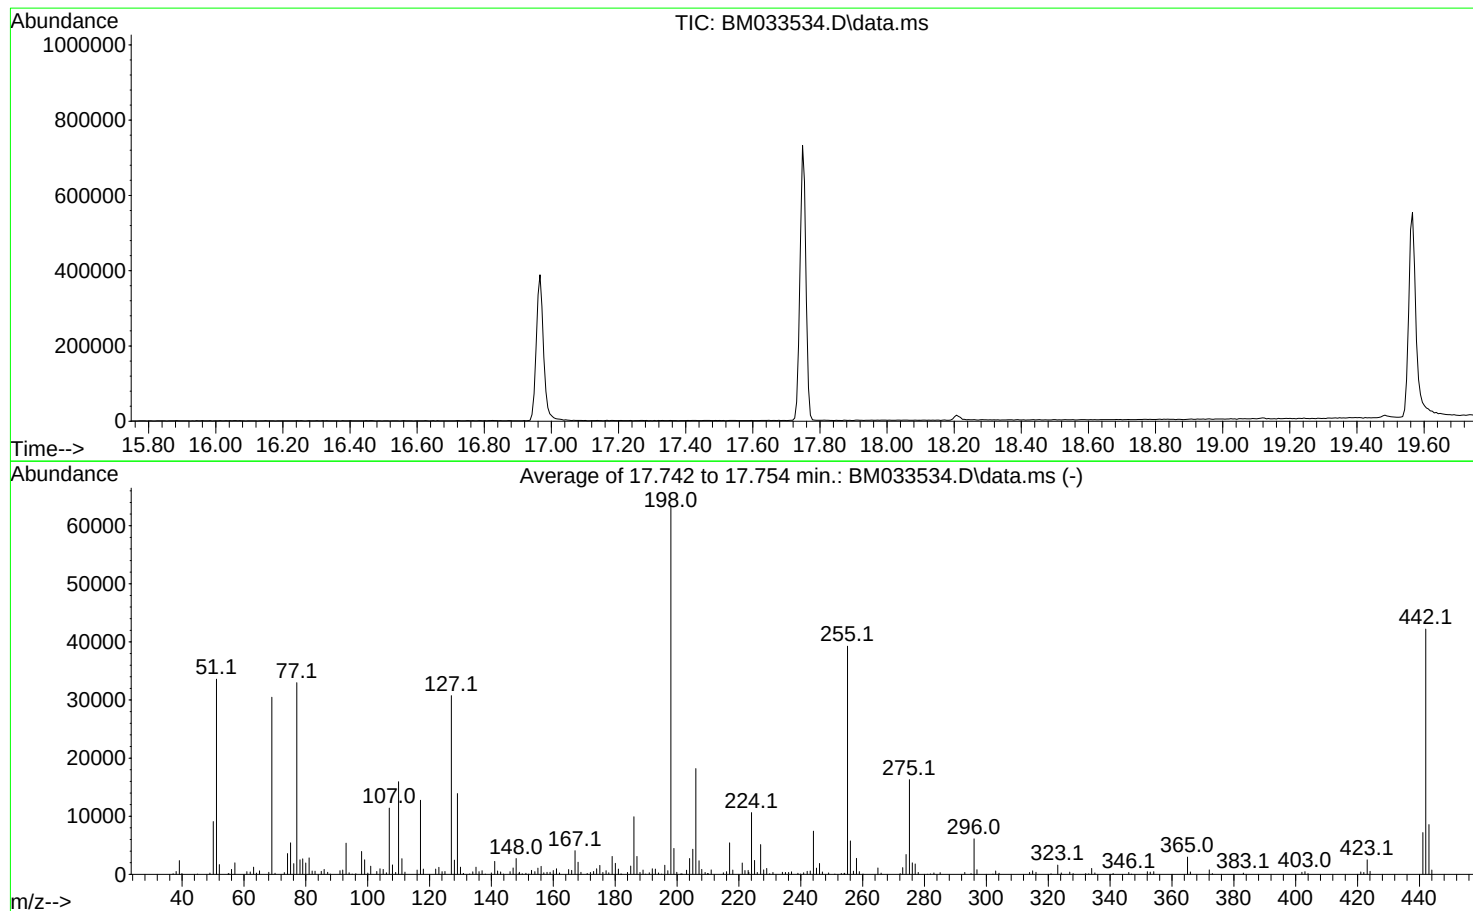




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	33589	PASS
68	69	0.00	2	1.2	364	PASS
69	198	0.00	100	48.1	30472	PASS
70	69	0.00	2	0.7	202	PASS
127	198	10	80	48.6	30757	PASS
197	198	0.00	2	1.0	628	PASS
198	198	100	100	100.0	63304	PASS
199	198	5	9	7.0	4453	PASS
275	198	10	60	25.8	16314	PASS
365	198	1	100	4.7	2976	PASS
441	198	0.01	100	11.4	7199	PASS
442	442	50	100	100.0	42208	PASS
443	442	15	24	20.3	8574	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122021\  
Data File : BM033534.D  
Acq On    : 20 Dec 2021  10:55  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 21 04:24:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 21 03:57:10 2021
Response via : Initial Calibration

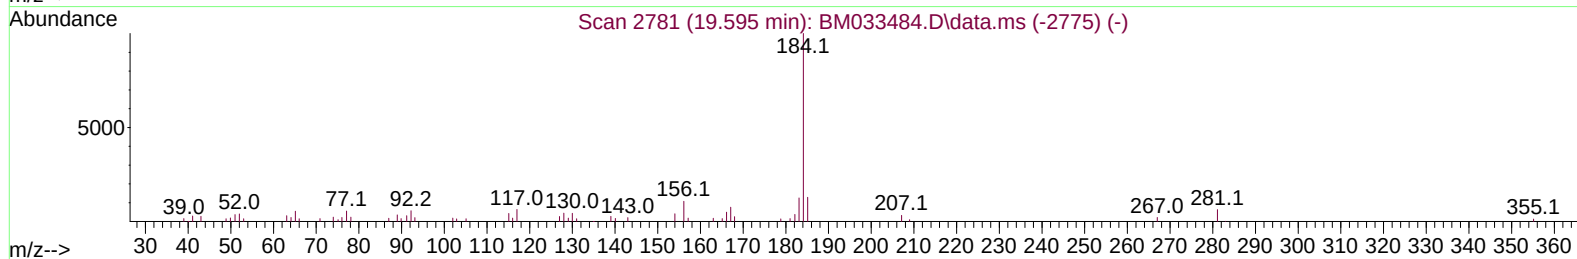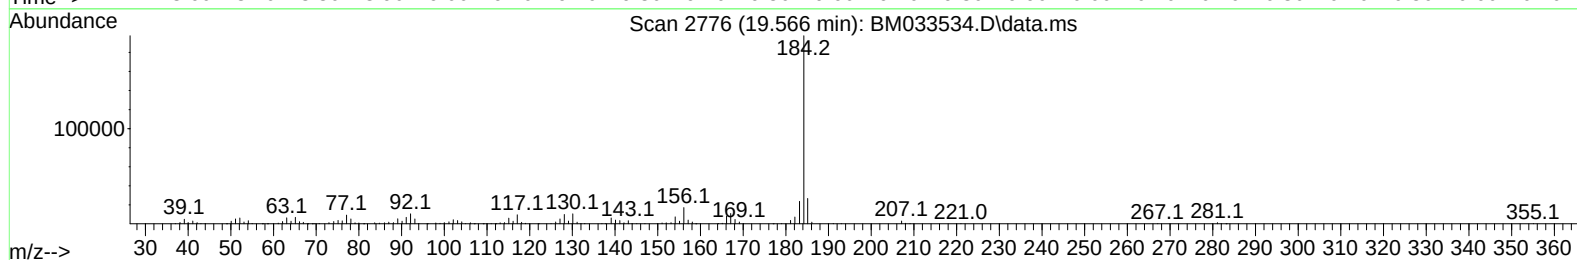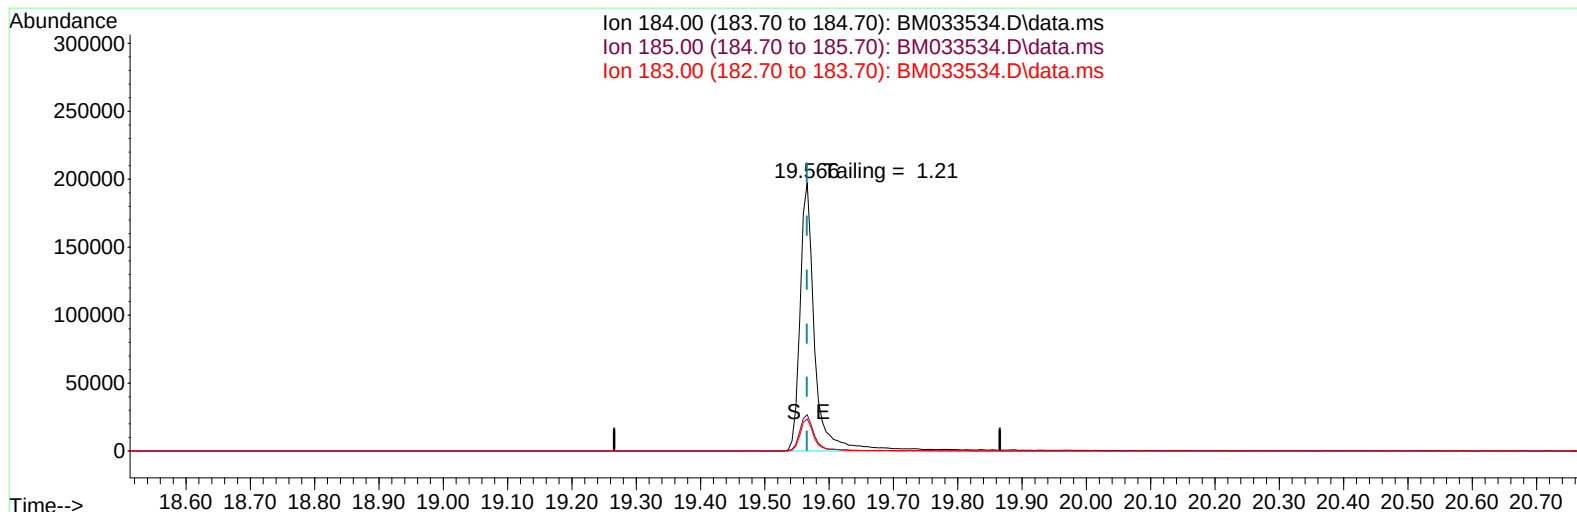

TIC: BM033534.D\data.ms

(77) Benzidine

19.566min (+ 0.000) 1185013.68 ng

response **315823**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.20	13.55
--------	-------	-------




183.00	12.10	12.03
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122021\
Data File : BM033534.D
Acq On : 20 Dec 2021 10:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 21 04:24:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 21 03:57:10 2021
Response via : Initial Calibration

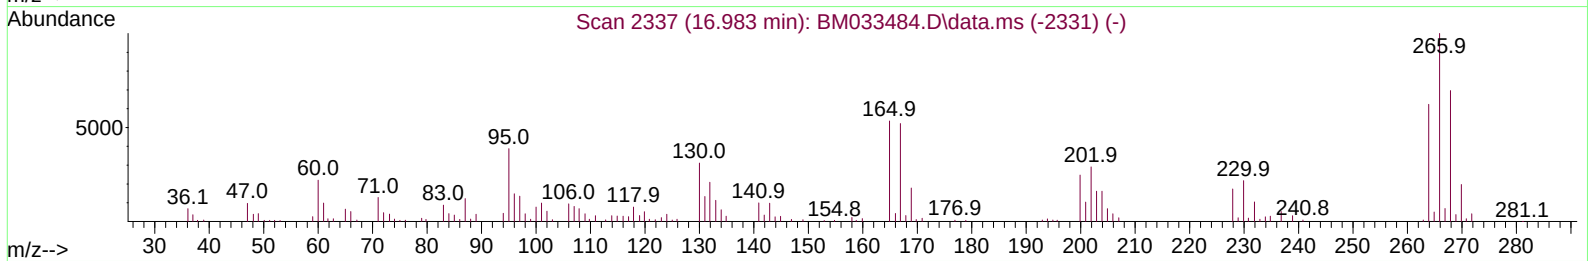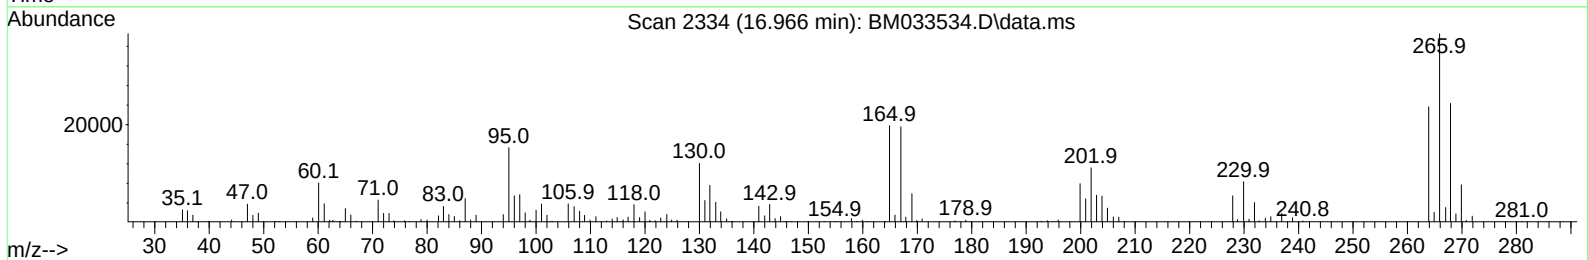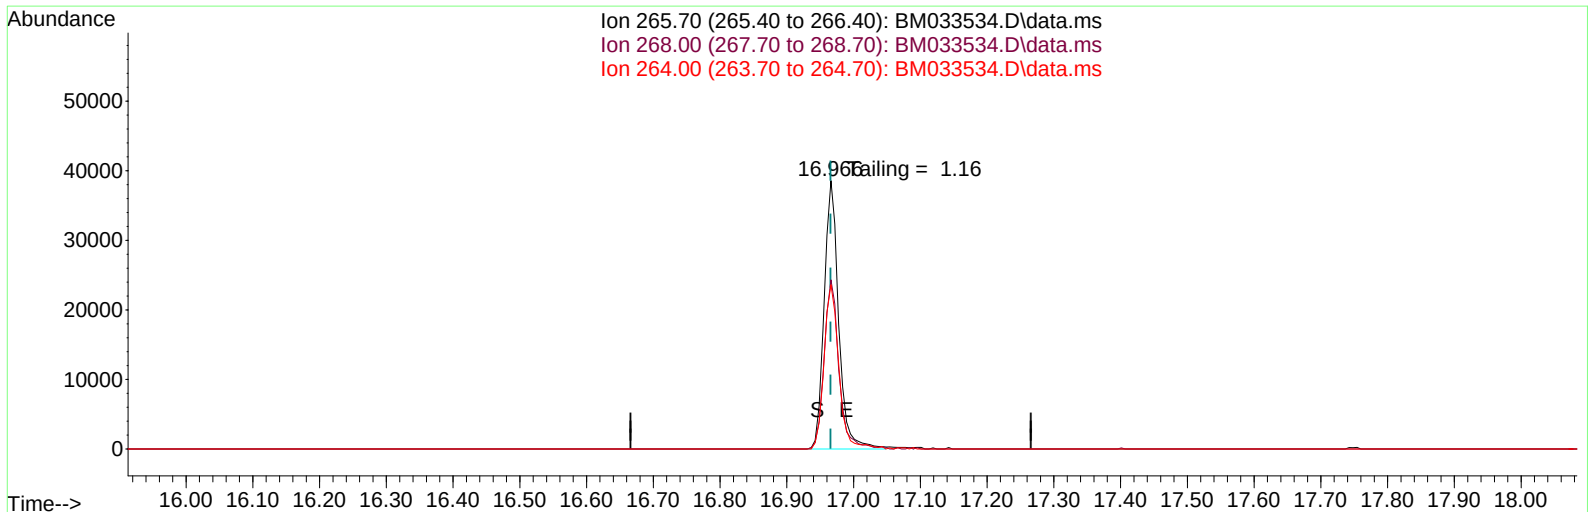

TIC: BM033534.D\data.ms

(70) Pentachlorophenol (C)

16.966min (+ 0.000) 0.00 ng

response 58895

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.01
264.00	61.40	61.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/20/2021	BNA_M	<u>BM033534.D</u>
Compound Name	Response	Retention Time
DDT	202793	20.789
DDD	2310	20.348
DDE	68	19.842
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2378	205171	1.16