

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038137.D
 Acq On : 20 Dec 2022 16:45
 Operator : CG/JU
 Sample : N6008-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBYB0

Quant Time: Dec 21 00:15:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 00:11:56 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.045	152	187413	20.000	ng/ul	0.00
20) Naphthalene-d8	10.863	136	803802	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.674	164	510809	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.409	188	1174960	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	1215425	20.000	ng/ul	0.00
88) Perylene-d12	24.032	264	1242469	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	19159	4.642	ng/uL	0.00
4) Pyridine-d5	3.840	84	144301	11.785	ng/ul	0.00
7) Phenol-d5	7.204	99	413877	27.176	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	242765	26.179	ng/ul	0.00
11) 2-Chlorophenol-d4	7.575	132	350779	28.078	ng/ul	0.00
15) 4-Methylphenol-d8	8.757	113	324525	27.299	ng/ul	0.00
21) Nitrobenzene-d5	9.216	128	187236	29.420	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	215517	32.314	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.480	165	399605	31.545	ng/ul	0.00
31) 4-Chloroaniline-d4	11.004	131	425008	24.305	ng/ul	0.00
46) Dimethylphthalate-d6	14.080	166	1319356	36.229	ng/ul	0.00
49) Acenaphthylene-d8	14.368	160	1553267	34.898	ng/ul	0.00
54) 4-Nitrophenol-d4	14.868	143	225949	36.406	ng/ul	0.00
60) Fluorene-d10	15.662	176	1230651	37.930	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.780	200	203533	32.400	ng/ul	0.00
73) Anthracene-d10	17.509	188	1998569	36.446	ng/ul	0.00
81) Pyrene-d10	19.797	212	2662736	36.470	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	2311723	37.251	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.875	105	22143	1.184	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038137.D
Acq On : 20 Dec 2022 16:45
Operator : CG/JU
Sample : N6008-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBYB0


Quant Time: Dec 21 00:15:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 21 00:11:56 2022
Response via : Initial Calibration

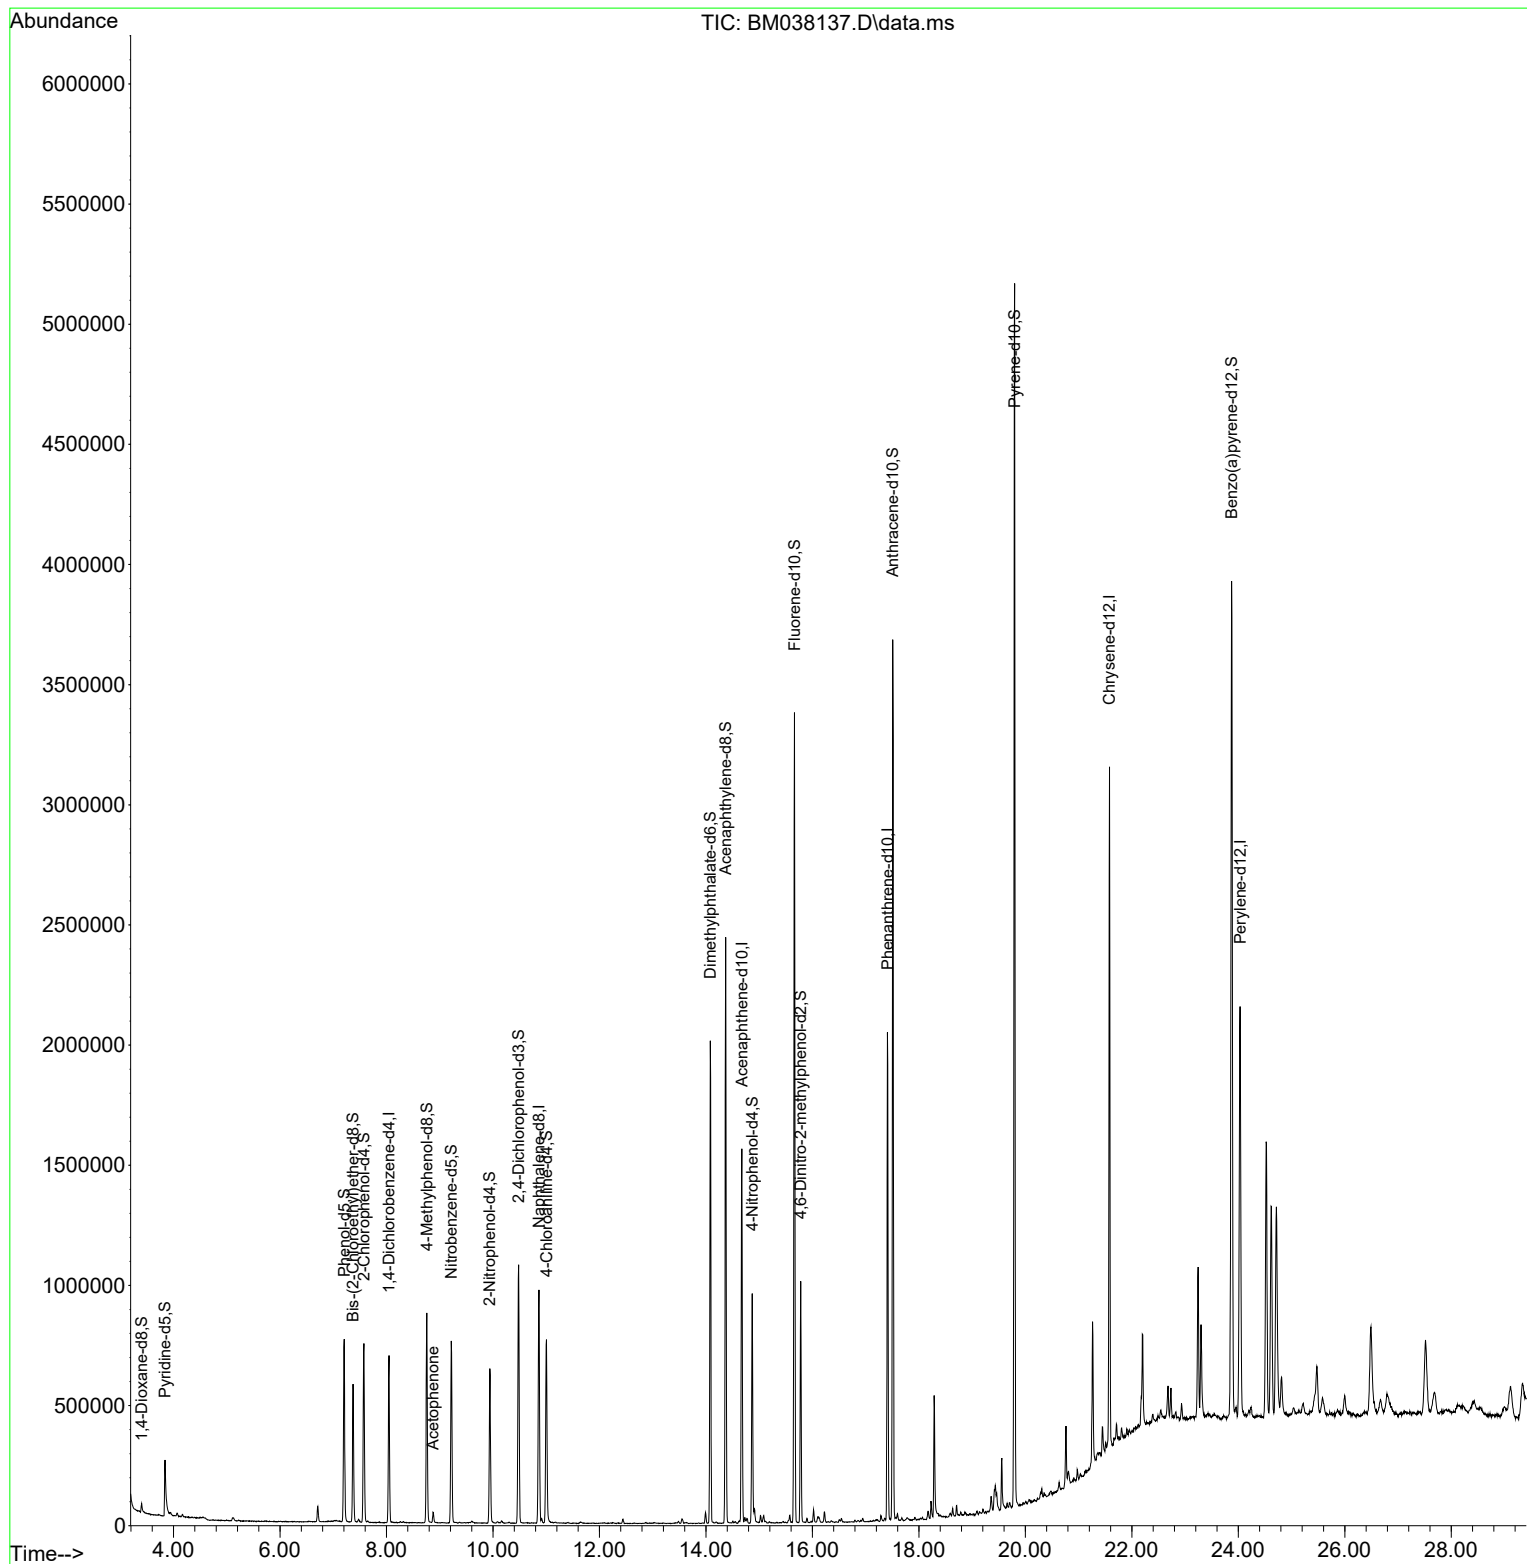

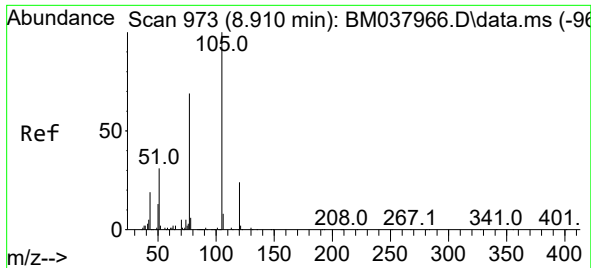

#16
 Acetophenone
 Concen: 1.184 ng/ul
 RT: 8.875 min Scan# 90
 Delta R.T. -0.000 min
 Lab File: BM038137.D
 Acq: 20 Dec 2022 16:45

Instrument :
 BNA_M
 ClientSampleId :
 DBYB0

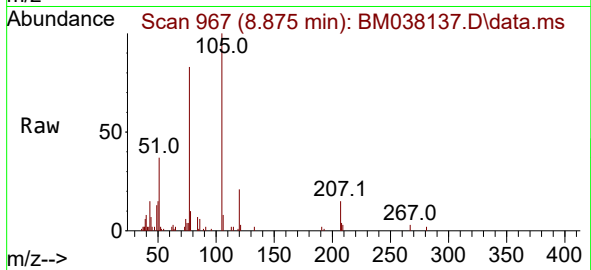

Tgt Ion:	105	Resp:	22143
Ion Ratio	Lower	Upper	
105	100		
77	82.7	59.7	89.5
51	36.9	27.2	40.8

