

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038141.D
 Acq On : 20 Dec 2022 19:13
 Operator : CG/JU
 Sample : N6008-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXW8

Quant Time: Dec 21 00:16:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 00:11:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.045	152	148813	20.000	ng/ul	0.00
20) Naphthalene-d8	10.863	136	660072	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.674	164	412387	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.410	188	903362	20.000	ng/ul	0.00
79) Chrysene-d12	21.574	240	775015	20.000	ng/ul	0.00
88) Perylene-d12	24.027	264	709702	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	15905	4.853	ng/uL	0.00
4) Pyridine-d5	3.834	84	209877	21.587	ng/ul	0.00
7) Phenol-d5	7.204	99	331135	27.383	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	184343	25.035	ng/ul	0.00
11) 2-Chlorophenol-d4	7.575	132	291086	29.343	ng/ul	0.00
15) 4-Methylphenol-d8	8.757	113	255265	27.043	ng/ul	0.00
21) Nitrobenzene-d5	9.216	128	142922	27.347	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	165135	30.152	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	304732	29.294	ng/ul	0.00
31) 4-Chloroaniline-d4	10.998	131	326856	22.762	ng/ul	0.00
46) Dimethylphthalate-d6	14.080	166	885152	30.107	ng/ul	0.00
49) Acenaphthylene-d8	14.369	160	1052805	29.299	ng/ul	0.00
54) 4-Nitrophenol-d4	14.868	143	139656	27.872	ng/ul	0.00
60) Fluorene-d10	15.657	176	794108	30.317	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.780	200	118465	24.528	ng/ul	0.00
73) Anthracene-d10	17.509	188	1217196	28.870	ng/ul	0.00
81) Pyrene-d10	19.792	212	1424343	30.595	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	1064779	30.038	ng/ul	0.00


Target Compounds					Qvalue
10) Bis(2-Chloroethyl)ether	7.469	93	24428	2.453 ng/ul#	21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038141.D
Acq On : 20 Dec 2022 19:13
Operator : CG/JU
Sample : N6008-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXW8

Quant Time: Dec 21 00:16:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 21 00:11:56 2022
Response via : Initial Calibration

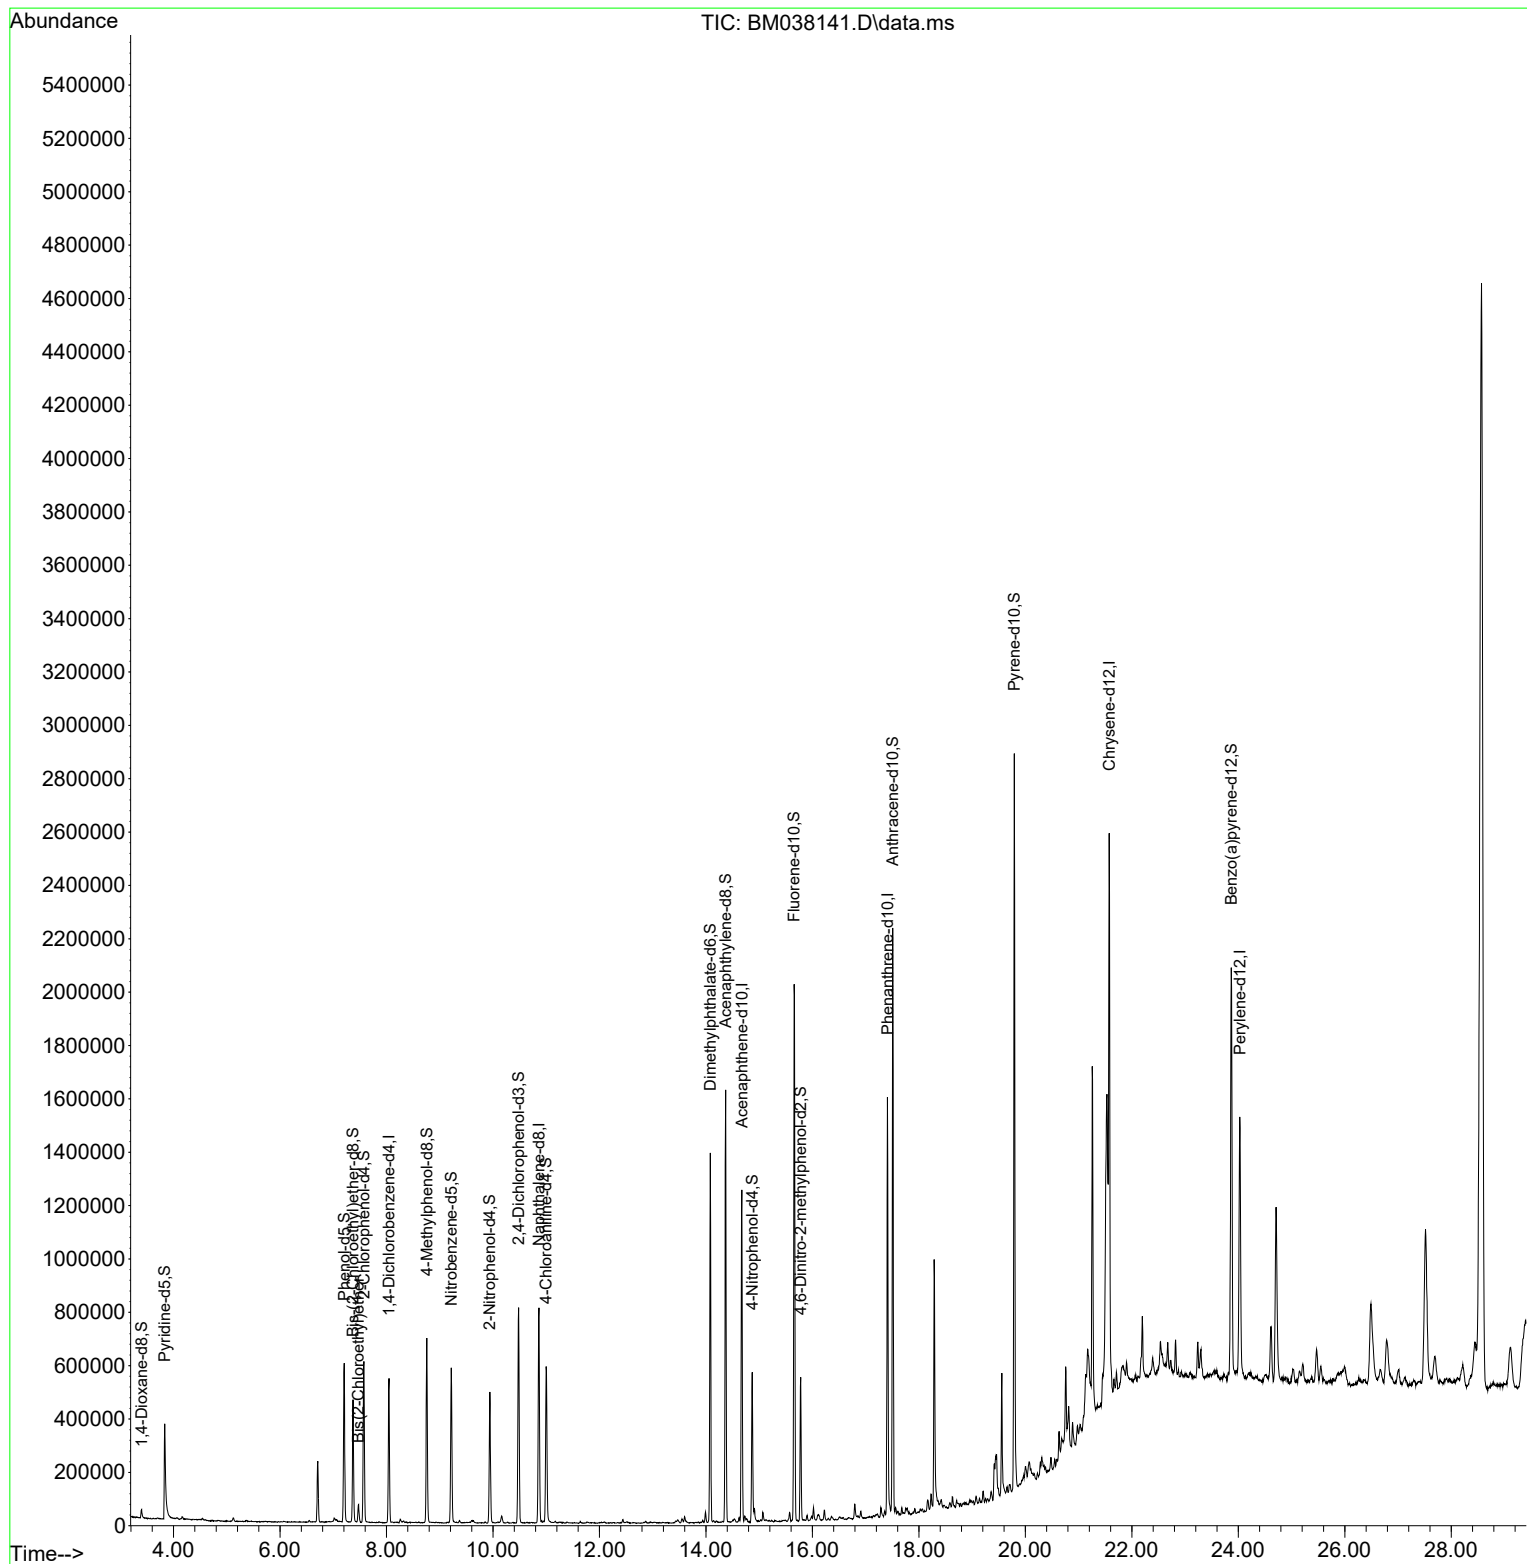

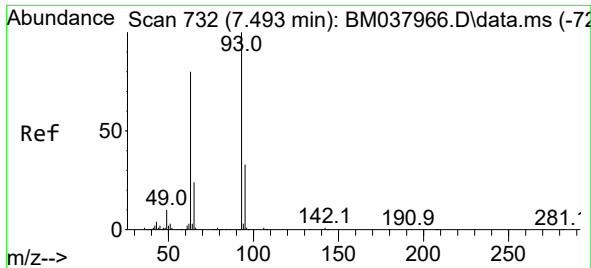

#10
 Bis(2-Chloroethyl)ether
 Concen: 2.453 ng/ul
 RT: 7.469 min Scan# 71
 Delta R.T. 0.006 min
 Lab File: BM038141.D
 Acq: 20 Dec 2022 19:13

Instrument :
 BNA_M
 ClientSampleId :
 DBXW8

Tgt Ion: 93 Resp: 24428
 Ion Ratio Lower Upper
 93 100
 63 2.5 66.3 99.5#
 95 2.5 25.7 38.5#

