

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038147.D
 Acq On : 20 Dec 2022 22:53
 Operator : CG/JU
 Sample : N6008-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXX9

Quant Time: Dec 21 00:17:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 00:11:56 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.045	152	177341	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	765203	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.674	164	485289	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.409	188	1033714	20.000	ng/ul	0.00
79) Chrysene-d12	21.574	240	840490	20.000	ng/ul	0.00
88) Perylene-d12	24.027	264	761806	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	14594	3.737	ng/uL	0.00
4) Pyridine-d5	3.834	84	225600	19.471	ng/ul	0.00
7) Phenol-d5	7.204	99	370975	25.743	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	208149	23.721	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132	313734	26.539	ng/ul	0.00
15) 4-Methylphenol-d8	8.757	113	323679	28.774	ng/ul	0.00
21) Nitrobenzene-d5	9.216	128	168962	27.888	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	196452	30.942	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.480	165	372899	30.922	ng/ul	0.00
31) 4-Chloroaniline-d4	10.998	131	445385	26.755	ng/ul	0.00
46) Dimethylphthalate-d6	14.080	166	1199461	34.669	ng/ul	0.00
49) Acenaphthylene-d8	14.368	160	1375176	32.522	ng/ul	0.00
54) 4-Nitrophenol-d4	14.868	143	193350	32.791	ng/ul	0.00
60) Fluorene-d10	15.657	176	1059140	34.361	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.780	200	158592	28.696	ng/ul	0.00
73) Anthracene-d10	17.509	188	1620623	33.592	ng/ul	0.00
81) Pyrene-d10	19.792	212	1868277	37.004	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	1341335	35.251	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.468	149	75864	2.261	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038147.D
Acq On : 20 Dec 2022 22:53
Operator : CG/JU
Sample : N6008-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXX9

Quant Time: Dec 21 00:17:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 21 00:11:56 2022
Response via : Initial Calibration

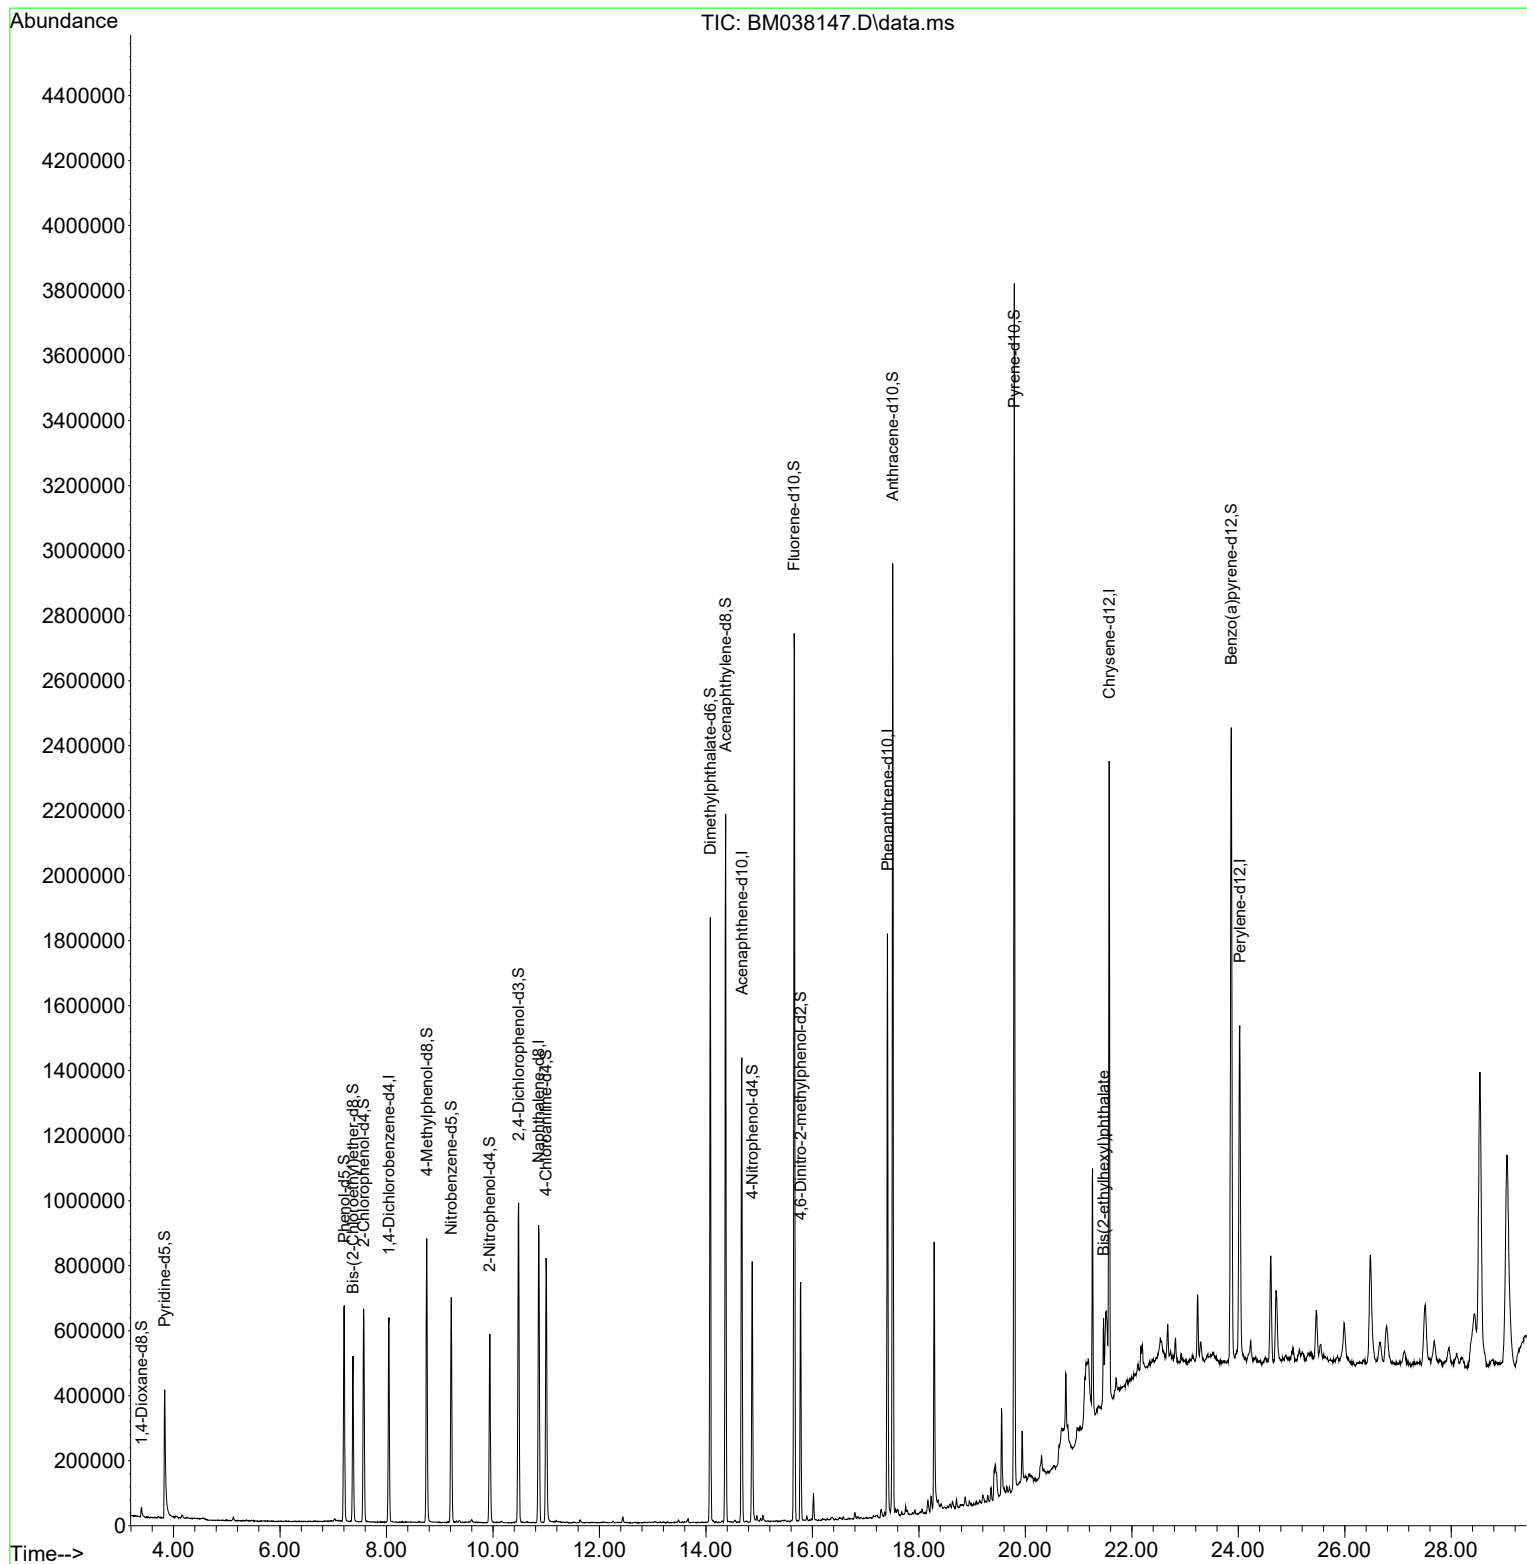

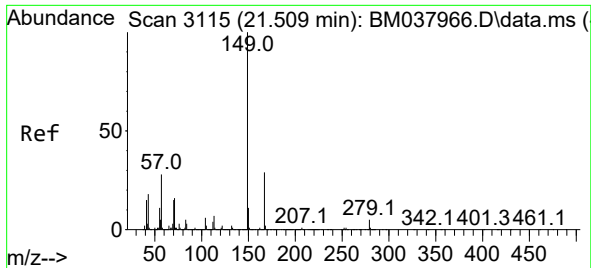

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.261 ng/ul
 RT: 21.468 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BM038147.D
 Acq: 20 Dec 2022 22:53

Instrument :
 BNA_M
 ClientSampleId :
 DBXX9

Tgt Ion:149 Resp: 75864
 Ion Ratio Lower Upper
 149 100
 167 26.5 21.5 32.3
 279 4.3 3.2 4.8

