

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038166.D
 Acq On : 21 Dec 2022 11:33
 Operator : CG/JU
 Sample : N6014-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 21 23:30:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 00:11:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	186594	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	786340	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.668	164	470080	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.409	188	952963	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.574	240	670942	20.000	ng/ul	0.00
88) Perylene-d12	24.027	264	698558	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	16688	4.061	ng/uL	0.00
4) Pyridine-d5	3.834	84	169318	13.889	ng/ul	0.00
7) Phenol-d5	7.198	99	343846	22.677	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	200879	21.757	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132	302080	24.286	ng/ul	0.00
15) 4-Methylphenol-d8	8.751	113	280743	23.720	ng/ul	0.00
21) Nitrobenzene-d5	9.216	128	152972	24.570	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	172765	26.479	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.475	165	315890	25.490	ng/ul	0.00
31) 4-Chloroaniline-d4	10.998	131	365937	21.392	ng/ul	0.00
46) Dimethylphthalate-d6	14.080	166	885533	26.423	ng/ul	0.00
49) Acenaphthylene-d8	14.368	160	1055276	25.764	ng/ul	0.00
54) 4-Nitrophenol-d4	14.868	143	120603	21.116	ng/ul	0.00
60) Fluorene-d10	15.657	176	779374	26.103	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.774	200	77639	15.238	ng/ul	0.00
73) Anthracene-d10	17.504	188	1138898	25.607	ng/ul	0.00
81) Pyrene-d10	19.792	212	1137914	28.234	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	899149	25.770	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.468	149	29842	1.114	ng/ul	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038166.D
Acq On : 21 Dec 2022 11:33
Operator : CG/JU
Sample : N6014-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 21 23:30:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 21 00:11:56 2022
Response via : Initial Calibration

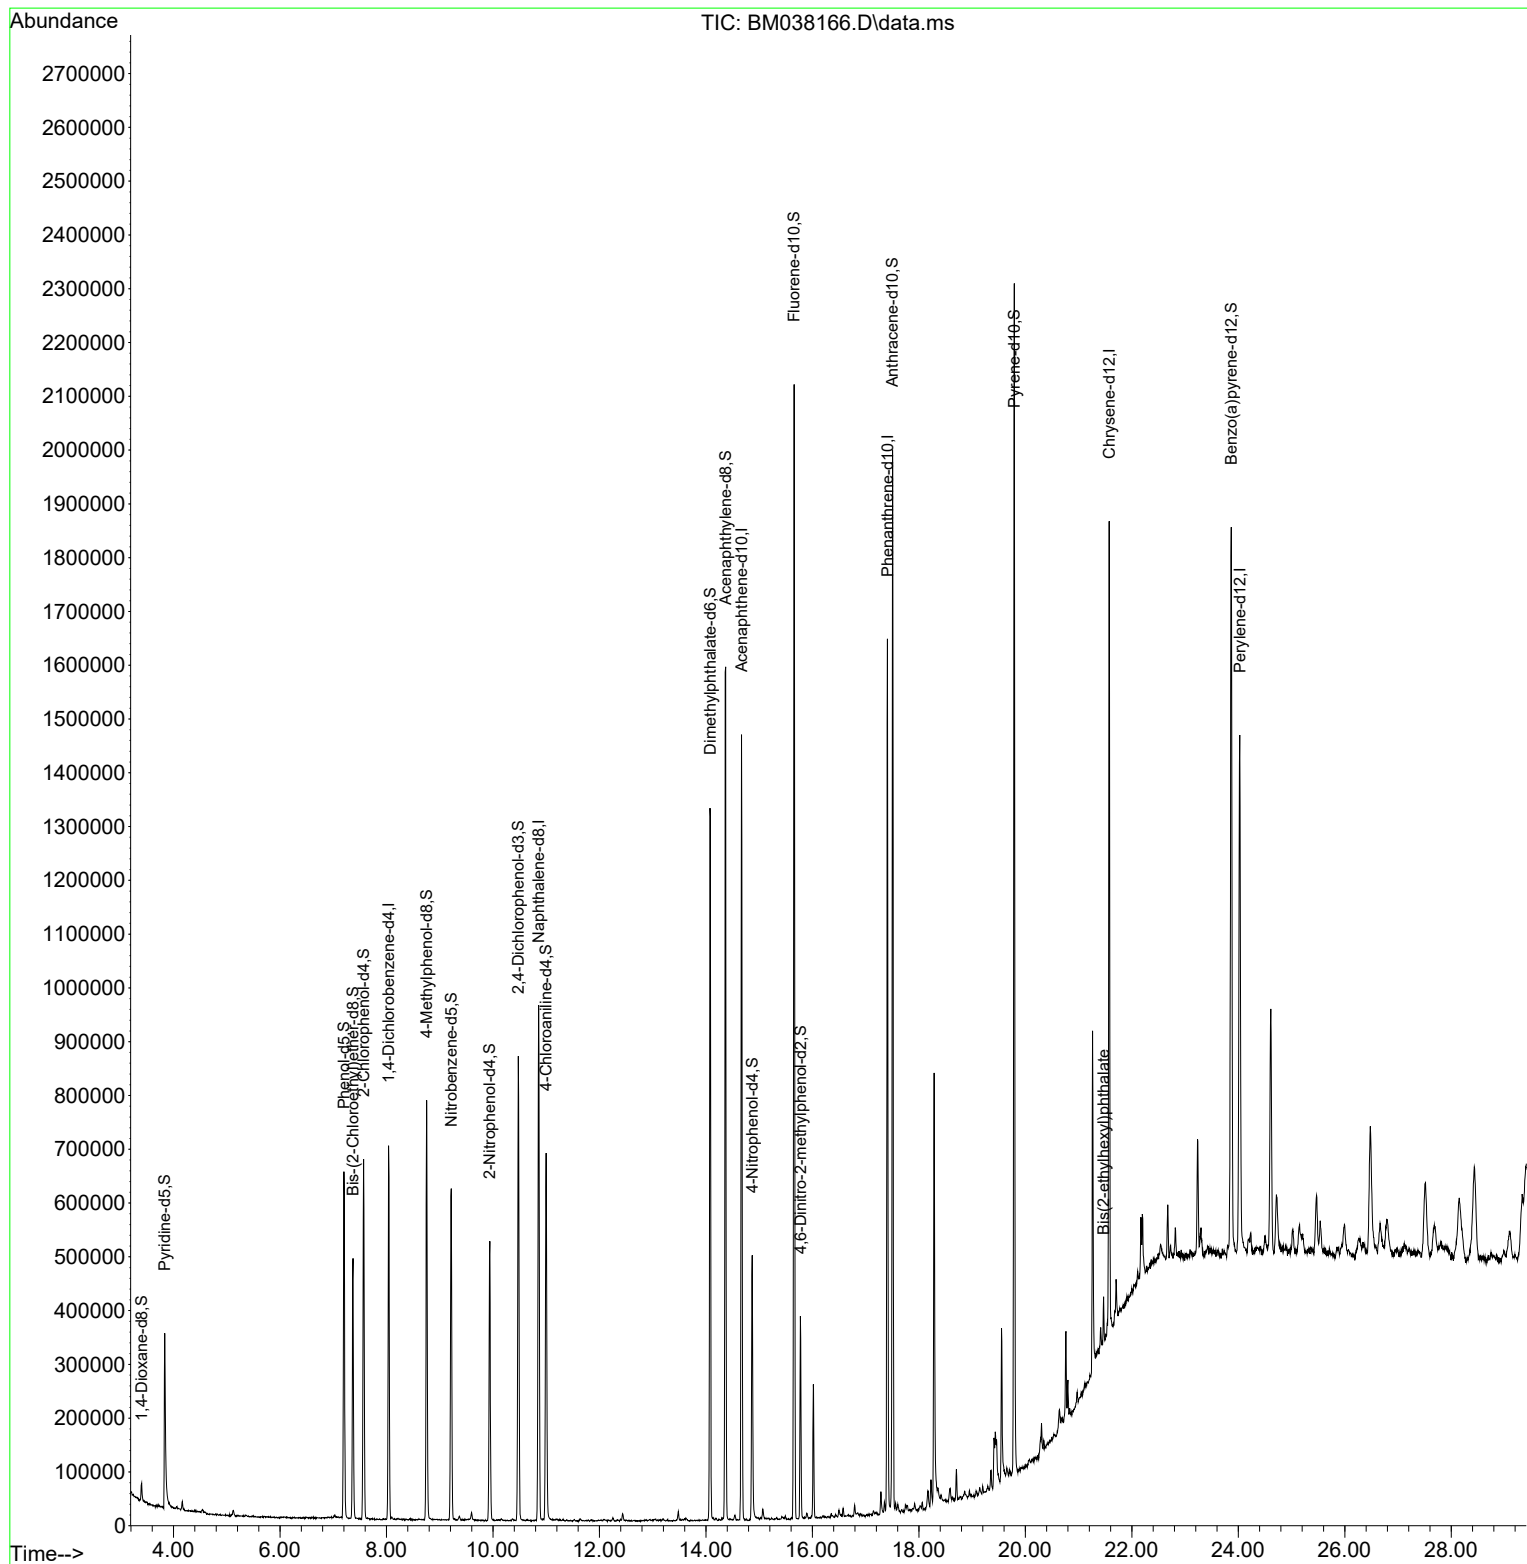

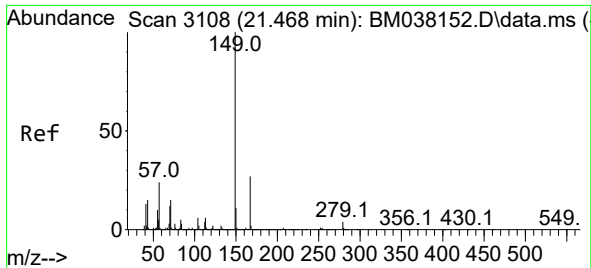

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.114 ng/ul
 RT: 21.468 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BM038166.D
 Acq: 21 Dec 2022 11:33

Instrument :
 BNA_M
 ClientSampleId :

Tgt Ion:149 Resp: 29842
 Ion Ratio Lower Upper
 149 100
 167 24.2 21.5 32.3
 279 4.1 3.2 4.8

