

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038172.D
 Acq On : 21 Dec 2022 15:12
 Operator : CG/JU
 Sample : N6014-12
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 21 23:32:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 00:11:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.039	152	169391	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	704719	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.668	164	427594	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.409	188	882757	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.574	240	630546	20.000	ng/ul	0.00
88) Perylene-d12	24.027	264	628747	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	23995	6.432	ng/uL	0.00
4) Pyridine-d5	3.828	84	340787	30.793	ng/ul	0.00
7) Phenol-d5	7.204	99	492503	35.780	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	274388	32.737	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132	439221	38.898	ng/ul	0.00
15) 4-Methylphenol-d8	8.757	113	399286	37.161	ng/ul	0.00
21) Nitrobenzene-d5	9.216	128	221551	39.707	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	254618	43.545	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.480	165	465194	41.886	ng/ul	0.00
31) 4-Chloroaniline-d4	10.998	131	551275	35.959	ng/ul	0.00
46) Dimethylphthalate-d6	14.080	166	1296958	42.545	ng/ul	0.00
49) Acenaphthylene-d8	14.368	160	1535517	41.213	ng/ul	0.00
54) 4-Nitrophenol-d4	14.868	143	197517	38.018	ng/ul	0.00
60) Fluorene-d10	15.657	176	1141461	42.028	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.780	200	94054	19.928	ng/ul	0.00
73) Anthracene-d10	17.509	188	1708459	41.468	ng/ul	0.00
81) Pyrene-d10	19.792	212	1778021	46.942	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	1291810	41.134	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.757	70	9469	1.189 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038172.D
Acq On : 21 Dec 2022 15:12
Operator : CG/JU
Sample : N6014-12
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Dec 21 23:32:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 21 00:11:56 2022
Response via : Initial Calibration

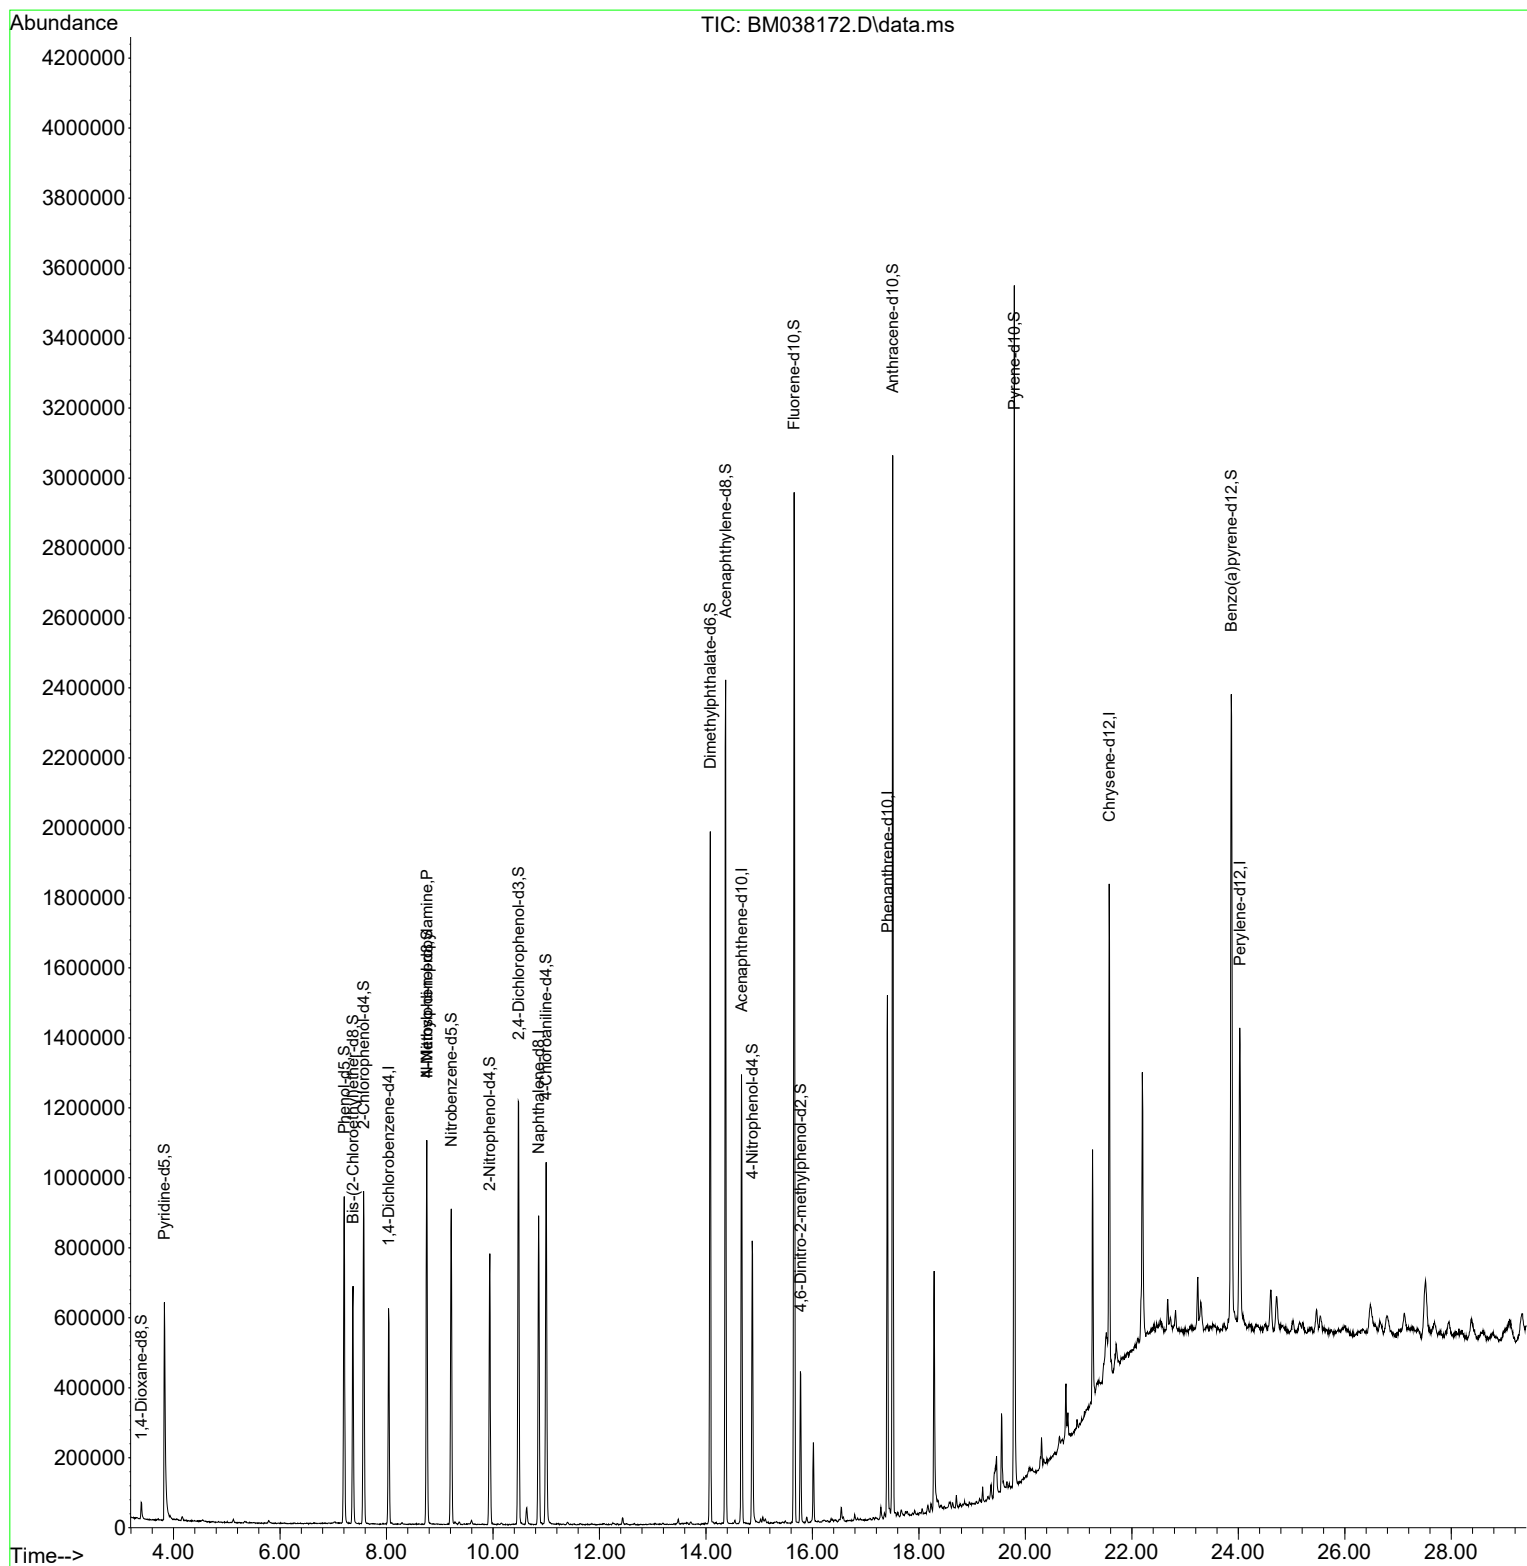

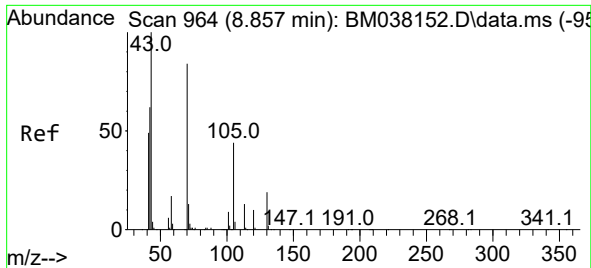

#17
N-Nitroso-di-n-propylamine
Concen: 1.189 ng/ul
RT: 8.757 min Scan# 947
Delta R.T. -0.100 min
Lab File: BM038172.D
Acq: 21 Dec 2022 15:12

Instrument :
BNA_M
ClientSampleId :

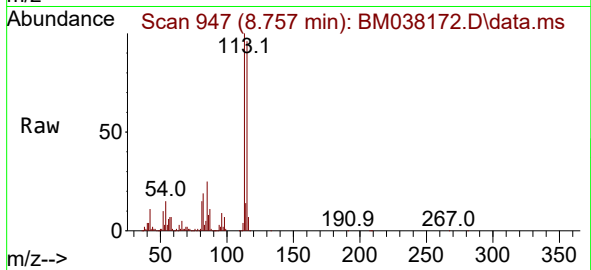

Tgt Ion: 70 Resp: 9469

Ion	Ratio	Lower	Upper
70	100		
42	485.1	62.3	93.5#
101	0.0	8.0	12.0#
130	0.0	17.6	26.4#

