




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038149.D
 Acq On : 21 Dec 2022 00:06
 Operator : CG/JU
 Sample : N6008-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXW9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 01:31:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 00:11:56 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/21/2022
 Supervised By :mohammad ahmed 12/21/2022

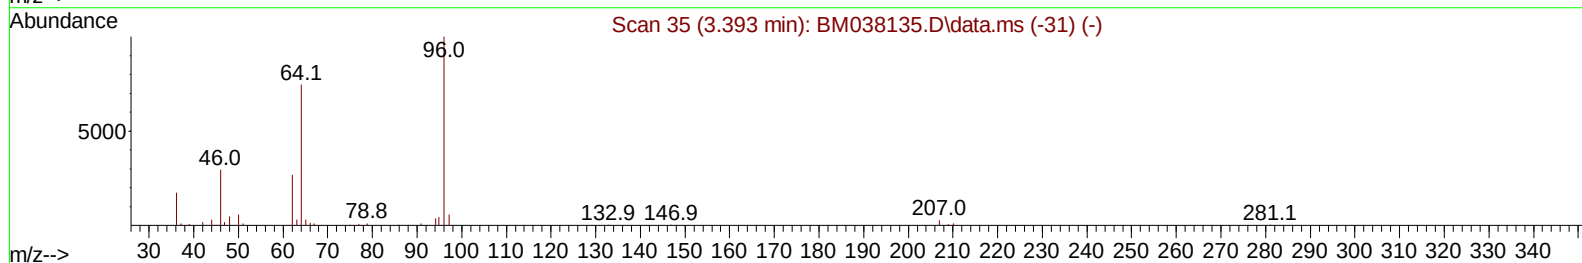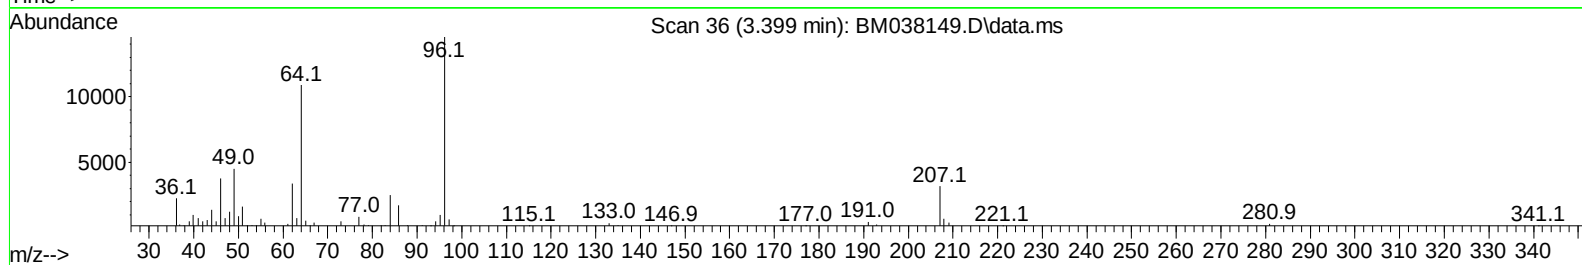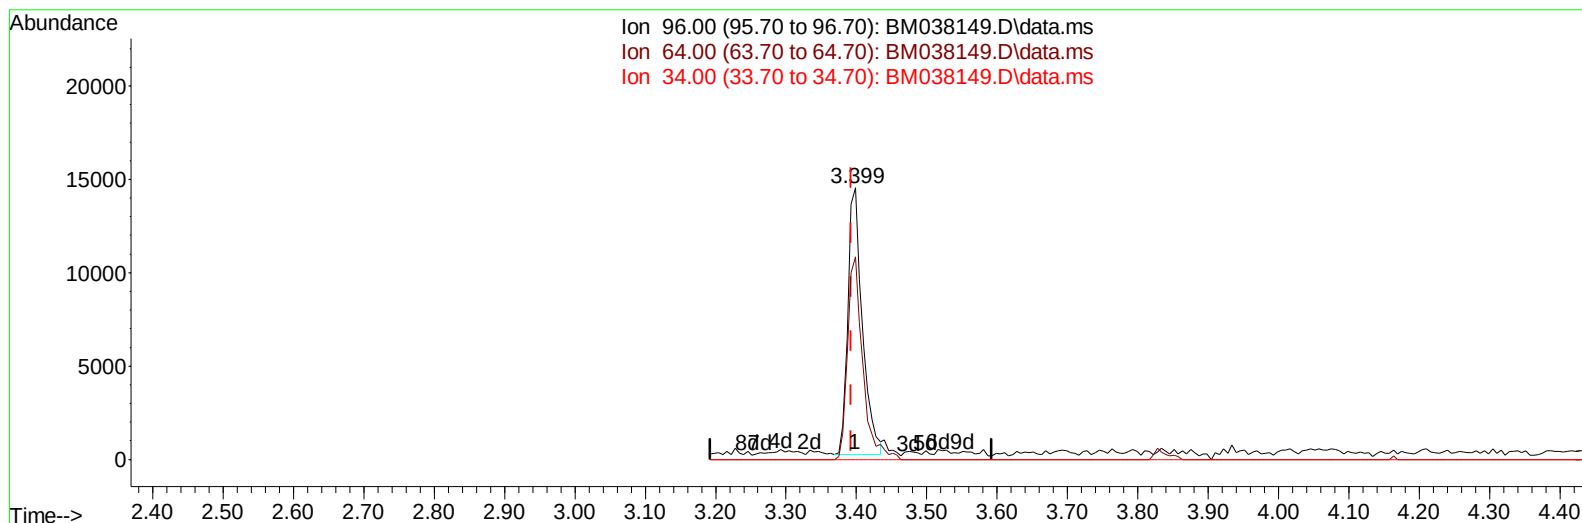

TIC: BM038149.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.399min (+ 0.006) 5.21 ng/uL

response 20240

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	74.70
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038149.D
 Acq On : 21 Dec 2022 00:06
 Operator : CG/JU
 Sample : N6008-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXW9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 01:31:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 00:11:56 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/21/2022
 Supervised By :mohammad ahmed 12/21/2022

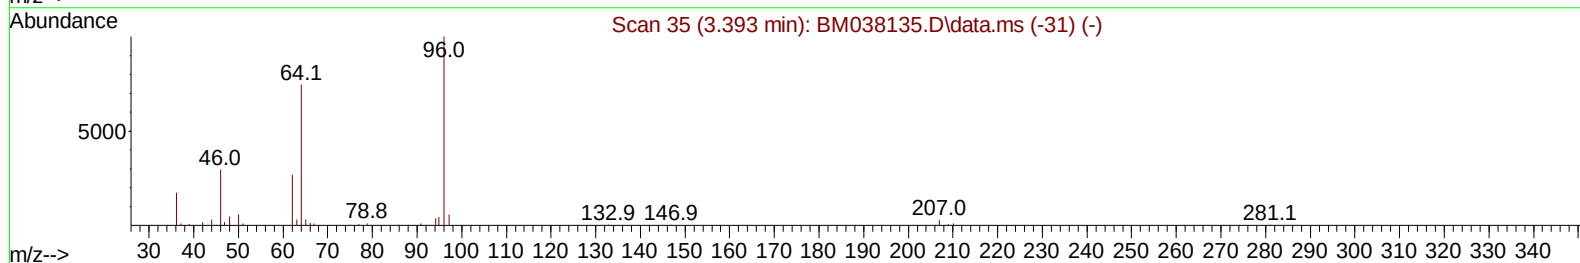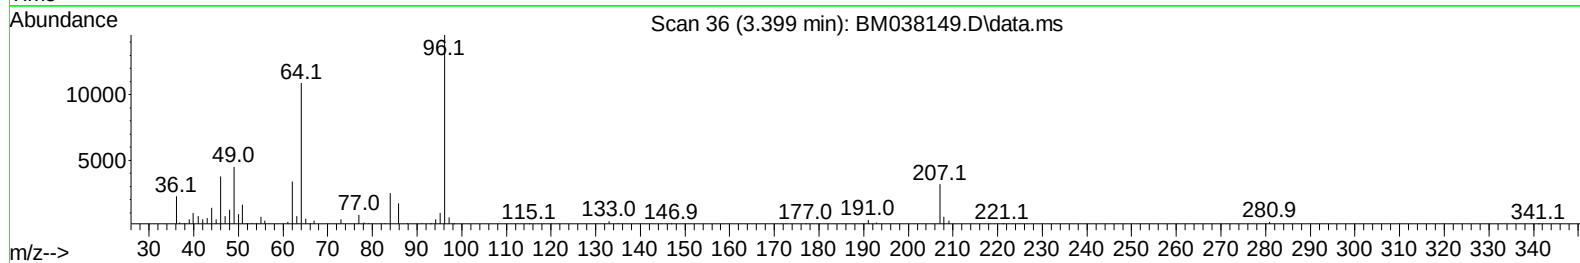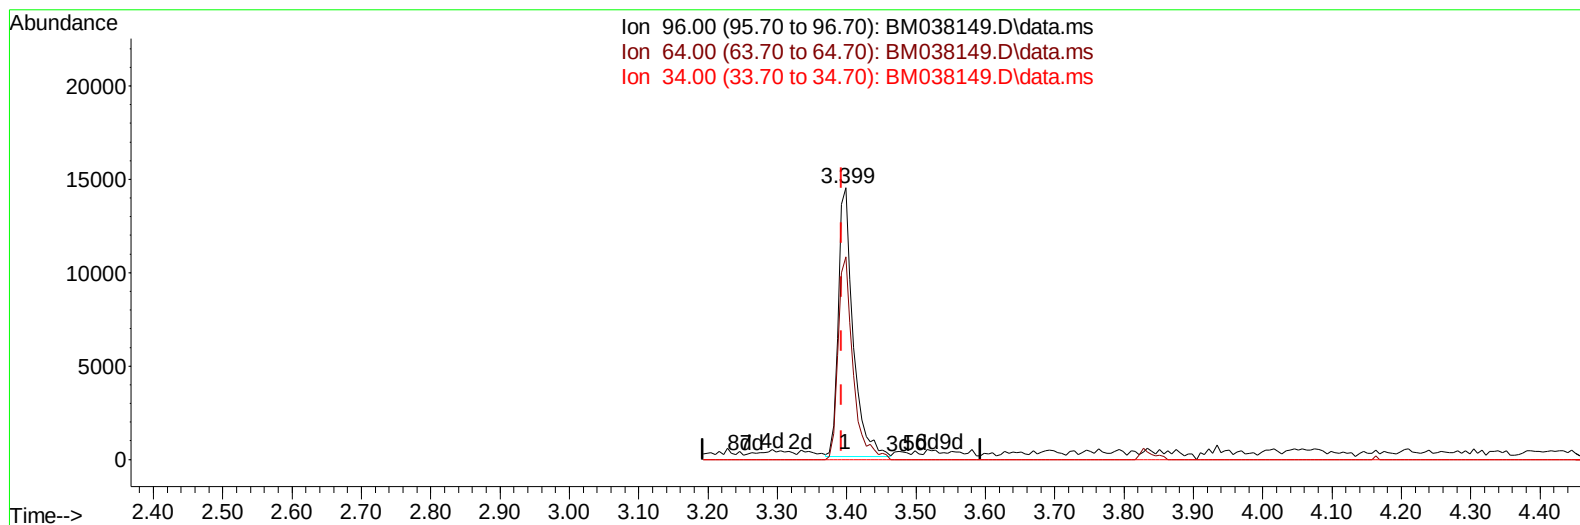

TIC: BM038149.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.399min (+ 0.006) 5.51 ng/uL m

response 21402

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	74.70
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038149.D
 Acq On : 21 Dec 2022 00:06
 Operator : CG/JU
 Sample : N6008-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXW9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/21/2022
 Supervised By :mohammad ahmed 12/21/2022

Quant Time: Dec 21 01:31:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 00:11:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.045	152	176373	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	771002	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.668	164	479488	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.409	188	1021595	20.000	ng/ul	0.00
79) Chrysene-d12	21.574	240	823543	20.000	ng/ul	0.00
88) Perylene-d12	24.027	264	743128	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	21402m	5.510	ng/uL	0.00
4) Pyridine-d5	3.834	84	291170	25.268	ng/ul	0.00
7) Phenol-d5	7.204	99	436879	30.482	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	247296	28.336	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132	381403	32.440	ng/ul	0.00
15) 4-Methylphenol-d8	8.757	113	357518	31.957	ng/ul	0.00
21) Nitrobenzene-d5	9.216	128	191890	31.434	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	223125	34.878	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.480	165	406738	33.474	ng/ul	0.00
31) 4-Chloroaniline-d4	10.998	131	484138	28.865	ng/ul	0.00
46) Dimethylphthalate-d6	14.080	166	1186004	34.694	ng/ul	0.00
49) Acenaphthylene-d8	14.368	160	1387933	33.220	ng/ul	0.00
54) 4-Nitrophenol-d4	14.868	143	193656	33.241	ng/ul	0.00
60) Fluorene-d10	15.657	176	1040694	34.171	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.780	200	154743	28.331	ng/ul	0.00
73) Anthracene-d10	17.509	188	1561407	32.748	ng/ul	0.00
81) Pyrene-d10	19.792	212	1780090	35.983	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	1264560	34.069	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038149.D
Acq On : 21 Dec 2022 00:06
Operator : CG/JU
Sample : N6008-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXW9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/21/2022
Supervised By :mohammad ahmed 12/21/2022

Quant Time: Dec 21 01:31:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 21 00:11:56 2022
Response via : Initial Calibration

