

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038163.D
 Acq On : 21 Dec 2022 09:44
 Operator : CG/JU
 Sample : PB149779BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK779

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	43	rVB	39191	56001	1.39%	0.133%
2	3.828	106	109	128	rBV	501152	882833	21.94%	2.100%
3	4.163	162	166	171	rVB3	9075	14139	0.35%	0.034%
4	7.198	676	682	692	rBV	685507	1085206	26.97%	2.581%
5	7.369	704	711	721	rVB	512821	778508	19.35%	1.852%
6	7.569	734	745	756	rBV	717042	1121336	27.87%	2.667%
7	8.039	818	825	833	rBV	589883	900954	22.39%	2.143%
8	8.751	939	946	961	rVB	877076	1390717	34.56%	3.308%
9	9.216	1016	1025	1034	rBV	665804	1096861	27.26%	2.609%
10	9.939	1139	1148	1156	rBV	576495	947644	23.55%	2.254%
11	10.475	1232	1239	1249	rBV	943491	1513658	37.62%	3.600%
12	10.857	1296	1304	1314	rBV	847636	1389441	34.53%	3.305%
13	10.998	1321	1328	1341	rBV	885683	1492432	37.09%	3.550%
14	11.639	1431	1437	1438	rBV5	2755	5028	0.12%	0.012%
15	12.080	1504	1512	1514	rBV6	2644	4378	0.11%	0.010%
16	12.433	1566	1572	1578	rVB2	15957	25966	0.65%	0.062%
17	14.080	1841	1852	1862	rBV	1557828	2113503	52.53%	5.027%
18	14.368	1893	1901	1912	rBV	1813894	2665418	66.25%	6.340%
19	14.668	1944	1952	1961	rBV	1352362	1893326	47.06%	4.503%
20	14.868	1979	1986	1997	rBV	727886	1050772	26.12%	2.499%
21	15.080	2015	2022	2027	rVB8	4076	10258	0.25%	0.024%
22	15.333	2061	2065	2070	rBV8	3147	4887	0.12%	0.012%
23	15.610	2107	2112	2114	rBV5	4616	6536	0.16%	0.016%
24	15.657	2114	2120	2127	rVB	2404871	3255139	80.90%	7.743%
25	15.774	2134	2140	2151	rBV	595524	783962	19.48%	1.865%
26	15.892	2156	2160	2166	rVB2	11393	15032	0.37%	0.036%
27	16.851	2320	2323	2327	rVB4	4707	6003	0.15%	0.014%
28	17.409	2411	2418	2424	rBV	1643382	2225858	55.32%	5.294%
29	17.509	2428	2435	2444	rBV	2571954	3607199	89.65%	8.580%
30	17.668	2455	2462	2470	rBV4	17878	39942	0.99%	0.095%
31	17.786	2480	2482	2484	rVB3	7331	5366	0.13%	0.013%
32	17.921	2502	2505	2510	rVB5	8553	9895	0.25%	0.024%
33	18.068	2526	2530	2532	rBV4	5576	5154	0.13%	0.012%
34	18.286	2564	2567	2573	rVB7	9534	13739	0.34%	0.033%
35	18.415	2585	2589	2593	rBV7	8751	14776	0.37%	0.035%
36	19.356	2745	2749	2756	rVB4	30657	39543	0.98%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038163.D
Acq On : 21 Dec 2022 09:44
Operator : CG/JU
Sample : PB149779BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK779

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Title : SVOA CALIBRATION

37	19.427	2757	2761	2765	rVV	26789	36633	0.91%	0.087%
38	19.792	2817	2823	2829	rBV	3184939	4023546	100.00%	9.570%
39	20.762	2984	2988	2996	rVB	139196	170504	4.24%	0.406%
40	21.574	3121	3126	3132	rVB	1654229	2061341	51.23%	4.903%
41	23.868	3509	3516	3526	rVB2	1766493	3359654	83.50%	7.991%
42	24.027	3537	3543	3551	rVB2	988450	1919136	47.70%	4.565%




Sum of corrected areas: 42042224

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038163.D
Acq On : 21 Dec 2022 09:44
Operator : CG/JU
Sample : PB149779BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK779

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

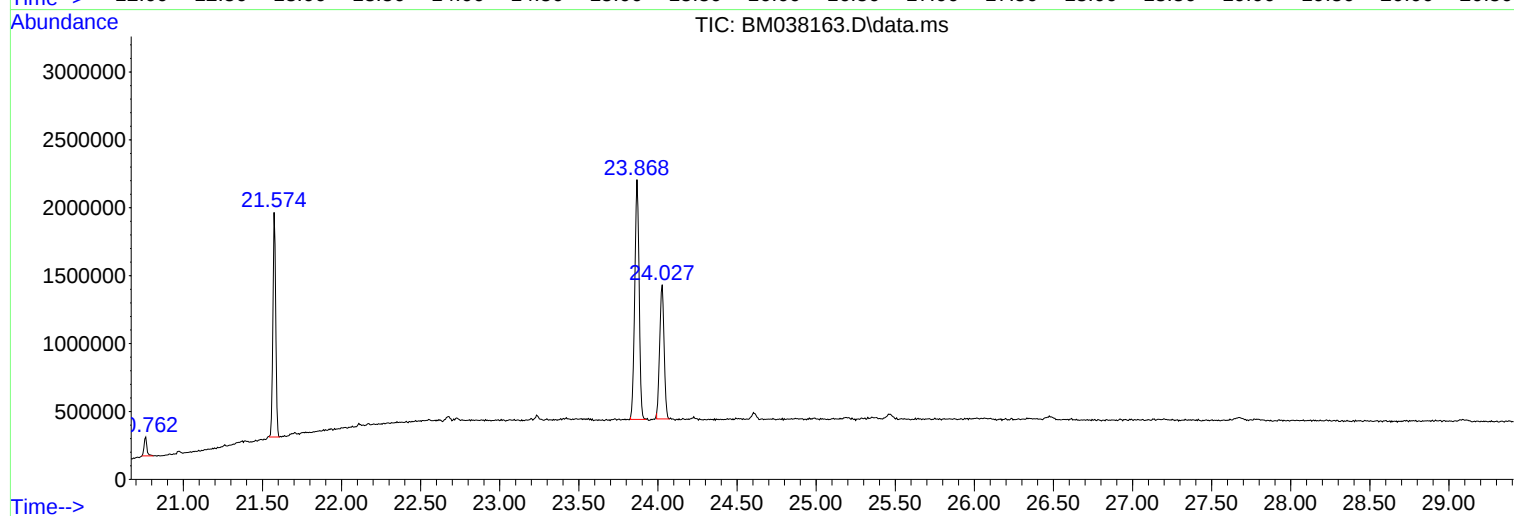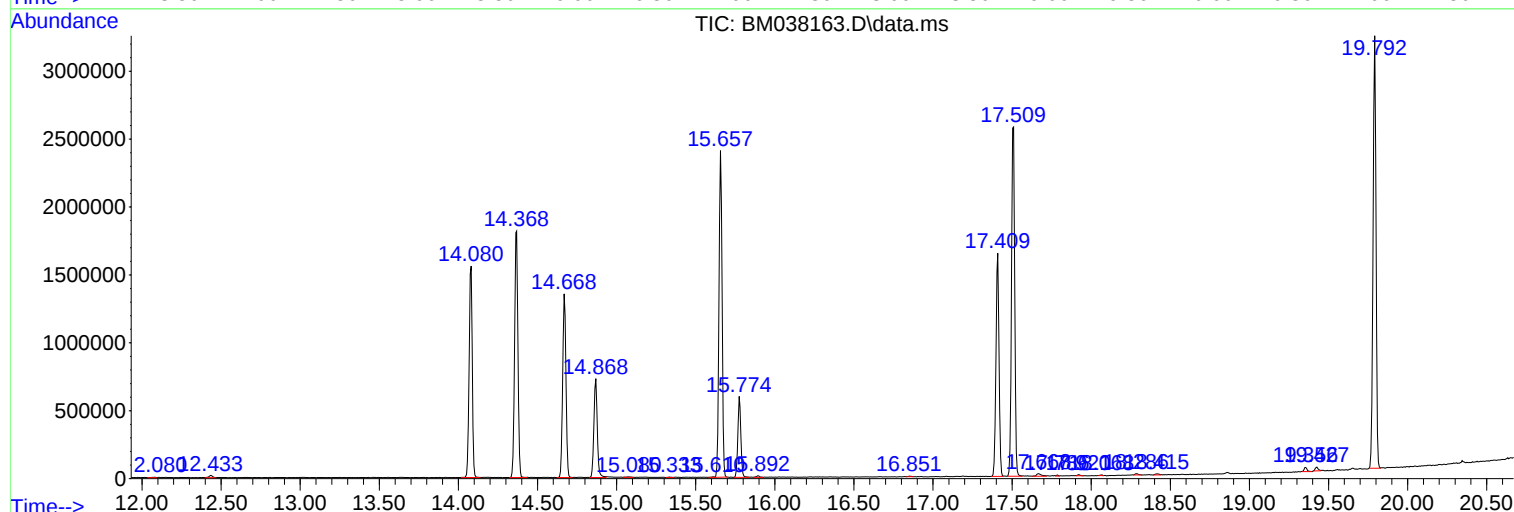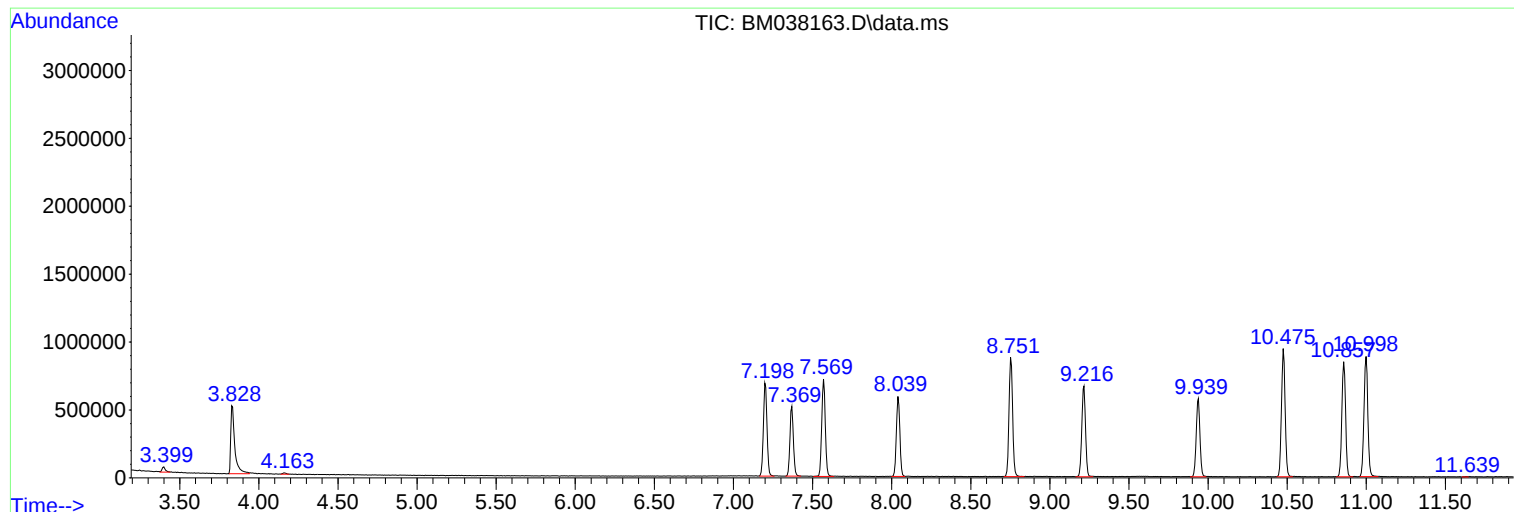

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038163.D
Acq On : 21 Dec 2022 09:44
Operator : CG/JU
Sample : PB149779BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK779

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038163.D
Acq On : 21 Dec 2022 09:44
Operator : CG/JU
Sample : PB149779BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK779

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc