

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038184.D
 Acq On : 21 Dec 2022 23:05
 Operator : CG/JU
 Sample : N6032-12
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	24	29	56	rVB	16401319	34086756	100.00%	47.393%
2	3.840	107	111	120	rBV2	96379	185582	0.54%	0.258%
3	4.158	162	165	172	rVB	23460	35795	0.11%	0.050%
4	4.281	181	186	193	rBV	41702	60072	0.18%	0.084%
5	5.116	319	328	337	rBV3	23515	53251	0.16%	0.074%
6	5.446	377	384	394	rBV	1026370	1480175	4.34%	2.058%
7	6.310	519	531	538	rVB3	29699	76043	0.22%	0.106%
8	7.199	675	682	692	rVB	151691	250443	0.73%	0.348%
9	7.363	704	710	719	rBV	510074	773942	2.27%	1.076%
10	7.569	738	745	752	rBV	480185	751805	2.21%	1.045%
11	8.040	818	825	832	rBV	640385	985929	2.89%	1.371%
12	8.751	939	946	955	rBV	390987	608032	1.78%	0.845%
13	9.210	1017	1024	1032	rBV	674081	1088254	3.19%	1.513%
14	9.934	1138	1147	1156	rBV	492103	797893	2.34%	1.109%
15	10.475	1232	1239	1252	rBV	731789	1198820	3.52%	1.667%
16	10.857	1296	1304	1311	rVB	859768	1434370	4.21%	1.994%
17	10.992	1319	1327	1341	rBV	464146	818354	2.40%	1.138%
18	14.075	1844	1851	1860	rBV	1566968	2090051	6.13%	2.906%
19	14.363	1893	1900	1907	rBV	1791866	2498398	7.33%	3.474%
20	14.669	1945	1952	1959	rVB	1330502	1858079	5.45%	2.583%
21	14.869	1980	1986	1998	rBV	118172	195469	0.57%	0.272%
22	15.657	2113	2120	2127	rBV	2332406	3142946	9.22%	4.370%
23	15.774	2134	2140	2147	rVB	379218	487775	1.43%	0.678%
24	16.698	2292	2297	2303	rBV3	26048	40795	0.12%	0.057%
25	17.404	2411	2417	2423	rBV	1573530	2087398	6.12%	2.902%
26	17.504	2428	2434	2441	rBV	2683074	3543414	10.40%	4.927%
27	17.657	2456	2460	2472	rBV4	28300	57400	0.17%	0.080%
28	18.280	2561	2566	2571	rBV	108228	154223	0.45%	0.214%
29	19.351	2745	2748	2753	rVB3	31872	41799	0.12%	0.058%
30	19.421	2756	2760	2764	rBV	34260	59342	0.17%	0.083%
31	19.551	2778	2782	2790	rBV3	55980	87002	0.26%	0.121%
32	19.786	2817	2822	2833	rVB	2948355	3810371	11.18%	5.298%
33	20.756	2984	2987	2990	rVB	148519	149283	0.44%	0.208%
34	21.262	3070	3073	3078	rVB2	73887	92544	0.27%	0.129%
35	21.568	3121	3125	3131	rVB	1370409	1787350	5.24%	2.485%
36	23.862	3508	3515	3524	rVB2	1696848	3276370	9.61%	4.555%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038184.D
Acq On : 21 Dec 2022 23:05
Operator : CG/JU
Sample : N6032-12
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LB4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Title : SVOA CALIBRATION

37	24.021	3536	3542	3553	rVB2	907897	1778346	5.22%	2.473%
----	--------	------	------	------	------	--------	---------	-------	--------




Sum of corrected areas: 71923871

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038184.D
Acq On : 21 Dec 2022 23:05
Operator : CG/JU
Sample : N6032-12
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

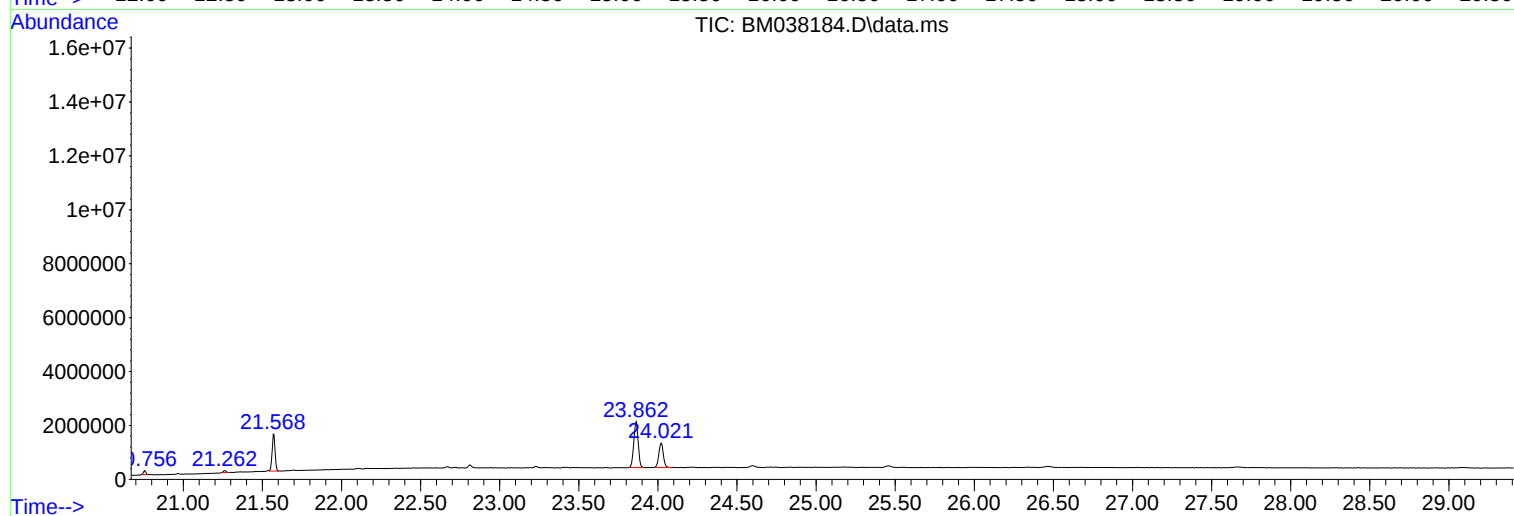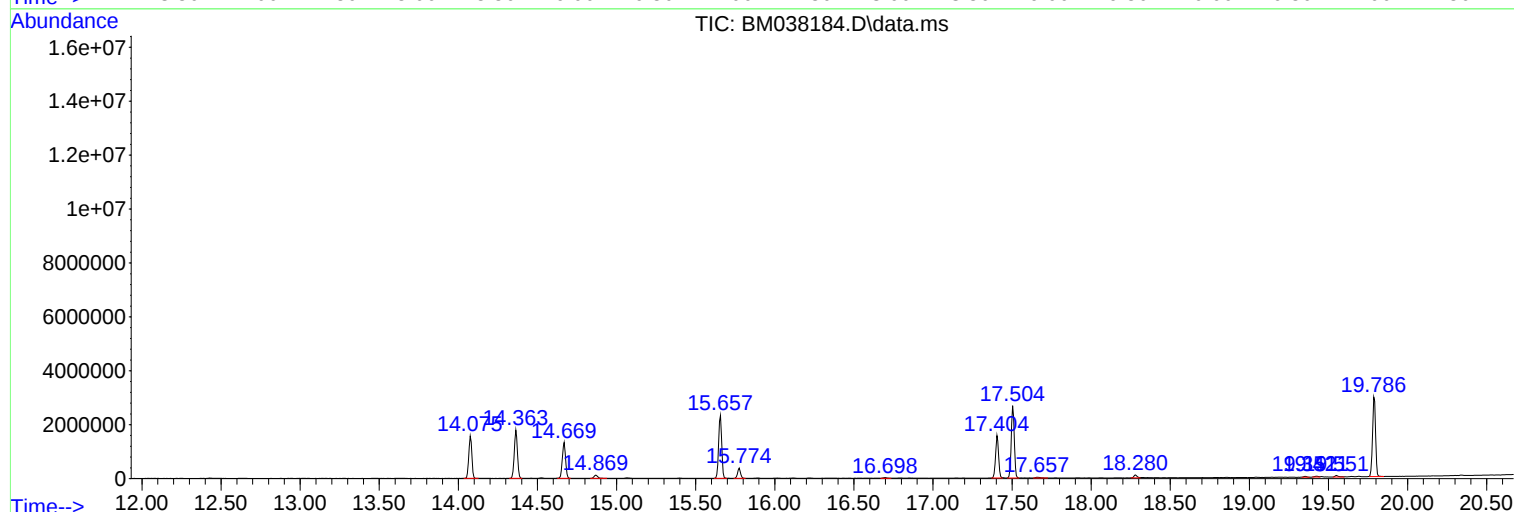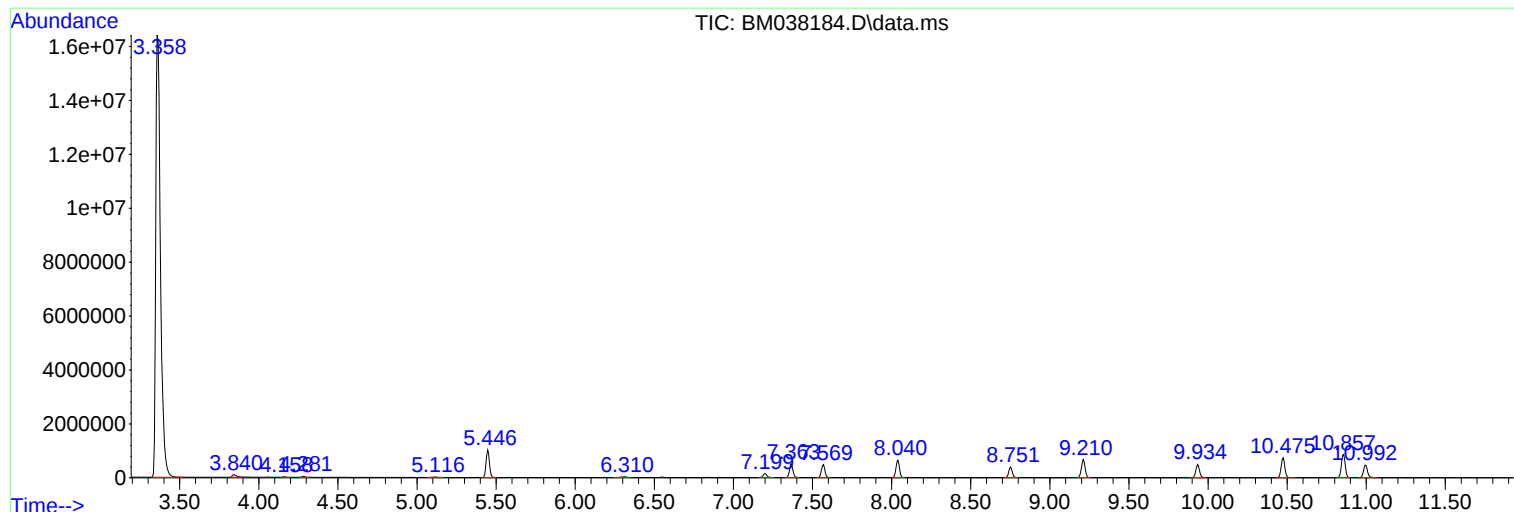

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038184.D
Acq On : 21 Dec 2022 23:05
Operator : CG/JU
Sample : N6032-12
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLB4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butanamide, 3,3-dimethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.446	30.03 ng/ul	1480180	1,4-Dichlorobenzene-d4	8.040

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butanamide, 3,3-dimethyl-	115	C6H13NO	000926-04-5	72
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	50
3			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	40
4			2-Hexanol, methyl ether	116	C7H16O	1000333-92-0	9
5			4-Hydroxy-3-hexanone	116	C6H12O2	004984-85-4	9

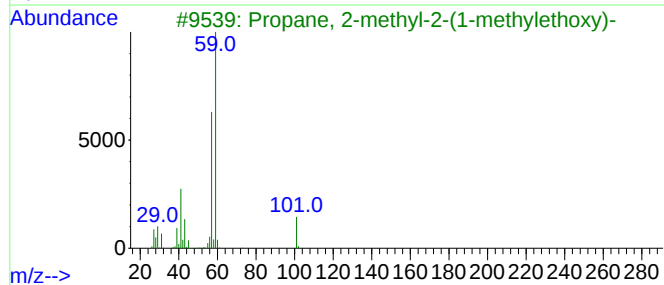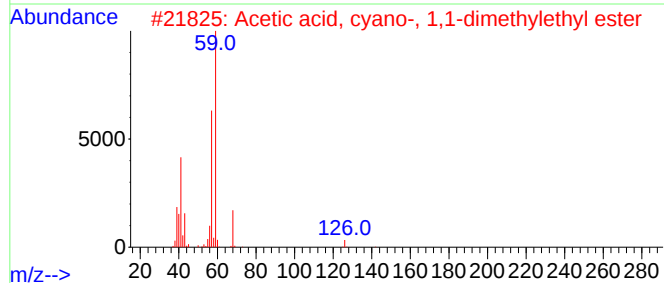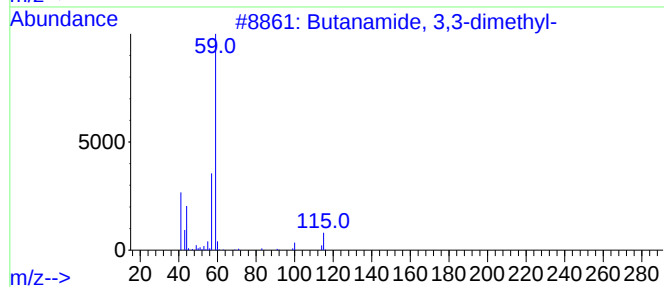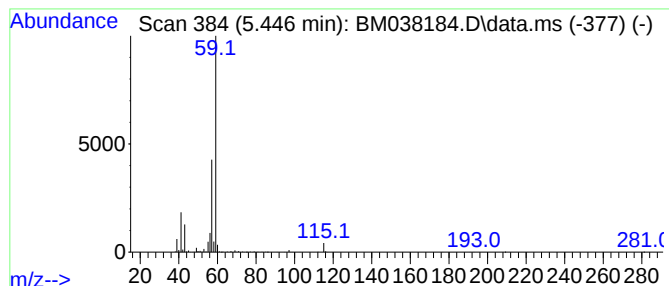

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038184.D
Acq On : 21 Dec 2022 23:05
Operator : CG/JU
Sample : N6032-12
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butanamide, 3,3...	5.446	30.0	ng/ul	1480180	1	8.040	985929	20.0