

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038185.D
 Acq On : 21 Dec 2022 23:41
 Operator : CG/JU
 Sample : N6032-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	24	29	48	rVB	3174619	5058305	100.00%	13.409%
2	3.857	111	114	122	rBV2	18126	42967	0.85%	0.114%
3	4.057	145	148	152	rVB2	8105	10182	0.20%	0.027%
4	4.157	162	165	170	rVB3	11041	16388	0.32%	0.043%
5	4.269	181	184	189	rVB6	5133	6693	0.13%	0.018%
6	4.704	251	258	269	rVB	473273	750293	14.83%	1.989%
7	5.116	322	328	338	rVB2	22529	40363	0.80%	0.107%
8	7.198	676	682	689	rVB	111025	175199	3.46%	0.464%
9	7.363	701	710	719	rBV	400614	614941	12.16%	1.630%
10	7.569	739	745	753	rVB	260377	409973	8.10%	1.087%
11	8.039	818	825	835	rBV	684414	1055932	20.88%	2.799%
12	8.751	940	946	953	rBV	243866	377586	7.46%	1.001%
13	9.210	1016	1024	1032	rBV	579099	925398	18.29%	2.453%
14	9.933	1140	1147	1155	rBV	259606	418093	8.27%	1.108%
15	10.475	1231	1239	1250	rBV	381815	622228	12.30%	1.649%
16	10.857	1296	1304	1314	rVB	953201	1544159	30.53%	4.093%
17	10.992	1320	1327	1340	rBV	339345	594490	11.75%	1.576%
18	12.427	1566	1571	1578	rVB2	13424	21810	0.43%	0.058%
19	13.298	1712	1719	1724	rBV6	4007	7947	0.16%	0.021%
20	13.621	1770	1774	1780	rBV8	4932	7749	0.15%	0.021%
21	14.074	1845	1851	1859	rBV	1094075	1450640	28.68%	3.845%
22	14.363	1893	1900	1912	rVB	1607546	2293163	45.33%	6.079%
23	14.668	1945	1952	1962	rVB	1404716	1974610	39.04%	5.234%
24	14.868	1981	1986	1998	rBV	73276	123474	2.44%	0.327%
25	15.080	2016	2022	2029	rBV8	11402	22674	0.45%	0.060%
26	15.398	2074	2076	2082	rBV6	3481	5938	0.12%	0.016%
27	15.657	2113	2120	2127	rVB	2191837	2942958	58.18%	7.801%
28	15.774	2135	2140	2147	rBV	173790	237763	4.70%	0.630%
29	15.892	2155	2160	2164	rBV2	10061	14347	0.28%	0.038%
30	16.851	2319	2323	2326	rBV6	5860	6659	0.13%	0.018%
31	17.151	2369	2374	2378	rVV7	7028	10785	0.21%	0.029%
32	17.198	2378	2382	2387	rVB7	3305	6209	0.12%	0.016%
33	17.404	2411	2417	2427	rVB	1620276	2192379	43.34%	5.812%
34	17.504	2427	2434	2445	rBV	2442925	3300042	65.24%	8.748%
35	17.604	2445	2451	2457	rVB3	9147	21365	0.42%	0.057%
36	17.668	2457	2462	2470	rBV6	16124	33937	0.67%	0.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
 Data File : BM038185.D
 Acq On : 21 Dec 2022 23:41
 Operator : CG/JU
 Sample : N6032-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	17.780	2476	2481	2485	rBV7	5323	8244	0.16%	0.022%
38	17.915	2501	2504	2511	rVB7	9121	15021	0.30%	0.040%
39	18.062	2525	2529	2535	rVB7	7249	9307	0.18%	0.025%
40	18.280	2562	2566	2573	rBV3	36200	50797	1.00%	0.135%
41	18.356	2576	2579	2583	rVB2	9183	11370	0.22%	0.030%
42	18.856	2661	2664	2669	rVB6	9619	11452	0.23%	0.030%
43	19.350	2744	2748	2753	rBV2	29043	40625	0.80%	0.108%
44	19.421	2756	2760	2764	rVV	28469	46214	0.91%	0.123%
45	19.456	2764	2766	2770	rVB4	15632	13327	0.26%	0.035%
46	19.550	2778	2782	2787	rBV3	34273	48351	0.96%	0.128%
47	19.650	2796	2799	2802	rBV3	11510	16008	0.32%	0.042%
48	19.692	2804	2806	2810	rVB4	19380	18869	0.37%	0.050%
49	19.786	2817	2822	2832	rBV	2577285	3300767	65.25%	8.750%
50	20.756	2984	2987	2991	rVB	136312	142374	2.81%	0.377%
51	21.574	3121	3126	3131	rVB	1439966	1811887	35.82%	4.803%
52	23.862	3508	3515	3525	rVB2	1556799	3005963	59.43%	7.968%
53	24.021	3536	3542	3551	rVB2	932817	1835403	36.28%	4.865%


Sum of corrected areas: 37723618

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038185.D
Acq On : 21 Dec 2022 23:41
Operator : CG/JU
Sample : N6032-13
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

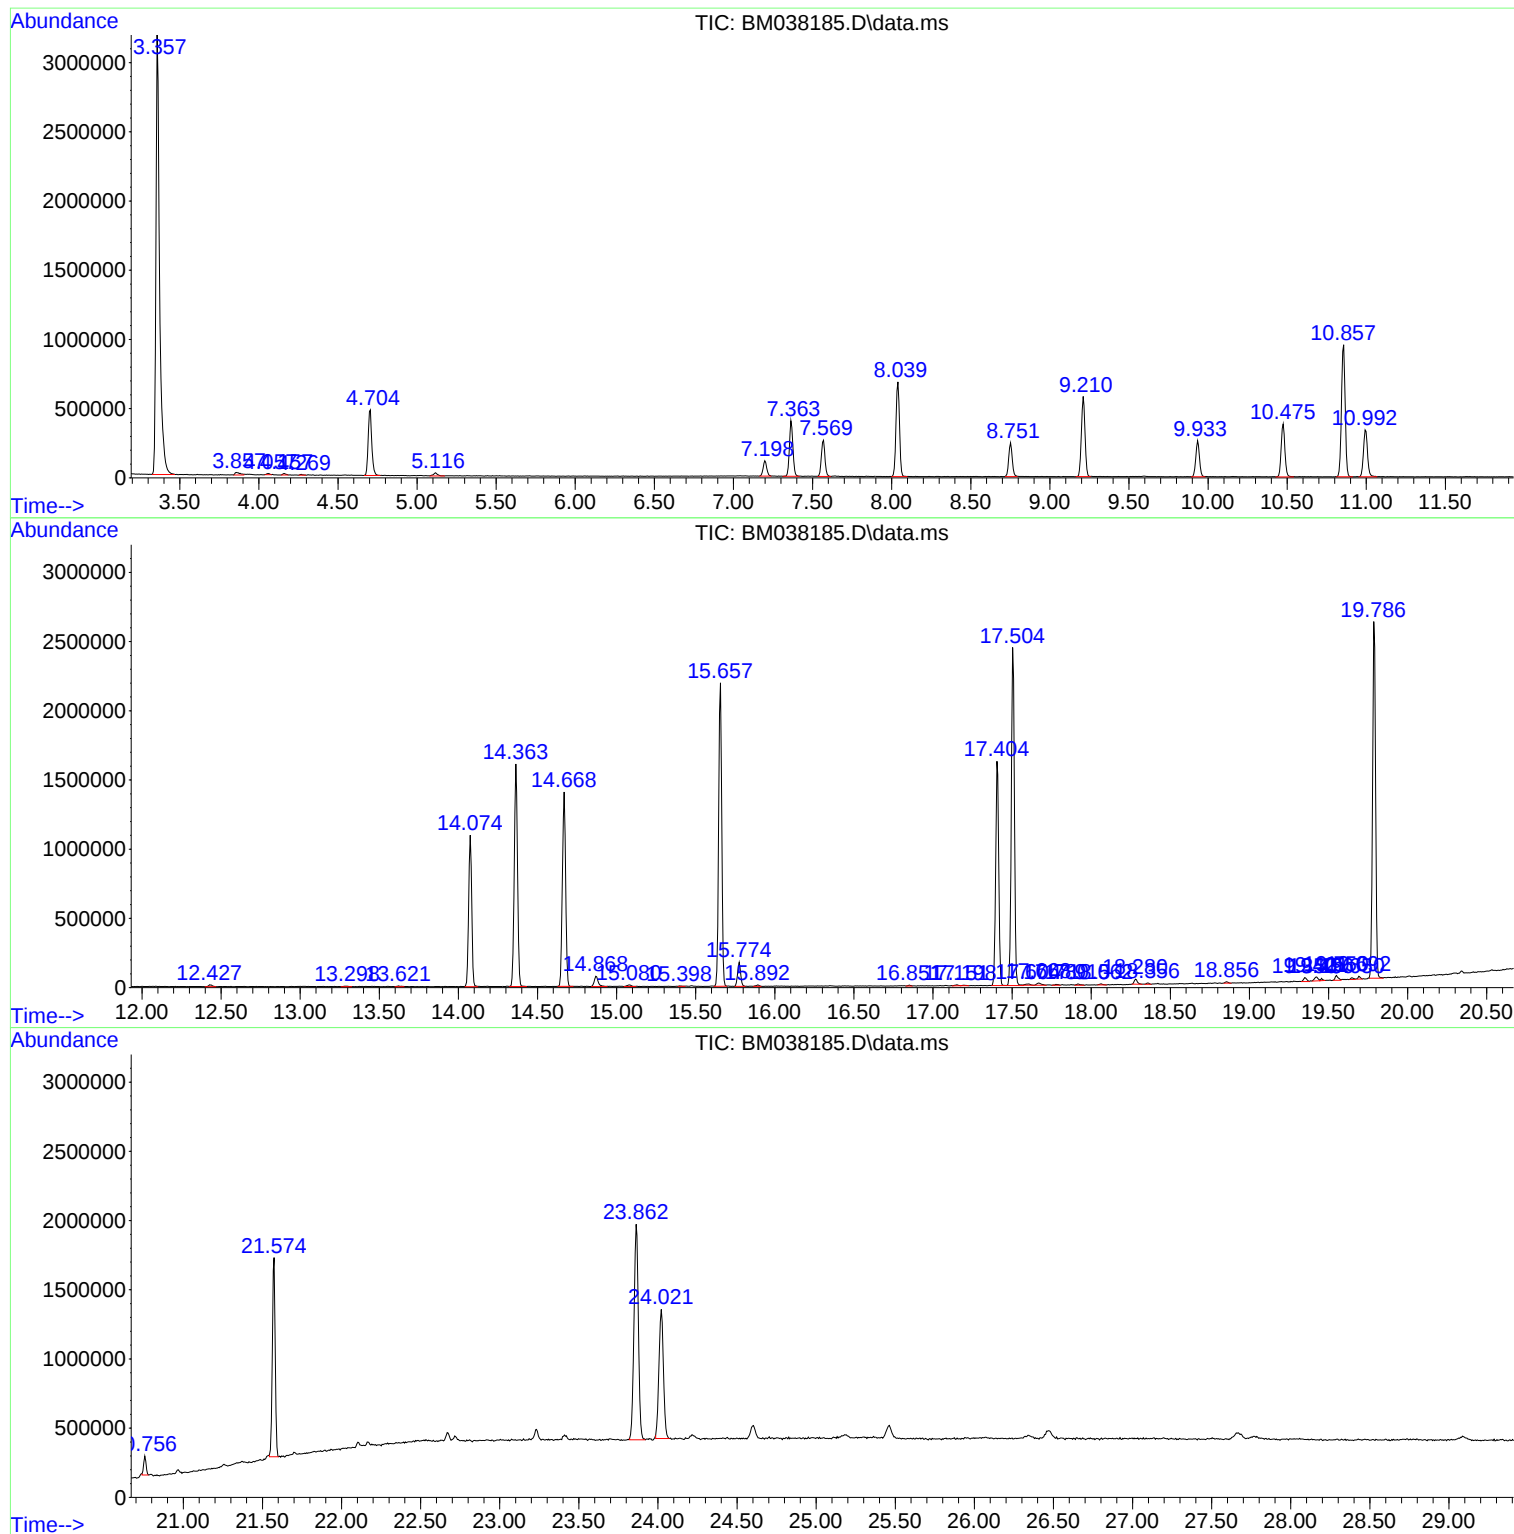

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038185.D
Acq On : 21 Dec 2022 23:41
Operator : CG/JU
Sample : N6032-13
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLB7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.704	14.21 ng/ul	750293	1,4-Dichlorobenzene-d4	8.039

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	64
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

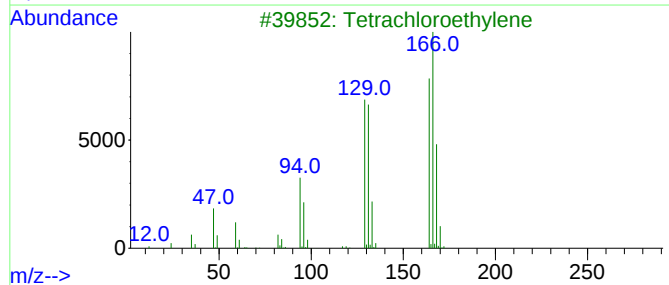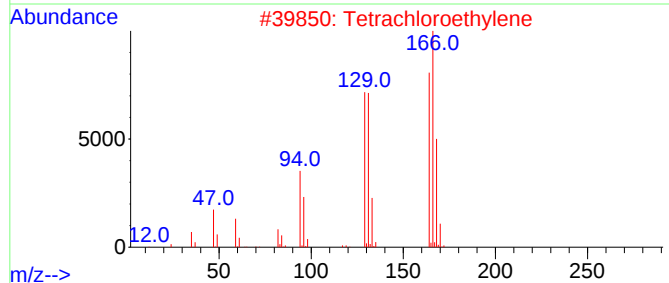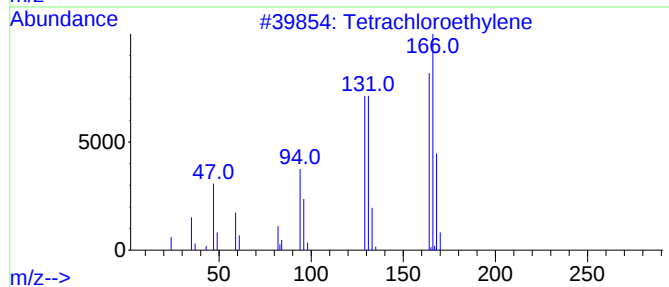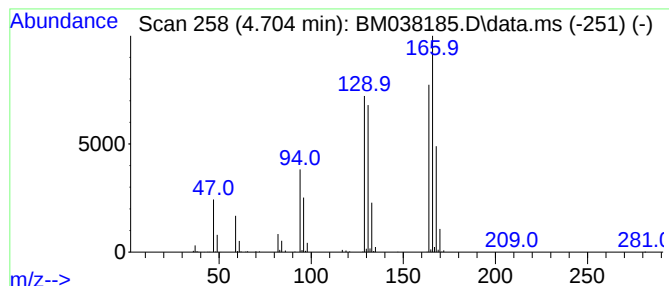

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122022\
Data File : BM038185.D
Acq On : 21 Dec 2022 23:41
Operator : CG/JU
Sample : N6032-13
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.704	14.2	ng/u1	750293	1	8.039	1055930	20.0