

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
 Data File : BM049138.D
 Acq On : 21 Dec 2024 15:01
 Operator : RC/JU
 Sample : SP6698
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP6698

Quant Time: Dec 22 23:08:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.565	152	6514	0.400	ng/ul	0.00
4) Naphthalene-d8	10.321	136	19671	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.192	164	10675	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.040	188	3495256	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.15
23) Perylene-d12	23.300	264	22857	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.185	96	109640	14.594	ng/ul	0.03
6) 2-Methylnaphthalene-d10	11.915	152	22208	0.840	ng/ul	0.00
18) Fluoranthene-d10	18.979	212	36942	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.191	166	6655	0.183	ng/ul#	13
26) Benzo(a)pyrene	23.168	252	12776	0.182	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049138.D
Acq On : 21 Dec 2024 15:01
Operator : RC/JU
Sample : SP6698
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP6698

Quant Time: Dec 22 23:08:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

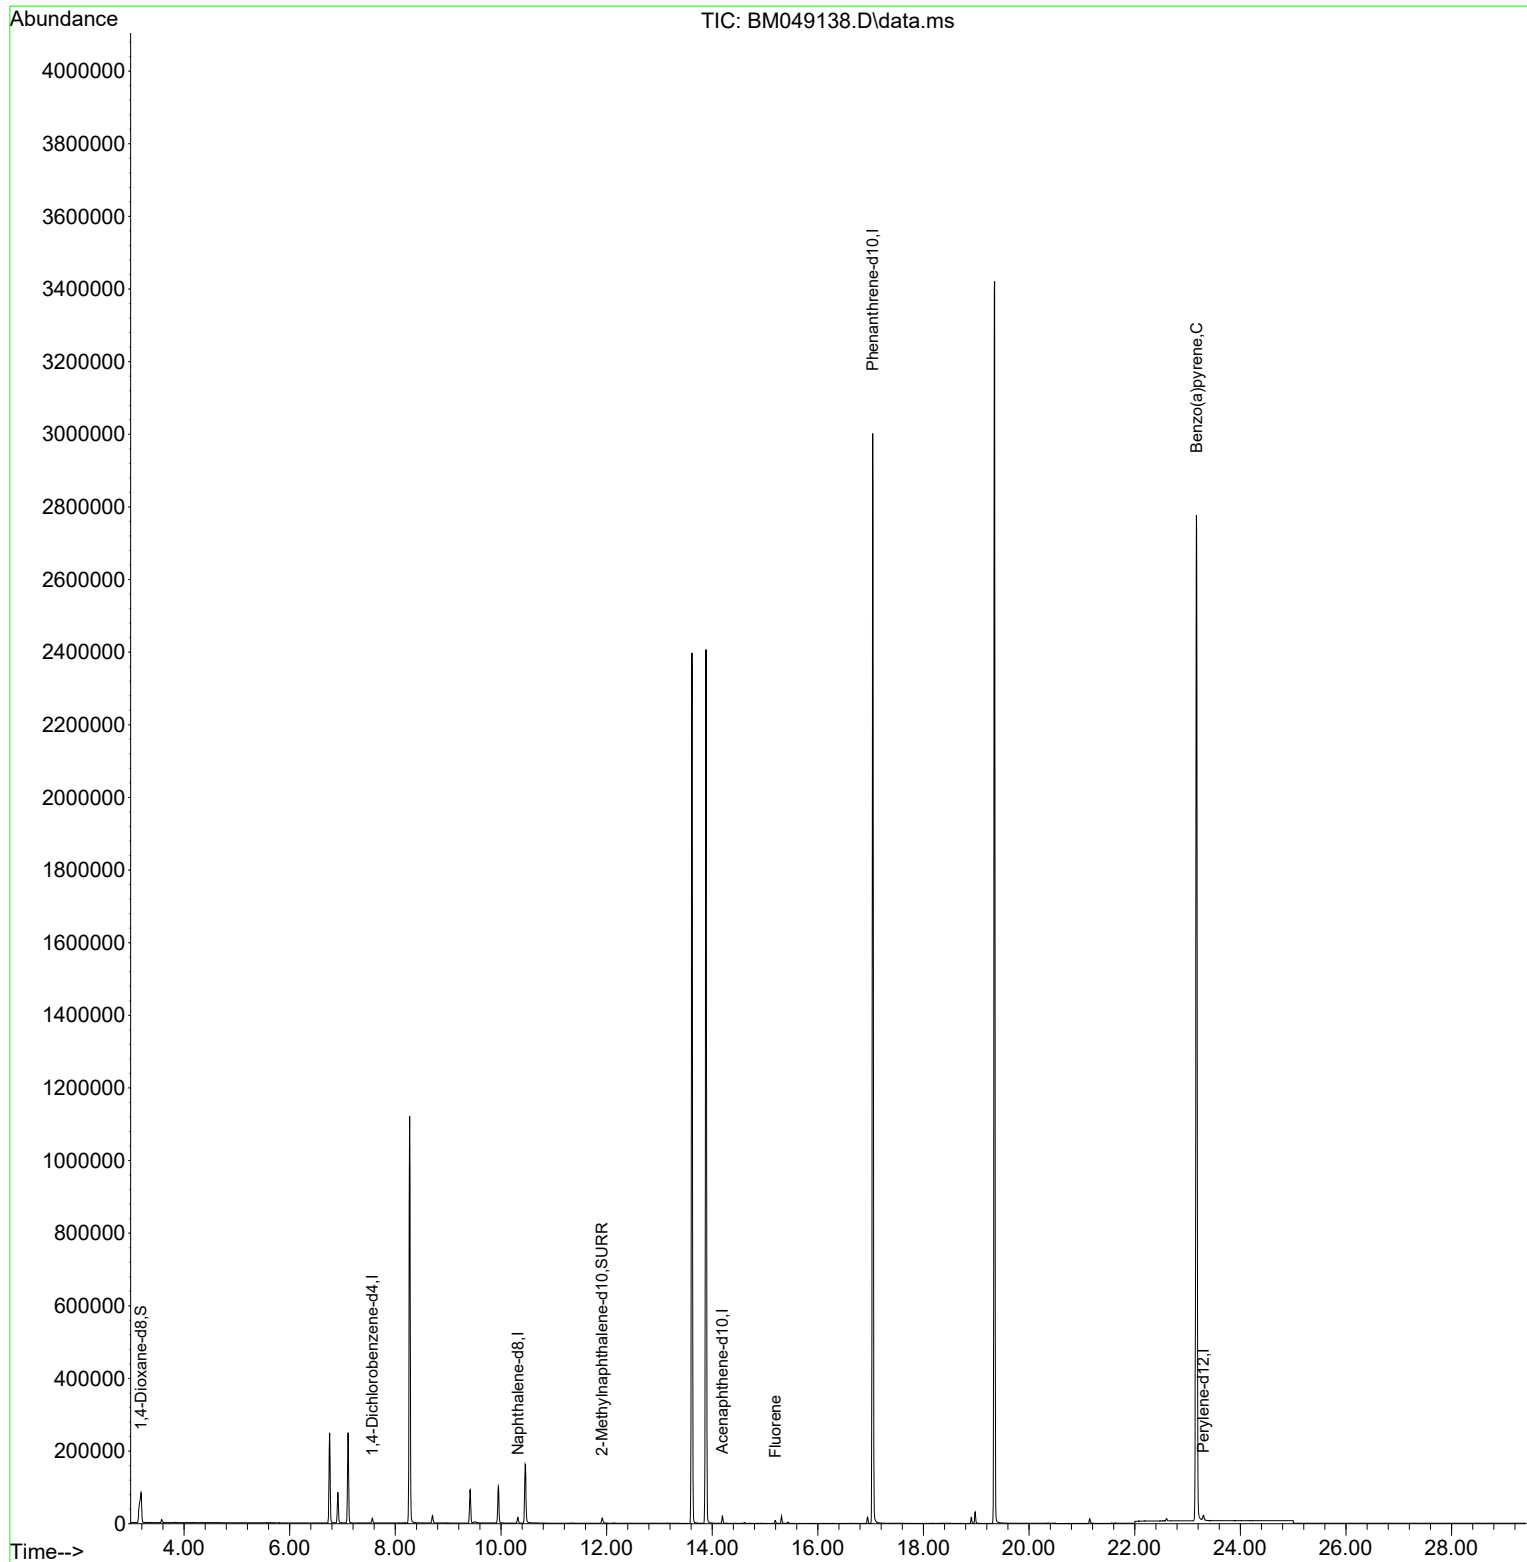

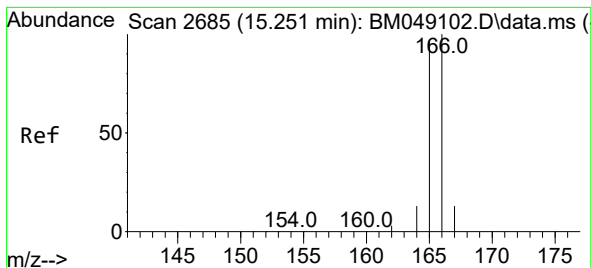

#12

Fluorene

Concen: 0.183 ng/ul

RT: 15.191 min Scan# 2

Delta R.T. -0.063 min

Lab File: BM049138.D

Acq: 21 Dec 2024 15:01

Instrument :

BNA_M

ClientSampleId :

SP6698





Tgt Ion:166 Resp: 6655

Ion Ratio Lower Upper

166 100

165 5.9 79.7 119.5#

167 31.4 11.4 17.0#

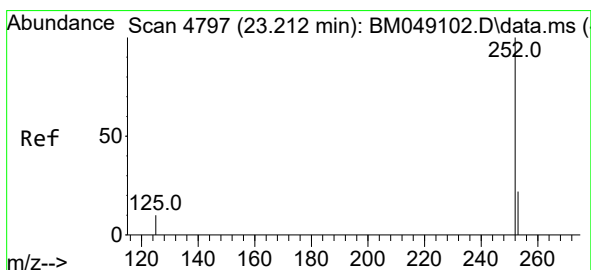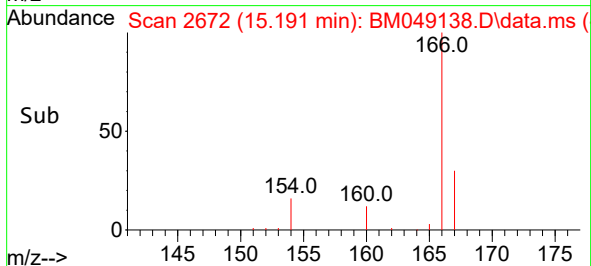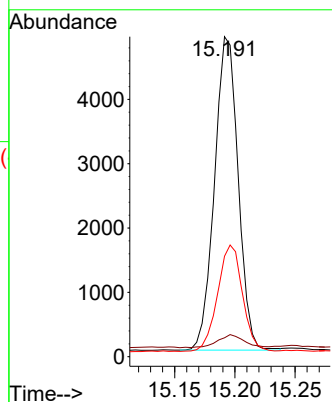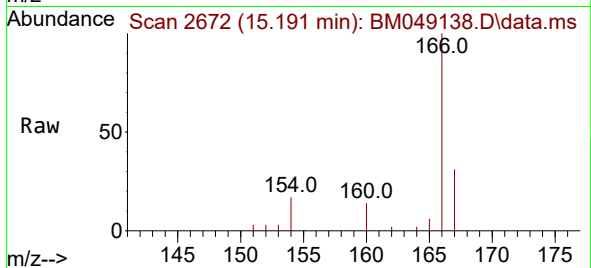

#26

Benzo(a)pyrene

Concen: 0.182 ng/ul

RT: 23.168 min Scan# 4782

Delta R.T. -0.041 min

Lab File: BM049138.D

Acq: 21 Dec 2024 15:01

Tgt Ion:252 Resp: 12776

Ion Ratio Lower Upper

252 100

253 36.2 22.4 33.6#

125 26.7 14.8 22.2#

