




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

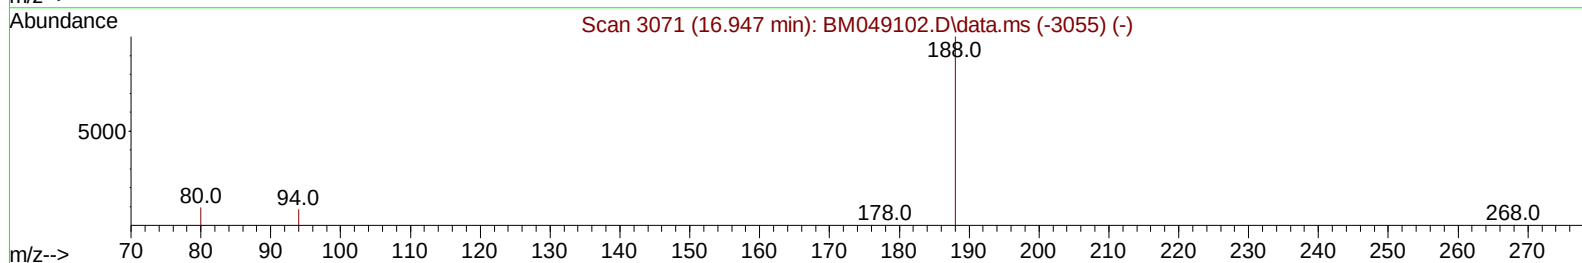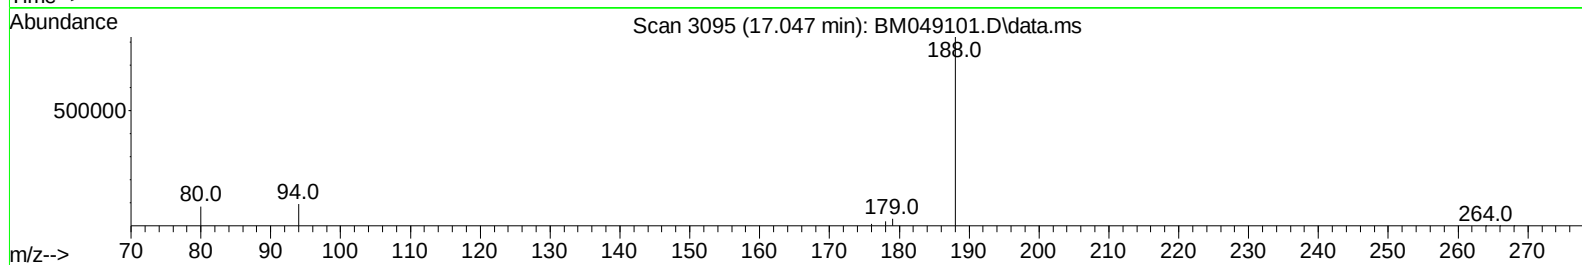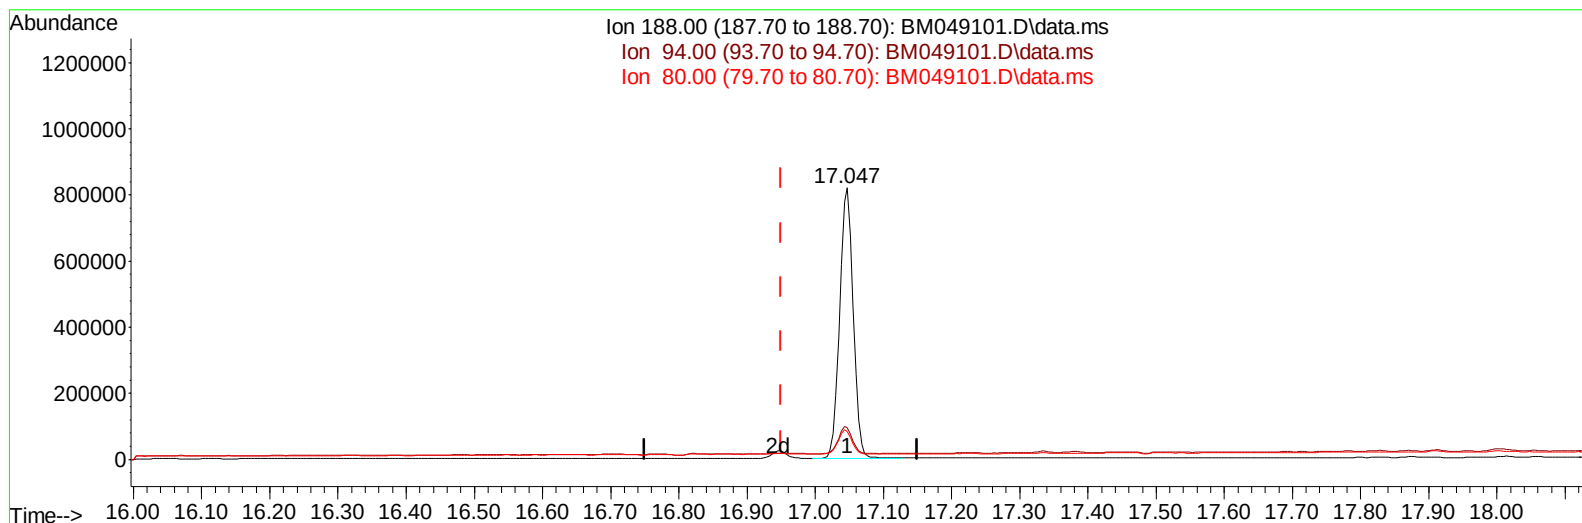

TIC: BM049101.D\data.ms

(13) Phenanthrene-d10 (I)

17.047min (+ 0.097) 0.40 ng/u1

response 1125190

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	11.63
80.00	10.70	10.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

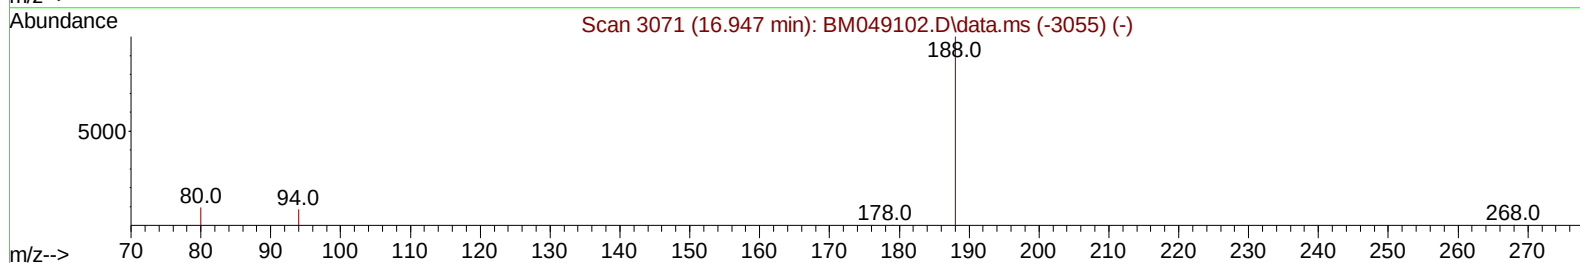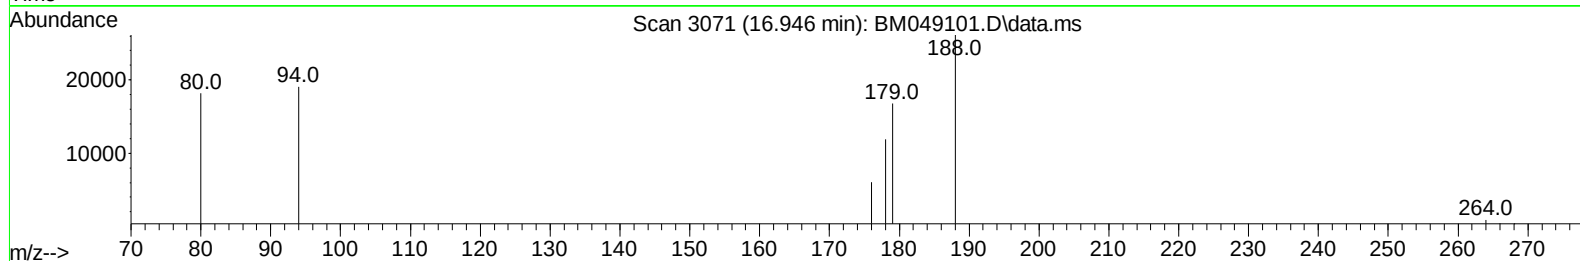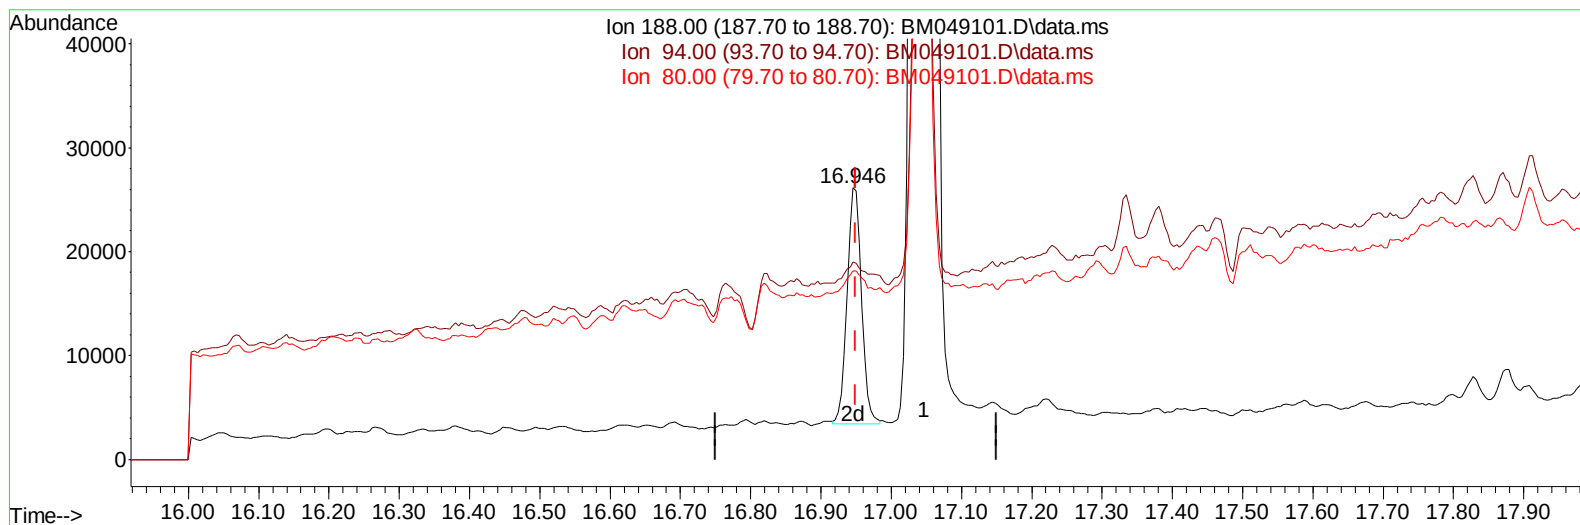

TIC: BM049101.D\data.ms

(13) Phenanthrene-d10 (I)

16.946min (-0.004) 0.40 ng/ul m

response 32439

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	72.79#
80.00	10.70	69.48#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
 Data File : BM049101.D
 Acq On : 20 Dec 2024 15:03
 Operator : RC/JU
 Sample : P5265-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2829

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
 Supervised By :mohammad ahmed 12/24/2024

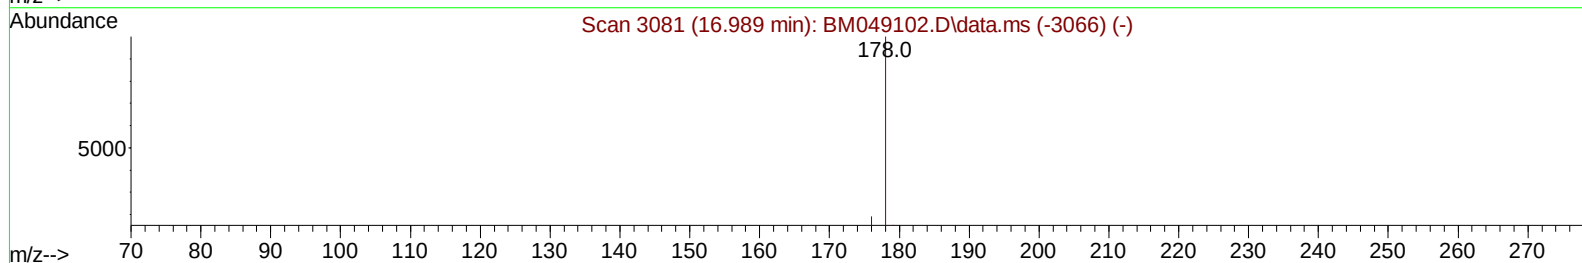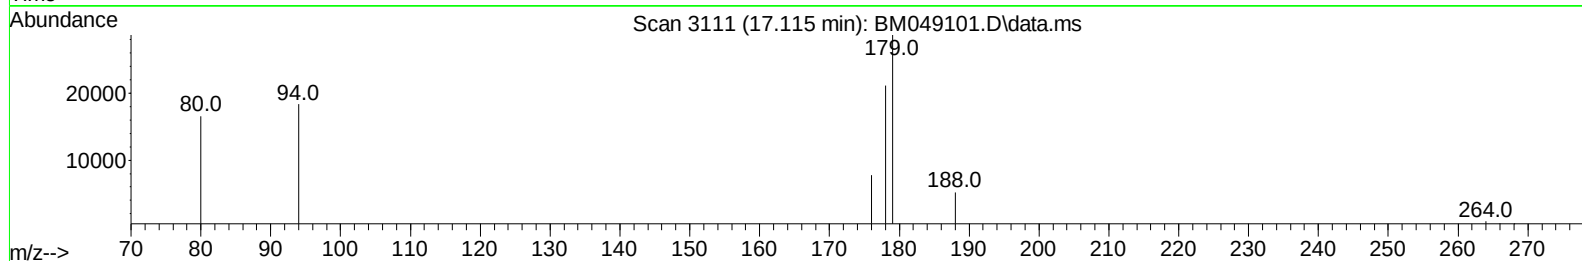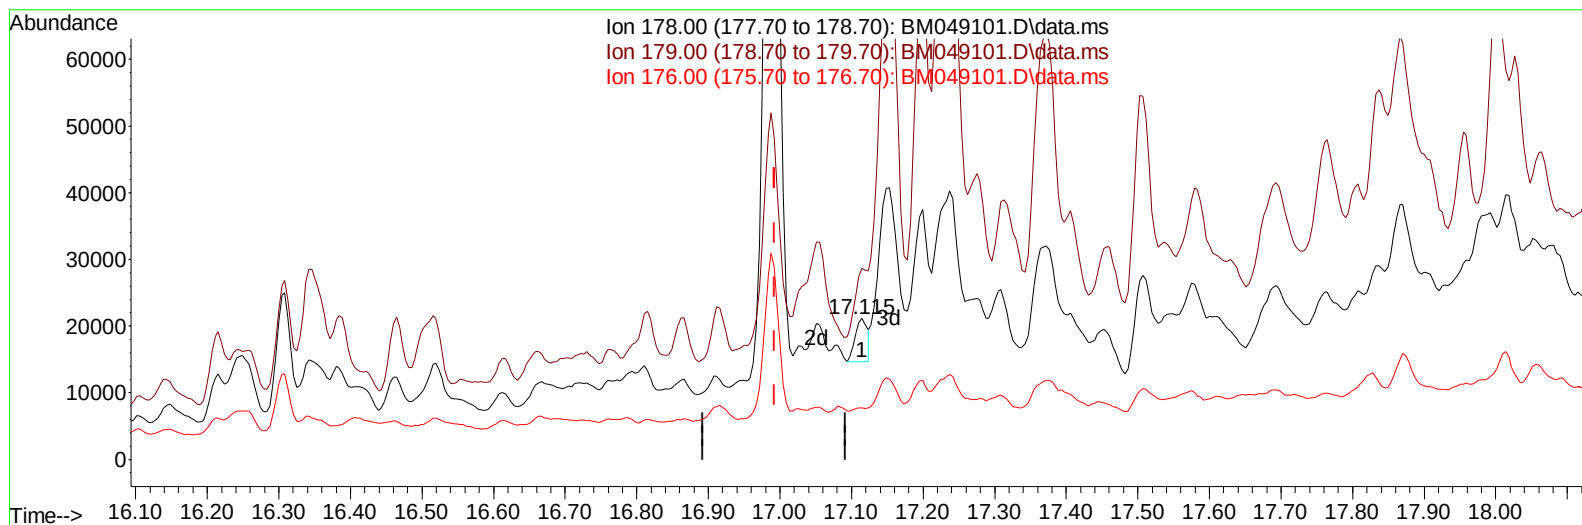

TIC: BM049101.D\data.ms

(15) Phenanthrene

17.115min (+ 0.122) 0.09 ng/u1

response 7563

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.20	135.69#
176.00	20.20	36.77#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

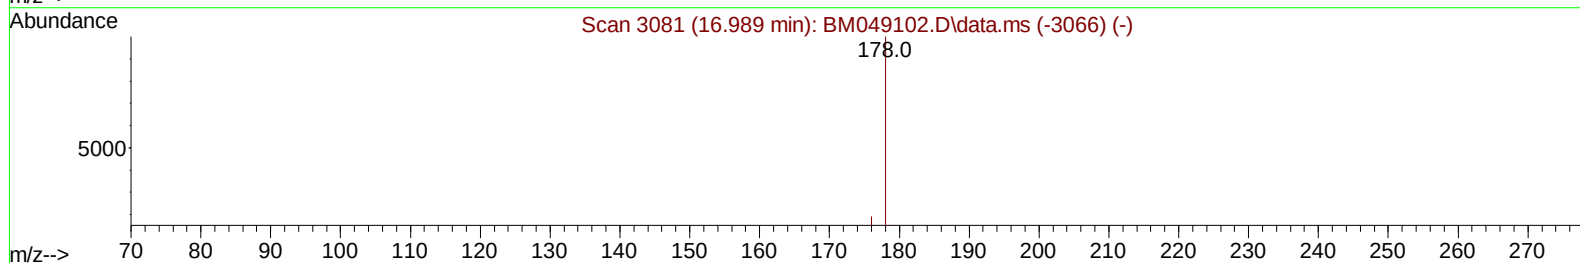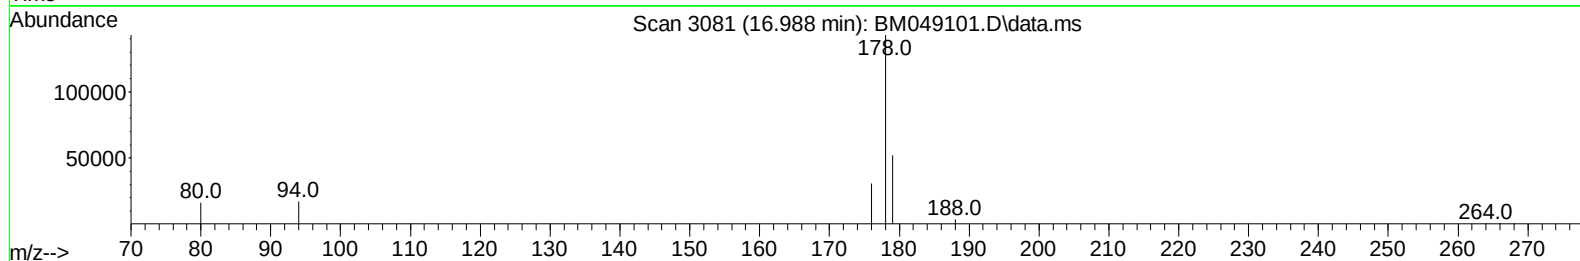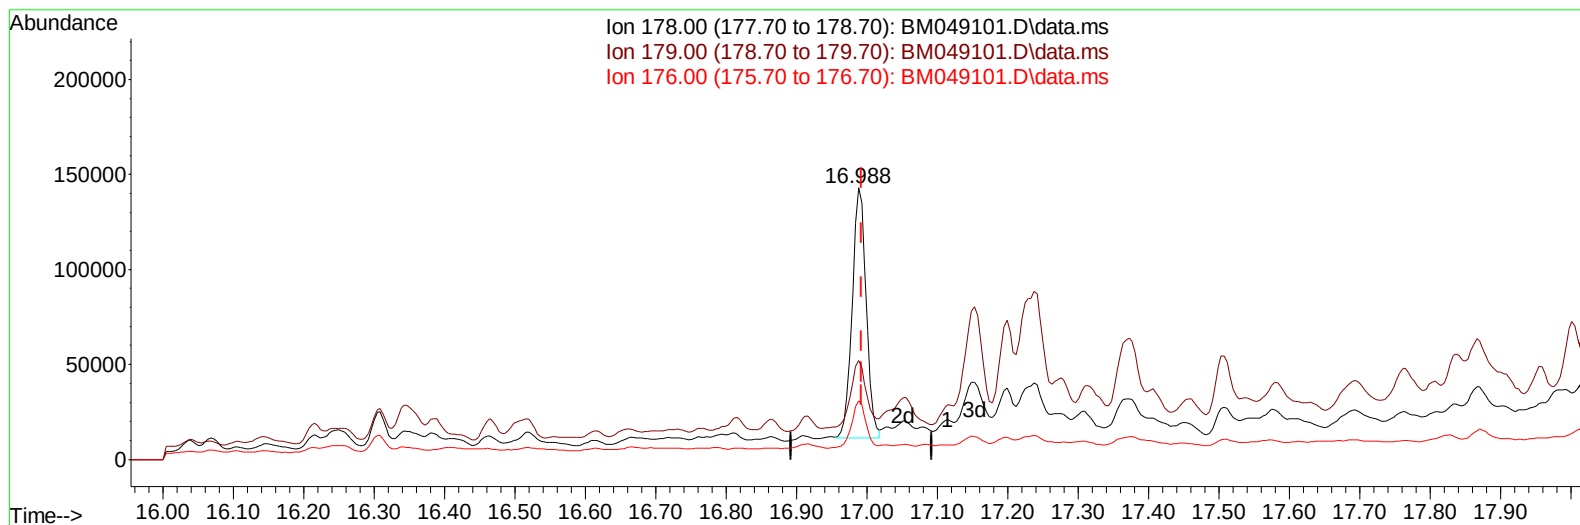

TIC: BM049101.D\data.ms

(15) Phenanthrene

16.988min (-0.004) 2.15 ng/ul m

response 181996

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.20	36.40#
176.00	20.20	21.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

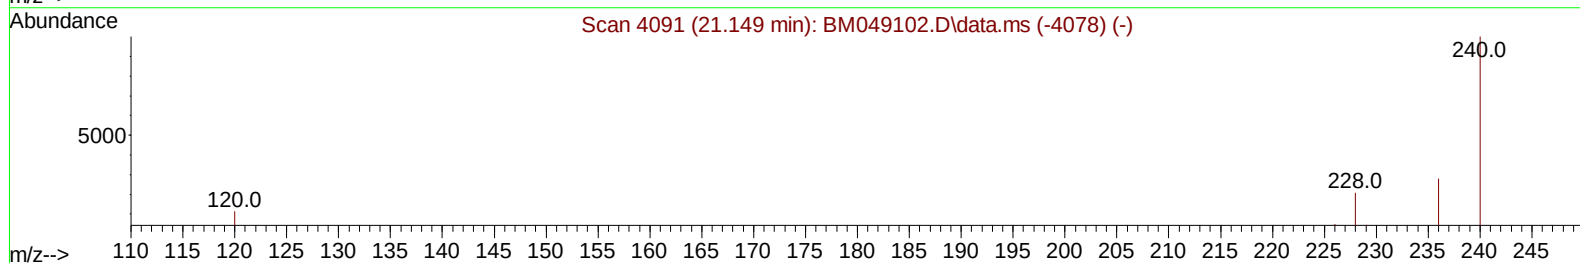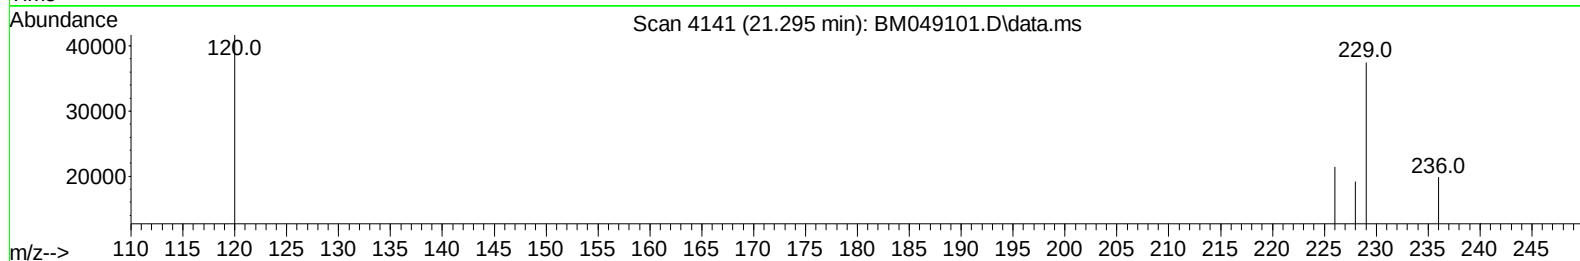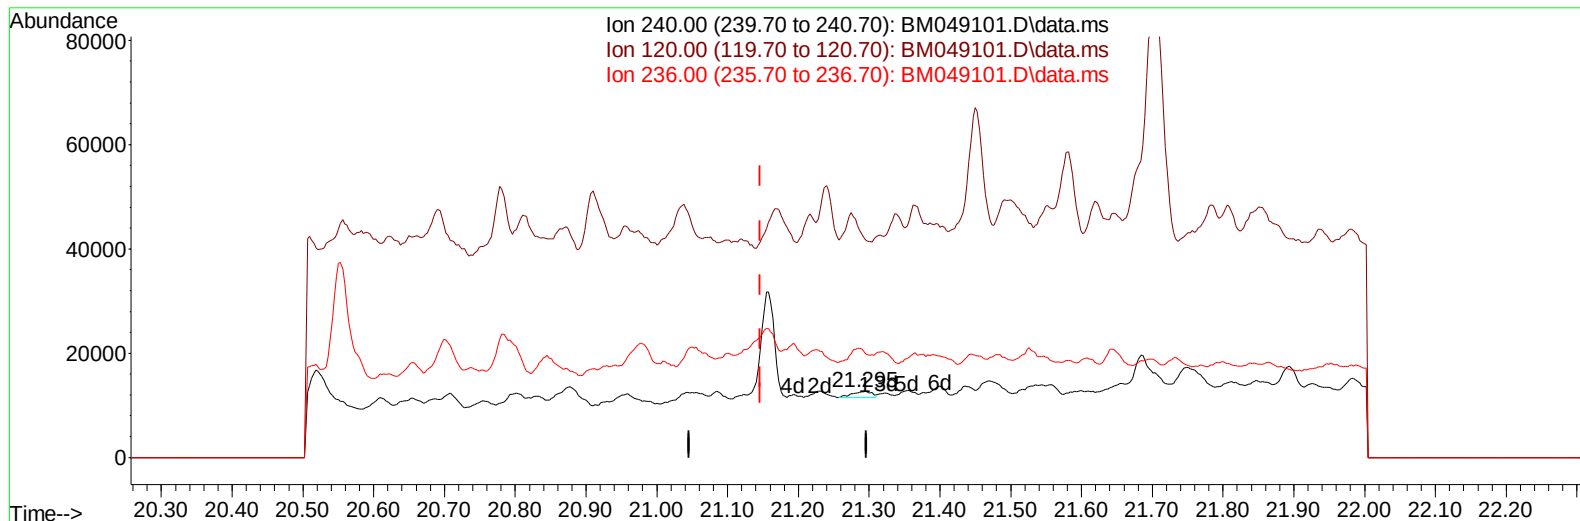

TIC: BM049101.D\data.ms

(17) Chrysene-d12

21.295min (+ 0.149) 0.40 ng/u1

response 2296

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	14.50	328.13#
236.00	29.80	156.16#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

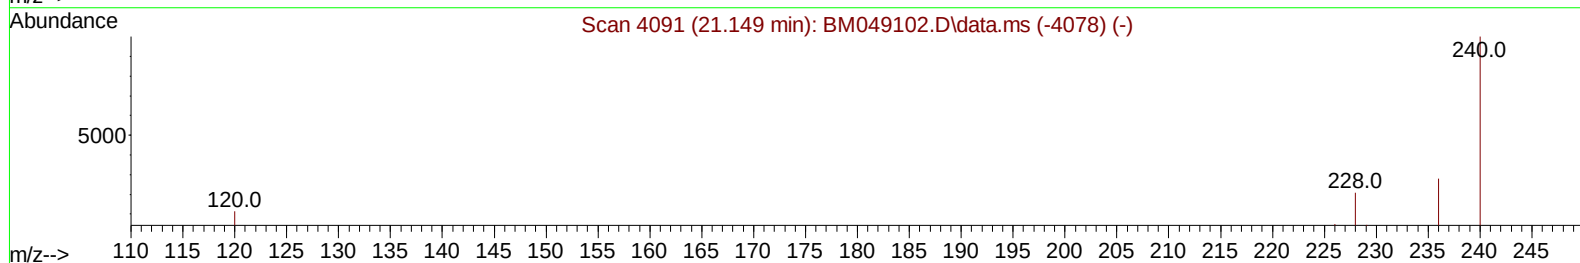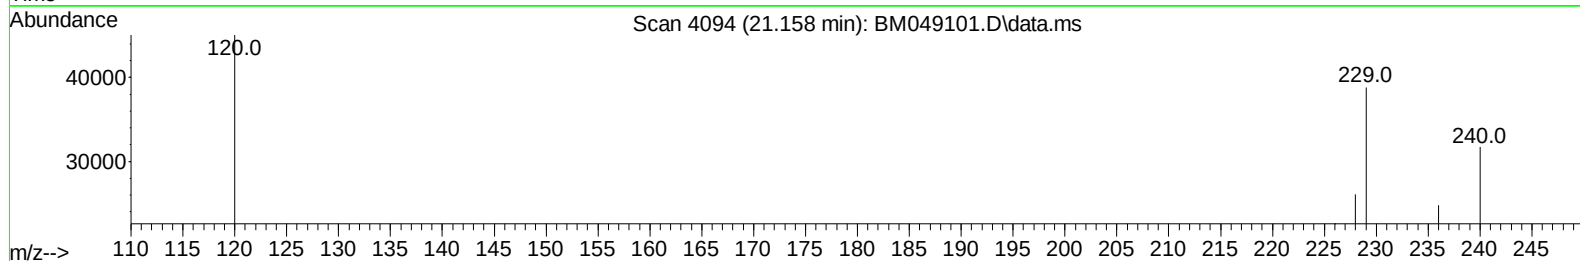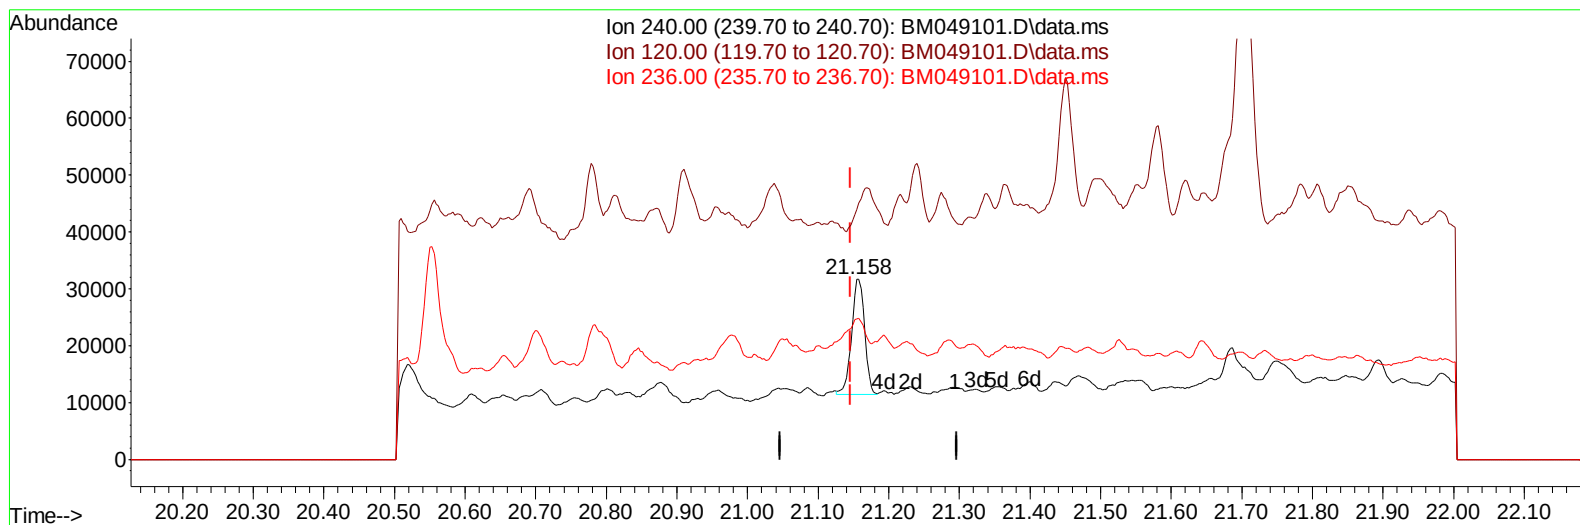

TIC: BM049101.D\data.ms

(17) Chrysene-d12

21.158min (+ 0.012) 0.40 ng/ul m

response 26055

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	14.50	142.07#
236.00	29.80	78.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

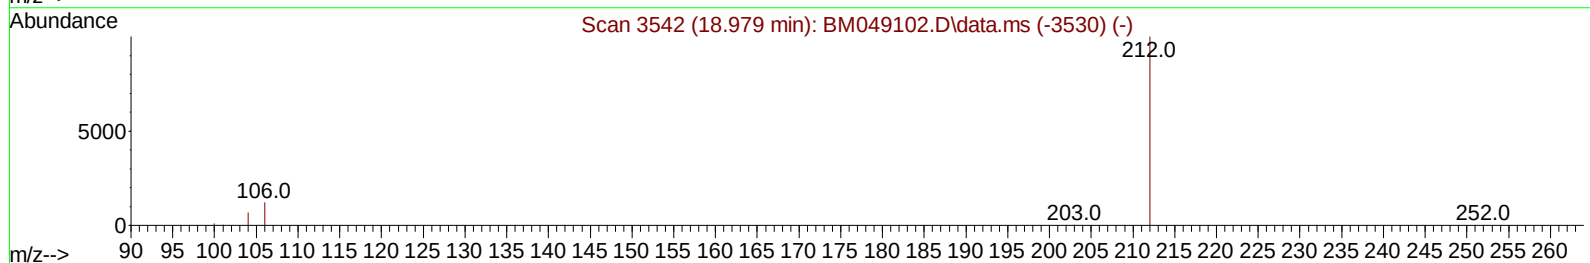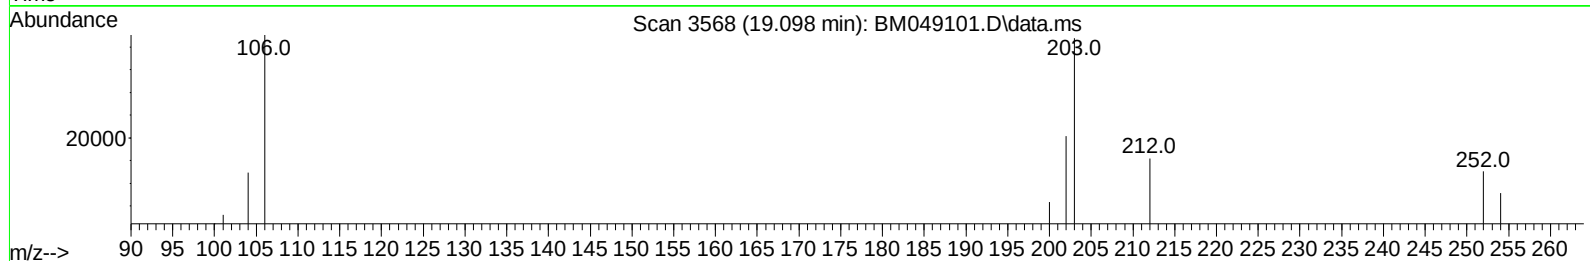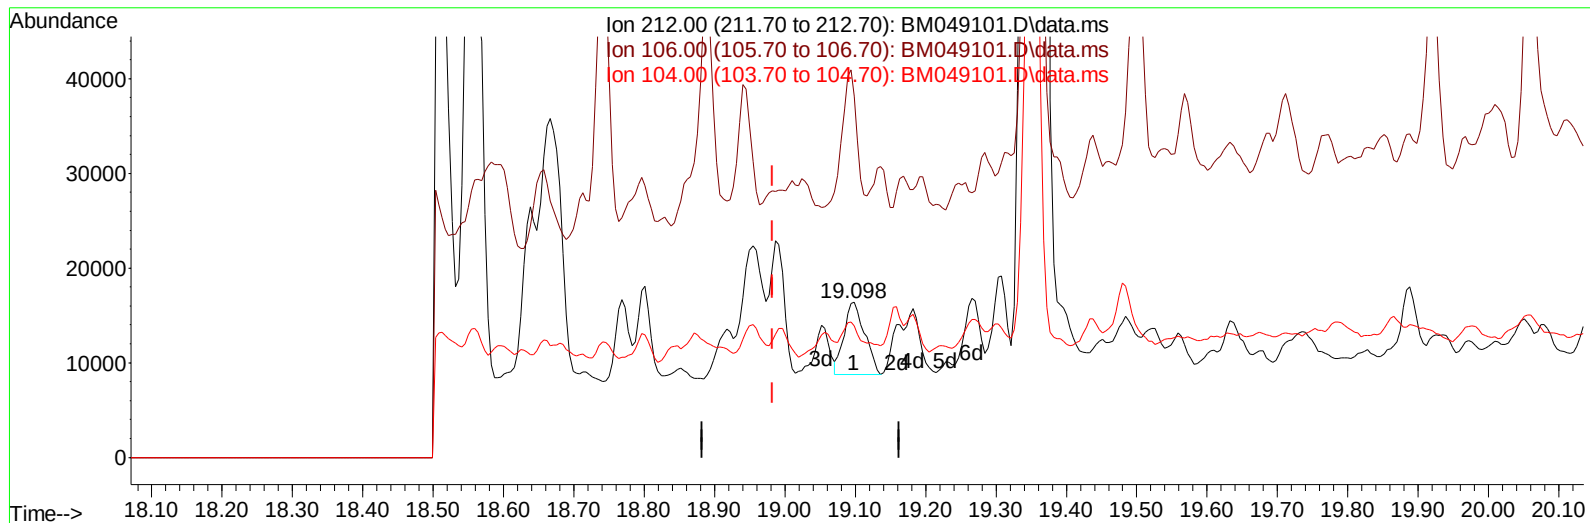

TIC: BM049101.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.098min (+ 0.116) 0.21 ng/u1

response 15552

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	11.60	136.73#
104.00	6.50	28.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

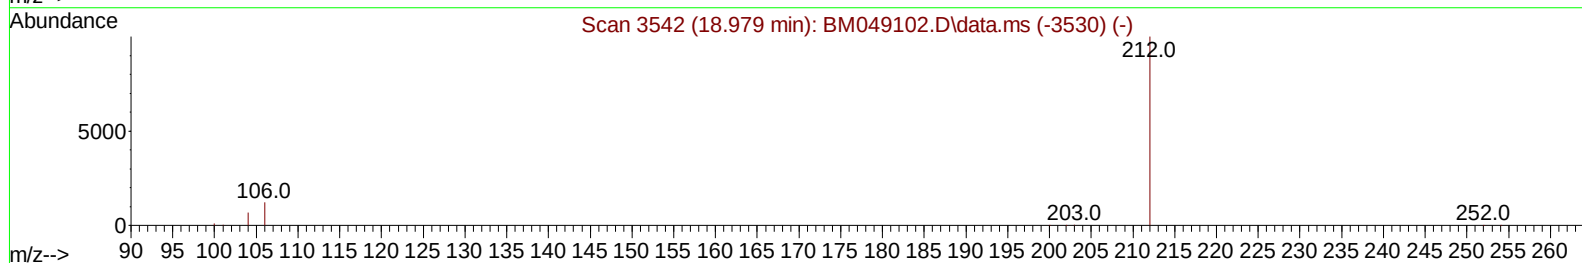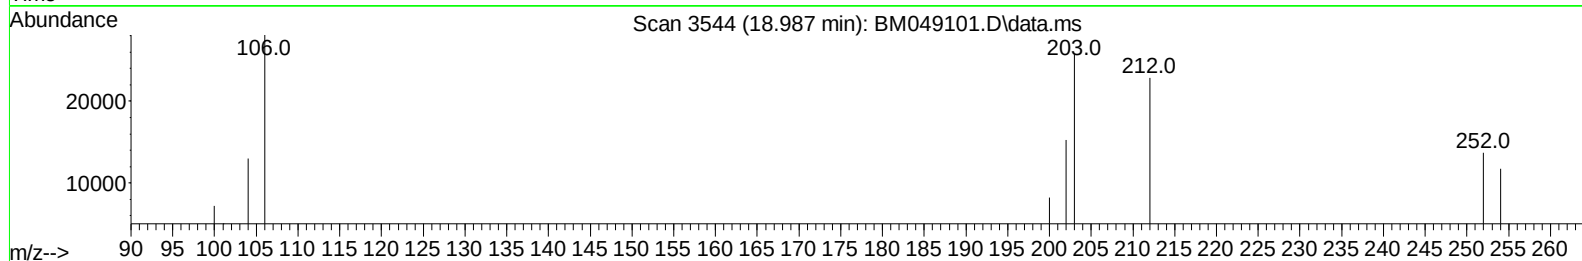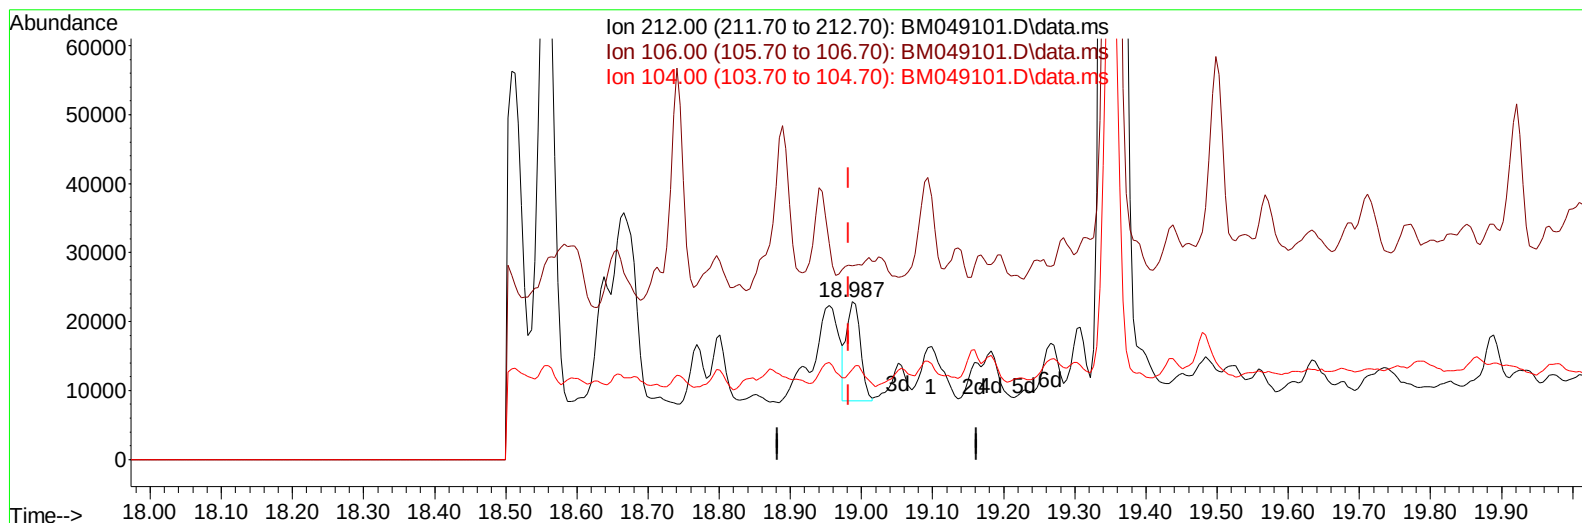

TIC: BM049101.D\data.ms

(18) Fluoranthene-d10 (SURR)

18.987min (+ 0.005) 0.26 ng/ul m

response 19425

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	11.60	109.47#
104.00	6.50	22.53#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
 Data File : BM049101.D
 Acq On : 20 Dec 2024 15:03
 Operator : RC/JU
 Sample : P5265-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
 Supervised By :mohammad ahmed 12/24/2024

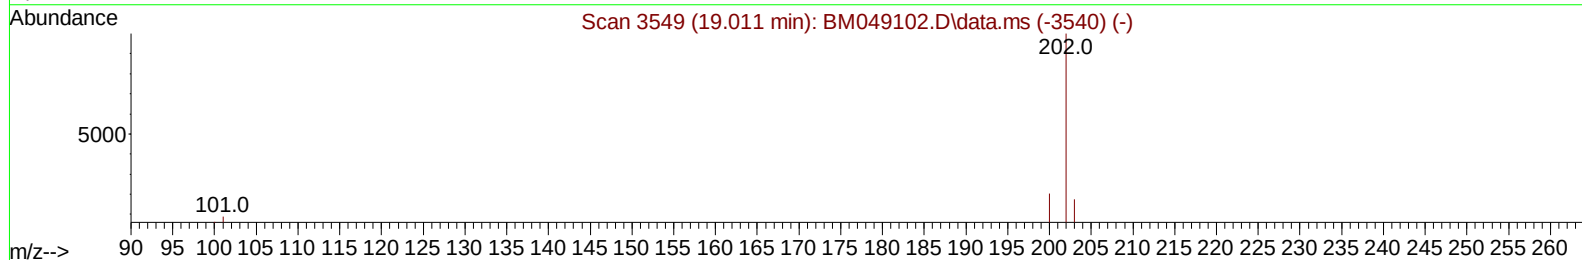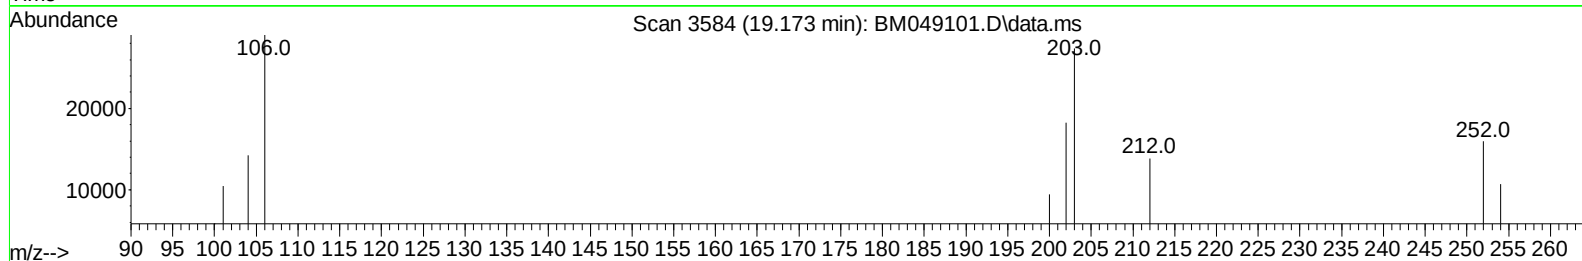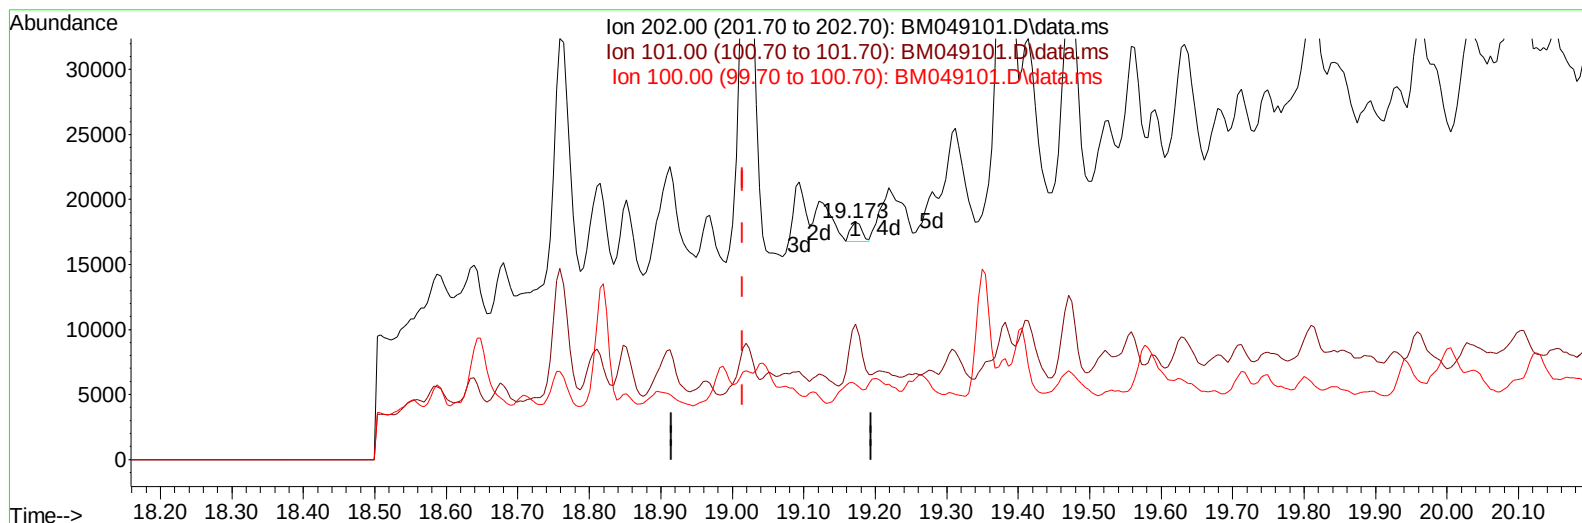

TIC: BM049101.D\data.ms

(19) Fluoranthene (C)

19.173min (+ 0.158) 0.02 ng/u1

response 1590

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	9.50	57.19#
100.00	6.90	31.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

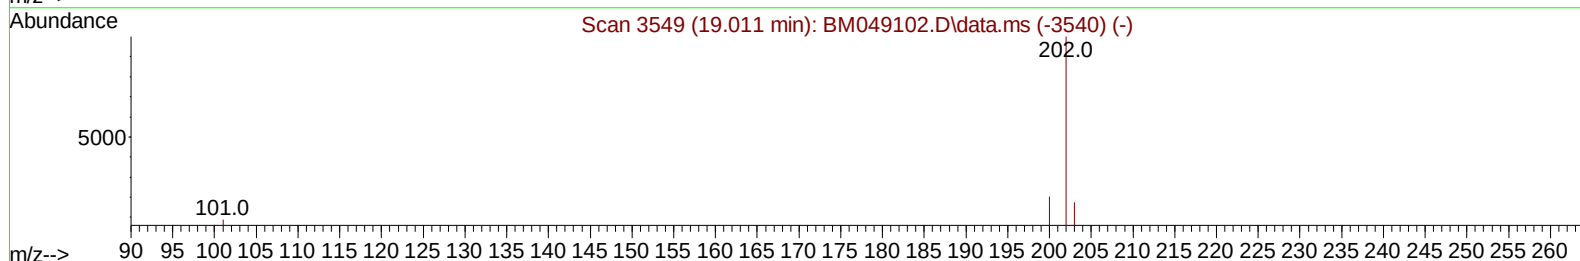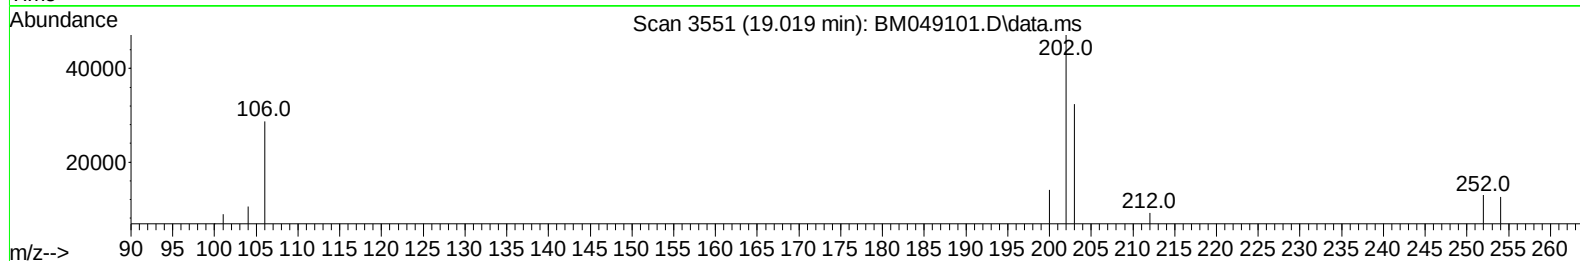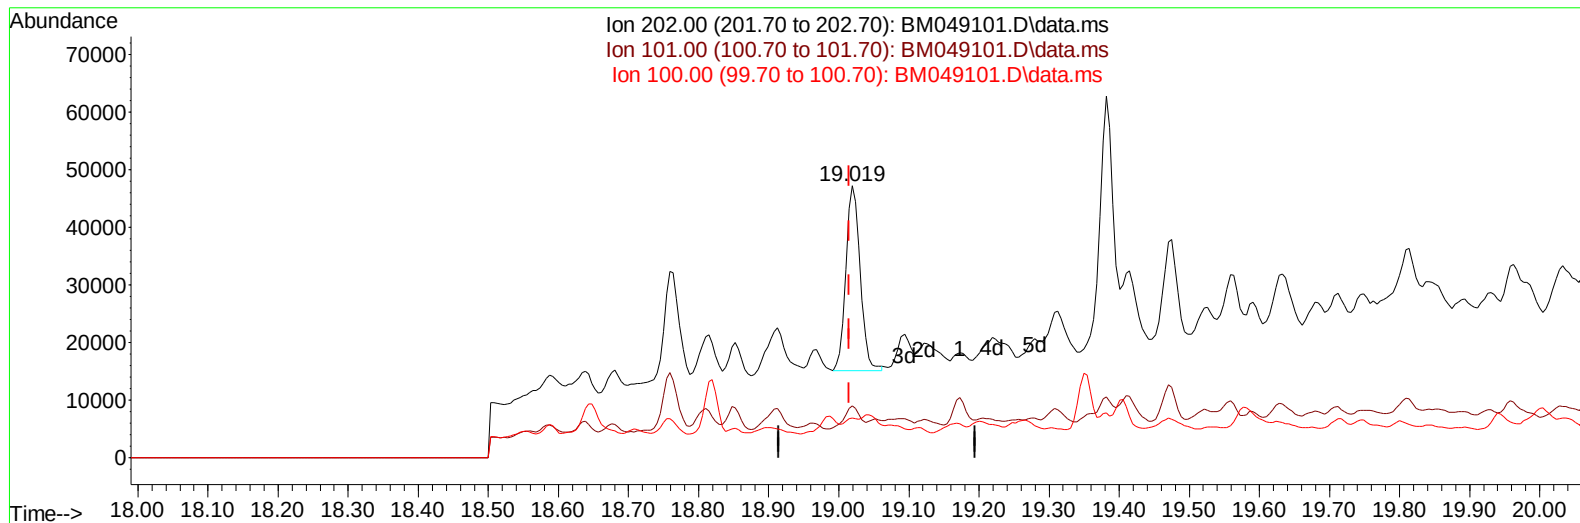

TIC: BM049101.D\data.ms

(19) Fluoranthene (C)

19.019min (+ 0.005) 0.49 ng/ul m

response 45997

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	9.50	18.97#
100.00	6.90	14.47#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

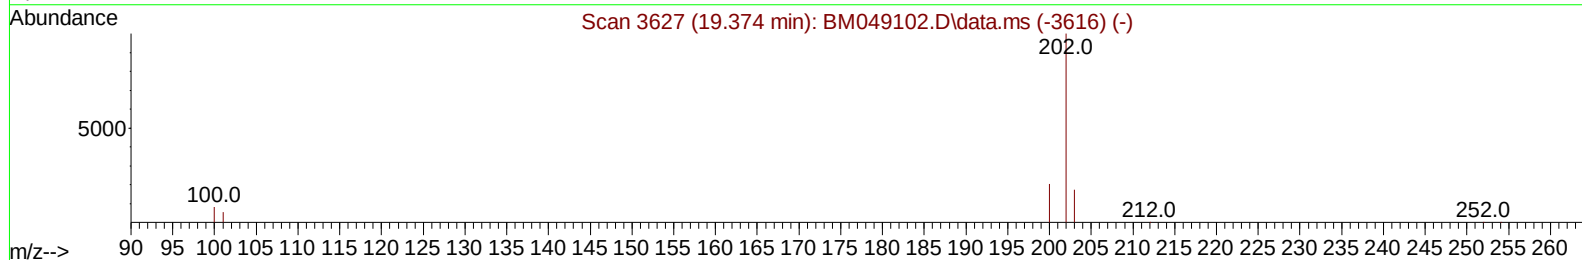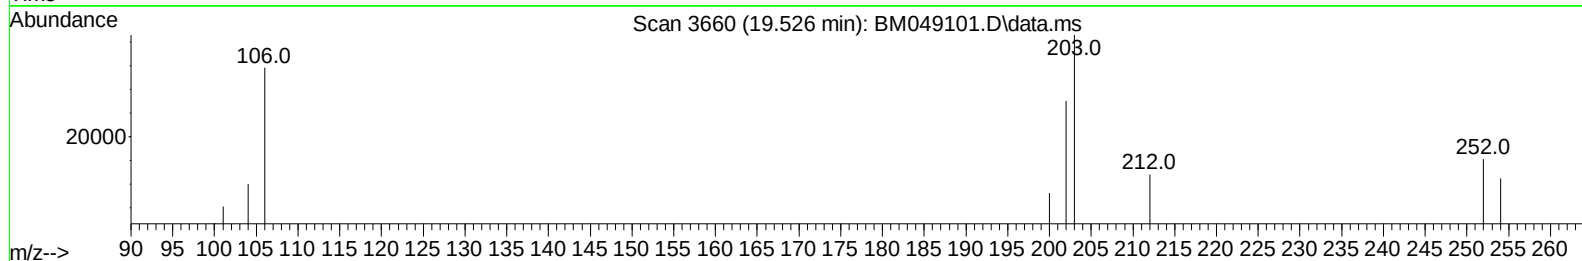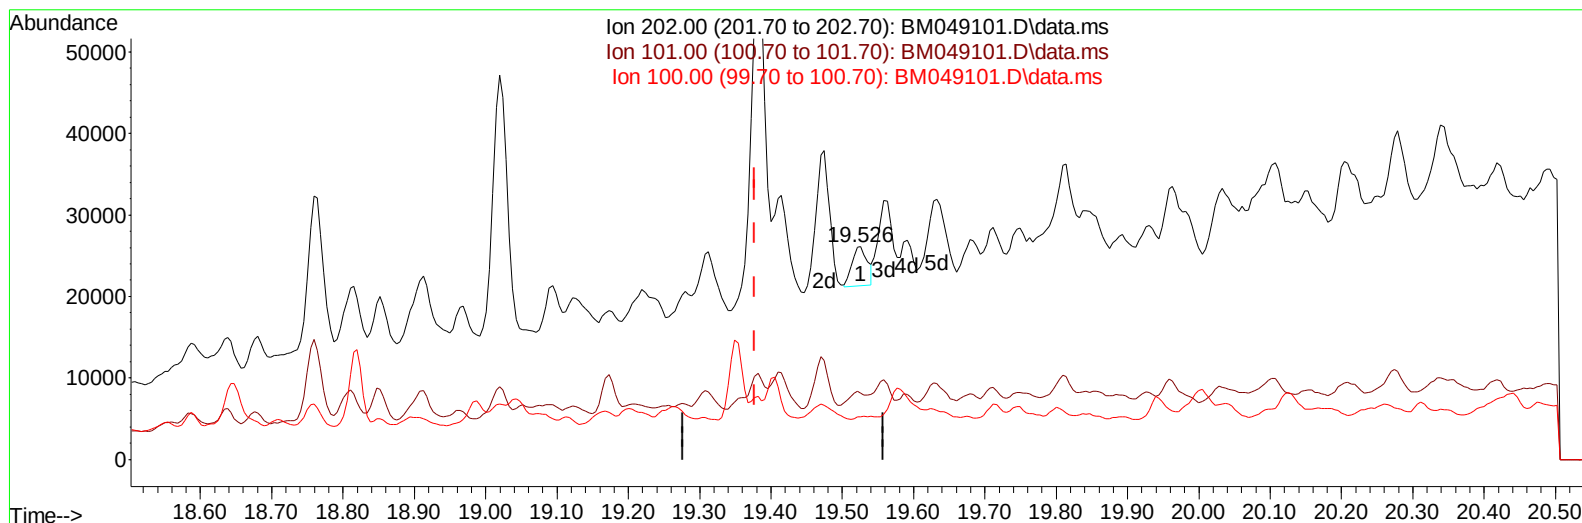

TIC: BM049101.D\data.ms

(20) Pyrene

19.526min (+ 0.149) 0.07 ng/u1

response 7284

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.10	31.17#
100.00	8.60	20.11#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

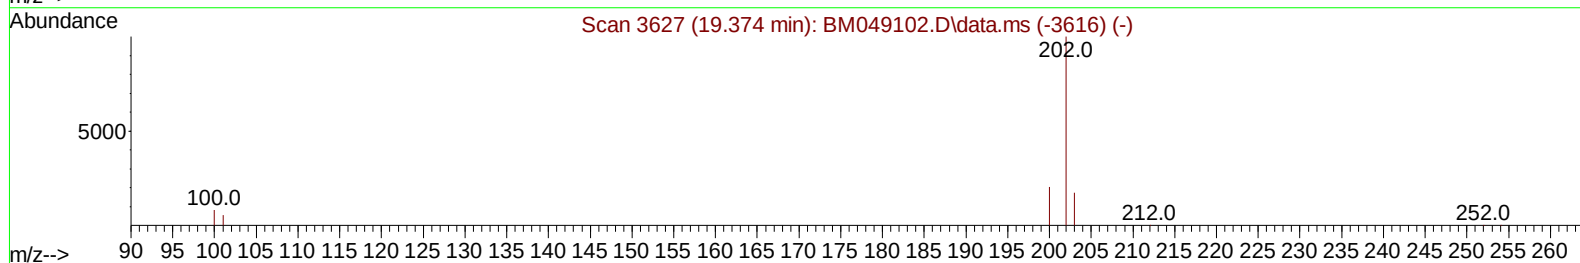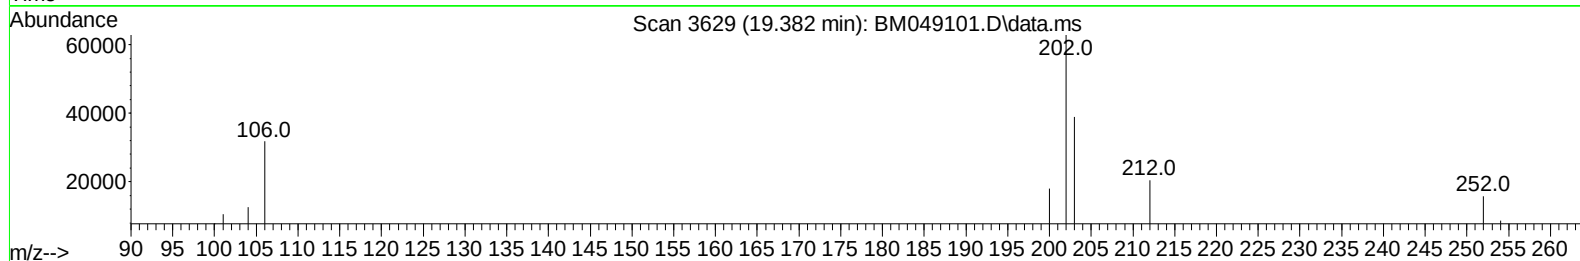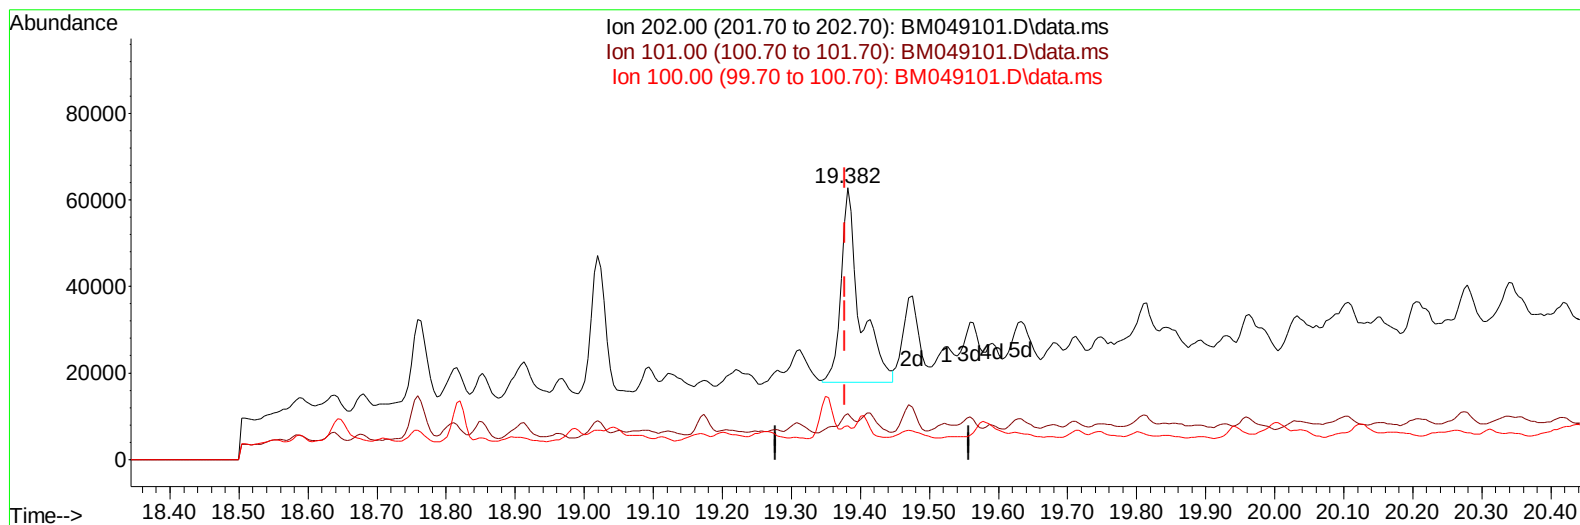

TIC: BM049101.D\data.ms

(20) Pyrene

19.382min (+ 0.005) 0.85 ng/ul m

response 85112

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.10	16.80#
100.00	8.60	12.32#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

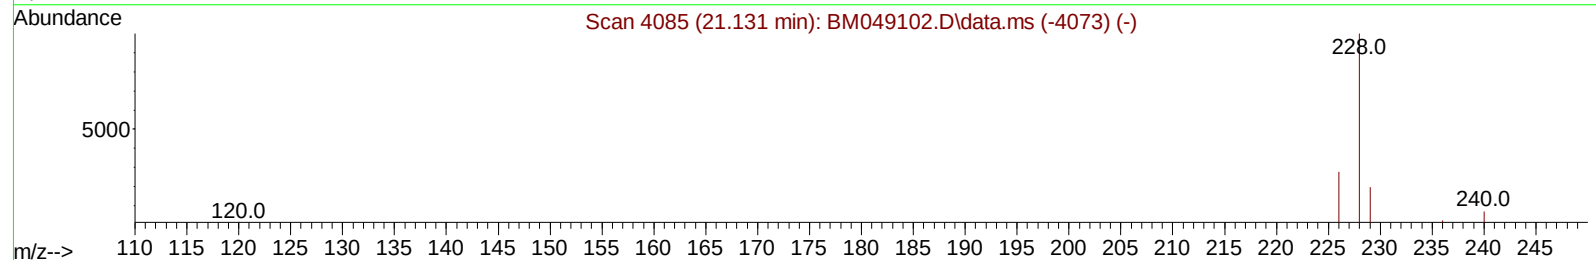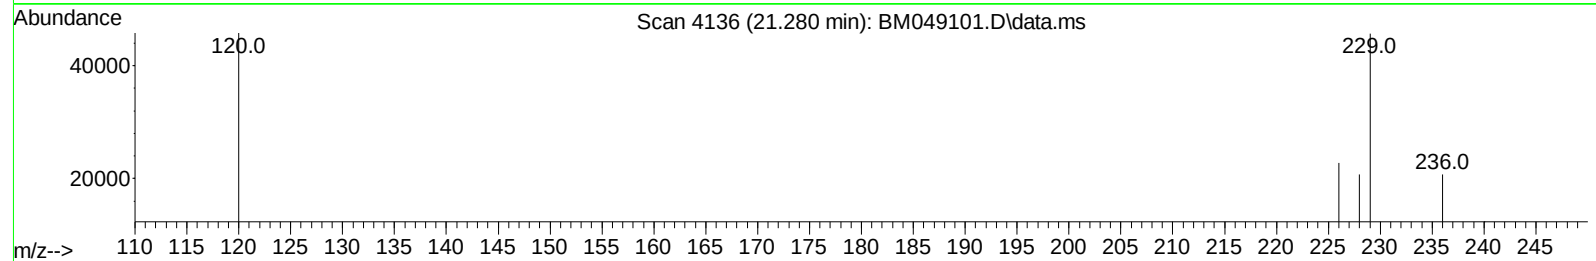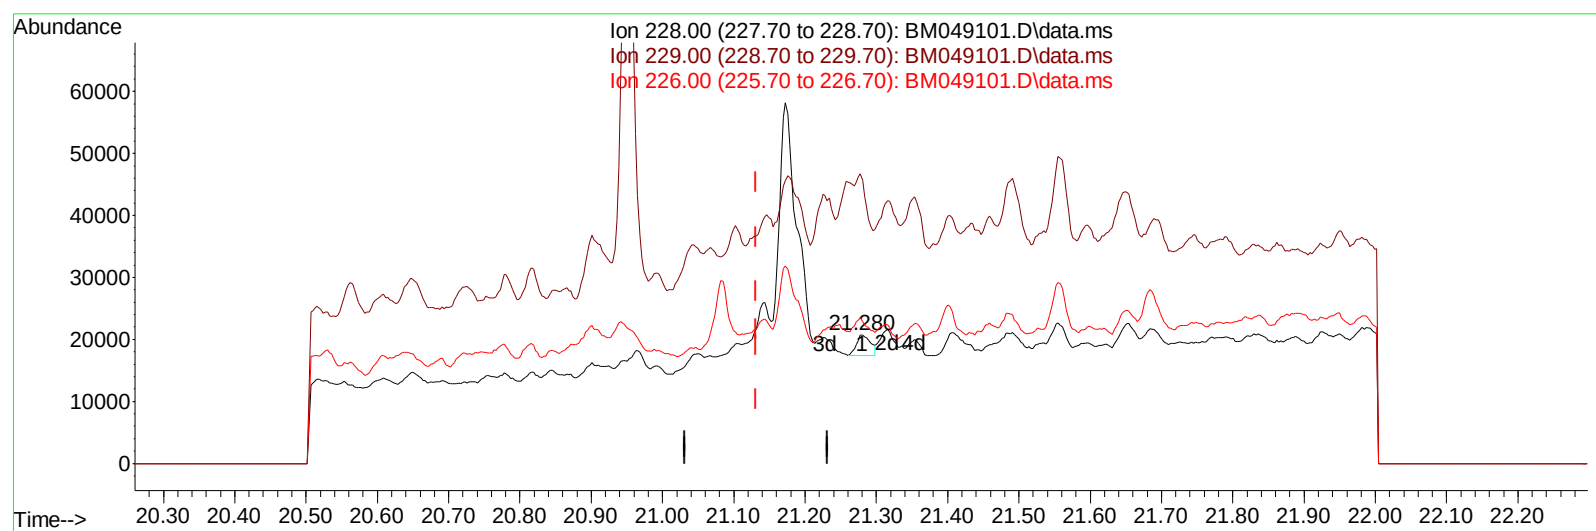

TIC: BM049101.D\data.ms

(21) Benzo(a)anthracene

21.280min (+ 0.149) 0.05 ng/u1

response 4651

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.90	220.22#
226.00	28.30	110.11#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

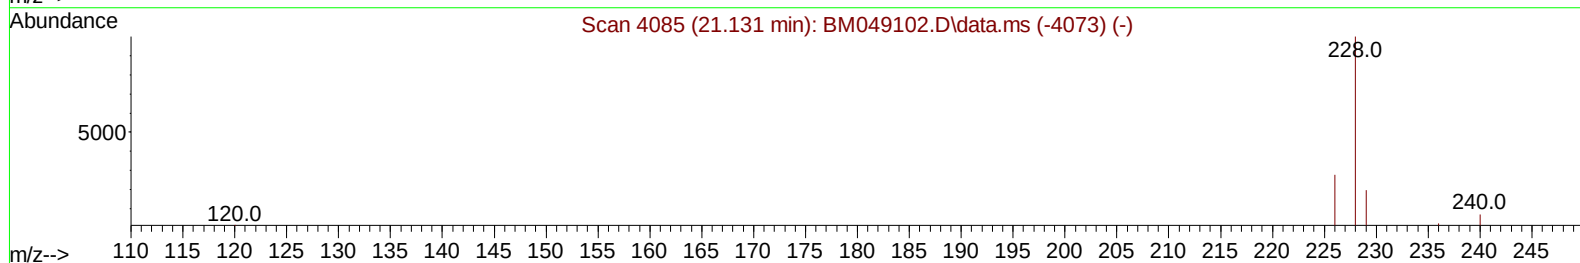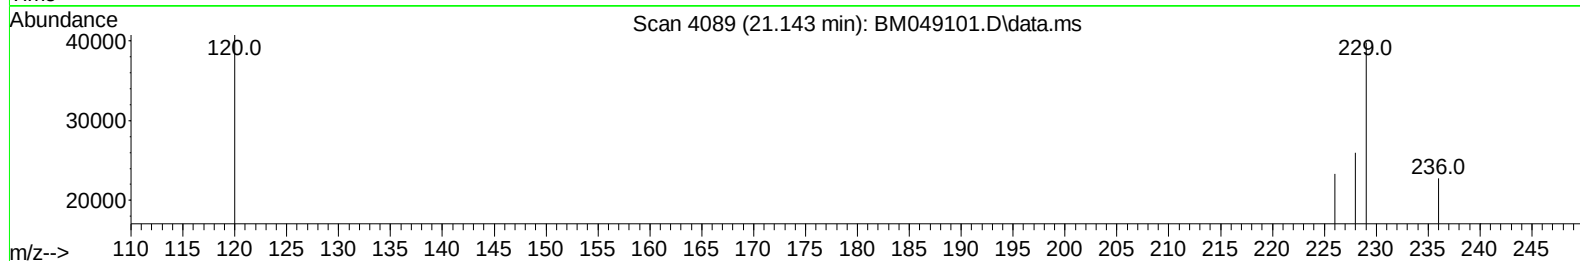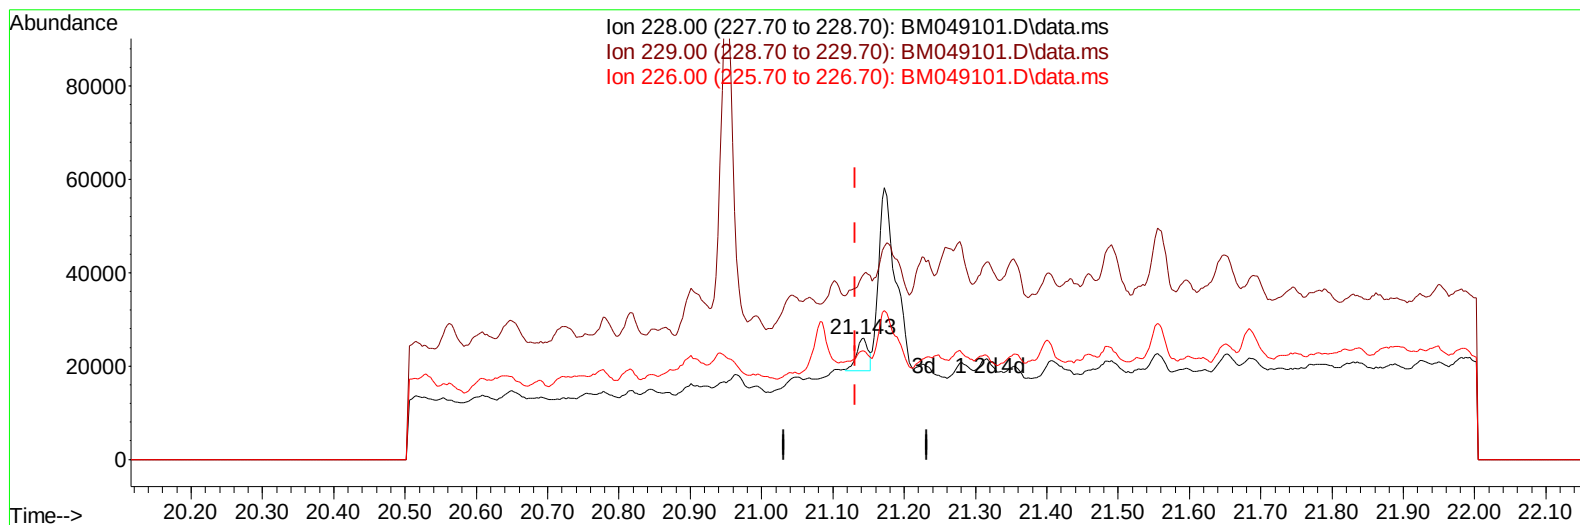

TIC: BM049101.D\data.ms

(21) Benzo(a)anthracene

21.143min (+ 0.012) 0.09 ng/ul m

response 7994

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.90	153.36#
226.00	28.30	89.85#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

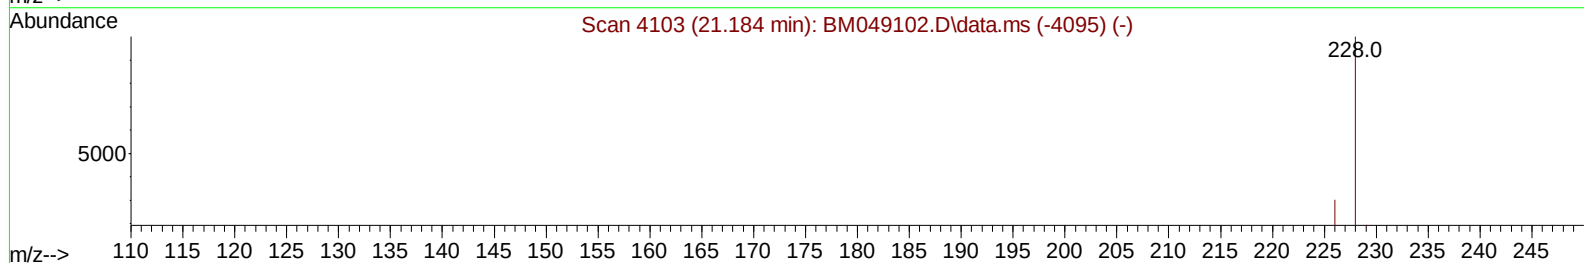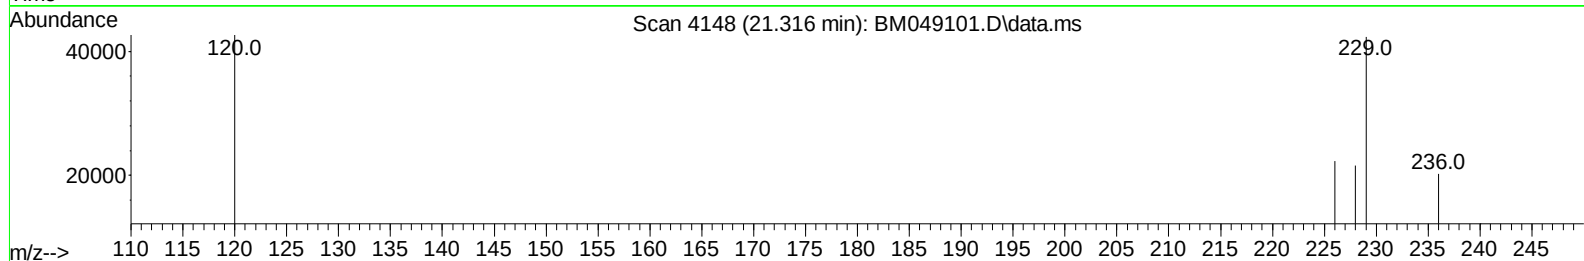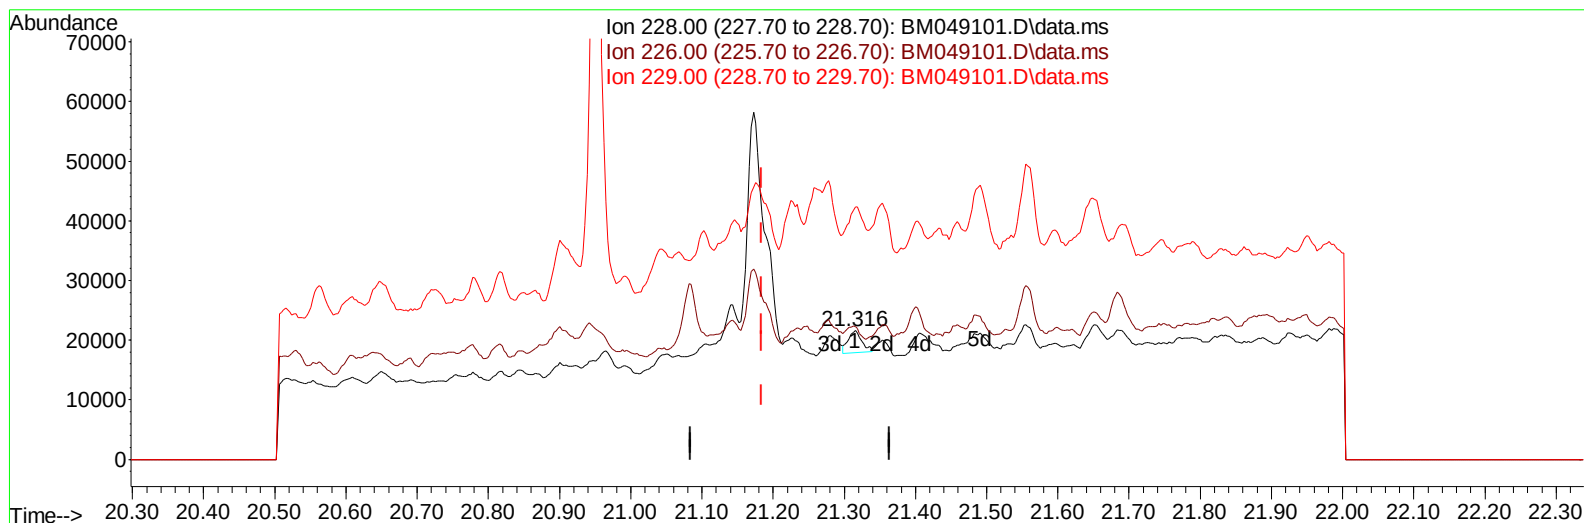

TIC: BM049101.D\data.ms

(22) Chrysene

21.316min (+ 0.131) 0.05 ng/u1

response 4919

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.10	103.33#
229.00	19.80	196.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 3

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

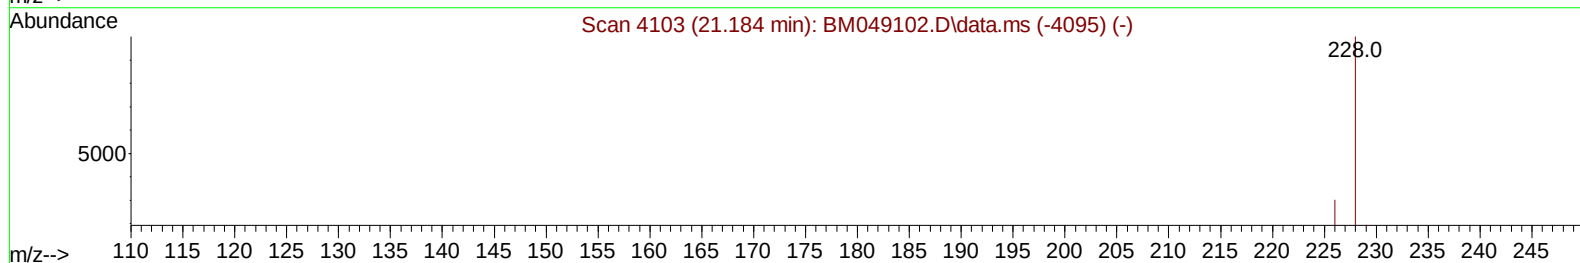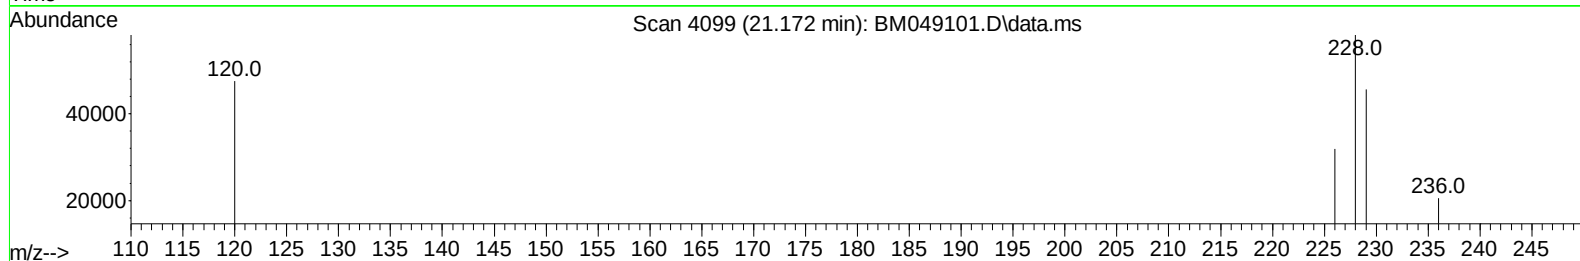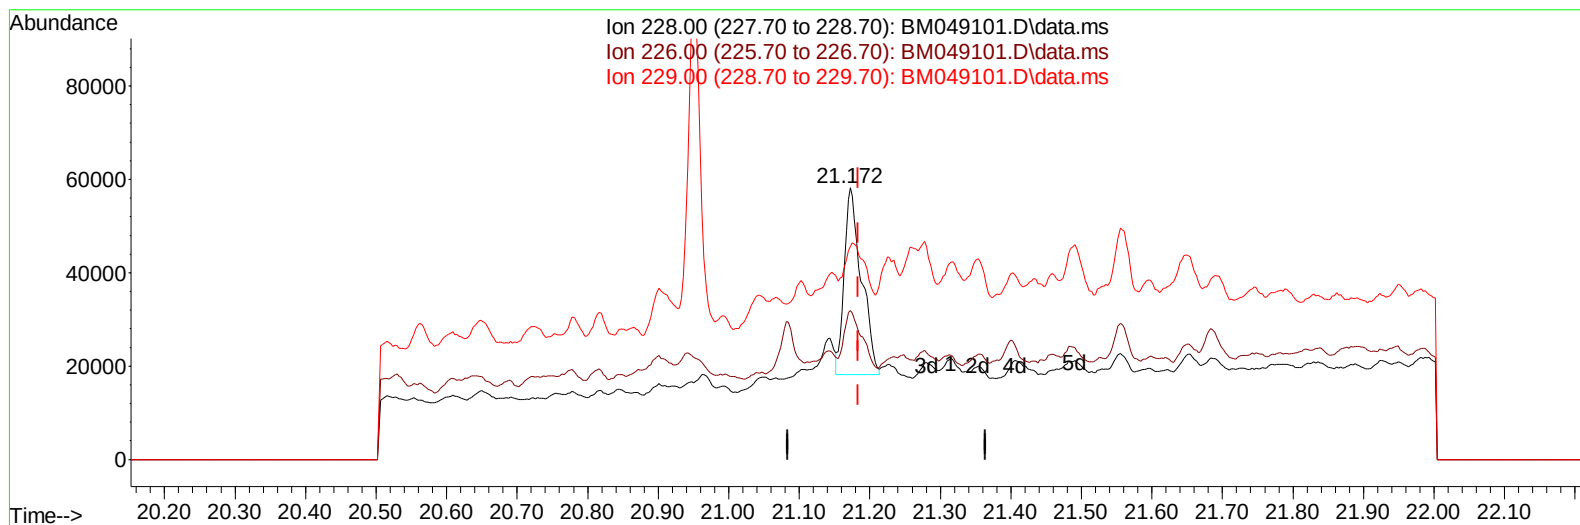

TIC: BM049101.D\data.ms

(22) Chrysene

21.172min (-0.012) 0.69 ng/ul m

response 67465

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.10	54.81#
229.00	19.80	78.42#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

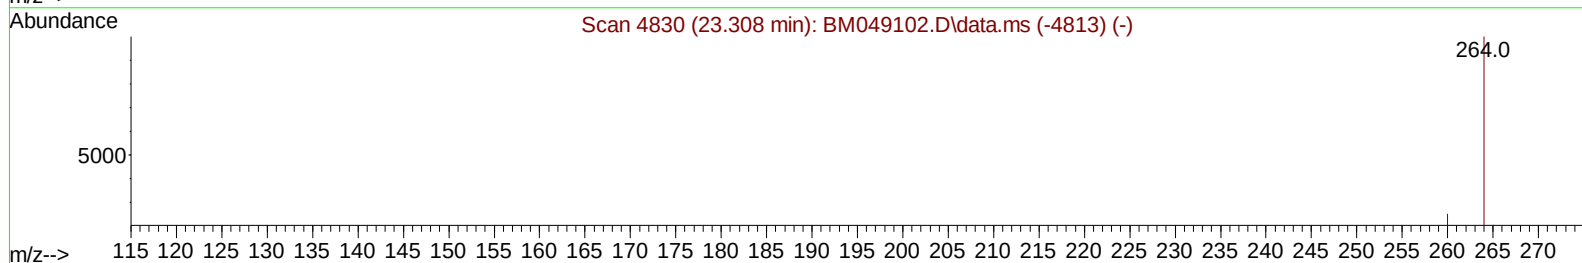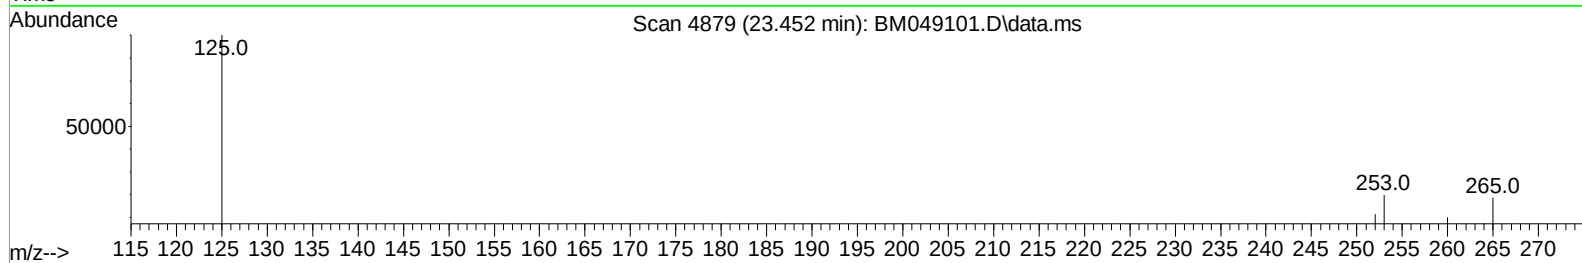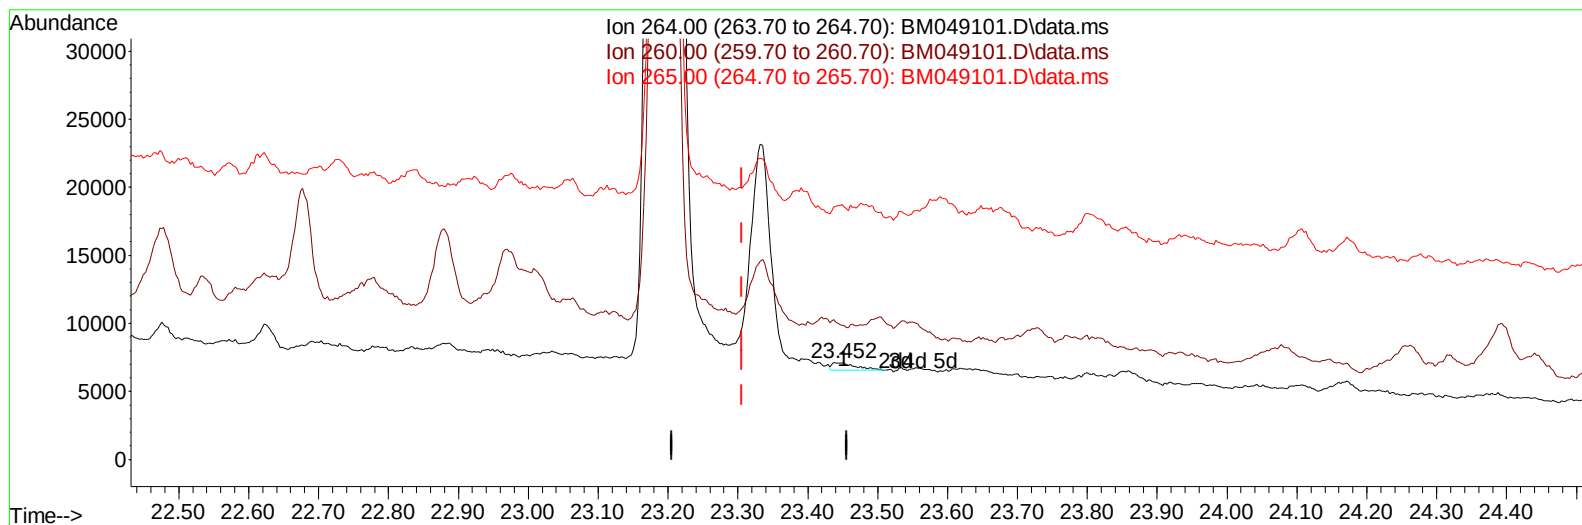

TIC: BM049101.D\data.ms

(23) Perylene-d12 (I)

23.452min (+ 0.146) 0.40 ng/u1

response 1301

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	138.09#
265.00	78.30	260.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

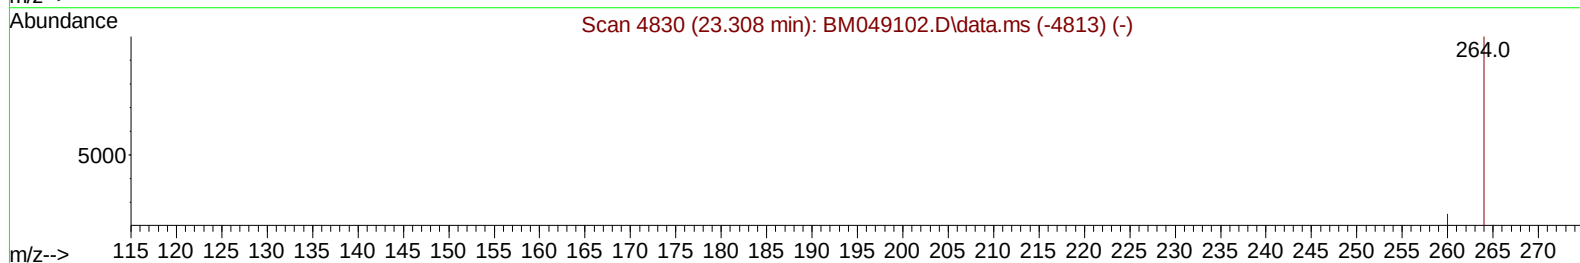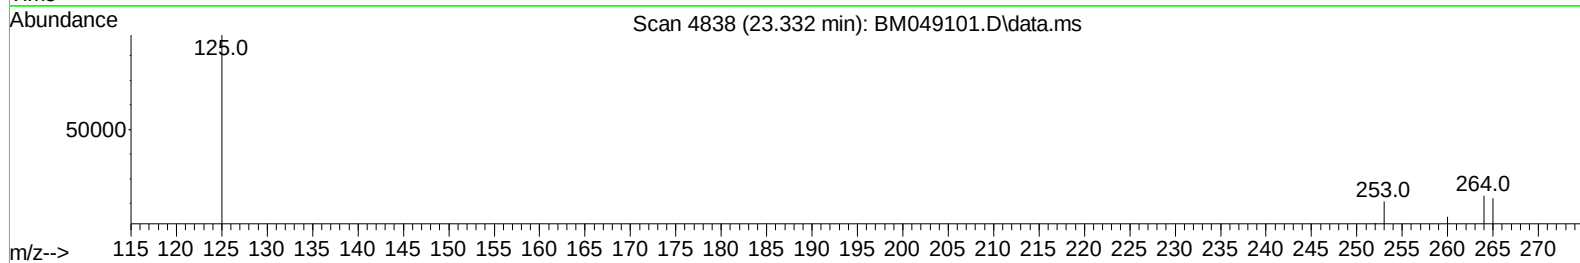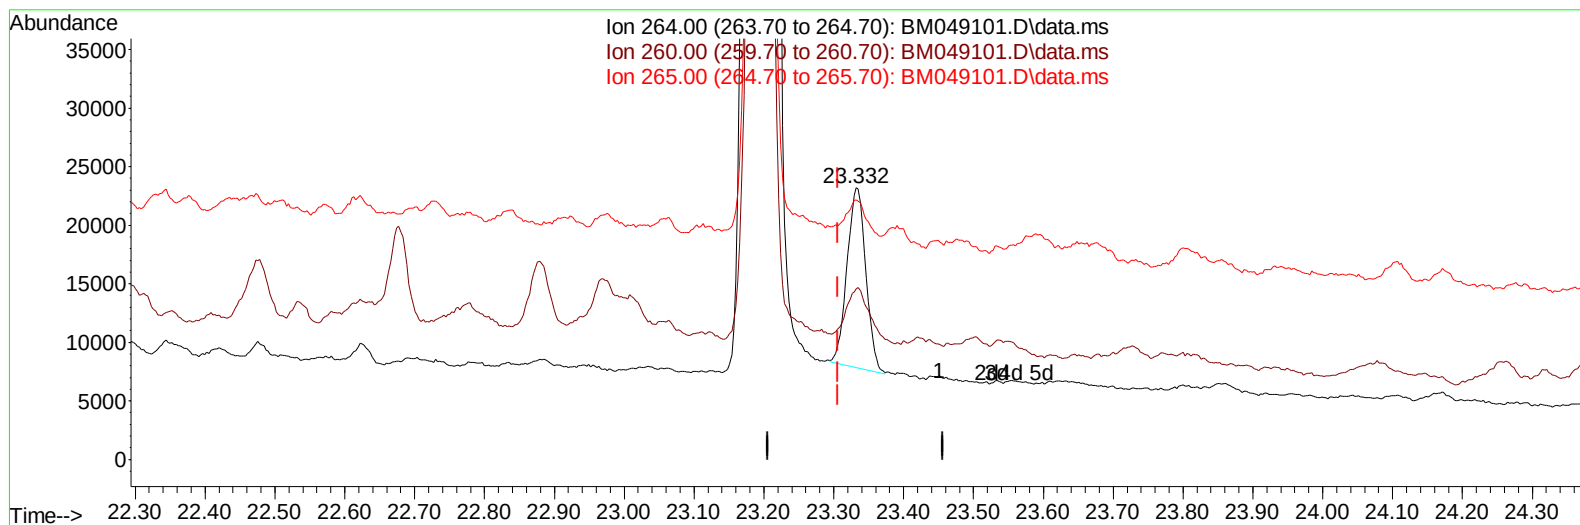

TIC: BM049101.D\data.ms

(23) Perylene-d12 (I)

23.332min (+ 0.026) 0.40 ng/ul m

response 28482

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	62.84#
265.00	78.30	95.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

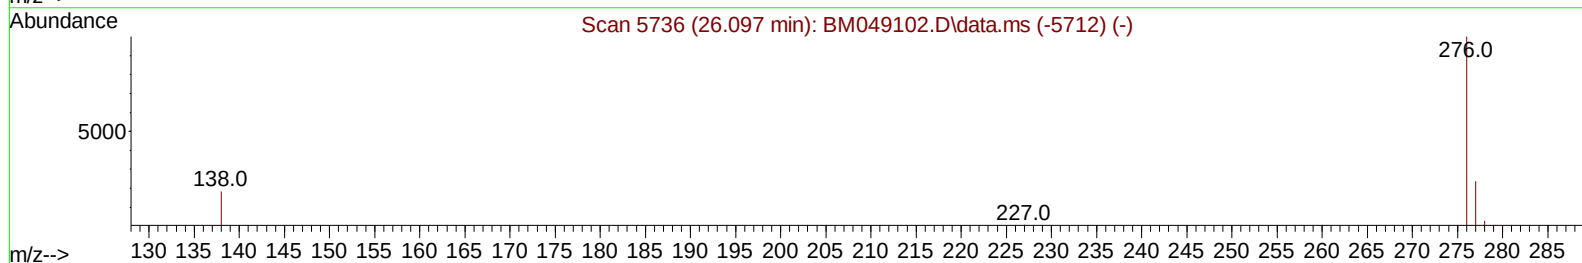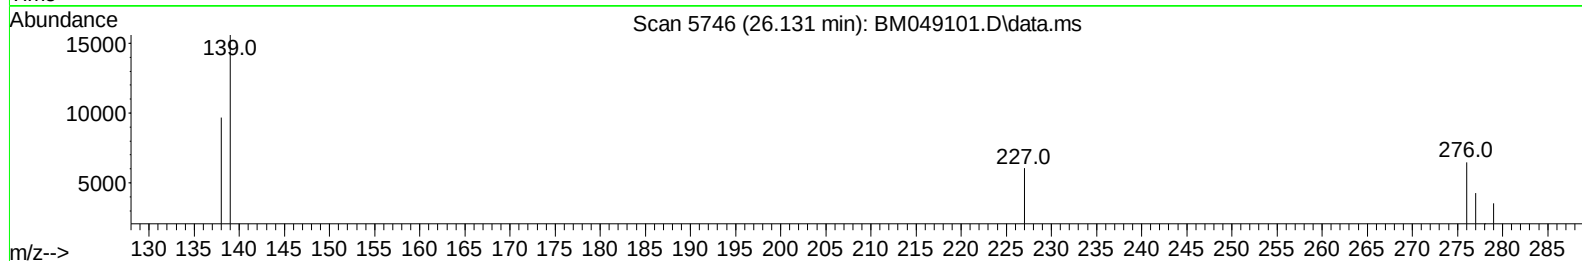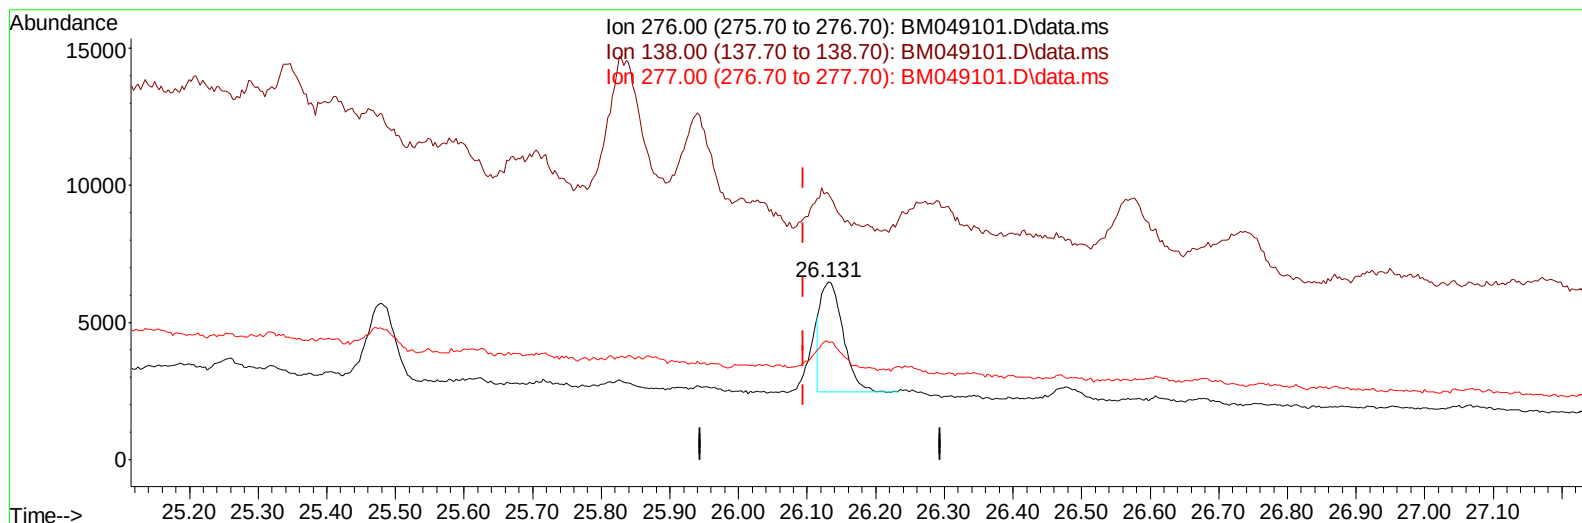

TIC: BM049101.D\data.ms

(29) Benzo(g,h,i)perylene

26.131min (+ 0.037) 0.09 ng/u1

response 9210

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	20.90	149.23#
277.00	24.90	65.68#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

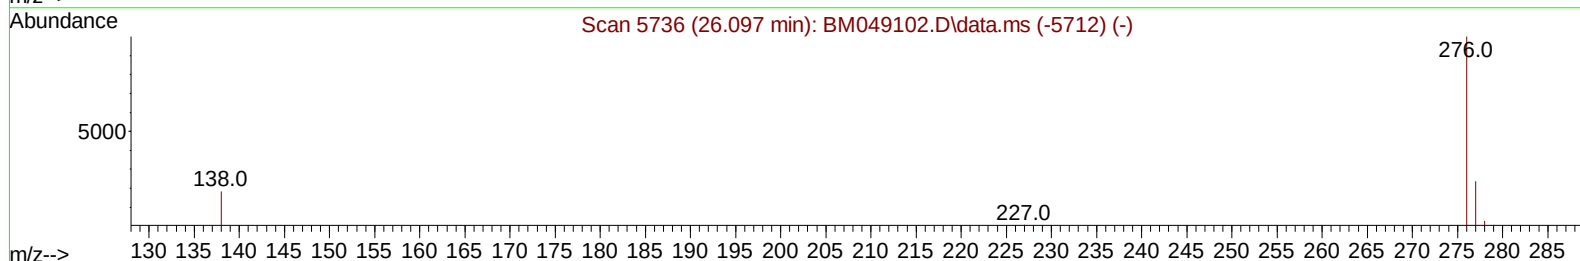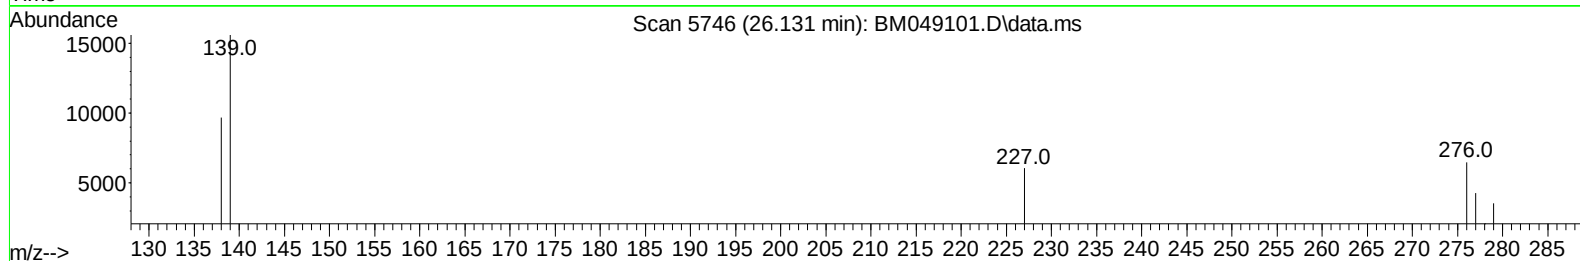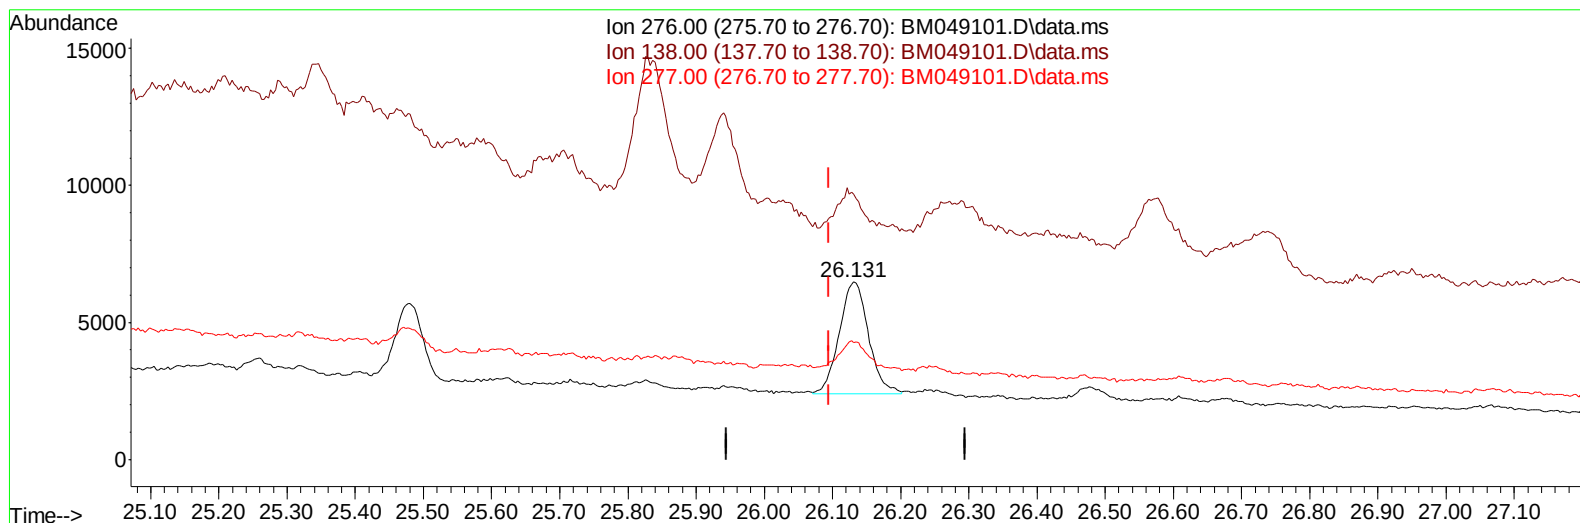

TIC: BM049101.D\data.ms

(29) Benzo(g,h,i)perylene

26.131min (+ 0.037) 0.12 ng/u1 m

response 12235

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	20.90	149.23#
277.00	24.90	65.68#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
 Data File : BM049101.D
 Acq On : 20 Dec 2024 15:03
 Operator : RC/JU
 Sample : P5265-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E28Z9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
 Supervised By :mohammad ahmed 12/24/2024

Quant Time: Dec 21 04:17:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.560	152		8189	0.400	ng/ul	0.00
4) Naphthalene-d8	10.319	136		25525	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.195	164		19961	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.946	188		32439m	0.400	ng/ul	0.00
17) Chrysene-d12	21.158	240		26055m	0.400	ng/ul	0.01
23) Perylene-d12	23.332	264		28482m	0.400	ng/ul	0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.151	96		31246	3.308	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.919	152		7143	0.208	ng/ul	0.00
18) Fluoranthene-d10	18.987	212		19425m	0.263	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.369	128		8546	0.134	ng/ul#	91
7) 2-Methylnaphthalene	11.991	142		21018	0.519	ng/ul	99
8) 1-Methylnaphthalene	12.216	142		21713	0.524	ng/ul	92
10) Acenaphthylene	13.927	152		8557	0.103	ng/ul#	1
11) Acenaphthene	14.256	153		4275	0.071	ng/ul#	74
12) Fluorene	15.250	166		25579	0.375	ng/ul#	58
15) Phenanthrene	16.988	178		181996m	2.148	ng/ul	
19) Fluoranthene	19.019	202		45997m	0.488	ng/ul	
20) Pyrene	19.382	202		85112m	0.847	ng/ul	
21) Benzo(a)anthracene	21.143	228		7994m	0.088	ng/ul	
22) Chrysene	21.172	228		67465m	0.694	ng/ul	
29) Benzo(g,h,i)perylene	26.131	276		12235m	0.123	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122024\
Data File : BM049101.D
Acq On : 20 Dec 2024 15:03
Operator : RC/JU
Sample : P5265-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E28Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 21 04:17:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

