




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

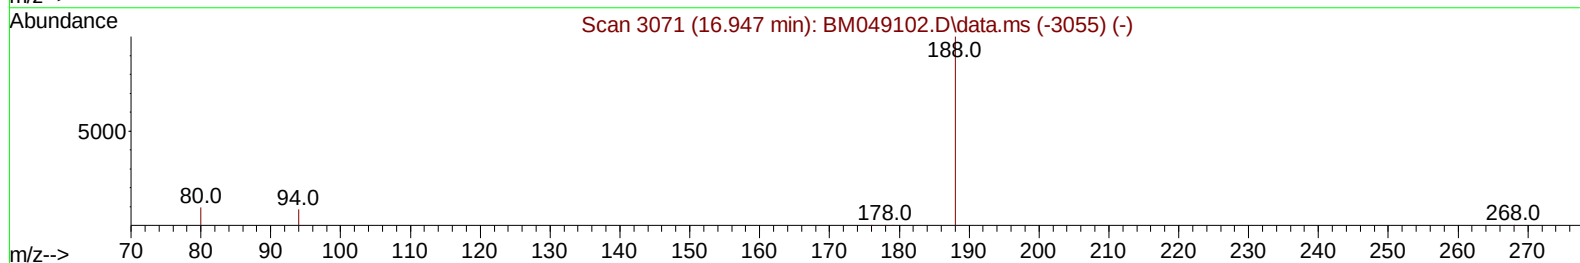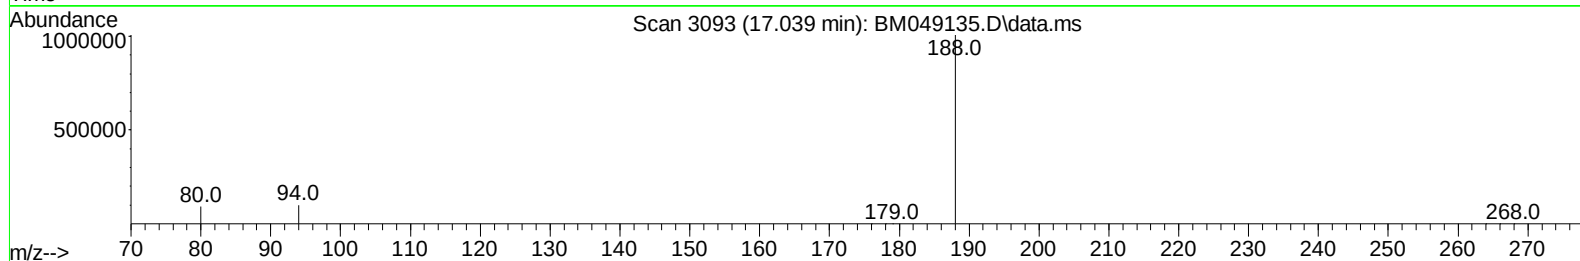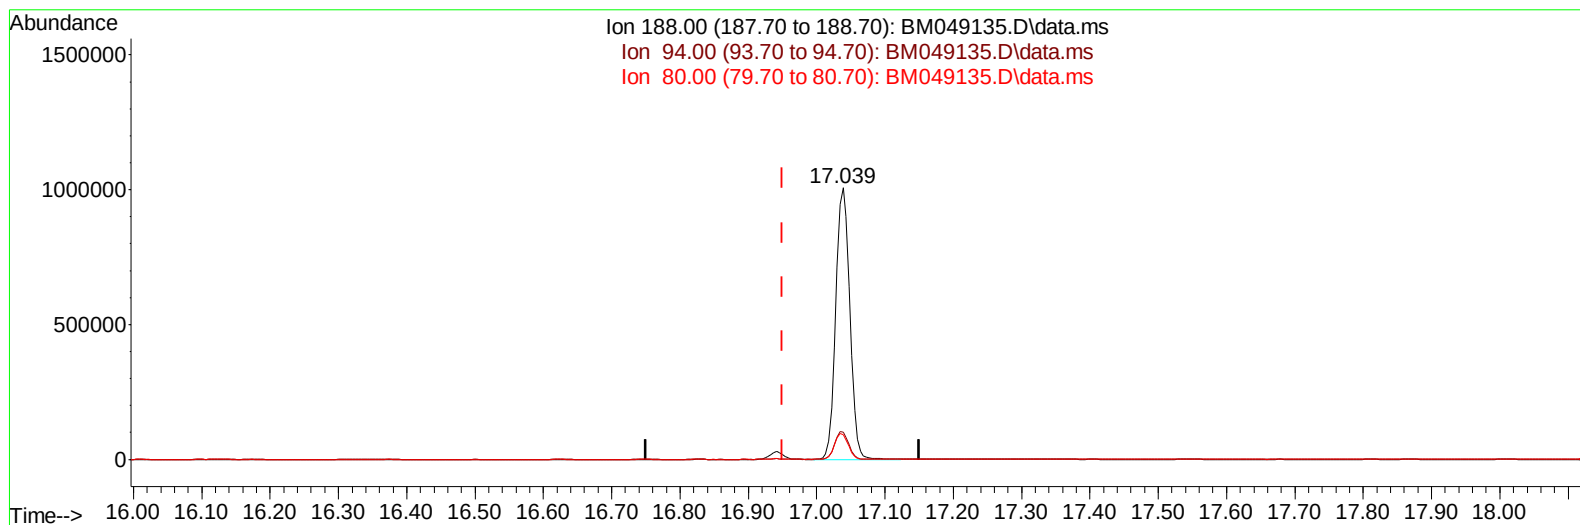

TIC: BM049135.D\data.ms

**(13) Phenanthrene-d10 (I)**

**17.039min (+ 0.089) 0.40 ng/u1**

**response 1426055**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 188.00 | 100.00 | 100.00 |
| 94.00  | 9.80   | 9.96   |
| 80.00  | 10.70  | 9.15   |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

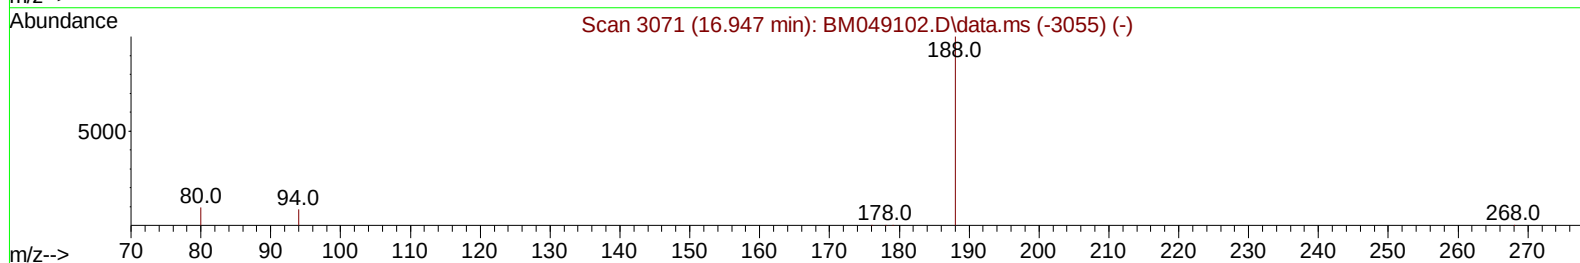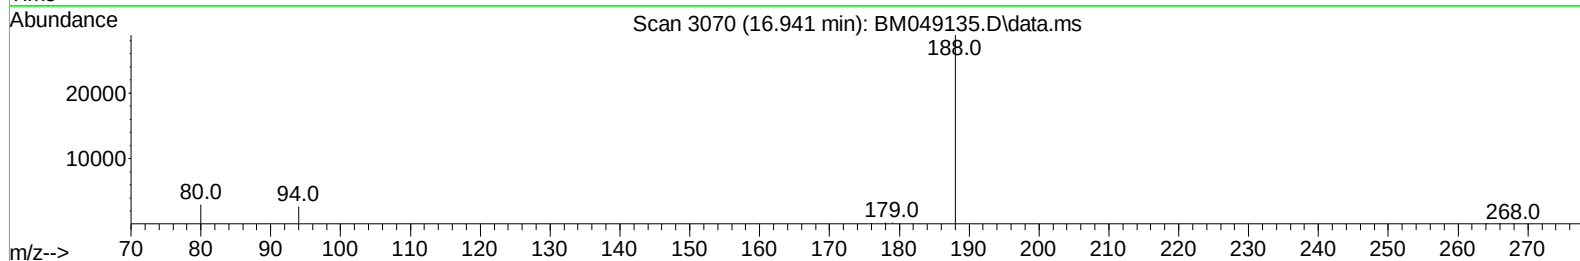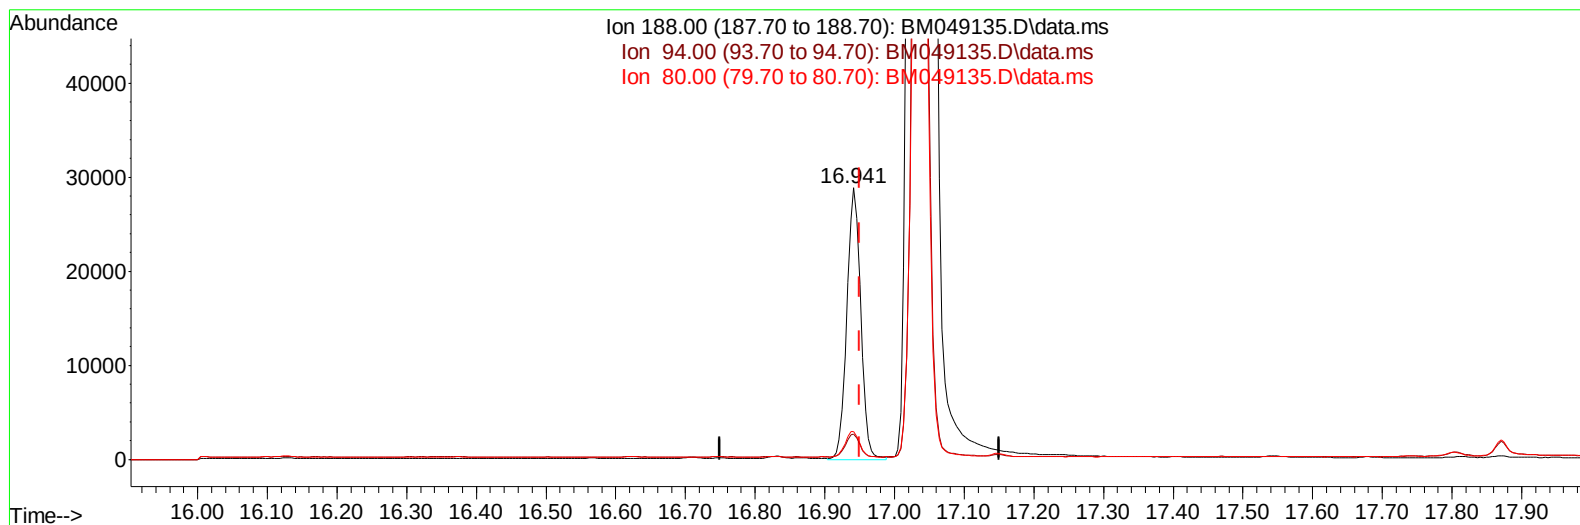

TIC: BM049135.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-0.008) 0.40 ng/ul m

response 39950

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 188.00 | 100.00 | 100.00 |
| 94.00  | 9.80   | 9.44   |
| 80.00  | 10.70  | 10.35  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

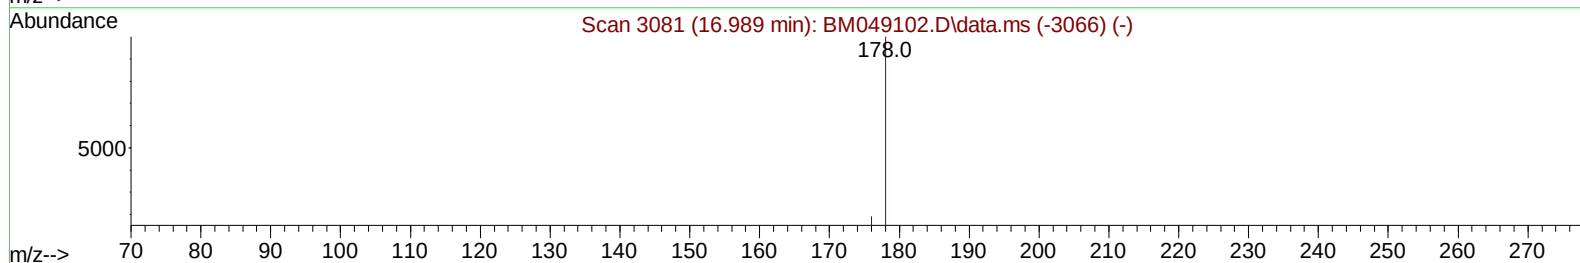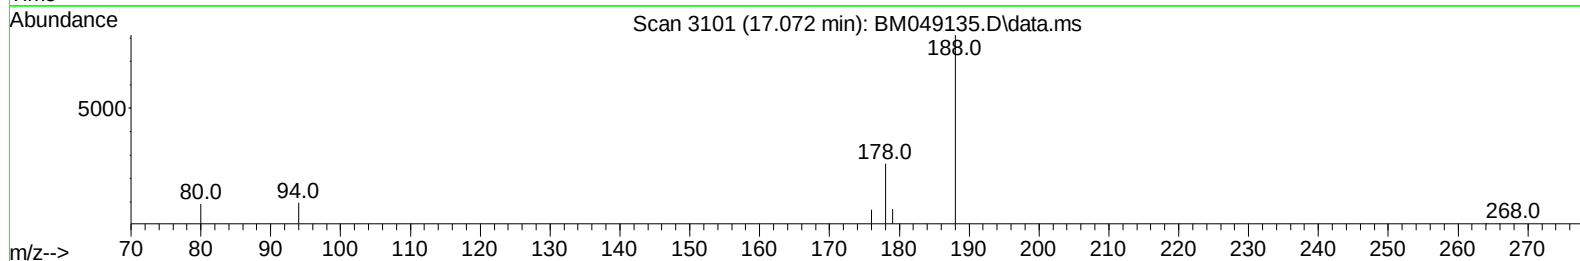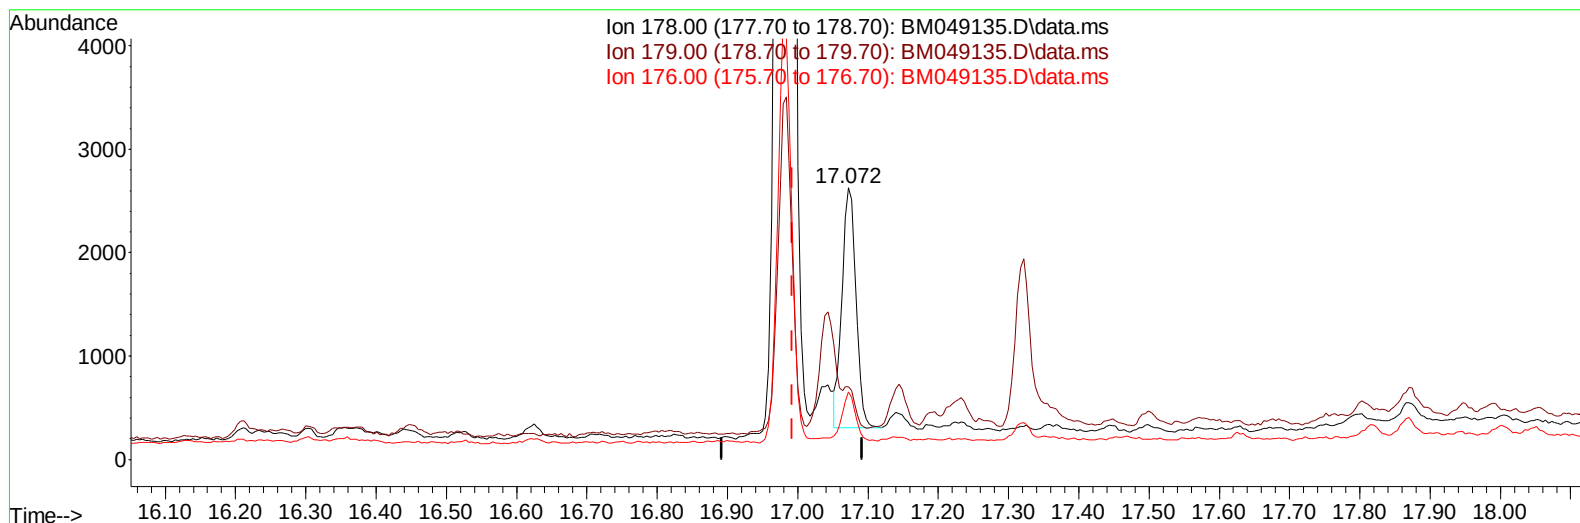

TIC: BM049135.D\data.ms

(15) Phenanthrene

17.072min (+ 0.080) 0.03 ng/u1

response 3220

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 178.00 | 100.00 | 100.00 |
| 179.00 | 16.20  | 26.69# |
| 176.00 | 20.20  | 24.90# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

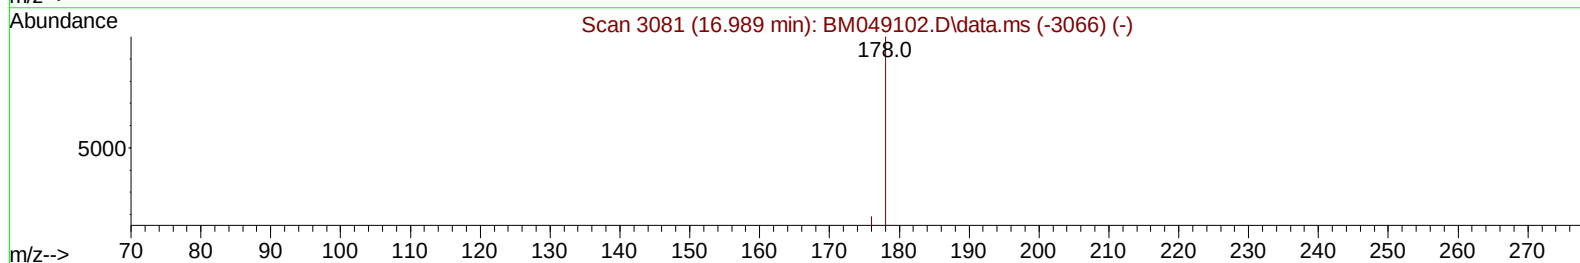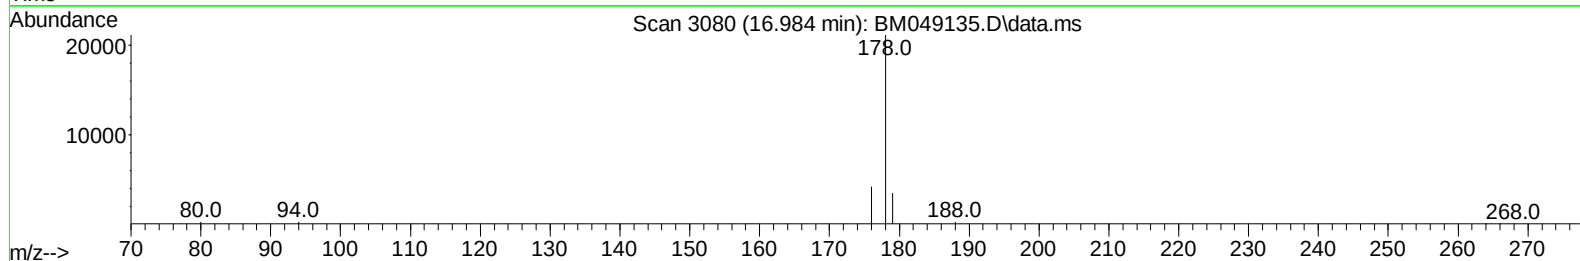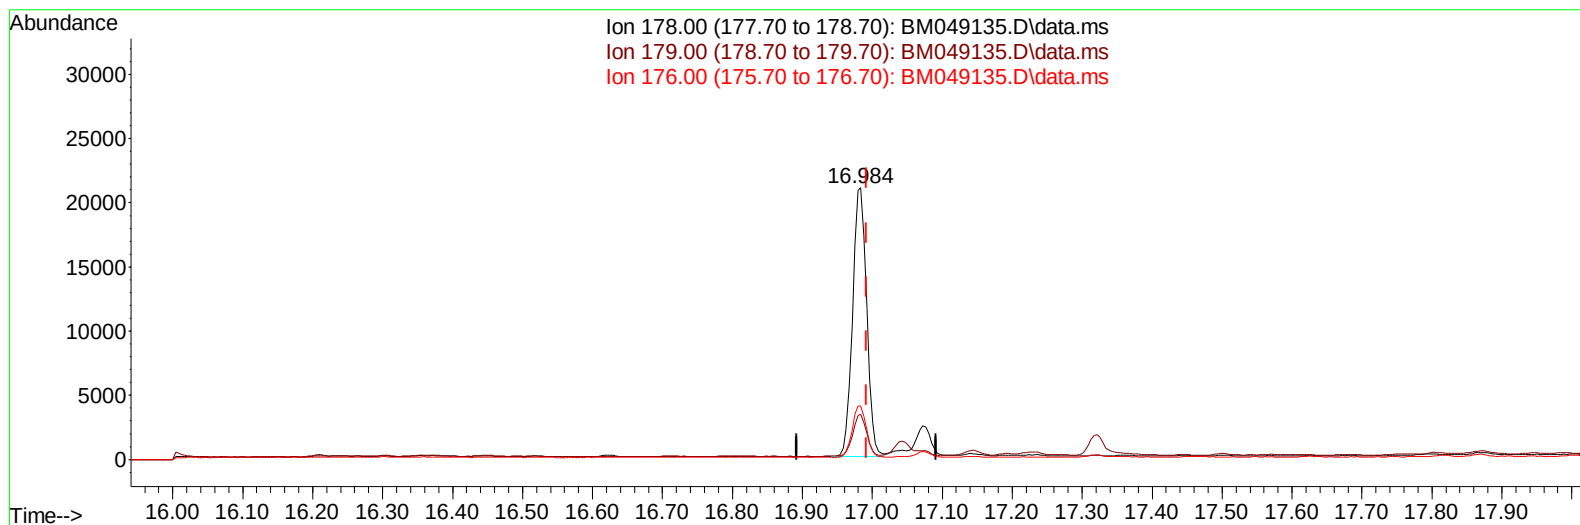

TIC: BM049135.D\data.ms

(15) Phenanthrene

16.984min (-0.008) 0.28 ng/ul m

response 29274

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 178.00 | 100.00 | 100.00 |
| 179.00 | 16.20  | 16.57  |
| 176.00 | 20.20  | 19.75  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

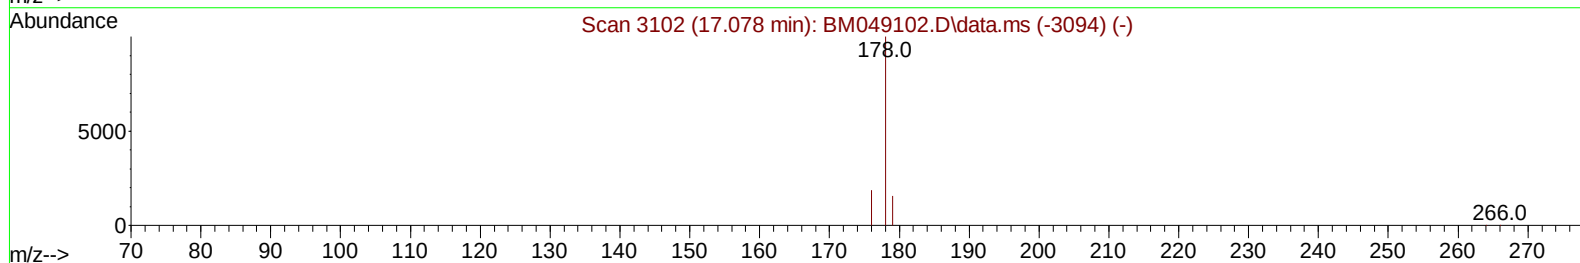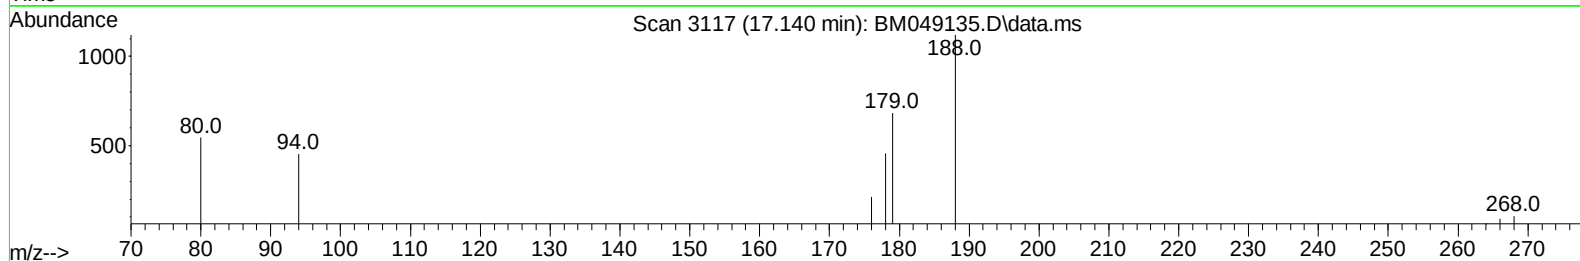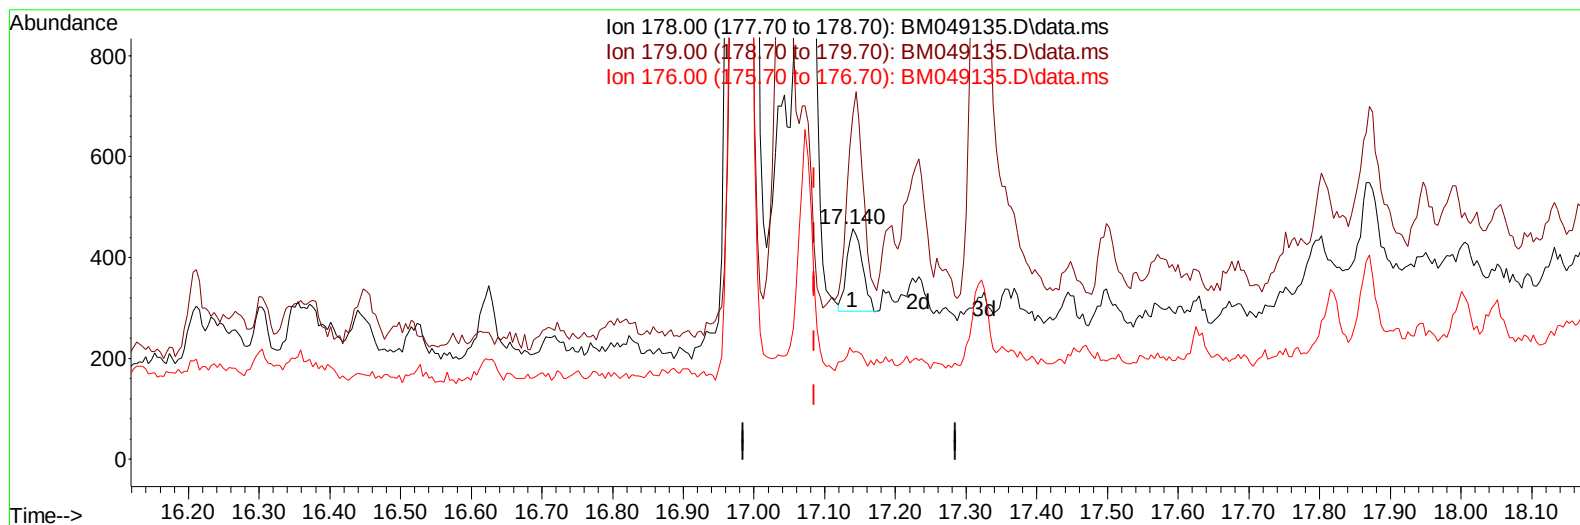

TIC: BM049135.D\data.ms

(16) Anthracene

17.140min (+ 0.055) 0.00 ng/u1

response 252

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 178.00 | 100.00 | 100.00  |
| 179.00 | 16.10  | 149.67# |
| 176.00 | 19.10  | 46.39#  |
| 0.00   | 0.00   | 0.00    |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

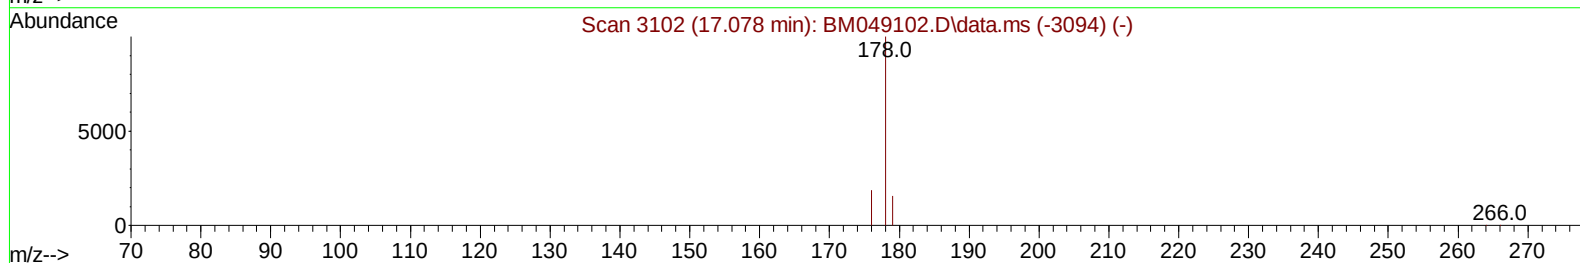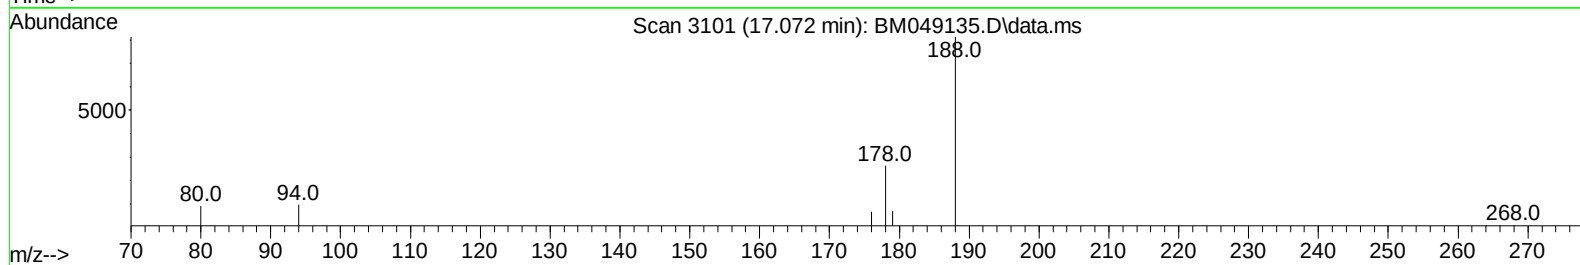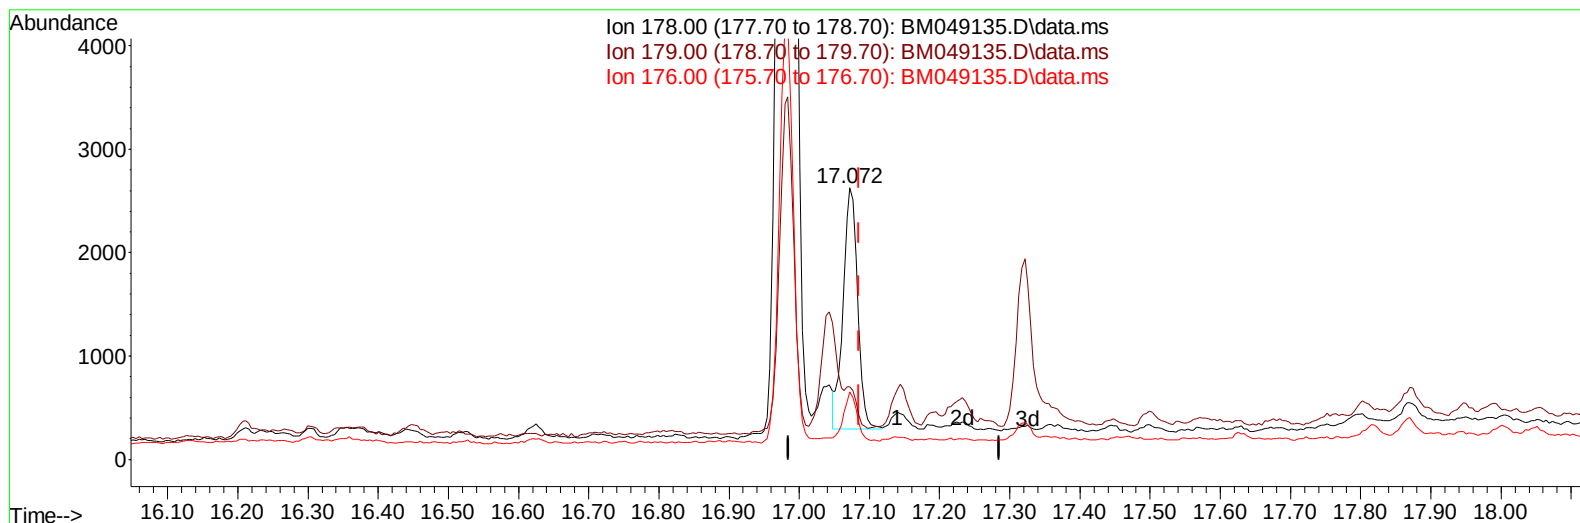

TIC: BM049135.D\data.ms

(16) Anthracene

17.072min (-0.013) 0.04 ng/ul m

response 3356

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 178.00 | 100.00 | 100.00 |
| 179.00 | 16.10  | 26.69# |
| 176.00 | 19.10  | 24.90# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

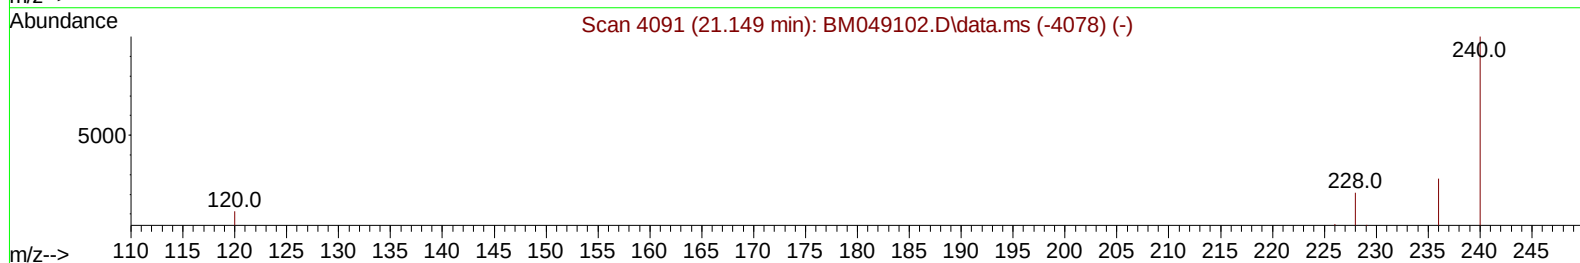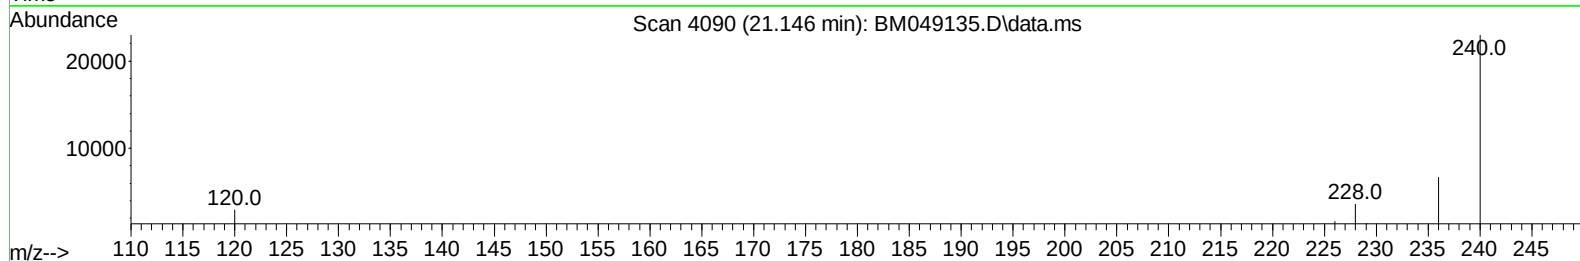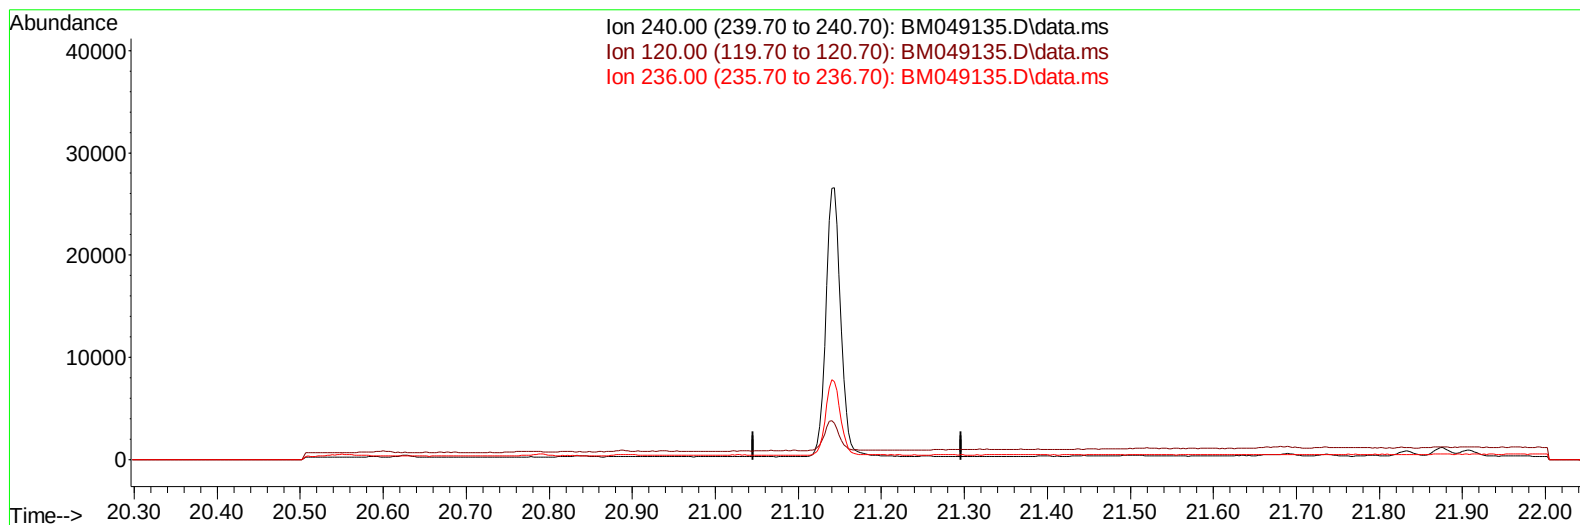

TIC: BM049135.D\data.ms

(17) Chrysene-d12

21.146min (-21.146) 0.00 ng/u1

response 0

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 240.00 | 100.00 | 0.00  |
| 120.00 | 14.50  | 0.00# |
| 236.00 | 29.80  | 0.00# |
| 0.00   | 0.00   | 0.00  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

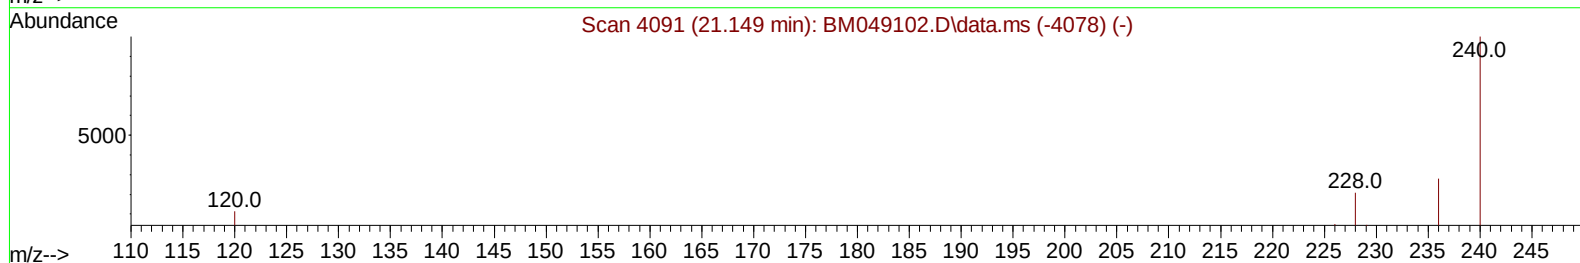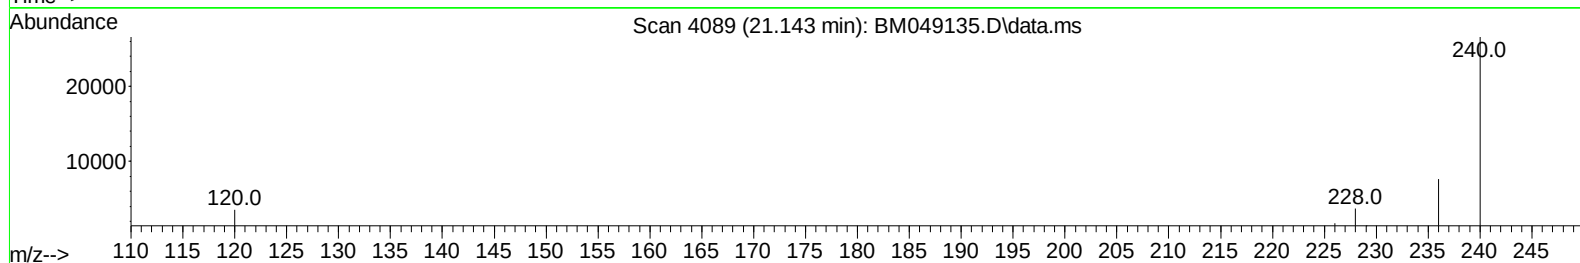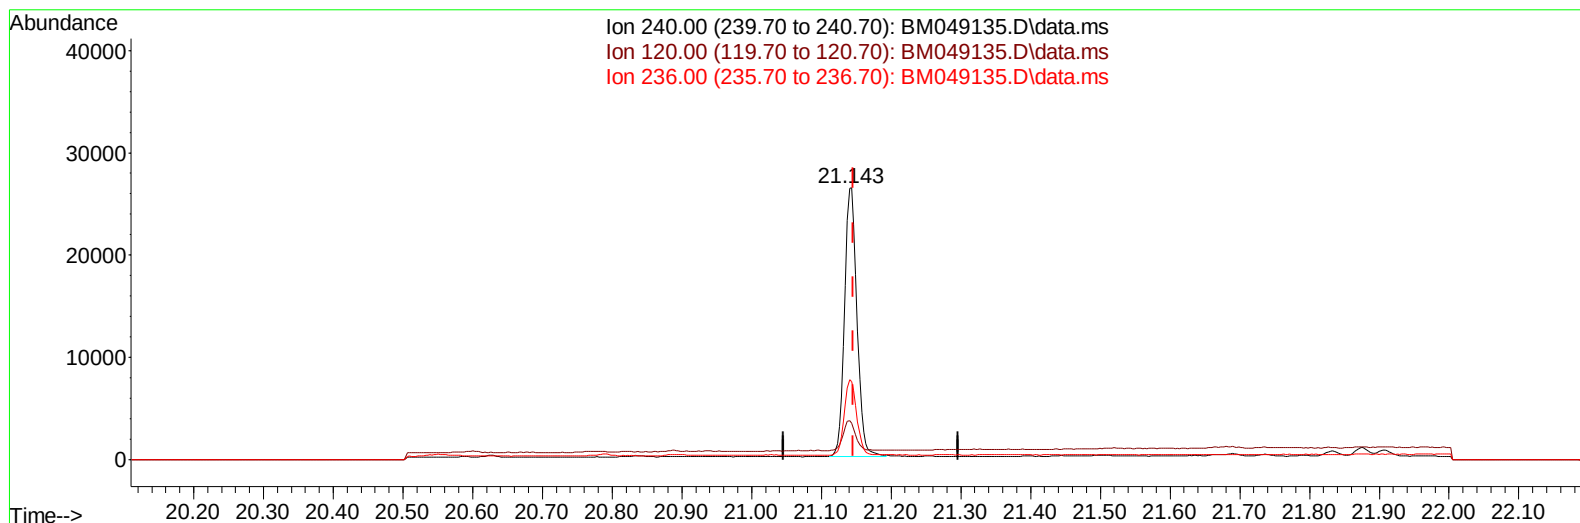

TIC: BM049135.D\data.ms

(17) Chrysene-d12

21.143min (-0.003) 0.40 ng/ul m

response 32604

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 240.00 | 100.00 | 100.00 |
| 120.00 | 14.50  | 13.35  |
| 236.00 | 29.80  | 28.75  |
| 0.00   | 0.00   | 0.00   |






Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

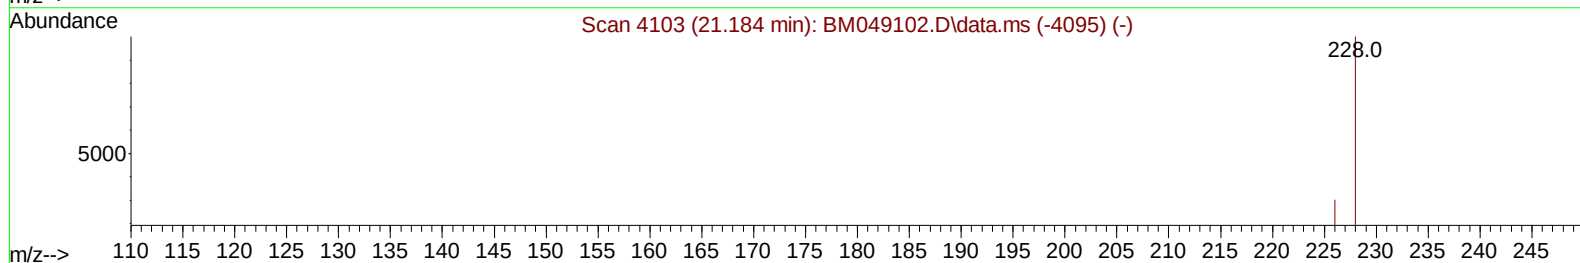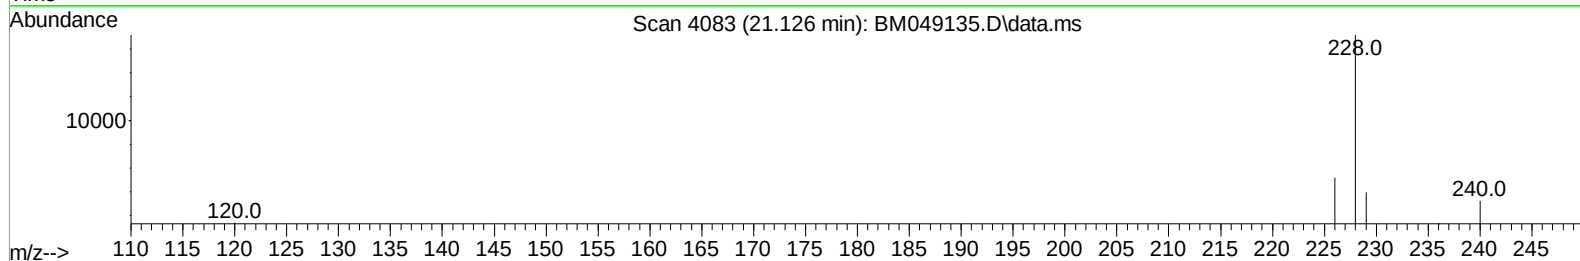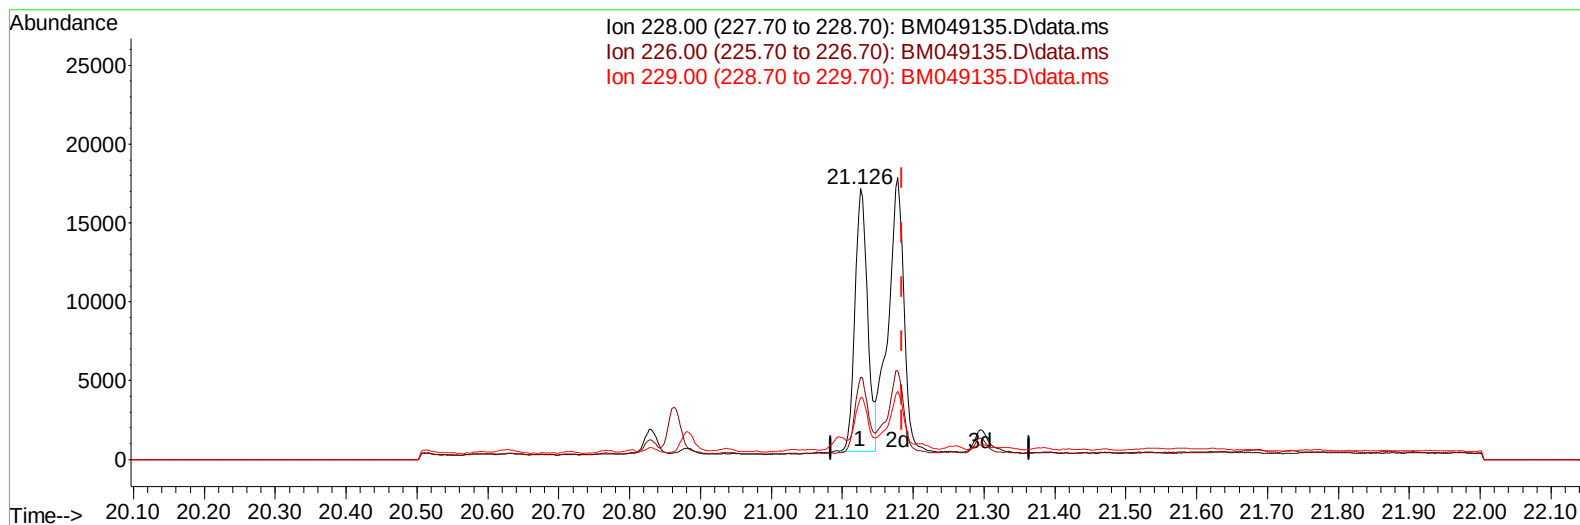

TIC: BM049135.D\data.ms

(22) Chrysene

21.126min (-0.058) 0.17 ng/u1

response 20517

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 228.00 | 100.00 | 100.00 |
| 226.00 | 30.10  | 30.26  |
| 229.00 | 19.80  | 22.84  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

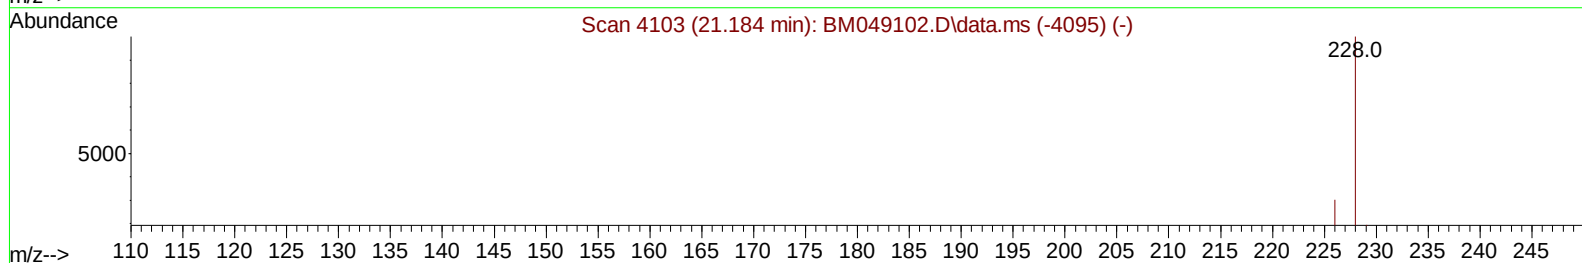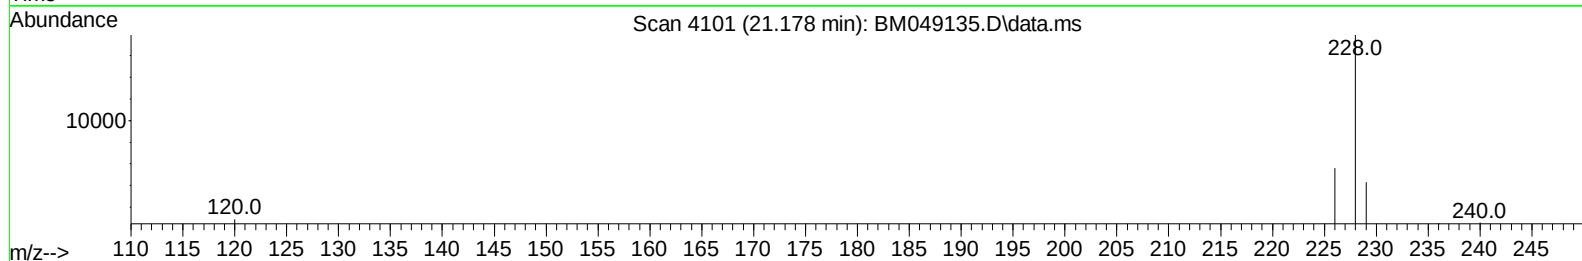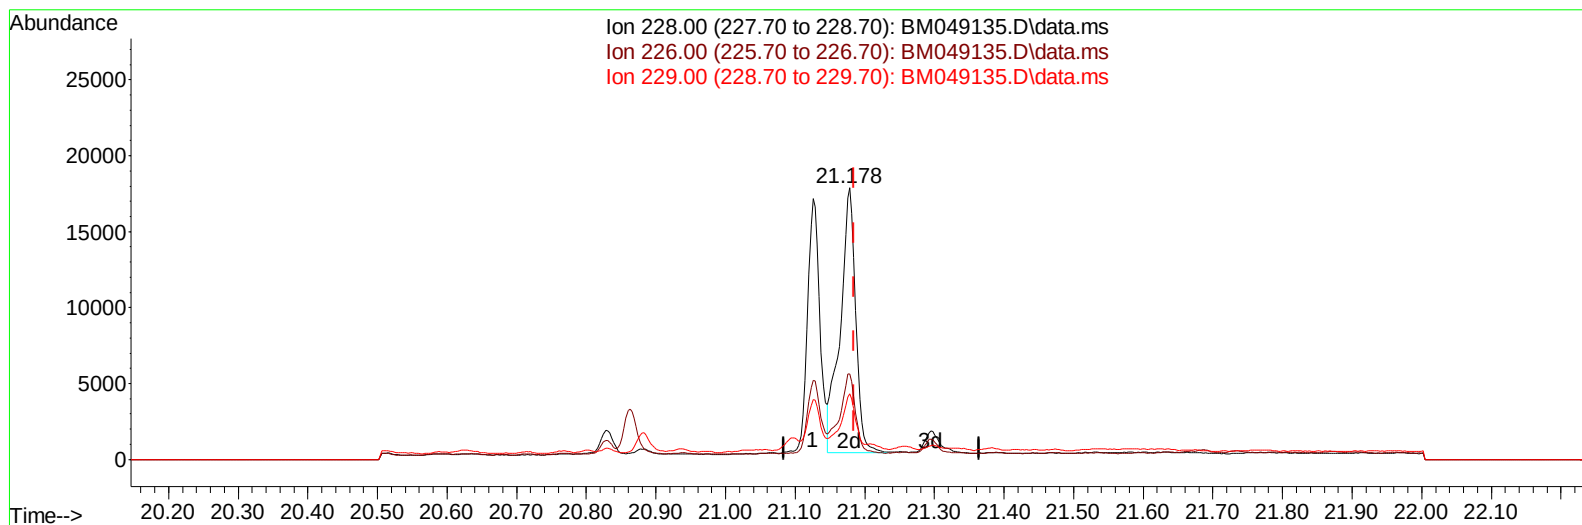

TIC: BM049135.D\data.ms

(22) Chrysene

21.178min (-0.006) 0.22 ng/ul m

response 27177

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 228.00 | 100.00 | 100.00 |
| 226.00 | 30.10  | 31.40  |
| 229.00 | 19.80  | 24.23# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

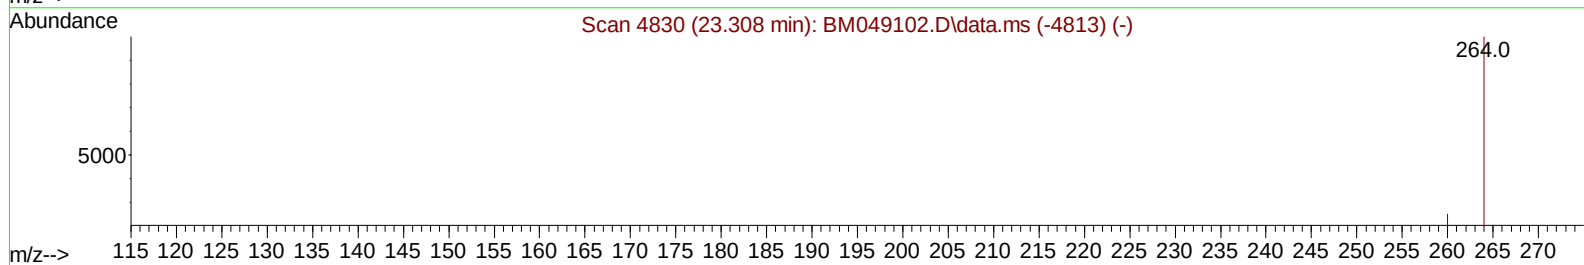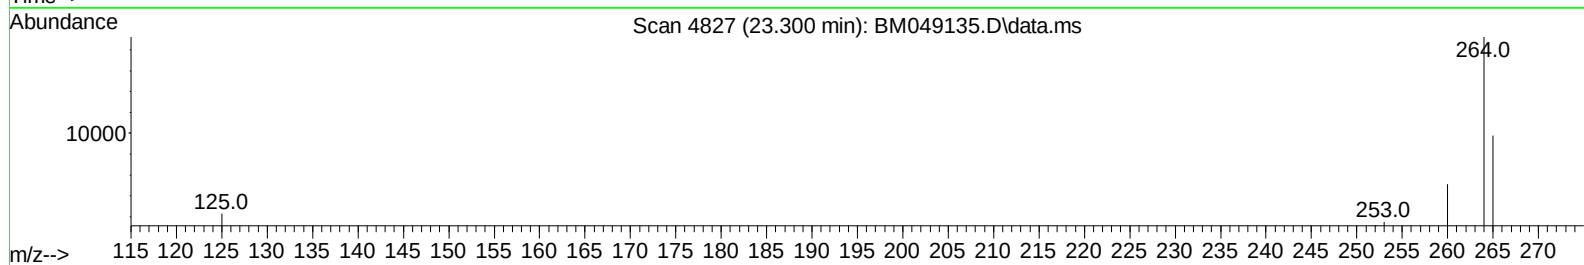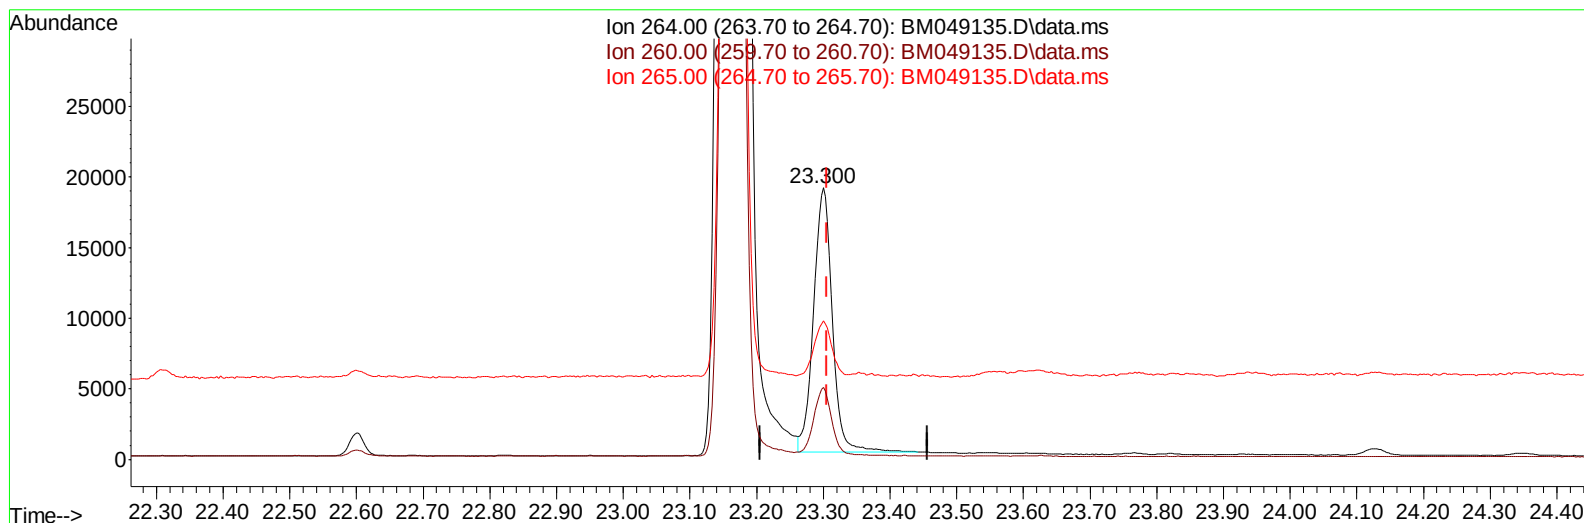

TIC: BM049135.D\data.ms

(23) Perylene-d12 (I)

23.300min (-0.006) 0.40 ng/u1

response 36123

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 25.80  | 26.48  |
| 265.00 | 78.30  | 51.01# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

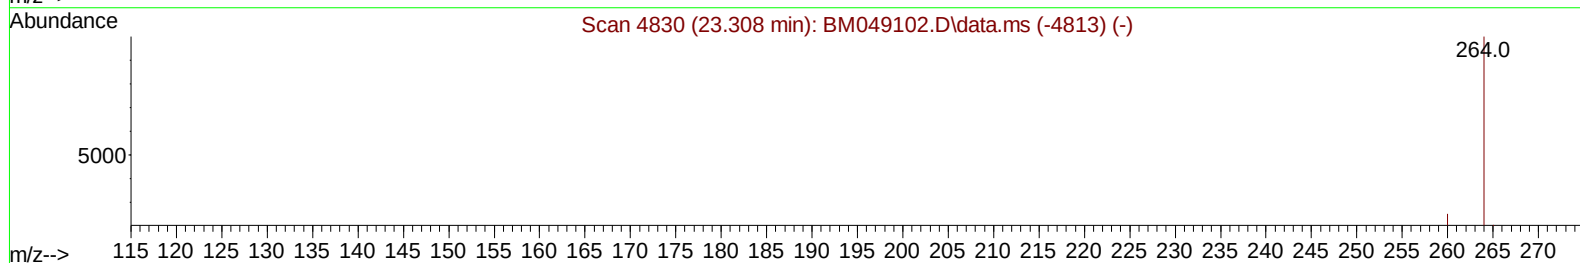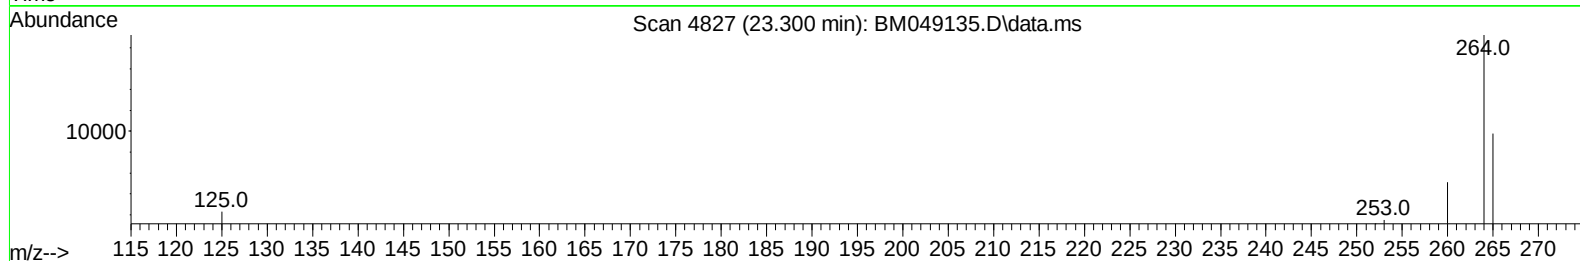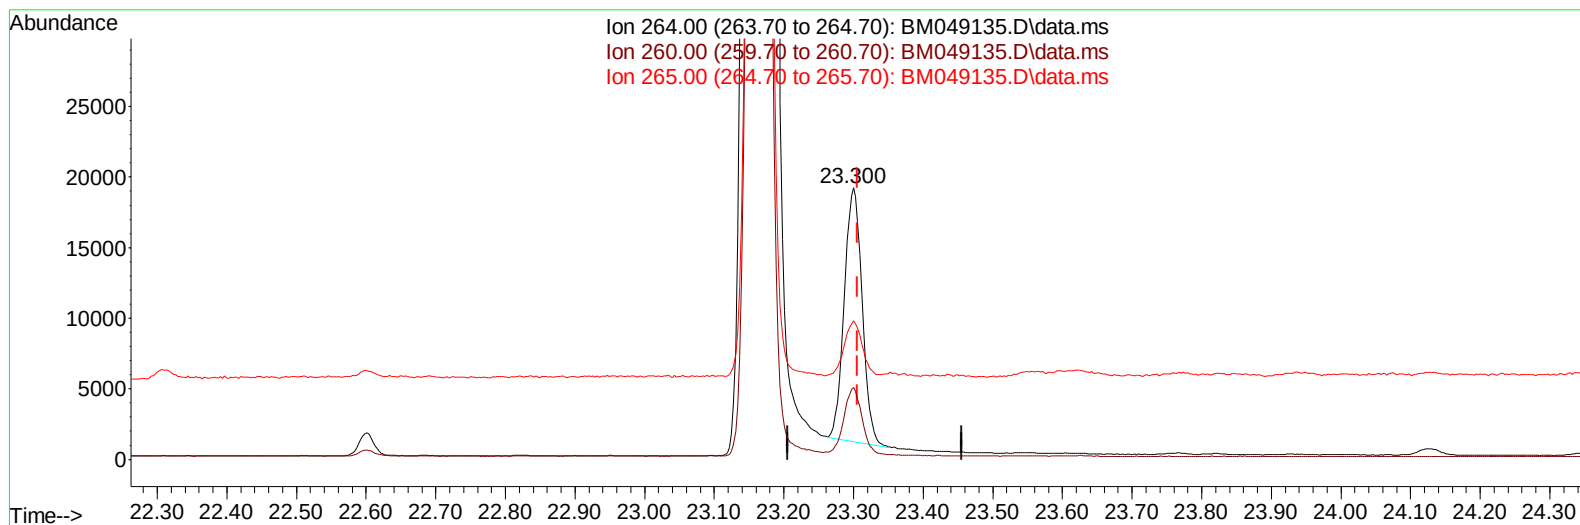

TIC: BM049135.D\data.ms

(23) Perylene-d12 (I)

23.300min (-0.006) 0.40 ng/ul m

response 32036

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 25.80  | 26.48  |
| 265.00 | 78.30  | 51.01# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

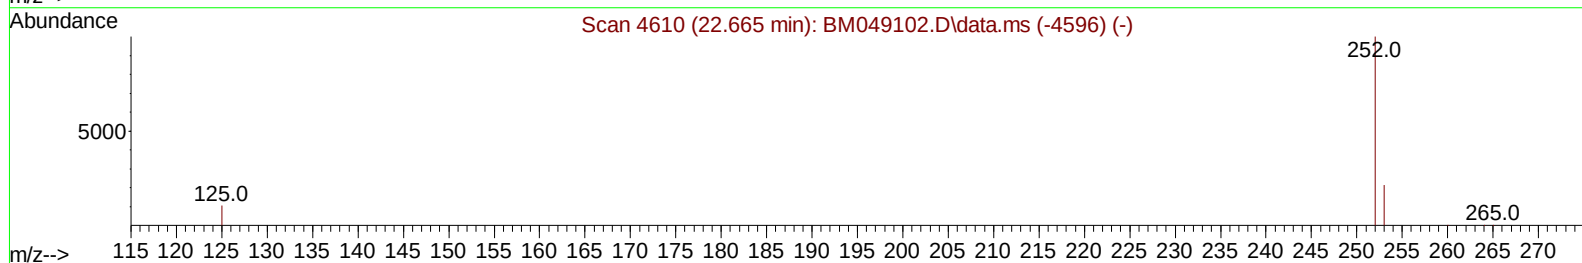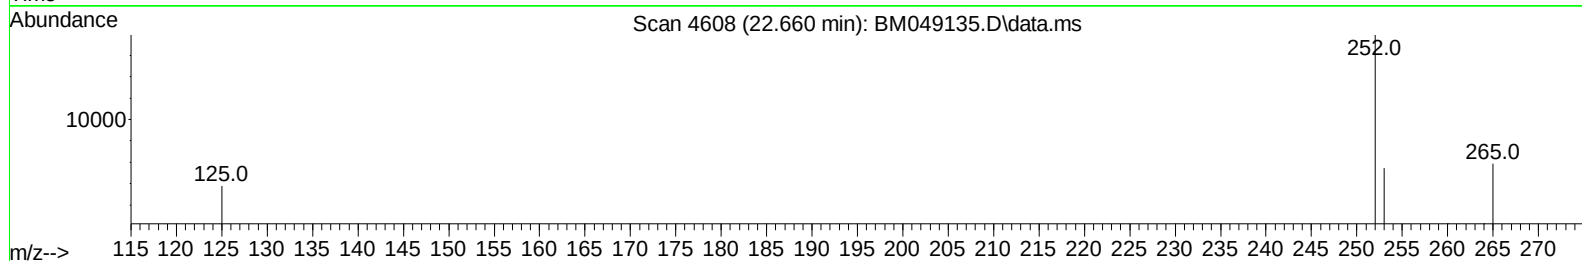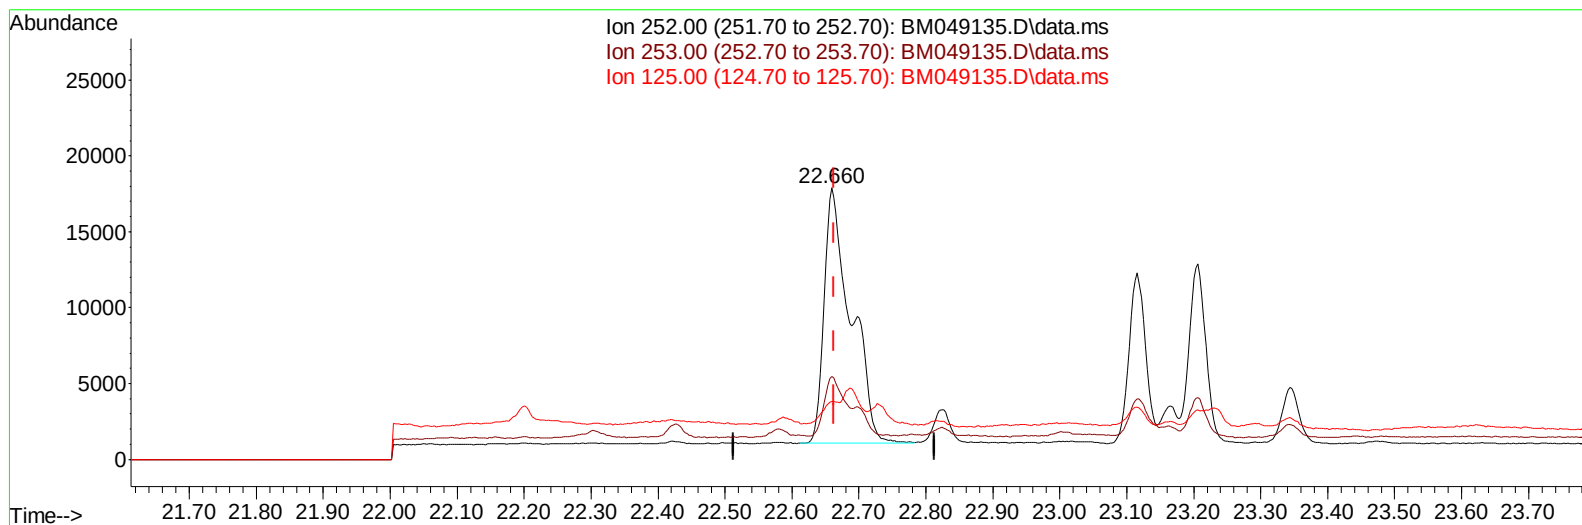

TIC: BM049135.D\data.ms

(24) Benzo(b)fluoranthene

22.660min (-0.003) 0.46 ng/u1

response 46855

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 26.30  | 30.49  |
| 125.00 | 15.40  | 21.30  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

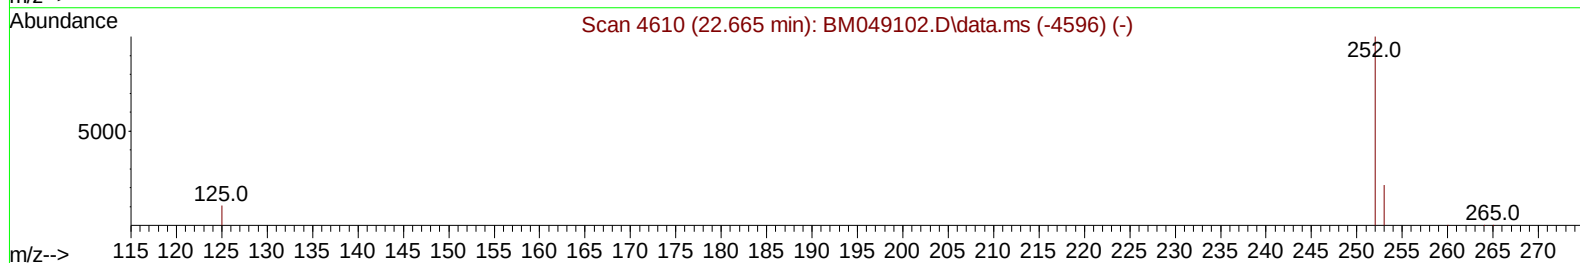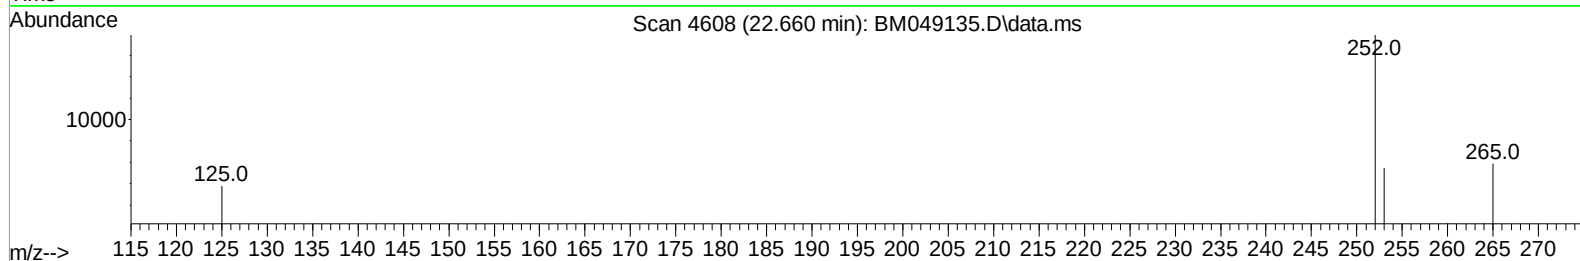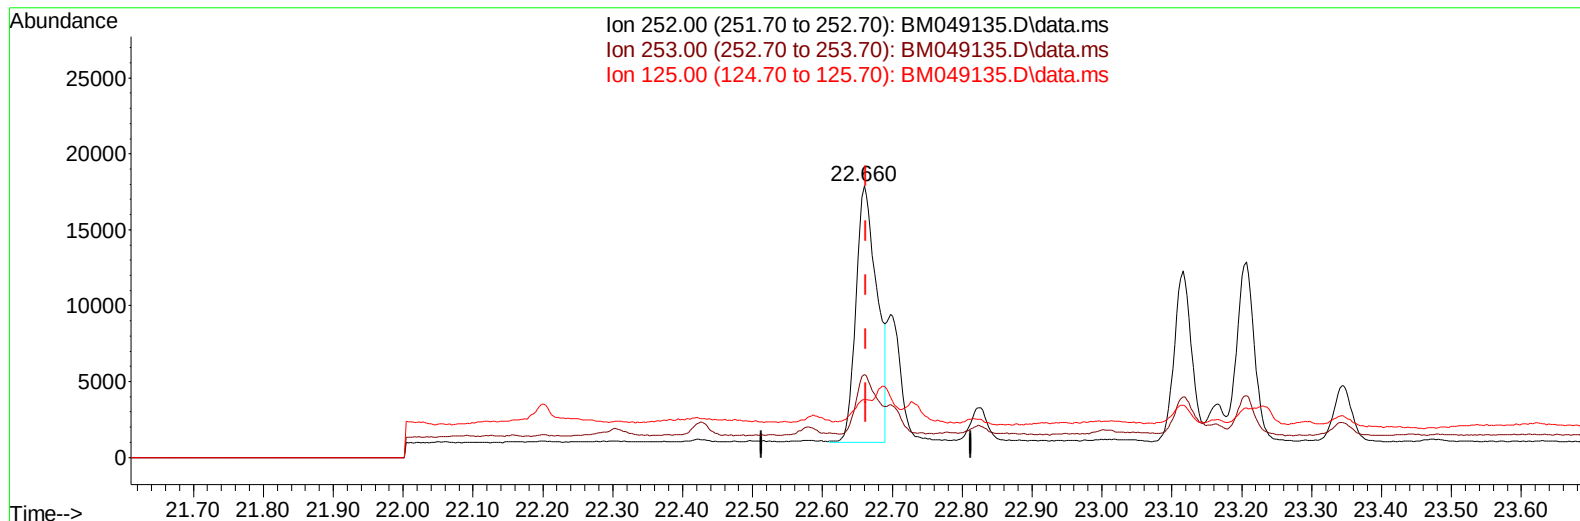

TIC: BM049135.D\data.ms

(24) Benzo(b)fluoranthene

22.660min (-0.003) 0.34 ng/ul m

response 35135

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 26.30  | 30.49  |
| 125.00 | 15.40  | 21.30  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

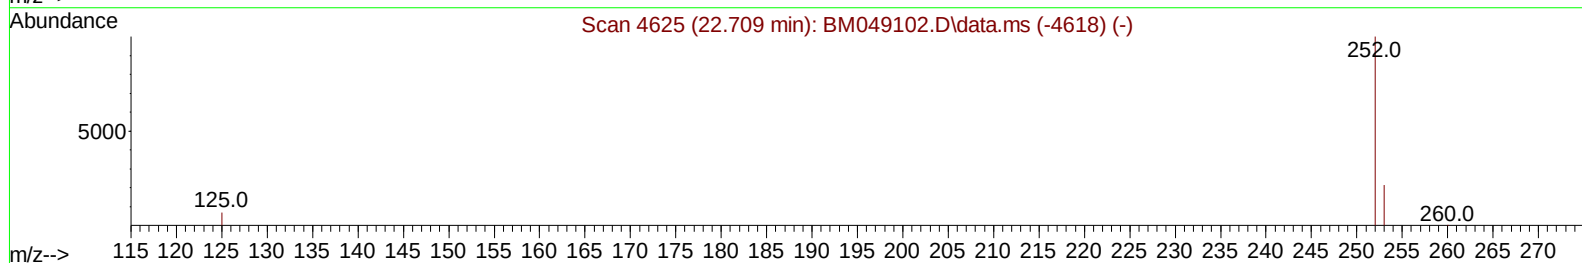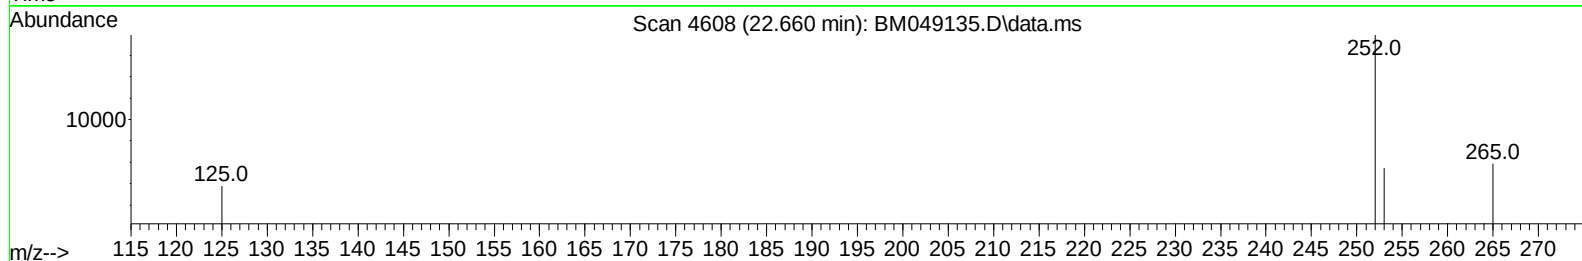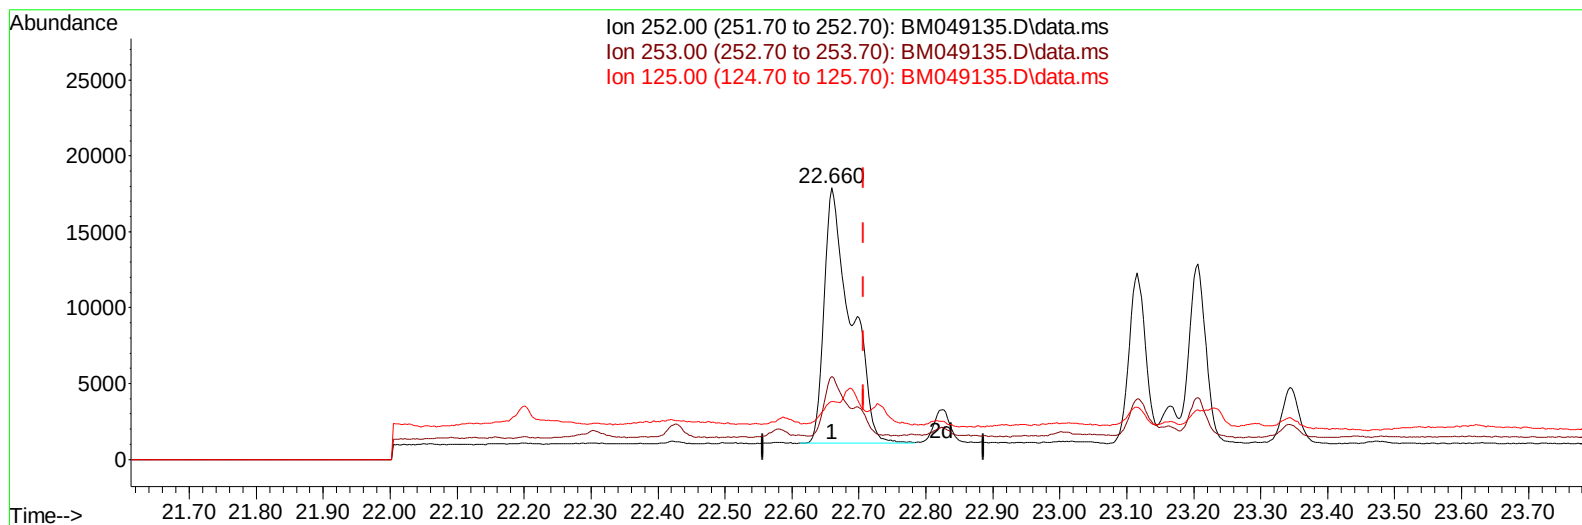

TIC: BM049135.D\data.ms

(25) Benzo(k)fluoranthene

22.660min (-0.047) 0.42 ng/u1

response 46855

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 26.60  | 30.49  |
| 125.00 | 15.70  | 21.30# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

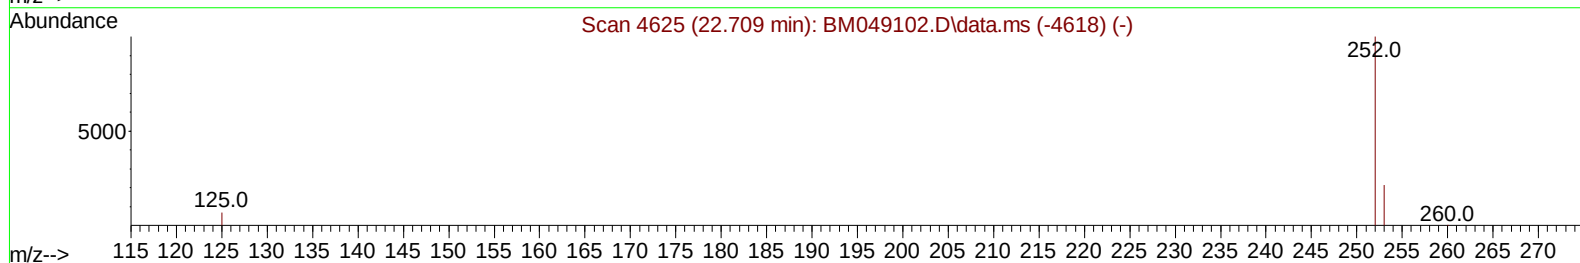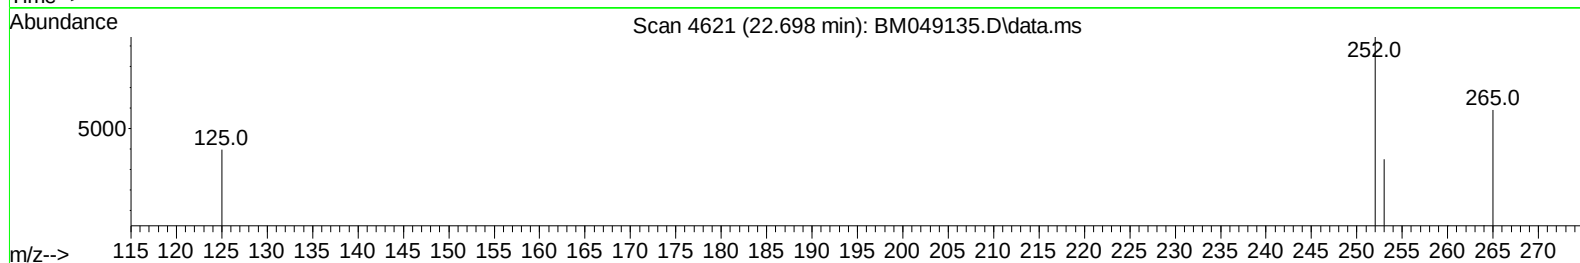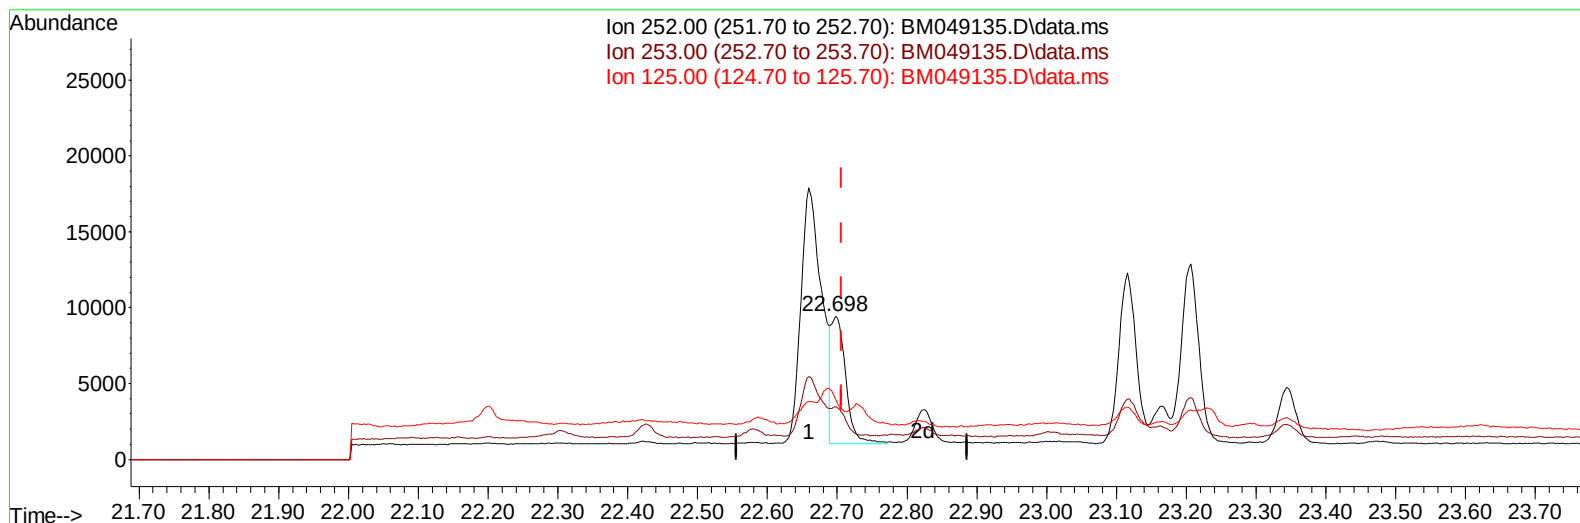

TIC: BM049135.D\data.ms

(25) Benzo(k)fluoranthene

22.698min (-0.009) 0.11 ng/ul m

response 12210

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 26.60  | 37.02# |
| 125.00 | 15.70  | 41.98# |
| 0.00   | 0.00   | 0.00   |



Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
 Data File : BM049135.D  
 Acq On : 21 Dec 2024 12:37  
 Operator : RC/JU  
 Sample : P5265-15  
 Misc :  
 ALS Vial : 36 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 E2900

Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 18 15:33:13 2024  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
 Supervised By :mohammad ahmed 12/24/2024

| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| -----                       |        |      |          |       |        |          |
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.556  | 152  | 10288    | 0.400 | ng/ul  | -0.01    |
| 4) Naphthalene-d8           | 10.319 | 136  | 32562    | 0.400 | ng/ul  | -0.01    |
| 9) Acenaphthene-d10         | 14.191 | 164  | 18394    | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 16.941 | 188  | 39950m   | 0.400 | ng/ul  | 0.00     |
| 17) Chrysene-d12            | 21.143 | 240  | 32604m   | 0.400 | ng/ul  | 0.00     |
| 23) Perylene-d12            | 23.300 | 264  | 32036m   | 0.400 | ng/ul  | 0.00     |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.151  | 96   | 43238    | 3.644 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 11.914 | 152  | 9244     | 0.211 | ng/ul  | -0.01    |
| 18) Fluoranthene-d10        | 18.977 | 212  | 16534    | 0.179 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       | Qvalue |          |
| 5) Naphthalene              | 10.369 | 128  | 3952     | 0.048 | ng/ul# | 90       |
| 7) 2-Methylnaphthalene      | 11.991 | 142  | 2911     | 0.056 | ng/ul  | 99       |
| 8) 1-Methylnaphthalene      | 12.216 | 142  | 2224     | 0.042 | ng/ul  | 99       |
| 15) Phenanthrene            | 16.984 | 178  | 29274m   | 0.281 | ng/ul  |          |
| 16) Anthracene              | 17.072 | 178  | 3356m    | 0.035 | ng/ul  |          |
| 19) Fluoranthene            | 19.005 | 202  | 57528    | 0.488 | ng/ul  | 100      |
| 20) Pyrene                  | 19.368 | 202  | 51278    | 0.408 | ng/ul  | 99       |
| 21) Benzo(a)anthracene      | 21.126 | 228  | 20920    | 0.184 | ng/ul  | 95       |
| 22) Chrysene                | 21.178 | 228  | 27177m   | 0.223 | ng/ul  |          |
| 24) Benzo(b)fluoranthene    | 22.660 | 252  | 35135m   | 0.343 | ng/ul  |          |
| 25) Benzo(k)fluoranthene    | 22.698 | 252  | 12210m   | 0.109 | ng/ul  |          |
| 26) Benzo(a)pyrene          | 23.206 | 252  | 20655    | 0.210 | ng/ul# | 90       |
| 27) Indeno(1,2,3-cd)pyrene  | 25.437 | 276  | 18556    | 0.134 | ng/ul# | 98       |
| 28) Dibenzo(a,h)anthracene  | 25.444 | 278  | 4076     | 0.038 | ng/ul# | 39       |
| 29) Benzo(g,h,i)perylene    | 26.091 | 276  | 22124    | 0.198 | ng/ul  | 96       |
| -----                       |        |      |          |       |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM122024\  
Data File : BM049135.D  
Acq On : 21 Dec 2024 12:37  
Operator : RC/JU  
Sample : P5265-15  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E2900

## Manual IntegrationsAPPROVED

Quant Time: Dec 22 23:07:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM121824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 18 15:33:13 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2024  
Supervised By :mohammad ahmed 12/24/2024

