

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122115\
 Data File : BM003684.D
 Acq On : 21 Dec 2015 19:18
 Operator : UM/SJ
 Sample : G4792-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N26

Quant Time: Dec 22 02:21:45 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 22 02:16:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	27944	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	114699	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.34	164	60834	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	129542	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	139241	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	138656	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	860	1.66	ng/uL	0.00
5) Phenol-d5	6.87	99	16019	6.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	41209	32.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	52051	27.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	31007	15.20	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	29601	35.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	32357	34.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	52416	30.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	3781	1.66	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	178951	35.59	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	216808	37.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	3814	3.89	ng/ul	0.00
58) Fluorene-d10	15.34	176	153257	36.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	21297	29.17	ng/ul	0.00
71) Anthracene-d10	17.19	188	229453	38.93	ng/ul	0.00
79) Pyrene-d10	19.50	212	249324	40.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	265970	38.61	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
46) 2,6-Dinitrotoluene	13.76	165	1075	1.07	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122115\
Data File : BM003684.D
Acq On : 21 Dec 2015 19:18
Operator : UM/SJ
Sample : G4792-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9N26

Quant Time: Dec 22 02:21:45 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 22 02:16:02 2015
Response via : Initial Calibration

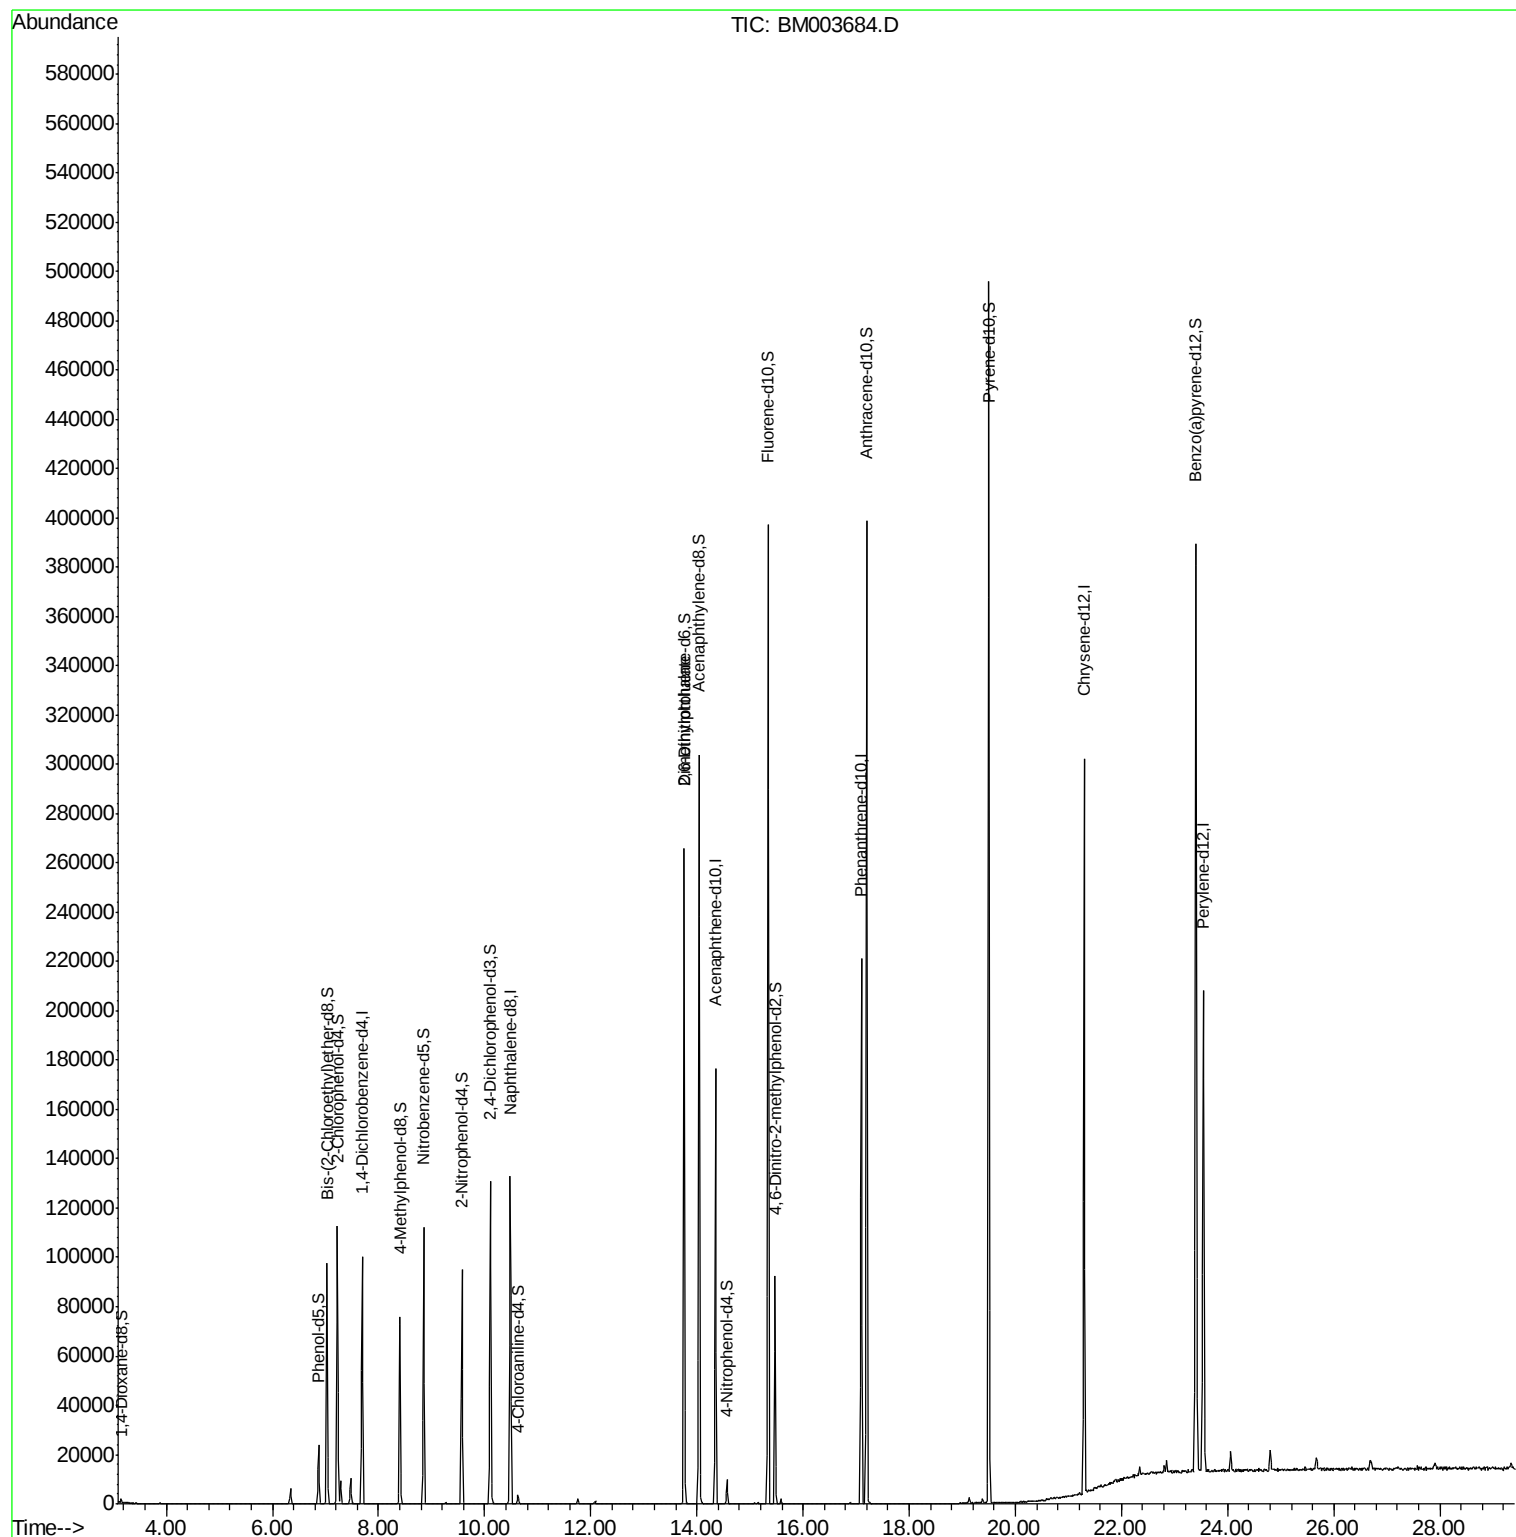

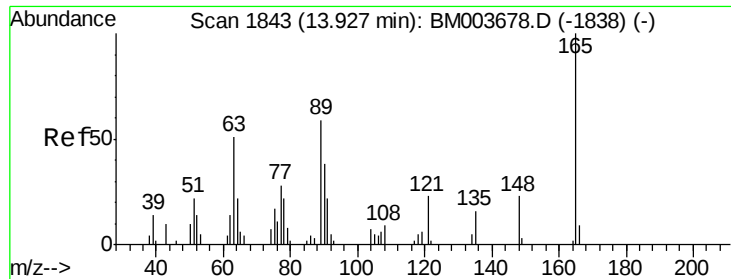

#46

2,6-Dinitrotoluene

Concen: 1.07 ng/ul

RT: 13.76 min Scan# 1815

Delta R.T. -0.16 min

Lab File: BM003684.D


Acq: 21 Dec 2015 19:18

Instrument :

BNA_M

ClientSampleId :

D9N26

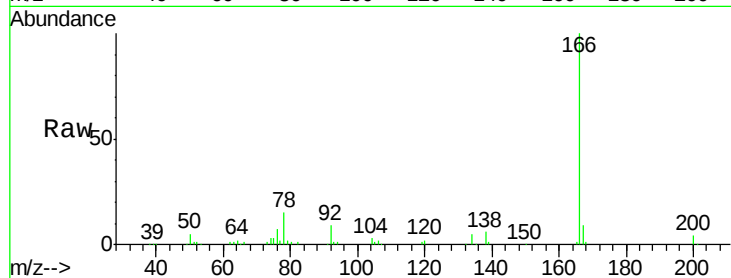

Tgt Ion:	165	Resp:	1075
Ion Ratio	Lower	Upper	
165	100		
89	0.0	42.4	63.6#
121	0.0	16.6	24.8#

