

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122115\
 Data File : BM003690.D
 Acq On : 21 Dec 2015 23:30
 Operator : UM/SJ
 Sample : G4867-15RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9DB0

Quant Time: Dec 22 02:47:28 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 22 02:40:18 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	27465	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	110313	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	58959	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.09	188	128605	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	149077	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	154647	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	931	1.83	ng/uL	0.00
5) Phenol-d5	6.87	99	17326	7.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	43635	35.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	56498	29.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	33482	16.70	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	31491	39.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	34100	37.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	55432	33.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	5634	2.57	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	183291	37.62	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	219872	39.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	4597	4.84	ng/ul	0.00
58) Fluorene-d10	15.34	176	157344	39.03	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	23384	32.26	ng/ul	0.00
71) Anthracene-d10	17.19	188	236231	40.37	ng/ul	0.00
79) Pyrene-d10	19.50	212	268569	41.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	307258	40.00	ng/ul	0.00


Target Compounds					Qvalue
17) Hexachloroethane	8.87	117	873	1.17 ng/ul#	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122115\
Data File : BM003690.D
Acq On : 21 Dec 2015 23:30
Operator : UM/SJ
Sample : G4867-15RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9DB0

Quant Time: Dec 22 02:47:28 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 22 02:40:18 2015
Response via : Initial Calibration

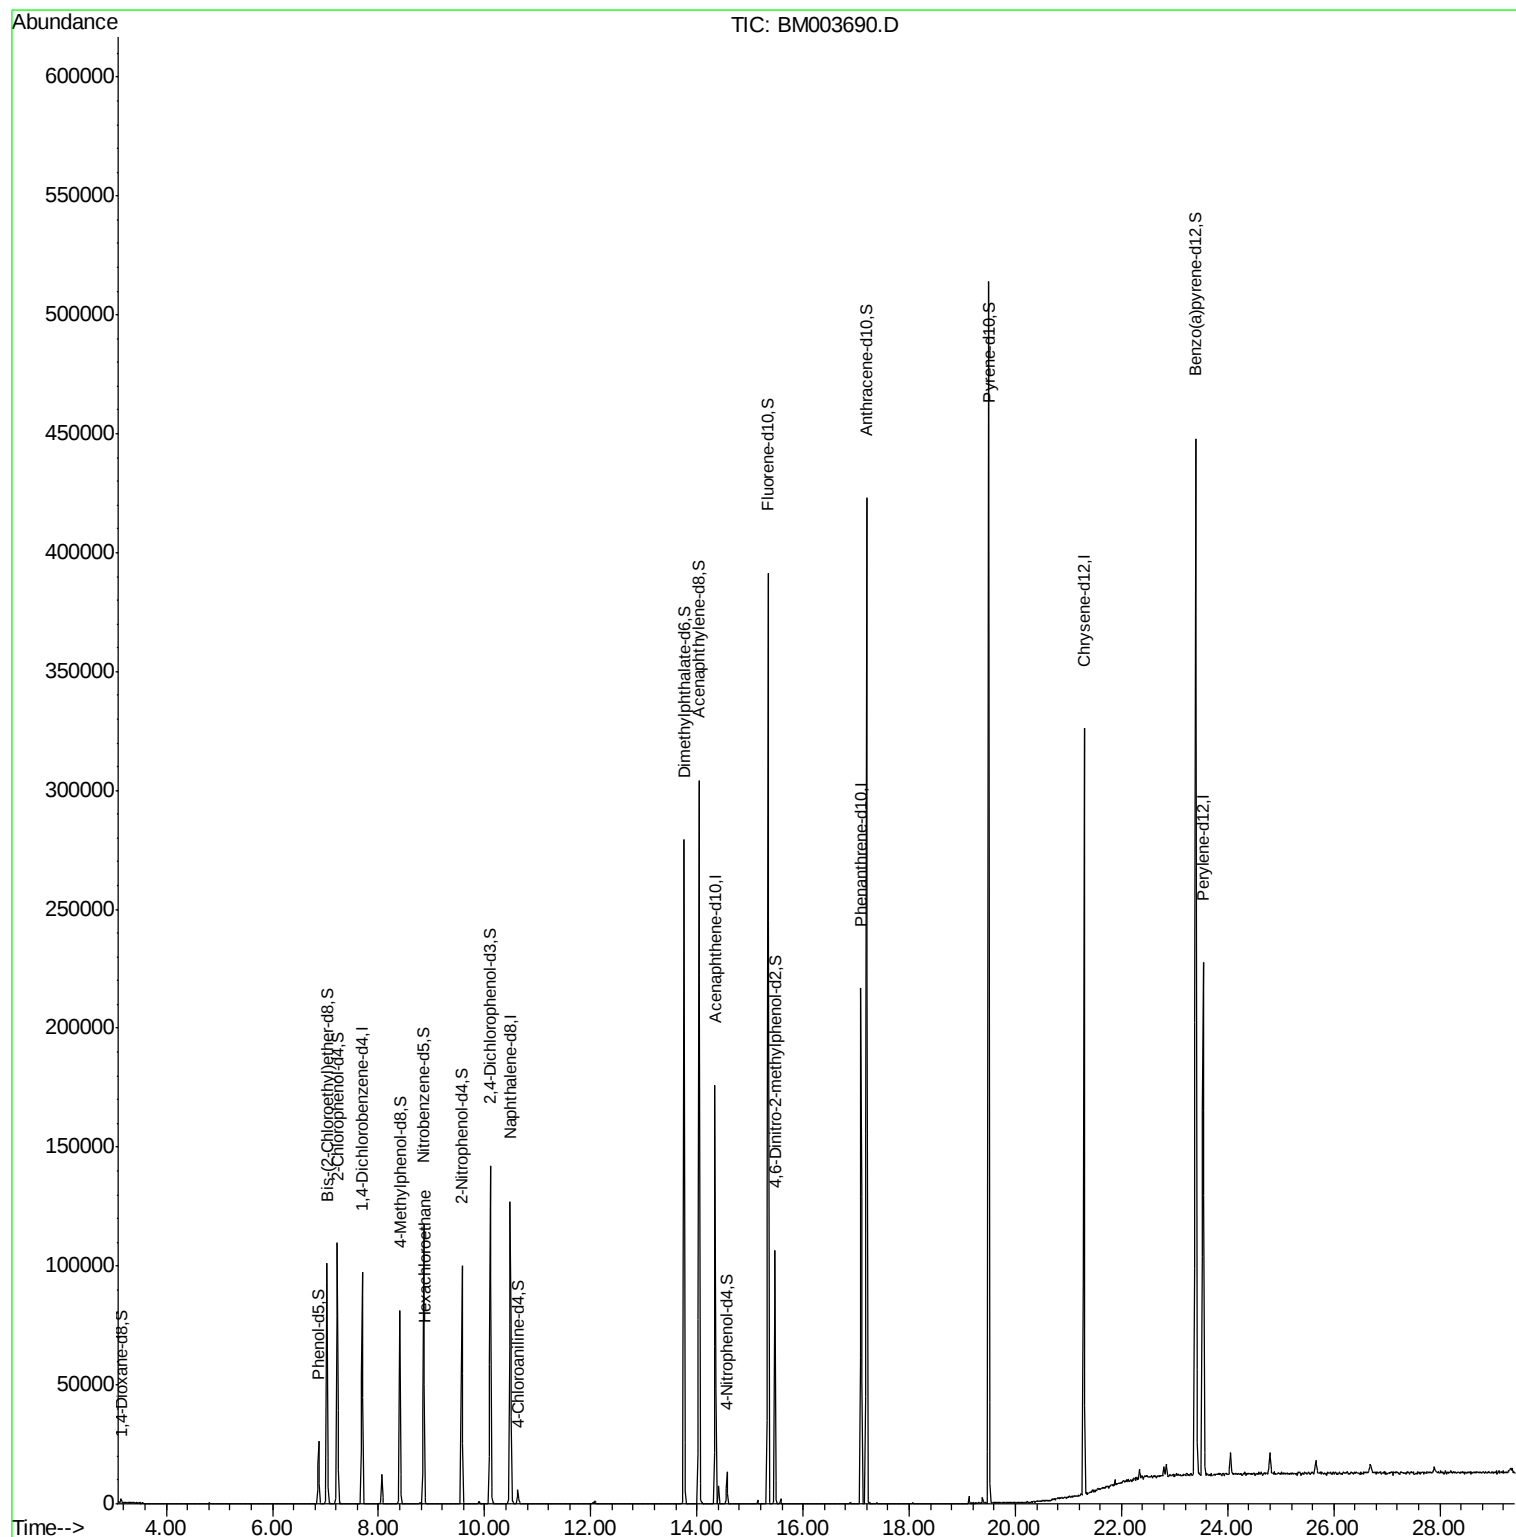

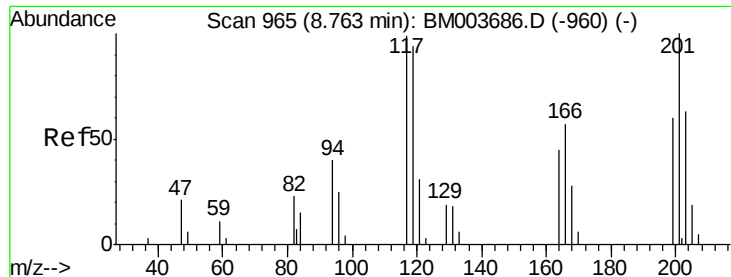

#17
 Hexachloroethane
 Concen: 1.17 ng/ul
 RT: 8.87 min Scan# 983
 Delta R.T. 0.11 min
 Lab File: BM003690.D
 Acq: 21 Dec 2015 23:30

Instrument :
 BNA_M
 ClientSampleId :
 G9DB0

Tgt Ion: 117 Resp: 873
 Ion Ratio Lower Upper
 117 100
 201 0.0 81.5 122.3#
 199 0.0 50.6 76.0#

