


Data Path : Z:\HPCHEM1\BNA M\Data\BM122115\
 Data File : BM003677.D
 Acq On : 21 Dec 2015 08:57
 Operator : UM/SJ
 Sample : DFTPP62
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP62

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
 Title : SVOA CALIBRATION
 Last Update : Tue Dec 22 02:40:18 2015

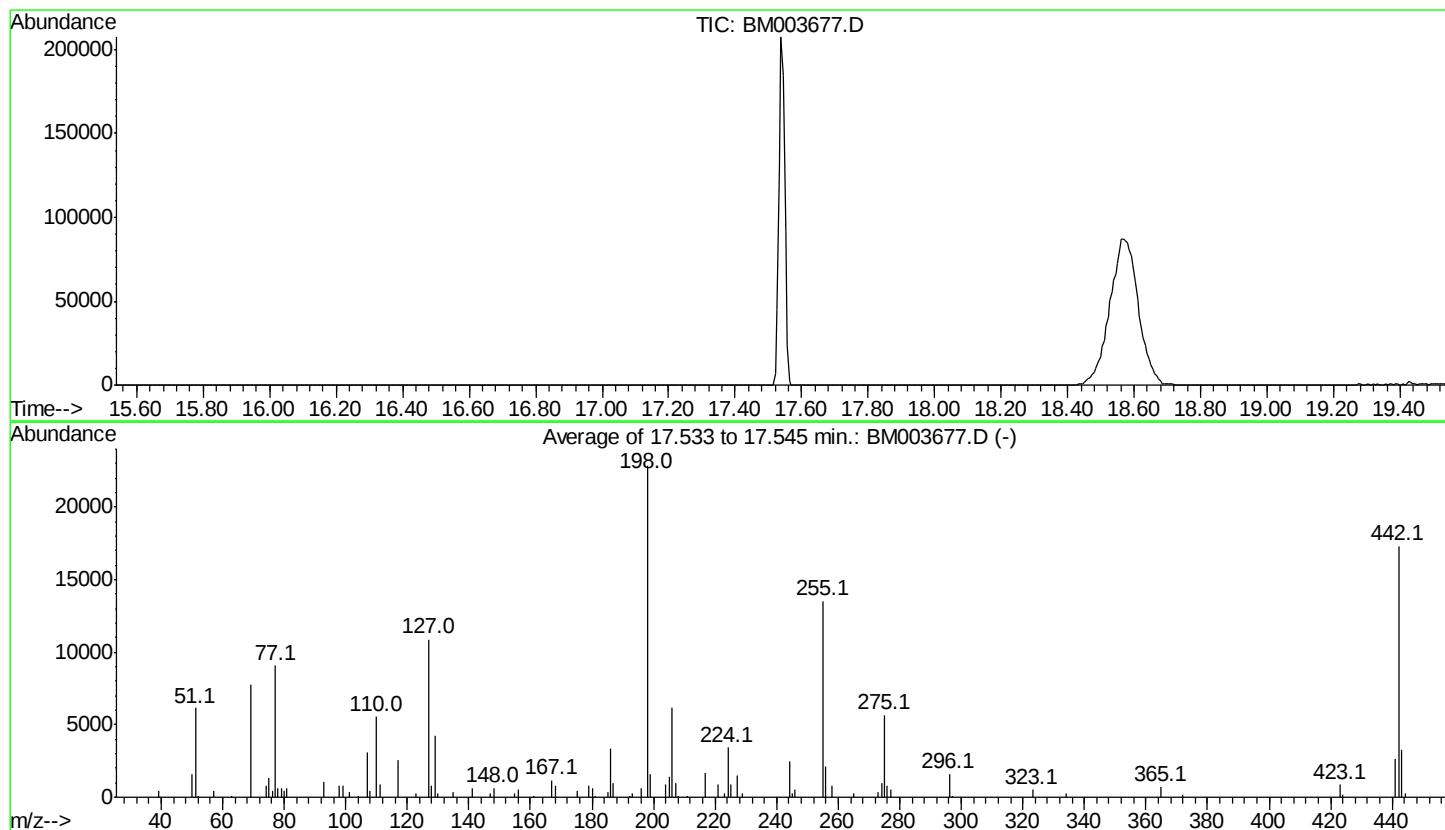

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	6171	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.0	7763	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	10894	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22864	PASS
199	198	5	9	6.8	1562	PASS
275	198	10	60	24.8	5674	PASS
365	198	1	100	3.3	745	PASS
441	443	0.01	100	81.0	2652	PASS
442	198	50	100	75.7	17304	PASS
443	442	15	24	18.9	3274	PASS

m/z	Abundance
39.00	420.0
50.10	1432.0
51.10	5522.0
56.90	375.0
69.00	6899.0
74.00	702.0
75.00	1175.0
76.00	382.0
77.10	7999.0
78.00	578.0
79.00	514.0
80.00	432.0
81.00	546.0
93.00	915.0
98.00	736.0
99.00	738.0
101.00	345.0
107.00	2586.0
108.00	443.0
110.00	4716.0
111.00	847.0
117.00	2145.0
127.00	9046.0
128.00	703.0
129.00	3466.0
135.00	317.0
141.00	479.0
148.00	562.0
156.00	402.0
167.00	920.0
168.00	704.0
175.00	368.0
179.00	657.0
180.00	535.0
185.00	320.0
186.00	2527.0
187.00	807.0
196.00	507.0
198.00	17656.0
199.00	1333.0
204.00	628.0
205.00	1037.0
206.10	4640.0
207.10	690.0
217.00	1313.0
221.10	687.0
224.10	2558.0
225.10	712.0
227.00	1090.0
244.10	1814.0
246.00	401.0
255.10	10062.0
256.10	1544.0
258.00	562.0
274.10	736.0
275.10	4034.0
276.00	575.0
277.00	358.0
296.10	1222.0
323.10	345.0
365.10	476.0
423.10	460.0
441.10	1595.0
442.20	10136.0
443.10	2029.0

Instrument :
BNA_M
ClientSampleId :
DFTPP62

m/z	Abundance
39.10	537.0
50.10	1878.0
51.10	7277.0
52.00	362.0
57.00	511.0
63.00	334.0
69.00	8980.0
74.00	936.0
75.00	1561.0
76.10	557.0
77.10	10833.0
78.00	712.0
79.00	739.0
80.00	604.0
81.00	814.0
93.00	1297.0
98.00	964.0
99.00	902.0
101.00	412.0
104.00	309.0
107.00	3821.0
108.00	539.0
110.00	6475.0
111.00	990.0
117.00	3035.0
123.00	405.0
127.00	12670.0
128.00	921.0
129.00	5201.0
130.00	414.0
135.00	442.0
141.00	673.0
147.00	385.0
148.00	717.0
155.00	382.0
156.00	592.0
161.00	300.0
167.10	1410.0
168.00	857.0
175.00	589.0
179.00	1001.0
180.00	803.0
181.00	330.0
185.00	473.0
186.10	4057.0
187.00	1196.0
192.10	315.0
193.10	409.0
196.00	759.0
198.00	27152.0
199.00	1879.0
204.00	1010.0
205.10	1680.0
206.10	7253.0
207.10	1099.0
208.00	304.0
211.10	318.0
217.00	1848.0
221.10	942.0
223.10	407.0
224.10	4050.0
225.00	1017.0
227.00	1757.0
229.00	355.0
244.10	2914.0
245.10	459.0
246.00	695.0
255.10	15722.0
256.00	2567.0
258.00	976.0
265.00	397.0
273.00	500.0
274.00	1155.0
275.10	6653.0
276.00	945.0
277.10	635.0
296.10	1771.0
323.10	594.0
334.10	354.0
365.00	900.0
372.10	309.0
423.10	982.0
424.10	308.0
441.10	2987.0
442.10	19776.0
443.20	3781.0
444.10	363.0

Instrument :
BNA_M
ClientSampleId :
DFTPP62

m/z	Abundance
39.00	483.0
50.10	1519.0
51.10	5715.0
57.00	366.0
69.00	7412.0
74.00	732.0
75.00	1254.0
76.00	473.0
77.10	8392.0
78.00	585.0
79.00	598.0
80.00	401.0
81.00	603.0
93.00	1010.0
98.00	800.0
99.00	678.0
101.00	370.0
107.00	2953.0
108.00	399.0
110.00	5456.0
111.00	897.0
117.00	2478.0
123.00	361.0
127.00	10966.0
128.00	812.0
129.00	4121.0
130.00	360.0
135.00	344.0
141.00	601.0
147.00	330.0
148.00	627.0
155.00	367.0
156.00	490.0
167.00	1173.0
168.00	753.0
175.10	503.0
179.00	841.0
180.00	640.0
185.00	395.0
186.10	3423.0
187.00	1012.0
193.00	323.0
196.00	712.0
198.00	23784.0
199.00	1475.0
204.00	907.0
205.10	1471.0
206.10	6699.0
207.10	1001.0
217.00	1935.0
221.00	981.0
223.00	339.0
224.10	3634.0
225.00	934.0
227.00	1599.0
229.00	323.0
244.10	2708.0
245.10	361.0
246.00	616.0
255.10	14736.0
256.00	2154.0
258.00	907.0
265.00	374.0
273.10	457.0
274.10	1142.0
275.10	6336.0
276.10	827.0
277.00	578.0
296.10	1779.0
297.00	328.0
323.10	547.0
334.10	363.0
365.00	860.0
372.10	316.0
423.10	1169.0
424.10	323.0
441.10	3375.0
442.10	22000.0
443.10	4014.0
444.10	359.0

Instrument :
BNA_M
ClientSampleId :
DFTPP62