

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
 Data File : BM008517.D
 Acq On : 21 Dec 2016 15:09
 Operator : UM/SJ
 Sample : H5996-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA872

Quant Time: Dec 22 00:04:05 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 00:00:17 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	329	0.40	ng/ul	-0.05
2) Naphthalene-d8	10.44	136	1050	0.40	ng/ul	-0.05
6) Acenaphthene-d10	14.30	164	604	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.14	188	53694	0.40	ng/ul	0.05
16) Chrysene-d12	21.28	240	1075	0.40	ng/ul	0.01
20) Perylene-d12	23.49	264	1532	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.09	152	265	0.16	ng/ul	0.00
14) Fluoranthene-d10	19.10	212	623	0.00	ng/ul	-0.01
Target Compounds						
9) Fluorene	15.29	166	138	0.06	ng/ul#	49
17) Pyrene	19.45	202	141	0.03	ng/ul#	1
23) Benzo(a)pyrene	23.34	252	282	0.05	ng/ul#	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008517.D
Acq On : 21 Dec 2016 15:09
Operator : UM/SJ
Sample : H5996-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA872

Quant Time: Dec 22 00:04:05 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:00:17 2016
Response via : Initial Calibration

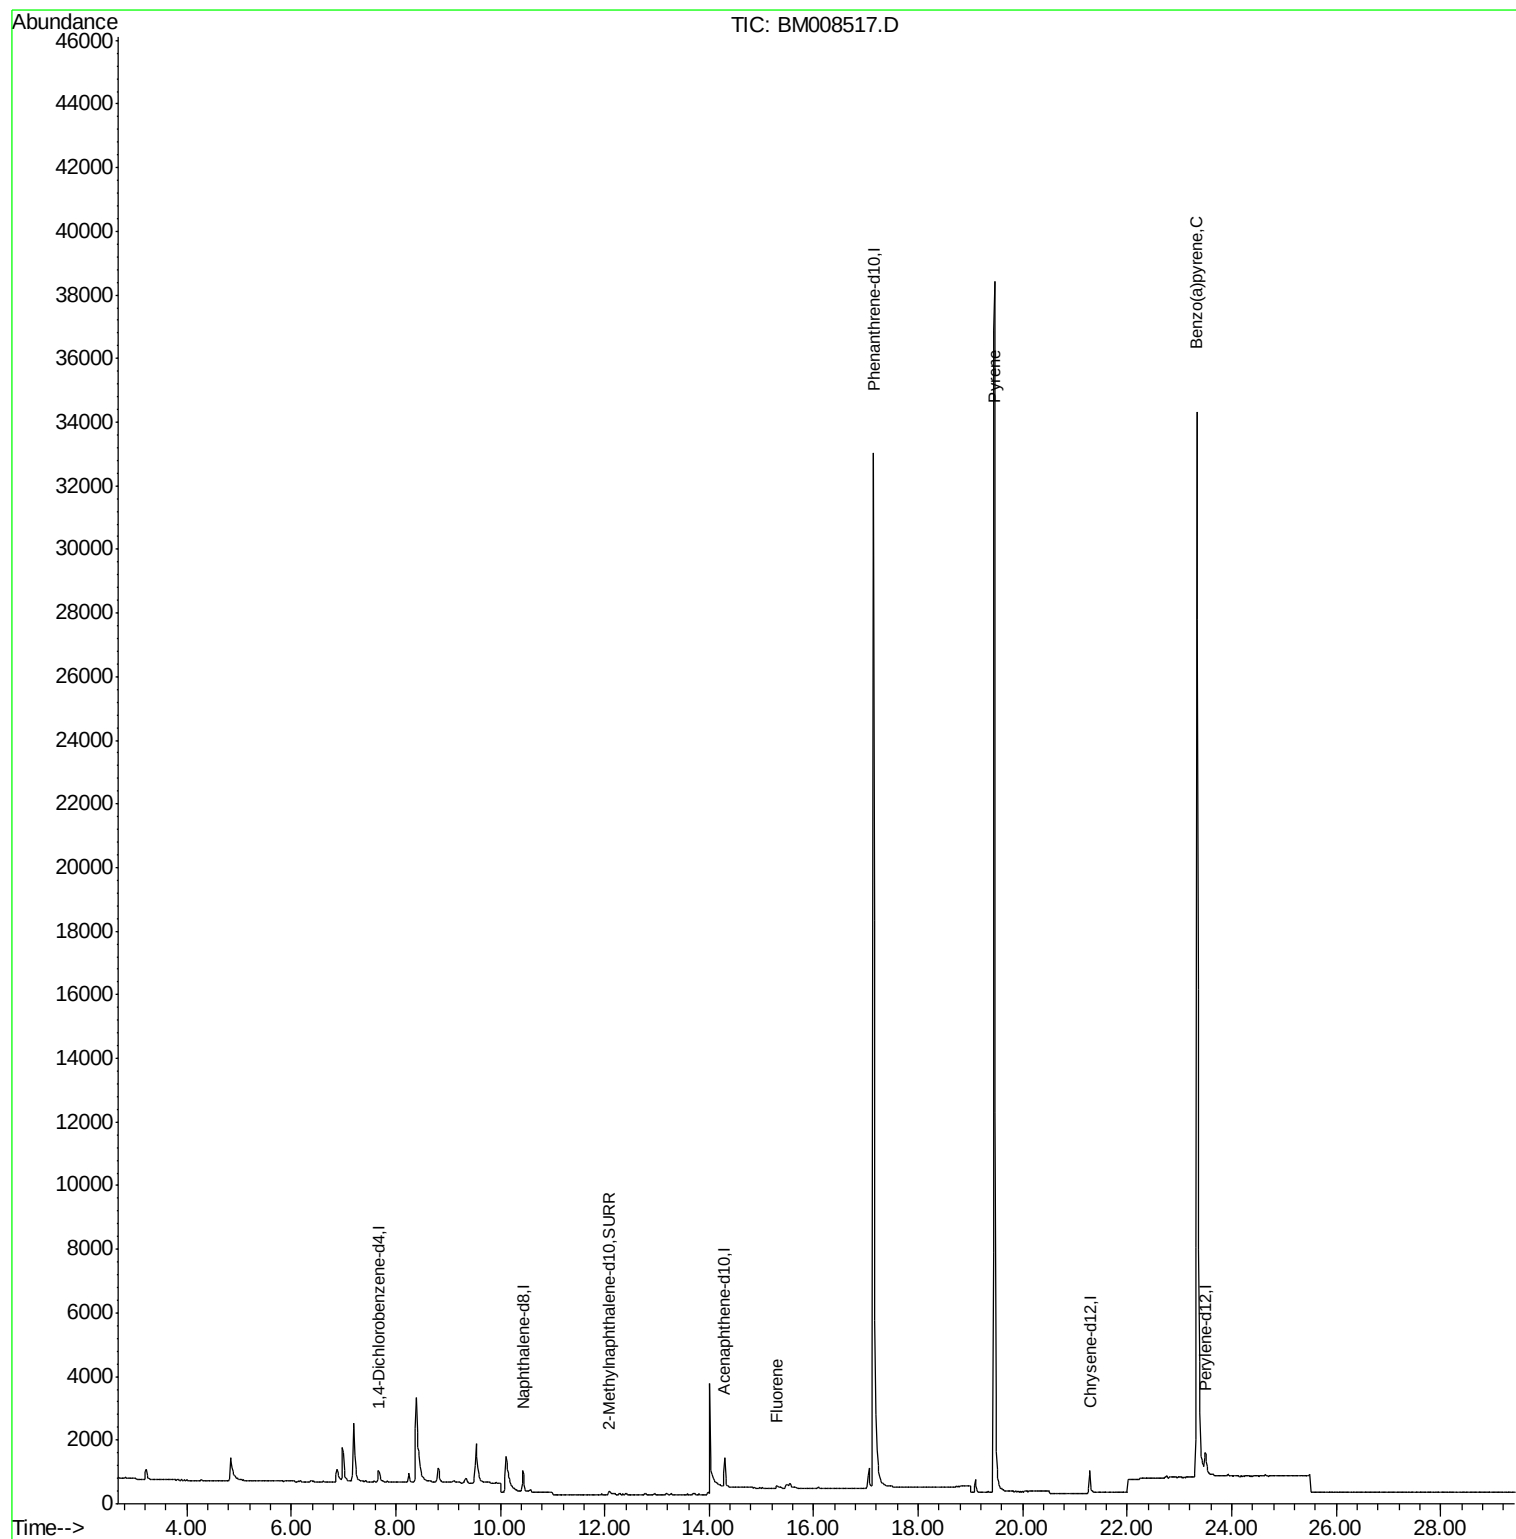

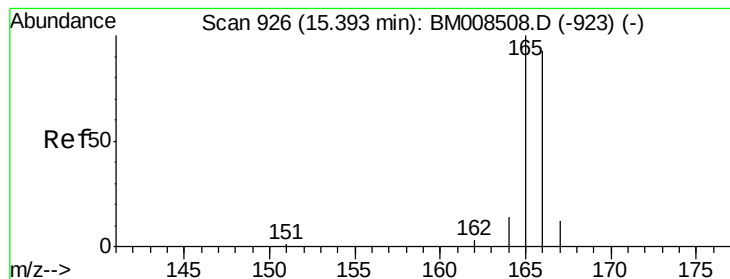

#9

Fluorene

Concen: 0.06 ng/ul

RT: 15.29 min Scan# 920

Delta R.T. -0.10 min

Lab File: BM008517.D

Acq: 21 Dec 2016 15:09

Instrument :

BNA_M

ClientSampleId :

DA872


Tgt Ion:166 Resp: 138

Ion Ratio Lower Upper

166 100

165 51.5 73.4 110.2#




167 60.2 14.6 22.0#

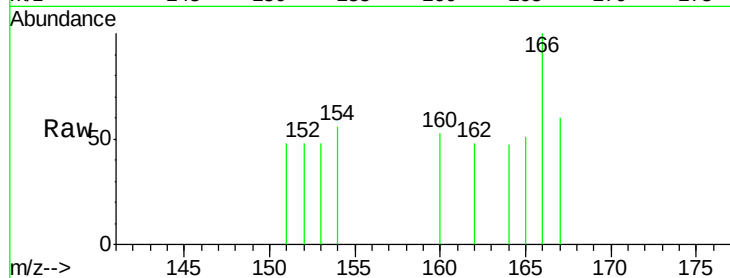

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

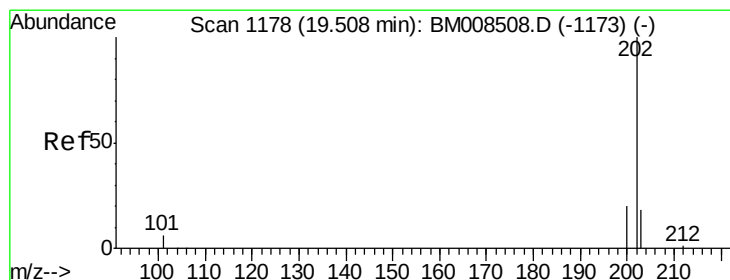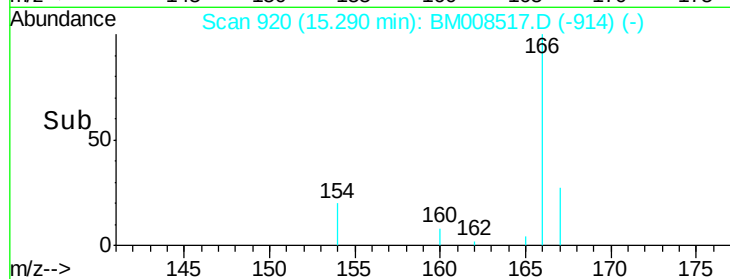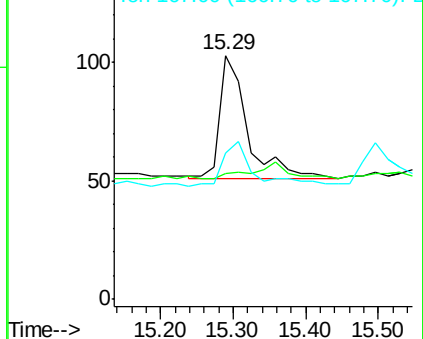

#17

Pyrene

Concen: 0.03 ng/ul

RT: 19.45 min Scan# 1173

Delta R.T. -0.06 min

Lab File: BM008517.D

Acq: 21 Dec 2016 15:09


Tgt Ion:202 Resp: 141

Ion Ratio Lower Upper

202 100

200 45.9 18.2 27.4#



203 122.0 15.6 23.4#

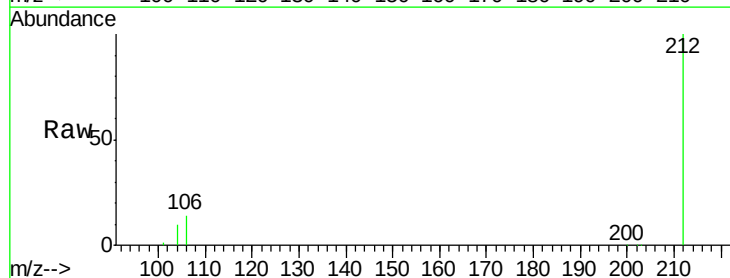


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

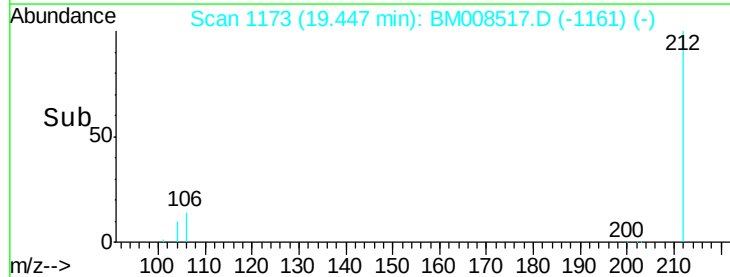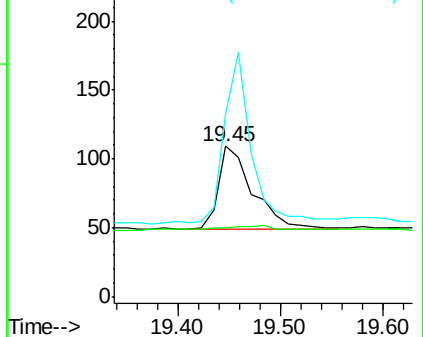

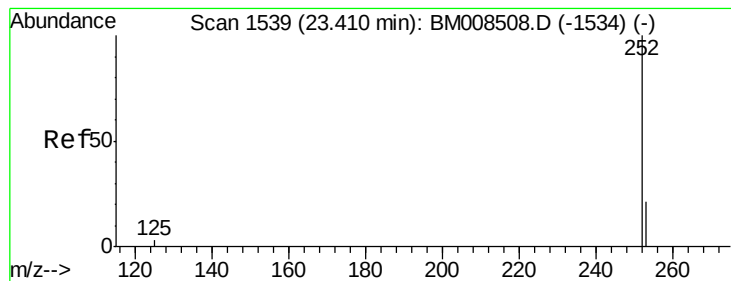

#23

Benzo(a)pyrene

Concen: 0.05 ng/ul

RT: 23.34 min Scan# 1532

Delta R.T. -0.07 min

Lab File: BM008517.D


Acq: 21 Dec 2016 15:09

Instrument :

BNA_M

ClientSampleId :

DA872

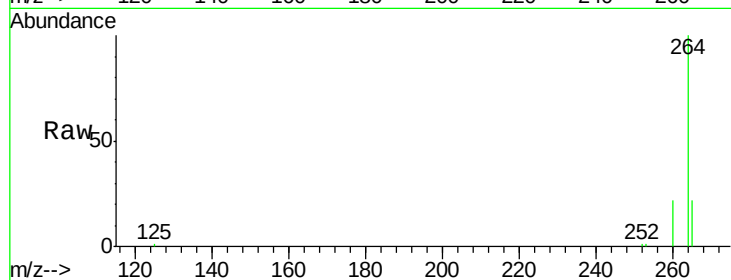


Tgt Ion: 252 Resp: 282

Ion Ratio Lower Upper

252 100

253 91.5 28.5 42.7#

125 63.7 18.1 27.1#

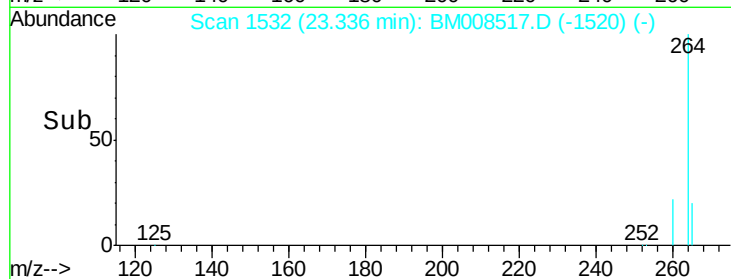

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

