




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:28:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

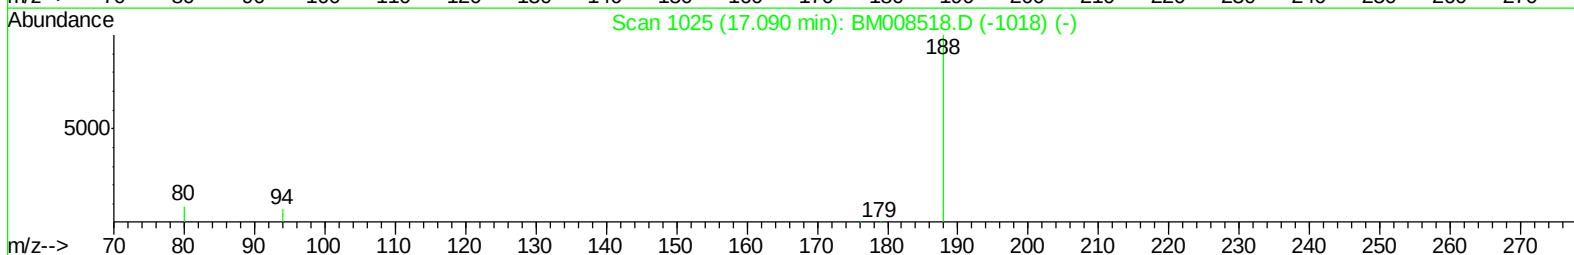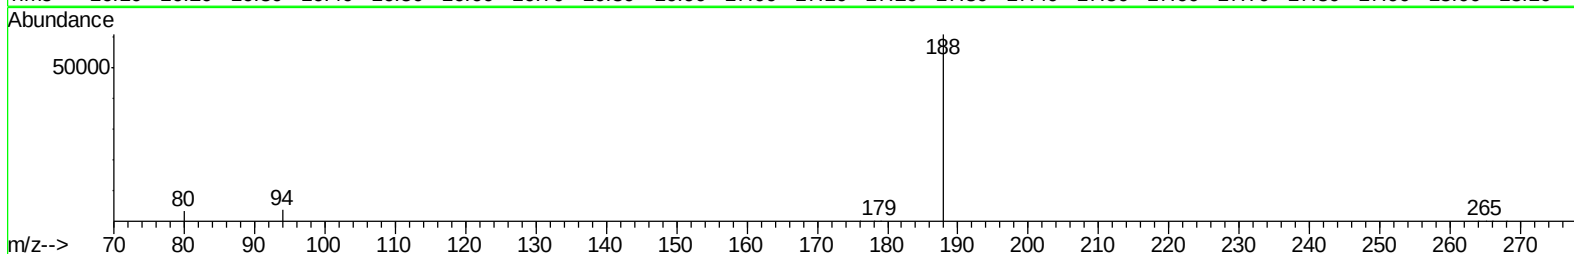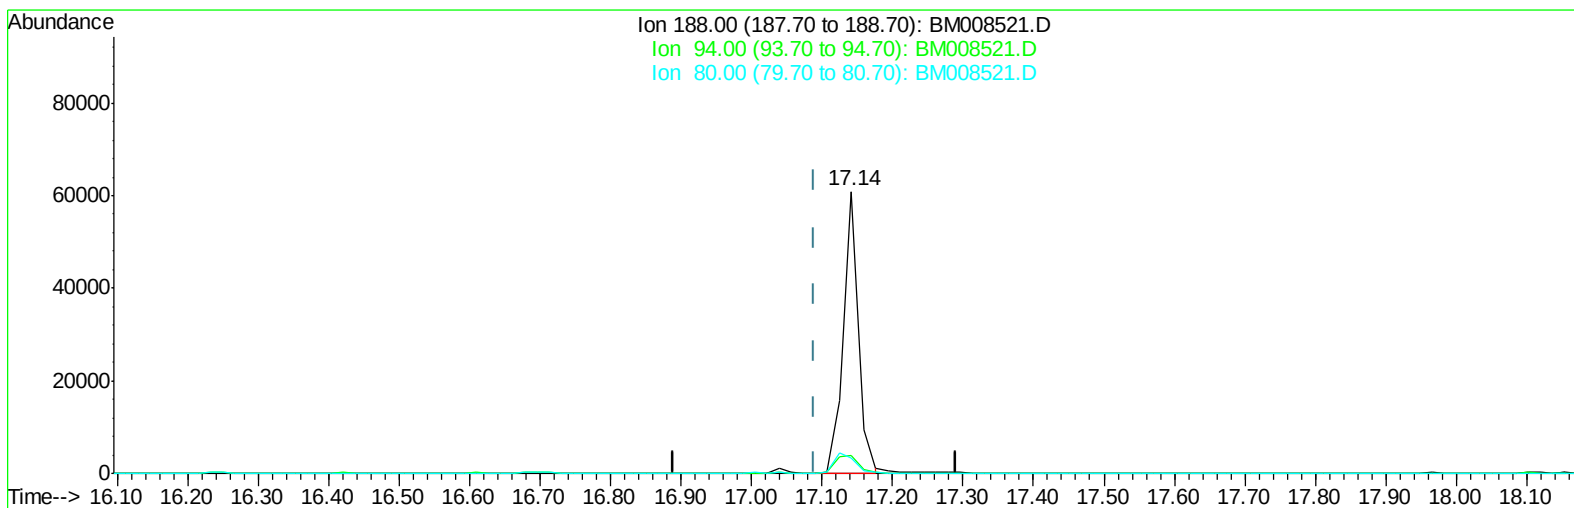

TIC: BM008521.D

(10) Phenanthrene-d10 (I)

17.142min (+0.051) 0.40ng/ul

response 89541

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.18#
80.00	11.80	5.38#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:28:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

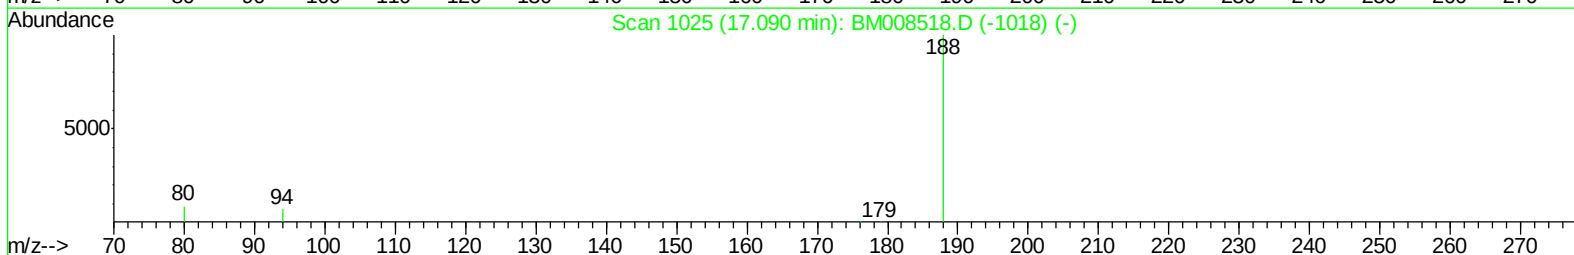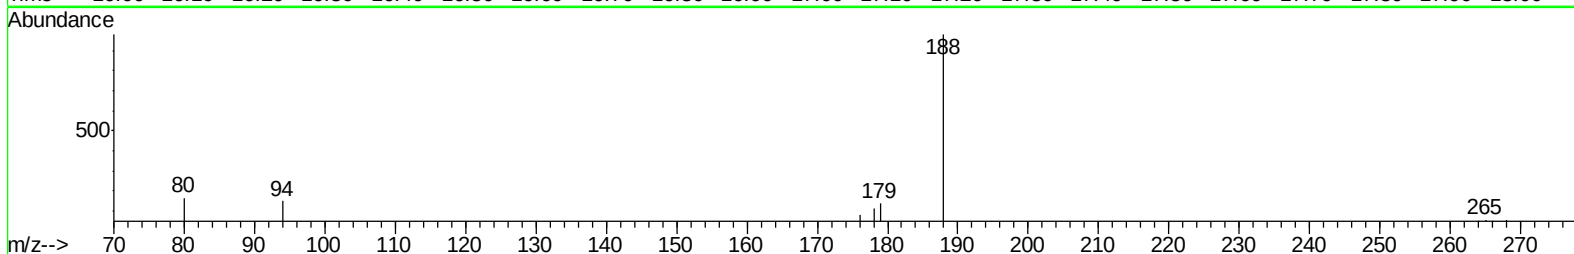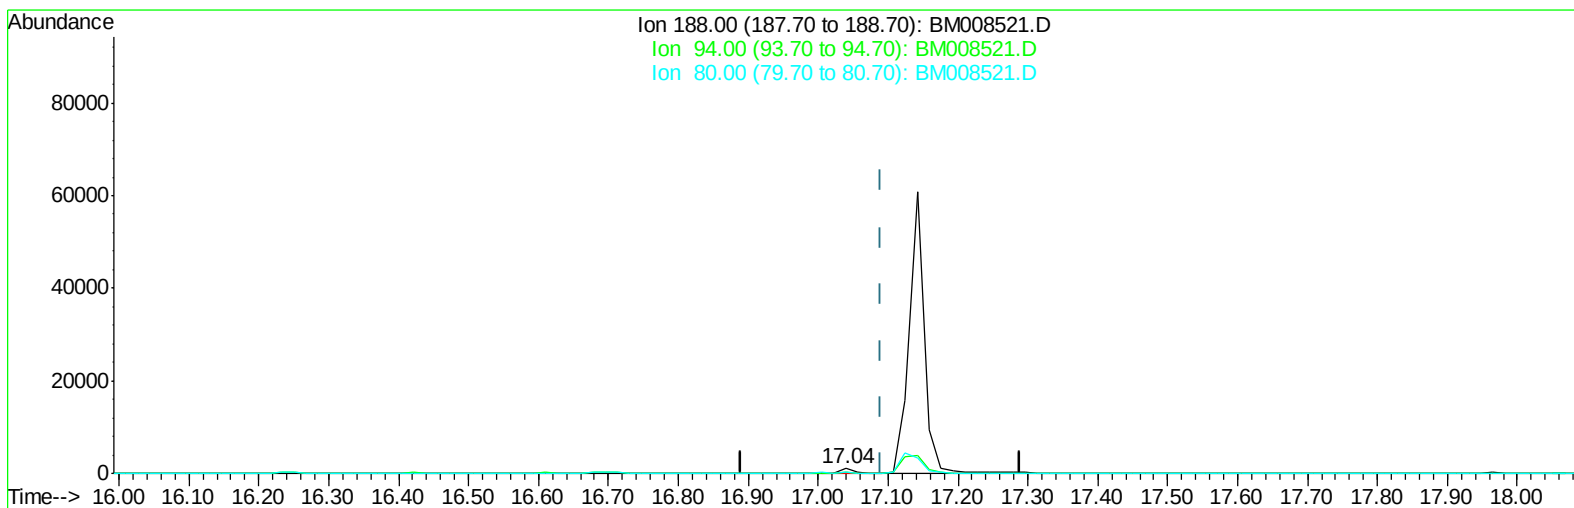

TIC: BM008521.D

(10) Phenanthrene-d10 (I)

17.039min (-0.052) 0.40ng/ul m

response 1515

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	15.31#
80.00	11.80	16.73#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:28:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

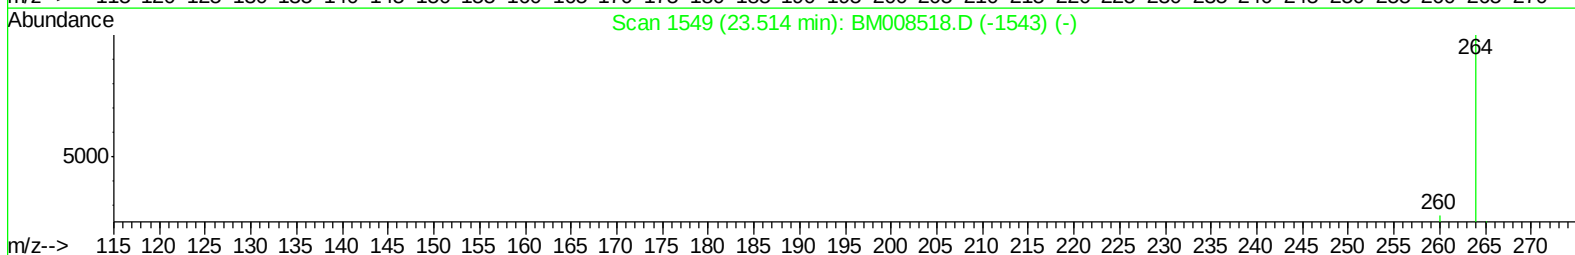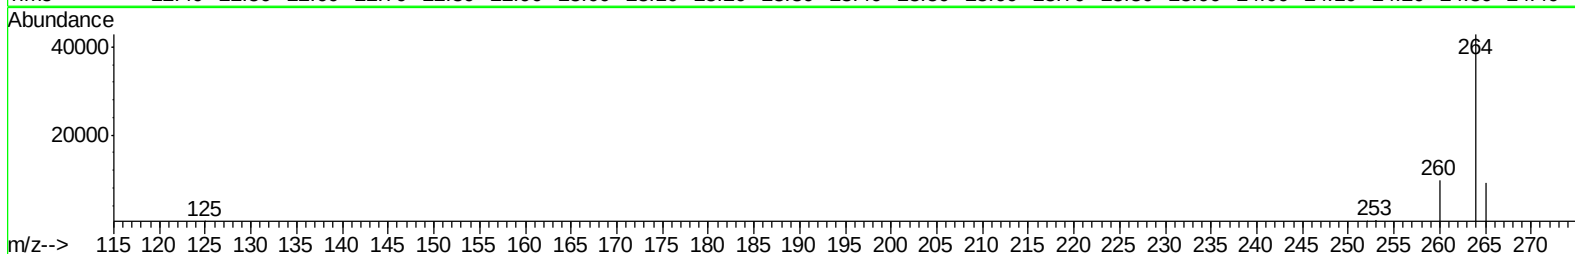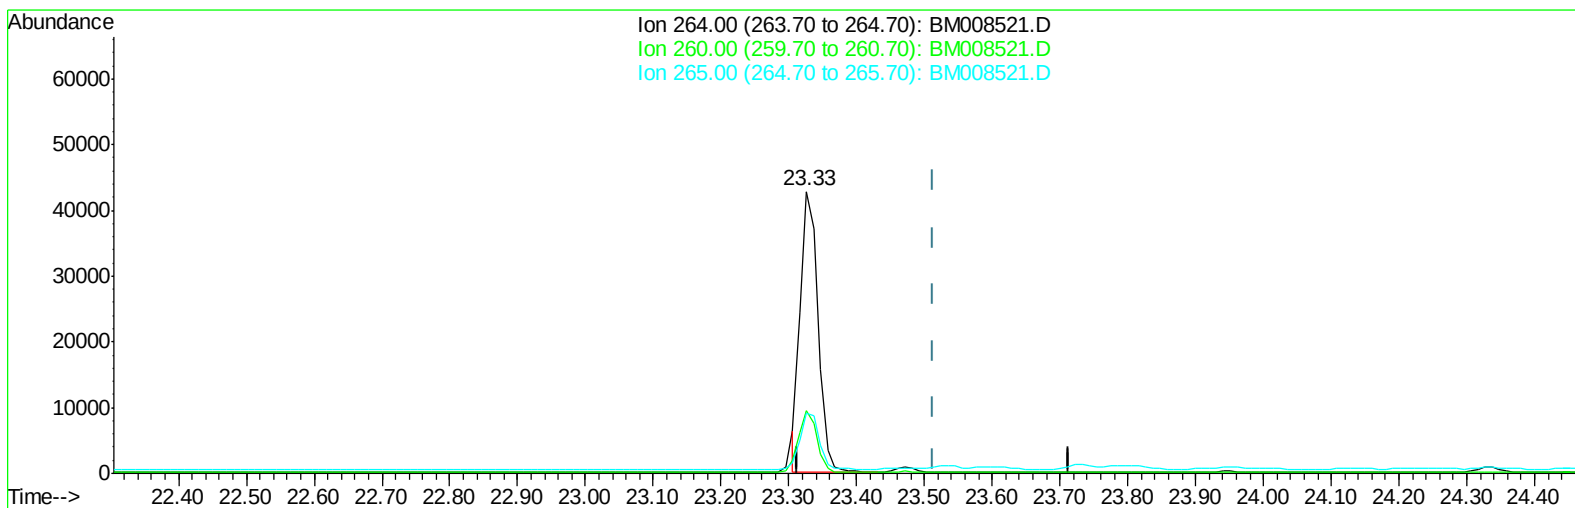

TIC: BM008521.D

(20) Perylene-d12 (I)

23.326min (-0.188) 0.40ng/ul

response 77601

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.47#
265.00	103.50	21.18#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:28:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

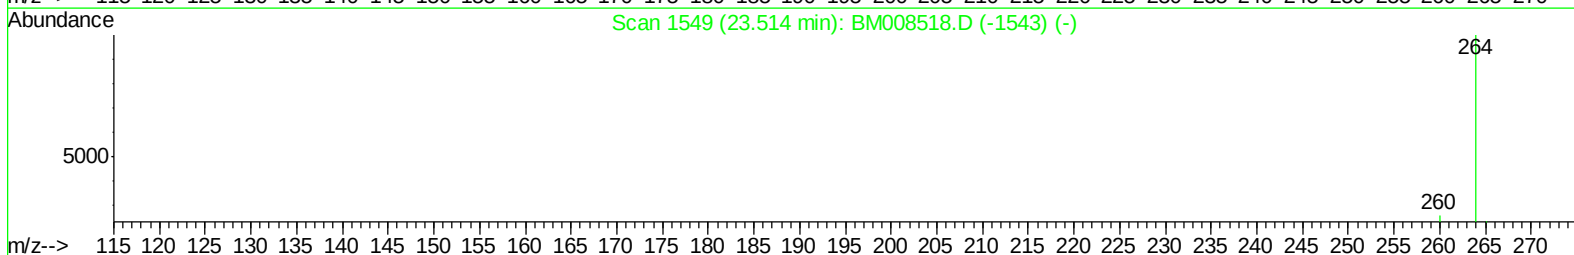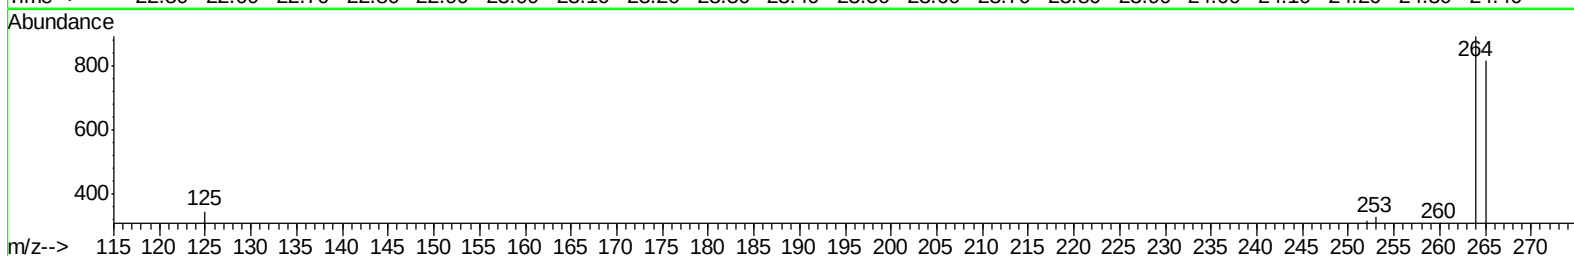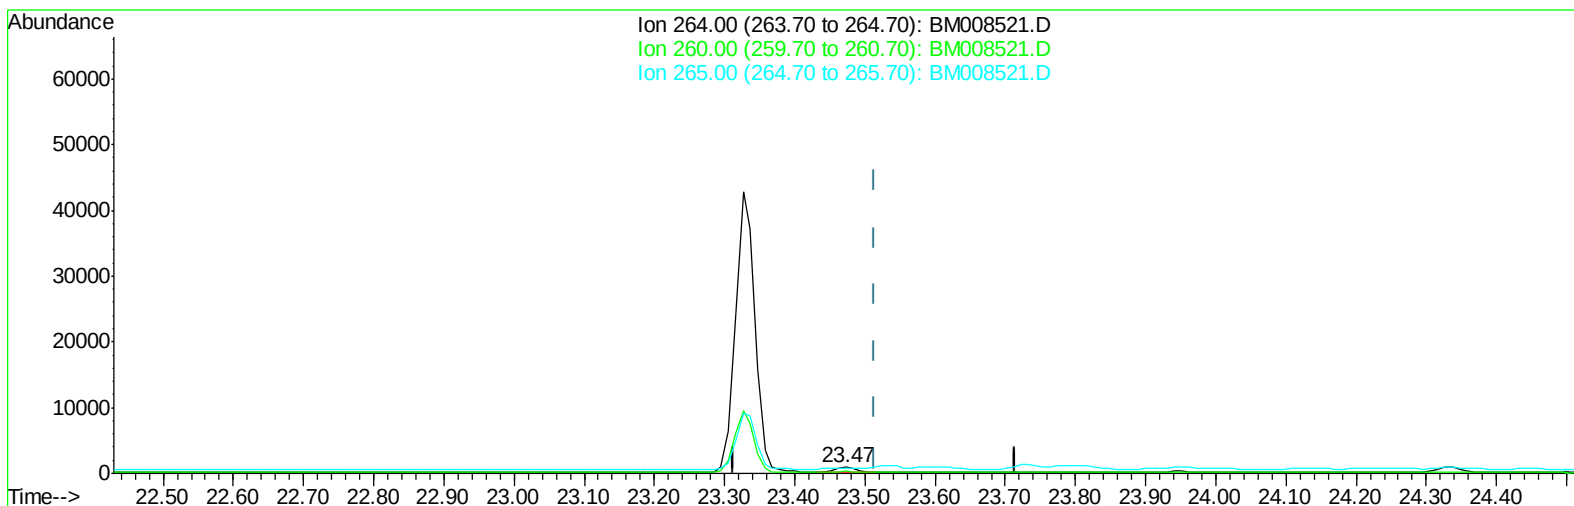

TIC: BM008521.D

(20) Perylene-d12 (I)

23.472min (-0.042) 0.40ng/ul m

response 1638

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	34.49
265.00	103.50	91.60
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

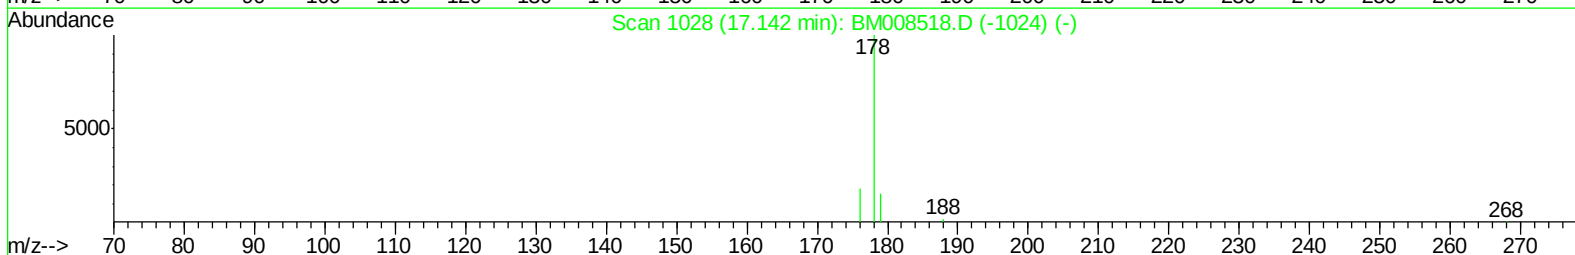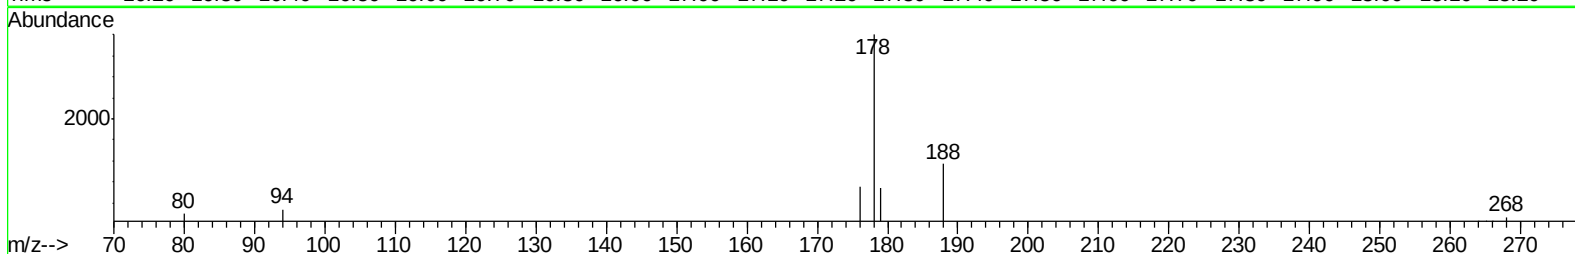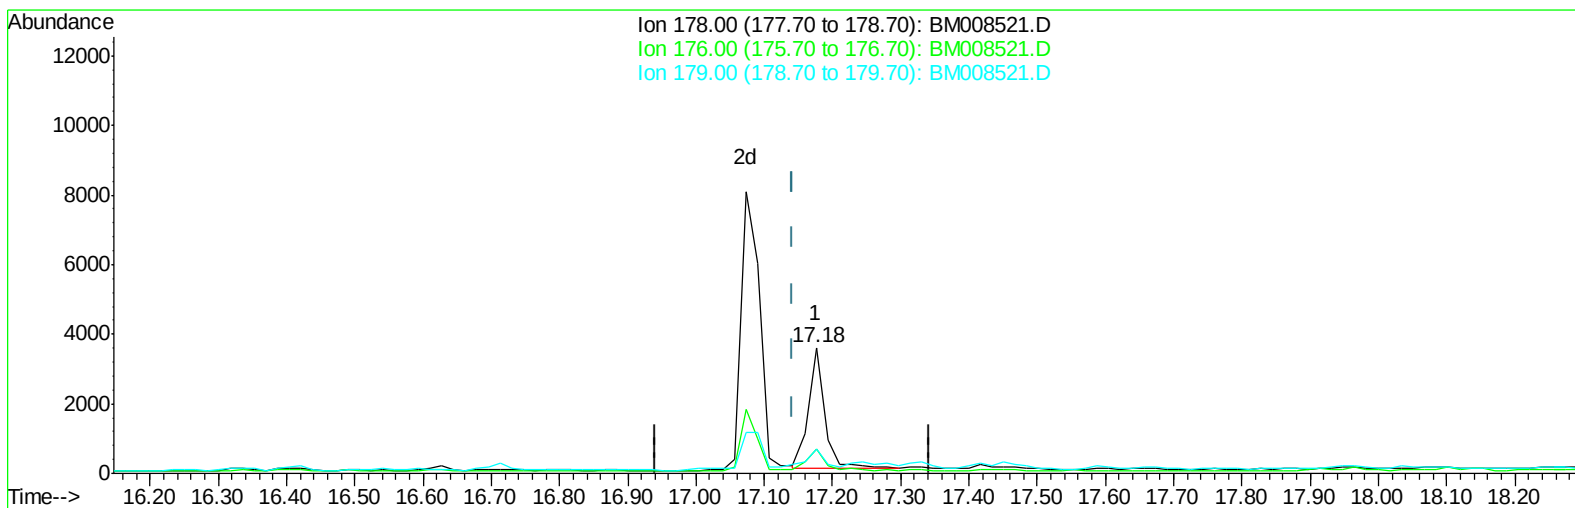

TIC: BM008521.D

(12) Phenanthrene

17.176min (+0.034) 1.26ng/ul

response 5847

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	19.83
179.00	17.00	19.27
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

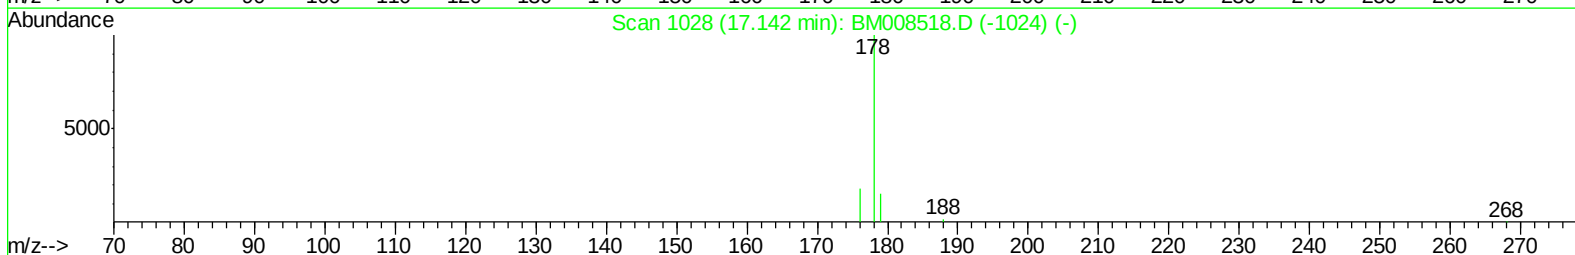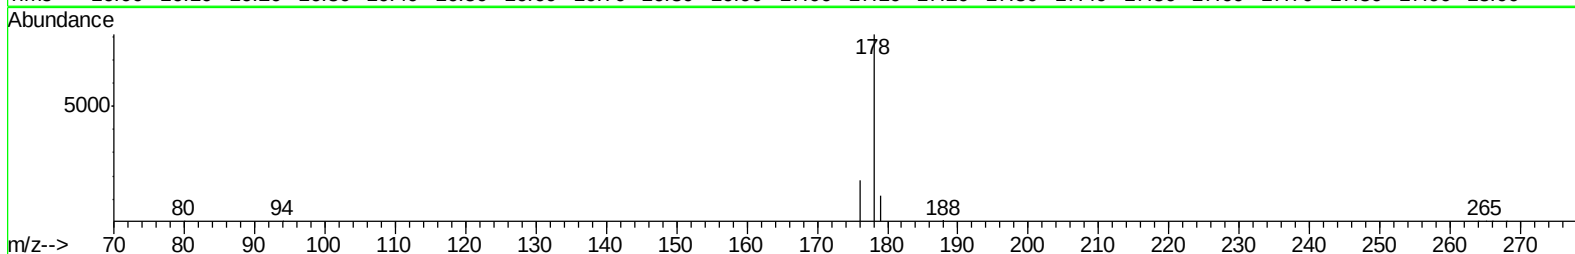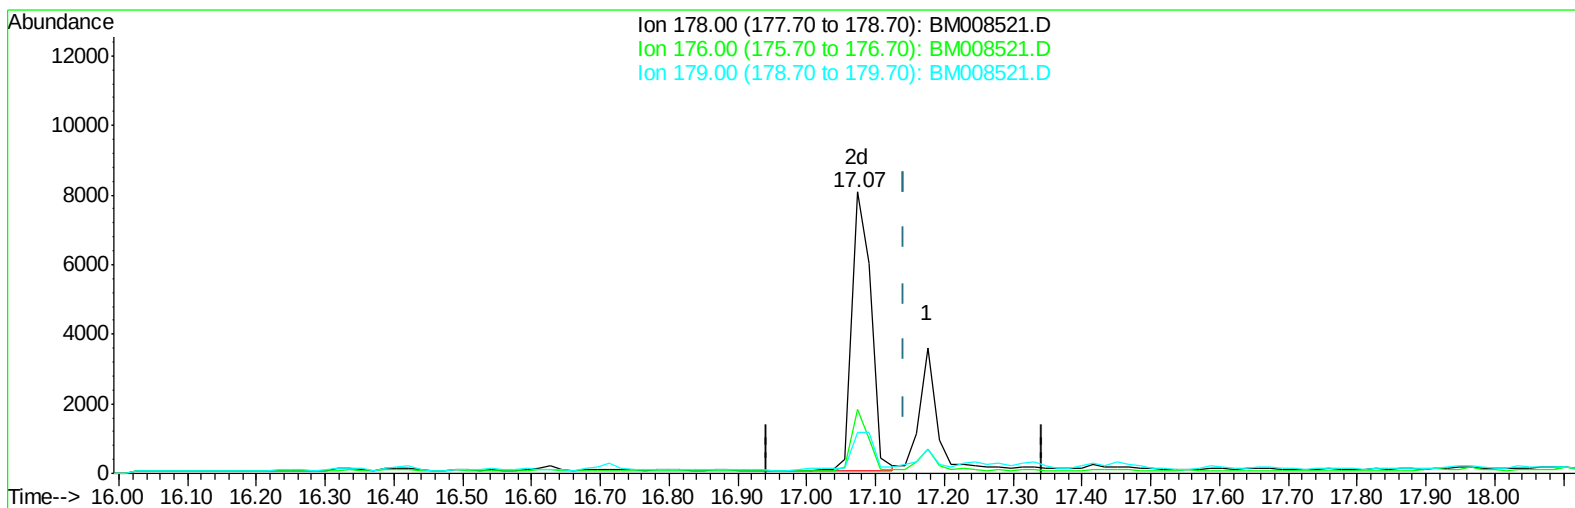

TIC: BM008521.D

(12) Phenanthrene

17.073min (-0.069) 3.33ng/ul m

response 15421

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	22.63
179.00	17.00	14.53
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

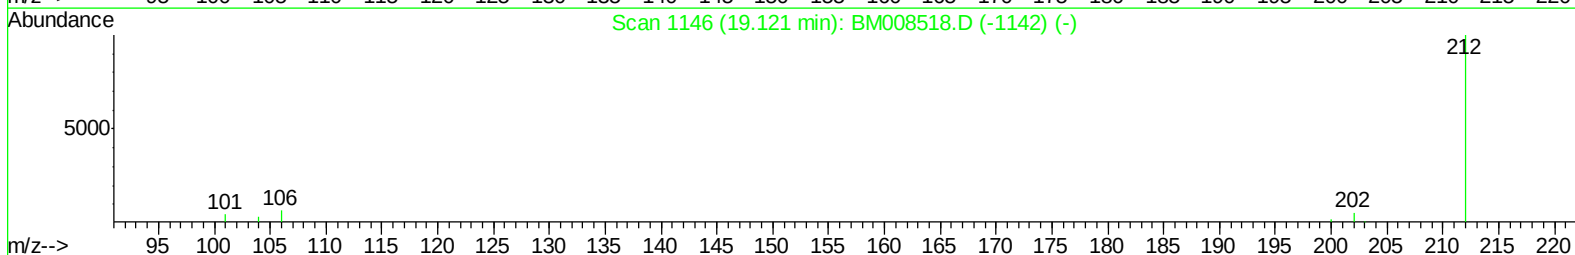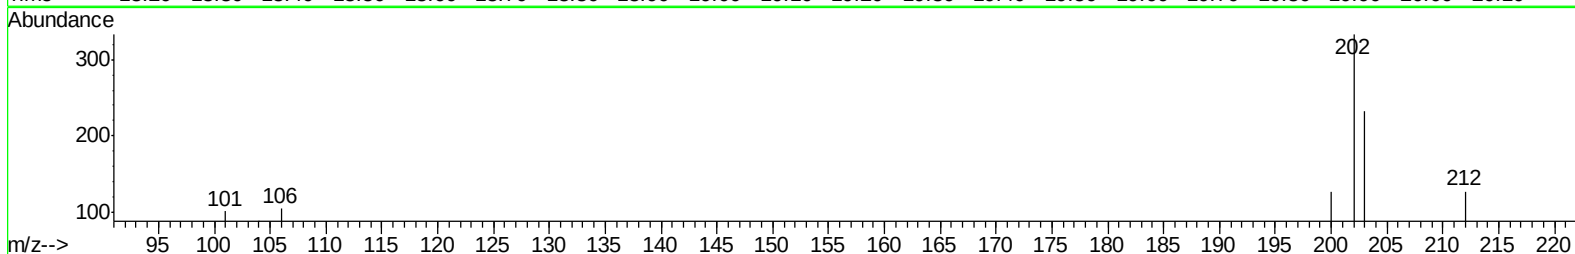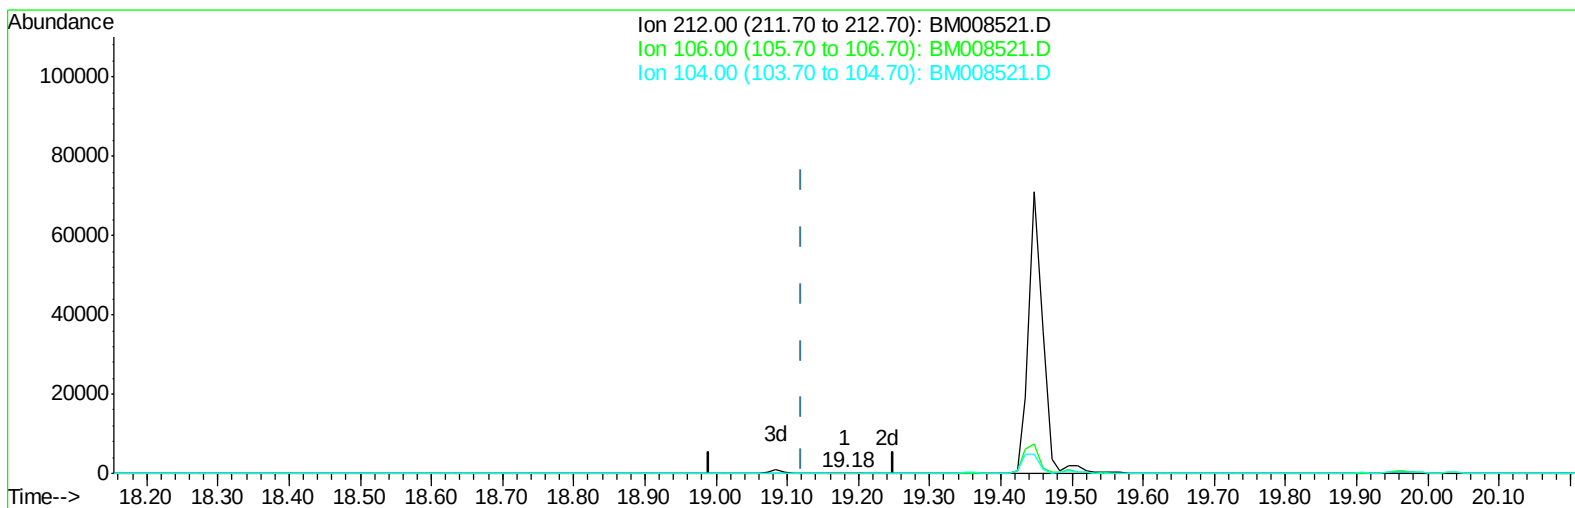

TIC: BM008521.D

(14) Fluoranthene-d10 (SURR)

19.181min (+0.060) 0.01ng/ul

response 54

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	51.85#
104.00	15.60	29.63#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

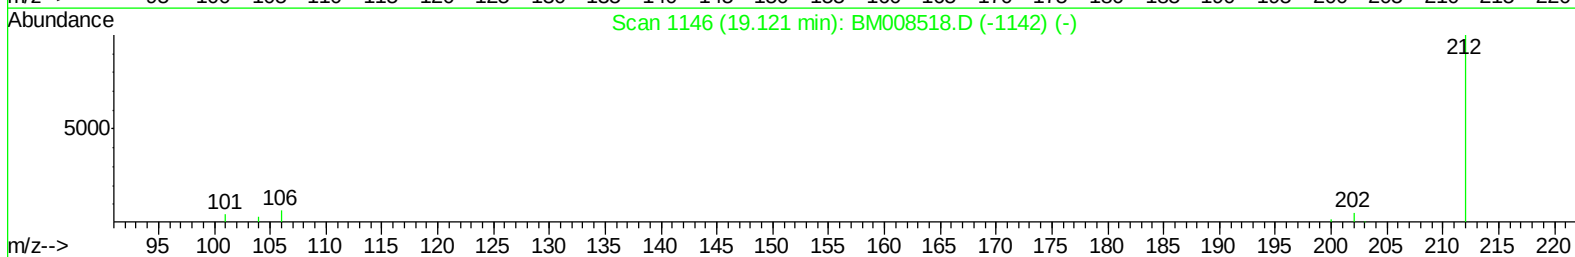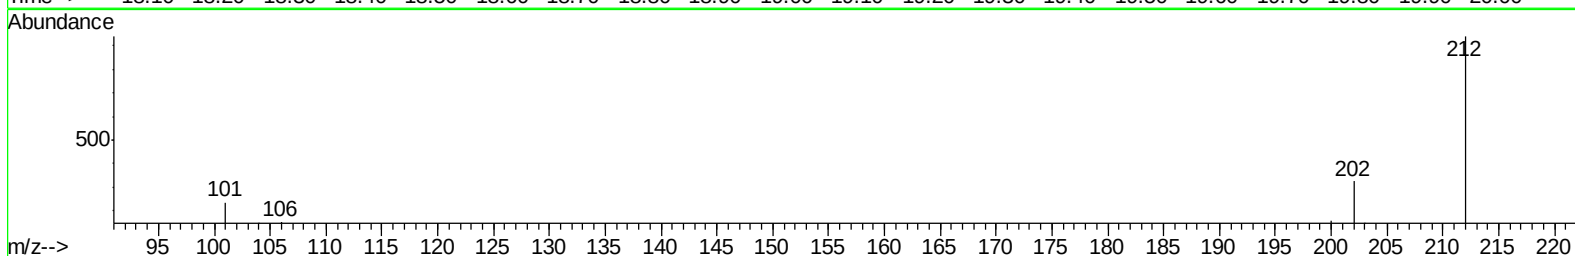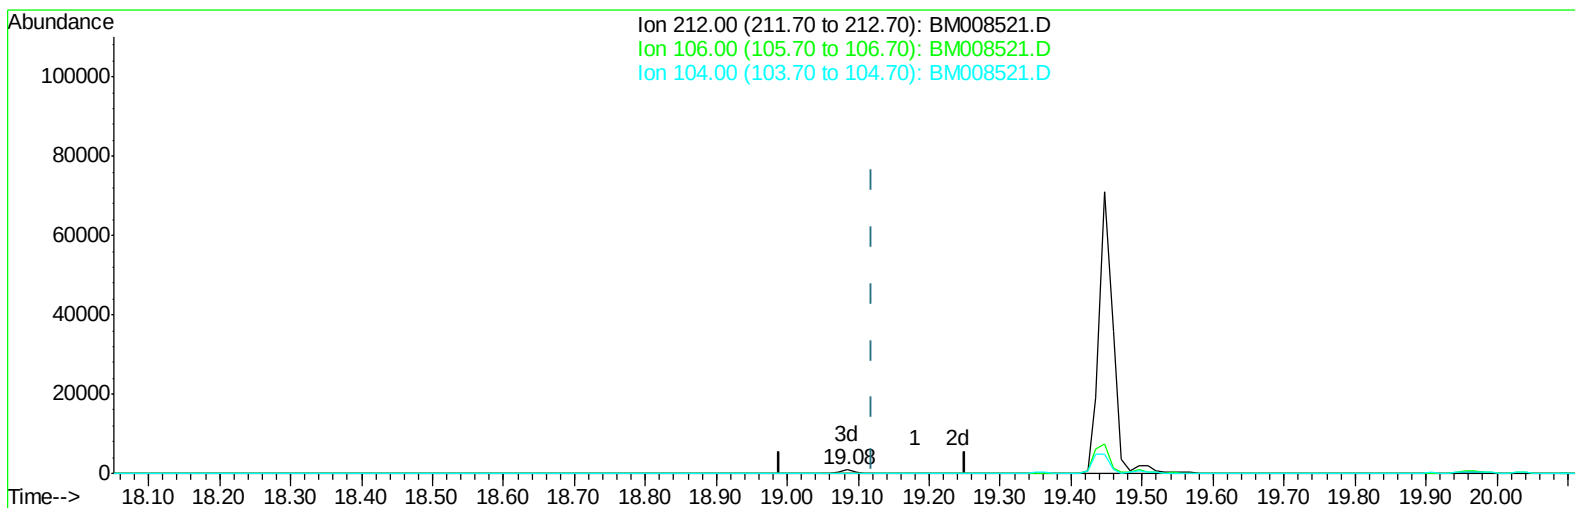

TIC: BM008521.D

(14) Fluoranthene-d10 (SURR)

19.084min (-0.036) 0.27ng/ul m

response 1145

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	2.45#
104.00	15.60	1.40#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

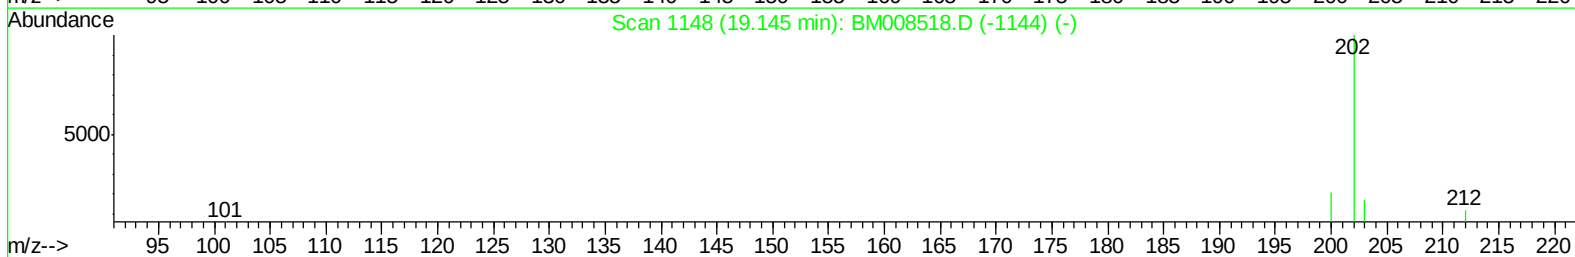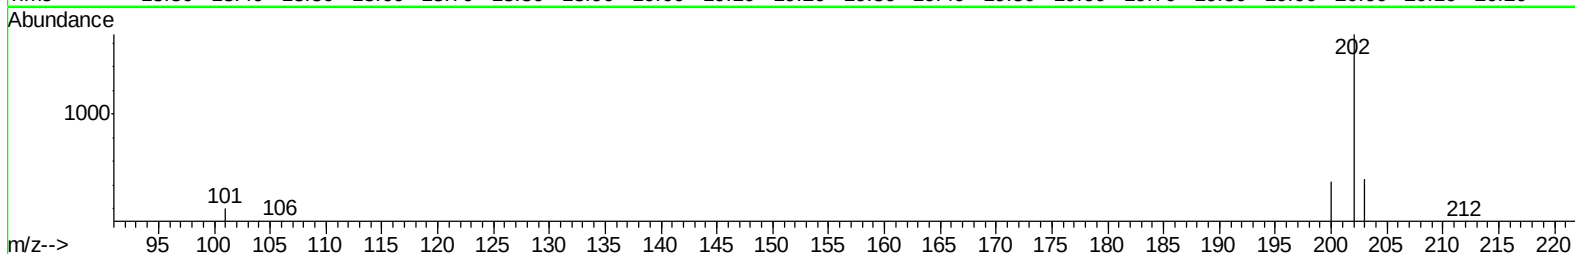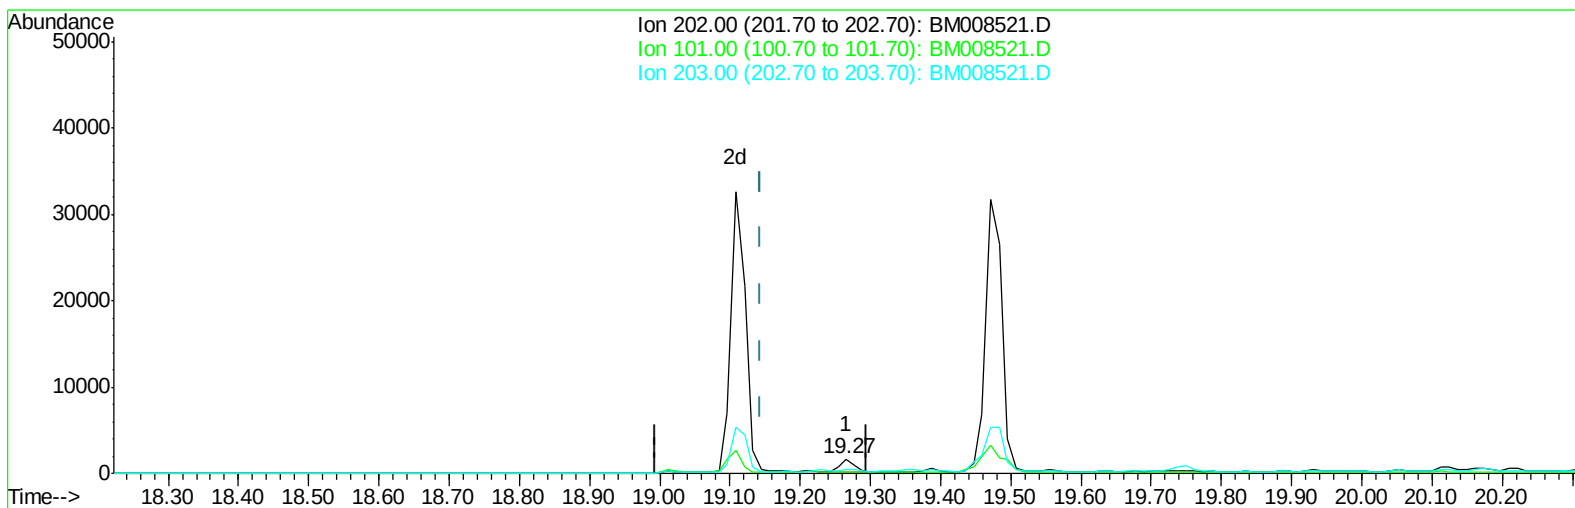

TIC: BM008521.D

(15) Fluoranthene (C)

19.266min (+0.121) 0.34ng/ul

response 1939

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	11.71
203.00	19.50	26.88
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

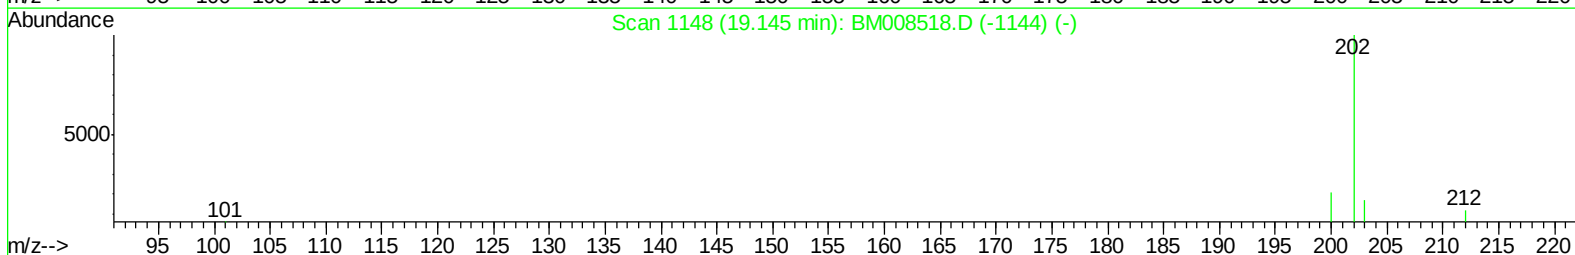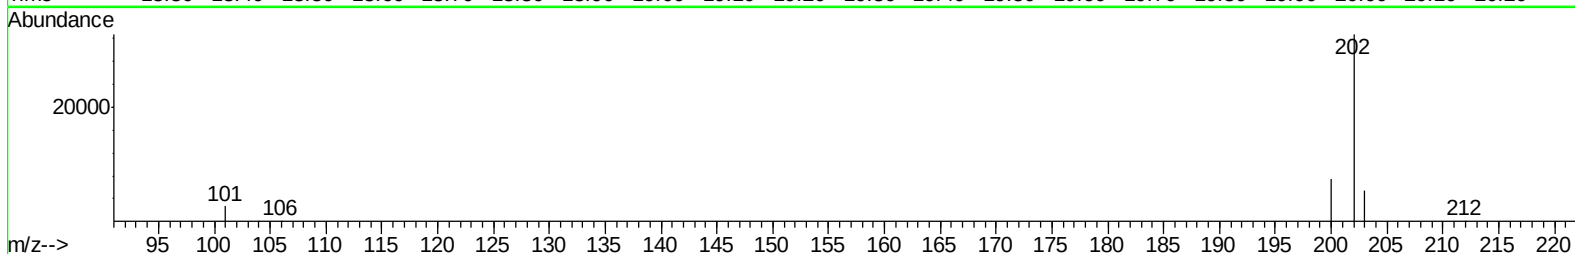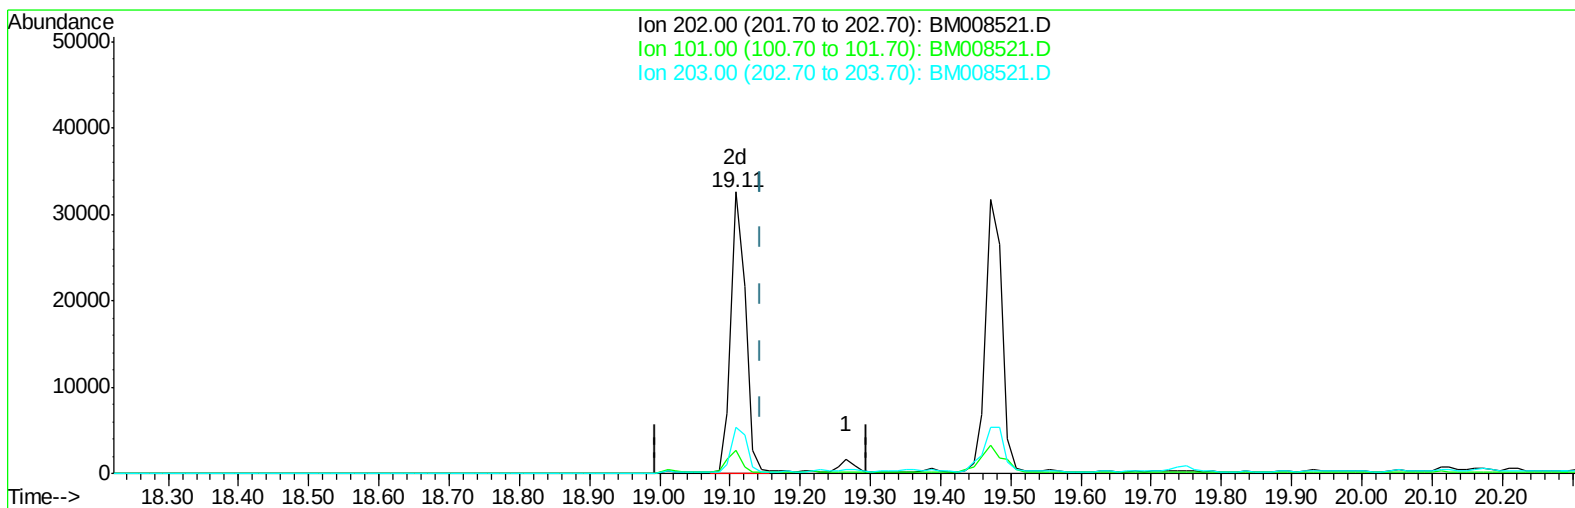

TIC: BM008521.D

(15) Fluoranthene (C)

19.108min (-0.036) 8.31ng/ul m

response 47128

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	8.18
203.00	19.50	16.46
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

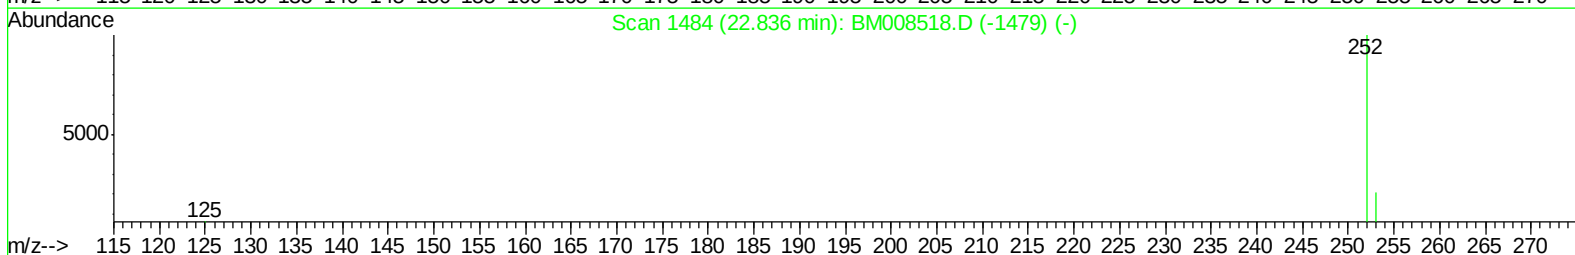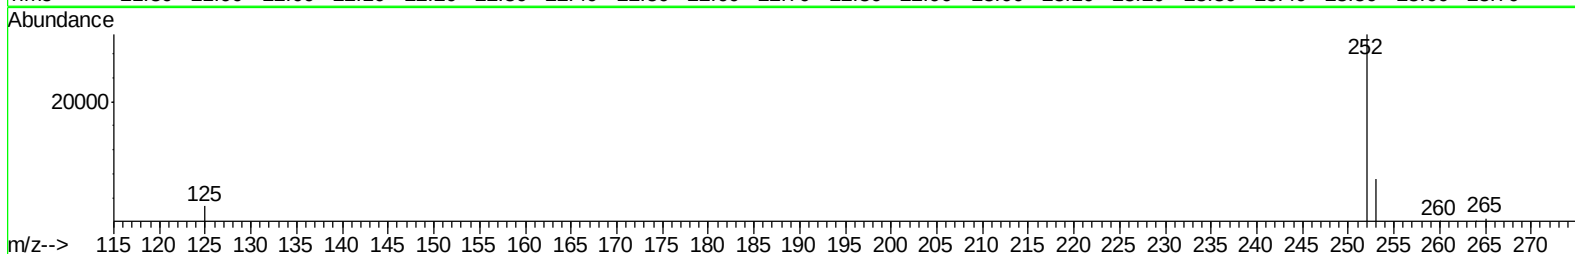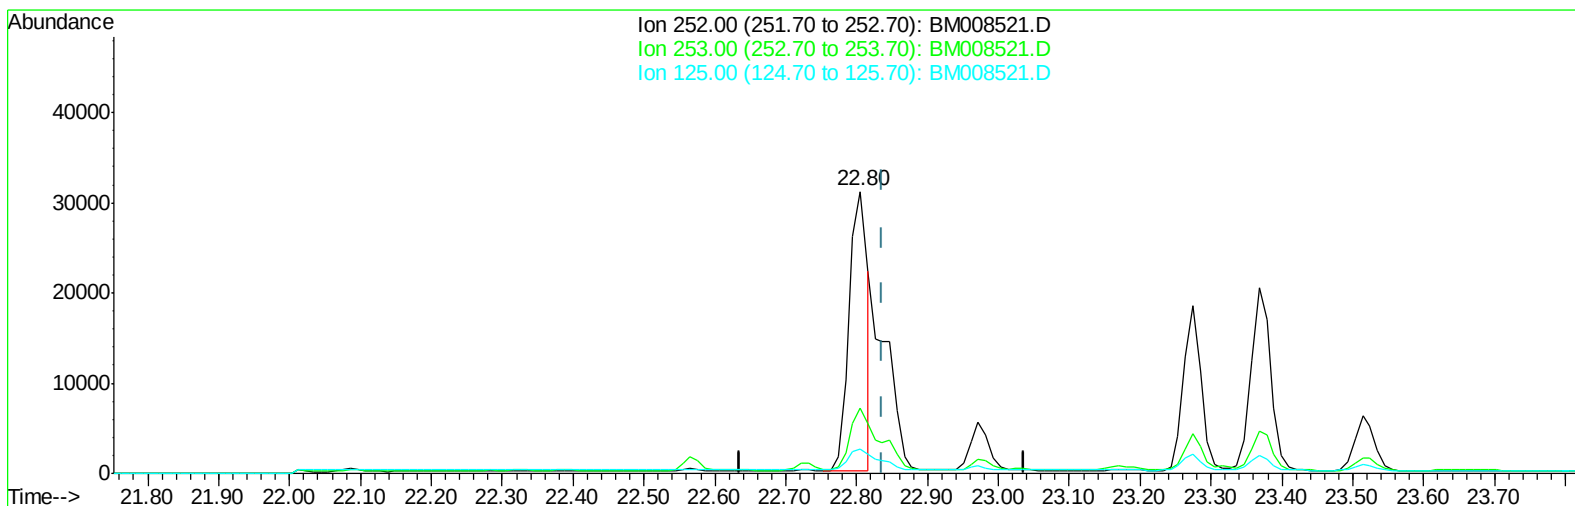

TIC: BM008521.D

(21) Benzo(b)fluoranthene
22.805min (-0.031) 8.80ng/ul
response 56753

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.22
125.00	17.50	8.43
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

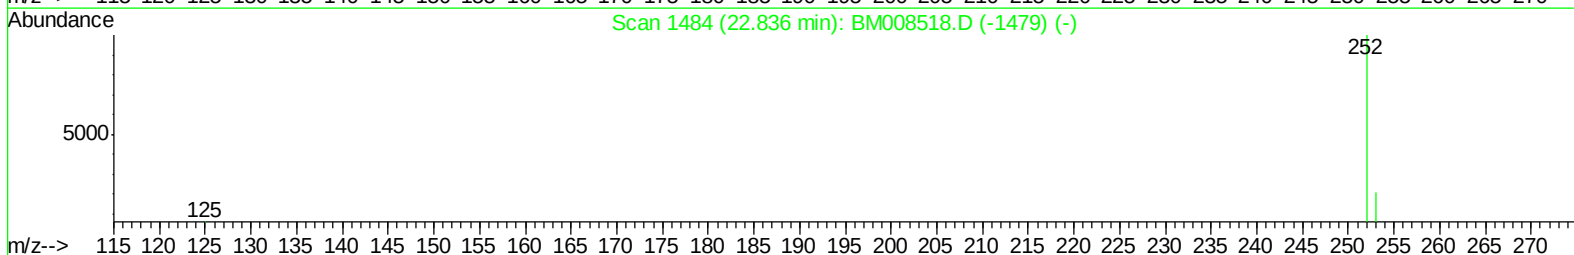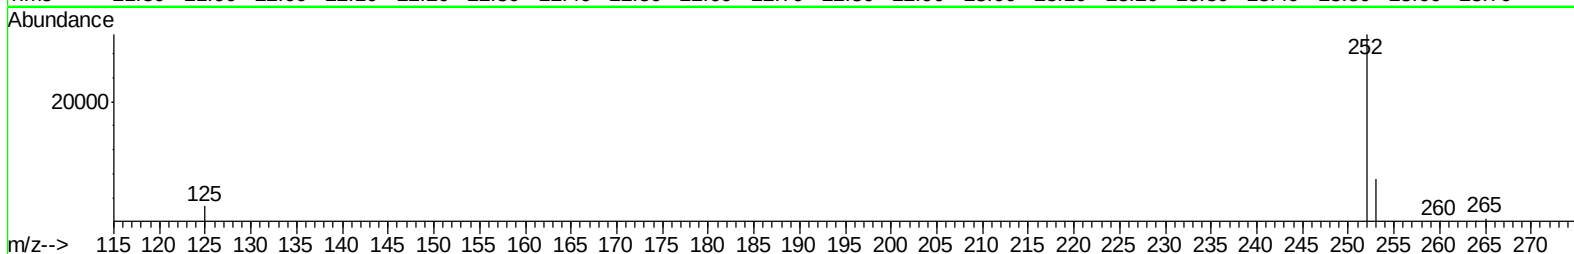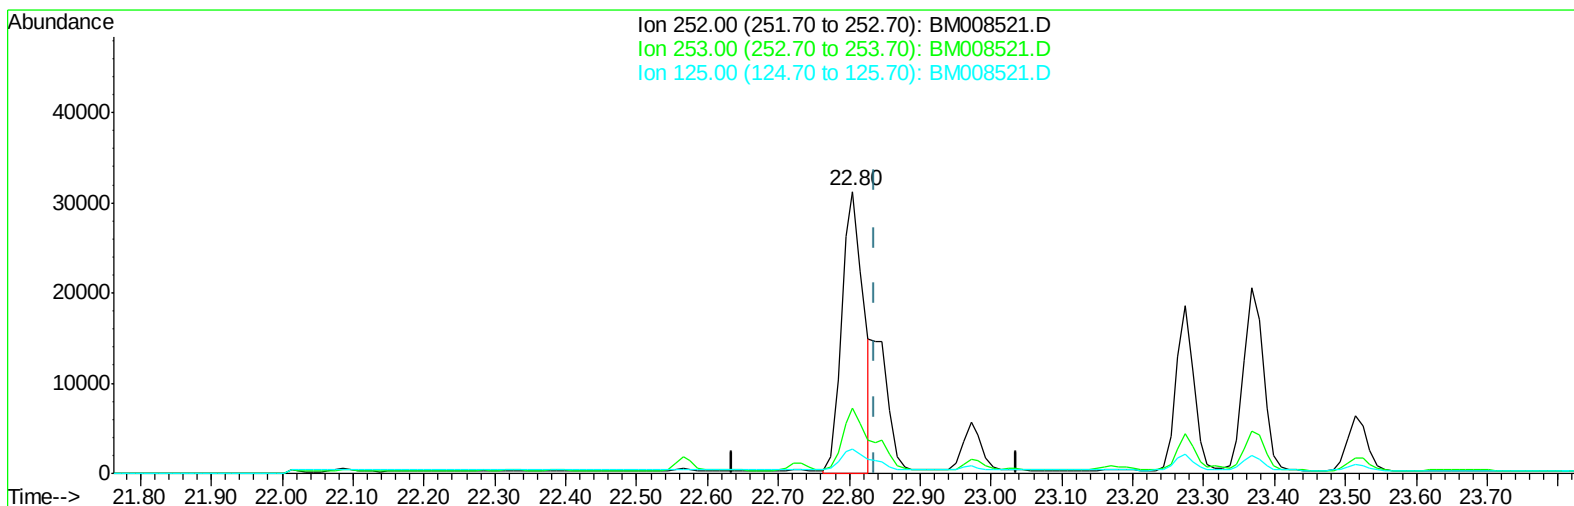

TIC: BM008521.D

(21) Benzo(b)fluoranthene

22.805min (-0.031) 10.38ng/ul m

response 66978

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.22
125.00	17.50	8.43
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

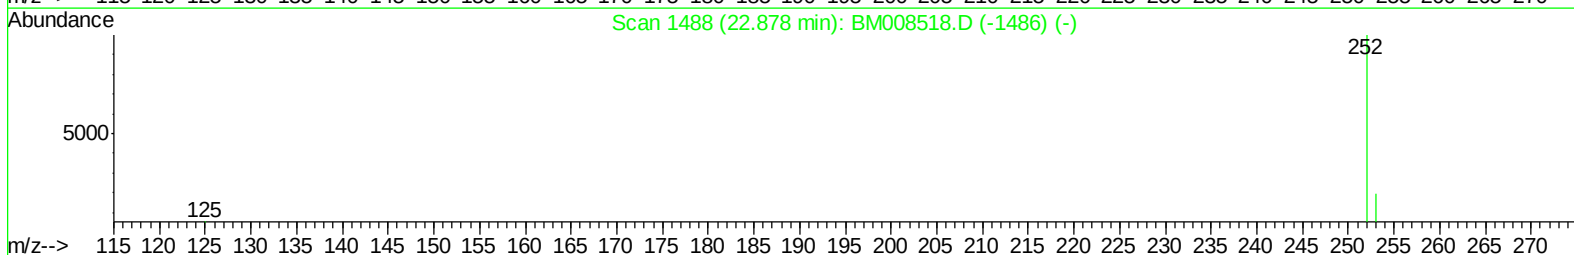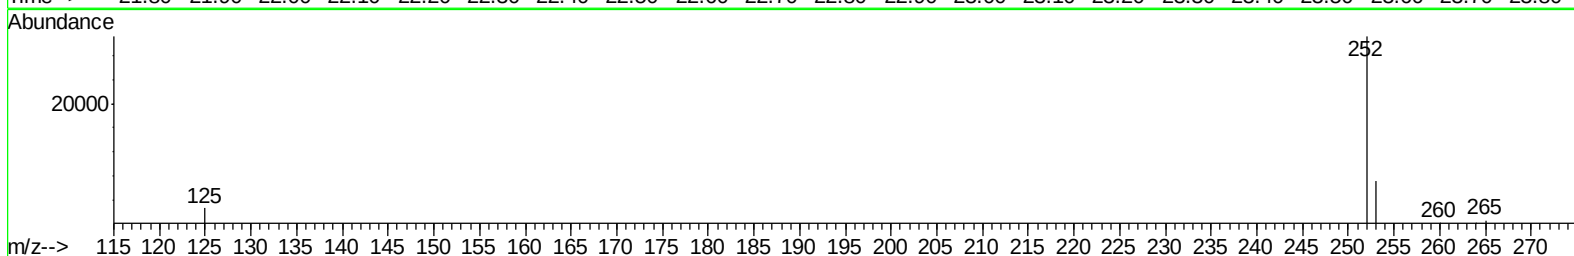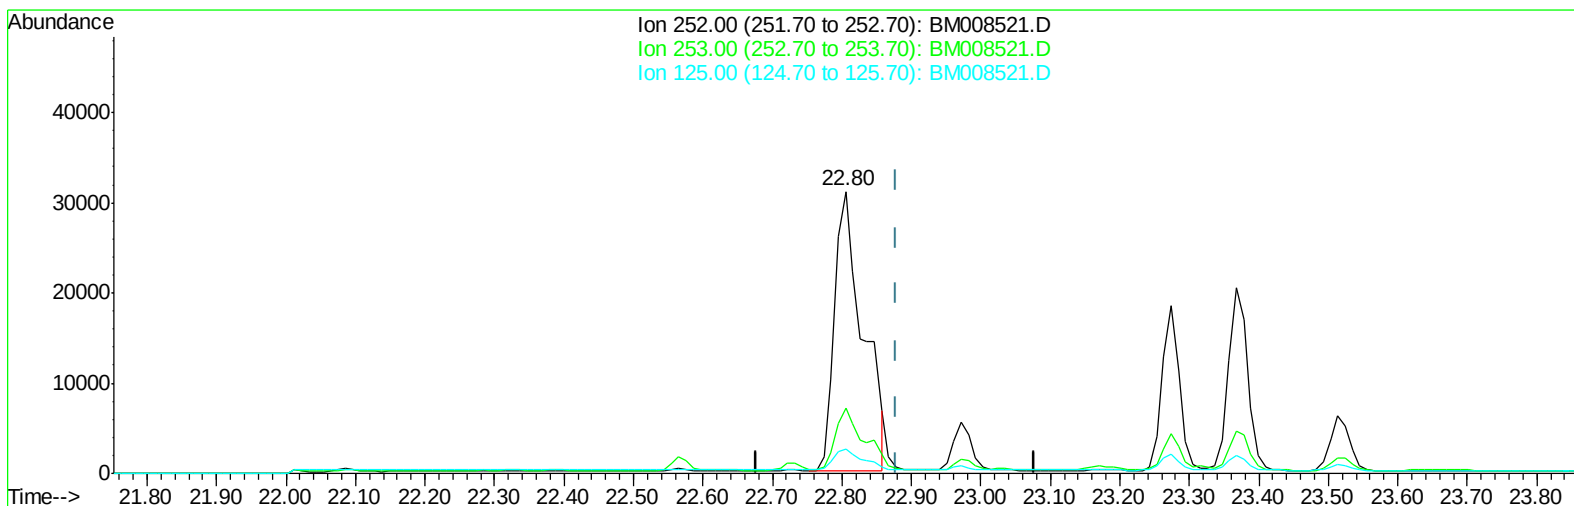

TIC: BM008521.D

(22) Benzo(k)fluoranthene

22.805min (-0.073) 13.98ng/ul

response 87956

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.22#
125.00	17.10	8.43#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

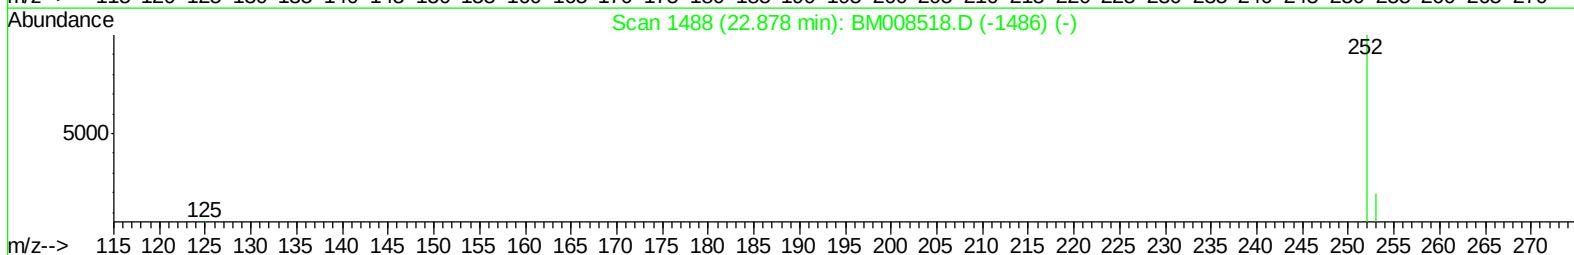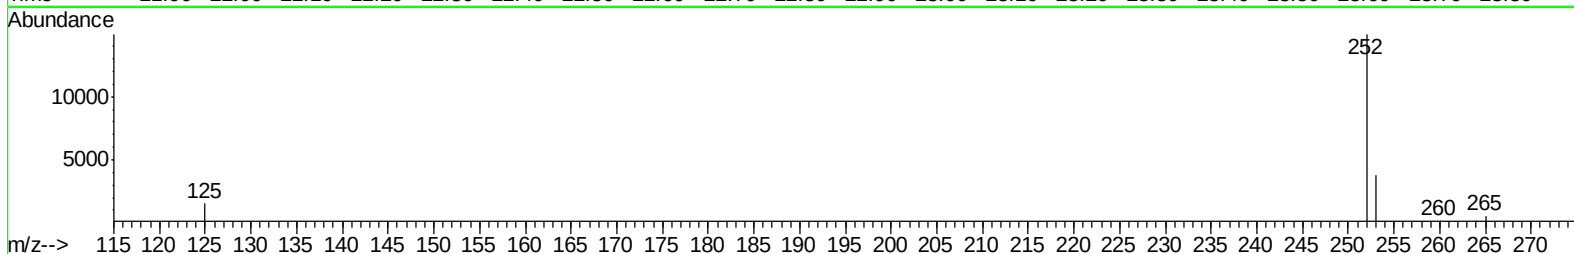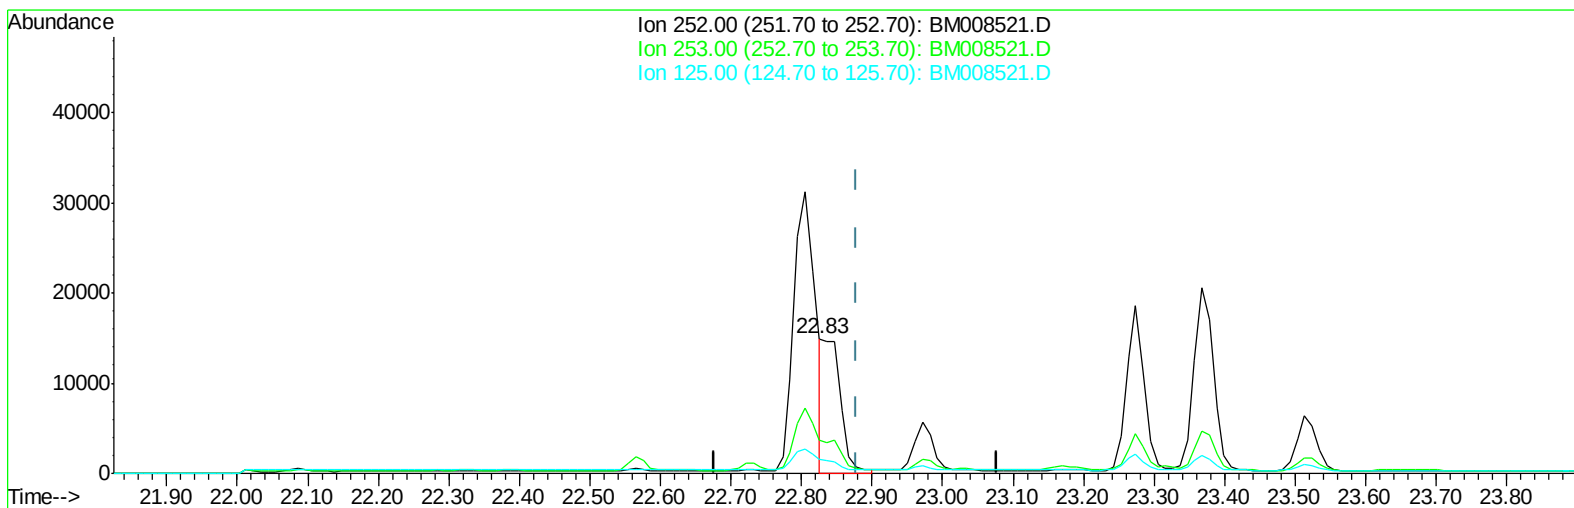

TIC: BM008521.D

(22) Benzo(k)fluoranthene

22.826min (-0.052) 3.92ng/ul m

response 24696

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	25.05
125.00	17.10	10.19#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

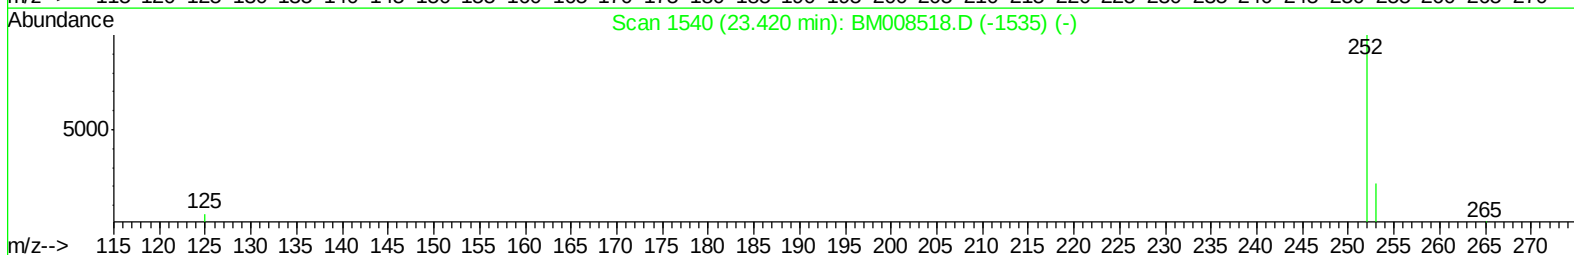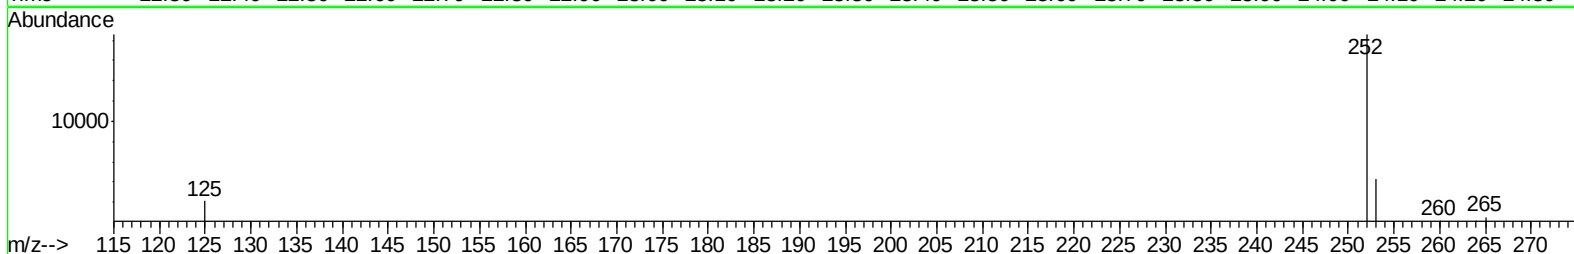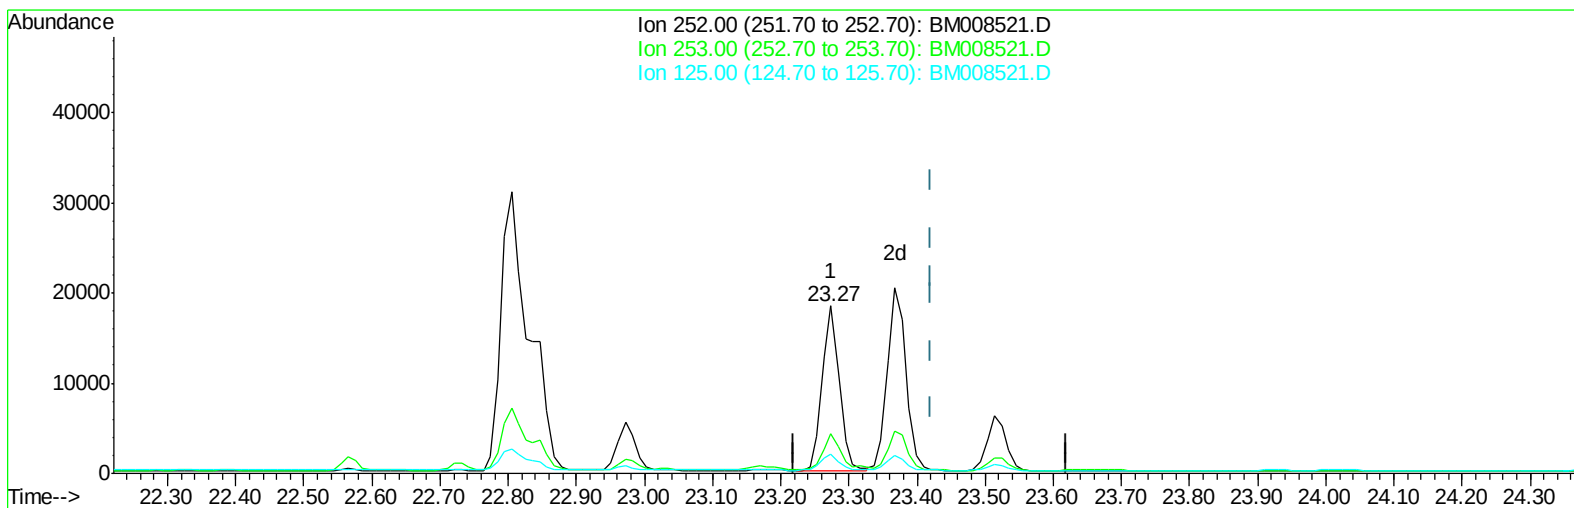

TIC: BM008521.D

(23) Benzo(a)pyrene (C)

23.274min (-0.146) 5.33ng/ul

response 31850

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	23.43#
125.00	22.60	11.39#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

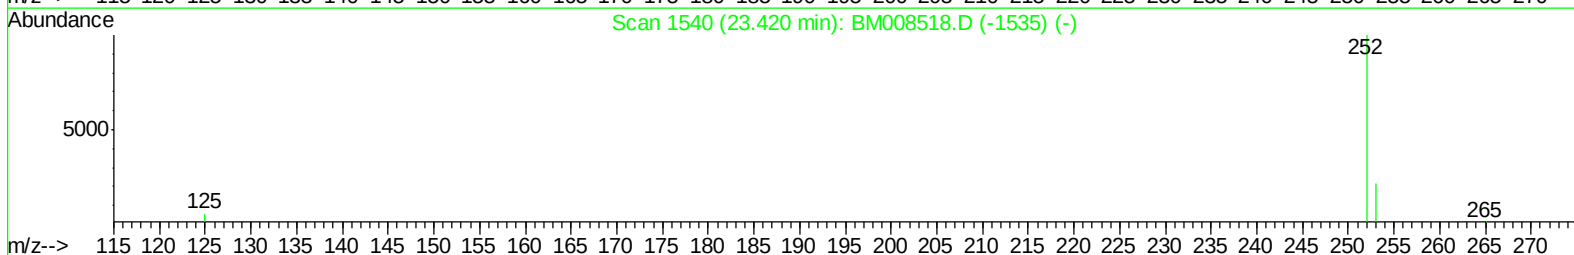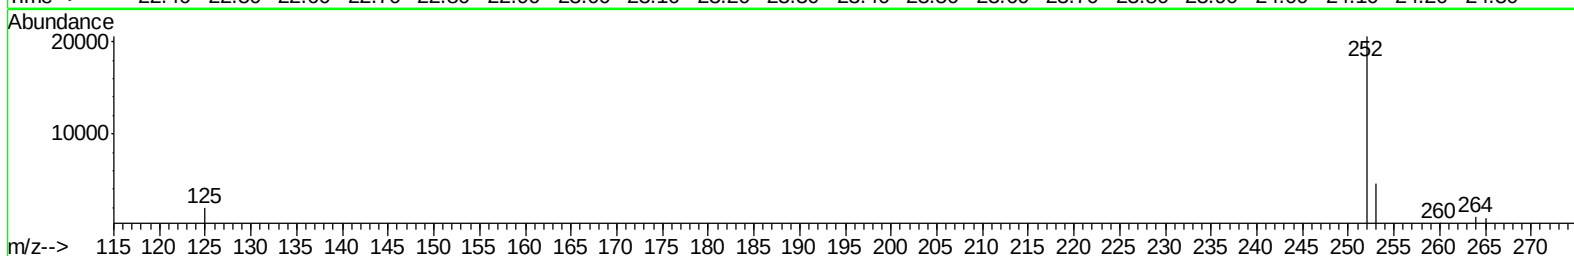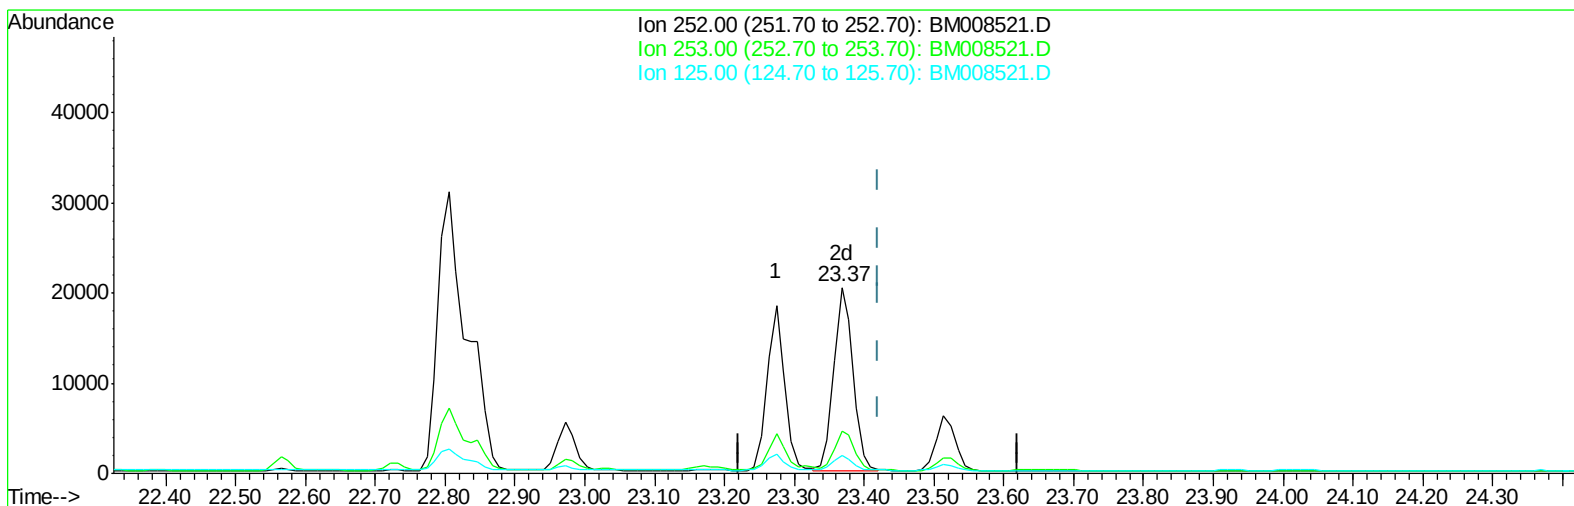

TIC: BM008521.D

(23) Benzo(a)pyrene (C)

23.368min (-0.052) 6.60ng/ul m

response 39503

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	22.57#
125.00	22.60	9.42#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

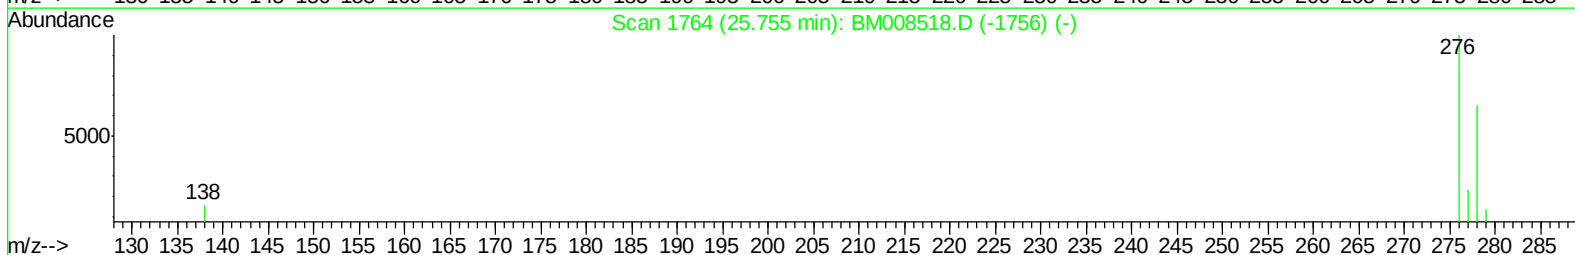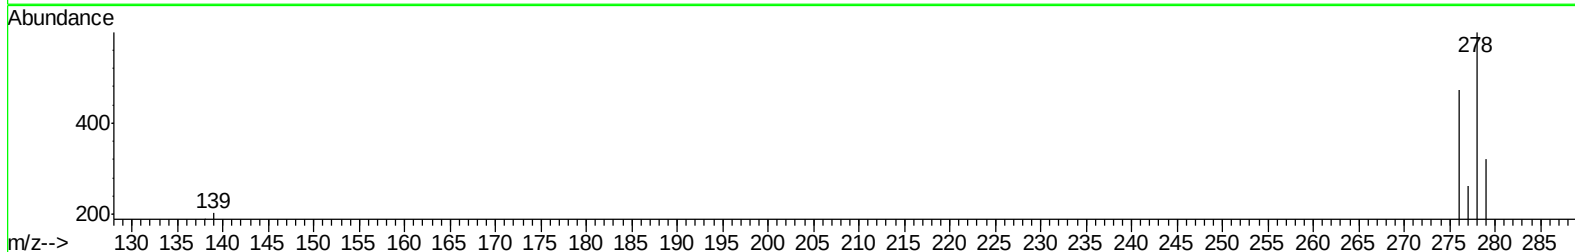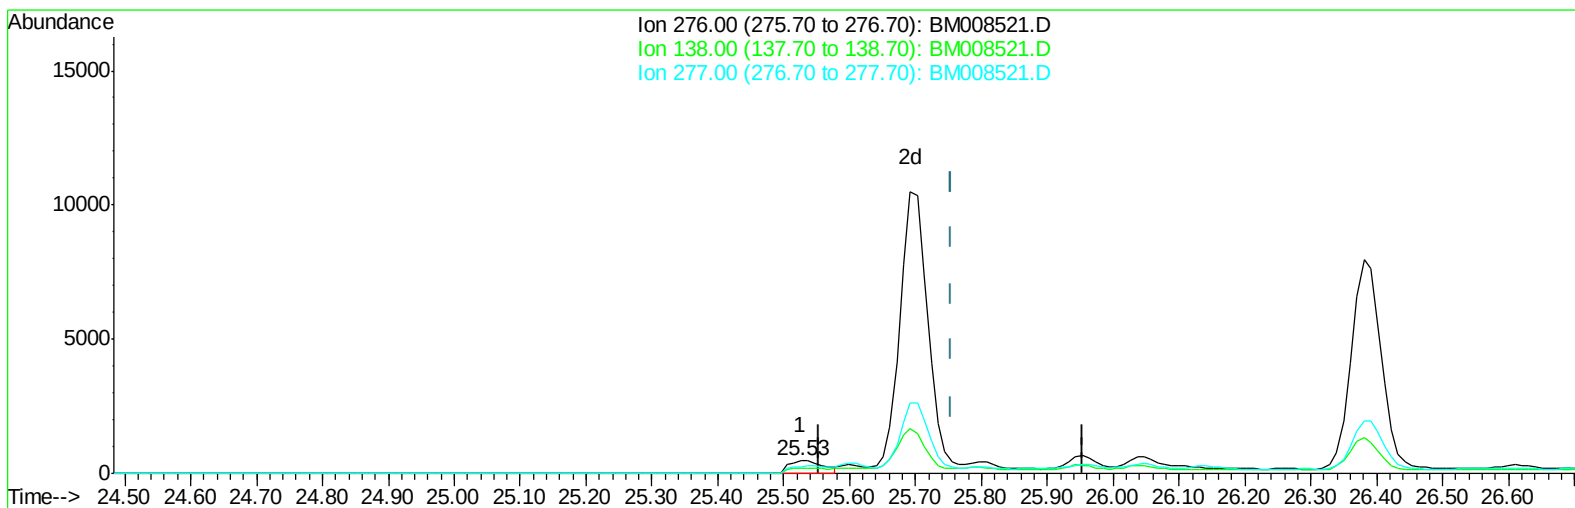

TIC: BM008521.D

(24) Indeno(1,2,3-cd)pyrene

25.526min (-0.230) 0.25ng/ul

response 1775

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	60.28#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

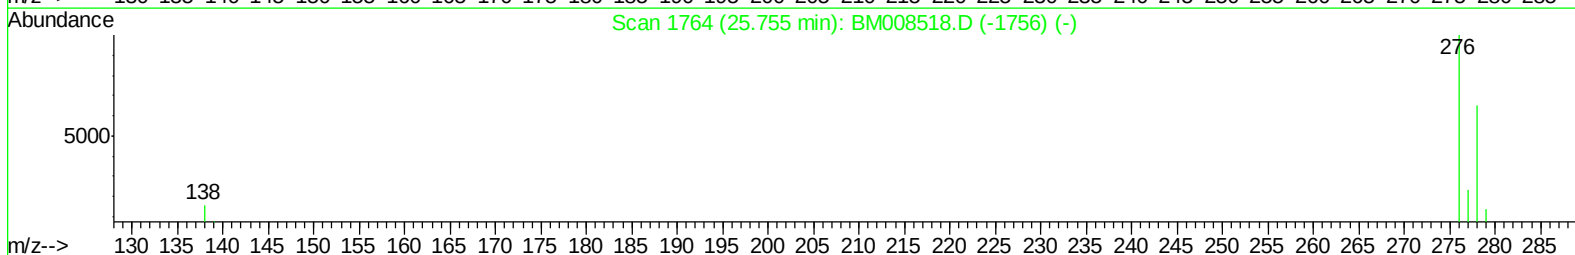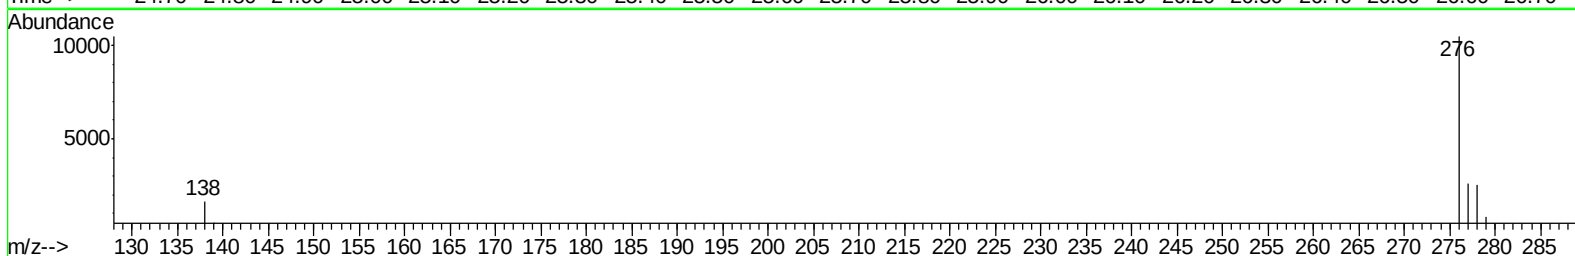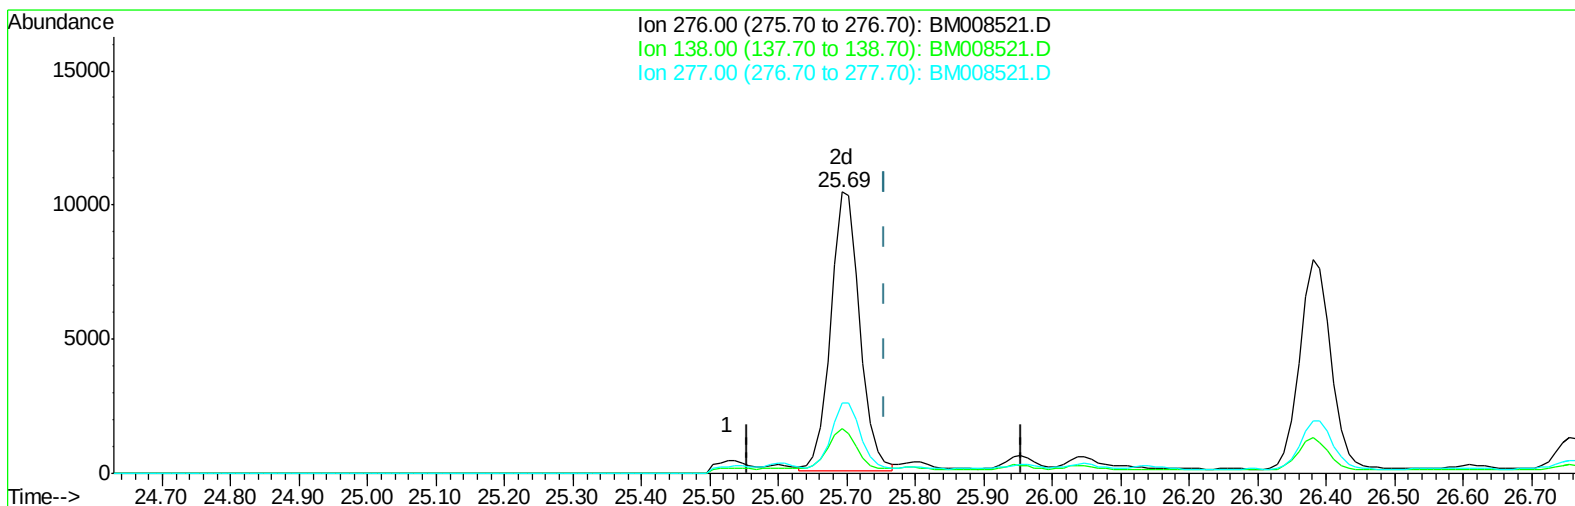

TIC: BM008521.D

(24) Indeno(1,2,3-cd)pyrene

25.692min (-0.063) 4.31ng/ul m

response 30740

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	3.48#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

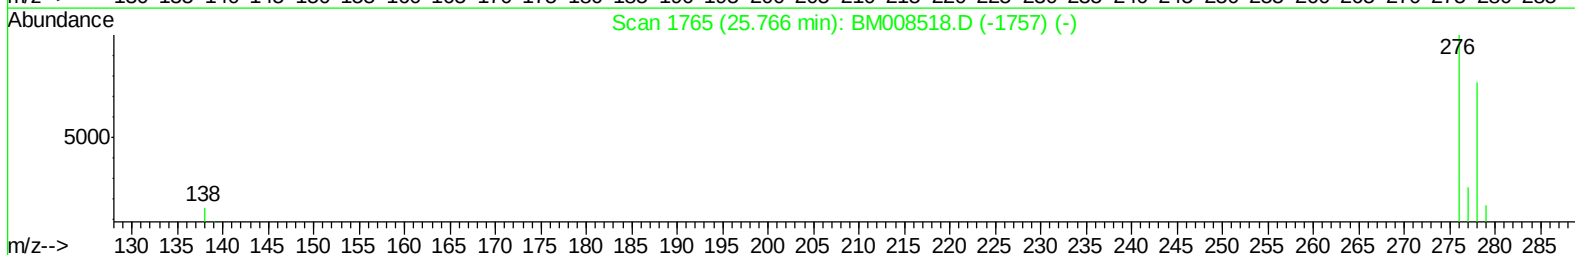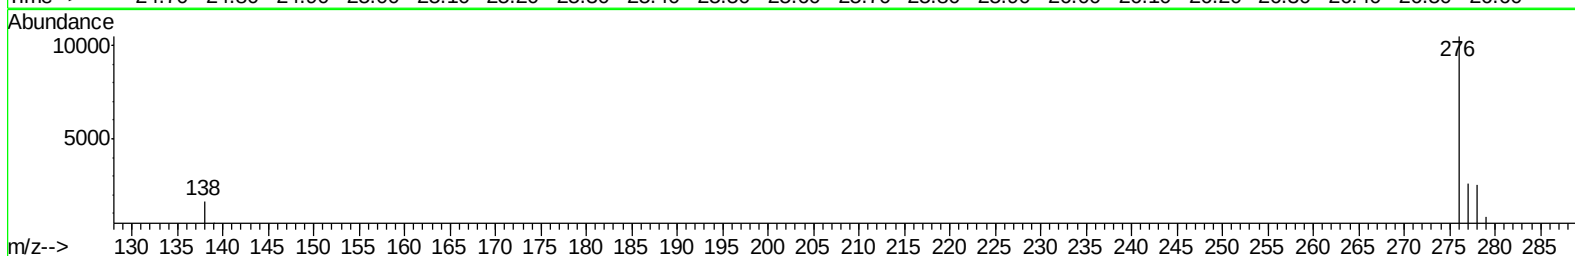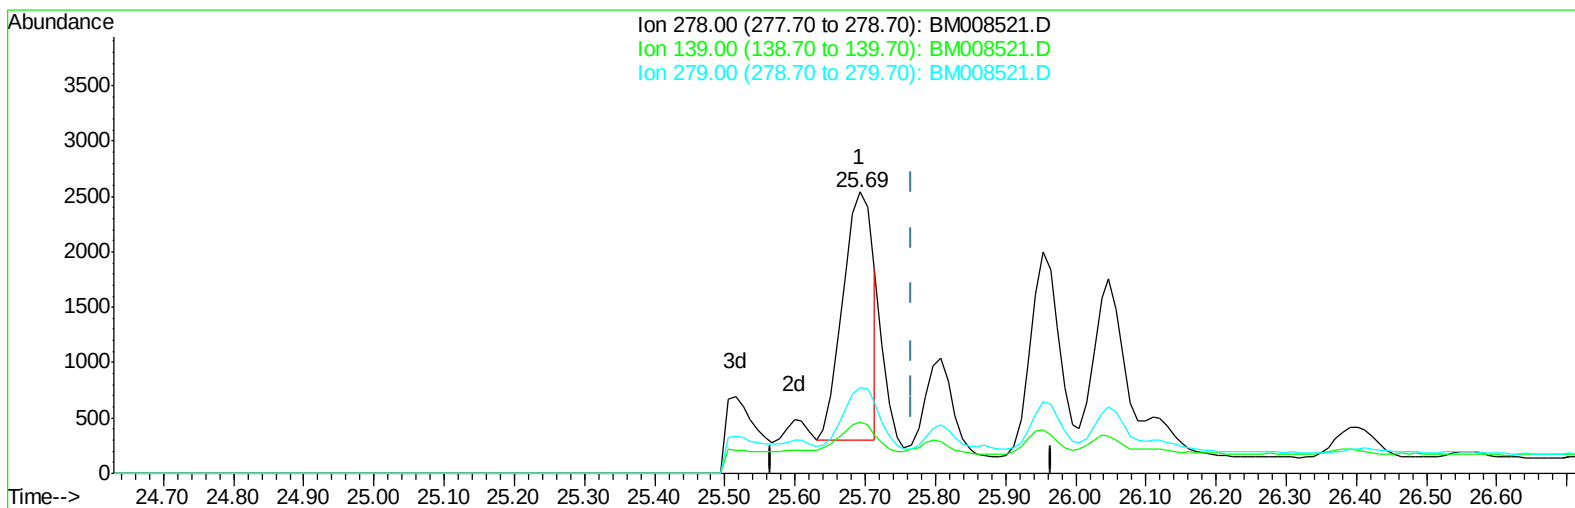

TIC: BM008521.D

(25) Dibenzo(a,h)anthracene

25.692min (-0.073) 1.19ng/ul

response 6794

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	18.18
279.00	32.40	30.70
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

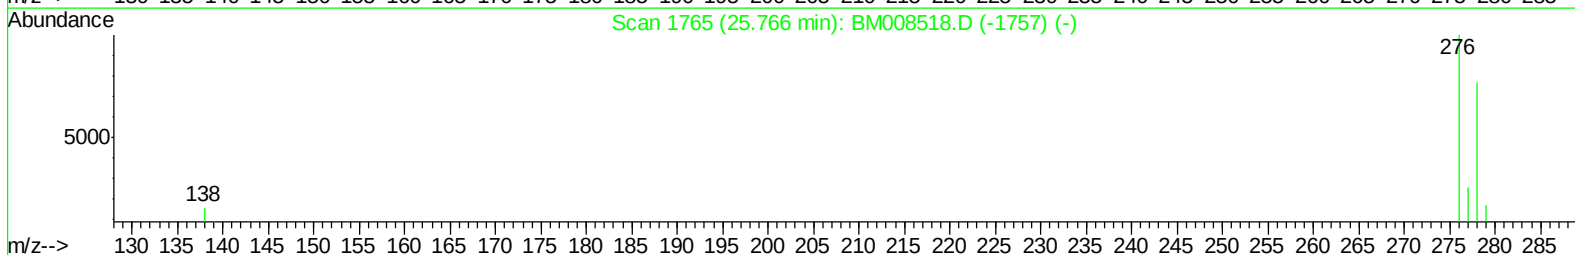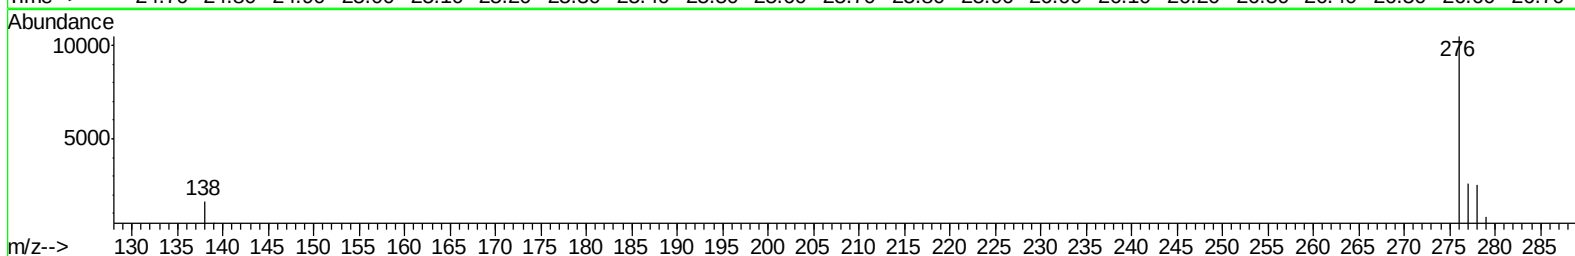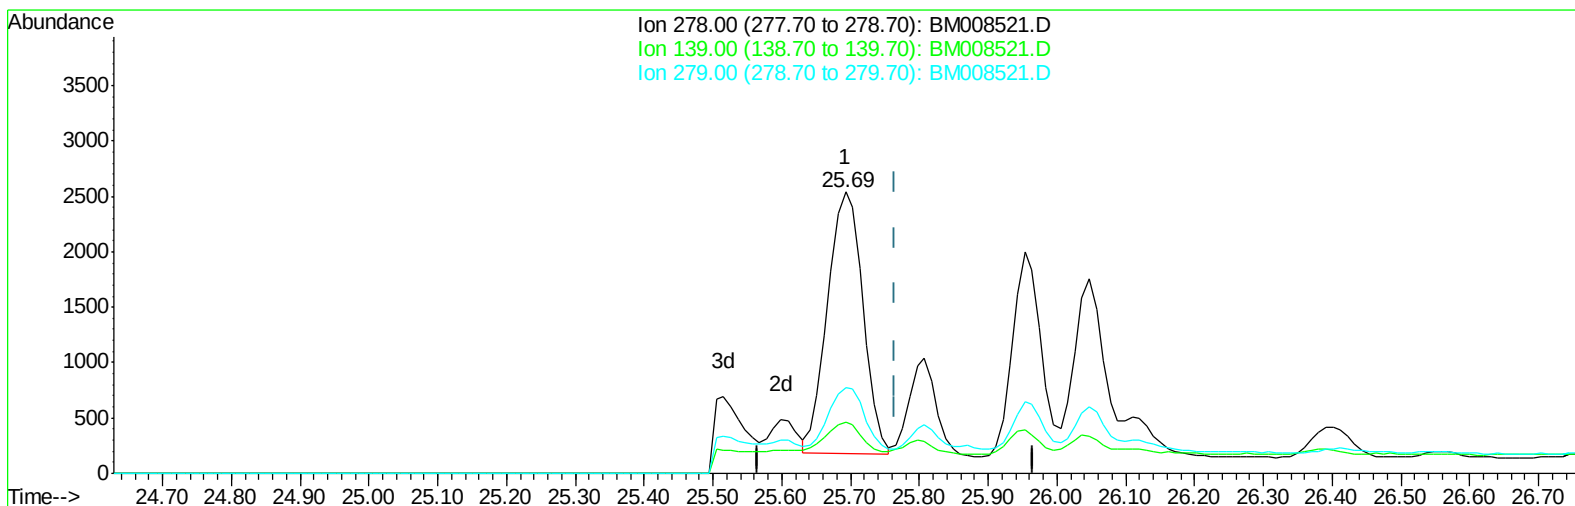

TIC: BM008521.D

(25) Dibenzo(a,h)anthracene

25.692min (-0.073) 1.48ng/ul m

response 8439

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	18.18
279.00	32.40	30.70
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

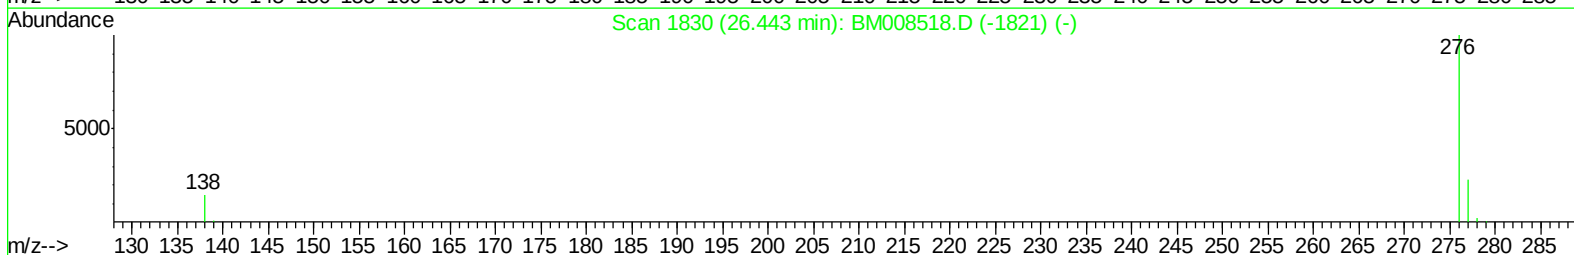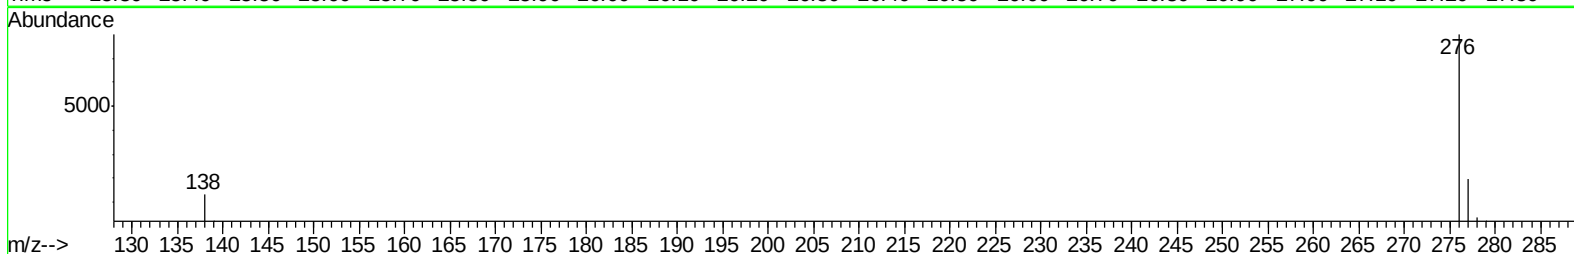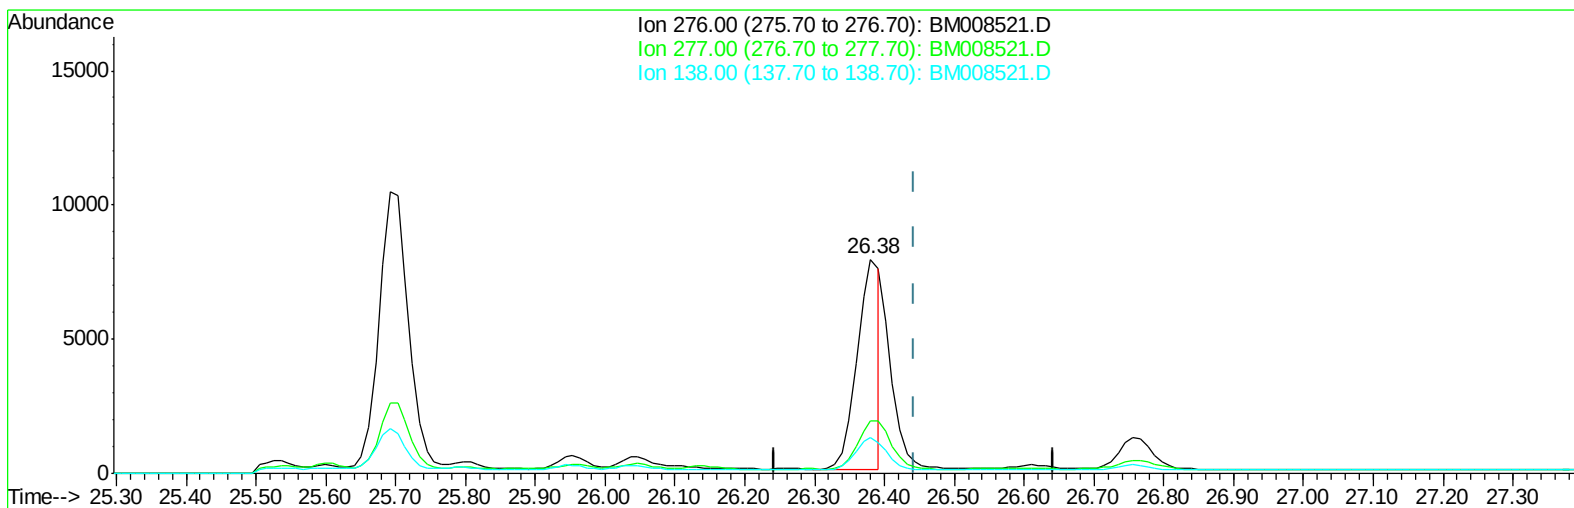

TIC: BM008521.D

(26) Benzo(g,h,i)perylene

26.380min (-0.063) 2.89ng/ul

response 17641

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	24.71
138.00	25.60	16.51#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:40:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

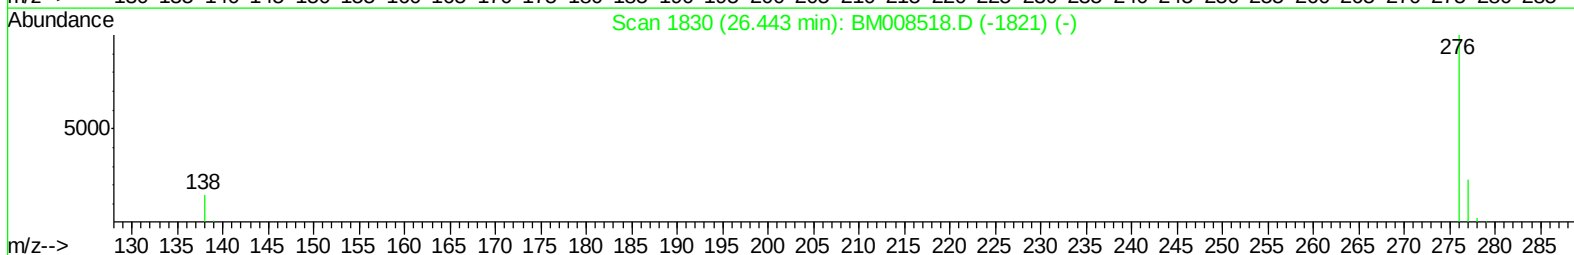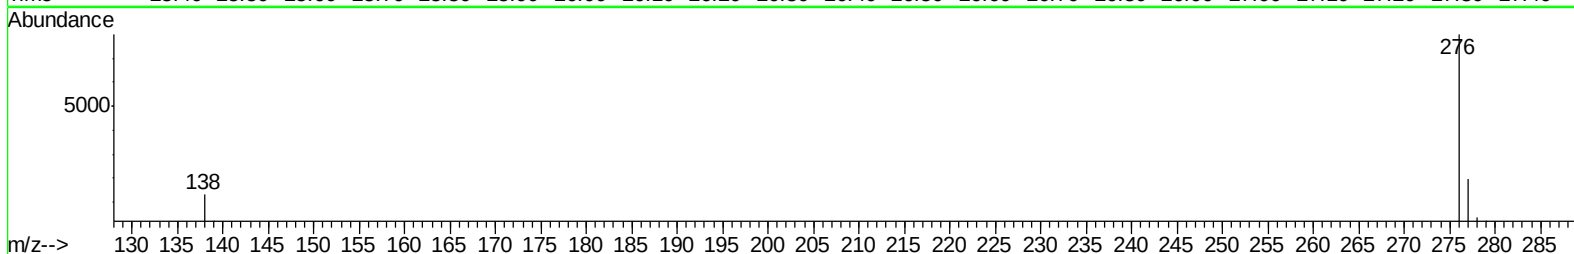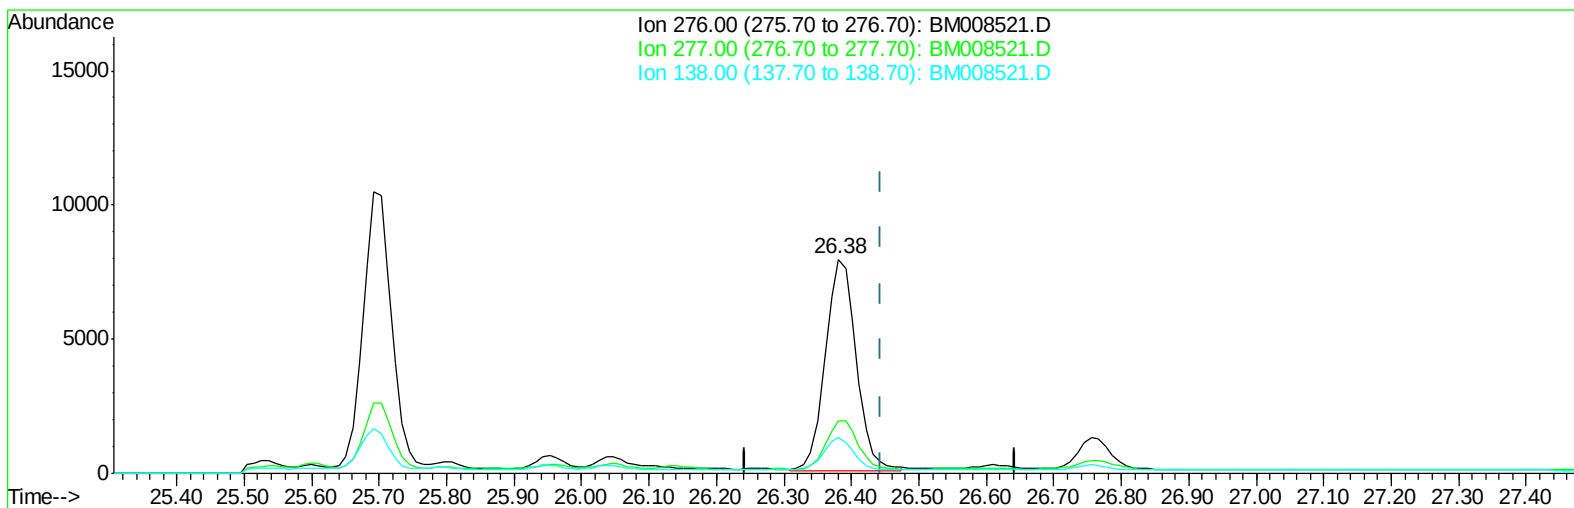

TIC: BM008521.D

(26) Benzo(g,h,i)perylene

26.380min (-0.063) 4.14ng/ul m

response 25306

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	24.71
138.00	25.60	16.51#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
 Data File : BM008521.D
 Acq On : 21 Dec 2016 17:34
 Operator : UM/SJ
 Sample : H5995-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA880

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:43:17 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 00:24:45 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	409	0.40	ng/ul	-0.08
2) Naphthalene-d8	10.43	136	1325	0.40	ng/ul	-0.07
6) Acenaphthene-d10	14.30	164	817	0.40	ng/ul	-0.03
10) Phenanthrene-d10	17.04	188	1515m	0.40	ng/ul	-0.05
16) Chrysene-d12	21.25	240	1550	0.40	ng/ul	-0.03
20) Perylene-d12	23.47	264	1638m	0.40	ng/ul	-0.04
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	503	0.25	ng/ul	-0.08
14) Fluoranthene-d10	19.08	212	1145m	0.27	ng/ul	-0.04
Target Compounds						Qvalue
3) Naphthalene	10.48	128	4643	1.25	ng/ul	98
5) 2-Methylnaphthalene	12.09	142	5954	2.37	ng/ul	93
7) Acenaphthylene	14.01	152	4644	1.26	ng/ul	97
8) Acenaphthene	14.35	153	878	0.32	ng/ul	97
9) Fluorene	15.34	166	810	0.26	ng/ul#	65
12) Phenanthrene	17.07	178	15421m	3.33	ng/ul	
13) Anthracene	17.18	178	5750	1.28	ng/ul	96
15) Fluoranthene	19.11	202	47128m	8.31	ng/ul	
17) Pyrene	19.47	202	51061	8.52	ng/ul	96
18) Benzo(a)anthracene	21.23	228	36953	7.26	ng/ul	98
19) Chrysene	21.28	228	30219	5.42	ng/ul	99
21) Benzo(b)fluoranthene	22.80	252	66978m	10.38	ng/ul	
22) Benzo(k)fluoranthene	22.83	252	24696m	3.92	ng/ul	
23) Benzo(a)pyrene	23.37	252	39503m	6.60	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.69	276	30740m	4.31	ng/ul	
25) Dibenzo(a,h)anthracene	25.69	278	8439m	1.48	ng/ul	
26) Benzo(g,h,i)perylene	26.38	276	25306m	4.14	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008521.D
Acq On : 21 Dec 2016 17:34
Operator : UM/SJ
Sample : H5995-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA880

Manual Integrations
APPROVED

Sohil
12/22/2016 12:35:24 PM

Quant Time: Dec 22 00:43:17 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

